

CALIBRATION REPORT

Details of Device Under Calibration :

Date: 05-08-19

Customer Name & Address: General Hoospital, Bharuch	Certificate ID : AZ/19-20/ 1014A
	Date of Issue : 05-08-19
Name of Equipment: Domestic refrigerator	Calibration Date : 01-08-19
Manufacturer : Godrej	Calibration Due Date : 31-07-20
Model : F-5	Location of equipment :
Serial No : NS	Ambient Temperature : 22 °C

Test Equipment Used:

sr no	Test equipment	Company	Model	Sr no.	Cali. date	Cali. due date
1	Temperature Indicator with RTD sensor	Masibus	408	1002ME11278	17-01-19	16-01-20


Condition Of Equipment at the time of Calibration : GOOD


Test Report:


Sr No	Test	Unit	Range	Reading at	Observed Value by Test equipment	Result
1	Temperature	Deg.° C	2°C	Rack 1	4.3	Pass
2			to	Rack 2	4.4	Pass
3			8 °C	Container	4.4	Pass
4			N.S.	Freezer	-16.7	Pass

Note:

- Results reported are valid at the time of and under the stated conditions of measurement.
- Calibration has been done as per customer's requirement.
- Measurements are traceable to the National Standard
- NS means Not Specified and DUC means Device Under Calibration
- The reported measurement uncertainty is estimated at a level of confidence of approx 95 % with a coverage factor $k = 2$.
- Cali means calibration .

Calibrated By: 
Anal Patel

Approved By: 
Gaurav Desai

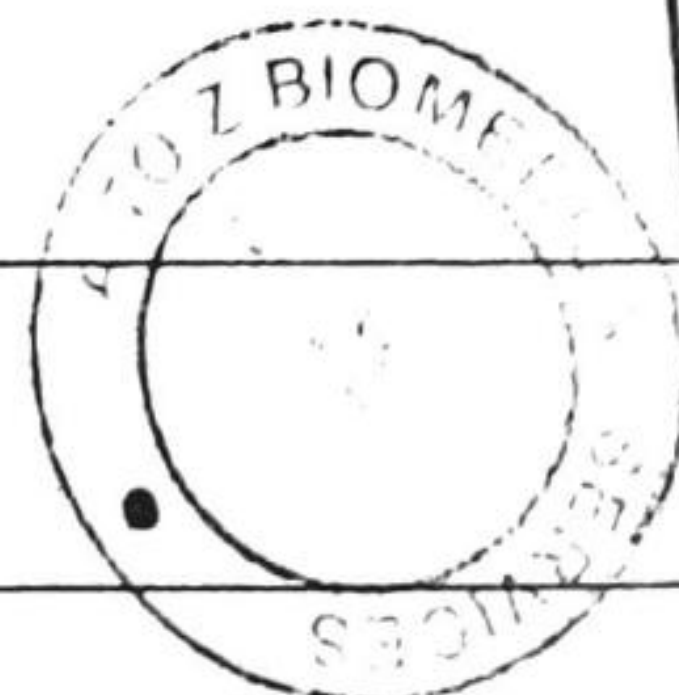

THIS DOCUMENT SHALL NOT BE REPRODUCED, EXCEPT IN FULL, WITHOUT THE WRITTEN APPROVAL OF "A TO Z BIOMEDICAL SERVICES"