



PHARMTECH SERVICES

(Accredited by ISO : 9001 - 2015)

303, 3rd Floor, Ushakiran Building, Raopura Main Road,
Raopura, Vadodara - 390 001, Gujarat, India.
pharmtech.services@yahoo.com + 91 9712539054
www.pharmtech.co.in

CALIBRATION CERTIFICATE

CERTIFICATE NO.	CALIBRATION DATE	NEXT DUE DATE	Page No
19-20/Patho Laboratories/ RPM-01	05-11-2019	04-11-2020	1 of 2
NAME & ADDRESS OF CUSTOMER :		S S HOSPITAL PETLAD	

SPECIFICATION OF UNIT UNDER CALIBRATION

INSTRUMENT NAME :	Centrifuge	DEPARTMENT :	Patho Laboratories
INSTRUMENT ID NO :	Patho Laboratories/ RPM-01	SER.REQ. DATE :	N.A
INST RANGE :	0 to 5000 RPM	DATE OF RECEIPT :	05-11-2019
LEAST COUNT :	250 RPM	CONDITION OF RECEIPT:	OK
ACCEPTANCE LIMIT:	± 1%FS	LOCATION OF CALIBRATION :	AT SITE
MAKE/MODEL NO :	Hettich	AMBIENT TEMPERATURE :	22°C TO 32 °C
SR.NO :	NA	AMBIENT HUMIDITY :	30 TO 70 % RH
CALIBRATION SOP NO:	PTS/SOP/CAL/25		
LOCATION :	Patho Laboratories		

STANDARDS INSTRUMENTS USED FOR CALIBRATION

NAME & MAKE	SERIAL. NO	RANGE	INST ID NO	CERTIFICATE NO & CERTIFIED BY	DUE DATE
Digital Tachometer	5806389	2.5 - 99999 rpm	PTS/TM/01	ACPL/PR/0341/03/2019, ARCHERCHEM	17/04/2020

OBSERVATION TABLE :

(UNIT OF MEASUREMENT: RPM)

STANDARD READING	UUC READING	(±) DEVIATION
(RPM)	(RPM)	(RPM)
499.9	500	0.1

STANDARD READING	UUC READING	(±) DEVIATION
(RPM)	(RPM)	(RPM)
1997	2000	0.3

STANDARD READING	UUC READING	(±) DEVIATION
(RPM)	(RPM)	(RPM)
2997	3000	0.3

STANDARD READING	UUC READING	(±) DEVIATION
(RPM)	(RPM)	(RPM)
4996	5000	0.4



PHARMTECH SERVICES

(Accredited by ISO : 9001 - 2015)



303, 3rd Floor, Ushakiran Building, Raopura Main Road,
Raopura, Vadodara - 390 001, Gujarat, India.



pharmtech.services@yahoo.com



+ 91 9712539054



www.pharmtech.co.in

CERTIFICATE NO.	CALIBRATION DATE	NEXT DUE DATE	Page No
19-20/Patho Laboratories/ RPM-01	05-11-2019	04-11-2020	2 of 2
NAME & ADDRESS OF CUSTOMER :		S S HOSPITAL PETLAD	


Remarks :

- DEVIATION=UUC READING-STD READING
- The Deviation (Error) reported is within the Specified Acceptance Limit

Note :

- This report refers only to the particular item Calibrated at site/Laboratory.
- The Standard(s) used for calibration is/are calibrated using reference Standards traceable to National/ International Standards.
- The calibration results reported are valid at the time of and under the conditions of measurement.
- This certificate should not be reproduced, except in full, without the prior permission of Pharmtech Services .
- Any correction in this certificate invalidates the certificate.

Abb: UUC: UNIT UNDER CALIBRATION, FS: FULL SCALE, SOP: STANDARD OPERATING PROCEDURE

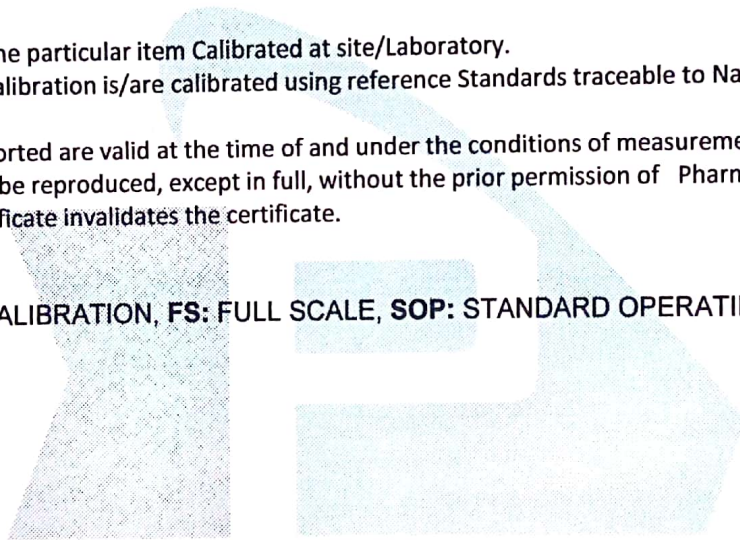

PHARMTECH

CALIBRATED BY:	APPROVED BY:
V.A.R	
CALIBRATION ENGINEER	TECHNICAL MANAGER