

METHOD (1)

	Units	Level 1 - 26441		Level 2 - 26442	
		Mean	Range	Mean	Range
BILIRUBIN (TOTAL)					
Advanced Instruments BR2 Bilirubin Stat-Analyzer (Photometric) (4)	mg/dL	1.86	1.50 – 2.20	4.61	3.70 – 5.50
Catachem ChemWell-T (4)	mg/dL	0.900	0.500 – 1.30	4.10	3.25 – 4.95
DPD (3)	mg/dL	1.11	0.774 – 1.45	4.63	3.83 – 5.43
Jendrassik Grof (3)	mg/dL	1.02	0.719 – 1.33	4.51	3.92 – 5.11
Teco Diagnostics TC-Matrix (Sulphanilic acid, DMSO)	mg/dL	▲		▲	
Vanadate Oxidation (3)	mg/dL	1.05	0.888 – 1.22	4.64	4.12 – 5.16
Wako L-Type (AU480) (4)	mg/dL	0.973	0.930 – 1.02	4.27	4.06 – 4.48
CALCIUM					
Arsenazo III (3)	mg/dL	10.1	9.09 – 11.2	11.8	10.7 – 13.0
Catachem ChemWell-T (4)	mg/dL	10.5	9.30 – 11.7	12.1	10.9 – 13.3
o-cresolphthalein complexone (3)	mg/dL	9.89	8.96 – 10.8	12.0	10.9 – 13.0
Teco Diagnostics TC-Matrix (Arsenazo III)	mg/dL	▲		▲	
Teco Diagnostics TC-Matrix (o-cresolphthalein complexone)	mg/dL	▲		▲	
CALCIUM (IONIZED)					
ISE Direct	mg/dL	§		§	

Date

13/1/20

8.0 - 20

Calcium - 9.4
 K⁺ - 3.5/2.5
 Na⁺ - 142.5
 Pho - 3.8.P - ~~muscle~~
 Amylase - 71
 CRP - 123

2/1/20

Calcium - 10.8

14/1/20

Calcium - 9.1

20/1/20

Amylase - 72

IQC RESULT FOR CALCIUM IN LOG BOOK DATE 14/01/2020

COLLATED REPORT BY DATE.

DATE: 14/01/20

000003	14/01/20	CA-A	10.32	mg/dl	H
000004	14/01/20	CA-A	8.77	mg/dl	
000005	14/01/20	CA-A	9.14	mg/dl	
000006	14/01/20	CA-A	6.77	mg/dl	L
000007	14/01/20	CA-A	7.22	mg/dl	L

READING SHOWN IN THE MACHINE FOR THE IQC CALCIUM SAMPLE 14/01/2020

Date ___/___/___

21/1/20

DB - 0.3

25/1/20

calcium - 9.6

27/1/20

Calcium - 10.0

Na⁺ - 138.8

K⁺ - 3.5

Phosph - 3.9

CPK - 113

Amylase - 74.4

DB - ~~0.3~~ 0.5

7/2/20

Glucose - 76

cho - 233

1QC RESULT FOR CALCIUM IN LOG BOOK DATE 25/01/2020 & 27/01/2020

COLLATED REPORT BY DATE.

DATE: 27/01/20

000025	27/01/20	CKN	92.77	IU/l	
000026	27/01/20	CKN	94.52	IU/l	
000027	27/01/20	CA-A	10.11	mg/dl	
000028	27/01/20	CA-A	10.05	mg/dl	
000029	27/01/20	PHOS	5.07	mg/dl	H

READING SHOWN IN THE MACHINE FOR THE IQC CALCIUM SAMPLE 27/01/2020


COLLATED REPORT BY DATE.

DATE: 25/01/20

000019	25/01/20	RFRK	0.44	IU/ml	
000020	25/01/20	CA-A	10.24	mg/dl	H
000021	25/01/20	CA-A	9.68	mg/dl	
000022	25/01/20	CA-A	9.90	mg/dl	

READING SHOWN IN THE MACHINE FOR THE IQC CALCIUM SAMPLE 25/01/2020

QC RESULT FOR CALCIUM IN LOG BOOK DATE 17/02/2020 AND 18/02/2020

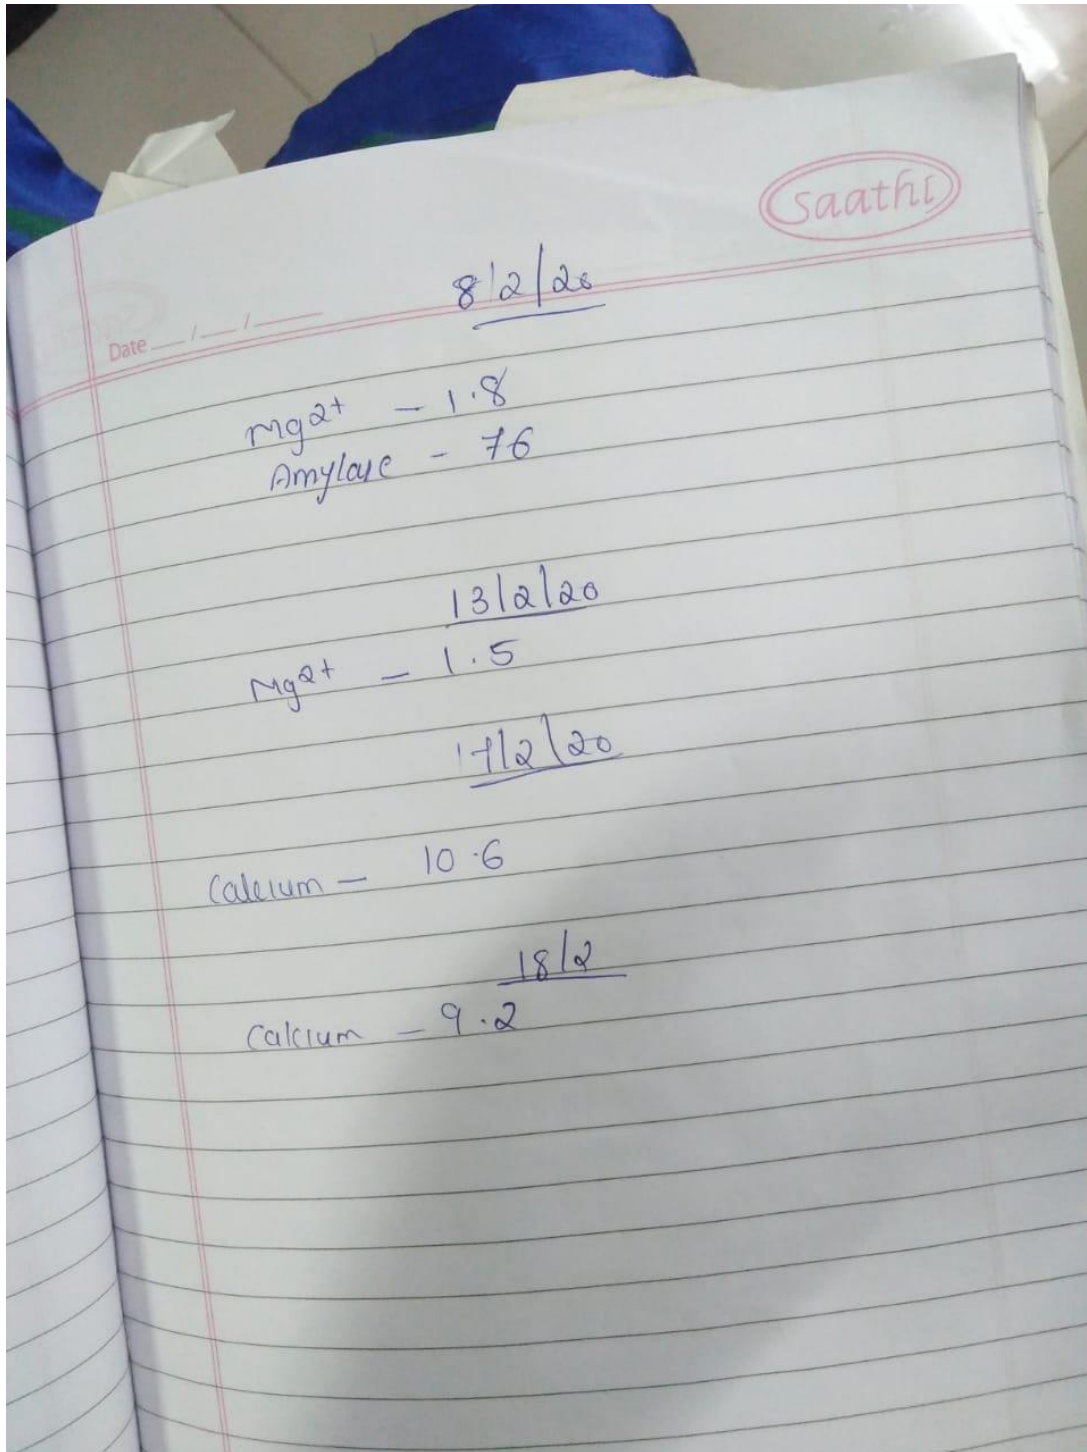

COLLATED REPORT BY DATE.

DATE: 17/02/20

000079	17/02/20	CA-A	11.44	mg/dl	HHH
000080	17/02/20	CA-A	10.64	mg/dl	
000081	17/02/20	PHOS	5.13	mg/dl	
000082	17/02/20	PHOS	4.50	mg/dl	
000083	17/02/20	PHOS	4.36	mg/dl	

READING SHOWN IN THE MACHINE FOR THE IQC CALCIUM SAMPLE 17/02/2020

COLLATED REPORT BY DATE.

DATE: 18/02/20

000087	18/02/20	CA-A	9.22	mg/dl
000088	18/02/20	CA-A	9.17	mg/dl

READING SHOWN IN THE MACHINE FOR THE IQC CALCIUM SAMPLE 18/02/2020