



JEYAM LAB

LAB X-RAY E.C.G BIOPSY

K.PUDUR | KADACHANENDAL | S.S. COLONY



E-mail : info@jeyamlab.com

LABORATORY REPORT

From,

JEYAM CLINICAL LAB
User Id : NABLBCL000997
K.Pudur
Madurai
Tamilnadu.


To,

NABL
New Delhi
India

Dear sir,

while uploading QC result our staff has done a mistake our result is 6.2 mg/dl she mentioned on 10.2 mg/dl sorry for the inconvenience

Date - 19/10/20

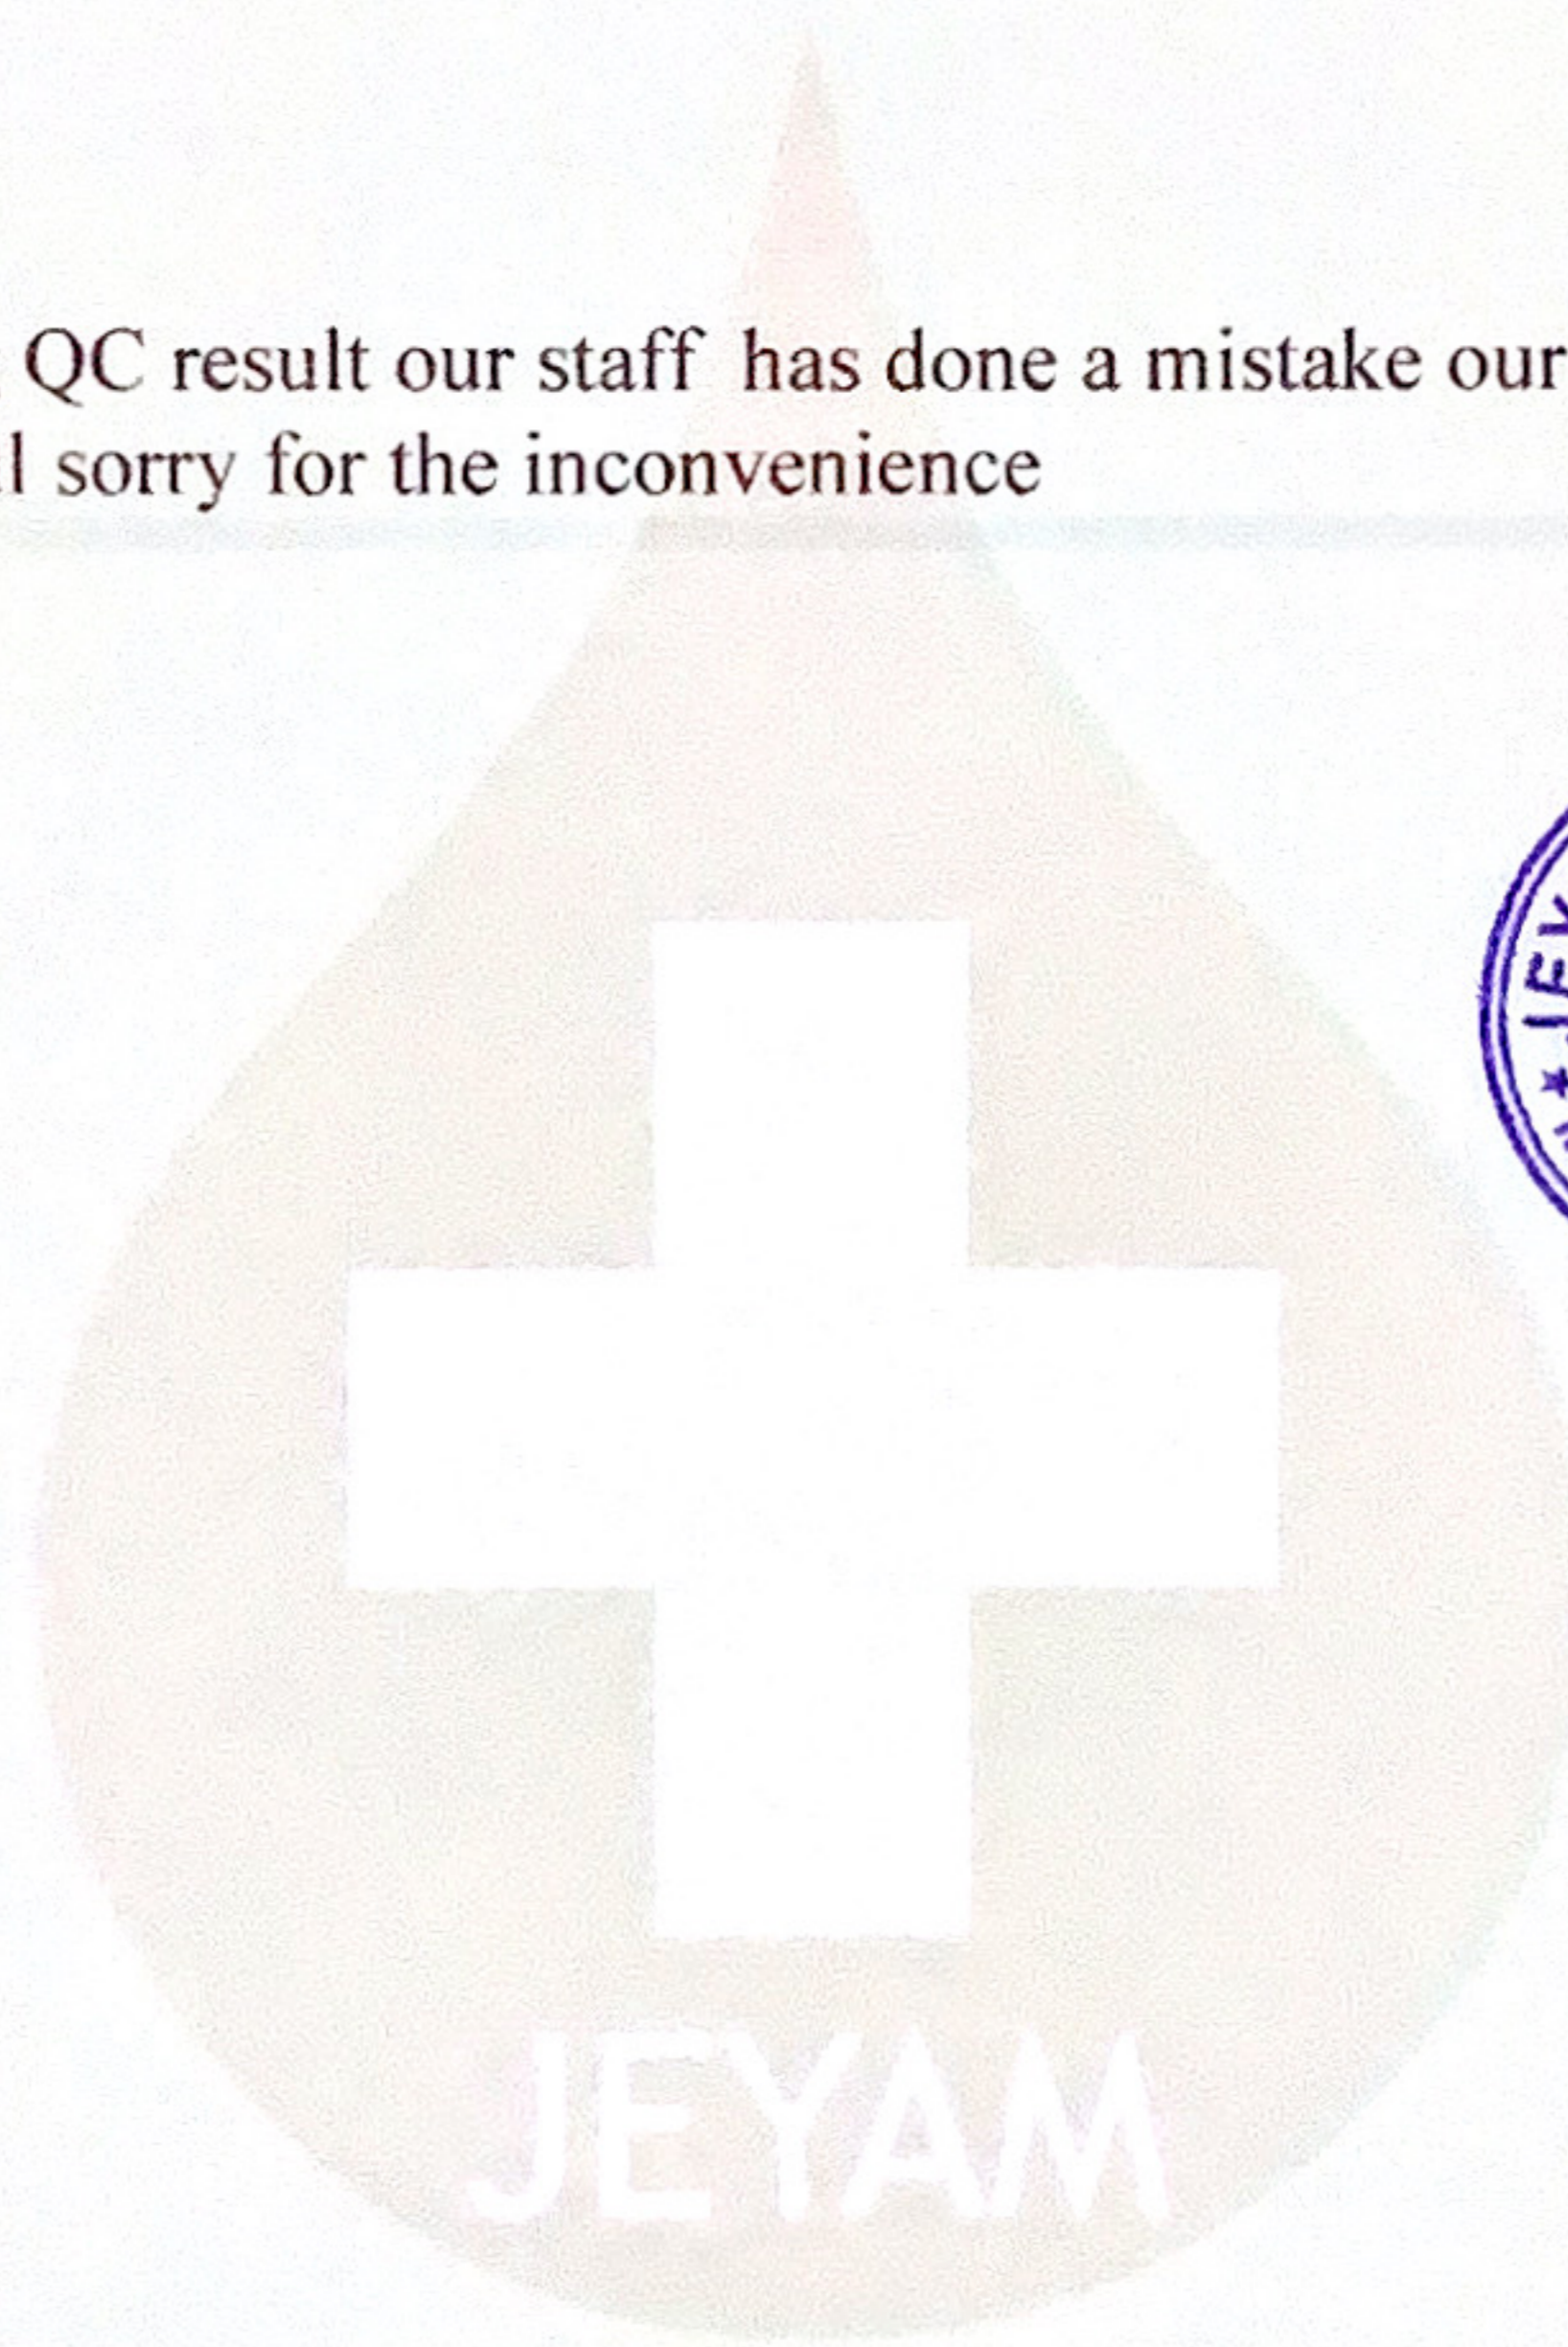

Verified By

www.jeyamlab.com

Lab Technologist

All investigations have their limitation which are imposed by the limits of sensitivity and specificity of individual assay procedures as well as the specimen received by the laboratory. Isolated laboratory investigations never confirm the final diagnosis of the disease. They only help in arriving at a diagnosis in conjunction with clinical presentation and other related investigations.

PARTIAL REPRODUCTION OF THIS REPORT IS NOT PERMITTED

LAB MONTHLY SUMMARY

Lab Name JEYAM CLINICALLAB

Lab No 5872

Month August

Year 2020

Constituent Group Chemistry II

Date of Result Entered : 19/08/2020

Date of Report Published : 10/09/2020

1	GLUCOSE I	GOD-POD	Mindray	114	112.14	10.01	11.22	116 mg/dl	0.34	2.10
2	UREA I	UREASE UV / GLDH	Mindray	95	75.75	9.79	7.41	60.4 mg/dl	-2.07	1.52
3	CREATININE I	OTHERS (Any Other Principles / Methods)	Any Analyser	107	8.65	12.21	1.06	8.9 mg/dl	0.24	0.20
4	T.BILIRUBIN I	OTHERS (Any Other Principles / Methods)	Any Analyser	128	5.83	13.22	0.77	10.4 mg/dl	5.94	0.14
5	T-PROTEIN I	OTHERS (Any Other Principles / Methods)	Any Analyser	49	5.53	10.07	0.56	5 g/dl	-0.95	0.16
6	ALBUMIN I	OTHERS (Any Other Principles / Methods)	Any Analyser	68	3.24	11.15	0.36	2.9 g/dl	-0.94	0.09
7	URIC ACID I	OTHERS (Any Other Principles / Methods)	Any Analyser	81	5.98	11.51	0.69	3.8 mg/dl	-3.16	0.15
8	CHOLESTEROL I	CHOD-PAP	Mindray	96	108.55	9.29	10.08	98 mg/dl	-1.05	2.06
9	TRIGLYCERIDE I	GPO-PAP / Enzymatic Colorimetric / End Point	Mindray	96	276.33	11.02	30.44	279 mg/dl	0.09	6.21

SDI Range	Interpretation
Within -1.0 to +1.0	Excellent.
Between ± 1.0 to ± 2.0	Good.
Between ± 2.0 to ± 3.0	Accept with caution. Warning Signal.
Beyond ± 3.0	Unacceptable performance. Action Signal.

Page 1 of 1

Homogeneity and Stability of the sample is passed.

Data in CMC EQAS reports is confidential

Contact details:

Email: clinqc@cmcvellore.ac.in

Contact Number: 0416-2283102

Pamela Christudoss

Dr. Pamela Christudoss
 CMC EQAS Co-Ordinator
 Christian Medical College, Vellore

***** End of Report *****