



# Calibration Verification Report

Client Name: Dr. Raghav Patel Lab & Imaging

Address: Kapil Complex MUKANI CROSSING KALADUGI ROAD .  
Haldwani - Uttarakhand .

Analyser Model :AU480

Serial Number : 2012081548

Date of Inspection: 21/10/19

Valid Upto: 30/4/20

Mechanical modules								
Centering							Height	Alignment Jig
	Cuvette	Washwell	Rack	Stat	ISE	Reagent bottle	Cuvette	Light path
FA	1 mm or more <i>OK</i>	0.5 mm or more <i>OK</i>	1mm or more <i>OK</i>	1mm or more <i>OK</i>	4mm or more <i>OK</i>		14 mm <i>OK</i>	
FB	0.5 mm <i>OK</i>							
FC	<i>OK</i> 1mm/0.5 mm	1 mm <i>OK</i>					14 mm <i>OK</i>	
FD	0.5 mm or more <i>OK</i>	0.5 mm or more				<i>OK</i> 1 mm or more	14.5 mm <i>OK</i>	
GA								

## Calibration Verification Report

Electronic Modules									
Power supply Nomenclature	MEASURED VOLTAGE	TARGET	RANGE	MEASURED VOLTAGE	TARGET	RANGE	MEASURED VOLTAGE	TARGET	RANGE
PS1	4.9V	5 V	+/-0.5 v	15.1V	15 V	+/-0.5 v	15.1V	-15V	+/-0.5 V
PS2	4.9V	5 V	+/-0.5 v	15.1V	15 V	+/-0.5 v	15.1V	-15V	+/-0.5V
PS3	23.8 V	24V	+/-0.5						
PS4	23.8 V	24 v	+/-0.5 v						
PS5	15.1V	15V	+/-0.5 v	15.1V	-15V	+/-0.5 v	12.2V	12V	+/-0.5 v

**Photometric Check:**

Requirement: O.D. value at all the wavelengths should be less than 1.7 ABS units.

Wavelength (in nm)	Optical Density (In ABS Units)	Result
340	0.8794	Pass
380	0.7685	Pass
410	0.7516	Pass
450	0.7619	Pass
480	0.6458	Pass
520	0.6855	Pass
540	0.6560	Pass
570	0.6882	Pass
600	0.6991	Pass
660	0.6688	Pass
700	0.6642	Pass
750	0.6486	Pass
800	0.6263	Pass

## Calibration Verification Report

**Pipetting Check:**

Requirement: The C.V. should be less than 3%.

Test name	No. of Replicates	Mean Value of the replicates	C.V. (In %)	S.D	Remarks
AUT	4	19.45	0.51	0.100	Good
AST	4	16.90	1.93	0.327	Good
REATING	4	0.798	1.88	0.150	Good
Glucose	4	84.5	0.68	0.58	Good
K	4	4.68	1.08	0.050	Good
U	4	101.8	0.94	0.96	Good.

**Incubation temperature:**

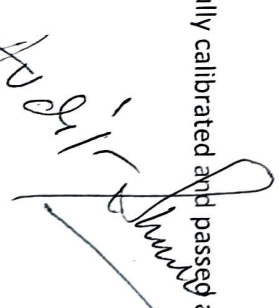
Range: 37°C ± 0.5°C — **OK**

On display, the temperature is 37.0 °C and is stable.

**Appendix:**

Measuring Instruments	Calibration Record	Validity
Digital multimeter	<i>Calibrated</i>	<i>14/6/20</i>
Light path alignment jig	No calibration required	-
Measuring scale	No calibration required	-
Glass Measuring Flask	No calibration required	-

We hereby confirm that Beckman Coulter AU480 has been successfully calibrated and passed all the above quality checks.

  
 Authorised Signatory