

mindray
BC-20s

Golden
Harvest Industries
1800 420 4444

Menu Sample Analysis Table Review QC Reagent Setup Diluent Print




Sample ID 3 Name mohan Gender
Time 27-10-2020 10:45 Mode WB Age

Parameter	Result	Unit	Parameter	Result	Unit	Parameter	Result	Unit
WBC	R 6.9	$10^3/\mu\text{L}$	RBC	4.34	$10^6/\mu\text{L}$	PLT	174	$10^3/\mu\text{L}$
Lymph#	R 1.7	$10^3/\mu\text{L}$	HGB	12.1	g/dL	MPV	10.2	fL
Mid#	R 0.5	$10^3/\mu\text{L}$	HCT	38.6	%	PDW	16.8	
Gran#	R 4.7	$10^3/\mu\text{L}$	MCV	88.9	fL	PCT	1.78	mL/L
Lymph%	R 24.6	%	MCH	27.9	pg			
Mid%	R 7.2	%	MCHC	L 31.4	g/dL			
Gran%	R 68.2	%	RDW-CV	0.135				
			RDW-SD	42.1	fL			

WBC RBC PLT histograms

Next Sample Mode

Sample ID 4 Mode WB 27-10-2020 21:27

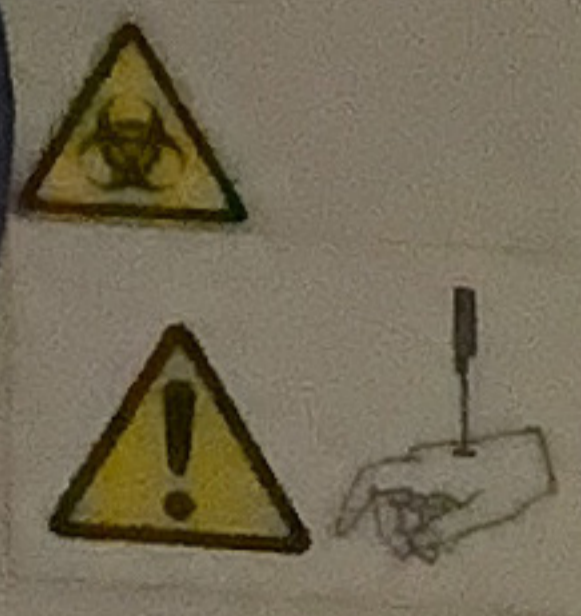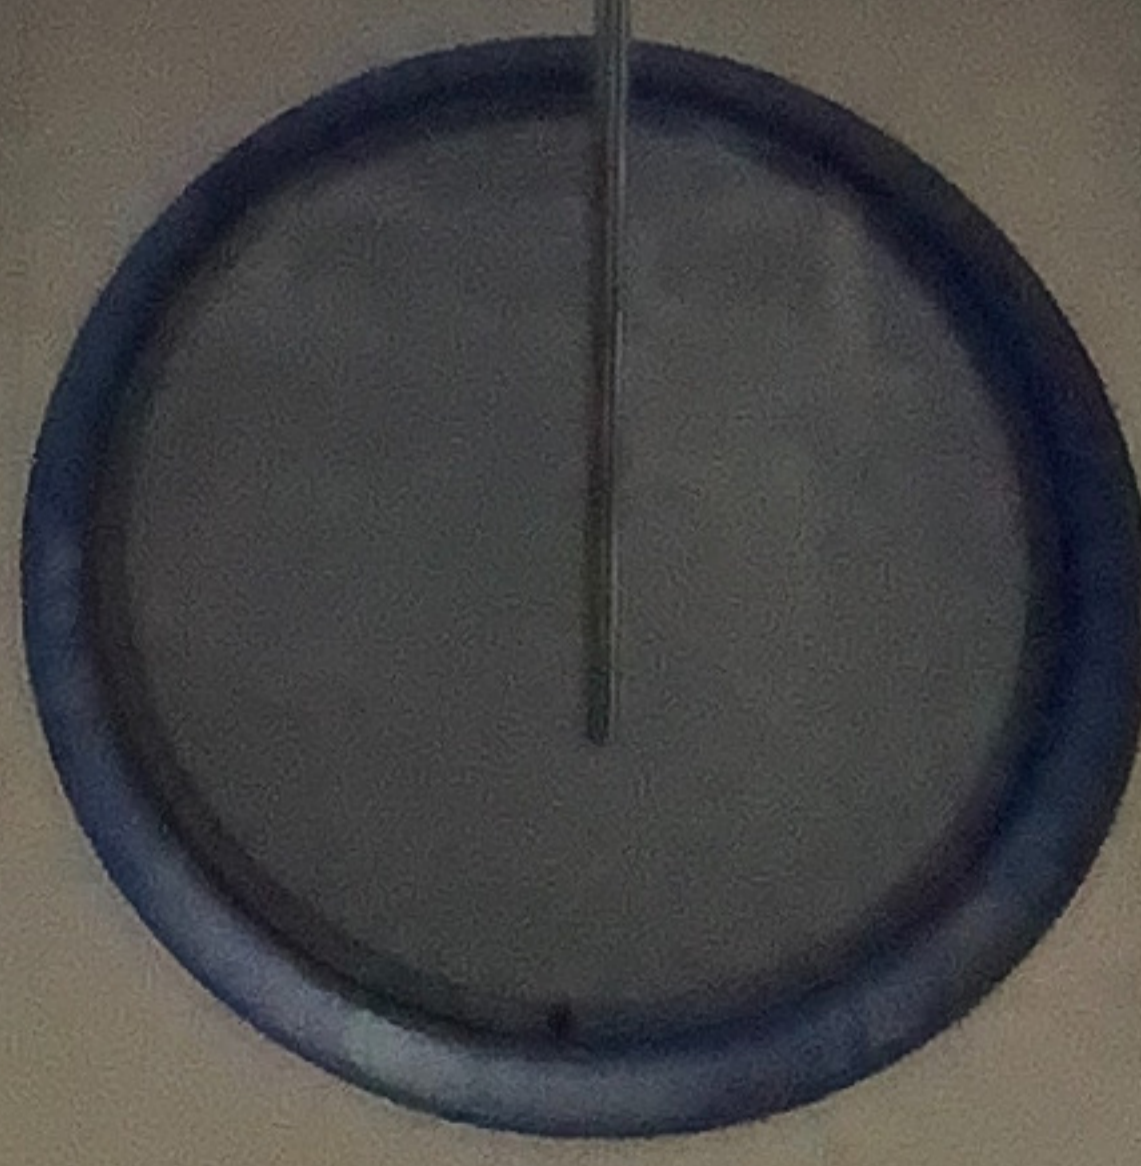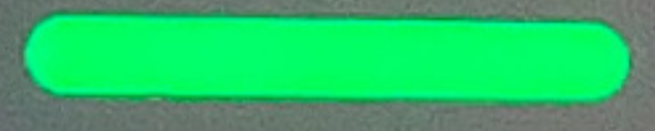

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No : 3/751, 1st Cross Street, Surveyor Colony, K.Pudur, Madurai - 625 007.

Phone : 0452 - 2561691 Mobile : +91 94434 74610



GSTIN: 33AAHCA8053H1ZR • DL No. MDU/4205/20B,MDU/3971/21B • CIN : U33110TN2009PTC072140

CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Jeyam Clinical Lab, K.Pudur, Ayyappan Kovil, Madurai.	Certificate No:	AMS/LAB/2887251
		Issuing Date:	03/01/2020
		Page No:	1 of 2

Details of Device under Calibration (DUC):

DUC:	Haematology Analyser	Id. No:	JCL/AYKL/HA/001
Make:	Mindray	Department:	Laboratory
Model:	BC 20S	Calibrated On:	02/01/2020
Sl. No:	---	Calibration Due Suggested:	01/01/2021
Type:	3 Part	DUC Condition on Receipt:	OK
Range & Least Count:	---		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electrical Safety Analyser	RigelSafeTest60	PSG/CIRD/BMCC/3879/2019	20/01/2020
2	Thermo Hygrometer	HTC	QC/MD/20190218	10/02/2020

Room Temperature: 25°C±2 Room Humidity: 30-60%

(At the time of Calibration)

ESA Test Results:

SL.No	Parameter	ESA Reading	Unit	Normal Range	Condition
1	Current	1.2	Amps	1	Normal
2	Frequency	50.1	Hz	49 -50	Normal
3	Mains Voltage Line - Neutral	234.3	Volts	220 - 240	Normal
4	Mains Voltage Line - Earth	235.5	Volts	220 - 240	Normal
5	Mains Voltage Neutral - Earth	4.2	Volts	< 7	Normal

*Electrical Safety: Please check the attached log sheet

Note:

1. Calibration Points were selected as per customer request.
2. Each reading were taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

Calibrated By:

(Calibration Engineer)

B. S. S.



Approved by:

(Technical Manager)

B. S. S.