

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No : 3/751, 1st Cross Street, Surveyor Colony, K.Pudur, Madurai - 625 007.

Phone : 0452 - 2561691 Mobile : +91 94434 74610



GSTIN. 33AAHCA8053H1ZR • DL No. MDU/4205/20B,MDU/3971/21B • CIN : U33110TN2009PTC072140

CALIBRATION CERTIFICATE

Customer Name & Address:	M/s. Srinivasa X-Ray & Clinical Laboratory, 83,A.K.S Theatre road, Kovilpatti - 628502.	Certificate No:	AMS/LAB/2888277
		Issuing Date:	21/09/2020
		Page No:	1 of 2

Details of Device under Calibration (DUC):

DUC:	Auto Bio Chemistry Analyser	Id. No:	SCL/LAB/A-BCA/001
Make:	TRANSASIA	Department:	Laboratory
Model:	EM200	Calibrated On:	19/09/2020
Sl. No:	B2001051	Calibration	
Type:	Fully Auto	Due Suggested:	18/09/2021
Range & Least Count:	---	DUC Condition on Receipt:	OK

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electrical Safety Analyser	RigelSafeTest60	PSG/CIRD/BMCC/4424/2020	19/01/2021
2	Thermo Hygrometer	HTC	QC/AMS-DTI-004	22/02/2021

Room Temperature: 25°C±2 Room Humidity: 30-60% (At the time of Calibration)

ESA Test Results:

SL.No	Parameter	ESA Reading	Unit	Normal Range	Condition
1	Current	1428	mA	1	Normal
2	Frequency	49.98	Hz	49 -50	Normal
3	Mains Voltage Line - Neutral	228.5	Volts	220 - 240	Normal
4	Mains Voltage Line - Earth	228.4	Volts	220 - 240	Normal
5	Mains Voltage Neutral - Earth	4.1	Volts	< 7	Normal

*Electrical Safety: Please check the attached log sheet

SL.No	Parameter	Measured	Standard	Correction	Unit
1	Lamp Voltage	11.92	12.00	-0.08	Volts
2	Detector Sensitivity	-0.00	0.0	0.0	% Absorbance
3	Sipper Volume	320	350	-80	
4	Pump pressure	13.71	15	-1.29	cmH2G.

Allowable Tolerance: set by Customer


Note:

1. Calibration Points were selected as per customer request.
2. Each reading were taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

Calibrated By:

(Calibration Engineer)

B. S. S.

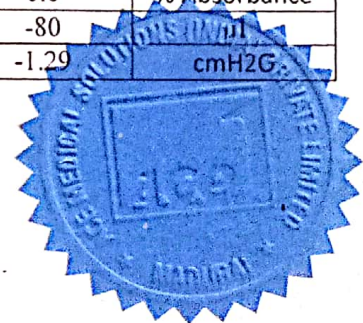

Approved by:

(Technical Manager)

B. S. S.