



COMMITTED TO THE  
CUSTOMER SINCE - 1996

# VAIDYANATHESHWARA INSTRUMENTS

## CERTIFICATE OF CALIBRATION



CERTIFICATE NO  
CC-2473

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Page 1 of 2

**1 Name and Address of the Customer** : M/s. FOSTR HEALTH CARE & DIAGNOSTICS.,  
No 12 , 2nd Floor, Panathur Main Road ,  
Panathur Bangalore - 560087.

**2 Customer Reference**

2.1 ULR No. : CC247320100021889F  
2.2 SRF No. : 1991  
2.4 Certificate No. : VI/20-21/1991-01  
2.6 Format No. : VI-FRM-ME-105  
2.7 Date Of Issue : 13-08-2020

**3 Details Of Device Under Calibration(DUC).**

3.1 Nomenclature : Pipette  
3.2 Make / Model : Thermo Scientific / Finnpiquette®F3  
3.3 Range : 5 - 50 µl  
3.4 SL No. : OW06373  
3.5 DUC Condition : Satisfactory  
3.6 Calibration Procedure No. : SM/WI/M-10 Based On ISO 8655-6:2002 E  
3.7 No.of Pages : 2  
3.8 Calibration Date : 13-08-2020  
3.9 Calibration Due : 12-08-2021  
3.10 Calibration done at : VI Volumetric Lab  
3.11 Discipline : Mechanical (Mass & volume)

**4 Environmenetal Condition**

Temperature 20.6 °C Humidity 51 %Rh

**5 Standards Used for calibration**

Sl. No.	Nomenclature	Make & Model	Sl. No	Range	Traceable to /Cert. No.	Validity
1	Digital Weighing Balance	RADWAG/MYA5.4Y	544953	0.1mg to 5g	VI/19-20/INT-ME-121	20-09-2020
2	E1 Class Weights	LCGC	VI-E1-ME-001	1mg to 200g	TVC SPL 19/04/339-01	02 - 04 - 2022

**6 Note:**

- The Calibration Certificate relates only to the above DUC
- Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab..
- Corrections/erasing, invalidate the Calibration Certificate.
- Calibration of the DUC are traceable to National standards/International Standards
- Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- Results Reported are valid at the time of and under the stated conditions of measurements.
- The usage of NABL symbol is as per NABL guidelines given in NABL-133.

Calibrated By

*Sameer M S*

Sameer M S

(Calibration Engineer)

Checked By

*Afjal Basha S*

Afjal Basha S

(Lab In-Charge)



## CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No: VI/20-21/1991-01

Page 2 of 2

Range: 5 - 50 $\mu$ l

**Results:**

Range	Cal Point	Volume observed	Expanded Uncertainty $\pm$
$\mu$ l	$\mu$ l	$\mu$ l	$\mu$ l
5 - 50 $\mu$ l	5.0	5.133	0.02
	20.0	20.367	0.04
	50.0	50.563	0.20


**Note:**

1. Visual Inspection : Found Well.
2. Tripple Distilled water is used to Calibrate the MicroPipette.


**Conclusion /Remarks:**

1. Ref. standard used are traceable to National/International Standard
2. The Expanded Uncertainty of associated with measurement at approximate 95.45% confidence level with coverage factor k=2

Calibrated By

  
Sameer M S  
(Calibration Engineer)

Checked By

  
Afjal Basha S  
(Lab In-Charge)



Authorized By

  
Gangadhar.C.K



COMMITTED TO THE  
CUSTOMER SINCE - 1996

# VAIDYANATHESHWARA INSTRUMENTS

## CERTIFICATE OF CALIBRATION



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Page 1 of 2

**1 Name and Address of the Customer** : M/s. FOSTR HEALTH CARE & DIAGNOSTICS.,  
No 12 , 2nd Floor, Panathur Main Road ,  
Panathur Bangalore - 560087.

**2 Customer Reference**

2.1 ULR No. : CC247320100021890F  
2.2 SRF No. : 1991  
2.4 Certificate No. : VI/20-21/1991-02  
2.6 Format No. : VI-FRM-ME-105  
2.7 Date Of Issue : 13-08-2020

**3 Details Of Device Under Calibration(DUC).**

3.1 Nomenclature : Pipette  
3.2 Make / Model : Thermo Scientific / Finnpiquette®F3  
3.3 Range : 10 - 100 µl  
3.4 SL No. : OW10740  
3.5 DUC Condition : Satisfactory  
3.6 Calibration Procedure No. : SM/WI/M-10 Based On ISO 8655-6:2002 E  
3.7 No.of Pages : 2  
3.8 Calibration Date : 13-08-2020  
3.9 Calibration Due : 12-08-2021  
3.10 Calibration done at : VI Volumetric Lab  
3.11 Discipline : Mechanical (Mass & volume)

**4 Environmental Condition**

Temperature 20.5 °C Humidity 53 %Rh

**5 Standards Used for calibration**

Sl. No.	Nomenclature	Make & Model	Sl. No	Range	Traceable to /Cert. No.	Validity
1	Digital Weighing Balance	RADWAG/MYA5.4Y	544953	0.1mg to 5g	VI/19-20/INT-ME-121	20-09-2020
2	E1 Class Weights	LCGC	VI-E1-ME-001	1mg to 200g	TVCSPL 19/04/339-01	02 - 04 - 2022

**6 Note:**

- 6.1. The Calibration Certificate relates only to the above DUC
- 6.2. Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab..
- 6.3. Corrections/erasing, invalidate the Calibration Certificate.
- 6.4. Calibration of the DUC are traceable to National standards/International Standards
- 6.5. Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6. Results Reported are valid at the time of and under the stated conditions of measurements
- 6.7. The usage of NABL symbol is as per NABL guidelines given in NABL-133.

Calibrated By  
*Sameer M S*  
Sameer M S  
(Calibration Engineer)

Checked By  
*Afjal Basha S*  
Afjal Basha S  
(Lab In-Charge)





## CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No: VI/20-21/1991-02

Page 2 of 2

Range: 10 - 100µl

### Results:

Range	Cal Point	Volume observed	Expanded Uncertainty ±
	µl	µl	µl
10 - 100µl	10.0	10.090	0.03
	50.0	49.956	0.20
	100.0	100.390	0.62

### Note:

1. Visual Inspection : Found Well.
2. Tripple Distilled water is used to Calibrate the MicroPipette.

### Conclusion /Remarks:


1. Ref. standard used are traceable to National/International Standard
2. The Expanded Uncertainty of associated with measurement at approximate 95.45% confidence level with coverage factor k=2

Calibrated By

Sameer M S  
(Calibration Engineer)

Checked By

Afjal Basha S  
(Lab In-Charge)

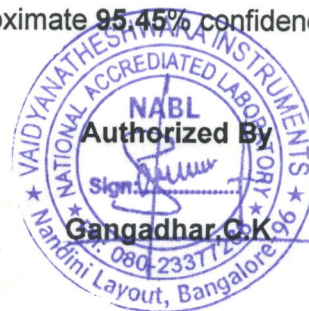



COMMITTED TO THE  
CUSTOMER SINCE - 1996

# VAIDYANATHESHWARA INSTRUMENTS

## CERTIFICATE OF CALIBRATION



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Page 1 of 2

**1 Name and Address of the Customer** : M/s. FOSTR HEALTH CARE & DIAGNOSTICS.,  
No 12 , 2nd Floor, Panathur Main Road ,  
Panathur Bangalore - 560087.

**2 Customer Reference**

2.1 ULR No. : CC247320100021891F  
2.2 SRF No. : 1991  
2.3 Certificate No. : VI/20-21/1991-03  
2.4 Format No. : VI-FRM-ME-105  
2.5 Date Of Issue : 13-08-2020

**3 Details Of Device Under Calibration(DUC).**

3.1 Nomenclature : Pipette  
3.2 Make / Model : Thermo Scientific / Finnpipette®F3  
3.3 Range : 100 - 1000 µl  
3.4 SL No. : OW09290  
3.5 DUC Condition : Satisfactory  
3.6 Calibration Procedure No. : SM/WI/M-10 Based On ISO 8655-6:2002 E  
3.7 No.of Pages : 2  
3.8 Calibration Date : 13-08-2020  
3.9 Calibration Due : 12-08-2021  
3.10 Calibration done at : VI Volumetric Lab  
3.11 Discipline : Mechanical (Mass & volume)

**4 Environmentel Condition**

Temperature 20.1 °C Humidity 55 %Rh

**5 Standards Used for calibration**

Sl. No.	Nomenclature	Make & Model	Sl. No	Range	Traceable to /Cert. No.	Validity
1	Digital Weighing Balance	RADWAG/MYA5.4Y	544953	0.1mg to 5g	Vi/19-20/INT-ME-121	20-09-2020
2	E1 Class Weights	LCGC	VI-E1-ME-001	1mg to 200g	TVC SPL 19/04/339-01	02 - 04 - 2022

**6 Note:**

- 6.1. The Calibration Certificate relates only to the above DUC
- 6.2. Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab..
- 6.3. Corrections/erasing, invalidate the Calibration Certificate.
- 6.4. Calibration of the DUC are traceable to National standards/International Standards
- 6.5. Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6. Results Reported are valid at the time of and under the stated conditions of measurements
- 6.7. The usage of NABL symbol is as per NABL guidelines given in NABL-133.

Calibrated By

*Sameer M S*

Sameer M S

(Calibration Engineer)

Checked By

*Afjal Basha S*

Afjal Basha S

(Lab In-Charge)





COMMITTED TO THE CUSTOMER SINCE - 1996

# Vaidyanatheshwara INSTRUMENTS

## CERTIFICATE OF CALIBRATION



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No: VI/20-21/1991-03

Page 2 of 2

Range: 100 - 1000µl

Results:

Range	Cal Point	Volume observed	Expanded Uncertainty ±
	µl	µl	µl
100 - 1000µl	100.0	99.897	0.62
	500.0	499.979	3.10
	1000.0	1000.150	6.20

**Note:**

1. Visual Inspection : Found Well.
2. Trippe Distilled water is used to Calibrate the MicroPipette.

**Conclusion /Remarks:**

1. Ref. standard used are traceable to National/International Standard
2. The Expanded Uncertainty of associated with measurement at approximate 95.45% confidence level with coverage factor k=2

Calibrated By

Sameer M S

(Calibration Engineer)

Checked By

Afjal Basha S

(Lab In-Charge)

Authorized By

Gangadhar.C.K

