

# AUSSIN (ASH) BIOMED CALIBRATION LABORATORY

508- DEV PRIME, B/H DIVYA BHASKAR PRESS, OFF S.G ROAD, AHMEDABAD, GUJARAT.

Ph. +91 9925063777, +91 9978163777

E-mail: monil.bmed@gmail.com

[www.ashbme.com](http://www.ashbme.com)



Calibrator machine is calibrated under NABL Laboratory.

## CERTIFICATE

CERTIFICATE /ID NO: ASH-5977

COMPANY / HOSPITAL: SANKALP LABORATORY.

ADDRESS: STATION ROAD, OPP. AKASH GANGA APPARTMENT, JAM-KHAMBHALIYA-361305.

DESCRIPTION OF INSTRUMENT: CENTRIFUGE MACHINE.

MAKE: REMI.

MODEL: C-854/6.

SR NO: ZGEN-10705.

LOCATION: LABORATORY.

TESTED BY: RAHUL PATEL

DATE OF CALIBRATION: 14/10/2020

NEXT CALIBRATION DATE: 13/10/2021

USE OF CALIBRATOR: RPM CALIBRATOR

USE OF CALIBRATOR	MAKE	MODEL	SR NO
DIGITAL TECO METER	LUTRON	DT 2234C	S015345

### A: CALIBRATION DATA:

Standard RPM	UUC* RPM	Error RPM	Uncertainty $\pm 3\%$
1000	1001	1	$\pm 3\%$
2000	2002	2	$\pm 3\%$
3000	2997	-3	$\pm 3\%$
4000	4002	2	$\pm 3\%$


\* Mean of Five readings

Note: The indicated Uncertainties are estimated expanded Uncertainties for

Coverage factor 'k'=2 providing a level of confidence approx. = 95% for distribution

CALIBRATED/TESTED BY:

DATE: 16/10/2020

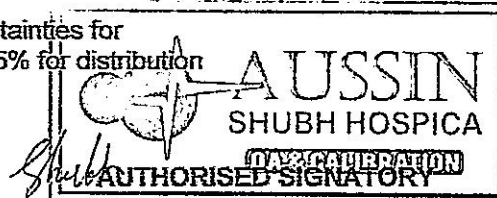

The calibration results reported in this certificate are valid at the time of and under the stated conditions of measurement. This report is not to be used to claim product endorsement by Aussin any agency. This document shall not be reproduced, except in full, without the written approval of Aussin. This is for technical information of the client only and not for advertisement, promotion, publicity of litigation.