

Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 1
Sample Date : 28-12-2020


Biochemistry, Albumin, g/dL

	N	Mean	SD	CV%	Excluded
All Methods	144	3.96	0.42	10.66	3
Bromcresol Green (BCG)	140	3.96	0.42	10.67	3
Erba EM 200	4	3.39	0.14	4.22	--

Your Result	3.20	SDI / z-Score	-1.84
Assigned Value	3.71	Average SDI	-1.79
SDPA	0.278	Uncertainty of AV	0.02
Standard Unit Result Val	3.20	%DEV	-19.13

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

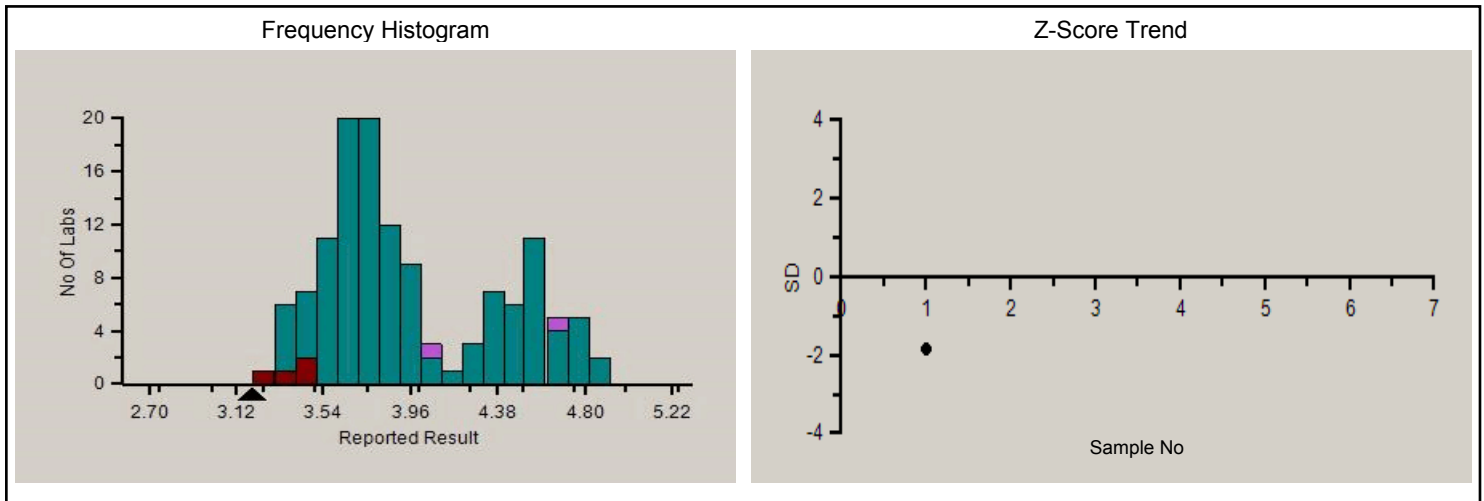

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 1
Sample Date : 28-12-2020

Biochemistry, Albumin		N	Mean	SD	CV%	Excluded
	All Analyzer	144	3.96	0.42	10.66	3
Your Analyzer :	Erba EM 200	4	3.39	0.14	4.22	--
	Fuji Dri-Chem NX500/i	26	4.56	0.20	4.43	1
	Roche cobas c 311	26	3.77	0.09	2.39	1
	Fuji Dri-Chem 4000i	15	4.55	0.19	4.06	--
	Horiba ABX Pentra C200	11	3.62	0.15	4.09	--
	Roche cobas c 111	10	3.78	0.15	4.04	--
	Roche cobas INTEGRA	10	3.77	0.12	3.13	--
	Roche cobas 6000	7	3.77	0.11	2.94	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 1
Sample Date : 28-12-2020


Biochemistry, ALP, U/L

	N	Mean	SD	CV%	Excluded
All Methods	142	85.45	13.80	16.15	8
PNPP, AMP Buffer	64	92.63	15.47	16.70	3
Star 20	1	--	--	--	--

Your Result	77.10	SDI / z-Score	-0.11
Assigned Value	78.40	Average SDI	0.42
SDPA	11.759	Uncertainty of AV	0.78
Standard Unit Result Val	77.10	%DEV	-16.76

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

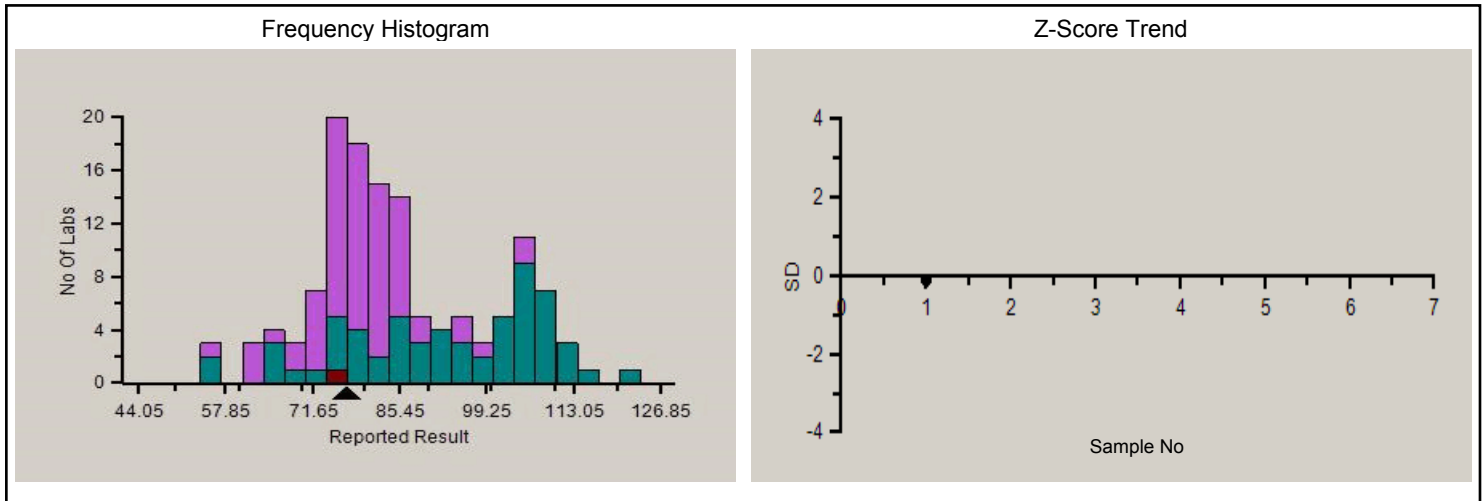

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 361
 Lab Name : SANJEEVANI LABORATORY
 Report Date : 14/01/2021

Cycle No : 200312
 Sample No : 1
 Sample Date : 28-12-2020

Biochemistry, ALP		N	Mean	SD	CV%	Excluded
	All Analyzer	142	85.45	13.80	16.15	8
Your Analyzer :	Star 20	1	--	--	--	--
	Roche cobas c 311	26	79.46	3.56	4.48	--
	Fuji Dri-Chem NX500/i	25	104.72	6.06	5.79	--
	Fuji Dri-Chem 4000i	15	99.79	10.45	10.48	1
	Horiba ABX Pentra C200	12	75.00	9.59	12.78	1
	Roche cobas c 111	11	75.15	6.77	9.01	1
	Roche cobas INTEGRA	10	78.97	8.02	10.16	--
	Roche cobas 6000	7	81.29	4.19	5.16	--
	Roche cobas 8000	4	81.50	1.73	2.13	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 1
Sample Date : 28-12-2020


Biochemistry, ALT, U/L

	N	Mean	SD	CV%	Excluded
All Methods	144	23.45	11.24	47.91	26
IFCC-Kinetic	5	17.76	0.50	2.82	2
Erba EM 200	4	19.15	1.20	6.28	2

Your Result	18.30	SDI / z-Score	0.10
Assigned Value	17.95	Average SDI	0.01
SDPA	3.590	Uncertainty of AV	0.83
Standard Unit Result Val	18.30	%DEV	3.02

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

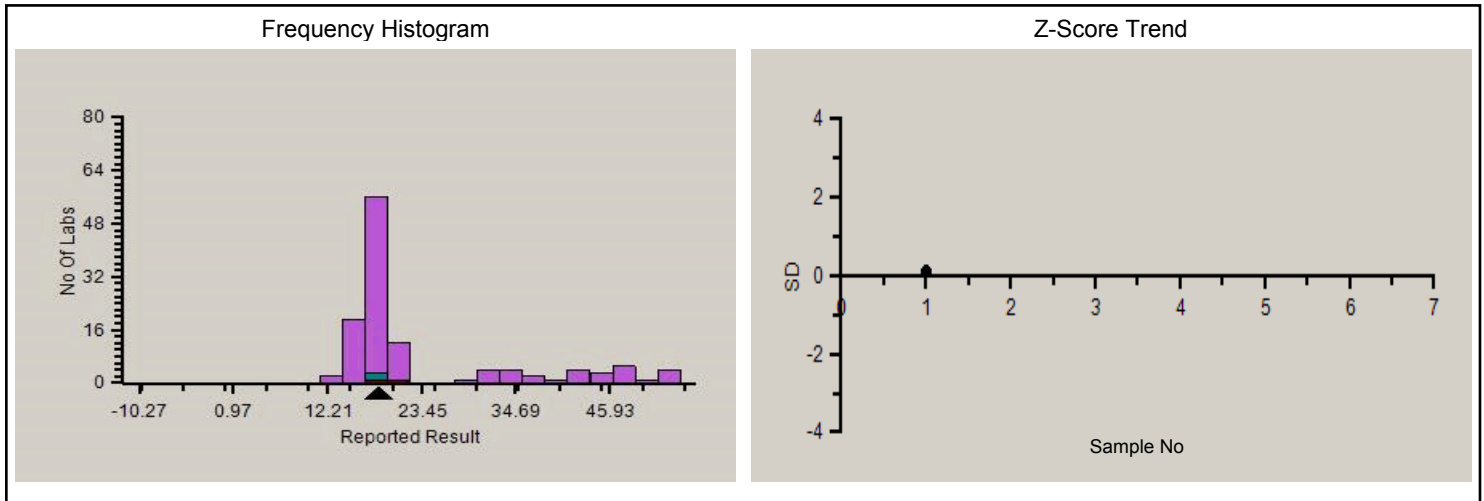

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 1
Sample Date : 28-12-2020

Biochemistry, ALT		N	Mean	SD	CV%	Excluded
	All Analyzer	144	23.45	11.24	47.91	26
Your Analyzer :	Erba EM 200	4	19.15	1.20	6.28	2
	Fuji Dri-Chem NX500/i	25	42.41	8.25	19.45	8
	Roche cobas c 311	25	17.50	1.64	9.38	--
	Fuji Dri-Chem 4000i	15	41.33	6.75	16.32	6
	Horiba ABX Pentra C200	12	18.05	1.80	9.95	--
	Roche cobas c 111	11	17.13	1.28	7.45	--
	Roche cobas INTEGRA	10	16.71	1.26	7.53	--
	Roche cobas 6000	7	17.26	0.51	2.97	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 1
Sample Date : 28-12-2020


Biochemistry, Amylase, IU/L

	N	Mean	SD	CV%	Excluded
■ All Methods	88	68.42	8.23	12.03	5
■ Gal-G2 CNP	4	79.44	13.28	16.72	1
■ Star 20	1	--	--	--	--

Your Result	94.10	SDI / z-Score	2.19
Assigned Value	74.54	Average SDI	0.08
SDPA	8.944	Uncertainty of AV	0.58
Standard Unit Result Val	94.10	%DEV	18.46

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

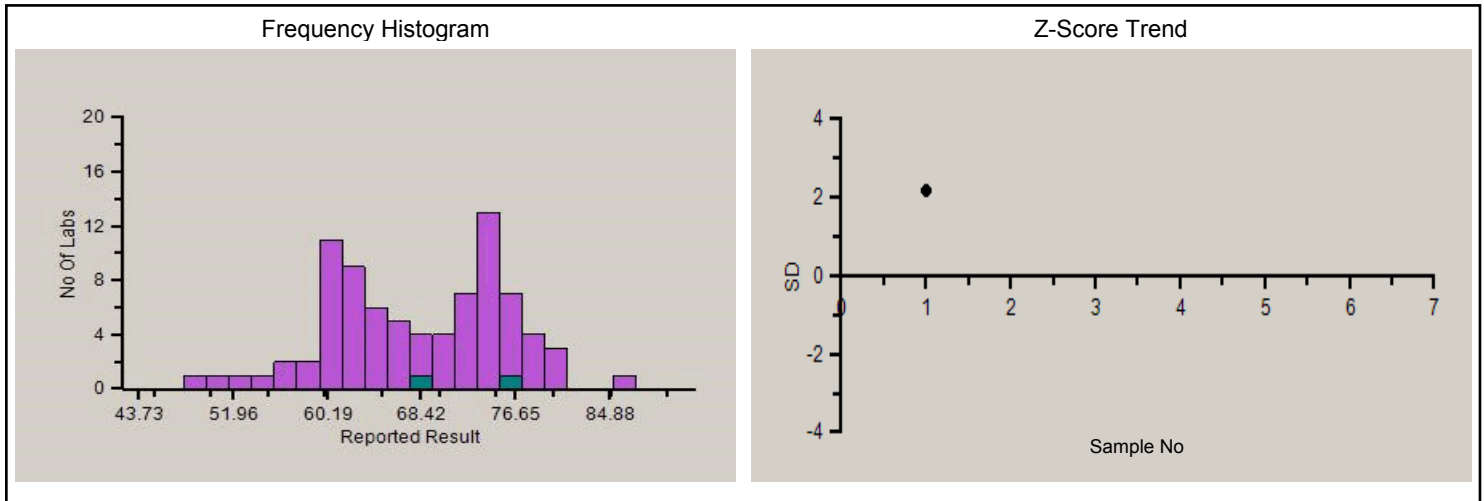

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 361
 Lab Name : SANJEEVANI LABORATORY
 Report Date : 14/01/2021

Cycle No : 200312
 Sample No : 1
 Sample Date : 28-12-2020

Biochemistry, Amylase		N	Mean	SD	CV%	Excluded
	All Analyzer	88	68.42	8.23	12.03	5
Your Analyzer :	Star 20	1	--	--	--	--
	Fuji Dri-Chem NX500/i	18	62.65	3.79	6.05	1
	Fuji Dri-Chem 4000i	14	61.86	2.32	3.74	--
	Roche cobas c 311	12	75.56	1.92	2.54	--
	Roche cobas INTEGRA	7	73.05	1.61	2.21	--
	Roche cobas 6000	6	74.18	2.54	3.42	--
	Roche cobas 8000	4	74.50	0.58	0.77	--
	Roche cobas c 111	4	77.30	6.61	8.56	--
	Horiba ABX Pentra C200	3	74.10	8.34	11.26	1

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 1
Sample Date : 28-12-2020


Biochemistry, AST, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	145	23.81	3.93	16.51	30
■ IFCC-Kinetic	5	27.13	3.70	13.62	2
■ Erba EM 200	4	24.00	0.00	0.00	3

Your Result	14.90	SDI / z-Score	-1.69
Assigned Value	25.71	Average SDI	-0.23
SDPA	6.394	Uncertainty of AV	2.14
Standard Unit Result Val	14.90	%DEV	-45.09

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

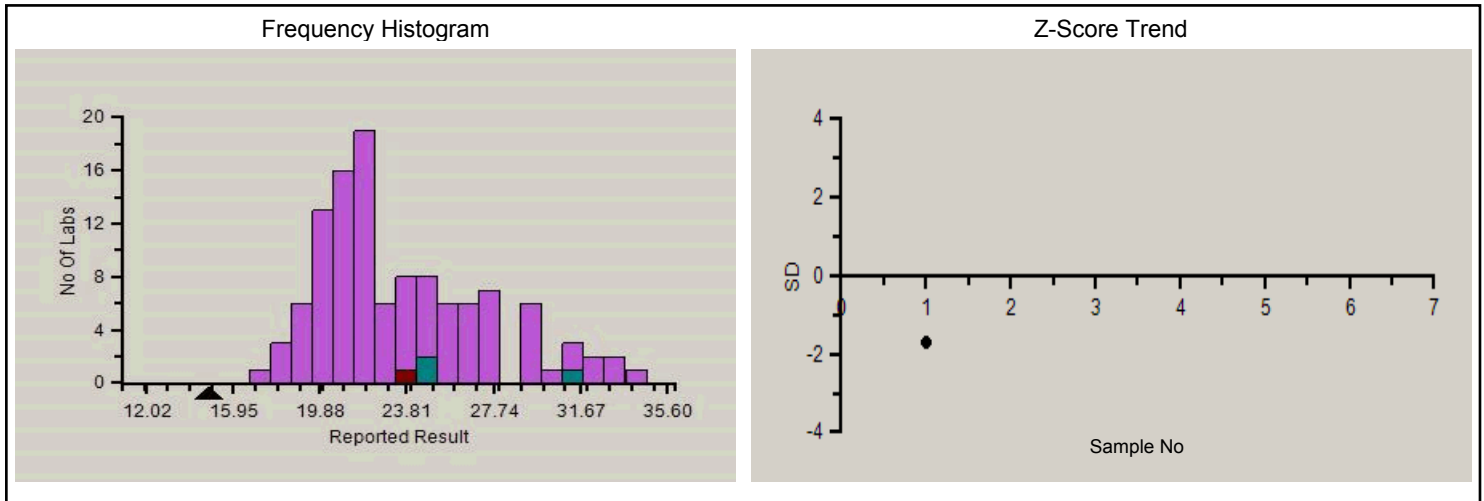

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 1
Sample Date : 28-12-2020

Biochemistry, AST		N	Mean	SD	CV%	Excluded
	All Analyzer	145	23.81	3.93	16.51	30
Your Analyzer :	Erba EM 200	4	24.00	0.00	0.00	3
	Fuji Dri-Chem NX500/i	26	29.56	2.97	10.03	10
	Roche cobas c 311	25	21.56	2.44	11.30	--
	Fuji Dri-Chem 4000i	15	27.11	3.55	13.10	6
	Roche cobas c 111	12	23.48	2.53	10.79	1
	Horiba ABX Pentra C200	11	22.05	2.42	10.99	--
	Roche cobas INTEGRA	10	20.81	1.25	5.99	--
	Roche cobas 6000	7	21.66	1.70	7.85	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 1
Sample Date : 28-12-2020


Biochemistry, Bilirubin Direct, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	143	0.10	0.02	17.82	34
Diazotization	115	0.10	0.02	16.16	24
Erba EM 200	4	0.11	0.03	26.36	--

Your Result	0.15	SDI / z-Score	0.42
Assigned Value	0.12	Average SDI	0.43
SDPA	0.067	Uncertainty of AV	0.01
Standard Unit Result Val	0.15	%DEV	51.52

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

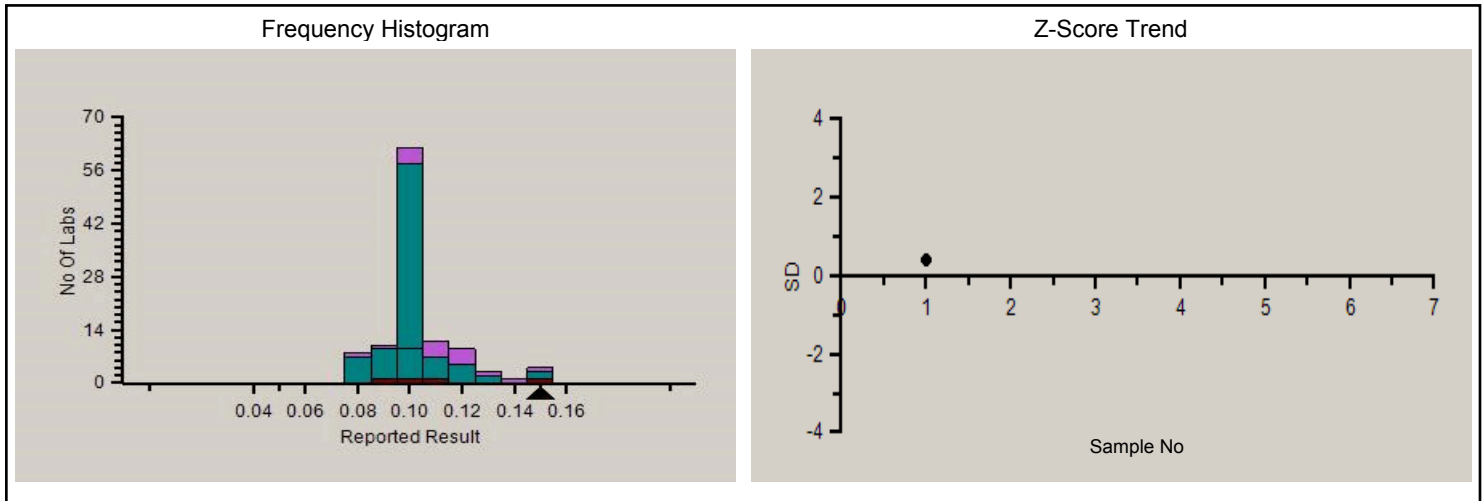

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 361
 Lab Name : SANJEEVANI LABORATORY
 Report Date : 14/01/2021

Cycle No : 200312
 Sample No : 1
 Sample Date : 28-12-2020

Biochemistry, Bilirubin Direct		N	Mean	SD	CV%	Excluded
	All Analyzer	143	0.10	0.02	17.82	34
Your Analyzer :	Erba EM 200	4	0.11	0.03	26.36	--
	Fuji Dri-Chem NX500/i	25	0.10	0.00	0.00	8
	Roche cobas c 311	24	0.09	0.02	16.67	3
	Fuji Dri-Chem 4000i	15	0.10	0.00	0.00	7
	Horiba ABX Pentra C200	12	0.12	0.02	13.22	--
	Roche cobas c 111	11	0.10	0.01	11.11	1
	Roche cobas INTEGRA	10	0.11	0.01	12.38	--
	Roche cobas 6000	7	0.10	0.01	4.85	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 1
Sample Date : 28-12-2020


Biochemistry, Bilirubin Total, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	144	0.33	0.13	38.55	27
■ Diazotization	36	0.29	0.08	27.21	7
■ Erba EM 200	4	0.25	0.05	21.63	--

Your Result	0.28	SDI / z-Score	0.98
Assigned Value	0.24	Average SDI	0.78
SDPA	0.043	Uncertainty of AV	0.01
Standard Unit Result Val	0.28	%DEV	-4.76

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

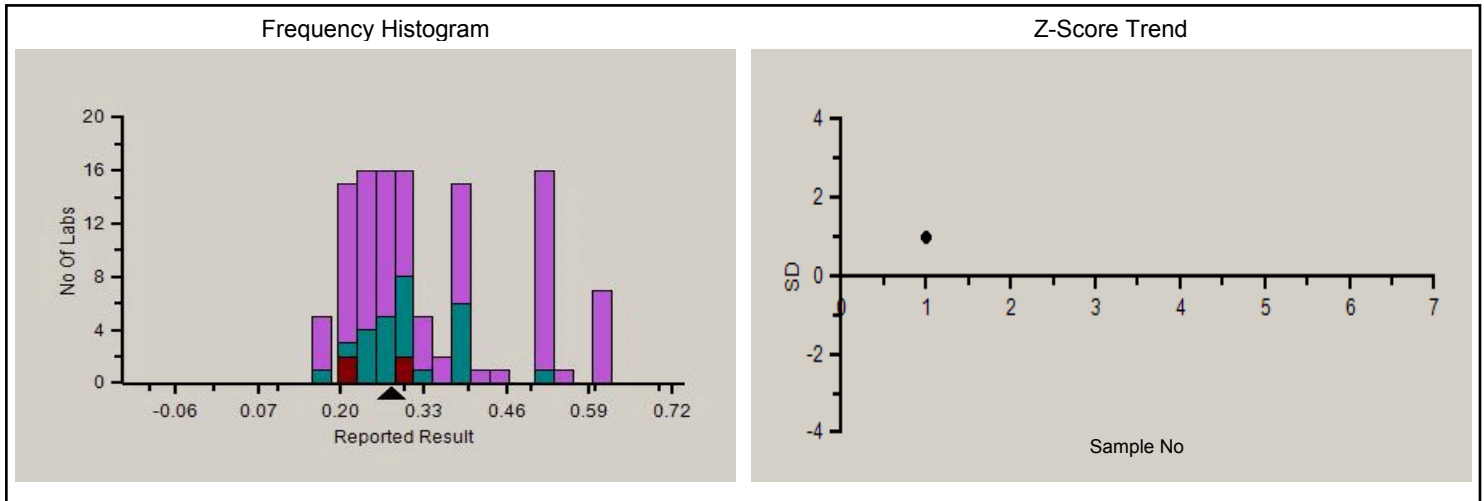

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
 Lab Name : SANJEEVANI LABORATORY
 Report Date : 14/01/2021

Cycle No : 200312
 Sample No : 1
 Sample Date : 28-12-2020

Biochemistry, Bilirubin Total		N	Mean	SD	CV%	Excluded
	All Analyzer	144	0.33	0.13	38.55	27
Your Analyzer :	Erba EM 200	4	0.25	0.05	21.63	--
	Fuji Dri-Chem NX500/i	26	0.47	0.06	12.13	6
	Roche cobas c 311	25	0.24	0.04	14.40	2
	Fuji Dri-Chem 4000i	15	0.49	0.09	18.66	1
	Horiba ABX Pentra C200	11	0.29	0.03	11.60	4
	Roche cobas c 111	10	0.23	0.06	24.23	3
	Roche cobas INTEGRA	10	0.21	0.03	12.14	--
	Roche cobas 6000	7	0.22	0.02	9.38	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 1
Sample Date : 28-12-2020


Biochemistry, Calcium, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	137	7.82	0.57	7.31	2
Arsenazo III	39	8.02	0.61	7.60	1
Star 20	2	8.01	--	--	--

Your Result	9.10	SDI / z-Score	0.87
Assigned Value	8.20	Average SDI	0.64
SDPA	1.035	Uncertainty of AV	0.46
Standard Unit Result Val	9.10	%DEV	13.51

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

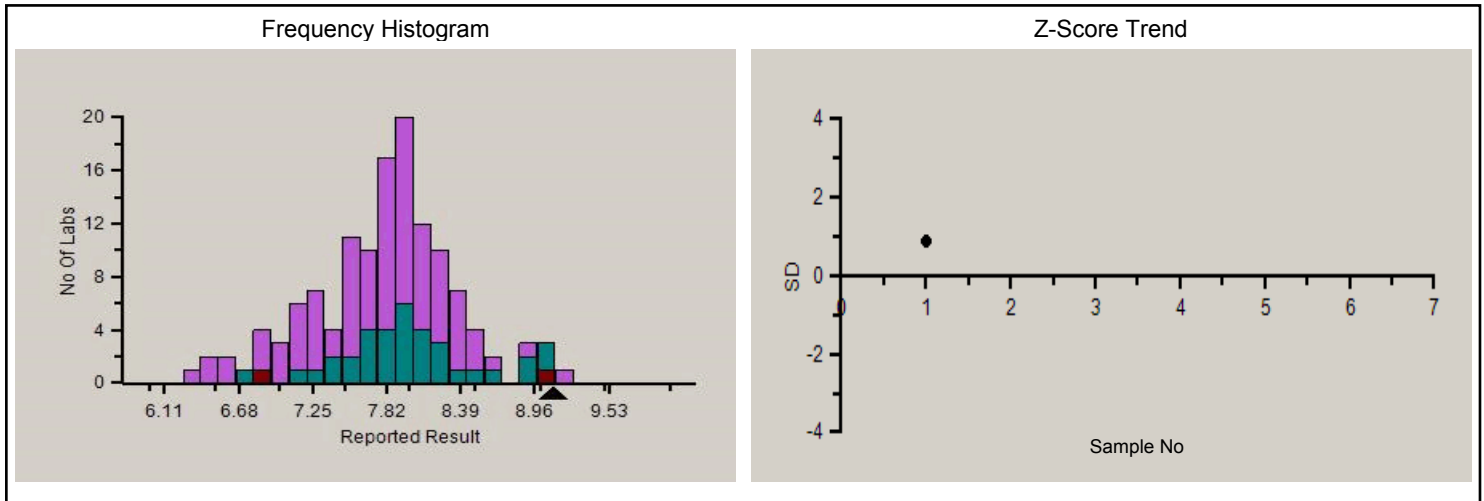

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
 Lab Name : SANJEEVANI LABORATORY
 Report Date : 14/01/2021

Cycle No : 200312
 Sample No : 1
 Sample Date : 28-12-2020

Biochemistry, Calcium		N	Mean	SD	CV%	Excluded
	All Analyzer	137	7.82	0.57	7.31	2
Your Analyzer :	Star 20	2	8.01	--	--	--
	Fuji Dri-Chem NX500/i	24	7.20	0.40	5.59	--
	Roche cobas c 311	24	8.11	0.30	3.74	--
	Fuji Dri-Chem 4000i	16	7.33	0.49	6.72	1
	Roche cobas c 111	12	7.98	0.28	3.51	--
	Roche cobas INTEGRA	11	7.94	0.20	2.52	--
	Horiba ABX Pentra C200	7	8.04	0.36	4.43	--
	Roche cobas 6000	6	7.95	0.06	0.69	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 1
Sample Date : 28-12-2020


Biochemistry, CK, U/L

	N	Mean	SD	CV%	Excluded
All Methods	63	98.47	16.40	16.66	2
NAC activated	30	110.23	11.16	10.13	1
Star 20	1	--	--	--	--

Your Result	85.30	SDI / z-Score	-2.26
Assigned Value	110.22	Average SDI	-3.75
SDPA	11.022	Uncertainty of AV	0.93
Standard Unit Result Val	85.30	%DEV	-22.61

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

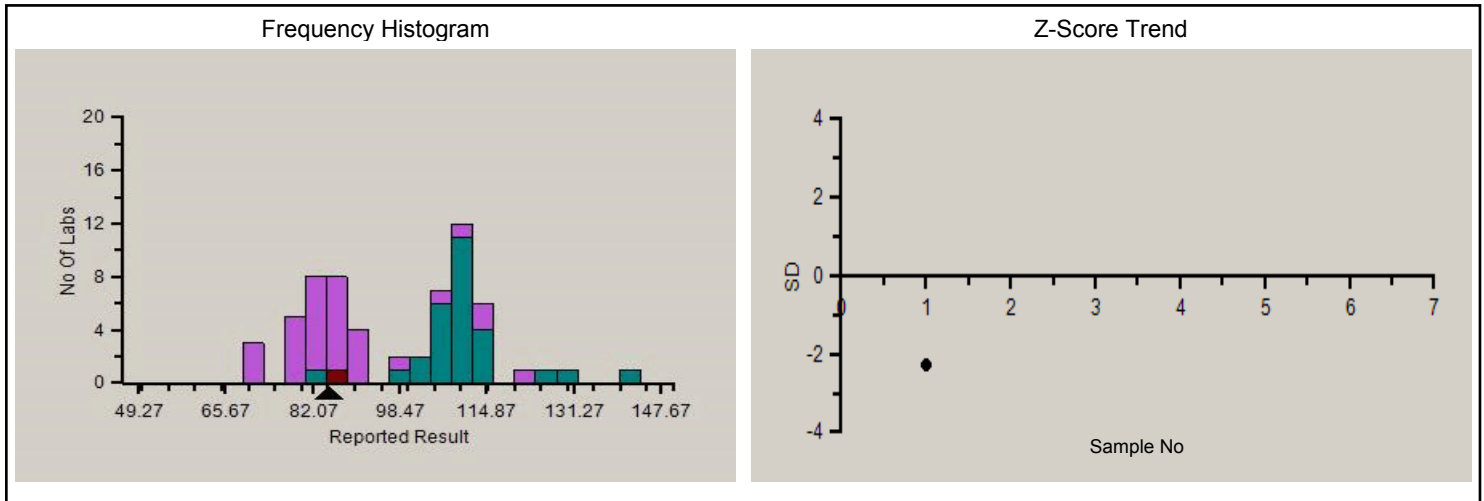

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 361
 Lab Name : SANJEEVANI LABORATORY
 Report Date : 14/01/2021

Cycle No : 200312
 Sample No : 1
 Sample Date : 28-12-2020

Biochemistry, CK		N	Mean	SD	CV%	Excluded
	All Analyzer	63	98.47	16.40	16.66	2
Your Analyzer :	Star 20	1	--	--	--	--
	Fuji Dri-Chem NX500/i	13	82.58	7.09	8.59	1
	Fuji Dri-Chem 4000i	12	84.08	7.04	8.37	--
	Roche cobas c 311	11	113.09	6.33	5.60	--
	Roche cobas INTEGRA	7	107.65	4.95	4.60	--
	Roche cobas 6000	4	110.50	1.00	0.91	--
	Roche cobas 8000	4	115.25	7.46	6.47	--
	Fuji Nx 700	3	81.67	2.89	3.54	--
	Horiba ABX Pentra C200	2	129.10	--	--	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 1
Sample Date : 28-12-2020


Biochemistry, LDH, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	72	146.99	24.00	16.33	9
■ IFCC	4	149.50	33.23	22.23	2
■ Erba EM 200	1	--	--	--	1

Your Result	312.80	SDI / z-Score	-1.04
Assigned Value	325.90	Average SDI	-1.09
SDPA	12.604	Uncertainty of AV	7.88
Standard Unit Result Val	312.80	%DEV	109.23

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

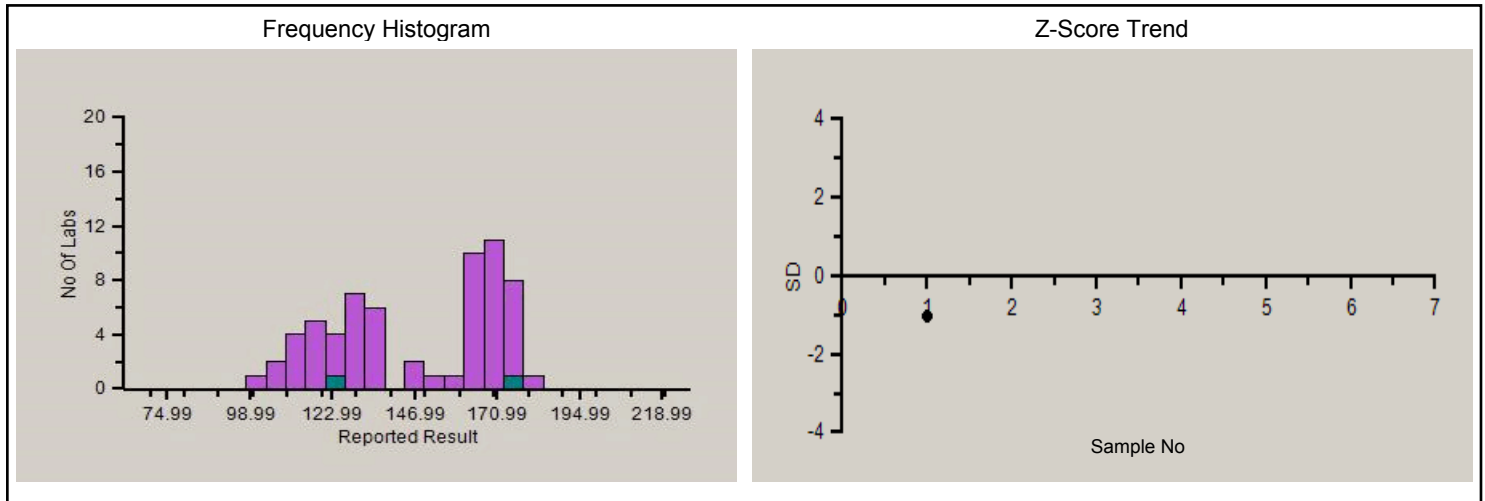

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 361
 Lab Name : SANJEEVANI LABORATORY
 Report Date : 14/01/2021

Cycle No : 200312
 Sample No : 1
 Sample Date : 28-12-2020

Biochemistry, LDH		N	Mean	SD	CV%	Excluded
	All Analyzer	72	146.99	24.00	16.33	9
Your Analyzer :	Erba EM 200	1	--	--	--	1
	Fuji Dri-Chem NX500/i	16	121.81	9.51	7.81	--
	Fuji Dri-Chem 4000i	11	125.55	11.73	9.35	--
	Roche cobas c 311	10	170.20	3.74	2.20	--
	Roche cobas INTEGRA	7	163.31	7.14	4.37	--
	Roche cobas 6000	5	166.20	8.87	5.34	--
	Roche cobas 8000	4	170.00	2.16	1.27	--
	Horiba ABX Pentra C200	3	--	--	--	3
	Fuji Nx 700	3	126.00	7.21	5.72	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 1
Sample Date : 28-12-2020


Biochemistry, Potassium, mEq/L

	N	Mean	SD	CV%	Excluded
■ All Methods	126	5.67	0.94	16.50	3
■ Colorimetric	3	3.87	0.32	8.30	--
■ Star 20	1	--	--	--	--

Your Result	3.50	SDI / z-Score	-2.54
Assigned Value	4.26	Average SDI	-2.58
SDPA	0.298	Uncertainty of AV	0.03
Standard Unit Result Val	3.50	%DEV	-9.49

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

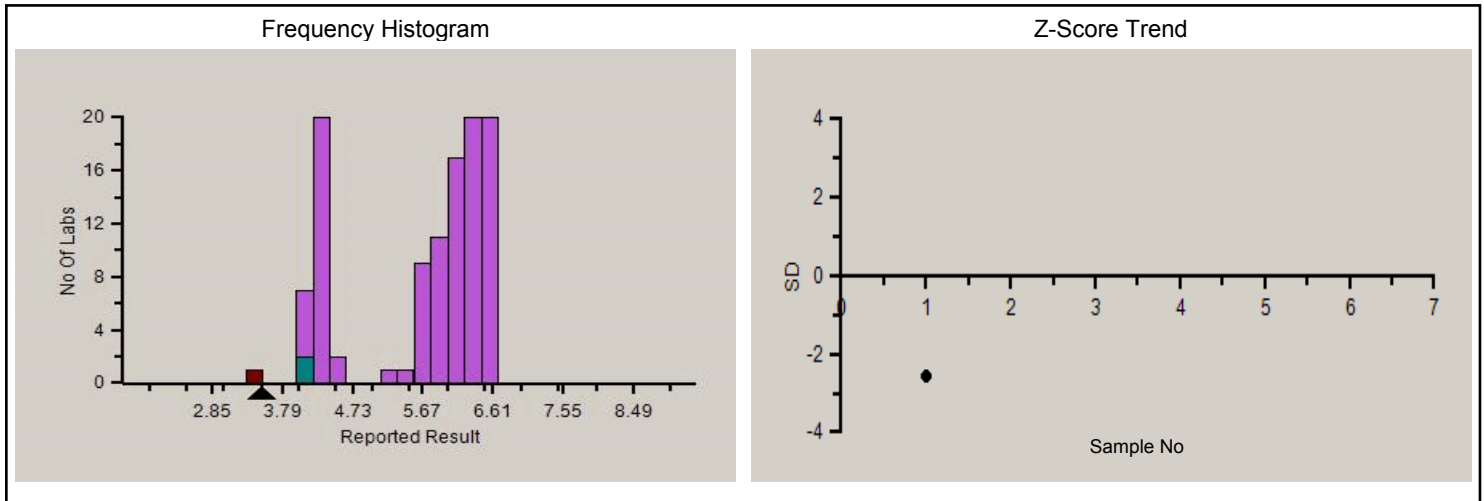

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
 Lab Name : SANJEEVANI LABORATORY
 Report Date : 14/01/2021

Cycle No : 200312
 Sample No : 1
 Sample Date : 28-12-2020

Biochemistry, Potassium		N	Mean	SD	CV%	Excluded
	All Analyzer	126	5.67	0.94	16.50	3
Your Analyzer :	Star 20	1	--	--	--	--
	Fuji Dri-Chem NX500/i	25	6.43	0.10	1.53	--
	Fuji Dri-Chem 4000i	17	6.32	0.22	3.47	--
	Roche cobas c 311	13	4.26	0.09	2.21	--
	EasyLyte	12	5.77	0.13	2.20	--
	Roche AVL 9180	11	6.50	0.09	1.37	--
	Roche cobas 6000	7	4.30	0.11	2.58	--
	Roche cobas 8000	4	4.18	0.05	1.12	--
	Roche cobas INTEGRA	4	4.39	0.07	1.50	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 1
Sample Date : 28-12-2020


Biochemistry, Sodium, mEq/L

	N	Mean	SD	CV%	Excluded
■ All Methods	126	157.26	22.66	14.41	3
■ Colorimetric	3	131.17	6.53	4.98	--
■ Star 20	1	--	--	--	--

Your Result	130.50	SDI / z-Score	1.53
Assigned Value	121.23	Average SDI	1.67
SDPA	6.062	Uncertainty of AV	0.47
Standard Unit Result Val	130.50	%DEV	-0.51

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

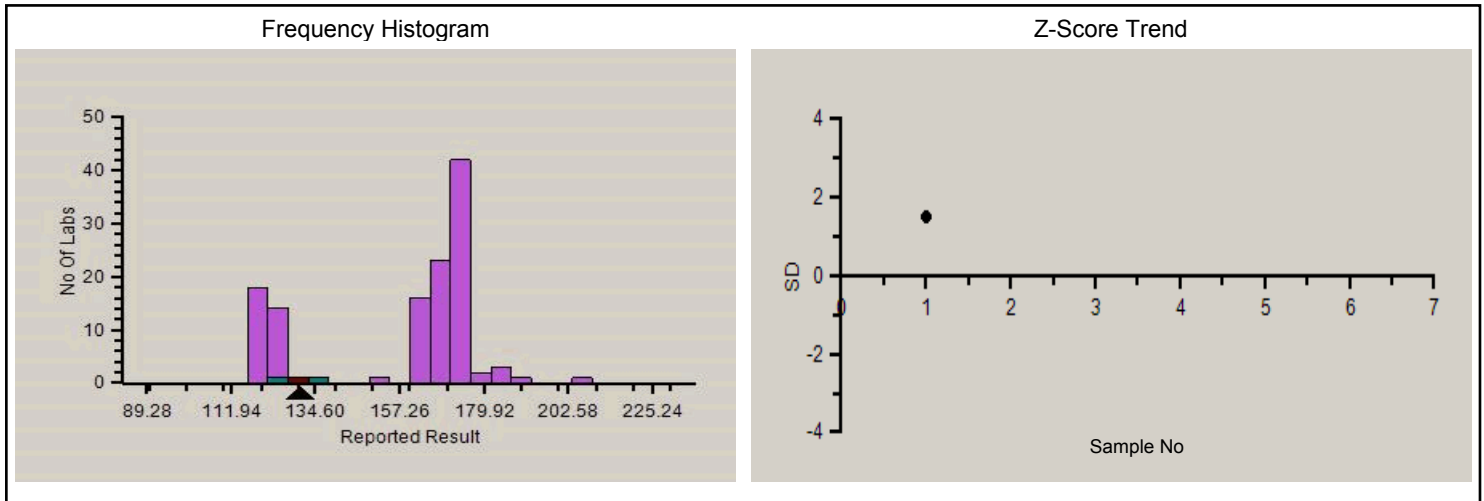

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 361
 Lab Name : SANJEEVANI LABORATORY
 Report Date : 14/01/2021

Cycle No : 200312
 Sample No : 1
 Sample Date : 28-12-2020

Biochemistry, Sodium		N	Mean	SD	CV%	Excluded
	All Analyzer	126	157.26	22.66	14.41	3
Your Analyzer :	Star 20	1	--	--	--	--
	Fuji Dri-Chem NX500/i	26	171.08	3.95	2.31	--
	Fuji Dri-Chem 4000i	16	169.88	4.49	2.64	--
	Roche cobas c 311	13	120.62	1.26	1.05	--
	EasyLyte	12	164.79	3.60	2.19	--
	Roche AVL 9180	11	175.13	3.52	2.01	--
	Roche cobas 6000	7	120.86	2.19	1.82	--
	Roche cobas 8000	4	120.75	2.87	2.38	--
	Roche cobas INTEGRA	4	124.16	1.83	1.48	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 1
Sample Date : 28-12-2020


Biochemistry, Total Protein, g/L

	N	Mean	SD	CV%	Excluded
■ All Methods	143	6.37	0.29	4.54	3
■ Biuret	140	6.37	0.29	4.57	2
■ Erba EM 200	4	6.58	0.38	5.79	1

Your Result	5.87	SDI / z-Score	*
Assigned Value	6.29	Average SDI	0.00
SDPA	0.247	Uncertainty of AV	0.03
Standard Unit Result Val	0.59	%DEV	-90.74

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

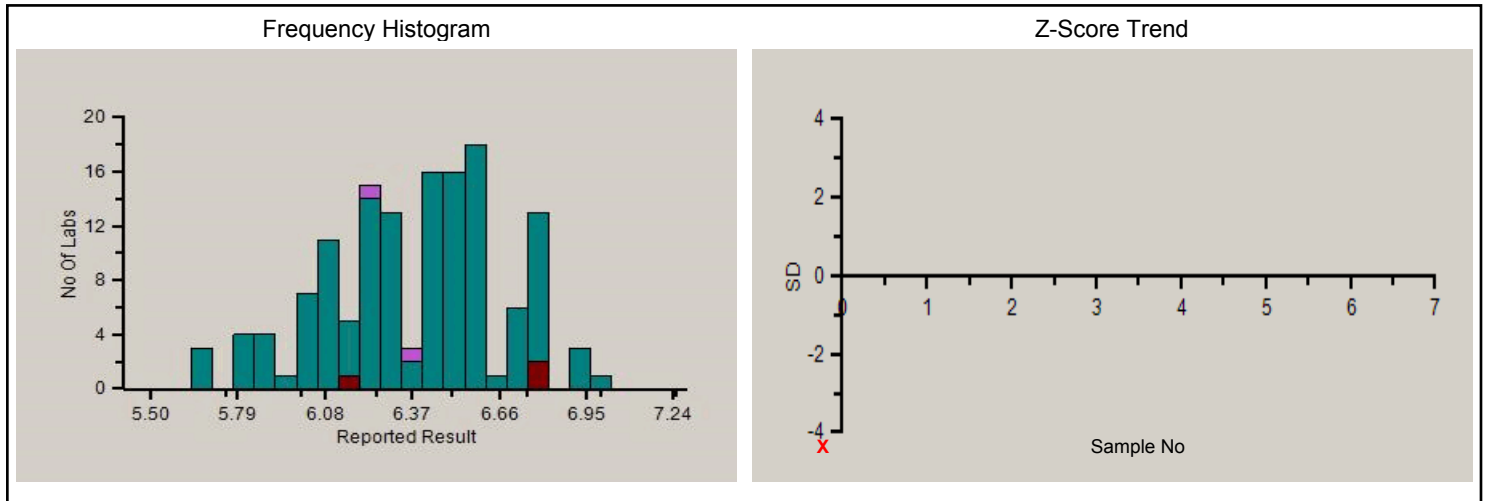

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 361
 Lab Name : SANJEEVANI LABORATORY
 Report Date : 14/01/2021

Cycle No : 200312
 Sample No : 1
 Sample Date : 28-12-2020

Biochemistry, Total Protein		N	Mean	SD	CV%	Excluded
	All Analyzer	143	6.37	0.29	4.54	3
Your Analyzer :	Erba EM 200	4	6.58	0.38	5.79	1
	Fuji Dri-Chem NX500/i	26	6.63	0.19	2.85	--
	Roche cobas c 311	26	6.37	0.14	2.26	--
	Fuji Dri-Chem 4000i	15	6.61	0.20	3.07	--
	Roche cobas c 111	11	6.32	0.27	4.32	--
	Horiba ABX Pentra C200	10	6.10	0.24	3.88	--
	Roche cobas INTEGRA	10	5.99	0.19	3.21	--
	Roche cobas 6000	7	6.31	0.07	1.05	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 1
Sample Date : 28-12-2020


Biochemistry, Triglycerides, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	144	128.34	9.45	7.37	4
■ GPO - Peroxidase	9	122.11	10.31	8.45	--
■ Erba EM 200	4	124.80	16.99	13.62	--

Your Result	124.50	SDI / z-Score	0.29
Assigned Value	120.25	Average SDI	0.22
SDPA	14.604	Uncertainty of AV	4.88
Standard Unit Result Val	124.50	%DEV	1.96

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

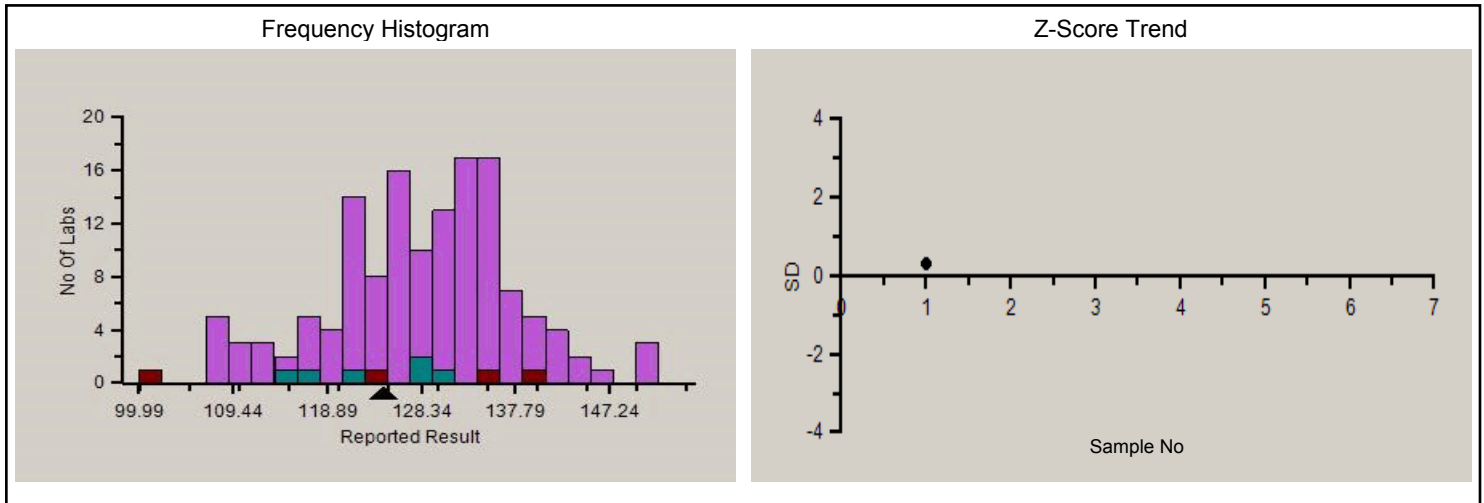

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 361
 Lab Name : SANJEEVANI LABORATORY
 Report Date : 14/01/2021

Cycle No : 200312
 Sample No : 1
 Sample Date : 28-12-2020

Biochemistry, Triglycerides		N	Mean	SD	CV%	Excluded
	All Analyzer	144	128.34	9.45	7.37	4
Your Analyzer :	Erba EM 200	4	124.80	16.99	13.62	--
	Fuji Dri-Chem NX500/i	26	120.39	6.34	5.27	--
	Roche cobas c 311	26	134.25	4.38	3.26	--
	Fuji Dri-Chem 4000i	15	119.57	8.01	6.70	1
	Roche cobas c 111	12	135.90	7.62	5.60	--
	Horiba ABX Pentra C200	11	128.70	5.21	4.05	--
	Roche cobas INTEGRA	10	129.77	4.13	3.18	--
	Roche cobas 6000	7	132.43	2.76	2.08	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 1
Sample Date : 28-12-2020


Biochemistry, Uric Acid, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	144	4.22	0.32	7.55	4
Uricase - POD	19	4.28	0.30	7.06	3
Erba EM 200	4	4.43	0.47	10.67	1

Your Result	4.80	SDI / z-Score	0.32
Assigned Value	4.62	Average SDI	0.32
SDPA	0.553	Uncertainty of AV	0.18
Standard Unit Result Val	4.80	%DEV	12.15

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

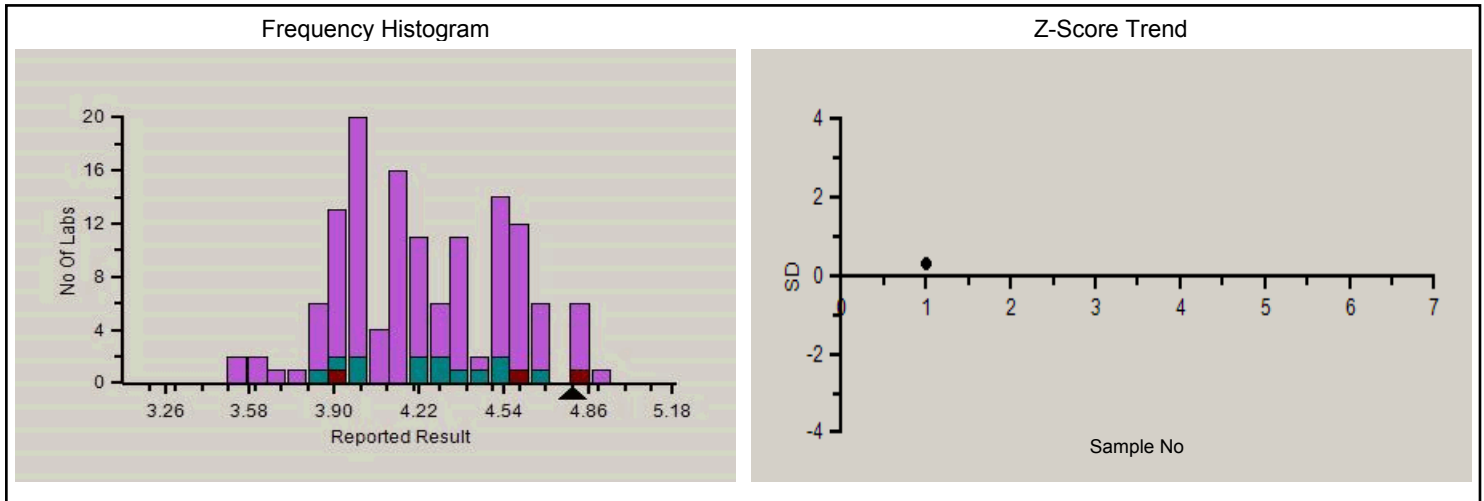

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
 Lab Name : SANJEEVANI LABORATORY
 Report Date : 14/01/2021

Cycle No : 200312
 Sample No : 1
 Sample Date : 28-12-2020

Biochemistry, Uric Acid		N	Mean	SD	CV%	Excluded
	All Analyzer	144	4.22	0.32	7.55	4
Your Analyzer :	Erba EM 200	4	4.43	0.47	10.67	1
	Fuji Dri-Chem NX500/i	25	4.46	0.26	5.85	--
	Roche cobas c 311	24	4.01	0.12	3.09	--
	Fuji Dri-Chem 4000i	18	4.48	0.27	5.91	1
	Roche cobas c 111	11	3.96	0.20	4.95	--
	Horiba ABX Pentra C200	10	4.05	0.19	4.57	--
	Roche cobas INTEGRA	10	4.07	0.19	4.64	--
	Roche cobas 6000	7	3.90	0.20	5.13	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
 Unit No. 409-416.
 Commercial Building - 1A,
 Kohinoor Mall, Kirool Road, Kuria (W),
 Mumbai - 400070



PC-1022