

Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 3
Sample Date : 28-12-2020


Biochemistry, Cholesterol, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	142	149.32	7.88	5.28	8
CHOD-PAP	28	152.47	8.11	5.32	5
Erba EM 200	3	148.67	7.02	4.73	--

Your Result	148.00	SDI / z-Score	-0.24
Assigned Value	150.15	Average SDI	-0.24
SDPA	9.008	Uncertainty of AV	0.66
Standard Unit Result Val	148.00	%DEV	-2.93

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

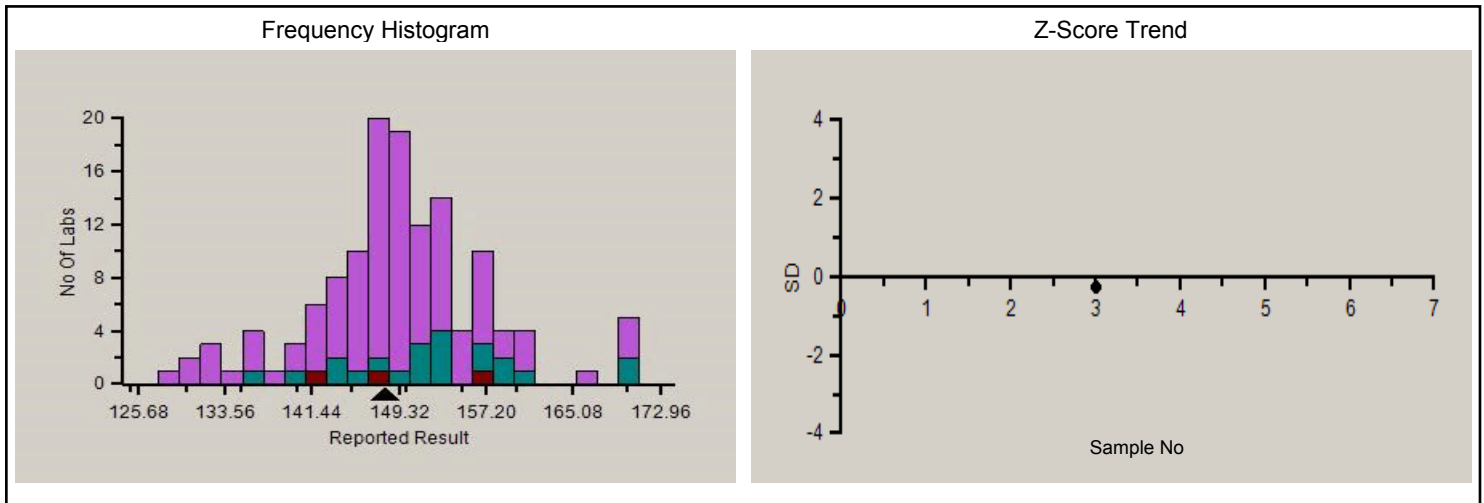

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
 Lab Name : SANJEEVANI LABORATORY
 Report Date : 14/01/2021

Cycle No : 200312
 Sample No : 3
 Sample Date : 28-12-2020

Biochemistry, Cholesterol		N	Mean	SD	CV%	Excluded
	All Analyzer	142	149.32	7.88	5.28	8
Your Analyzer :	Erba EM 200	3	148.67	7.02	4.73	--
	Roche cobas c 311	26	151.32	3.79	2.51	--
	Fuji Dri-Chem NX500/i	24	143.61	7.70	5.36	1
	Fuji Dri-Chem 4000i	15	143.67	8.17	5.68	--
	Roche cobas c 111	12	147.80	5.51	3.73	--
	Horiba ABX Pentra C200	11	152.82	5.54	3.62	3
	Roche cobas INTEGRA	10	148.87	2.62	1.76	--
	Roche cobas 6000	7	149.14	3.13	2.10	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 3
Sample Date : 28-12-2020


Biochemistry, Creatinine, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	146	0.55	0.19	33.94	13
■ Enzymatic	12	0.58	0.15	26.56	1
■ Erba EM 200	4	0.67	0.04	5.37	--

Your Result	0.63	SDI / z-Score	-0.01
Assigned Value	0.63	Average SDI	0.07
SDPA	0.088	Uncertainty of AV	0.01
Standard Unit Result Val	0.63	%DEV	9.38

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

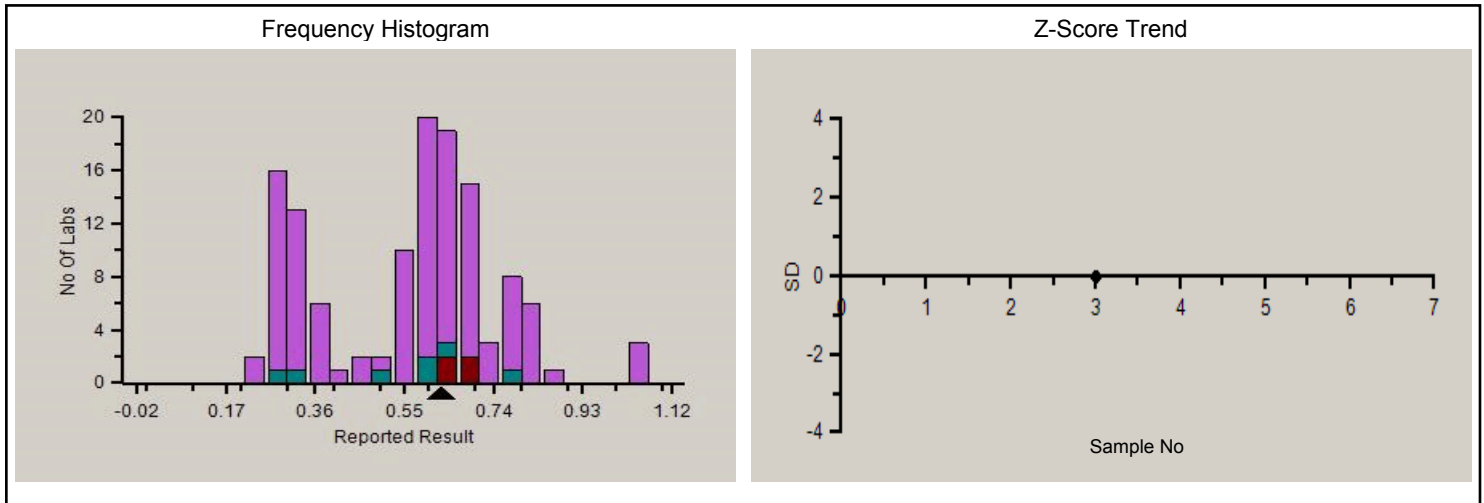

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
 Lab Name : SANJEEVANI LABORATORY
 Report Date : 14/01/2021

Cycle No : 200312
 Sample No : 3
 Sample Date : 28-12-2020

Biochemistry, Creatinine		N	Mean	SD	CV%	Excluded
	All Analyzer	146	0.55	0.19	33.94	13
Your Analyzer :	Erba EM 200	4	0.67	0.04	5.37	--
	Roche cobas c 311	26	0.61	0.04	7.03	--
	Fuji Dri-Chem NX500/i	25	0.29	0.04	12.15	3
	Fuji Dri-Chem 4000i	15	0.31	0.03	10.75	4
	Horiba ABX Pentra C200	12	0.72	0.08	11.05	4
	Roche cobas c 111	12	0.64	0.07	10.14	1
	Roche cobas INTEGRA	10	0.56	0.06	10.45	--
	Roche cobas 6000	7	0.61	0.02	3.26	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 3
Sample Date : 28-12-2020


Biochemistry, Glucose, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	146	74.70	4.02	5.39	5
GPO-POD	11	72.75	6.65	9.14	--
Erba EM 200	4	76.67	4.09	5.34	1

Your Result	77.90	SDI / z-Score	0.18
Assigned Value	76.50	Average SDI	1.20
SDPA	7.649	Uncertainty of AV	0.35
Standard Unit Result Val	77.90	%DEV	7.09

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

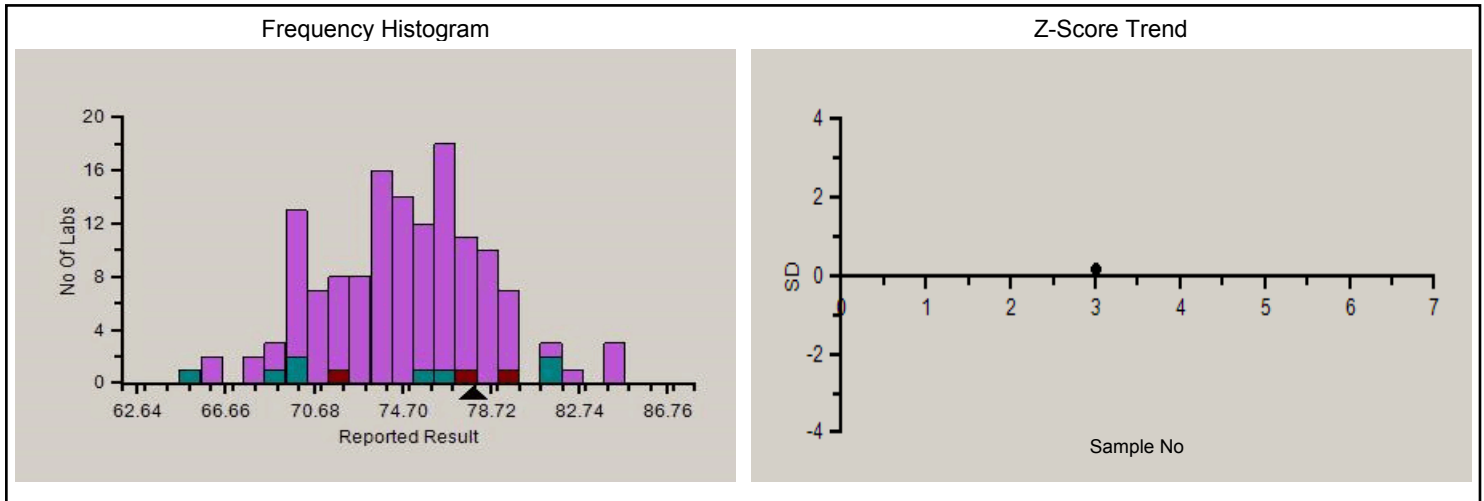

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 361
 Lab Name : SANJEEVANI LABORATORY
 Report Date : 14/01/2021

Cycle No : 200312
 Sample No : 3
 Sample Date : 28-12-2020

Biochemistry, Glucose		N	Mean	SD	CV%	Excluded
	All Analyzer	146	74.70	4.02	5.39	5
Your Analyzer :	Erba EM 200	4	76.67	4.09	5.34	1
	Roche cobas c 311	26	77.03	2.49	3.23	--
	Fuji Dri-Chem NX500/i	23	71.52	2.41	3.37	--
	Fuji Dri-Chem 4000i	16	71.73	3.03	4.22	1
	Horiba ABX Pentra C200	12	75.34	4.13	5.49	1
	Roche cobas c 111	12	76.92	2.55	3.32	1
	Roche cobas INTEGRA	10	75.74	3.21	4.24	--
	Roche cobas 6000	7	75.57	2.64	3.49	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 3
Sample Date : 28-12-2020


Biochemistry, HDL, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	130	35.38	2.99	8.46	6
■ Direct measure-PEG	17	36.05	3.97	11.02	3
■ Erba EM 200	2	33.85	--	--	--

Your Result	37.70	SDI / z-Score	1.13
Assigned Value	34.60	Average SDI	1.53
SDPA	2.760	Uncertainty of AV	0.45
Standard Unit Result Val	37.70	%DEV	4.58

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

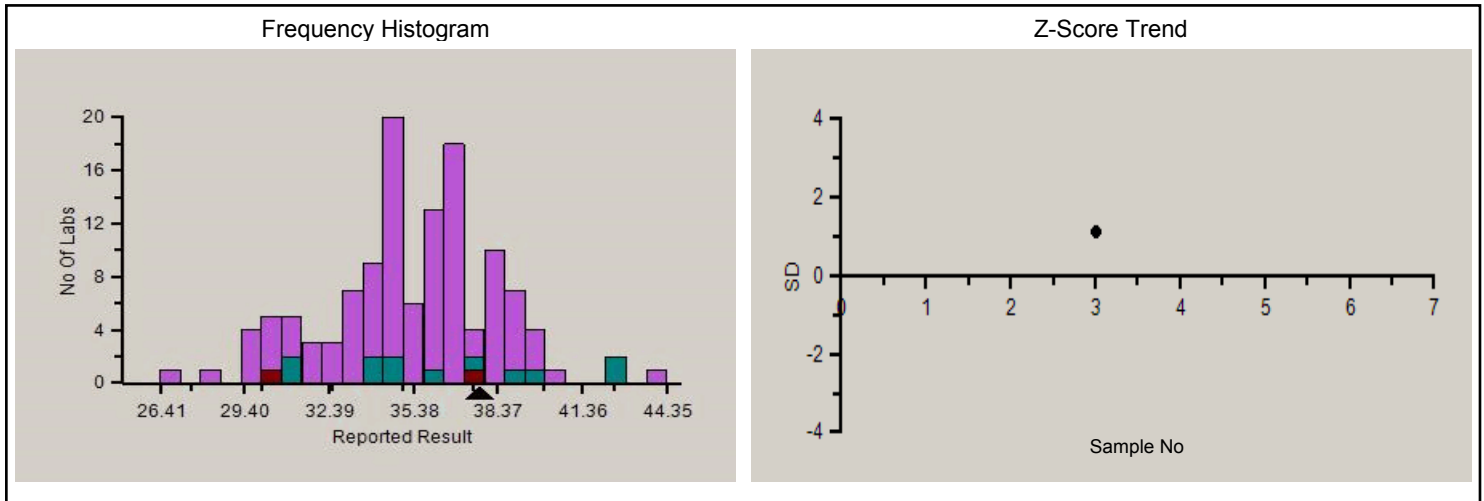

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 3
Sample Date : 28-12-2020

Biochemistry, HDL		N	Mean	SD	CV%	Excluded
	All Analyzer	130	35.38	2.99	8.46	6
Your Analyzer :	Erba EM 200	2	33.85	--	--	--
	Roche cobas c 311	26	33.85	2.13	6.29	--
	Fuji Dri-Chem NX500/i	23	36.32	1.39	3.84	1
	Fuji Dri-Chem 4000i	15	37.00	1.08	2.92	2
	Roche cobas c 111	12	32.06	3.10	9.68	--
	Horiba ABX Pentra C200	10	38.67	2.05	5.29	1
	Roche cobas INTEGRA	9	33.34	1.86	5.57	--
	Roche cobas 6000	7	34.86	1.95	5.60	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 3
Sample Date : 28-12-2020


Biochemistry, Phosphorous Inorganic, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	107	3.42	0.18	5.12	4
■ Phosphomolybdate method	51	3.39	0.13	3.72	1
■ Erba Chem 5/Plus	2	--	--	--	2

Your Result	5.20	SDI / z-Score	12.96
Assigned Value	3.40	Average SDI	8.22
SDPA	0.139	Uncertainty of AV	0.02
Standard Unit Result Val	5.20	%DEV	53.35

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

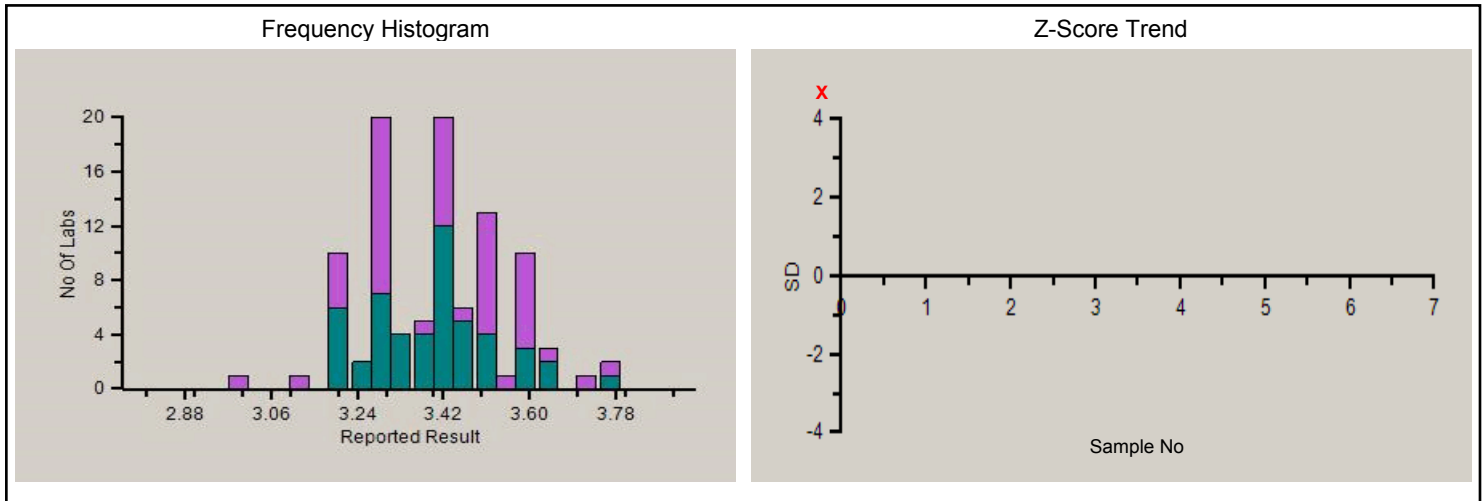

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 361
 Lab Name : SANJEEVANI LABORATORY
 Report Date : 14/01/2021

Cycle No : 200312
 Sample No : 3
 Sample Date : 28-12-2020

Biochemistry, Phosphorous Inorganic		N	Mean	SD	CV%	Excluded
	All Analyzer	107	3.42	0.18	5.12	4
Your Analyzer :	Erba Chem 5/Plus	2	--	--	--	2
	Roche cobas c 311	23	3.38	0.11	3.32	--
	Fuji Dri-Chem NX500/i	20	3.40	0.12	3.50	1
	Fuji Dri-Chem 4000i	13	3.35	0.15	4.32	--
	Roche cobas INTEGRA	8	3.41	0.16	4.58	--
	Roche cobas 6000	7	3.35	0.10	2.86	--
	Roche cobas c 111	5	3.54	0.09	2.63	--
	Roche cobas 8000	4	3.37	0.08	2.31	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 3
Sample Date : 28-12-2020


Biochemistry, Urea, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	145	19.40	3.51	18.10	12
Urease, GLDH	28	22.18	1.89	8.50	2
Erba EM 200	5	21.54	1.70	7.89	--

Your Result	21.30	SDI / z-Score	0.12
Assigned Value	21.04	Average SDI	0.26
SDPA	2.131	Uncertainty of AV	0.19
Standard Unit Result Val	21.30	%DEV	-1.12

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

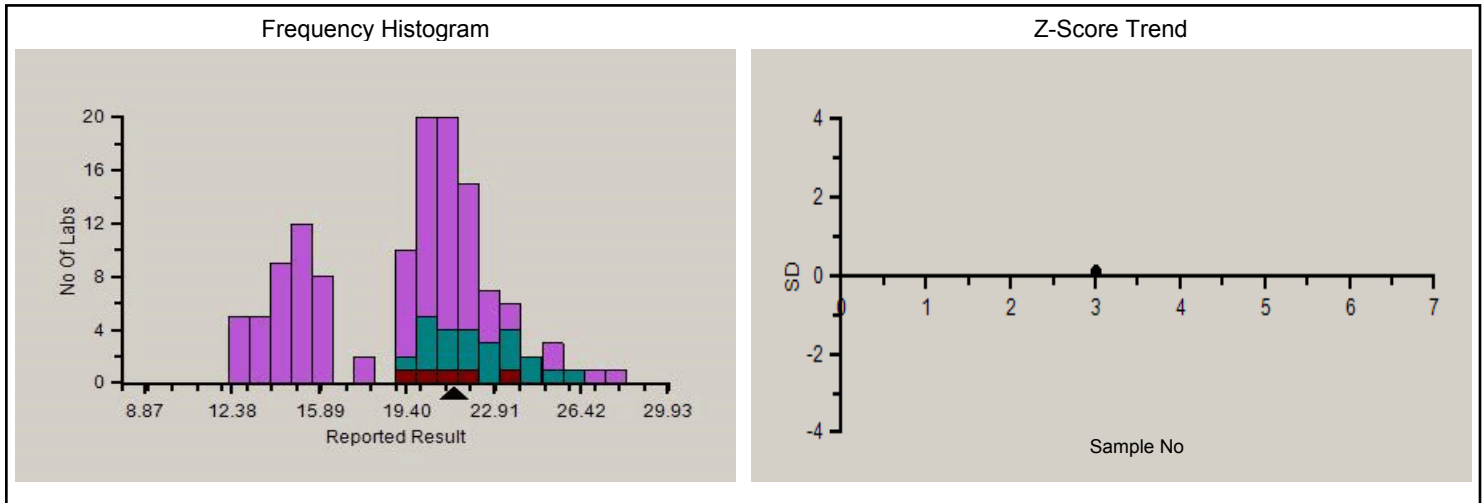

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 361
Lab Name : SANJEEVANI LABORATORY
Report Date : 14/01/2021

Cycle No : 200312
Sample No : 3
Sample Date : 28-12-2020

Biochemistry, Urea		N	Mean	SD	CV%	Excluded
	All Analyzer	145	19.40	3.51	18.10	12
Your Analyzer :	Erba EM 200	5	21.54	1.70	7.89	--
	Roche cobas c 311	26	21.15	0.94	4.44	--
	Fuji Dri-Chem NX500/i	25	14.62	0.94	6.42	3
	Fuji Dri-Chem 4000i	15	14.96	0.76	5.09	3
	Roche cobas c 111	12	19.91	0.89	4.48	--
	Horiba ABX Pentra C200	11	23.45	0.96	4.09	3
	Roche cobas INTEGRA	10	19.87	1.20	6.06	--
	Roche cobas 6000	7	20.64	0.68	3.27	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
Unit No. 409-416.
Commercial Building - 1A,
Kohinoor Mall, Kirool Road, Kuria (W),
Mumbai - 400070



PC-1022