


**MINDRAY BC 5300 - CALIBRATION CERTIFICATE**

<b>Customer Name</b>	<b>SVIMS HOSPITAL</b>					
<b>Department</b>	Department of Pathology-Laboratory Services					
<b>Address</b>	By pass road, Tirupathi , Andhra Pradesh-517507					
				<b>Date of Calibration</b>	16-06-2020	
<b>Instrument</b>	<b>BC-5300 Auto Haematology Analyzer</b>			<b>Next Calibration Date</b>	15-12-2020	
<b>Serial No</b>	RD-73101503			<b>Calibrator Lot Number</b>	PLUS0519	
				<b>Calibrator Expiry date</b>	05-07-2020	
<b><u>Calibration Values</u></b>	<b><u>Parameter</u></b>	<b><u>Target</u></b>	<b><u>Range</u></b>	<b><u>Mean of Measured Values</u></b>	<b><u>Factor</u></b>	<b><u>Old Factor</u></b>
	WBC x 10 <sup>9</sup> /L	9.40	9.20-9.60	9.36	106.43	105.70
	RBC x10 <sup>12</sup> /L	4.43	4.35-4.51	4.39	107.42	109.20
	HGB g/dL	13.3	13.1-13.5	13.2	111.02	112.00
	MCV fl	89.0	87.0-91.0	88.7	102.42	100.50
	PLT x 10 <sup>9</sup> /L	239	227-251	228	105.57	113.00
<p>This is to certify that the Mindray BC 5300 Hematology Analyzer with Serial No: RD-73101503, installed at Svims Hospital , Tirupathi has been calibrated using the standard reference material PLUS0620 Calibrator.</p>						

Reviewed By :

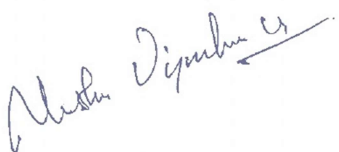


date: 20/06/2020

Manager – Application  
Golden Harvest Industries.