


Average	9.3	4.48	12.6	39.6	235	8.8
%BAL	4.0	1.04	9.2	1.5	0	0.9
CV	0.8	2.43	0.3	2.6	5	2.2
New Coef	0.97	0.84	1.19	1.02	1.15	0.95
Old Coef	1.01	0.83	1.08	1.04	1.15	0.96
Target	8.9	4.53	13.9	39.0	235	8.7
A 1	8.9	3.81	12.0	33.4	202	8.7
2	9.4	4.61	12.7	40.7	252	8.7
3	9.2	4.54	12.6	40.2	238	8.8
4	9.3	4.47	12.6	39.4	230	9.1
5	9.2	4.32	12.6	38.0	220	8.6
6						
7						
8						
9						
10						
11						

USA ABX 848
 100%
 100%
 100%
 100%

LOT CX 454

CAL

 (Exp.) 2021-02-05

Rev 1

Minilysebio

PARAMETRES PARAMETERS	UNITES UNITS	MICROS					PENITIA					TOLERANCES TOLERANCE
		ES90	CRP 200				60 8P	60 18P				
CO WBC	$10^9/mm^3 \cdot 10^9/l$	8.9	8.8				9.0					± 0.2
CR RBC	$10^6/mm^3 \cdot 10^6/l$	4.03	4.52				4.55					± 0.06
	g/dl	13.9	13.4				13.8					± 0.2
Hb HGB	g/l	128	124				138					± 2
	mmol/l	8.83	8.34				8.57					± 0.12
HT HCT	%	39.8	38.9				39.6					± 1.0
	g	0.398	0.389				0.396					± 0.010
PLAQ. PLTS	$10^9/mm^3 \cdot 10^9/l$	235	242				244					± 10
VPAL MPV	$10^3 \cdot l$	8.7	8.2				9.2					± 0.5

YYYY - MM - DD

ABX Minocal

RIBA ABX SAS
SAS
ecine
ée - BP 7290
ELLIER Cedex 4
14 15 16
14 15 17

LOT

CX 454

CAL



(Exp.) 2021-02-05
(YYYY-MM-DD)

Rev 1

LyseVet

PARAMETRES PARAMETERS	UMTES UNITS	MICROS		TOLERANCES TOLERANCE
		Scil Vet ABC	Scil Vet ABC Plus ESV 60	
GB WBC	10 ³ /mm ³ ; 10 ⁹ /l	8.7	8.7	± 0.2
GR RBC	10 ⁶ /mm ³ ; 10 ¹² /l	4.54	4.52	± 0.06
HB HGB	g/dl	13.6	13.5	± 0.2
	g/l	136	135	± 2
	mmol/l	8.45	8.38	± 0.12
HT HCT	%	39.0	38.9	± 1.0
	l/l	0.390	0.389	± 0.010
PLAQ. PLTS	10 ³ /mm ³ ; 10 ⁹ /l	240	249	± 10
VPM MPV	µm ³ ; fl	N/A	9.0	± 0.5

Explore the future

HORIBA India Private Limited

346, Okhla Industrial Estate Phase-II,

New Delhi 110020, India

Tel : +91 (11) 4646 5000 / 4669 5001

Fax : +91 (11) 4646 5020

http : //www.horiba.com

CIN : U73100DL2008PTC163232

HIN/MED/2020-2021/100654

25th Dec 2020


CALIBRATION CERTIFICATE

This is to certify that the hematology analyser **Micros ES60** bearing serial no: **306ESOH05900** installed at **SARDANA LABS, JALANDHAR** was calibrated on 25th Dec 2020

Calibrator : ABX MINOCAL
Lot No. : CX454
Expiry Date : 5th Feb 2021

The reports of Blank Cycle, Repeatability and Calibration Values were all found in acceptable range:

Next calibration cycle is due on 24th Dec 2021

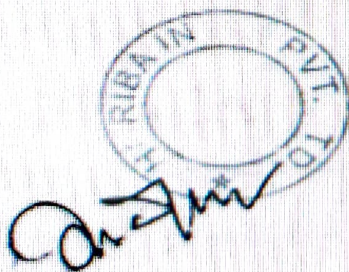

Shrish Dixit

(Head – Products & Marketing)

For Horiba India Pvt. Ltd.