

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, ALP, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	141	193.32	20.55	10.63	10
■ PNPP, AMP Buffer	65	196.76	21.76	11.06	5
■ RANDOX RX daytona	1	--	--	--	--

Your Result	179.00	SDI / z-Score	-0.23
Assigned Value	184.97	Average SDI	-1.16
SDPA	25.896	Uncertainty of AV	2.01
Standard Unit Result Val	179.00	%DEV	-9.03

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

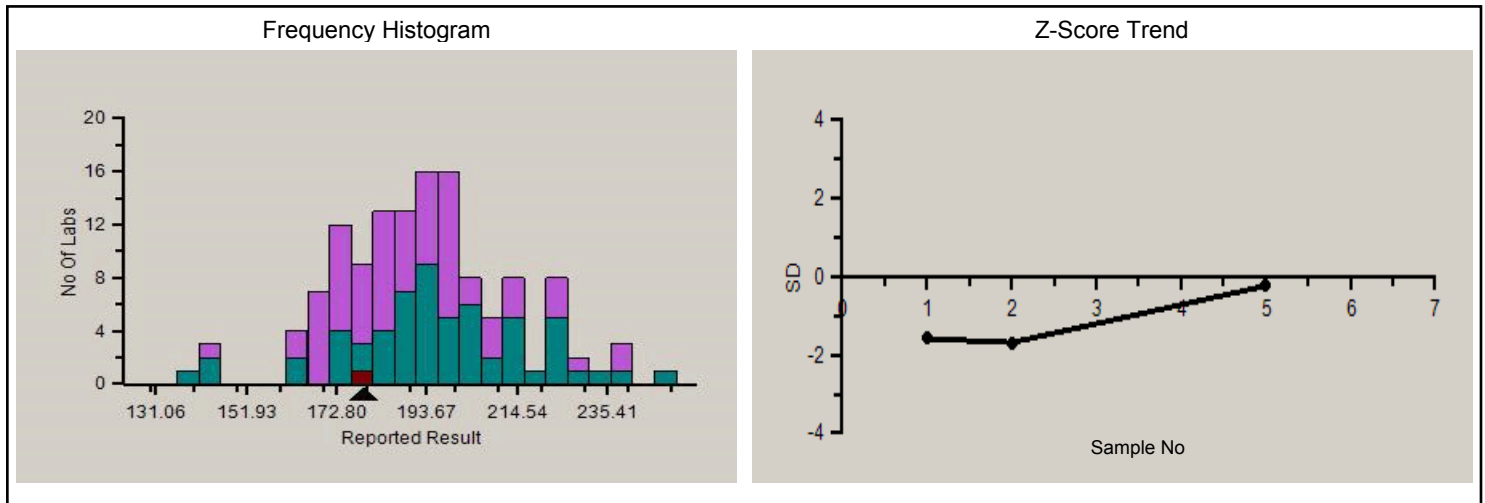

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, ALP		N	Mean	SD	CV%	Excluded
	All Analyzer	141	193.32	20.55	10.63	10
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	32	203.03	15.57	7.67	1
	Roche cobas c 311	27	181.23	9.50	5.24	--
	Fuji Dri-Chem 4000i	15	204.14	16.81	8.24	1
	Roche cobas c 111	11	191.72	21.02	10.96	--
	Horiba ABX Pentra C200	10	193.52	17.60	9.10	1
	Roche cobas c 111	10	186.89	14.35	7.68	--
	Roche cobas INTEGRA	9	190.45	16.85	8.85	--
	Roche cobas 6000	8	186.50	10.06	5.39	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, ALT, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	144	46.97	3.72	7.92	4
■ IFCC - UV without P5P	13	50.02	2.86	5.72	1
■ RANDOX RX daytona	1	--	--	--	--

Your Result	54.00	SDI / z-Score	1.66
Assigned Value	46.33	Average SDI	0.65
SDPA	4.623	Uncertainty of AV	0.38
Standard Unit Result Val	54.00	%DEV	7.95

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

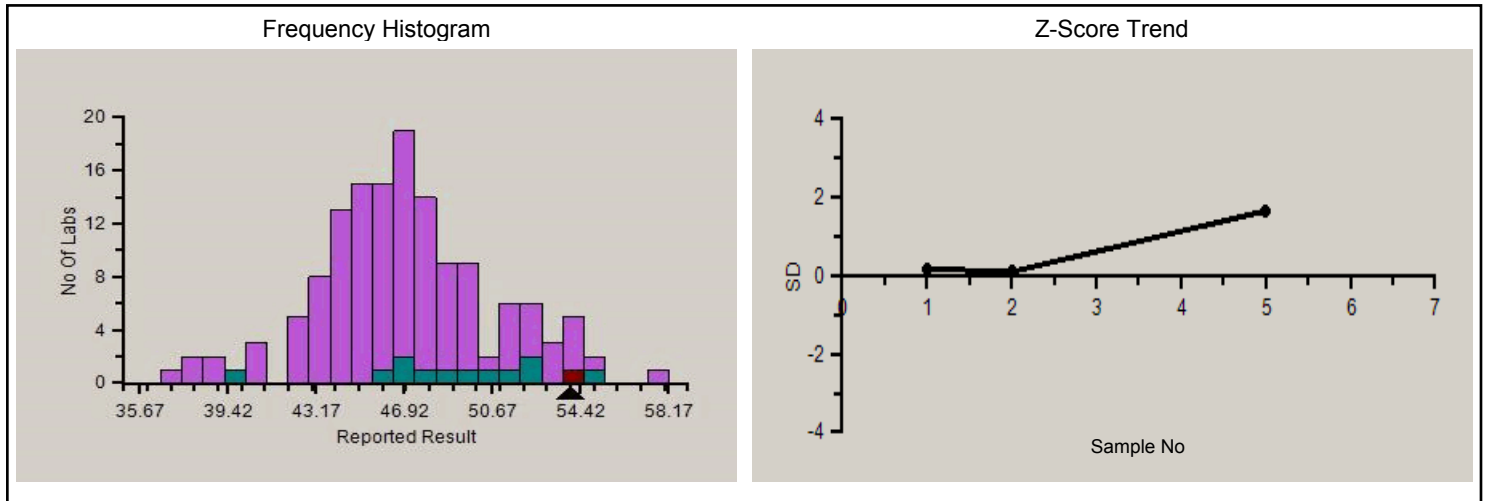

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, ALT		N	Mean	SD	CV%	Excluded
	All Analyzer	144	46.97	3.72	7.92	4
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	31	47.93	3.70	7.73	1
	Roche cobas c 311	27	45.76	2.41	5.27	--
	Fuji Dri-Chem 4000i	15	47.53	3.11	6.55	--
	Horiba ABX Pentra C200	12	49.66	3.01	6.06	--
	Roche cobas c 111	11	44.75	2.27	5.07	--
	Roche cobas c 111	10	45.22	1.72	3.81	--
	Roche cobas INTEGRA	9	45.93	3.95	8.59	--
	Roche cobas 6000	8	45.51	2.15	4.72	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Amylase, U/L

	N	Mean	SD	CV%	Excluded
All Methods	87	180.64	21.14	11.70	3
G7 PNP	64	180.36	11.74	6.51	2
RANDOX RX daytona	1	--	--	--	--

Your Result	194.00	SDI / z-Score	1.02
Assigned Value	176.12	Average SDI	1.04
SDPA	17.612	Uncertainty of AV	1.55
Standard Unit Result Val	194.00	%DEV	7.57

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

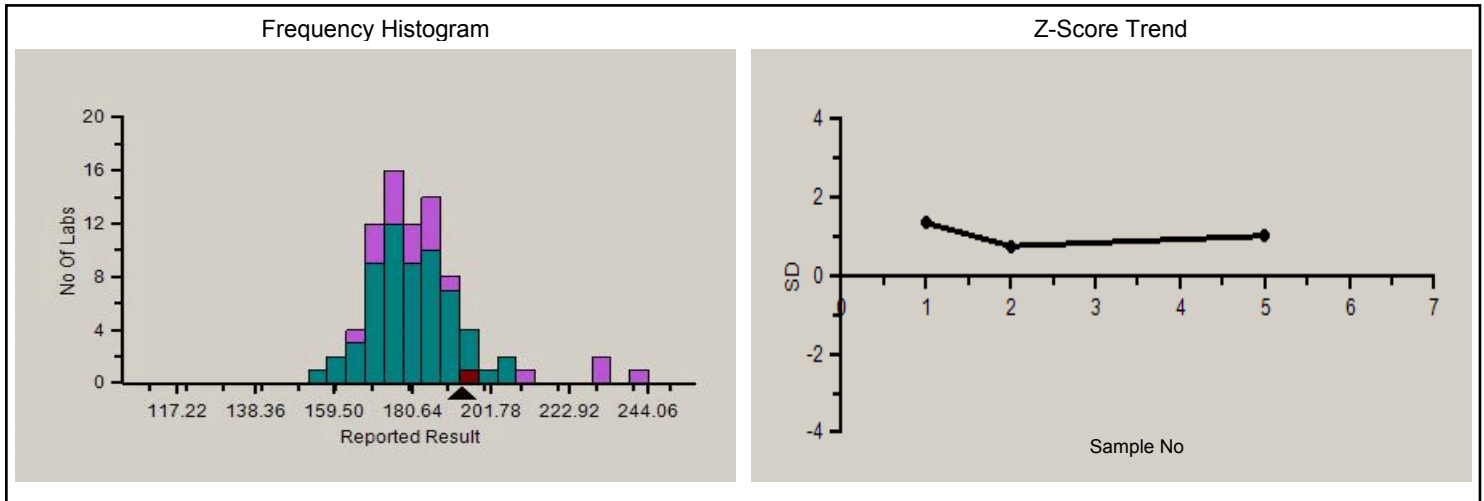

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, Amylase		N	Mean	SD	CV%	Excluded
	All Analyzer	87	180.64	21.14	11.70	3
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	22	182.50	14.55	7.97	1
	Fuji Dri-Chem 4000i	14	184.93	7.03	3.80	--
	Roche cobas c 311	13	174.41	7.72	4.43	--
	Roche cobas INTEGRA	7	178.57	4.78	2.68	--
	Roche cobas 6000	6	171.93	6.53	3.80	--
	Roche cobas 8000	4	168.75	3.95	2.34	--
	Roche cobas c 111	3	184.00	11.39	6.19	--
	Horiba ABX Pentra C200	2	193.15	--	--	1

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, AST, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	143	94.40	5.54	5.87	6
■ IFCC - UV without P5P	11	98.77	4.93	4.99	--
■ RANDOX RX daytona	1	--	--	--	--

Your Result	93.00	SDI / z-Score	-0.05
Assigned Value	93.61	Average SDI	-0.24
SDPA	11.233	Uncertainty of AV	0.64
Standard Unit Result Val	93.00	%DEV	-5.84

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

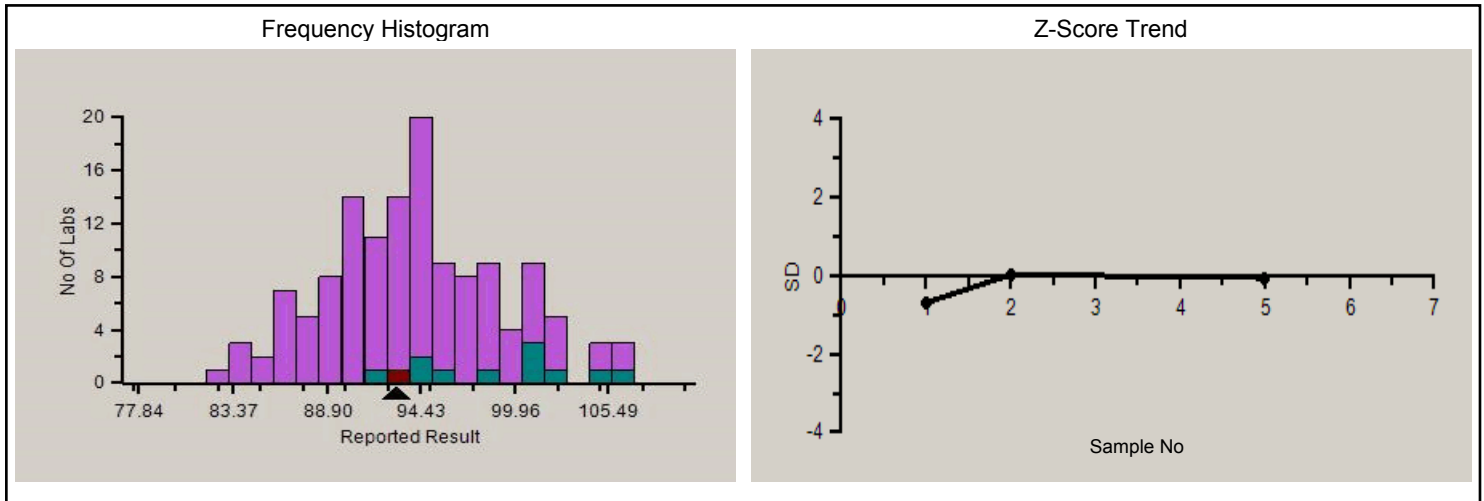

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, AST		N	Mean	SD	CV%	Excluded
	All Analyzer	143	94.40	5.54	5.87	6
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	32	94.40	5.84	6.19	2
	Roche cobas c 311	26	93.50	3.40	3.64	--
	Fuji Dri-Chem 4000i	15	91.53	4.00	4.37	--
	Roche cobas c 111	12	91.63	4.03	4.40	--
	Roche cobas c 111	11	91.04	3.63	3.99	--
	Horiba ABX Pentra C200	10	96.87	5.97	6.17	1
	Roche cobas INTEGRA	9	92.68	3.90	4.21	1
	Roche cobas 6000	8	93.26	4.69	5.03	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Bilirubin Direct, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	139	0.92	0.13	13.64	16
DMSO	1	--	--	--	--
RANDOX RX daytona	1	--	--	--	--

Your Result	0.69	SDI / z-Score	-1.32
Assigned Value	0.94	Average SDI	0.99
SDPA	0.188	Uncertainty of AV	0.02
Standard Unit Result Val	0.69	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

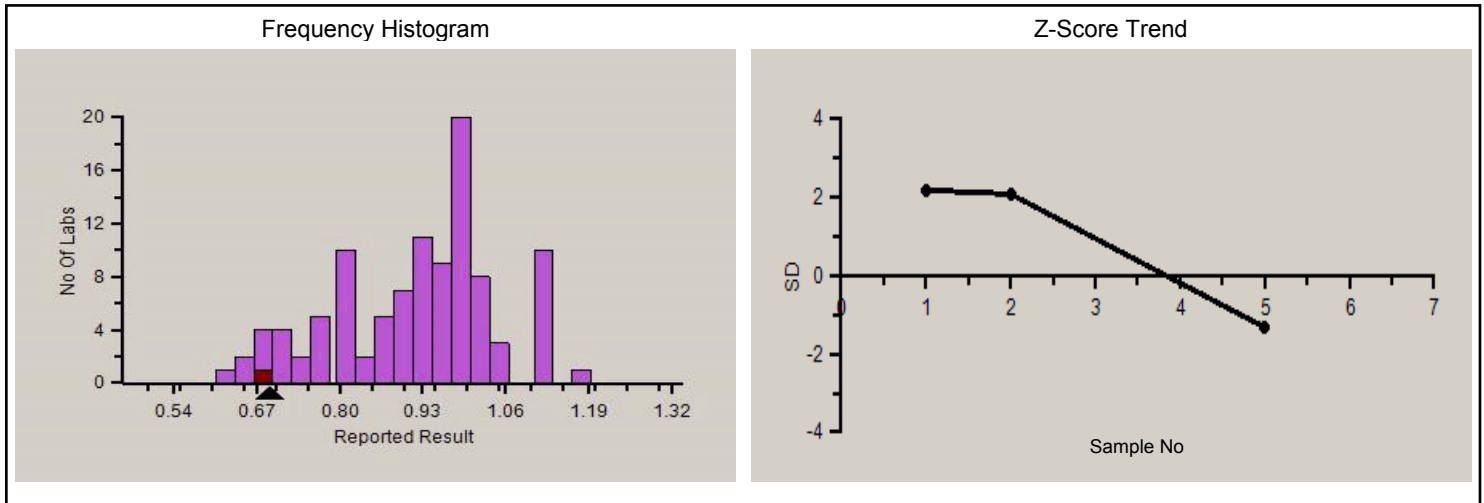

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, Bilirubin Direct		N	Mean	SD	CV%	Excluded
	All Analyzer	139	0.92	0.13	13.64	16
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	28	0.97	0.08	8.56	1
	Roche cobas c 311	26	0.94	0.11	11.24	1
	Fuji Dri-Chem 4000i	15	0.99	0.05	4.63	--
	Horiba ABX Pentra C200	11	0.75	0.07	8.98	1
	Roche cobas c 111	11	1.03	0.09	8.22	2
	Roche cobas c 111	10	1.04	0.09	8.67	2
	Roche cobas INTEGRA	9	0.90	0.08	8.56	--
	Roche cobas 6000	8	0.95	0.07	7.26	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Bilirubin Total, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	142	1.92	0.17	8.66	8
DMSO	1	--	--	--	--
RANDOX RX daytona	1	--	--	--	--

Your Result	2.33	SDI / z-Score	0.93
Assigned Value	2.16	Average SDI	1.97
SDPA	0.182	Uncertainty of AV	0.07
Standard Unit Result Val	2.33	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

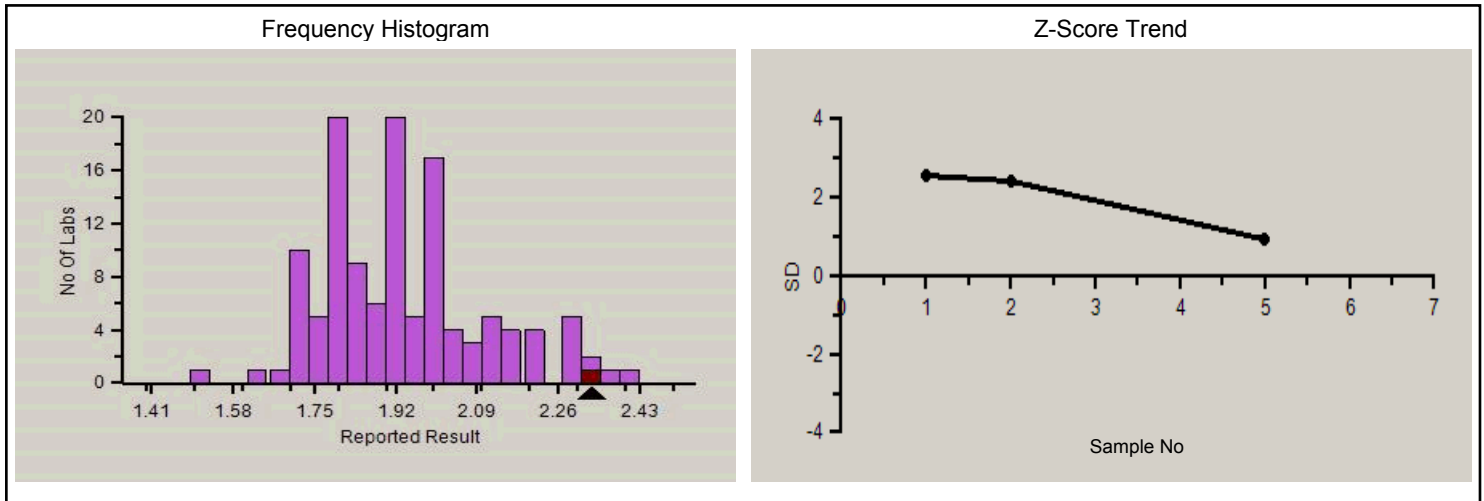

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, Bilirubin Total		N	Mean	SD	CV%	Excluded
	All Analyzer	142	1.92	0.17	8.66	8
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	29	1.83	0.13	7.25	2
	Roche cobas c 311	27	1.87	0.11	6.03	2
	Fuji Dri-Chem 4000i	15	1.87	0.11	5.62	--
	Horiba ABX Pentra C200	11	2.05	0.11	5.32	2
	Roche cobas c 111	10	1.99	0.20	10.20	--
	Roche cobas c 111	9	1.95	0.15	7.81	--
	Roche cobas INTEGRA	9	1.86	0.13	6.72	--
	Roche cobas 6000	8	1.83	0.09	5.08	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Calcium, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	131	5.77	0.34	5.91	10
Arsenazo III	34	5.81	0.41	7.10	6
RANDOX RX daytona	1	--	--	--	--

Your Result	5.60	SDI / z-Score	-0.44
Assigned Value	5.81	Average SDI	-0.29
SDPA	0.464	Uncertainty of AV	0.04
Standard Unit Result Val	5.60	%DEV	-3.55

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

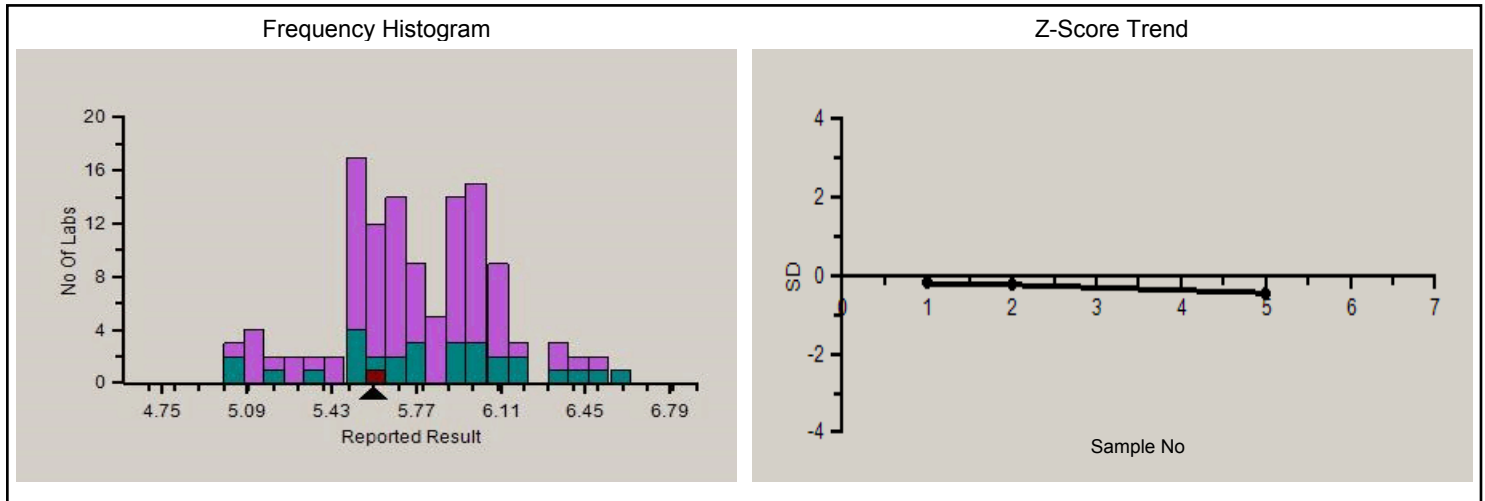

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, Calcium		N	Mean	SD	CV%	Excluded
	All Analyzer	131	5.77	0.34	5.91	10
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	27	5.61	0.34	6.00	2
	Roche cobas c 311	24	5.87	0.23	3.83	--
	Fuji Dri-Chem 4000i	15	5.64	0.29	5.14	--
	Roche cobas c 111	10	5.87	0.30	5.13	--
	Roche cobas INTEGRA	10	5.78	0.35	6.08	--
	Roche cobas c 111	9	5.84	0.31	5.27	--
	Roche cobas 6000	7	5.85	0.15	2.62	--
	Beckman Coulter AU480	5	5.77	0.21	3.55	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, CK, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	70	246.71	39.40	15.97	3
■ Colorimetric	1	--	--	--	--
■ Fuji Nx 700	3	278.00	33.96	12.21	--

Your Result	255.00	SDI / z-Score	-1.26
Assigned Value	282.95	Average SDI	0.05
SDPA	22.154	Uncertainty of AV	4.82
Standard Unit Result Val	255.00	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

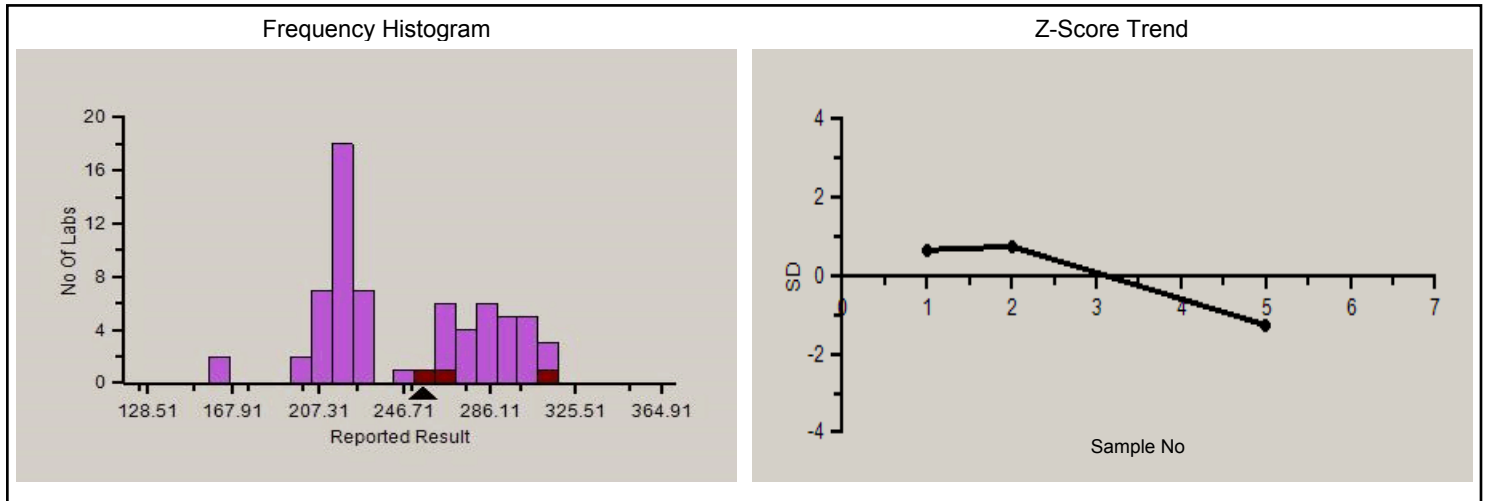

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, CK		N	Mean	SD	CV%	Excluded
	All Analyzer	70	246.71	39.40	15.97	3
Your Analyzer :	Fuji Nx 700	3	278.00	33.96	12.21	--
	Fuji Dri-Chem NX500/i	20	278.05	24.73	8.89	1
	Roche cobas c 311	12	219.54	6.09	2.77	--
	Fuji Dri-Chem 4000i	11	285.36	24.73	8.67	--
	Roche cobas INTEGRA	7	220.34	13.16	5.97	--
	Roche cobas 6000	5	215.44	8.49	3.94	--
	Roche cobas 8000	4	213.75	4.19	1.96	--
	Beckman Coulter AU480	1	--	--	--	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Creatinine, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	140	2.53	0.19	7.52	4
Ammonia Concentration Measurement - color change of BPB	42	2.39	0.12	4.98	2
Fuji Nx 700	1	--	--	--	--

Your Result	2.24	SDI / z-Score	-0.83
Assigned Value	2.38	Average SDI	1.23
SDPA	0.166	Uncertainty of AV	0.02
Standard Unit Result Val	2.24	%DEV	-6.20

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

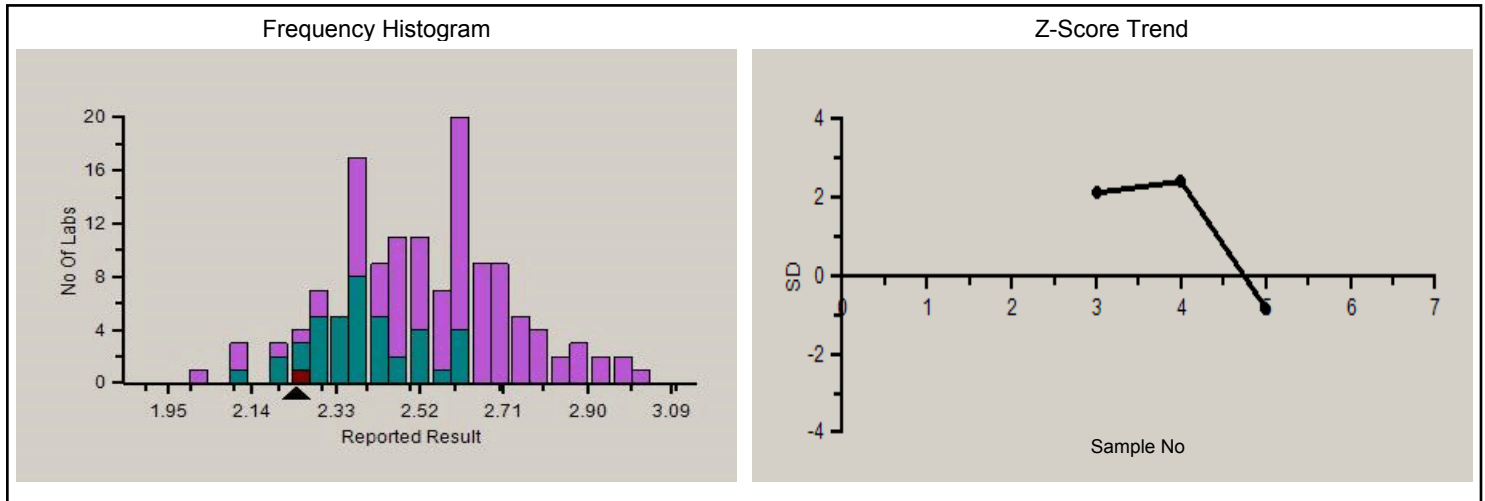

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, Creatinine		N	Mean	SD	CV%	Excluded
	All Analyzer	140	2.53	0.19	7.52	4
Your Analyzer :	Fuji Nx 700	1	--	--	--	--
	Fuji Dri-Chem NX500/i	28	2.38	0.11	4.71	2
	Roche cobas c 311	27	2.62	0.13	4.85	--
	Fuji Dri-Chem 4000i	15	2.39	0.12	5.11	1
	Horiba ABX Pentra C200	11	2.57	0.26	10.05	--
	Roche cobas c 111	11	2.55	0.18	7.03	--
	Roche cobas c 111	10	2.59	0.11	4.09	--
	Roche cobas INTEGRA	9	2.48	0.21	8.31	--
	Roche cobas 6000	8	2.60	0.11	4.38	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, GGT, U/L

	N	Mean	SD	CV%	Excluded
All Methods	123	90.79	16.32	17.97	6
IFCC	11	87.93	12.58	14.31	--
RANDOX RX daytona	1	--	--	--	--

Your Result	84.00	SDI / z-Score	0.53
Assigned Value	78.58	Average SDI	0.88
SDPA	10.215	Uncertainty of AV	0.65
Standard Unit Result Val	84.00	%DEV	-4.47

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

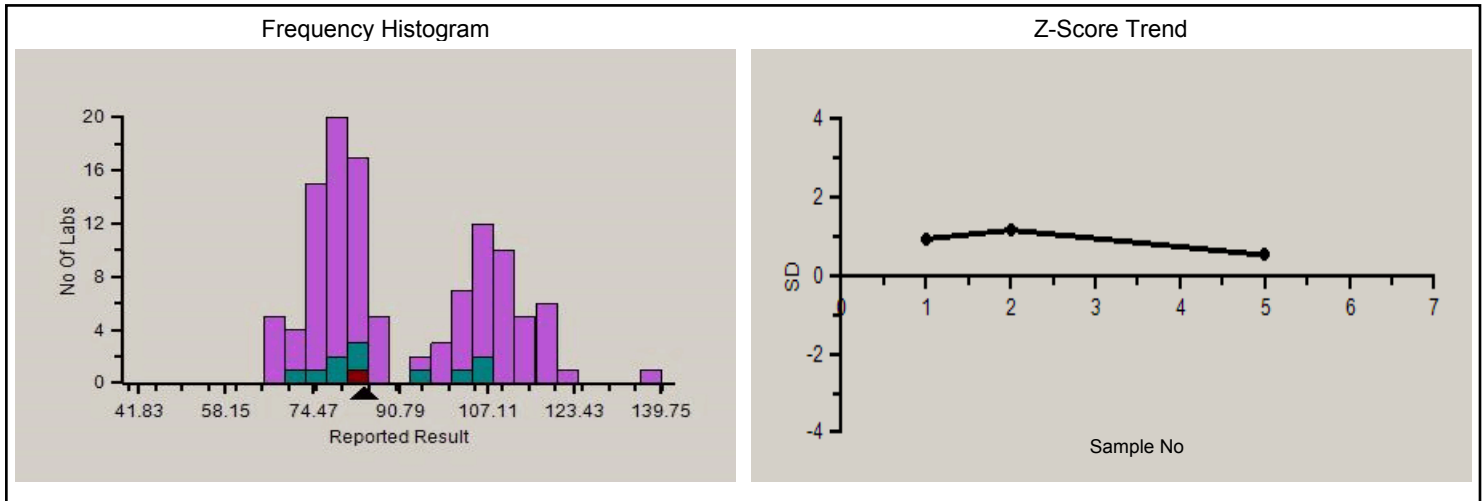

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, GGT		N	Mean	SD	CV%	Excluded
	All Analyzer	123	90.79	16.32	17.97	6
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	30	108.66	10.52	9.68	1
	Roche cobas c 311	24	78.70	4.47	5.68	1
	Fuji Dri-Chem 4000i	12	107.67	4.44	4.12	--
	Roche cobas INTEGRA	10	78.46	5.14	6.55	--
	Roche cobas c 111	9	80.35	5.89	7.34	1
	Horiba ABX Pentra C200	6	78.34	4.74	6.05	1
	Roche cobas 6000	6	77.83	3.55	4.56	--
	Beckman Coulter AU480	5	78.10	2.29	2.93	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Glucose, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	143	133.24	6.91	5.19	8
GOD-PAP	4	135.25	6.80	5.03	--
RANDOX RX daytona	1	--	--	--	--

Your Result	142.00	SDI / z-Score	0.61
Assigned Value	134.61	Average SDI	0.10
SDPA	12.115	Uncertainty of AV	0.92
Standard Unit Result Val	142.00	%DEV	4.99

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

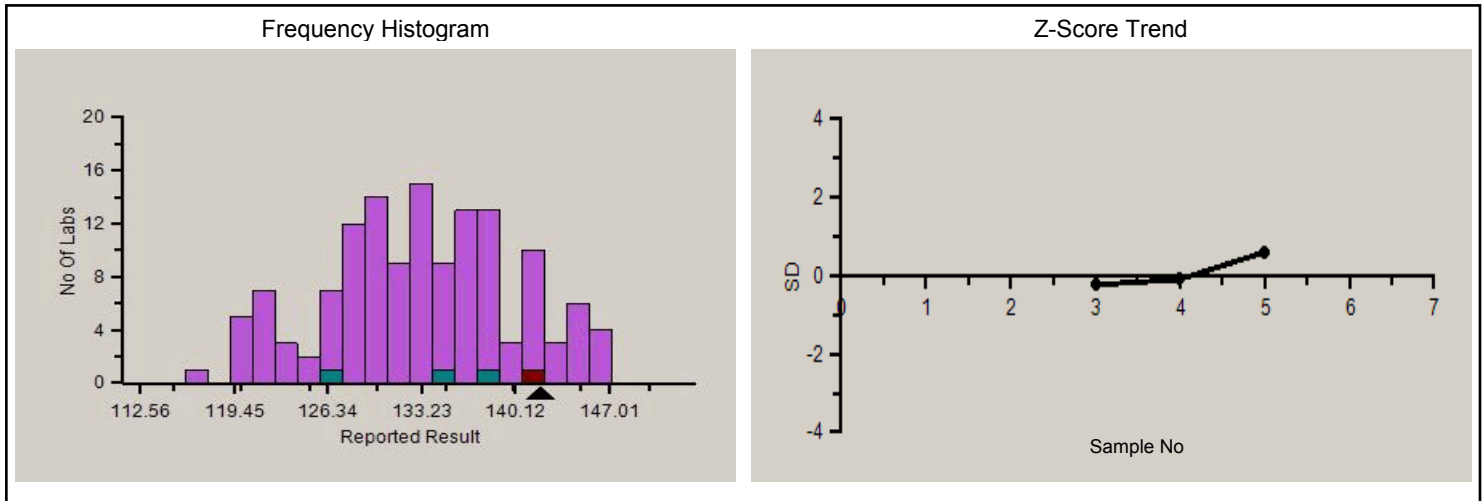

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, Glucose		N	Mean	SD	CV%	Excluded
	All Analyzer	143	133.24	6.91	5.19	8
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	30	131.57	7.66	5.82	2
	Roche cobas c 311	27	133.56	6.08	4.55	3
	Fuji Dri-Chem 4000i	15	130.60	5.72	4.38	--
	Horiba ABX Pentra C200	12	131.57	7.56	5.75	--
	Roche cobas c 111	10	136.47	4.44	3.25	1
	Roche cobas c 111	9	137.03	4.40	3.21	1
	Roche cobas INTEGRA	9	134.88	6.60	4.89	--
	Roche cobas 6000	8	135.25	4.37	3.23	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, LDH, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	81	194.07	49.12	25.31	10
■ L to P - IFCC Ref. Proc., Calibrated	2	139.00	--	--	1
■ Fuji Nx 700	3	156.00	18.68	11.98	--

Your Result	139.00	SDI / z-Score	-1.25
Assigned Value	168.36	Average SDI	-0.67
SDPA	23.570	Uncertainty of AV	2.78
Standard Unit Result Val	139.00	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

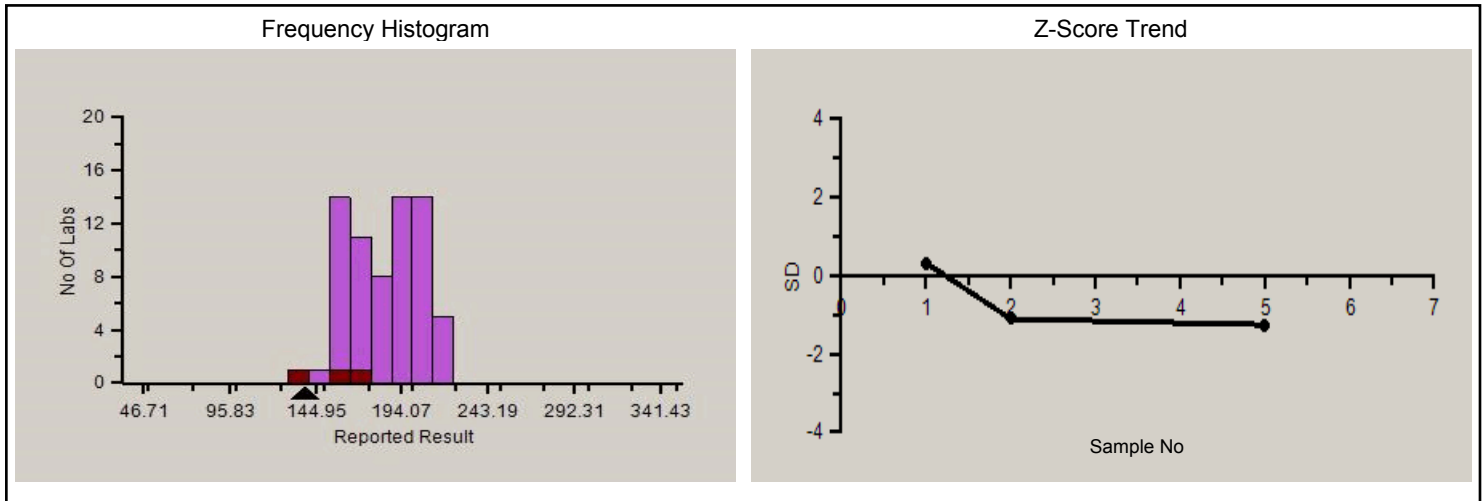

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, LDH		N	Mean	SD	CV%	Excluded
	All Analyzer	81	194.07	49.12	25.31	10
Your Analyzer :	Fuji Nx 700	3	156.00	18.68	11.98	--
	Fuji Dri-Chem NX500/i	22	168.45	10.07	5.98	2
	Fuji Dri-Chem 4000i	12	170.75	13.59	7.96	--
	Roche cobas c 311	10	201.50	6.31	3.13	--
	Roche cobas INTEGRA	7	209.65	9.68	4.62	--
	Roche cobas 6000	6	206.00	9.80	4.76	--
	Roche cobas 8000	4	199.50	6.86	3.44	--
	Beckman Coulter AU480	3	187.60	15.25	8.13	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Lipase, U/L

	N	Mean	SD	CV%	Excluded
All Methods	71	49.91	43.79	87.75	4
Enzymatic colorimetric	12	41.08	12.56	30.57	1
Fuji Nx 700	3	52.33	5.13	9.81	--

Your Result	48.00	SDI / z-Score	-0.88
Assigned Value	54.24	Average SDI	-0.41
SDPA	7.051	Uncertainty of AV	0.75
Standard Unit Result Val	48.00	%DEV	16.84

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

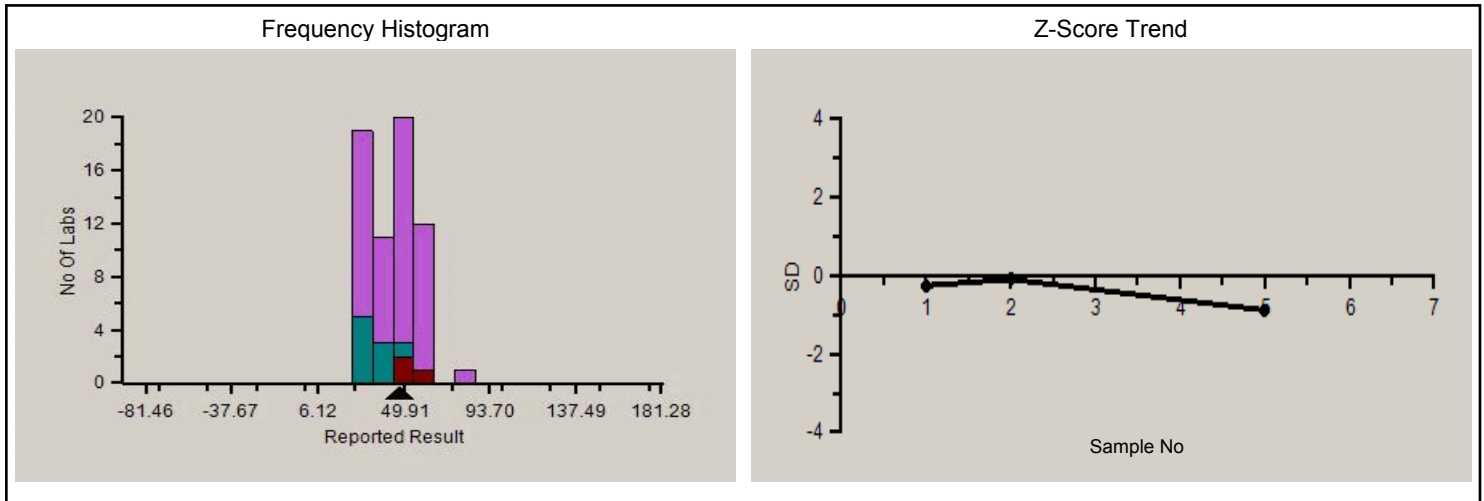

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, Lipase		N	Mean	SD	CV%	Excluded
	All Analyzer	71	49.91	43.79	87.75	4
Your Analyzer :	Fuji Nx 700	3	52.33	5.13	9.81	--
	Fuji Dri-Chem NX500/i	19	54.63	4.81	8.80	1
	Fuji Dri-Chem 4000i	14	54.79	2.26	4.12	--
	Roche cobas c 311	11	33.52	5.45	16.25	1
	Roche cobas INTEGRA	6	32.00	2.93	9.15	1
	Roche cobas 6000	5	33.22	4.10	12.35	--
	Roche cobas 8000	3	32.14	4.54	14.11	--
	Roche cobas c 111	3	32.25	4.60	14.25	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Magnesium, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	53	2.04	0.16	7.73	6
■ Enzymatic	2	1.85	--	--	--
■ Fuji Nx 700	2	1.85	--	--	--

Your Result	1.90	SDI / z-Score	-0.44
Assigned Value	2.01	Average SDI	-0.15
SDPA	0.262	Uncertainty of AV	0.05
Standard Unit Result Val	1.90	%DEV	2.70

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

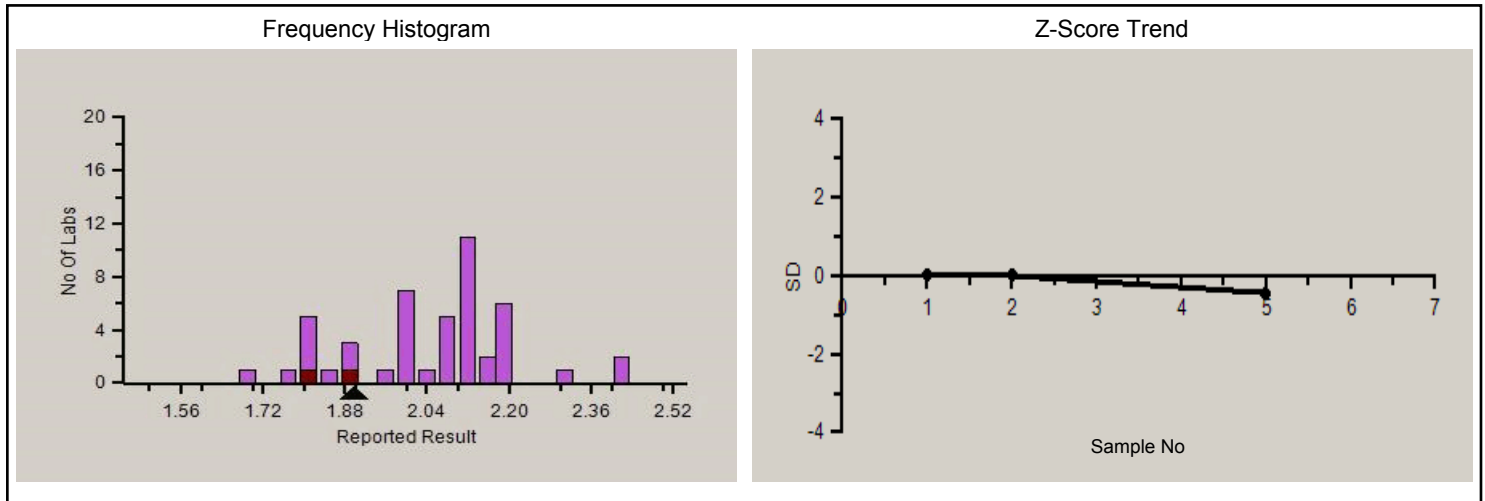

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, Magnesium		N	Mean	SD	CV%	Excluded
	All Analyzer	53	2.04	0.16	7.73	6
Your Analyzer :	Fuji Nx 700	2	1.85	--	--	--
	Fuji Dri-Chem NX500/i	16	2.04	0.20	9.55	2
	Fuji Dri-Chem 4000i	10	2.03	0.18	8.72	--
	Roche cobas c 311	7	2.10	0.08	4.01	--
	Roche cobas 6000	6	2.07	0.08	4.01	1
	Roche cobas 8000	4	2.11	0.08	3.98	--
	Roche cobas INTEGRA	2	2.02	--	--	1
	Beckman Coulter AU5800	1	--	--	--	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Phosphorous Inorganic, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	110	3.88	0.39	10.03	6
Phosphomolybdate method	57	3.63	0.23	6.25	3
RANDOX RX daytona	1	--	--	--	--

Your Result	3.50	SDI / z-Score	-0.33
Assigned Value	3.62	Average SDI	0.17
SDPA	0.362	Uncertainty of AV	0.03
Standard Unit Result Val	3.50	%DEV	-3.66

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

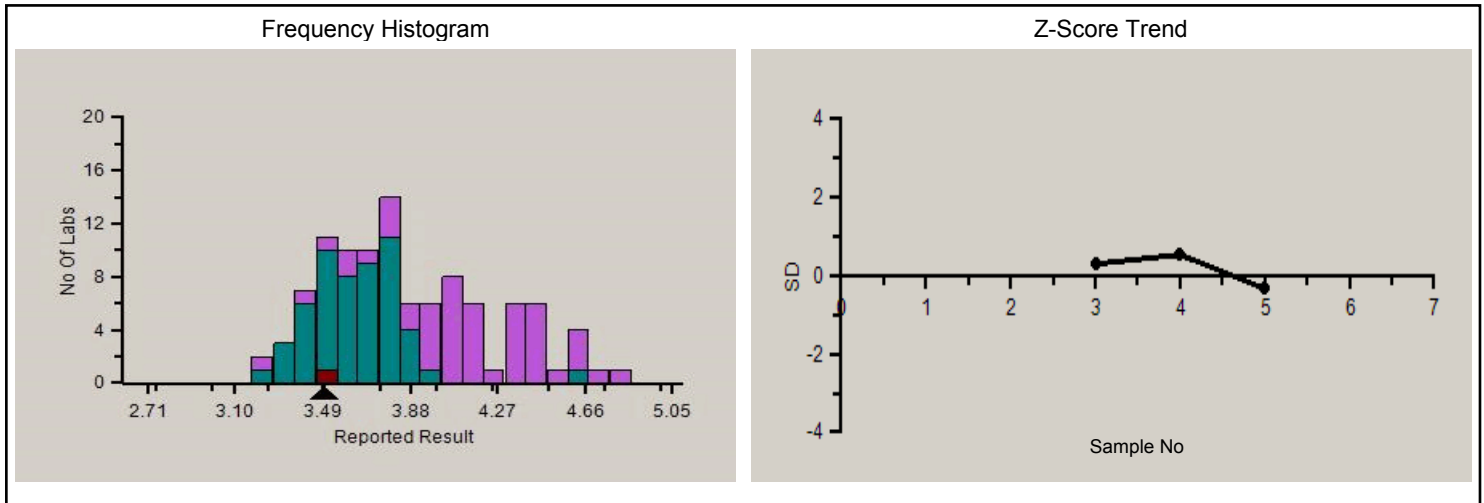

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, Phosphorous Inorganic						
	N	Mean	SD	CV%	Excluded	
All Analyzer	110	3.88	0.39	10.03	6	
Your Analyzer : RANDOX RX daytona	1	--	--	--	--	
Fuji Dri-Chem NX500/i	26	4.24	0.32	7.55	3	
Roche cobas c 311	22	3.64	0.19	5.19	--	
Fuji Dri-Chem 4000i	13	4.22	0.23	5.39	--	
Roche cobas 6000	8	3.54	0.18	5.00	--	
Roche cobas INTEGRA	7	3.66	0.17	4.72	--	
Roche cobas c 111	6	3.89	0.38	9.69	--	
Roche cobas 8000	4	3.55	0.22	6.11	--	
Beckman Coulter AU480	3	3.59	0.04	0.98	1	

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Urea, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	137	47.62	2.79	5.85	7
Urease, GLDH	16	47.56	4.02	8.45	--
RANDOX RX daytona	1	--	--	--	--

Your Result	50.00	SDI / z-Score	0.76
Assigned Value	47.76	Average SDI	1.07
SDPA	2.952	Uncertainty of AV	0.39
Standard Unit Result Val	50.00	%DEV	5.13

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

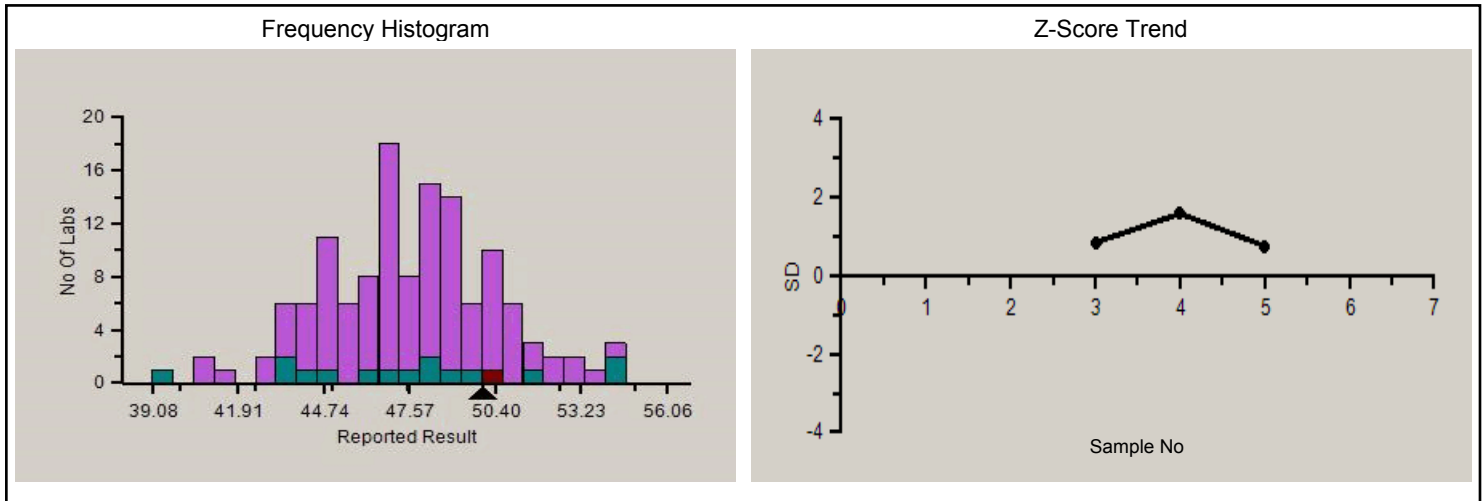

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021

Biochemistry, Urea		N	Mean	SD	CV%	Excluded
	All Analyzer	137	47.62	2.79	5.85	7
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Roche cobas c 311	27	49.40	1.50	3.04	--
	Fuji Dri-Chem NX500/i	25	47.59	2.18	4.57	4
	Fuji Dri-Chem 4000i	15	47.00	2.38	5.06	1
	Horiba ABX Pentra C200	12	45.25	4.30	9.50	--
	Roche cobas c 111	11	46.00	2.40	5.21	--
	Roche cobas c 111	10	46.50	1.83	3.93	--
	Roche cobas INTEGRA	9	45.40	1.39	3.05	--
	Roche cobas 6000	8	48.54	3.03	6.24	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS

Unit No. 409-416.
Commercial Building - 1A,
Kohinoor Mall, Kirool Road, Kuria (W),
Mumbai - 400070



PC-1022