

**Analyte Methodwise Result Report**

Lab : 427  
 Lab Name : VINAMRA SWARAJ HOSPITAL  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021


**Biochemistry, Albumin, g/dL**

	N	Mean	SD	CV%	Excluded
All Methods	166	3.97	0.46	11.62	6
Bromcresol Green (BCG)	158	3.97	0.46	11.50	5
RANDOX RX daytona	1	--	--	--	--

<b>Your Result</b>	3.60	<b>SDI / z-Score</b>	-0.42
<b>Assigned Value</b>	3.69	<b>Average SDI</b>	-0.43
<b>SDPA</b>	0.213	<b>Uncertainty of AV</b>	0.02
<b>Standard Unit Result Val</b>	3.60	<b>%DEV</b>	-9.41

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

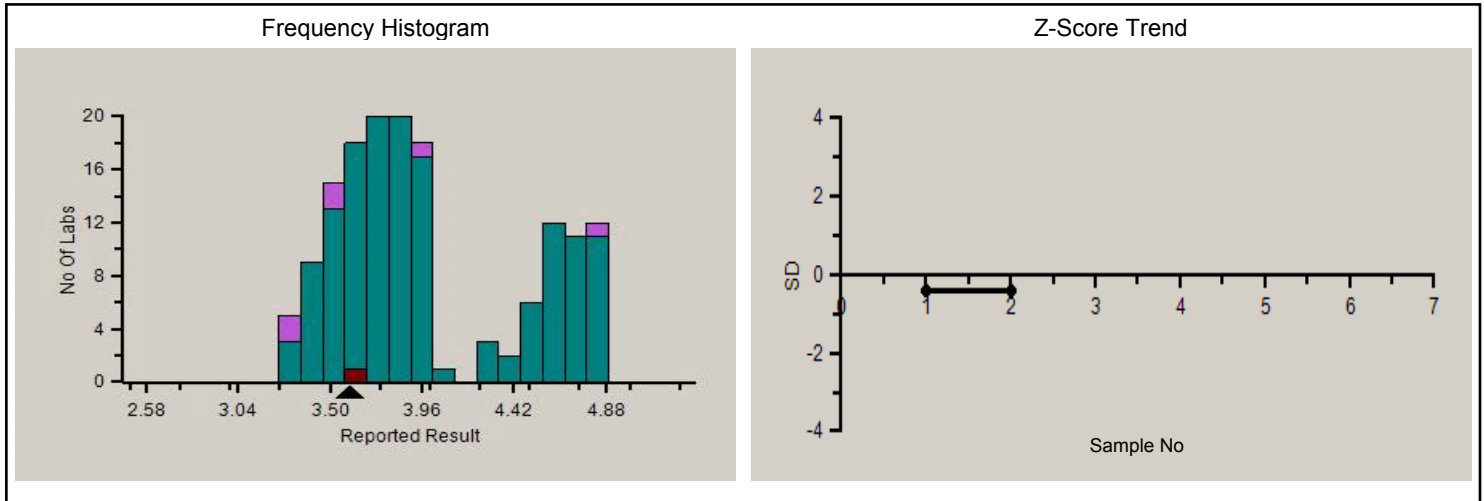

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 427  
 Lab Name : VINAMRA SWARAJ HOSPITAL  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

Biochemistry, Albumin		N	Mean	SD	CV%	Excluded
	All Analyzer	166	3.97	0.46	11.62	6
<b>Your Analyzer :</b>	<b>RANDOX RX daytona</b>	1	--	--	--	--
	Fuji Dri-Chem NX500/i	31	4.64	0.14	2.99	--
	Roche cobas c 311	27	3.79	0.11	2.98	--
	Fuji Dri-Chem 4000i	16	4.62	0.16	3.49	1
	Horiba ABX Pentra C200	10	3.51	0.11	3.02	1
	Roche cobas c 111	10	3.87	0.06	1.42	--
	Roche cobas INTEGRA	10	3.76	0.11	2.88	--
	Erba EM 200	8	3.55	0.09	2.45	--
	Roche cobas 6000	8	3.80	0.18	4.60	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, ALP, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	165	87.51	15.30	17.48	18
PNPP, AMP Buffer	77	95.81	16.01	16.71	7
RANDOX RX daytona	1	--	--	--	1

<b>Your Result</b>	54.00	<b>SDI / z-Score</b>	-1.68
<b>Assigned Value</b>	77.44	<b>Average SDI</b>	-1.16
<b>SDPA</b>	13.927	<b>Uncertainty of AV</b>	0.61
<b>Standard Unit Result Val</b>	54.00	<b>%DEV</b>	-43.64

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

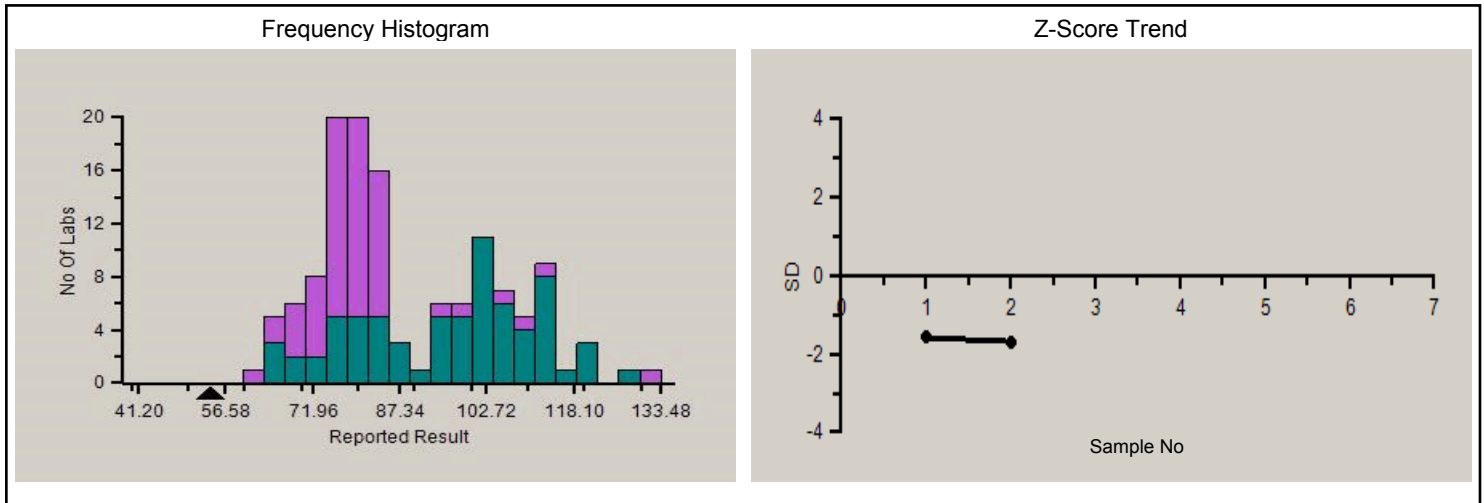

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 427  
 Lab Name : VINAMRA SWARAJ HOSPITAL  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

Biochemistry, ALP		N	Mean	SD	CV%	Excluded
	All Analyzer	165	87.51	15.30	17.48	18
<b>Your Analyzer :</b>	<b>RANDOX RX daytona</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	33	108.33	9.10	8.40	--
	Roche cobas c 311	27	77.38	3.66	4.73	--
	Fuji Dri-Chem 4000i	16	104.20	7.87	7.55	1
	Roche cobas c 111	11	75.16	6.85	9.11	--
	Horiba ABX Pentra C200	10	74.69	7.75	10.38	1
	Roche cobas INTEGRA	10	78.48	3.04	3.87	--
	Roche cobas 6000	8	78.38	3.38	4.31	--
	Erba EM 200	6	76.28	9.37	12.28	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, ALT, U/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	170	14.49	5.73	39.56	35
<span style="color: teal;">■</span> IFCC - UV without P5P	16	11.56	1.26	10.89	6
<span style="color: darkred;">■</span> RANDOX RX daytona	1	--	--	--	--

<b>Your Result</b>	11.00	<b>SDI / z-Score</b>	0.10
<b>Assigned Value</b>	10.77	<b>Average SDI</b>	0.65
<b>SDPA</b>	2.261	<b>Uncertainty of AV</b>	0.16
<b>Standard Unit Result Val</b>	11.00	<b>%DEV</b>	-4.84

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

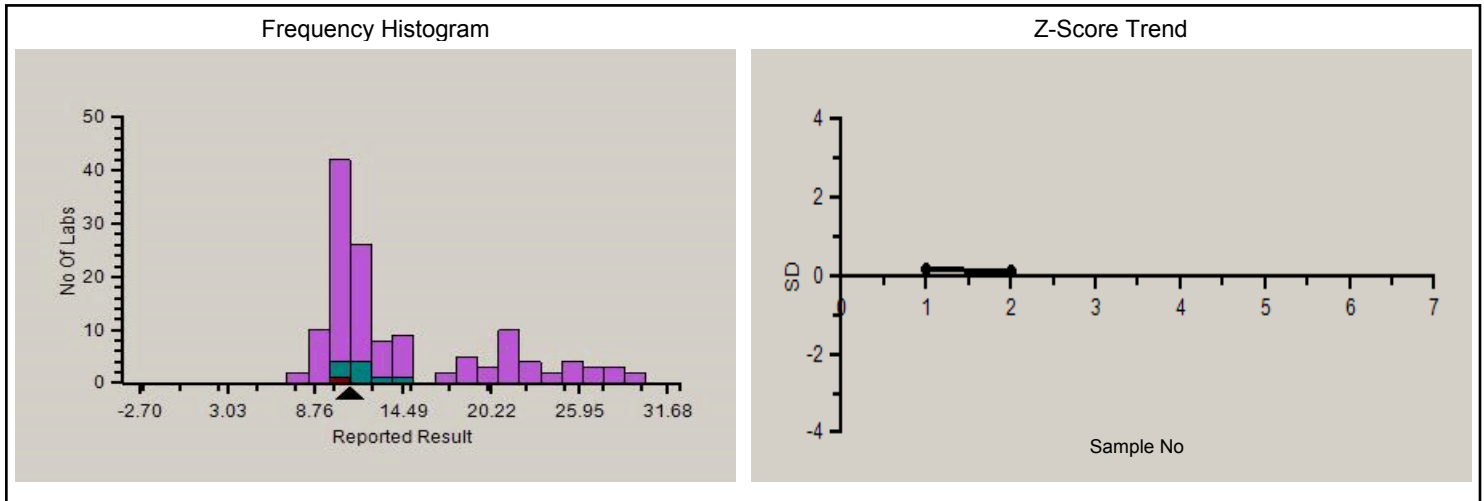

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 427  
 Lab Name : VINAMRA SWARAJ HOSPITAL  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

Biochemistry, ALT		N	Mean	SD	CV%	Excluded
	All Analyzer	170	14.49	5.73	39.56	35
<b>Your Analyzer :</b>	<b>RANDOX RX daytona</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	32	23.11	3.35	14.49	11
	Roche cobas c 311	27	10.81	1.27	11.77	1
	Fuji Dri-Chem 4000i	16	23.36	2.50	10.71	5
	Horiba ABX Pentra C200	11	11.23	1.29	11.50	1
	Roche cobas c 111	11	10.09	1.24	12.30	2
	Roche cobas INTEGRA	10	10.00	0.92	9.15	1
	Erba EM 200	8	13.41	1.77	13.16	1
	Roche cobas 6000	8	10.74	0.70	6.55	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, Amylase, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	99	60.37	7.20	11.93	10
G7 PNP	66	60.94	6.20	10.17	3
RANDOX RX daytona	1	--	--	--	--

<b>Your Result</b>	73.00	<b>SDI / z-Score</b>	0.76
<b>Assigned Value</b>	67.35	<b>Average SDI</b>	1.04
<b>SDPA</b>	7.408	<b>Uncertainty of AV</b>	0.41
<b>Standard Unit Result Val</b>	73.00	<b>%DEV</b>	19.78

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

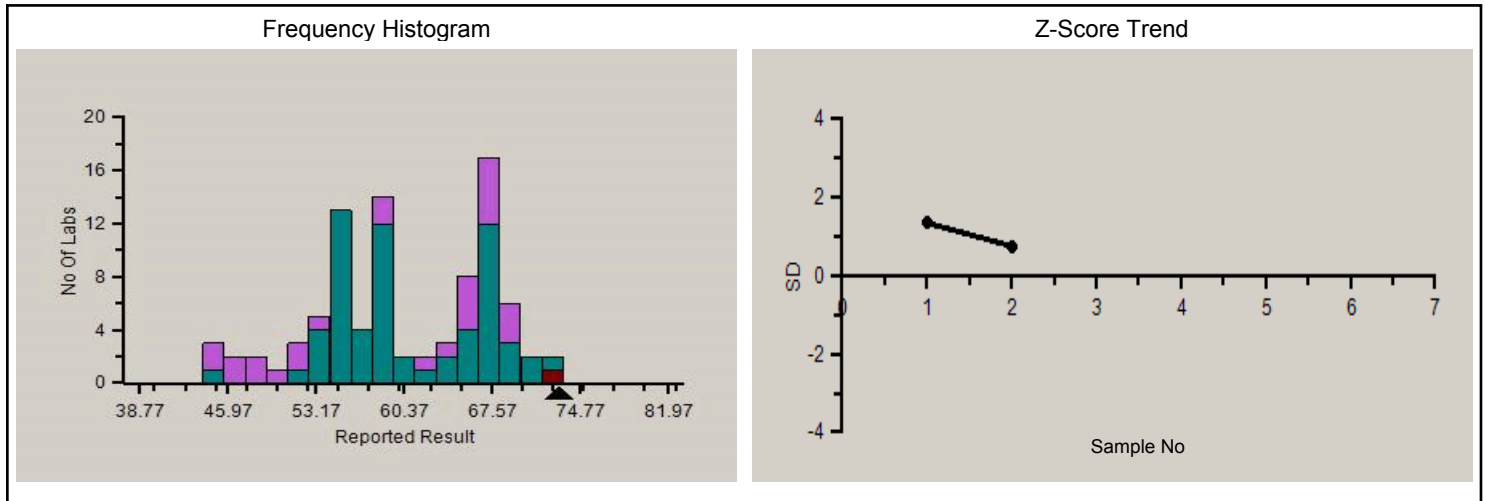

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 427  
 Lab Name : VINAMRA SWARAJ HOSPITAL  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

Biochemistry, Amylase		N	Mean	SD	CV%	Excluded
	All Analyzer	99	60.37	7.20	11.93	10
<b>Your Analyzer :</b>	<b>RANDOX RX daytona</b>	1	--	--	--	--
	Fuji Dri-Chem NX500/i	23	57.00	2.56	4.49	--
	Fuji Dri-Chem 4000i	14	56.43	1.91	3.39	--
	Roche cobas c 311	14	67.64	2.26	3.35	--
	Roche cobas INTEGRA	7	66.98	2.53	3.77	--
	Roche cobas 6000	6	67.18	1.46	2.17	--
	Roche cobas 8000	4	67.75	0.96	1.41	--
	Roche cobas c 111	3	66.90	2.97	4.44	1
	Star 20	3	--	--	--	3

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.





**Analyte Methodwise Result Report**

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, AST, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	167	19.79	2.98	15.05	22
IFCC - UV without P5P	14	18.60	1.39	7.47	5
RANDOX RX daytona	1	--	--	--	--

<b>Your Result</b>	18.00	<b>SDI / z-Score</b>	0.03
<b>Assigned Value</b>	17.88	<b>Average SDI</b>	-0.24
<b>SDPA</b>	3.576	<b>Uncertainty of AV</b>	0.22
<b>Standard Unit Result Val</b>	18.00	<b>%DEV</b>	-3.20

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

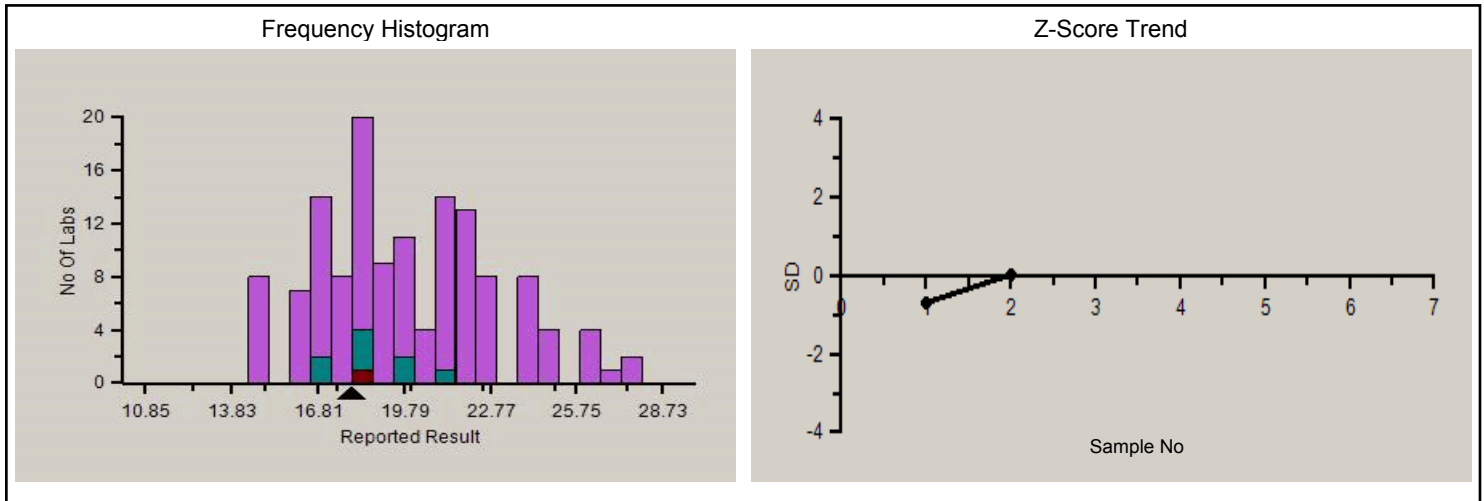

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 427  
 Lab Name : VINAMRA SWARAJ HOSPITAL  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

Biochemistry, AST		N	Mean	SD	CV%	Excluded
	All Analyzer	167	19.79	2.98	15.05	22
<b>Your Analyzer :</b>	<b>RANDOX RX daytona</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	32	23.35	2.33	9.99	6
	Roche cobas c 311	26	17.90	1.41	7.87	--
	Fuji Dri-Chem 4000i	16	22.19	2.14	9.63	--
	Roche cobas c 111	12	17.81	1.64	9.18	1
	Horiba ABX Pentra C200	10	18.07	1.63	9.01	--
	Roche cobas INTEGRA	10	16.50	1.09	6.57	1
	Erba EM 200	8	19.33	2.97	15.35	4
	Roche cobas 6000	8	17.30	0.78	4.50	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, Bilirubin Direct, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	164	0.10	0.02	15.53	39
<span style="color: teal;">■</span> DMSO	1	--	--	--	1
<span style="color: darkred;">■</span> RANDOX RX daytona	1	--	--	--	1

<b>Your Result</b>	0.19	<b>SDI / z-Score</b>	2.09
<b>Assigned Value</b>	0.10	<b>Average SDI</b>	0.99
<b>SDPA</b>	0.044	<b>Uncertainty of AV</b>	0.01
<b>Standard Unit Result Val</b>	0.19	<b>%DEV</b>	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

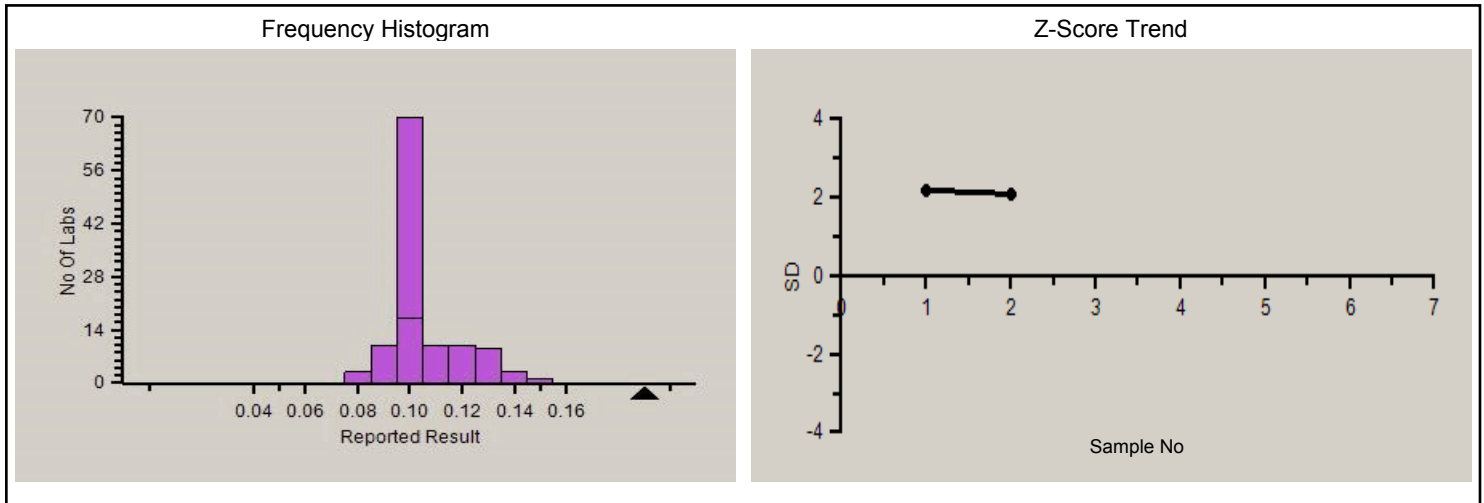

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021

Biochemistry, Bilirubin Direct		N	Mean	SD	CV%	Excluded
	All Analyzer	164	0.10	0.02	15.53	39
<b>Your Analyzer :</b>	<b>RANDOX RX daytona</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	28	0.10	0.00	4.04	8
	Roche cobas c 311	26	0.09	0.01	13.19	3
	Fuji Dri-Chem 4000i	16	0.10	0.00	0.00	6
	Horiba ABX Pentra C200	11	0.12	0.01	10.17	--
	Roche cobas c 111	11	0.11	0.01	12.73	3
	Roche cobas INTEGRA	10	0.10	0.01	7.00	--
	Erba EM 200	8	0.13	0.03	25.56	2
	Roche cobas 6000	8	0.10	0.01	8.42	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, Bilirubin Total, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	167	0.33	0.14	42.81	43
<span style="color: teal;">■</span> DMSO	1	--	--	--	1
<span style="color: darkred;">■</span> RANDOX RX daytona	1	--	--	--	1

<b>Your Result</b>	0.57	<b>SDI / z-Score</b>	2.42
<b>Assigned Value</b>	0.33	<b>Average SDI</b>	1.97
<b>SDPA</b>	0.099	<b>Uncertainty of AV</b>	0.02
<b>Standard Unit Result Val</b>	0.57	<b>%DEV</b>	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

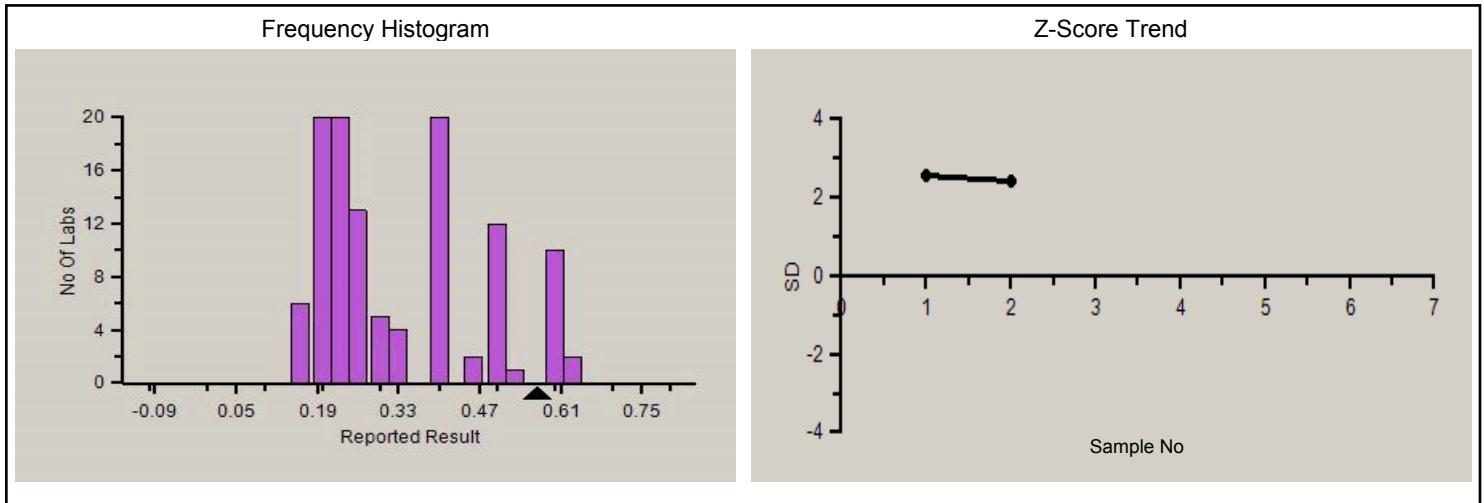

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 427  
 Lab Name : VINAMRA SWARAJ HOSPITAL  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

<b>Biochemistry, Bilirubin Total</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	167	0.33	0.14	42.81	43
<b>Your Analyzer :</b>	<b>RANDOX RX daytona</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	30	0.49	0.08	17.11	7
	Roche cobas c 311	26	0.21	0.03	13.53	3
	Fuji Dri-Chem 4000i	16	0.51	0.09	17.36	1
	Horiba ABX Pentra C200	11	0.24	0.02	9.92	6
	Roche cobas c 111	10	0.22	0.04	20.47	4
	Roche cobas INTEGRA	10	0.20	0.02	9.55	1
	Erba EM 200	8	0.24	0.04	16.88	1
	Roche cobas 6000	8	0.19	0.02	12.37	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, Calcium, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	156	7.58	0.57	7.57	8
Arsenazo III	53	7.84	0.49	6.23	5
RANDOX RX daytona	1	--	--	--	--

<b>Your Result</b>	8.00	<b>SDI / z-Score</b>	-0.23
<b>Assigned Value</b>	8.20	<b>Average SDI</b>	-0.29
<b>SDPA</b>	0.887	<b>Uncertainty of AV</b>	0.45
<b>Standard Unit Result Val</b>	8.00	<b>%DEV</b>	2.07

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

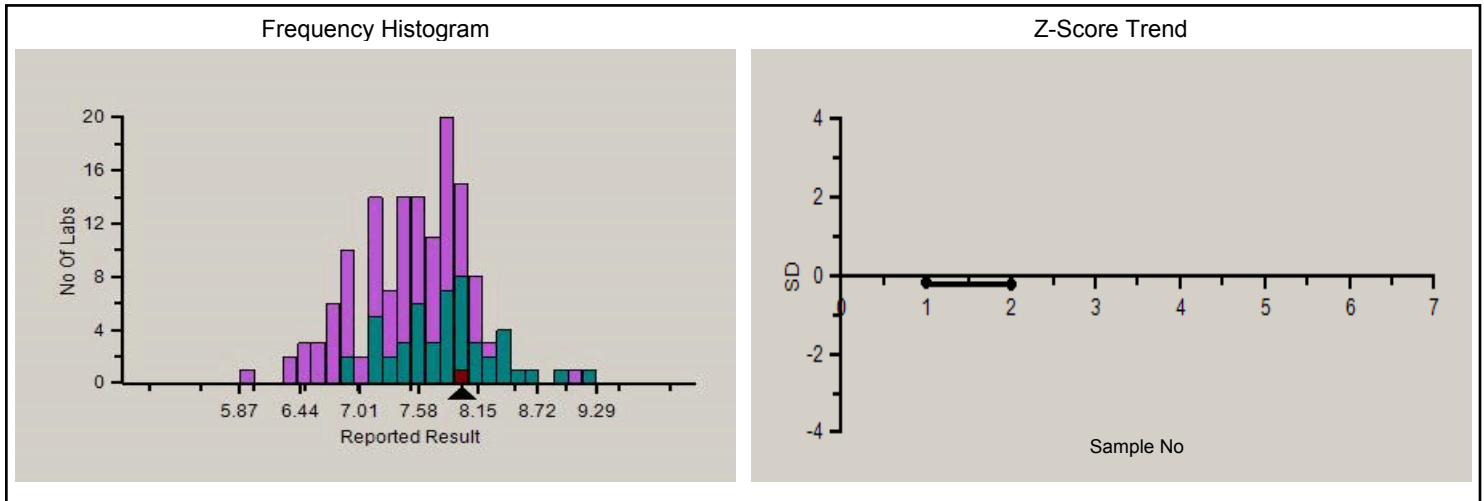

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 427  
 Lab Name : VINAMRA SWARAJ HOSPITAL  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

Biochemistry, Calcium		N	Mean	SD	CV%	Excluded
	All Analyzer	156	7.58	0.57	7.57	8
<b>Your Analyzer :</b>	<b>RANDOX RX daytona</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	28	6.90	0.32	4.61	--
	Roche cobas c 311	24	7.86	0.22	2.81	--
	Fuji Dri-Chem 4000i	16	7.06	0.48	6.73	--
	Roche cobas INTEGRA	11	7.75	0.28	3.67	--
	Roche cobas c 111	10	7.75	0.21	2.67	--
	Roche cobas 6000	7	7.76	0.14	1.84	1
	Erba EM 200	6	8.43	0.60	7.13	--
	Beckman Coulter AU480	5	7.89	0.19	2.36	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022



**Analyte Methodwise Result Report**

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, Chloride, mEq/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	138	105.29	12.55	11.92	15
<span style="color: teal;">■</span> ISE direct	94	0.00	0.00	0.00	8
<span style="color: darkred;">■</span> EasyLyte	8	0.00	0.00	0.00	1

<b>Your Result</b>	109.50	<b>SDI / z-Score</b>	-0.51
<b>Assigned Value</b>	113.22	<b>Average SDI</b>	-0.53
<b>SDPA</b>	7.350	<b>Uncertainty of AV</b>	0.48
<b>Standard Unit Result Val</b>	109.50	<b>%DEV</b>	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

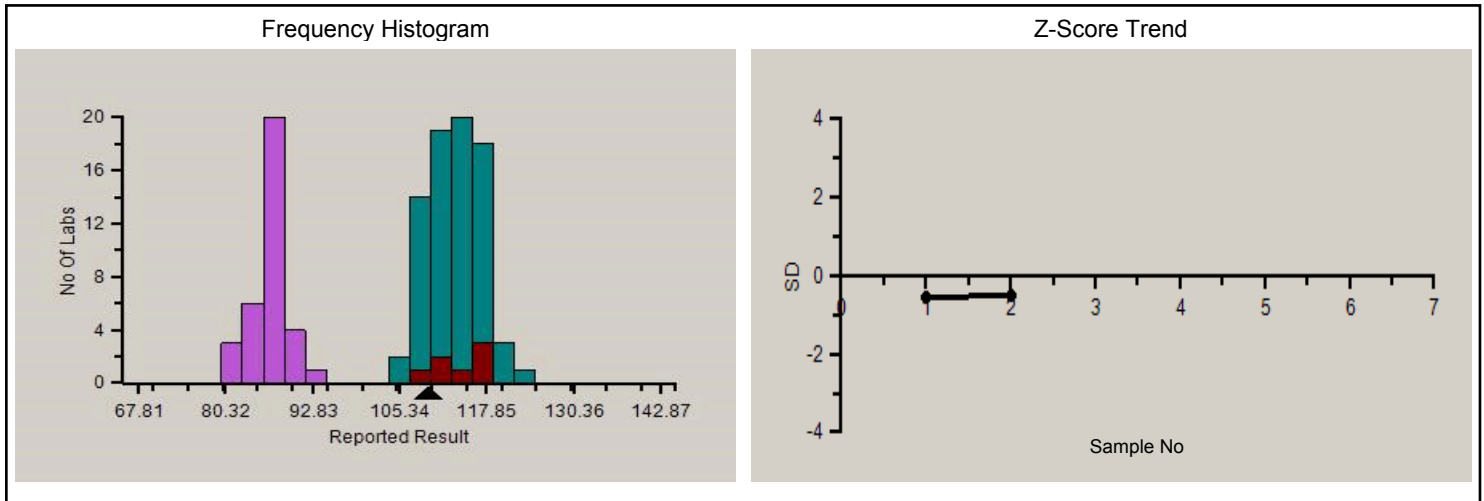

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427  
 Lab Name : VINAMRA SWARAJ HOSPITAL  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

Biochemistry, Chloride		N	Mean	SD	CV%	Excluded
	All Analyzer	138	105.29	12.55	11.92	15
<b>Your Analyzer :</b>	<b>EasyLyte</b>	<b>8</b>	<b>0.00</b>	<b>0.00</b>	<b>0.00</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	32	0.00	0.00	0.00	1
	Fuji Dri-Chem 4000i	17	0.00	0.00	0.00	1
	Roche cobas c 311	15	0.00	0.00	0.00	--
	Roche AVL 9180	11	108.93	1.85	1.70	--
	Roche AVL 9180	10	0.00	0.00	0.00	--
	Roche cobas 6000	8	0.00	0.00	0.00	1
	Roche cobas 8000	4	0.00	0.00	0.00	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, CK, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	76	85.17	15.66	18.39	5
Colorimetric	1	--	--	--	--
Fuji Nx 700	3	75.33	2.52	3.34	--

<b>Your Result</b>	78.00	<b>SDI / z-Score</b>	0.75
<b>Assigned Value</b>	71.26	<b>Average SDI</b>	0.05
<b>SDPA</b>	8.998	<b>Uncertainty of AV</b>	1.90
<b>Standard Unit Result Val</b>	78.00	<b>%DEV</b>	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

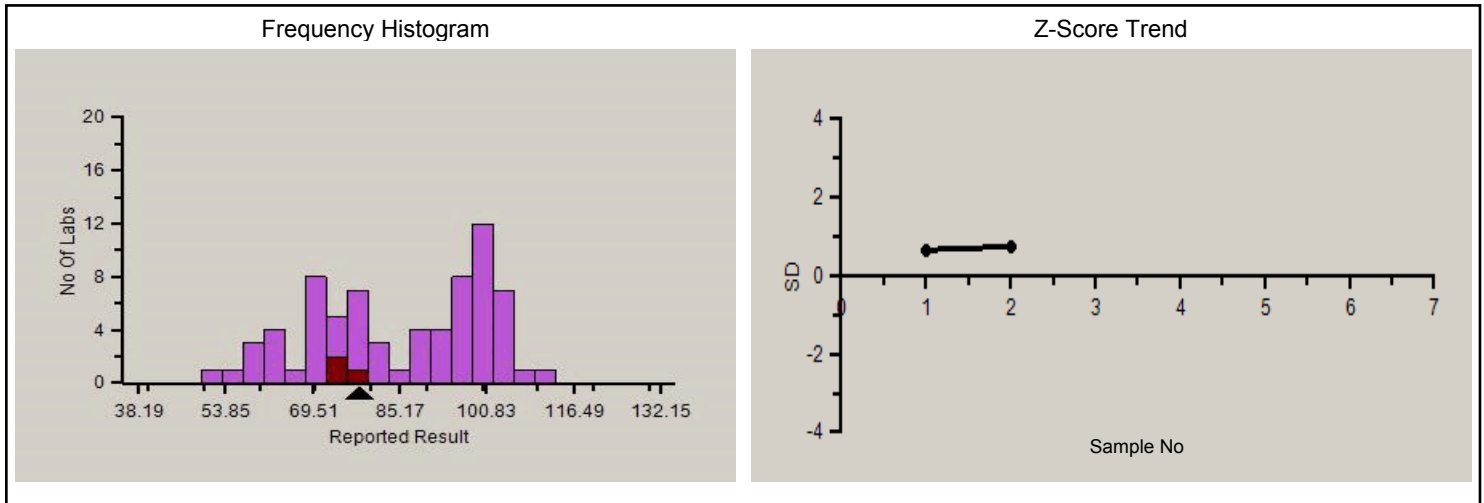

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427  
 Lab Name : VINAMRA SWARAJ HOSPITAL  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

Biochemistry, CK		N	Mean	SD	CV%	Excluded
	All Analyzer	76	85.17	15.66	18.39	5
<b>Your Analyzer :</b>	<b>Fuji Nx 700</b>	<b>3</b>	<b>75.33</b>	<b>2.52</b>	<b>3.34</b>	--
	Fuji Dri-Chem NX500/i	21	70.55	10.45	14.81	1
	Roche cobas c 311	13	99.33	3.90	3.93	--
	Fuji Dri-Chem 4000i	11	71.73	6.75	9.42	--
	Roche cobas INTEGRA	7	97.87	6.63	6.77	--
	Roche cobas 6000	5	96.82	2.29	2.37	--
	Roche cobas 8000	4	99.75	2.75	2.76	--
	Star 20	2	--	--	--	2

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, GGT, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	135	15.19	4.08	26.87	7
IFCC	12	15.74	3.82	24.27	--
RANDOX RX daytona	1	--	--	--	--

<b>Your Result</b>	20.00	<b>SDI / z-Score</b>	1.17
<b>Assigned Value</b>	17.54	<b>Average SDI</b>	0.88
<b>SDPA</b>	2.104	<b>Uncertainty of AV</b>	0.24
<b>Standard Unit Result Val</b>	20.00	<b>%DEV</b>	27.05

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

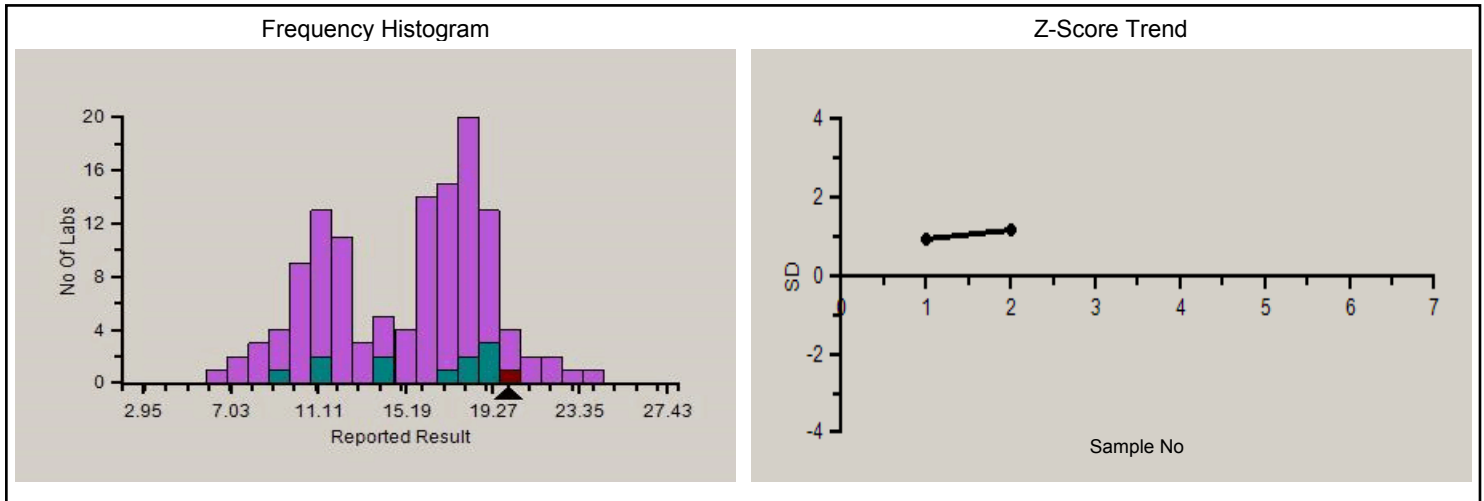

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 427  
 Lab Name : VINAMRA SWARAJ HOSPITAL  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

Biochemistry, GGT		N	Mean	SD	CV%	Excluded
	All Analyzer	135	15.19	4.08	26.87	7
<b>Your Analyzer :</b>	<b>RANDOX RX daytona</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	32	11.17	1.28	11.49	3
	Roche cobas c 311	24	17.57	1.20	6.83	1
	Fuji Dri-Chem 4000i	12	10.33	1.16	11.18	--
	Roche cobas INTEGRA	11	16.07	1.33	8.25	--
	Roche cobas c 111	10	17.46	3.05	17.48	1
	Horiba ABX Pentra C200	6	16.93	1.82	10.75	--
	Roche cobas 6000	6	17.33	1.37	7.88	--
	Beckman Coulter AU480	5	18.10	0.94	5.18	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, LDH, U/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	93	144.19	48.59	33.70	7
<span style="color: teal;">■</span> L to P - IFCC Ref. Proc., Calibrated	3	121.33	34.36	28.32	--
<span style="color: darkred;">■</span> Fuji Nx 700	3	106.67	4.04	3.79	--

<b>Your Result</b>	102.00	<b>SDI / z-Score</b>	-1.10
<b>Assigned Value</b>	110.86	<b>Average SDI</b>	-0.67
<b>SDPA</b>	8.026	<b>Uncertainty of AV</b>	1.61
<b>Standard Unit Result Val</b>	102.00	<b>%DEV</b>	-15.93

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

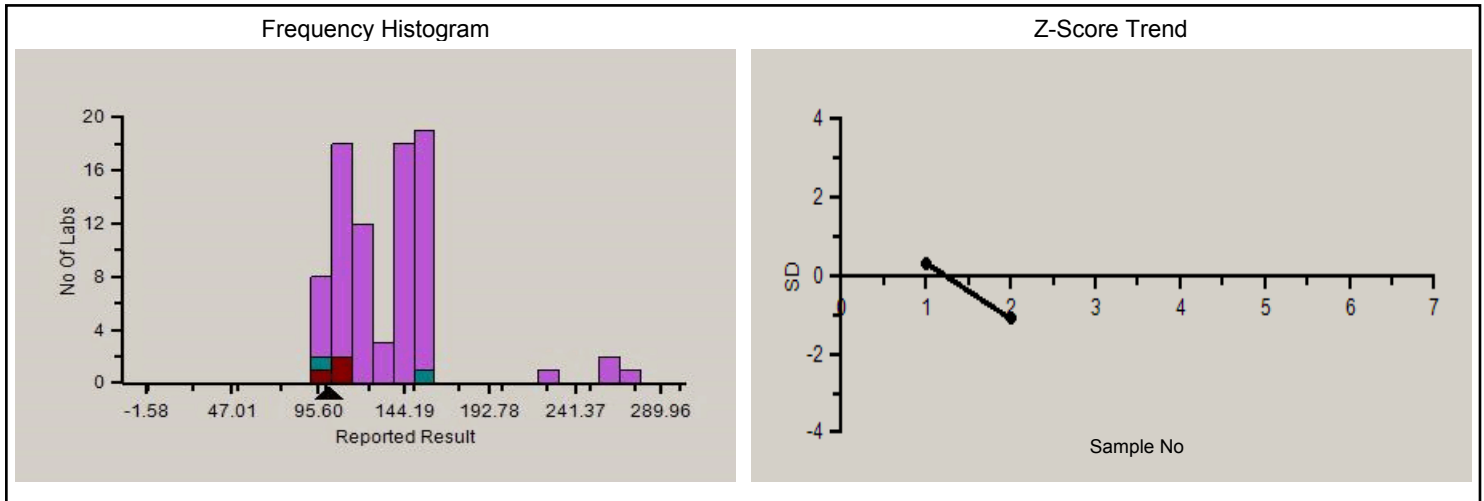

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427  
 Lab Name : VINAMRA SWARAJ HOSPITAL  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

Biochemistry, LDH		N	Mean	SD	CV%	Excluded
	All Analyzer	93	144.19	48.59	33.70	7
<b>Your Analyzer :</b>	<b>Fuji Nx 700</b>	<b>3</b>	<b>106.67</b>	<b>4.04</b>	<b>3.79</b>	--
	Fuji Dri-Chem NX500/i	24	110.46	7.38	6.68	--
	Fuji Dri-Chem 4000i	12	113.83	8.78	7.71	--
	Roche cobas c 311	11	149.36	5.09	3.40	--
	Roche cobas INTEGRA	7	148.56	3.73	2.51	--
	Roche cobas 6000	6	151.30	4.80	3.17	--
	Beckman Coulter AU480	4	268.20	0.00	0.00	--
	Roche cobas 8000	4	150.25	1.89	1.26	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022



**Analyte Methodwise Result Report**

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, Lipase, U/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	80	47.49	14.45	30.42	7
<span style="color: teal;">■</span> Enzymatic colorimetric	14	44.43	11.50	25.89	3
<span style="color: darkred;">■</span> Fuji Nx 700	3	55.33	7.10	12.82	--

<b>Your Result</b>	54.00	<b>SDI / z-Score</b>	-0.09
<b>Assigned Value</b>	54.41	<b>Average SDI</b>	-0.41
<b>SDPA</b>	4.841	<b>Uncertainty of AV</b>	0.99
<b>Standard Unit Result Val</b>	54.00	<b>%DEV</b>	21.54

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

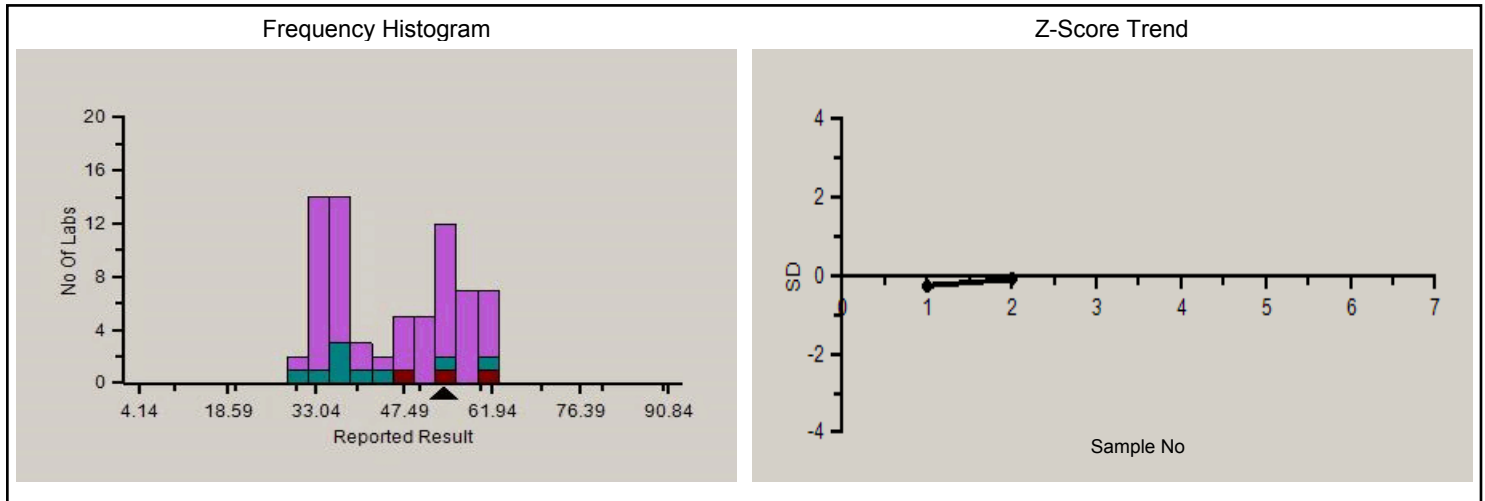

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427  
 Lab Name : VINAMRA SWARAJ HOSPITAL  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

Biochemistry, Lipase		N	Mean	SD	CV%	Excluded
	All Analyzer	80	47.49	14.45	30.42	7
<b>Your Analyzer :</b>	<b>Fuji Nx 700</b>	<b>3</b>	<b>55.33</b>	<b>7.10</b>	<b>12.82</b>	--
	Fuji Dri-Chem NX500/i	22	53.00	5.18	9.78	2
	Fuji Dri-Chem 4000i	14	55.86	3.30	5.91	--
	Roche cobas c 311	12	36.52	1.50	4.12	--
	Roche cobas INTEGRA	6	35.27	2.43	6.88	--
	Roche cobas 6000	5	35.04	1.29	3.69	--
	Roche cobas 8000	3	34.69	4.73	13.63	--
	Roche cobas c 111	2	36.70	--	--	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, Magnesium, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	55	1.07	0.67	62.72	6
Enzymatic	2	0.50	--	--	1
Fuji Nx 700	2	0.45	--	--	--

<b>Your Result</b>	0.50	<b>SDI / z-Score</b>	0.00
<b>Assigned Value</b>	0.50	<b>Average SDI</b>	-0.15
<b>SDPA</b>	0.070	<b>Uncertainty of AV</b>	0.01
<b>Standard Unit Result Val</b>	0.50	<b>%DEV</b>	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

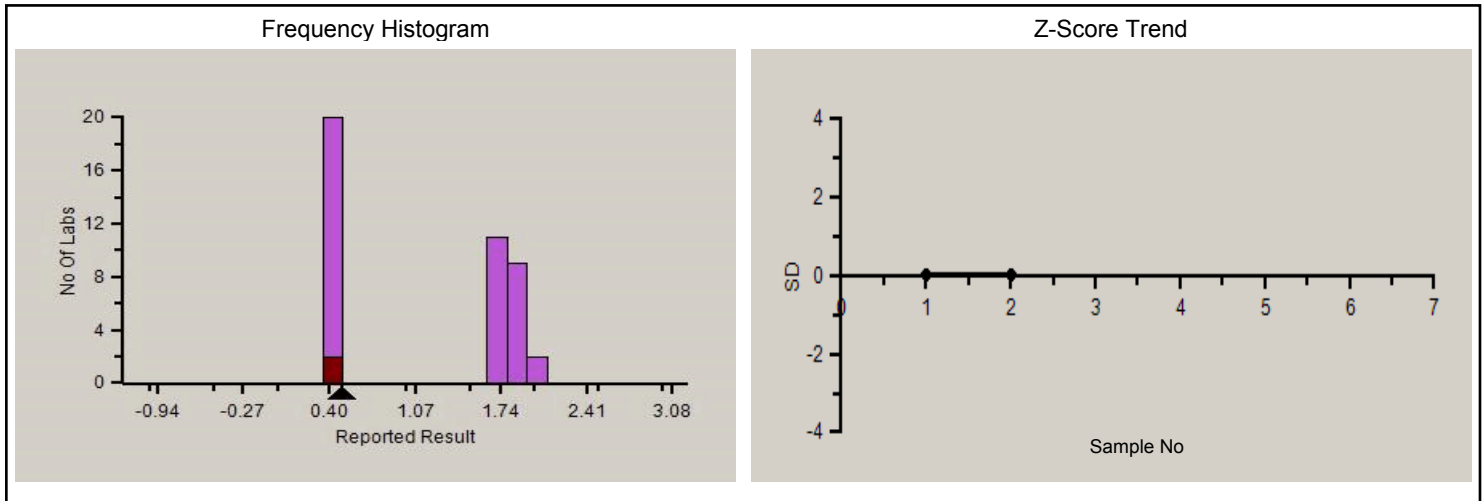

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427  
 Lab Name : VINAMRA SWARAJ HOSPITAL  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

Biochemistry, Magnesium		N	Mean	SD	CV%	Excluded
	All Analyzer	55	1.07	0.67	62.72	6
<b>Your Analyzer :</b>	<b>Fuji Nx 700</b>	<b>2</b>	<b>0.45</b>	--	--	--
	Fuji Dri-Chem NX500/i	17	0.47	0.03	7.27	2
	Fuji Dri-Chem 4000i	10	0.48	0.04	8.75	--
	Roche cobas c 311	7	1.75	0.04	2.23	--
	Roche cobas 6000	6	1.77	0.08	4.64	--
	Roche cobas 8000	4	1.89	0.09	4.83	--
	Roche cobas INTEGRA	2	1.70	--	--	1
	Beckman Coulter AU5800	1	--	--	--	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, Potassium, mEq/L**

	N	Mean	SD	CV%	Excluded
All Methods	149	5.70	0.93	16.35	10
ISE direct	104	0.00	0.00	0.00	3
EasyLyte	9	0.00	0.00	0.00	--

<b>Your Result</b>	5.64	<b>SDI / z-Score</b>	-1.78
<b>Assigned Value</b>	6.25	<b>Average SDI</b>	-1.85
<b>SDPA</b>	0.343	<b>Uncertainty of AV</b>	0.04
<b>Standard Unit Result Val</b>	5.64	<b>%DEV</b>	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

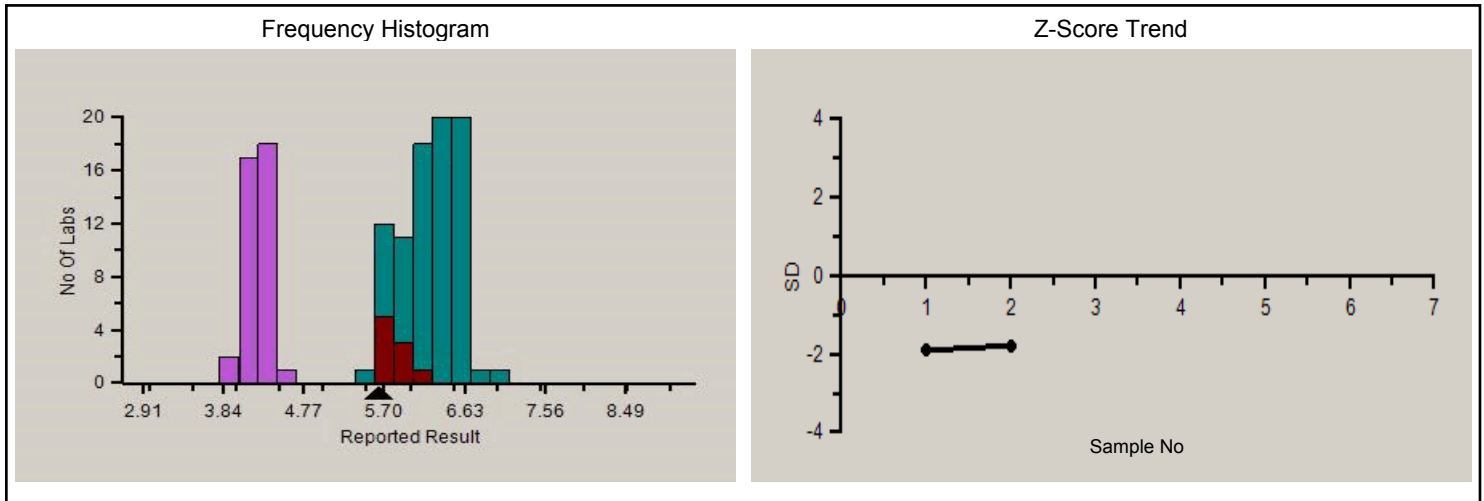

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 427  
 Lab Name : VINAMRA SWARAJ HOSPITAL  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

<b>Biochemistry, Potassium</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	149	5.70	0.93	16.35	10
<b>Your Analyzer :</b>	<b>EasyLyte</b>	<b>9</b>	<b>0.00</b>	<b>0.00</b>	<b>0.00</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	33	0.00	0.00	0.00	1
	Fuji Dri-Chem 4000i	19	0.00	0.00	0.00	1
	Roche cobas c 311	15	0.00	0.00	0.00	--
	Roche AVL 9180	13	6.27	0.37	5.87	--
	Roche AVL 9180	12	0.00	0.00	0.00	--
	Roche cobas 6000	8	0.00	0.00	0.00	--
	Sensa Core	5	0.00	0.00	0.00	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, Sodium, mEq/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	149	159.00	23.11	14.54	15
<span style="color: teal;">■</span> ISE direct	104	0.00	0.00	0.00	8
<span style="color: darkred;">■</span> EasyLyte	9	0.00	0.00	0.00	2

<b>Your Result</b>	168.50	<b>SDI / z-Score</b>	-0.57
<b>Assigned Value</b>	173.43	<b>Average SDI</b>	-0.57
<b>SDPA</b>	8.671	<b>Uncertainty of AV</b>	0.46
<b>Standard Unit Result Val</b>	168.50	<b>%DEV</b>	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

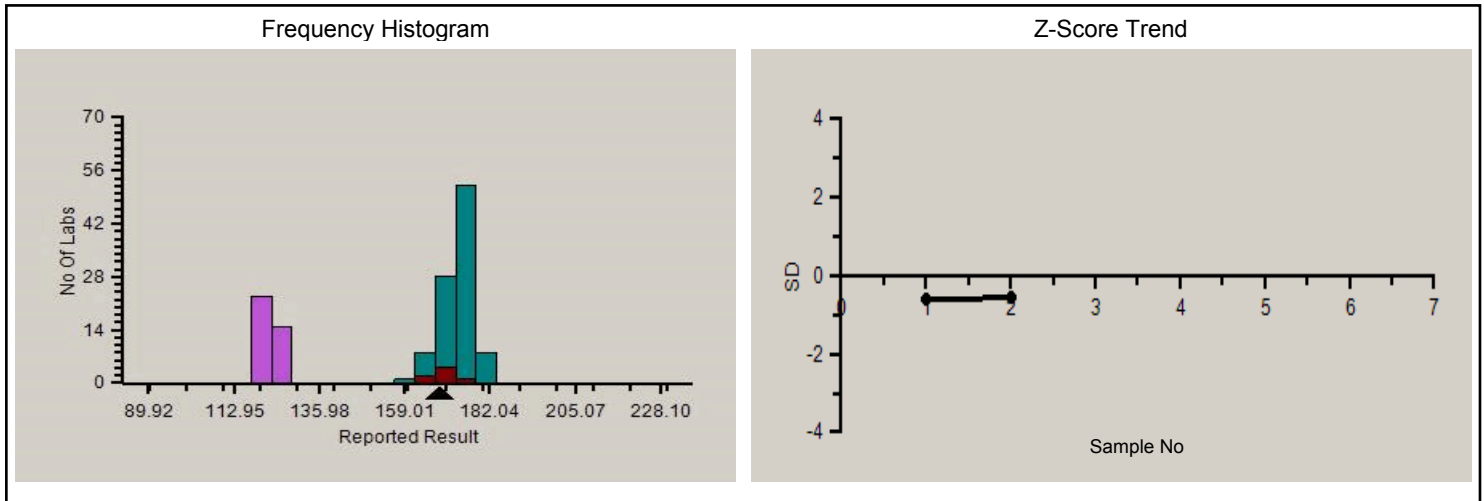

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427  
 Lab Name : VINAMRA SWARAJ HOSPITAL  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

Biochemistry, Sodium		N	Mean	SD	CV%	Excluded
	All Analyzer	149	159.00	23.11	14.54	15
<b>Your Analyzer :</b>	<b>EasyLyte</b>	<b>9</b>	<b>0.00</b>	<b>0.00</b>	<b>0.00</b>	<b>2</b>
	Fuji Dri-Chem NX500/i	34	0.00	0.00	0.00	3
	Fuji Dri-Chem 4000i	18	0.00	0.00	0.00	2
	Roche cobas c 311	15	0.00	0.00	0.00	--
	Roche AVL 9180	13	174.85	6.33	3.62	--
	Roche AVL 9180	12	0.00	0.00	0.00	--
	Roche cobas 6000	8	0.00	0.00	0.00	--
	Sensa Core	5	0.00	0.00	0.00	1

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022



**Analyte Methodwise Result Report**

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, Total Protein, g/dL**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	164	6.40	0.32	5.03	4
<span style="color: teal;">■</span> Biuret	161	6.40	0.32	5.03	4
<span style="color: darkred;">■</span> RANDOX RX daytona	1	--	--	--	--

<b>Your Result</b>	6.20	<b>SDI / z-Score</b>	-0.42
<b>Assigned Value</b>	6.31	<b>Average SDI</b>	-0.36
<b>SDPA</b>	0.252	<b>Uncertainty of AV</b>	0.03
<b>Standard Unit Result Val</b>	6.20	<b>%DEV</b>	-3.14

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

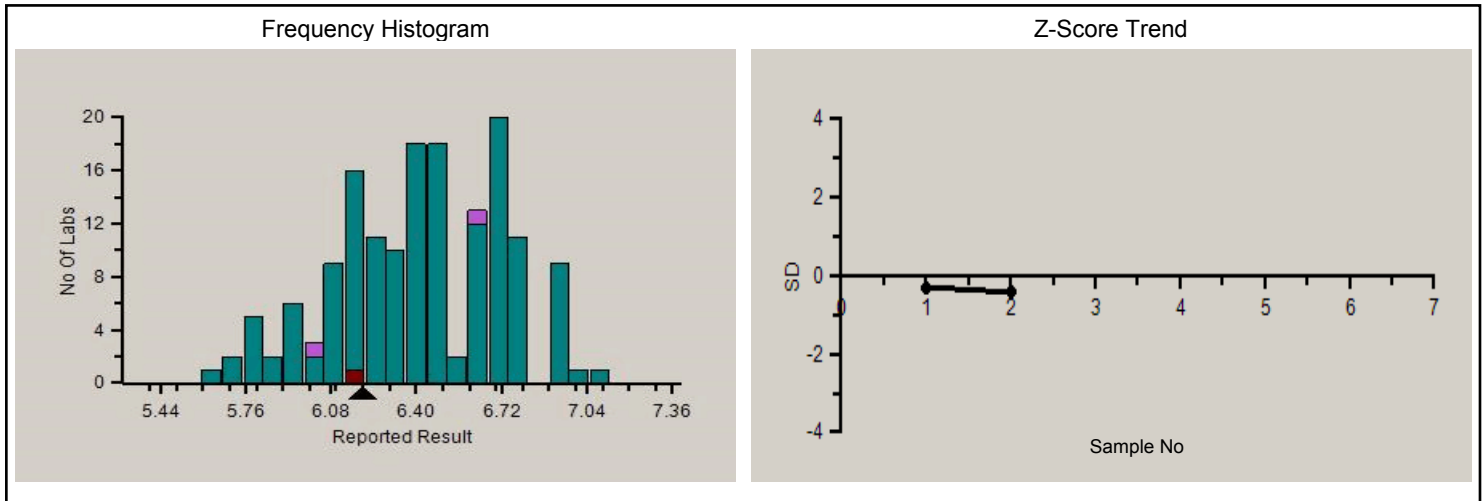

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 427  
 Lab Name : VINAMRA SWARAJ HOSPITAL  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

<b>Biochemistry, Total Protein</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	164	6.40	0.32	5.03	4
<b>Your Analyzer :</b>	<b>RANDOX RX daytona</b>	1	--	--	--	--
	Fuji Dri-Chem NX500/i	30	6.73	0.16	2.32	--
	Roche cobas c 311	27	6.37	0.19	3.04	--
	Fuji Dri-Chem 4000i	16	6.69	0.17	2.47	--
	Roche cobas c 111	11	6.27	0.29	4.69	--
	Roche cobas INTEGRA	10	6.12	0.26	4.23	--
	Horiba ABX Pentra C200	9	6.32	0.30	4.67	--
	Erba EM 200	8	6.31	0.29	4.52	1
	Roche cobas 6000	8	6.42	0.14	2.21	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, Triglycerides, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	164	110.59	9.47	8.56	10
<span style="color: teal;">■</span> GPO-PAP	14	116.69	7.08	6.07	1
<span style="color: darkred;">■</span> RANDOX RX daytona	1	--	--	--	--

<b>Your Result</b>	124.00	<b>SDI / z-Score</b>	0.65
<b>Assigned Value</b>	115.00	<b>Average SDI</b>	0.41
<b>SDPA</b>	13.799	<b>Uncertainty of AV</b>	0.84
<b>Standard Unit Result Val</b>	124.00	<b>%DEV</b>	6.27

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

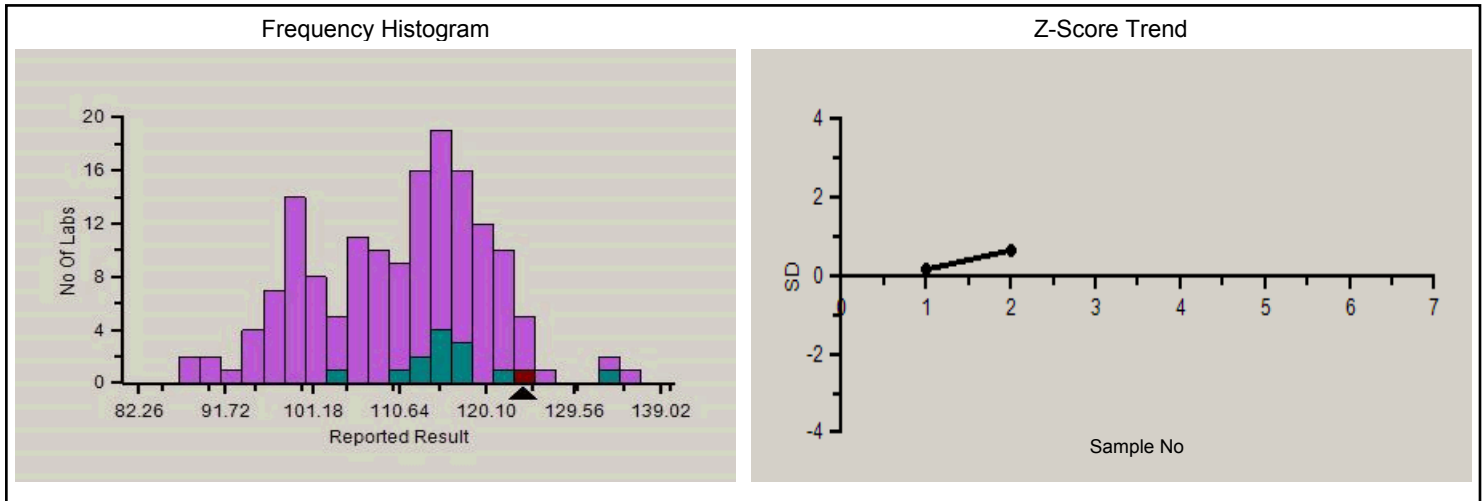

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 427  
 Lab Name : VINAMRA SWARAJ HOSPITAL  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

<b>Biochemistry, Triglycerides</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	164	110.59	9.47	8.56	10
<b>Your Analyzer :</b>	<b>RANDOX RX daytona</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	32	101.86	7.47	7.33	--
	Roche cobas c 311	27	116.34	7.35	6.32	2
	Fuji Dri-Chem 4000i	16	100.07	6.91	6.91	1
	Roche cobas c 111	11	115.74	4.07	3.51	--
	Horiba ABX Pentra C200	10	116.05	3.63	3.13	1
	Roche cobas INTEGRA	10	114.28	5.62	4.92	--
	Roche cobas 6000	8	117.43	3.98	3.39	--
	Erba EM 200	6	112.98	7.08	6.27	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, Uric Acid, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	166	4.18	0.34	8.11	10
Uricase	25	4.11	0.32	7.86	3
RANDOX RX daytona	1	--	--	--	1

<b>Your Result</b>	3.40	<b>SDI / z-Score</b>	-1.72
<b>Assigned Value</b>	3.94	<b>Average SDI</b>	-1.92
<b>SDPA</b>	0.315	<b>Uncertainty of AV</b>	0.02
<b>Standard Unit Result Val</b>	3.40	<b>%DEV</b>	-17.27

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

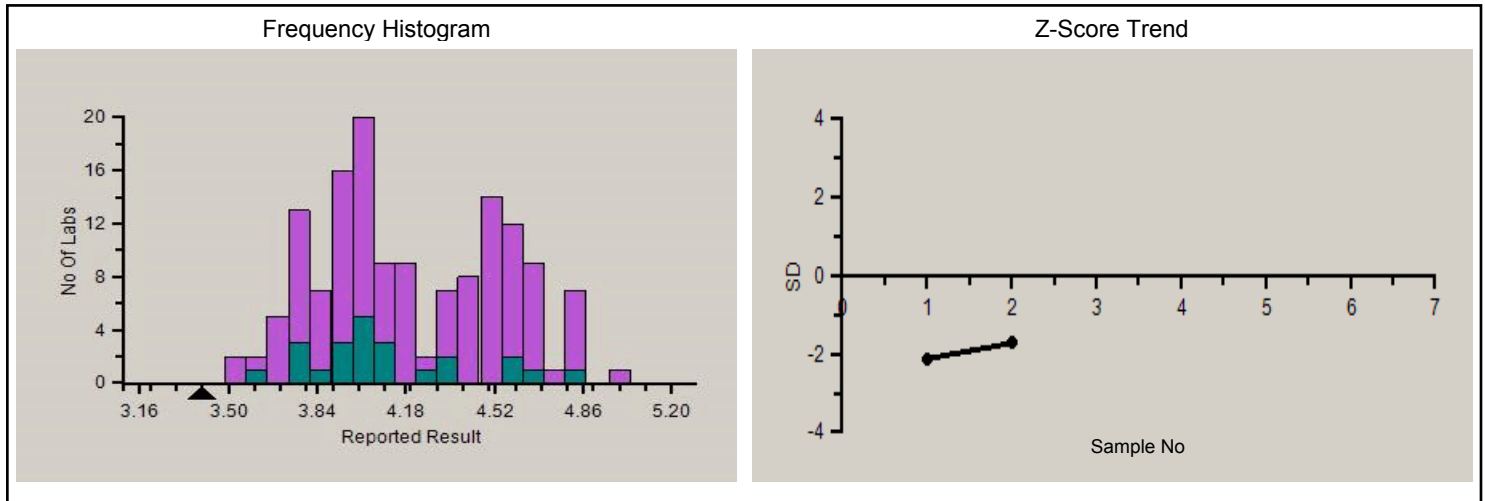

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 427  
Lab Name : VINAMRA SWARAJ HOSPITAL  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021

Biochemistry, Uric Acid		N	Mean	SD	CV%	Excluded
	All Analyzer	166	4.18	0.34	8.11	10
<b>Your Analyzer :</b>	<b>RANDOX RX daytona</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	31	4.49	0.18	4.05	1
	Roche cobas c 311	25	3.94	0.13	3.20	1
	Fuji Dri-Chem 4000i	19	4.53	0.23	5.07	1
	Roche cobas c 111	11	3.95	0.18	4.58	--
	Horiba ABX Pentra C200	10	3.91	0.15	3.79	--
	Roche cobas INTEGRA	10	3.96	0.11	2.68	--
	Roche cobas 6000	8	3.90	0.11	2.74	--
	Erba EM 200	6	4.54	0.42	9.26	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.

*Dr Puneet Kumar Nigam*

**Dr Puneet Kumar Nigam**  
**PT coordinator & Technical Manager, MHL EQAS**

Unit No. 409-416.  
Commercial Building - 1A,  
Kohinoor Mall, Kirool Road, Kuria (W),  
Mumbai - 400070



PC-1022