

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021


Biochemistry, Albumin, g/dL

	N	Mean	SD	CV%	Excluded
All Methods	168	3.99	0.47	11.65	4
Bromcresol Green (BCG)	160	4.01	0.46	11.41	4
RANDOX RX daytona	1	--	--	--	--

Your Result	3.60	SDI / z-Score	-0.43
Assigned Value	3.73	Average SDI	-0.43
SDPA	0.294	Uncertainty of AV	0.02
Standard Unit Result Val	3.60	%DEV	-10.13

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

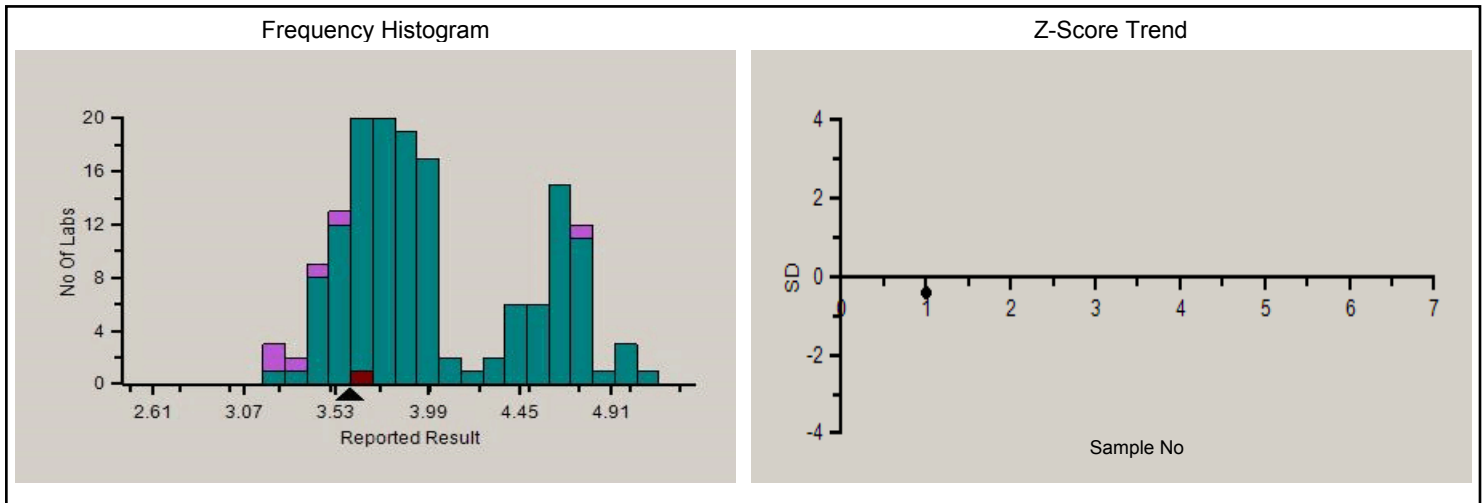

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Albumin		N	Mean	SD	CV%	Excluded
	All Analyzer	168	3.99	0.47	11.65	4
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	31	4.60	0.20	4.37	--
	Roche cobas c 311	28	3.82	0.13	3.38	--
	Fuji Dri-Chem 4000i	16	4.74	0.20	4.15	--
	Horiba ABX Pentra C200	10	3.55	0.15	4.12	--
	Roche cobas c 111	10	3.91	0.13	3.23	--
	Roche cobas INTEGRA	10	3.80	0.13	3.35	--
	Erba EM 200	8	3.58	0.10	2.71	--
	Roche cobas 6000	8	3.81	0.16	4.20	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, ALP, U/L

	N	Mean	SD	CV%	Excluded
All Methods	167	87.20	13.87	15.91	18
PNPP, AMP Buffer	77	95.05	14.81	15.59	7
RANDOX RX daytona	1	--	--	--	1

Your Result	56.00	SDI / z-Score	-1.58
Assigned Value	78.29	Average SDI	-1.16
SDPA	14.091	Uncertainty of AV	0.63
Standard Unit Result Val	56.00	%DEV	-41.09

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

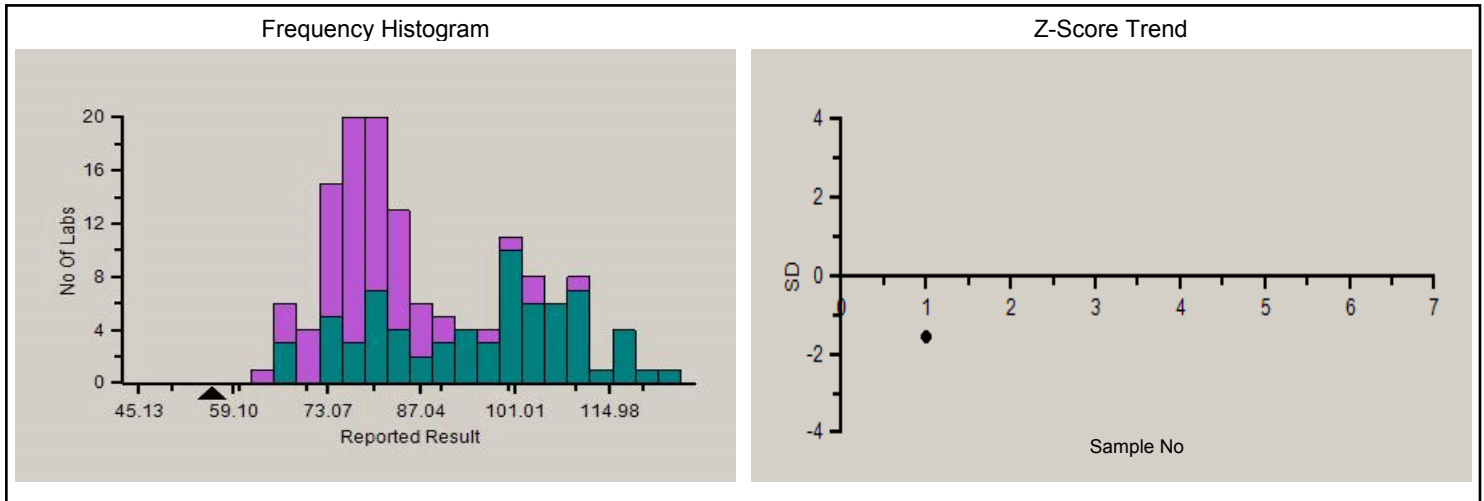

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, ALP		N	Mean	SD	CV%	Excluded
	All Analyzer	167	87.20	13.87	15.91	18
Your Analyzer :	RANDOX RX daytona	1	--	--	--	1
	Fuji Dri-Chem NX500/i	33	106.25	7.85	7.39	1
	Roche cobas c 311	28	78.32	3.62	4.62	--
	Fuji Dri-Chem 4000i	16	102.13	7.54	7.38	1
	Roche cobas c 111	11	76.60	6.07	7.92	--
	Horiba ABX Pentra C200	10	77.41	7.49	9.68	1
	Roche cobas INTEGRA	10	78.53	2.52	3.21	--
	Roche cobas 6000	8	79.38	4.31	5.43	--
	Erba EM 200	6	78.73	10.70	13.60	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, ALT, U/L

	N	Mean	SD	CV%	Excluded
All Methods	168	29.17	29.26	100.33	61
IFCC - UV without P5P	18	13.47	1.89	14.02	8
RANDOX RX daytona	1	--	--	--	--

Your Result	13.00	SDI / z-Score	0.18
Assigned Value	12.56	Average SDI	0.65
SDPA	2.510	Uncertainty of AV	0.21
Standard Unit Result Val	13.00	%DEV	-3.50

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

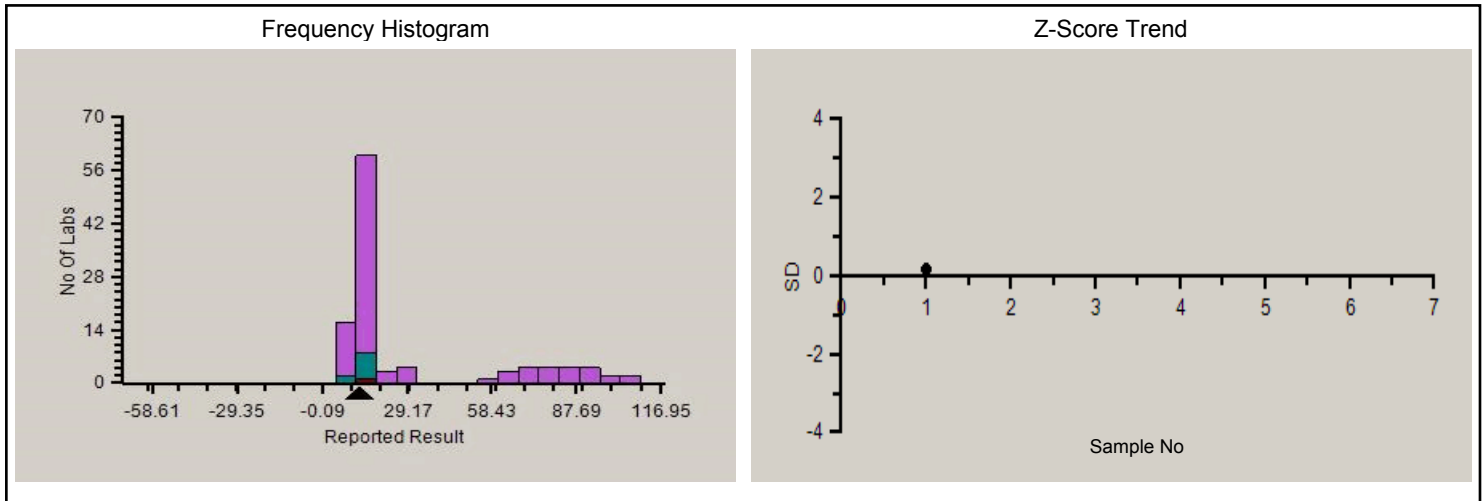

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, ALT		N	Mean	SD	CV%	Excluded
	All Analyzer	168	29.17	29.26	100.33	61
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	30	87.00	12.62	14.51	18
	Roche cobas c 311	28	13.02	1.36	10.46	6
	Fuji Dri-Chem 4000i	16	76.40	14.14	18.50	6
	Horiba ABX Pentra C200	11	12.64	1.59	12.60	--
	Roche cobas c 111	11	13.25	1.65	12.42	1
	Roche cobas INTEGRA	10	11.46	1.39	12.14	--
	Roche cobas 6000	8	12.51	1.41	11.27	--
	Erba EM 200	7	19.73	3.20	16.22	3

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Amylase, U/L

	N	Mean	SD	CV%	Excluded
All Methods	100	60.30	6.95	11.52	8
G7 PNP	66	60.12	6.81	11.33	--
RANDOX RX daytona	1	--	--	--	--

Your Result	74.00	SDI / z-Score	1.35
Assigned Value	66.36	Average SDI	1.04
SDPA	5.639	Uncertainty of AV	0.56
Standard Unit Result Val	74.00	%DEV	23.09

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

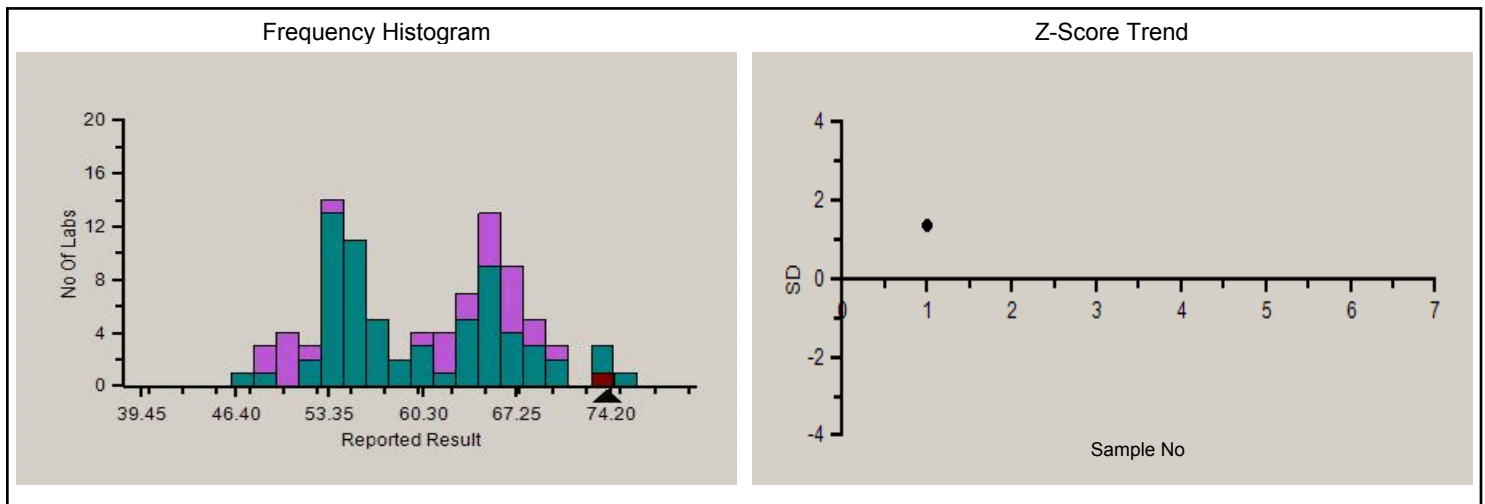

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Amylase		N	Mean	SD	CV%	Excluded
	All Analyzer	100	60.30	6.95	11.52	8
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	23	55.61	3.58	6.43	--
	Roche cobas c 311	15	66.72	3.00	4.49	--
	Fuji Dri-Chem 4000i	14	54.64	1.74	3.18	--
	Roche cobas INTEGRA	7	65.35	3.08	4.72	--
	Roche cobas 6000	6	66.22	1.83	2.77	--
	Roche cobas 8000	4	67.25	2.22	3.30	--
	Roche cobas c 111	3	69.10	5.67	8.20	--
	Star 20	3	62.50	0.00	0.00	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, AST, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	167	27.28	11.26	41.27	63
■ IFCC - UV without P5P	16	26.75	11.58	43.29	5
■ RANDOX RX daytona	1	--	--	--	--

Your Result	17.00	SDI / z-Score	-0.69
Assigned Value	19.73	Average SDI	-0.24
SDPA	3.945	Uncertainty of AV	0.35
Standard Unit Result Val	17.00	%DEV	-36.45

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

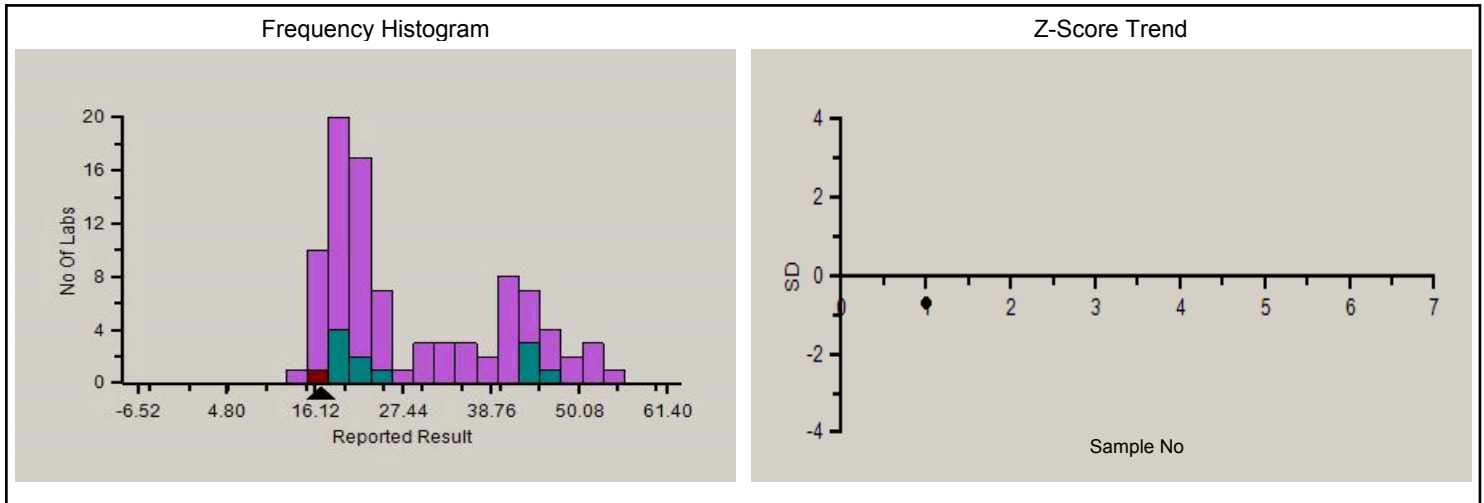

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, AST		N	Mean	SD	CV%	Excluded
	All Analyzer	167	27.28	11.26	41.27	63
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	31	42.36	7.61	17.95	20
	Roche cobas c 311	27	20.46	2.41	11.77	5
	Fuji Dri-Chem 4000i	16	45.89	6.86	14.96	7
	Roche cobas c 111	12	21.67	2.88	13.28	5
	Horiba ABX Pentra C200	10	18.60	0.95	5.13	1
	Roche cobas INTEGRA	10	17.58	1.54	8.74	1
	Roche cobas 6000	8	20.63	2.12	10.27	--
	Erba EM 200	7	41.00	7.95	19.38	3

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Bilirubin Direct, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	166	0.10	0.02	17.00	51
■ DMSO	1	--	--	--	1
■ RANDOX RX daytona	1	--	--	--	1

Your Result	0.19	SDI / z-Score	2.19
Assigned Value	0.10	Average SDI	0.99
SDPA	0.043	Uncertainty of AV	0.01
Standard Unit Result Val	0.19	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

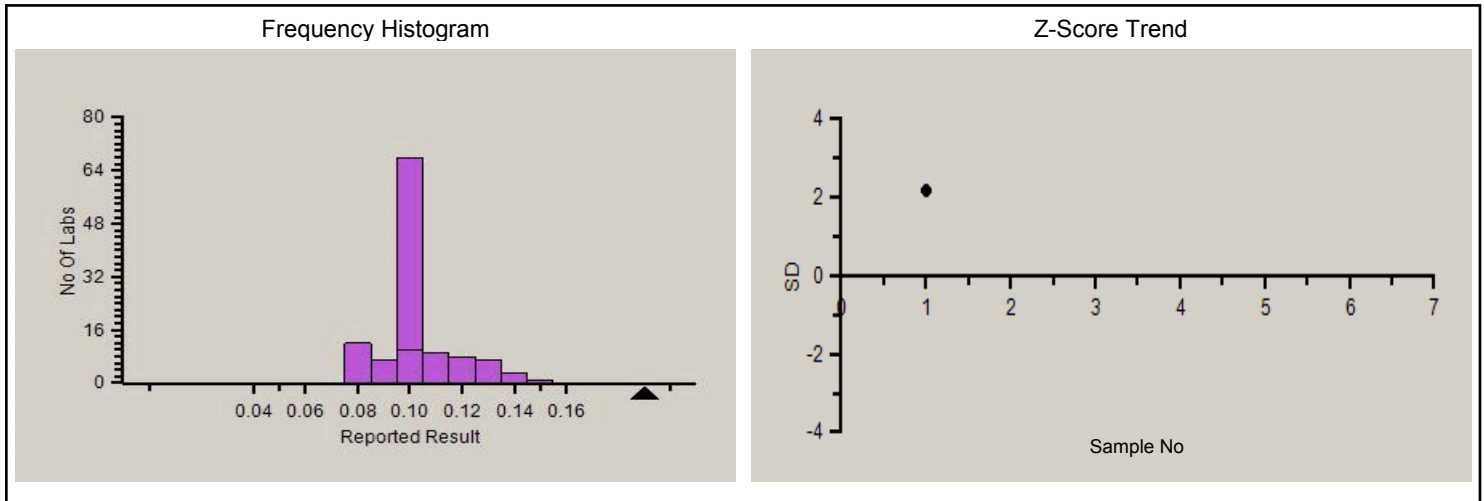

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Bilirubin Direct		N	Mean	SD	CV%	Excluded
	All Analyzer	166	0.10	0.02	17.00	51
Your Analyzer :	RANDOX RX daytona	1	--	--	--	1
	Fuji Dri-Chem NX500/i	28	0.10	0.01	8.08	9
	Roche cobas c 311	27	0.09	0.02	19.15	5
	Fuji Dri-Chem 4000i	16	0.10	0.00	0.00	9
	Horiba ABX Pentra C200	11	0.12	0.02	13.91	--
	Roche cobas c 111	11	0.11	0.01	11.01	4
	Roche cobas INTEGRA	10	0.10	0.01	13.54	--
	Erba EM 200	8	0.12	0.04	34.43	2
	Roche cobas 6000	8	0.10	0.01	9.38	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Bilirubin Total, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	170	0.31	0.14	45.05	49
DMSO	1	--	--	--	1
RANDOX RX daytona	1	--	--	--	1

Your Result	0.56	SDI / z-Score	2.56
Assigned Value	0.32	Average SDI	1.97
SDPA	0.095	Uncertainty of AV	0.02
Standard Unit Result Val	0.56	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

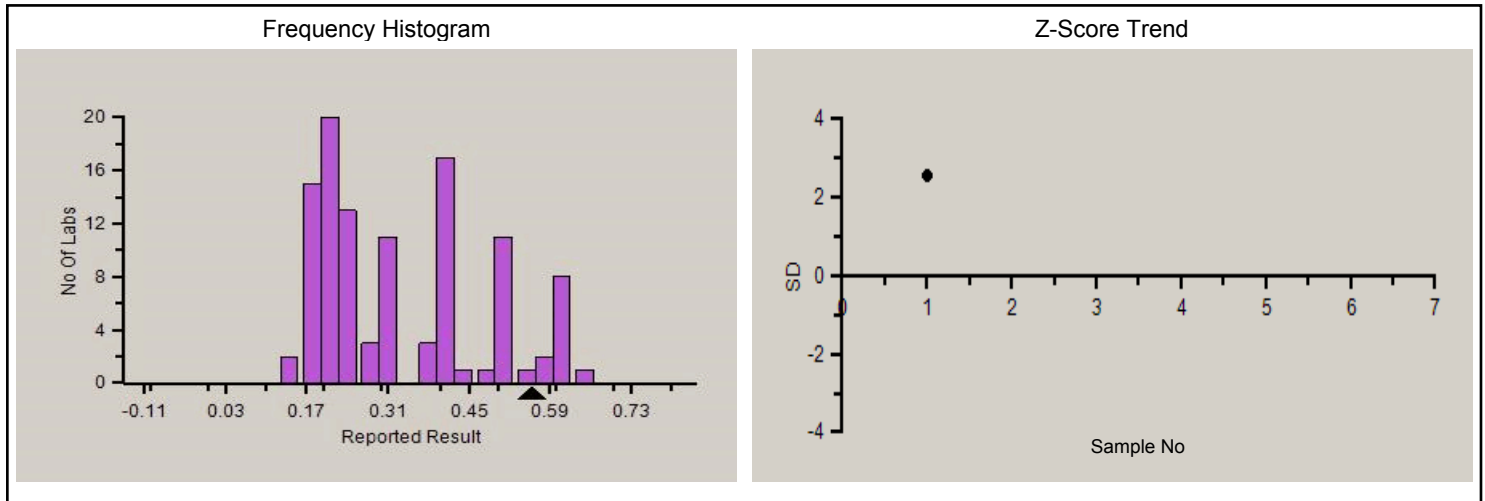

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Bilirubin Total		N	Mean	SD	CV%	Excluded
	All Analyzer	170	0.31	0.14	45.05	49
Your Analyzer :	RANDOX RX daytona	1	--	--	--	1
	Fuji Dri-Chem NX500/i	30	0.47	0.08	16.24	6
	Roche cobas c 311	28	0.20	0.03	14.50	6
	Fuji Dri-Chem 4000i	16	0.51	0.08	16.37	2
	Horiba ABX Pentra C200	11	0.22	0.03	11.26	6
	Roche cobas c 111	10	0.20	0.03	15.76	4
	Roche cobas INTEGRA	10	0.20	0.02	8.08	1
	Erba EM 200	8	0.22	0.03	14.93	1
	Roche cobas 6000	8	0.19	0.02	10.83	1

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Calcium, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	157	7.64	0.53	6.92	11
Arsenazo III	53	7.85	0.47	6.00	7
RANDOX RX daytona	1	--	--	--	--

Your Result	8.00	SDI / z-Score	-0.19
Assigned Value	8.15	Average SDI	-0.29
SDPA	0.806	Uncertainty of AV	0.41
Standard Unit Result Val	8.00	%DEV	1.91

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

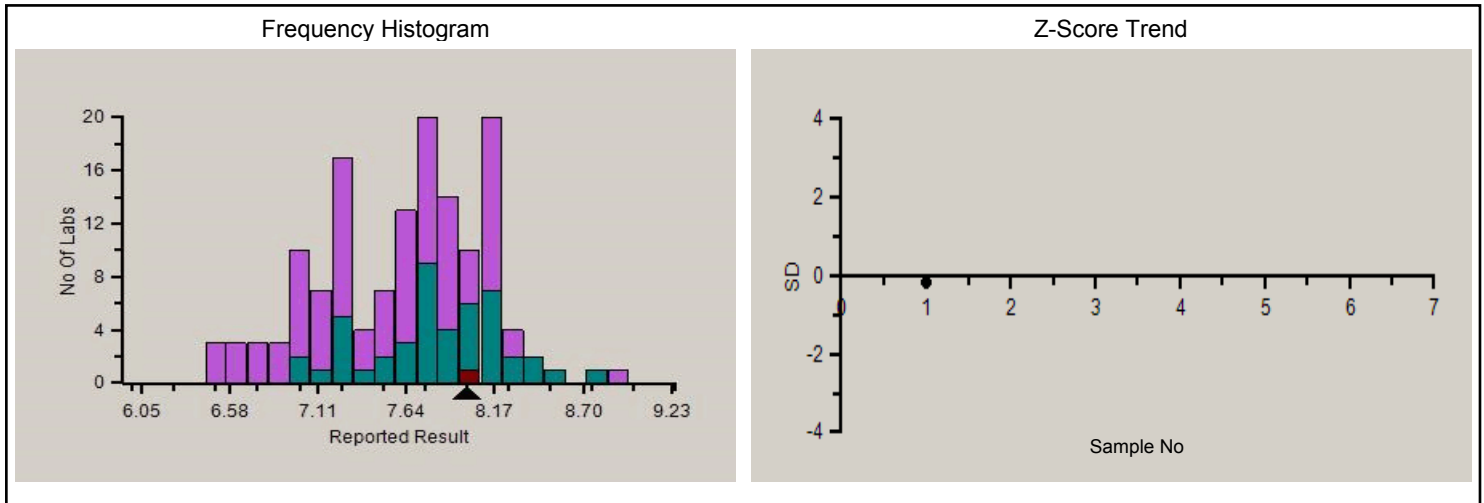

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Calcium		N	Mean	SD	CV%	Excluded
	All Analyzer	157	7.64	0.53	6.92	11
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	28	7.00	0.31	4.43	--
	Roche cobas c 311	25	7.92	0.25	3.18	1
	Fuji Dri-Chem 4000i	16	7.26	0.35	4.80	--
	Roche cobas INTEGRA	11	7.76	0.31	3.99	--
	Roche cobas c 111	10	7.83	0.26	3.27	1
	Roche cobas 6000	7	7.81	0.15	1.97	--
	Erba EM 200	6	8.43	0.62	7.31	--
	Beckman Coulter AU480	5	7.88	0.20	2.51	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Chloride, mEq/L

	N	Mean	SD	CV%	Excluded
■ All Methods	140	105.52	12.39	11.74	15
■ ISE direct	95	0.00	0.00	0.00	9
■ EasyLyte	8	0.00	0.00	0.00	1

Your Result	109.60	SDI / z-Score	-0.54
Assigned Value	113.62	Average SDI	-0.53
SDPA	7.385	Uncertainty of AV	0.47
Standard Unit Result Val	109.60	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

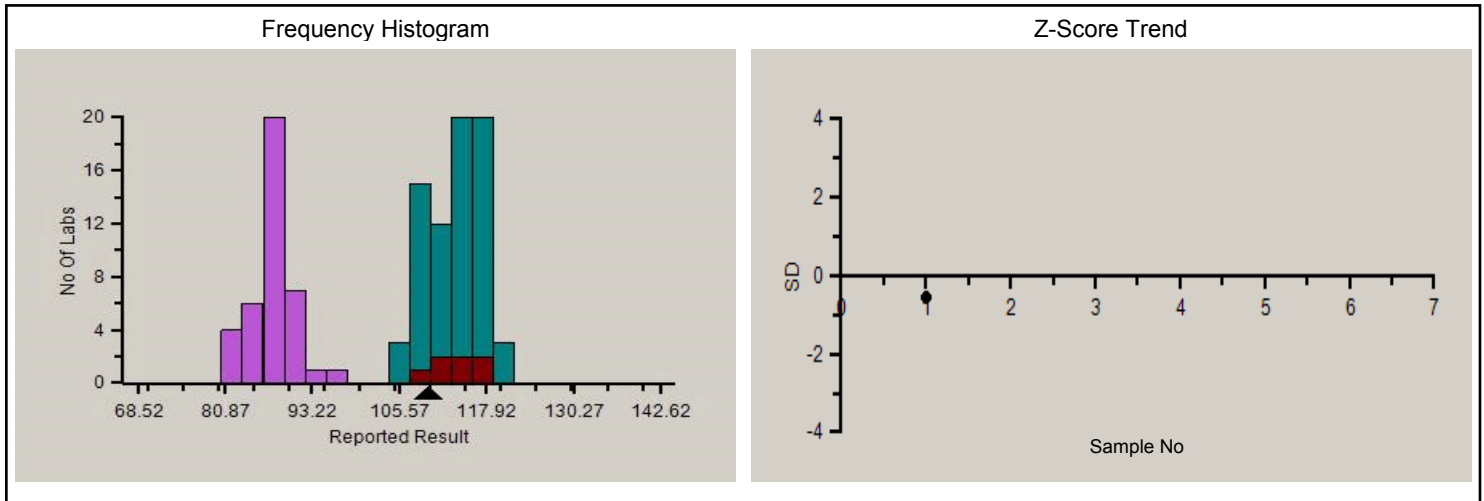

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Chloride		N	Mean	SD	CV%	Excluded
	All Analyzer	140	105.52	12.39	11.74	15
Your Analyzer :	EasyLyte	8	0.00	0.00	0.00	1
	Fuji Dri-Chem NX500/i	32	0.00	0.00	0.00	1
	Fuji Dri-Chem 4000i	17	0.00	0.00	0.00	1
	Roche cobas c 311	16	0.00	0.00	0.00	--
	Roche AVL 9180	11	110.17	1.91	1.74	--
	Roche AVL 9180	10	0.00	0.00	0.00	--
	Roche cobas 6000	8	0.00	0.00	0.00	1
	Roche cobas 8000	4	0.00	0.00	0.00	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, CK, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	76	80.59	15.40	19.11	8
■ Colorimetric	1	--	--	--	--
■ Fuji Nx 700	3	70.67	1.16	1.63	--

Your Result	72.00	SDI / z-Score	0.66
Assigned Value	66.28	Average SDI	0.05
SDPA	8.616	Uncertainty of AV	1.81
Standard Unit Result Val	72.00	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

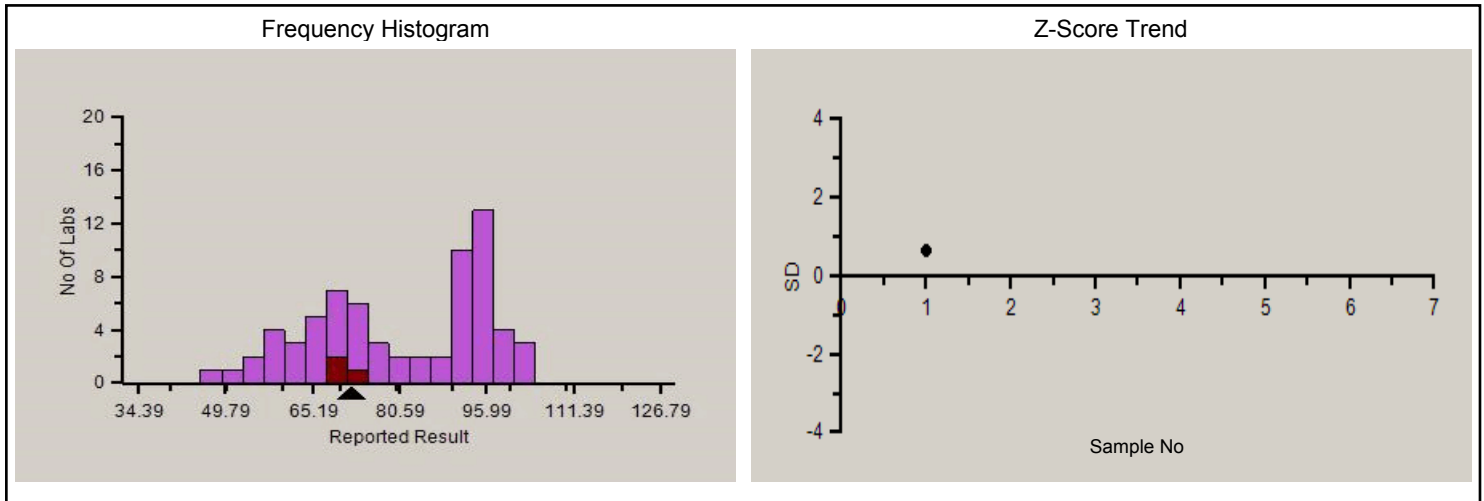

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, CK		N	Mean	SD	CV%	Excluded
	All Analyzer	76	80.59	15.40	19.11	8
Your Analyzer :	Fuji Nx 700	3	70.67	1.16	1.63	--
	Fuji Dri-Chem NX500/i	21	66.12	8.97	13.57	4
	Roche cobas c 311	13	94.52	4.02	4.26	--
	Fuji Dri-Chem 4000i	11	66.00	5.04	7.64	--
	Roche cobas INTEGRA	7	93.04	6.31	6.78	--
	Roche cobas 6000	5	92.20	2.95	3.20	--
	Roche cobas 8000	4	95.25	1.71	1.79	--
	Star 20	2	--	--	--	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, GGT, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	135	15.80	3.87	24.49	11
■ IFCC	12	16.84	3.85	22.88	--
■ RANDOX RX daytona	1	--	--	--	--

Your Result	21.00	SDI / z-Score	0.94
Assigned Value	18.40	Average SDI	0.88
SDPA	2.760	Uncertainty of AV	0.27
Standard Unit Result Val	21.00	%DEV	24.69

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

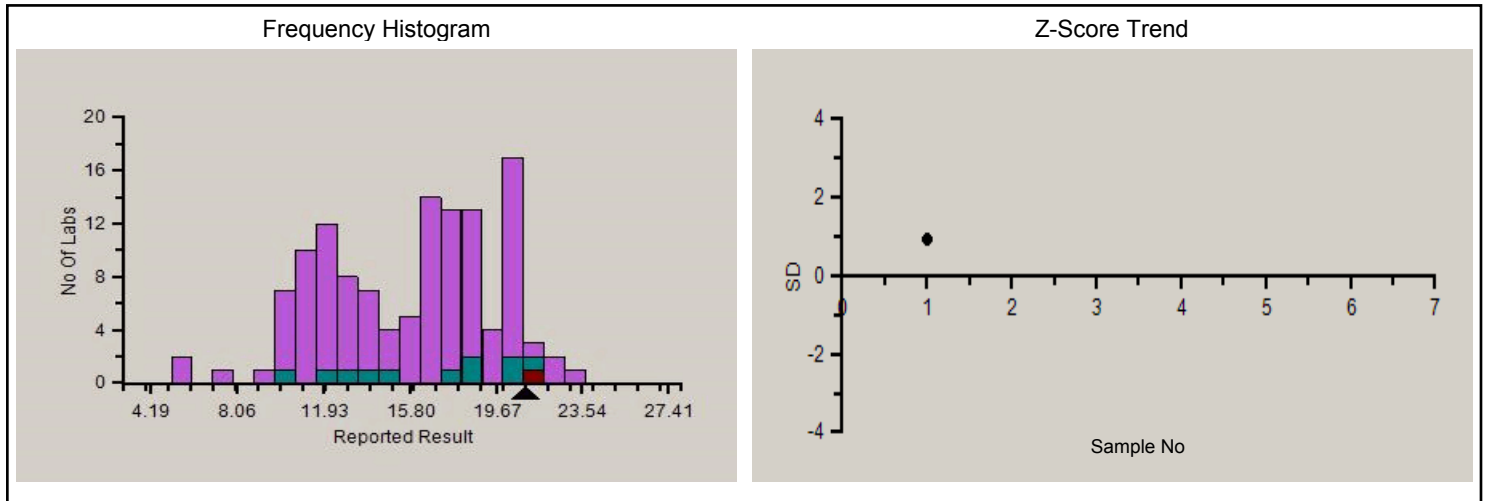

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, GGT		N	Mean	SD	CV%	Excluded
	All Analyzer	135	15.80	3.87	24.49	11
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	32	12.03	1.19	9.88	2
	Roche cobas c 311	24	19.00	1.23	6.50	2
	Fuji Dri-Chem 4000i	12	11.33	1.50	13.21	--
	Roche cobas INTEGRA	11	16.87	1.42	8.43	--
	Roche cobas c 111	10	16.97	1.39	8.18	1
	Horiba ABX Pentra C200	6	18.40	2.30	12.47	--
	Roche cobas 6000	6	18.33	1.51	8.22	--
	Beckman Coulter AU480	5	19.08	1.42	7.43	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, LDH, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	93	145.36	59.94	41.23	14
■ L to P - IFCC Ref. Proc., Calibrated	3	121.67	33.50	27.54	--
■ Fuji Nx 700	3	109.00	5.29	4.86	--

Your Result	107.00	SDI / z-Score	0.33
Assigned Value	102.59	Average SDI	-0.67
SDPA	13.360	Uncertainty of AV	1.85
Standard Unit Result Val	107.00	%DEV	-12.06

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

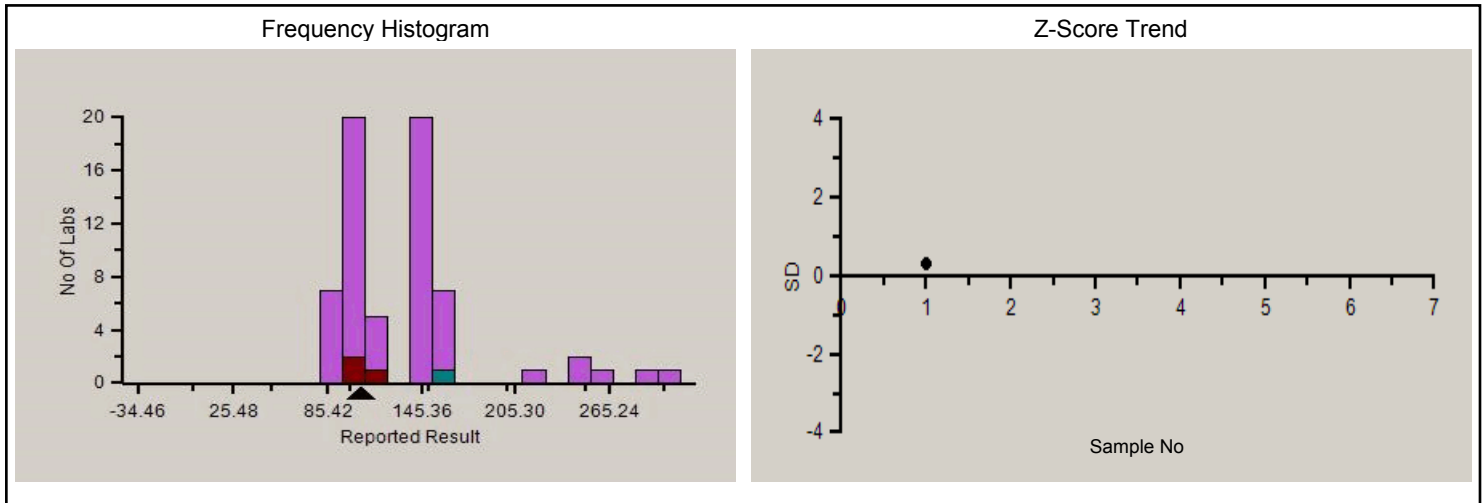

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, LDH		N	Mean	SD	CV%	Excluded
	All Analyzer	93	145.36	59.94	41.23	14
Your Analyzer :	Fuji Nx 700	3	109.00	5.29	4.86	--
	Fuji Dri-Chem NX500/i	25	100.00	8.03	8.03	6
	Fuji Dri-Chem 4000i	12	104.67	9.06	8.66	--
	Roche cobas c 311	11	149.91	5.11	3.41	--
	Roche cobas INTEGRA	7	146.55	2.93	2.00	--
	Roche cobas 6000	6	150.17	5.08	3.38	--
	Beckman Coulter AU480	4	197.00	0.00	0.00	2
	Roche cobas 8000	4	146.75	2.22	1.51	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Lipase, U/L

	N	Mean	SD	CV%	Excluded
All Methods	81	48.90	16.91	34.57	9
Enzymatic colorimetric	14	41.82	14.72	35.21	3
Fuji Nx 700	3	56.67	5.13	9.06	--

Your Result	58.00	SDI / z-Score	-0.25
Assigned Value	59.49	Average SDI	-0.41
SDPA	5.966	Uncertainty of AV	0.80
Standard Unit Result Val	58.00	%DEV	38.71

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

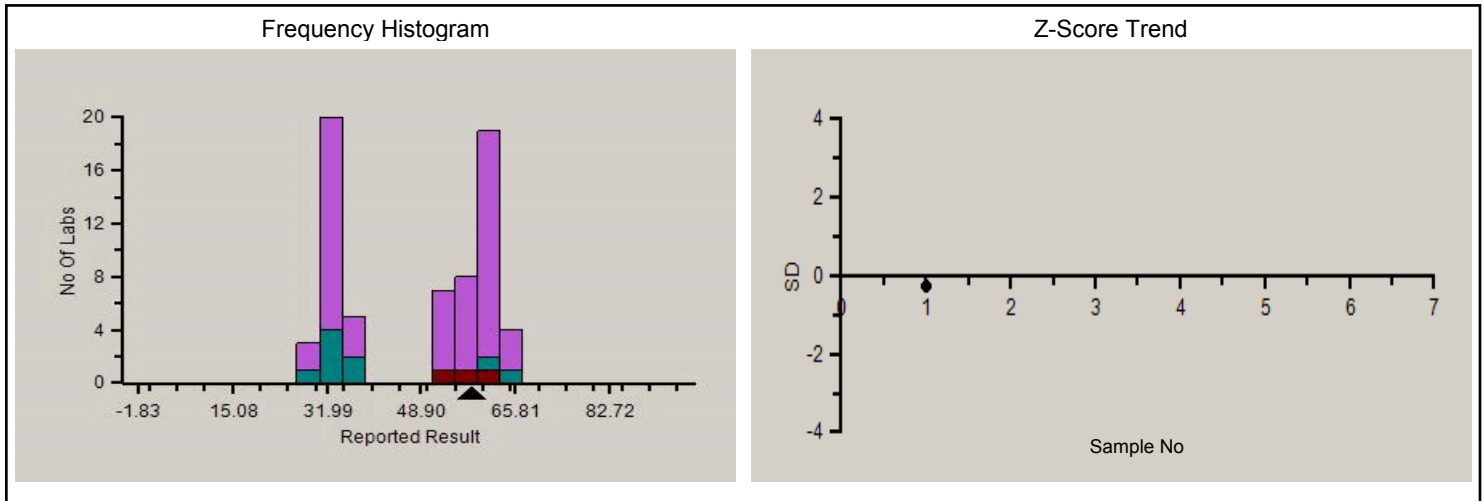

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Lipase		N	Mean	SD	CV%	Excluded
	All Analyzer	81	48.90	16.91	34.57	9
Your Analyzer :	Fuji Nx 700	3	56.67	5.13	9.06	--
	Fuji Dri-Chem NX500/i	22	59.81	4.08	6.83	1
	Fuji Dri-Chem 4000i	14	59.29	3.47	5.86	--
	Roche cobas c 311	12	33.62	1.74	5.16	2
	Roche cobas INTEGRA	6	33.04	2.43	7.36	--
	Roche cobas 6000	5	32.14	1.49	4.65	--
	Roche cobas 8000	3	31.92	3.05	9.55	--
	Star 20	3	69.00	0.00	0.00	1

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Magnesium, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	55	1.06	0.66	61.79	6
Enzymatic	2	0.50	--	--	1
Fuji Nx 700	2	0.50	--	--	--

Your Result	0.50	SDI / z-Score	0.00
Assigned Value	0.50	Average SDI	-0.15
SDPA	0.065	Uncertainty of AV	0.01
Standard Unit Result Val	0.50	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

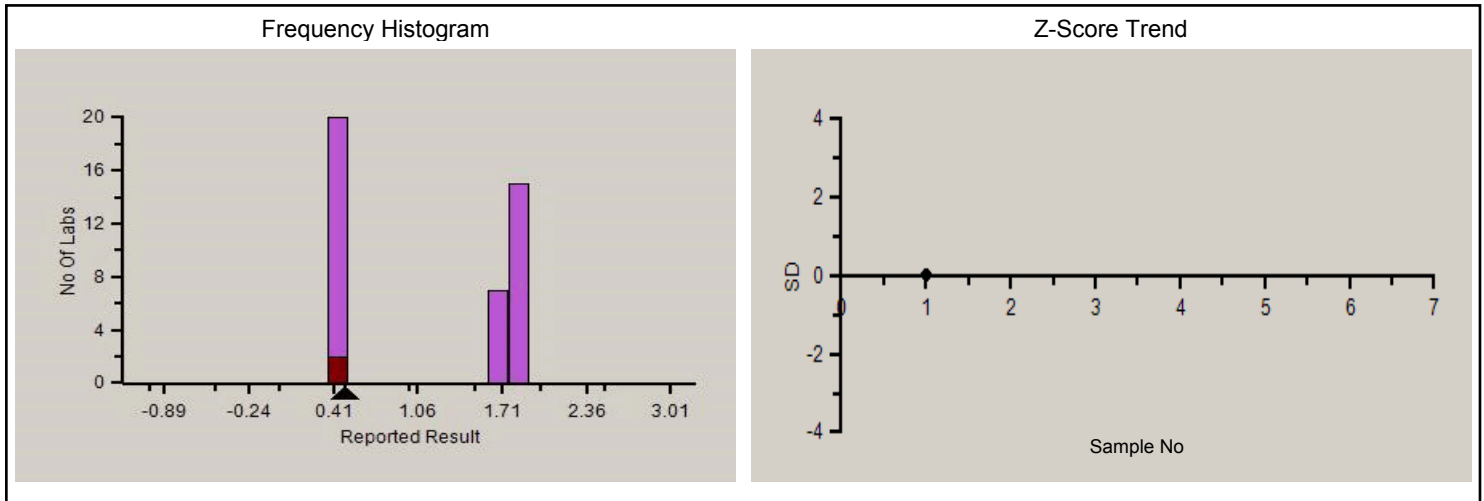

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Magnesium		N	Mean	SD	CV%	Excluded
	All Analyzer	55	1.06	0.66	61.79	6
Your Analyzer :	Fuji Nx 700	2	0.50	--	--	--
	Fuji Dri-Chem NX500/i	17	0.47	0.04	8.16	2
	Fuji Dri-Chem 4000i	10	0.49	0.03	6.53	--
	Roche cobas c 311	7	1.75	0.07	4.18	--
	Roche cobas 6000	6	1.77	0.05	2.83	--
	Roche cobas 8000	4	1.83	0.05	2.96	--
	Roche cobas INTEGRA	2	1.73	--	--	1
	Beckman Coulter AU5800	1	--	--	--	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Potassium, mEq/L

	N	Mean	SD	CV%	Excluded
■ All Methods	151	5.75	0.93	16.17	12
■ ISE direct	105	0.00	0.00	0.00	4
■ EasyLyte	9	0.00	0.00	0.00	--

Your Result	5.71	SDI / z-Score	-1.91
Assigned Value	6.31	Average SDI	-1.85
SDPA	0.316	Uncertainty of AV	0.04
Standard Unit Result Val	5.71	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

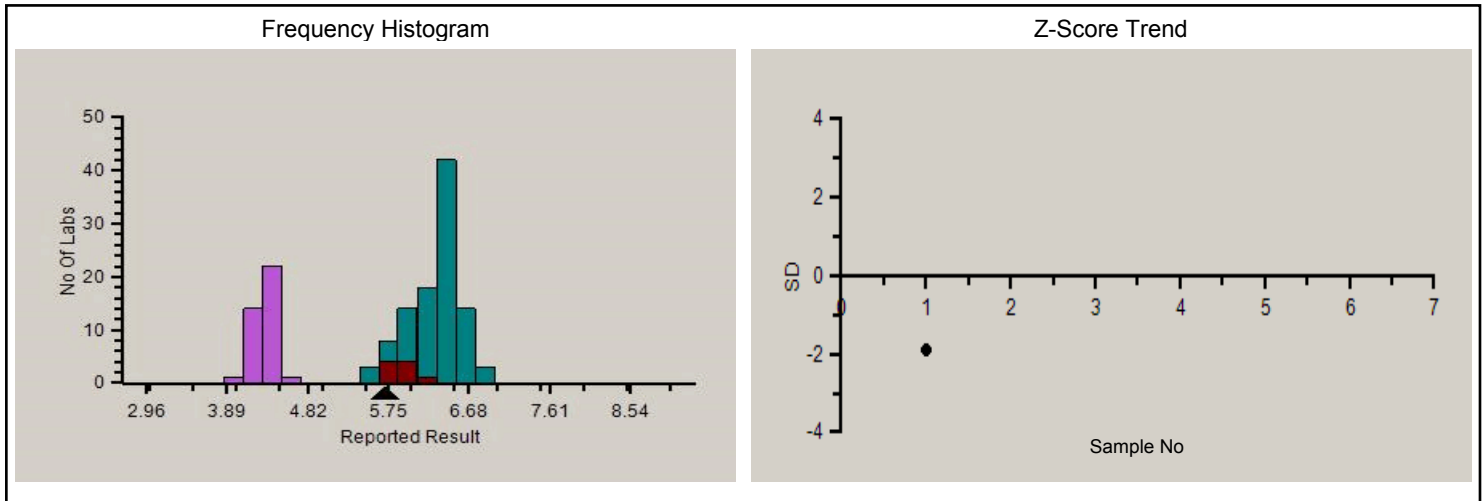

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Potassium		N	Mean	SD	CV%	Excluded
	All Analyzer	151	5.75	0.93	16.17	12
Your Analyzer :	EasyLyte	9	0.00	0.00	0.00	--
	Fuji Dri-Chem NX500/i	33	0.00	0.00	0.00	1
	Fuji Dri-Chem 4000i	19	0.00	0.00	0.00	1
	Roche cobas c 311	16	0.00	0.00	0.00	--
	Roche AVL 9180	13	6.33	0.43	6.81	--
	Roche AVL 9180	12	0.00	0.00	0.00	--
	Roche cobas 6000	8	0.00	0.00	0.00	--
	Sensa Core	5	0.00	0.00	0.00	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Sodium, mEq/L

	N	Mean	SD	CV%	Excluded
■ All Methods	151	159.57	23.46	14.70	18
■ ISE direct	105	0.00	0.00	0.00	11
■ EasyLyte	9	0.00	0.00	0.00	2

Your Result	169.40	SDI / z-Score	-0.58
Assigned Value	174.48	Average SDI	-0.57
SDPA	8.723	Uncertainty of AV	0.48
Standard Unit Result Val	169.40	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

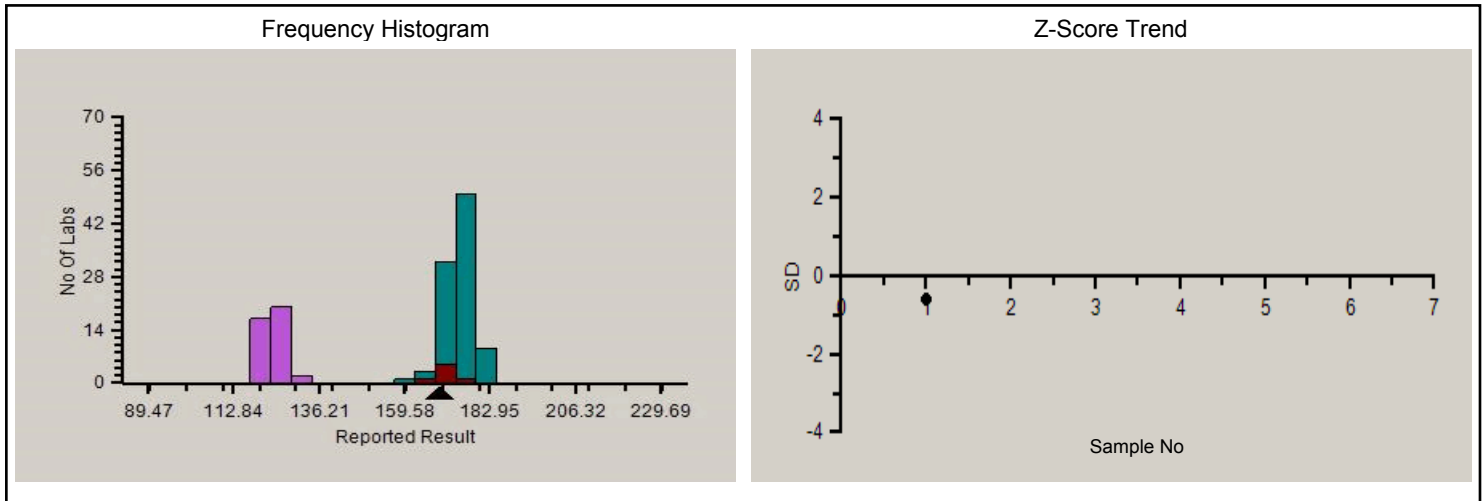

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Sodium		N	Mean	SD	CV%	Excluded
	All Analyzer	151	159.57	23.46	14.70	18
Your Analyzer :	EasyLyte	9	0.00	0.00	0.00	2
	Fuji Dri-Chem NX500/i	34	0.00	0.00	0.00	3
	Fuji Dri-Chem 4000i	18	0.00	0.00	0.00	3
	Roche cobas c 311	16	0.00	0.00	0.00	--
	Roche AVL 9180	13	175.22	5.44	3.11	--
	Roche AVL 9180	12	0.00	0.00	0.00	--
	Roche cobas 6000	8	0.00	0.00	0.00	--
	Sensa Core	5	0.00	0.00	0.00	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Total Protein, g/dL

	N	Mean	SD	CV%	Excluded
■ All Methods	166	6.47	0.32	4.96	3
■ Biuret	163	6.47	0.32	5.00	3
■ RANDOX RX daytona	1	--	--	--	--

Your Result	6.30	SDI / z-Score	-0.29
Assigned Value	6.38	Average SDI	-0.36
SDPA	0.283	Uncertainty of AV	0.03
Standard Unit Result Val	6.30	%DEV	-2.58

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

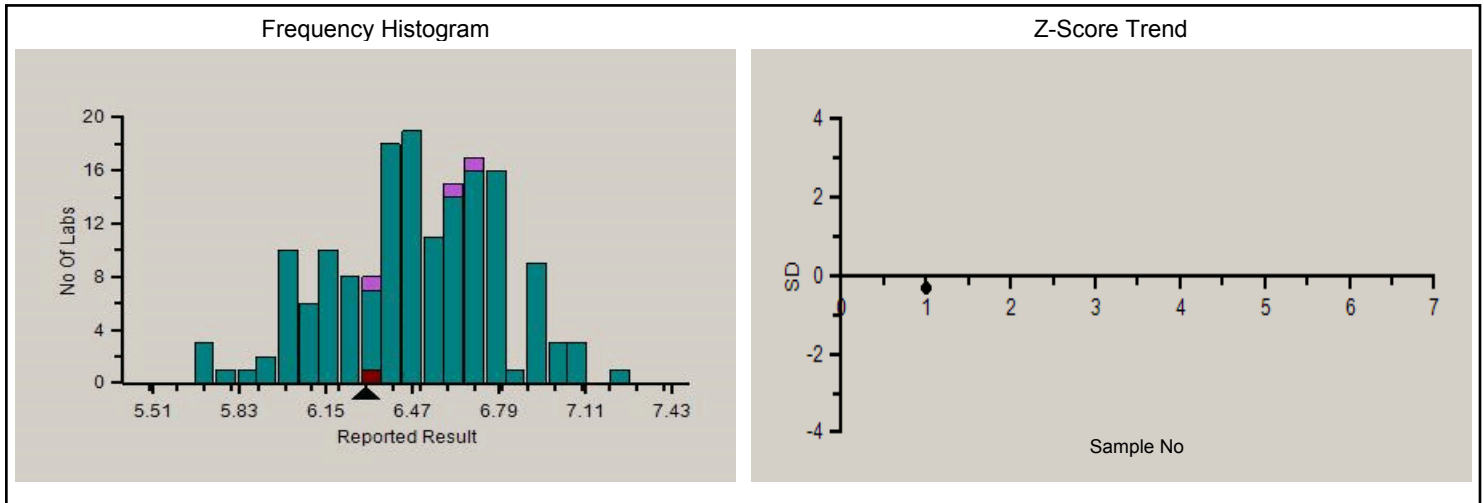

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Total Protein		N	Mean	SD	CV%	Excluded
	All Analyzer	166	6.47	0.32	4.96	3
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	30	6.73	0.17	2.53	--
	Roche cobas c 311	28	6.47	0.21	3.23	--
	Fuji Dri-Chem 4000i	16	6.77	0.15	2.20	--
	Roche cobas c 111	11	6.40	0.33	5.10	--
	Roche cobas INTEGRA	10	6.10	0.24	3.87	--
	Horiba ABX Pentra C200	9	6.42	0.17	2.60	--
	Erba EM 200	8	6.53	0.41	6.34	1
	Roche cobas 6000	8	6.46	0.17	2.59	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Triglycerides, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	166	121.71	8.69	7.14	8
GPO-PAP	15	124.65	10.76	8.63	--
RANDOX RX daytona	1	--	--	--	--

Your Result	128.00	SDI / z-Score	0.16
Assigned Value	125.53	Average SDI	0.41
SDPA	15.189	Uncertainty of AV	0.73
Standard Unit Result Val	128.00	%DEV	2.69

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

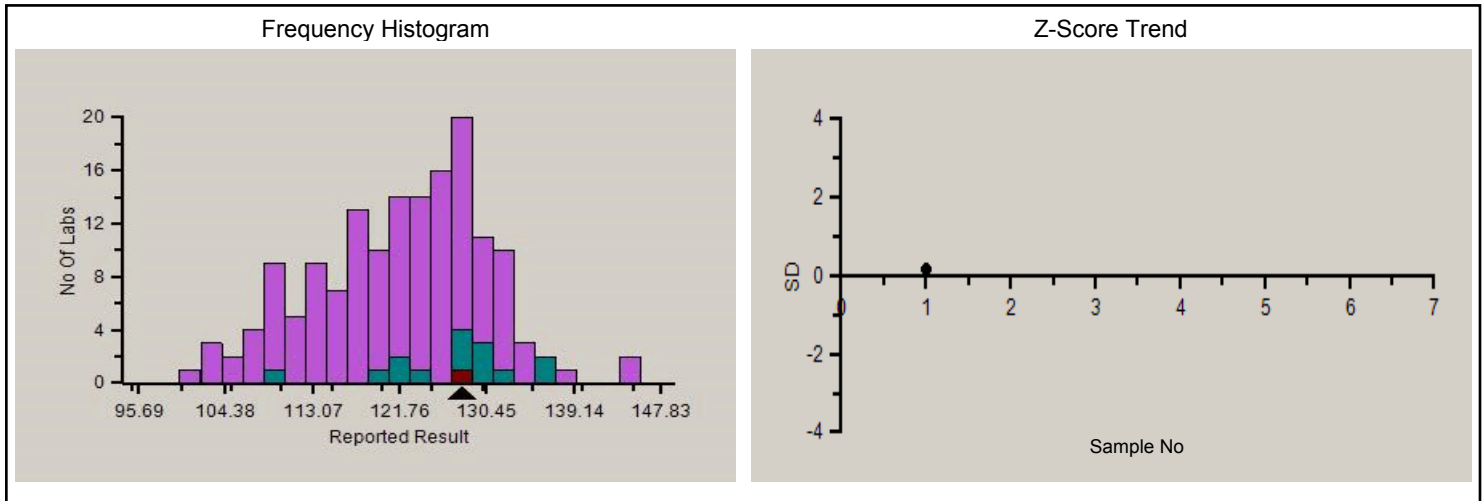

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Triglycerides		N	Mean	SD	CV%	Excluded
	All Analyzer	166	121.71	8.69	7.14	8
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	32	114.44	6.40	5.59	1
	Roche cobas c 311	28	127.01	5.98	4.71	--
	Fuji Dri-Chem 4000i	16	114.19	7.31	6.40	--
	Roche cobas c 111	11	128.25	4.39	3.43	--
	Horiba ABX Pentra C200	10	124.53	4.32	3.47	--
	Roche cobas INTEGRA	10	122.87	4.59	3.73	--
	Roche cobas 6000	8	126.29	1.50	1.19	1
	Erba EM 200	6	121.70	9.86	8.10	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Uric Acid, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	168	4.18	0.35	8.30	10
■ Uricase	25	4.09	0.39	9.56	5
■ RANDOX RX daytona	1	--	--	--	1

Your Result	3.30	SDI / z-Score	-2.12
Assigned Value	3.96	Average SDI	-1.92
SDPA	0.313	Uncertainty of AV	0.02
Standard Unit Result Val	3.30	%DEV	-19.32

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

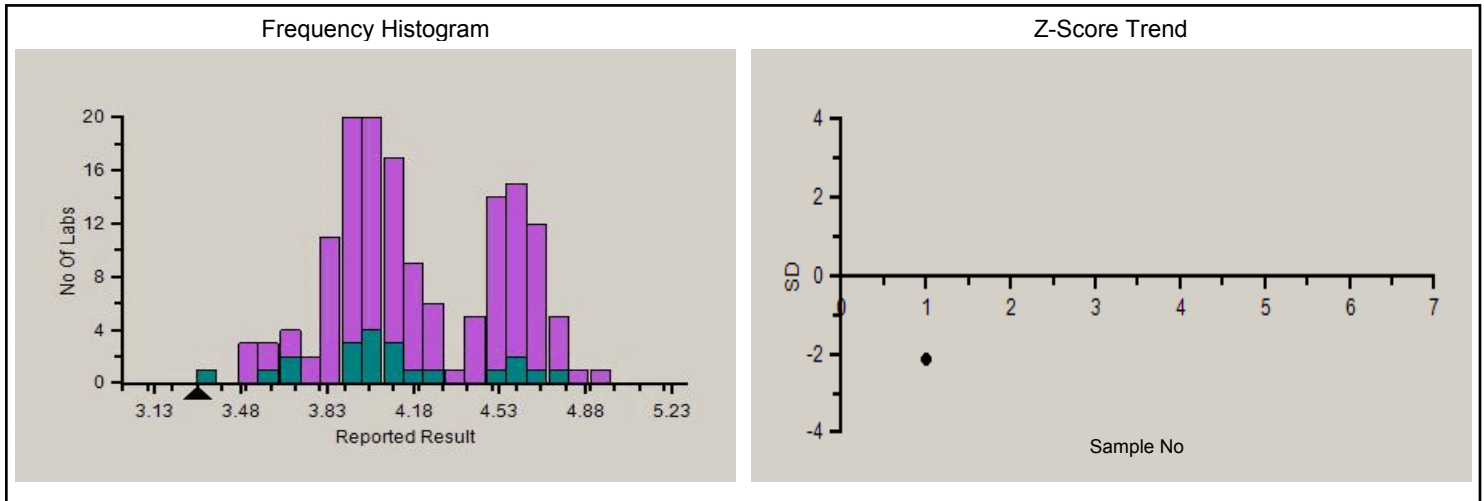

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Uric Acid		N	Mean	SD	CV%	Excluded
	All Analyzer	168	4.18	0.35	8.30	10
Your Analyzer :	RANDOX RX daytona	1	--	--	--	1
	Fuji Dri-Chem NX500/i	31	4.52	0.20	4.33	1
	Roche cobas c 311	26	3.95	0.17	4.35	1
	Fuji Dri-Chem 4000i	19	4.59	0.20	4.45	1
	Roche cobas c 111	11	4.00	0.17	4.12	--
	Horiba ABX Pentra C200	10	3.96	0.09	2.35	1
	Roche cobas INTEGRA	10	3.97	0.13	3.30	--
	Roche cobas 6000	8	3.94	0.07	1.88	--
	Erba EM 200	6	4.50	0.30	6.64	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
 Unit No. 409-416.
 Commercial Building - 1A,
 Kohinoor Mall, Kirol Road, Kuria (W),
 Mumbai - 400070



PC-1022