



COMMITTED TO THE CUSTOMER SINCE - 1994

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Contact : 080-23377285, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@vipgroup.com Web : www.vipgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

1 Name and Address of the Customer

M/s.: Energon Health.,
No.703, 3rd Cross Road, HRBR Layout,
1st Block, Kalyan Nagar, Bangalore - 560 043.

2 Customer Reference

2.1 ULR No. : CC2473215000023414F
2.2 SRF No : 0037
2.3 Certificate No. : VI/21-22/0037-05
2.4 Format No. : VI-FRM-ME-046 & VI-FRM-ET-011
2.5 Date of Issue : 09-04-2021

3 Details Of Device Under Calibration(DUC),

3.1 Nomenclature : Centrifuge
3.2 Make / Model : Remi / R-8C
3.3 Id.No. : EH/CF/01
3.4 DUC Condition : Satisfactory
3.5 Calibration Procedure No. : SOP-16- 42 & SOP-37-11
3.6 No.of Pages : 2
3.7 Calibration Date : 08-04-2021
3.8 Calibration Due : 07-04-2022
3.9 Calibration done at : Onsite
3.10 Instrument Location : Lab
3.11 Discipline : Mechanical

4 Environmental Condition

Temperature 25.3 °C Humidity: 52 %Rh

5 Standards Used for calibration

Sl. No.	Nomenclature	Make & Model	Sl. No. / Id.No.	Certificate No.	Validity
1	Digital Tachometer	SENTRY / ST723	SN1323004225	ULR- CC287920000004732F	10-09-2021
2	Time Totalizer	Beltronics / 501	251	VI/20-21/INT-ETH-426	23-02-2022

6 Notes:


- The Calibration Certificate relates only to the above DUC
- Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab.
- Corrections/erasing, invalidate the Calibration Certificate.
- Calibration of the DUC are traceable to National standards/International Standards
- Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- Results Reported are valid at the time of and under the stated conditions of measurements
- The usage of NABL Symbol is as per NABL guidelines given in NABL-133

Calibrated By
P. Teled
Madhusudhan

(Calibration Engineer)

Checked By
P. Ray
Umesh D

(Onsite In-Charge)

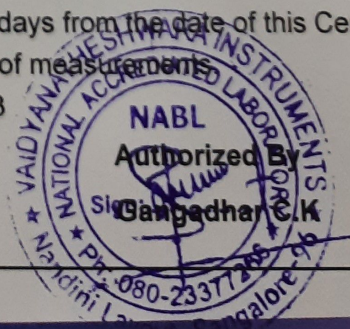

COMMITTED TO THE CUSTOMER SINCE - 1996

VAIDYANATHESHWARA INSTRUMENTS

CERTIFICATE OF CALIBRATION



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
 Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No.

RPM Results:

Page No: 2 of 2

Range: 0 to 5250 RPM

Resolution: 1 RPM

Sl. No.	Std Reading (RPM)	DUC Reading (RPM)	Error Observed in (RPM)	Measurement Uncertainty in \pm (%)	k Factor
1	199.9	200	0.1	1.2	2.0
2	599.7	600	0.3		2.0
3	999.5	1000	0.5		2.0
4	1999.2	2000	0.8		2.0
5	2998.9	3000	1.1		2.0
6	3998.6	4000	1.4		2.0
7	5248.3	5250	1.7		2.0

Timer Results:

Range: 0 to 99 min

Resolution: 1min


Sl. No.	Std Reading (hr:min:sec:msec)	DUC Reading (min)	Error Observed in (hr:min:sec:msec)	Measurement Uncertainty in \pm (%)	k Factor
1	00:00:00:000	0	00:00:00:000	----	----
2	00:15:00:012	15	-00:00:00:012	0.05	2.0
3	00:30:00:026	30	-00:00:00:026	0.05	2.0
4	00:45:00:042	45	-00:00:00:042	0.05	2.0
5	01:00:00:059	60	-00:00:00:059	0.05	2.0
6	01:39:00:067	99	-00:00:00:067	0.05	2.0

Conclusion :-

1. Measurement uncertainty reported is at 95.45 % confidence level.

Calibrated By
P. Tejo
 Madhusudhan
 (Calibration Engineer)

Checked By
P. Jay
 Umesh D
 (Onsite In-Charge)

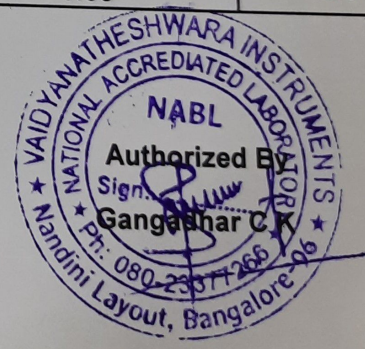



COMMITTED TO THE CUSTOMER SINCE - 1986

VAIDYANATHESHWARA INSTRUMENTS

CERTIFICATE OF CALIBRATION



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448090177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Page: 1 of 2

1 Name and Address of the Customer

M/s.: Energon Health ,
No.703, 3rd Cross Road, HRBR Layout ,
1 st Block, Kalyan Nagar, Bangalore - 560 043.

2 Customer Reference

2.1 ULR No. : CC247321500022901F
2.2 Format No. : VI-FRM-TH-006
2.3 SRF No. : 0032
2.4 Certificate No. : VI/21-22/0032-02
2.5 Date of Issue : 07-04-2021

3 Details Of Device Under Calibration(DUC).

3.1 Nomenclature : Refrigerator
3.2 Make : Whirpool
3.3 Id.No. : EH/REF/02
3.4 Range / Resolution : 2 to 8 °C / 0.1 °C
3.5 DUC Condition : Satisfactory
3.6 Calibration Procedure No. : SOP-38-06
3.7 No.of Pages : 2
3.8 Calibration Date : 06-04-2021
3.9 Calibration Due : 05-04-2022
3.10 Calibration done at : Onsite
3.11 Instrument Location : Clinical Pathology
3.12 Discipline : Thermal

4 Environmental Condition

Temperature 26.4 °C Humidity 54 %RH

5 Standards Used for Temperature Calibration

Sl. No.	Nomenclature	Make / Model	Sl. No.	Certificate. No.	Validity
1	Precision Thermometer with RTD Sensor	Lutron / TM-917	Q601311	VI/20-21/INT-TH-55	28-08-2021

6 Note:

- The Calibration Certificate relates only to the above DUC
- Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI.
- Corrections/erasing, invalidate the Calibration Certificate.
- Calibration of the DUC are traceable to National standards/International Standards
- Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- Results Reported are valid at the time of and under the stated conditions of measurements.
- The usage of NABL Symbol is as per NABL guidelines given in NABL-133

Calibrated By

F. Pruthi

Madhusudhan


(Calibration Engineer)

Checked By

Umesh D

Umesh D

(Onsite In-Charge)

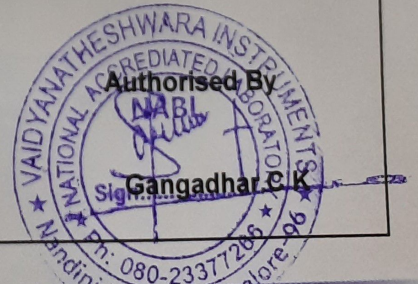

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No. VI/21-22/0032-02

Page: 2 of 2


Results:

Range : 2 to 8 °C

Resolution: 0.1 °C

SI No	STD Reading (°C)	DUC Reading (°C)	Error Observed (°C)	Measurement Uncertainty ± (°C)	k Factor
1	2.02	2.0	-0.02	1.6	2.0
2	3.05	3.0	-0.05	1.6	2.0
3	4.10	4.0	-0.10	1.6	2.0
4	6.15	6.0	-0.15	1.6	2.0
5	8.20	8.0	-0.20	1.6	2.0

Pictorial Representation of Sensors Placement

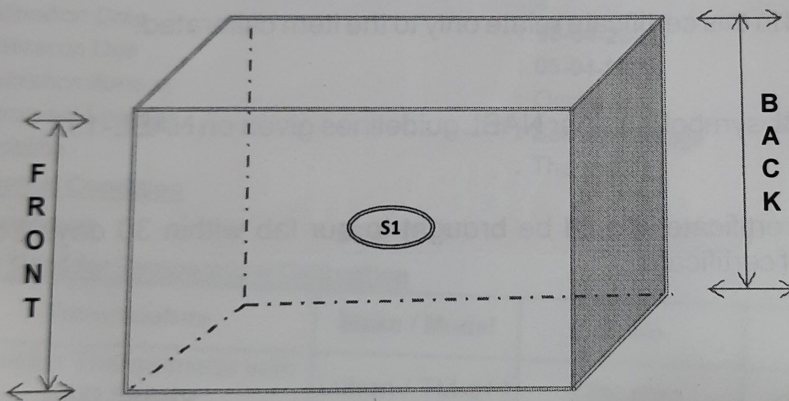

Note :

1. S1 Indicates Placement of Standard Sensor

Conclusion / Remarks:

- 1 Measurement Uncertainty reported is at 95.45% confidence level with k = 2


Calibrated By

F. Jeeithi
Madhusudan
(Calibration Engineer)

Checked By

Umesh D
Umesh D
(Onsite In-Charge)

Authorised By

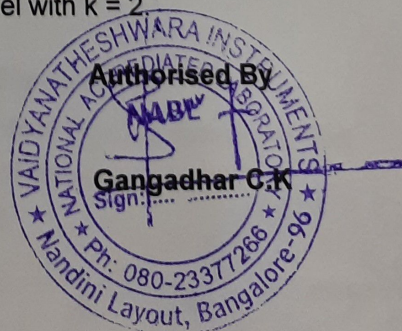



CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

1 Name and Address of Customer

M/s.: Energon Health.,
No.703, 3rd Cross, HRBR Layout, 1st Block,
Kalyan Nagar, Bangalore, Karnataka - 560 043.

2 Customer Reference

2.1 ULR No. : CC247321300001845F
2.2 Format No. : VI-FRM-TH-002
2.3 SRF No : 0087
2.4 DC No / Date : --- / ---
2.5 Certification No. : VI/21-22/0087-05
2.6 Date of Issue : 07-04-2021

3 Details Of Device Under Calibration(DUC).

3.1 Nomenclature : Digital Thermo-Hygrometer
3.2 Make / Model : --- / HTC-1
3.3 SI.No. / ID.No. : --- / DHTM-02
3.4 DUC Condition : Satisfactory
3.5 Calibration Procedure No. : SOP - 38-02
3.6 No.of Pages : 2
3.7 Calibration Date : 07-04-2021
3.8 Calibration Due : 06-04-2022
3.9 Calibration done at : VI Thermal Lab
3.10 Discipline : Thermal

4 Environmental Condition:

Temperature 25.4 °C Humidity 53 %RH

5 Standards Used for calibration:

Sl. No	Nomenclature	Make & Model	Sl. No	Certificate No.	Validity
1	Hygropalm With Sensor	Rotronic / HP23	60885044 & 20146871	CR/NCAL/51117	05-08-2021
2	Platinum Resistance Thermometer With Indicator	FLUKE / 5609 (Sensor) & 1524 (Indicator)	03520 (Sensor) & 3028237 (Indicator)	CR/NCAL/51263	27-11-2021
3	Humidity+Temperature Chamber is Used As a Source				

6 Note:

- The Calibration Certificate relates only to the above DUC
- Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab..
- Corrections/erasing, invalidate the Calibration Certificate.
- Calibration of the DUC are traceable to National standards/International Standards
- Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- Results Reported are valid at the time of and under the stated conditions of measurements
- The usage of NABL Symbol is as per NABL guidelines given in NABL-133

Calibrated By


Kiran. R

(Calibration Engineer)

Checked By

Umesh.D

(Lab In-Charge)

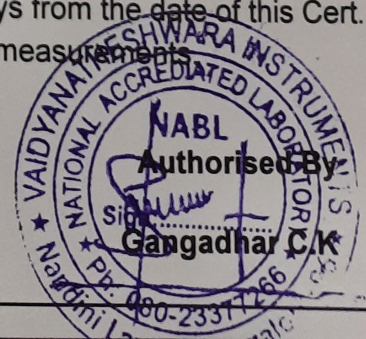

COMMITTED TO THE CUSTOMER SINCE - 1996

VAIDYANATHESHWARA INSTRUMENTS

CERTIFICATE OF CALIBRATION



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
 Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No.

RPM Results:

Page No: 2 of 2

Range: 0 to 5250 RPM

Resolution: 1 RPM

Sl. No.	Std Reading (RPM)	DUC Reading (RPM)	Error Observed in (RPM)	Measurement Uncertainty in \pm (%)	k Factor
1	199.9	200	0.1	1.2	2.0
2	599.7	600	0.3		2.0
3	999.5	1000	0.5		2.0
4	1999.2	2000	0.8		2.0
5	2998.9	3000	1.1		2.0
6	3998.6	4000	1.4		2.0
7	5248.3	5250	1.7		2.0

Timer Results:

Range: 0 to 99 min

Resolution: 1min


Sl. No.	Std Reading (hr:min:sec:msec)	DUC Reading (min)	Error Observed in (hr:min:sec:msec)	Measurement Uncertainty in \pm (%)	k Factor
1	00:00:00:000	0	00:00:00:000	----	----
2	00:15:00:012	15	-00:00:00:012	0.05	2.0
3	00:30:00:026	30	-00:00:00:026	0.05	2.0
4	00:45:00:042	45	-00:00:00:042	0.05	2.0
5	01:00:00:059	60	-00:00:00:059	0.05	2.0
6	01:39:00:067	99	-00:00:00:067	0.05	2.0

Conclusion :-

1. Measurement uncertainty reported is at 95.45 % confidence level.

Calibrated By
P. Tejo
 Madhusudhan
 (Calibration Engineer)

Checked By
P. Jay
 Umesh D
 (Onsite In-Charge)

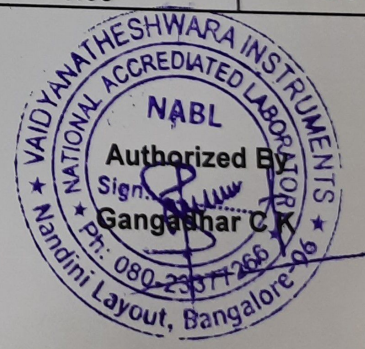



CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

1 Name and Address of the Customer : M/s. DIALOGIX HEALTH SERVICES PVT. LTD.,
Kalyan Nagar , Bangalore.

2 Customer Reference

2.1 ULR No : CC247321100010078F
2.2 SRF No : 0125
2.3 Certificate No. : VI/21-22/0125-02
2.4 Format No. : VI-FRM-ME-105
2.5 Receipt Date : 09 - 04 - 2021
2.6 Date Of Issue : 09 - 04 - 2021

3 Details Of Device Under Calibration(DUC).

3.1 Nomenclature : Pipette
3.2 Make : Merilette
3.3 Range : 100 - 1000 µl
3.4 SL No. : 317974
3.5 DUC Condition : Satisfactory
3.6 Calibration Procedure No. : SOP-16-71 Based On ISO 8655-6:2002 E
3.7 No.of Pages : 2
3.8 Calibration Date : 09-04-2021
3.9 Calibration Due : 08-04-2022
3.10 Calibration done at : VI Volumetric Lab
3.11 Discipline : Mechanical (Mass & volume)

4 Environmental Condition

Temperature 20.3 °C Humidity 53 %Rh

5 Standards Used for calibration


Sl. No.	Nomenclature	Make & Model	Sl. No	Range	Traceable to /Cert. No.	Validity
1	Digital Weighing Balance	RADWAG/MYA5.4Y	544953	0.1mg to 5g	VI/20-21/INT-ME-121	18-09-2021
2	E1 Class Weights	LCGC	VI-E1-ME-001	1mg to 200g	TVCSP1 19/04/339-01	02 - 04 - 2022

6 Note:

- 6.1. The Calibration Certificate relates only to the above DUC
- 6.2. Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab..
- 6.3. Corrections/erasing, invalidate the Calibration Certificate.
- 6.4. Calibration of the DUC are traceable to National standards/International Standards
- 6.5. Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6. Results Reported are valid at the time of and under the stated conditions of measurements
- 6.7. The usage of NABL symbol is as per NABL guidelines given in NABL-133.

Calibrated By
Sameer M S
Sameer M S
(Calibration Engineer)

Checked By
P. Santhosh Kumar
P. Santhosh Kumar
(Lab- In-Charge)

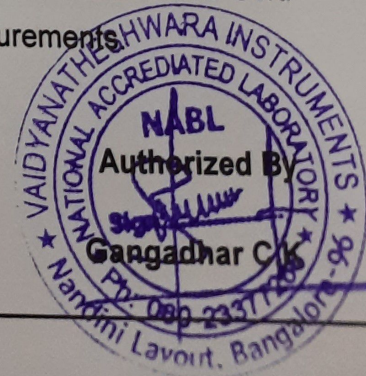

Certificate No: VI/21-22/0125-02

Page 2 of 2

Range: 100 - 1000 µl

Results:

Range	Cal Point	Volume observed	Expanded Uncertainty ±
	µl	µl	µl
100 - 1000 µl	100.0	100.328	0.62
	500.0	500.899	3.10
	1000.0	1001.456	6.20

Note:

1. Visual Inspection : Found Well.
2. Trippl Distilled water is used to Calibrate the MicroPipette.

Conclusion /Remarks:


1. Ref. standard used are traceable to National/International Standard
2. The Expanded Uncertainty of associated with measurement at approximate 95.45% confidence level with coverage factor k=2

Calibrated By

Sameer M S
(Calibration Engineer)

Checked By

P. Santhosh Kumar
(Lab- In-Charge)

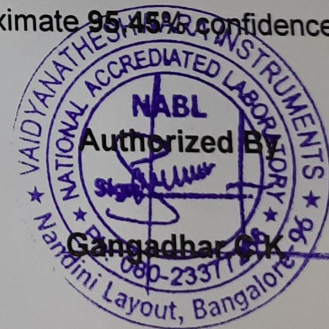



Vaidyanatheshwara INSTRUMENTS

CERTIFICATE OF CALIBRATION



COMMITTED TO THE CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

1 **Name and Address of the Customer** : M/s. DIALOGIX HEALTH SERVICES PVT. LTD.,
Kalyan Nagar , Bangalore.

2 **Customer Reference**

2.1 ULR No : CC247321100010077F
2.2 SRF No : 0125
2.3 Certificate No. : VI/21-22/0125-01
2.4 Format No. : VI-FRM-ME-105
2.5 Receipt Date : 09 - 04 - 2021
2.6 Date Of Issue : 09 - 04 - 2021

3 **Details Of Device Under Calibration(DUC).**

3.1 Nomenclature : Pipette
3.2 Make : Merilette
3.3 Range : 5 - 50 µl
3.4 SL No. : 317582
3.5 DUC Condition : Satisfactory
3.6 Calibration Procedure No. : SOP-16-71 Based On ISO 8655-6:2002 E
3.7 No.of Pages : 2
3.8 Calibration Date : 09-04-2021
3.9 Calibration Due : 08-04-2022
3.10 Calibration done at : VI Volumetric Lab
3.11 Discipline : Mechanical (Mass & volume)

4 **Environmental Condition**

Temperature 20.2 °C Humidity 51 %Rh

5 **Standards Used for calibration**

Sl. No.	Nomenclature	Make & Model	Sl. No	Range	Traceable to /Cert. No.	Validity
1	Digital Weighing Balance	RADWAG/MYA5.4Y	544953	0.1mg to 5g	VI/20-21/INT-ME-121	18-09-2021
2	E1 Class Weights	LCGC	VI-E1-ME-001	1mg to 200g	TVCSPL 19/04/339-01	02 - 04 - 2022


6 **Note:**

- 6.1. The Calibration Certificate relates only to the above DUC
- 6.2. Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab..
- 6.3. Corrections/erasing, invalidate the Calibration Certificate.
- 6.4. Calibration of the DUC are traceable to National standards/International Standards
- 6.5. Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6. Results Reported are valid at the time of and under the stated conditions of measurements
- 6.7. The usage of NABL symbol is as per NABL guidelines given in NABL-133.

Calibrated By
Sameer M S
Sameer M S
(Calibration Engineer)

Checked By
P. Santhosh Kumar
P. Santhosh Kumar
(Lab- In-Charge)





Vaidyanatheshwara INSTRUMENTS

CERTIFICATE OF CALIBRATION



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No: VI/21-22/0125-01

Page 2 of 2

Range: 5 - 50 µl

Results:

Range	Cal Point	Volume observed	Expanded Uncertainty ±
	µl	µl	µl
5 - 50 µl	5.0	5.207	0.02
	20.0	20.426	0.04
	50.0	50.946	0.20

Note:

1. Visual Inspection : Found Well.
2. Tripple Distilled water is used to Calibrate the MicroPipette.

Conclusion /Remarks:

1. Ref. standard used are traceable to National/International Standard
2. The Expanded Uncertainty of associated with measurement at approximate 95.45% confidence level with coverage factor k=2

Calibrated By

Sameer M S
(Calibration Engineer)

Checked By

P. Santhosh Kumar
(Lab- In-Charge)

