



# VAIDYANATHESHWARA INSTRUMENTS

## CERTIFICATE OF CALIBRATION



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.  
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

**1 Name and Address of the Customer**

M/s.: Energon Health...,  
No.703, 3rd Cross Road, HRBR Layout,  
1st Block, Kalyan Nagar, Bangalore - 560 043.

**2 Customer Reference**

- 2.1 ULR No. : CC2473215000023414F
- 2.2 SRF No : 0037
- 2.3 Certificate No. : VI/21-22/0037-05
- 2.4 Format No. : VI-FRM-ME-046 & VI-FRM-ET-011
- 2.5 Date of Issue : 09-04-2021

**3 Details Of Device Under Calibration(DUC).**

- 3.1 Nomenclature : Centrifuge
- 3.2 Make / Model : Remi / R-8C
- 3.3 Id.No. : EH/CF/01
- 3.4 DUC Condition : Satisfactory
- 3.5 Calibration Procedure No. : SOP-16- 42 & SOP-37-11
- 3.6 No.of Pages : 2
- 3.7 Calibration Date : 08-04-2021
- 3.8 Calibration Due : 07-04-2022
- 3.9 Calibration done at : Onsite
- 3.10 Instrument Location : Lab
- 3.11 Discipline : Mechanical

**4 Environmental Condition**

Temperature 25.3 °C Humidity: 52 %Rh

**5 Standards Used for calibration**


Sl. No.	Nomenclature	Make & Model	Sl. No. / Id.No.	Certificate No.	Validity
1	Digital Tachometer	SENTRY / ST723	SN1323004225	ULR- CC287920000004732F	10-09-2021
2	Time Totalizer	Beltronics / 501	251	VI/20-21/INT-ETH-426	23-02-2022

**6 Notes:**

- 6.1. The Calibration Certificate relates only to the above DUC
- 6.2. Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab.
- 6.3. Corrections/erasing, invalidate the Calibration Certificate.
- 6.4. Calibration of the DUC are traceable to National standards/International Standards
- 6.5. Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6. Results Reported are valid at the time of and under the stated conditions of measurements
- 6.7. The usage of NABL Symbol is as per NABL guidelines given in NABL-133

Calibrated By  
*F. Tejo*  
Madhusudhan  
(Calibration Engineer)

Checked By  
*P. Jay*  
Umesh D  
(Onsite In-Charge)

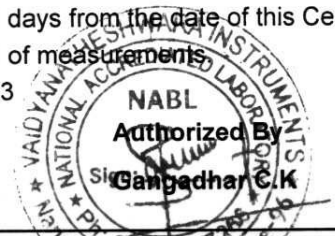



# VAIDYANATHESHWARA INSTRUMENTS

## CERTIFICATE OF CALIBRATION



COMMITTED TO THE  
CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No.

Page No: 2 of 2

**RPM Results:**

Range: 0 to 5250 RPM

Resolution: 1 RPM

Sl. No.	Std Reading (RPM)	DUC Reading (RPM)	Error Observed in (RPM)	Measurement Uncertainty in $\pm$ (%)	k Factor
1	199.9	200	0.1	1.2	2.0
2	599.7	600	0.3		2.0
3	999.5	1000	0.5		2.0
4	1999.2	2000	0.8		2.0
5	2998.9	3000	1.1		2.0
6	3998.6	4000	1.4		2.0
7	5248.3	5250	1.7		2.0

**Timer Results:**

Range: 0 to 99 min

Resolution: 1min

Sl. No.	Std Reading (hr:min:sec:msec)	DUC Reading (min)	Error Observed in (hr:min:sec:msec)	Measurement Uncertainty in $\pm$ (%)	k Factor
1	00:00:00:000	0	00:00:00:000	----	----
2	00:15:00:012	15	-00:00:00:012	0.05	2.0
3	00:30:00:026	30	-00:00:00:026	0.05	2.0
4	00:45:00:042	45	-00:00:00:042	0.05	2.0
5	01:00:00:059	60	-00:00:00:059	0.05	2.0
6	01:39:00:067	99	-00:00:00:067	0.05	2.0

**Conclusion :-**

1. Measurement uncertainty reported is at 95.45 % confidence level.

Calibrated By  
*P. Tejo*  
Madhusudhan  
(Calibration Engineer)

Checked By  
*P. Tejo*  
Umesh D  
(Onsite In-Charge)



15-04-2021 13:42:30  
13.0176318  
77.6433729



**WARNING**  
READ THE INSTRUCTIONS CAREFULLY  
BEFORE USING THE MACHINE  
DO NOT OVERLOAD THE MACHINE  
DO NOT USE HARSH DETERGENTS  
DO NOT USE BLEACH  
DO NOT USE HOT WATER  
DO NOT USE THE MACHINE FOR  
OTHER THAN WASHING CLOTHING  
DO NOT TOUCH THE DRUM  
DO NOT TOUCH THE MOTOR  
DO NOT TOUCH THE BELT  
DO NOT TOUCH THE PULLEY  
DO NOT TOUCH THE TUB  
DO NOT TOUCH THE LID  
DO NOT TOUCH THE DOOR  
DO NOT TOUCH THE HANDLE  
DO NOT TOUCH THE LOCK  
DO NOT TOUCH THE KEYS  
DO NOT TOUCH THE COIN  
DO NOT TOUCH THE DISPLAY  
DO NOT TOUCH THE BUTTONS  
DO NOT TOUCH THE SWITCHES  
DO NOT TOUCH THE DIALS  
DO NOT TOUCH THE ROTARY  
DO NOT TOUCH THE SLIDERS  
DO NOT TOUCH THE KNOBS  
DO NOT TOUCH THE LEVERS  
DO NOT TOUCH THE PEDALS  
DO NOT TOUCH THE FOOTRESTS  
DO NOT TOUCH THE SEATBELT  
DO NOT TOUCH THE SAFETY BELT  
DO NOT TOUCH THE HELMET  
DO NOT TOUCH THE GLOVES  
DO NOT TOUCH THE SHOES  
DO NOT TOUCH THE SOCKS  
DO NOT TOUCH THE TIGHTS  
DO NOT TOUCH THE UNDERWEAR  
DO NOT TOUCH THE LINGERIE  
DO NOT TOUCH THE HOSIERY  
DO NOT TOUCH THE KNITWEAR  
DO NOT TOUCH THE WOVENS  
DO NOT TOUCH THE DENIM  
DO NOT TOUCH THE JEANS  
DO NOT TOUCH THE T-SHIRTS  
DO NOT TOUCH THE BLOUSES  
DO NOT TOUCH THE DRESSES  
DO NOT TOUCH THE COATS  
DO NOT TOUCH THE SUITJACKETS  
DO NOT TOUCH THE RAINCOATS  
DO NOT TOUCH THE WINDCHEATS  
DO NOT TOUCH THE THERMALS  
DO NOT TOUCH THE WOOLLEN  
DO NOT TOUCH THE CASHMERE  
DO NOT TOUCH THE SILK  
DO NOT TOUCH THE LINEN  
DO NOT TOUCH THE COTTON  
DO NOT TOUCH THE POLYESTER  
DO NOT TOUCH THE NYLON  
DO NOT TOUCH THE SPANDEX  
DO NOT TOUCH THE ELASTIC  
DO NOT TOUCH THE RUBBER  
DO NOT TOUCH THE LEATHER  
DO NOT TOUCH THE SUEDE  
DO NOT TOUCH THE SATIN  
DO NOT TOUCH THE TAFFETA  
DO NOT TOUCH THE TULLE  
DO NOT TOUCH THE NETTING  
DO NOT TOUCH THE LACE  
DO NOT TOUCH THE EMBROIDERY  
DO NOT TOUCH THE PRINTING  
DO NOT TOUCH THE DYEING  
DO NOT TOUCH THE FINISHING  
DO NOT TOUCH THE PACKAGING  
DO NOT TOUCH THE LABELS  
DO NOT TOUCH THE TAGS  
DO NOT TOUCH THE STITCHES  
DO NOT TOUCH THE SEAMS  
DO NOT TOUCH THE COLLARS  
DO NOT TOUCH THE CUFFS  
DO NOT TOUCH THE PLEATS  
DO NOT TOUCH THE TUCKS  
DO NOT TOUCH THE GATHERINGS  
DO NOT TOUCH THE SMOCKINGS  
DO NOT TOUCH THE RUCHINGS  
DO NOT TOUCH THE SHIRTINGS  
DO NOT TOUCH THE TRIMMINGS  
DO NOT TOUCH THE ACCESSORIES  
DO NOT TOUCH THE ORNAMENTS  
DO NOT TOUCH THE DECORATIONS  
DO NOT TOUCH THE TRIMMINGS  
DO NOT TOUCH THE ACCESSORIES  
DO NOT TOUCH THE ORNAMENTS  
DO NOT TOUCH THE DECORATIONS

**REMI R-8C**

Energy Label  
Energy Class: A  
Energy Consumption (kWh/cycle): 0.85  
Water Consumption (liters/cycle): 45  
Spin Speed (rpm): 1000  
Spin Drying Class: A  
Annual Energy Consumption (kWh/year): 306  
Annual Water Consumption (liters/year): 16380  
Sound Power Level (dB(A)): 68  
Sound Pressure Level (dB(A)): 62

REMI R-8C  
Model No. R-8C  
Capacity: 8 kg  
Voltage: 230V  
Frequency: 50Hz  
Power: 1000W  
Water Inlet: 1/2 inch  
Water Outlet: 1/2 inch  
Drainage: Bottom  
Dimensions: 500x500x850 mm  
Weight: 15 kg



## CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

**1 Name and Address of the Customer** : M/s. DIALOGIX HEALTH SERVICES PVT. LTD.,  
Kalyan Nagar , Bangalore.

**2 Customer Reference**

- 2.1 ULR No : CC247321100009950F
- 2.2 SRF No : 0086
- 2.3 Certificate No. : VI/21-22/0086-01
- 2.4 Format No. : VI-FRM-ME-105
- 2.5 Receipt Date : 07 - 04 - 2021
- 2.6 Date Of Issue : 07 - 04 - 2021

**3 Details Of Device Under Calibration(DUC).**

- 3.1 Nomenclature : Pipette
- 3.2 Make : DRAGON LAB
- 3.3 Range : 5 - 50 µl
- 3.4 SL No. : YE209AS0035842
- 3.5 DUC Condition : Satisfactory
- 3.6 Calibration Procedure No. : SOP-16-71 Based On ISO 8655-6:2002 E
- 3.7 No.of Pages : 2
- 3.8 Calibration Date : 07-04-2021
- 3.9 Calibration Due : 06-04-2022
- 3.10 Calibration done at : VI Volumetric Lab
- 3.11 Discipline : Mechanical (Mass & volume)

**4 Environmental Condition**

Temperature 20.4 °C Humidity 52 %Rh

**5 Standards Used for calibration**

Sl. No.	Nomenclature	Make & Model	Sl. No	Range	Traceable to /Cert. No.	Validity
1	Digital Weighing Balance	RADWAG/MYA5.4Y	544953	0.1mg to 5g	VI/20-21/INT-ME-121	18-09-2021
2	E1 Class Weights	LCGC	VI-E1-ME-001	1mg to 200g	TVCSP 19/04/339-01	02 - 04 - 2022

**6 Note:**

- 6.1. The Calibration Certificate relates only to the above DUC
- 6.2. Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab..
- 6.3. Corrections/erasing, invalidate the Calibration Certificate.
- 6.4. Calibration of the DUC are traceable to National standards/International Standards
- 6.5. Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6. Results Reported are valid at the time of and under the stated conditions of measurements
- 6.7. The usage of NABL symbol is as per NABL guidelines given in NABL-133.

Calibrated By  
*Veda Murthy K.S*  
Veda Murthy K.S  
(Calibration Engineer)

Checked By  
*P. Santhosh Kumar*  
P. Santhosh Kumar  
(Lab- In-Charge)







# Vaidyanatheshwara Instruments



## CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No: VI/21-22/0086-01

Page 2 of 2

Range: 5 - 50 µl

Results:

Range	Cal Point	Volume observed	Expanded Uncertainty ±
	µl	µl	µl
5 - 50 µl	5.0	5.014	0.02
	20.0	20.025	0.04
	50.0	50.046	0.20

**Note:**

1. Visual Inspection : Found Well.
2. Triple Distilled water is used to Calibrate the MicroPipette.


**Conclusion /Remarks:**

1. Ref. standard used are traceable to National/International Standard
2. The Expanded Uncertainty of associated with measurement at approximate 95.45% confidence level with coverage factor k=2

Calibrated By

Veda Murthy K.S  
(Calibration Engineer)

Checked By

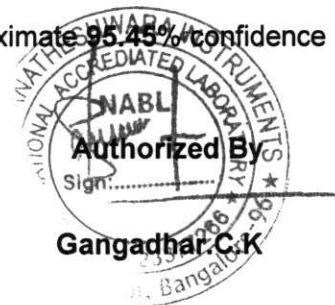  
P. Santhosh Kumar  
(Lab- In-Charge)

Gangadhar C.K



# Vaidyanatheshwara Instruments



COMMITTED TO THE CUSTOMER SINCE - 1996

## CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

**1 Name and Address of the Customer** : M/s. DIALOGIX HEALTH SERVICES PVT. LTD.,  
Kalyan Nagar , Bangalore.

**2 Customer Reference**

- 2.1 ULR No : CC247321100009951F
- 2.2 SRF No : 0086
- 2.3 Certificate No. : VI/21-22/0086-02
- 2.4 Format No. : VI-FRM-ME-105
- 2.5 Receipt Date : 07 - 04 - 2021
- 2.6 Date Of Issue : 07 - 04 - 2021

**3 Details Of Device Under Calibration(DUC).**

- 3.1 Nomenclature : Pipette
- 3.2 Make : DRAGON LAB
- 3.3 Range : 100 - 1000 µl
- 3.4 SL No. : YEAA9AD0013272
- 3.5 DUC Condition : Satisfactory
- 3.6 Calibration Procedure No. : SM/WI/M-10 Based On ISO 8655-6:2002 E
- 3.7 No.of Pages : 2
- 3.8 Calibration Date : 07-04-2021
- 3.9 Calibration Due : 06-04-2022
- 3.10 Calibration done at : VI Volumetric Lab
- 3.11 Discipline : Mechanical (Mass & Volume)

**4 Environmental Condition**

Temperature 20.4 °C Humidity 51 %Rh

**5 Standards Used for calibration**


Sl. No.	Nomenclature	Make & Model	Sl. No	Range	Traceable to /Cert. No.	Validity
1	Digital Weighing Balance	RADWAG/MYA5.4Y	544953	0.1mg to 5g	VI/20-21/INT-ME-121	18-09-2021
2	E1 Class Weights	LCGC	VI-E1-ME-001	1mg to 200g	TVCSP1 19/04/339-01	02 - 04 - 2022

**6 Note:**

- 6.1. The Calibration Certificate relates only to the above DUC
- 6.2. Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab..
- 6.3. Corrections/erasing, invalidate the Calibration Certificate.
- 6.4. Calibration of the DUC are traceable to National standards/International Standards
- 6.5. Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6. Results Reported are valid at the time of and under the stated conditions of measurements
- 6.7. The usage of NABL symbol is as per NABL guidelines given in NABL-133.

Calibrated By  
*Veda Murthy K.S*  
Veda Murthy K.S  
(Calibration Engineer)

Checked By  
*P Santhosh Kumar*  
P Santhosh Kumar  
(Lab In-Charge)

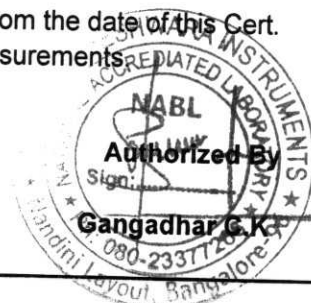



COMMITTED TO THE  
CUSTOMER SINCE - 1996

# Vaidyanatheshwara INSTRUMENTS

## CERTIFICATE OF CALIBRATION



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.  
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No: VI/21-22/0086-02

Page 2 of 2

Range: 100 - 1000  $\mu$ l

### Results:

Range	Cal Point	Volume observed	Expanded Uncertainty $\pm$
	$\mu$ l	$\mu$ l	$\mu$ l
100 - 1000 $\mu$ l	100.0	99.459	0.62
	500.0	498.838	3.10
	1000.0	998.159	6.20

### Note:

1. Visual Inspection : Found Well.
2. Tripple Distilled water is used to Calibrate the MicroPipette.

### Conclusion /Remarks:

1. Ref. standard used are traceable to National/International Standard
2. The Expanded Uncertainty of associated with measurement at approximate 95.45% confidence level with coverage factor k=2

Calibrated By

Veda Murthy K.S  
(Calibration Engineer)

Checked By

P Santhosh Kumar  
(Lab In-Charge)




**VI** Vaidyanatheshwara Ins 23377268  
Cert. No.: VI/21-22/0125-01  
SIID No.: 317582  
Cal On: 09-04-2021  
Cal Due: 08-04-2022

**VI** Vaidyanatheshwara Ins 23377268  
Cert. No.: VI/21-22/0125-02  
SIID No.: 317974  
Cal On: 09-04-2021  
Cal Due: 08-04-2022


Meril Life More Meril Life More Meril Life More  
OPTIC SEAL IS BROKEN IF SE REPORT  
REPORT IT TO



Vaidyanatheshwara  
INSTRUMENTS  
9800  
x/B  
086

	<b>Vaidyanatheshwara INS</b> ☎ 23377266
Cert. No.:	VI/21-22/0086-02
SI/ID No.:	YE209A0003272
Cal On:	07/04/2021
Cal Due:	06/04/2022

Vaidyanatheshwara  
INSTRUMENTS  
9800  
x/B  
086

	<b>Vaidyanatheshwara INS</b> ☎ 23377266
Cert. No.:	VI/21-22/0086-01
SI/ID No.:	YE209A50035842
Cal On:	07/04/2021
Cal Due:	06/04/2022



# VAIDYANATHESHWARA INSTRUMENTS

## CERTIFICATE OF CALIBRATION



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.  
 Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

**1 Name and Address of the Customer** M/s.: **Energon Health ,**  
**No.703, 3rd Cross Road, HRBR Layout ,**  
**1 st Block, Kalyan Nagar, Bangalore - 560 043.**

**2 Customer Reference**  
 2.1 ULR No. : CC247321500022900F  
 2.2 Format No. : VI-FRM-TH-006  
 2.3 SRF No. : 0032  
 2.4 Certificate No. : **VI/21-22/0032-01**  
 2.5 Date of Issue : 07-04-2021

**3 Details Of Device Under Calibration(DUC).**  
 3.1 Nomenclature : **Refrigerator**  
 3.2 Make : LG  
 3.3 Id.No. : EH/REF/01  
 3.4 Range / Resolution : 2 to 8 °C / 0.1 °C  
 3.5 DUC Condition : Satisfactory  
 3.6 Calibration Procedure No. : SOP-38-06  
 3.7 No.of Pages : 2  
 3.8 Calibration Date : **06-04-2021**  
 3.9 Calibration Due : **05-04-2022**  
 3.10 Calibration done at : Onsite  
 3.11 Instrument Location : Sample Storage  
 3.12 Discipline : Thermal


**4 Environmental Condition**  
 Temperature 26.4 °C Humidity 54 %RH


**5 Standards Used for Temperature Calibration**


Sl. No.	Nomenclature	Make / Model	Sl. No.	Certificate. No.	Validity
1	Precision Thermometer with RTD Sensor	Lutron / TM-917	Q601311	VI/20-21/INT-TH-55	28-08-2021

**6 Note:**

- 6.1.The Calibration Certificate relates only to the above DUC
- 6.2.Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI.
- 6.3.Corrections/erasing, invalidate the Calibration Certificate.
- 6.4.Calibration of the DUC are traceable to National standards/International Standards
- 6.5.Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6.Results Reported are valid at the time of and under the stated conditions of measurements.
- 6.7.The usage of NABL Symbol is as per NABL guidelines given in NABL-133

Calibrated By  
  
 Madhusudhan  
 (Calibration Engineer)

Checked By  
  
 Umesh D  
 (Onsite In-Charge)

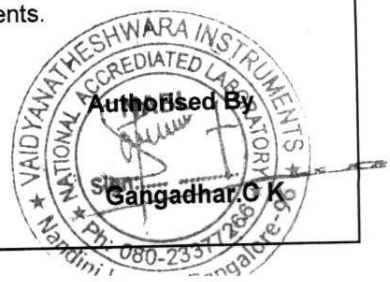





# VAIDYANATHESHWARA INSTRUMENTS

## CERTIFICATE OF CALIBRATION



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.  
 Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No. VI/21-22/0032-01


**Results:**

Range : 2 to 8 °C

Resolution: 0.1 °C

SI No	STD Reading (°C)	DUC Reading (°C)	Error Observed (°C)	Measurement Uncertainty ± (°C)	k Factor
1	2.05	2.0	-0.05	1.6	2.0
2	3.09	3.0	-0.09	1.6	2.0
3	4.13	4.0	-0.13	1.6	2.0
4	6.18	6.0	-0.18	1.6	2.0
5	8.25	8.0	-0.25	1.6	2.0

**Pictorial Representation of Sensors Placement**

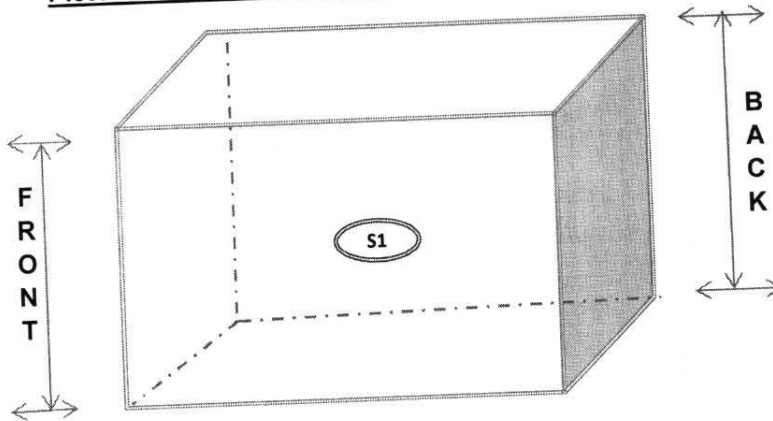

**Note :**

- S1 Indicates Placement of Standard Sensor

**Conclusion / Remarks:**

1 Measurement Uncertainty reported is at 95.45% confidence level with k = 2.

Calibrated By

*J. Prathe*  
 Madhusudan  
 (Calibration Engineer)

Checked By

*Umesh D*  
 Umesh D  
 (Onsite In-Charge)

Authorised By



15-04-2021 14:04:19

13.0176114

77.643385







# Vaidyanatheshwara Instruments

## CERTIFICATE OF CALIBRATION



COMMITTED TO THE  
CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No. VI/21-22/0087-03

Page: 2 of 2

**Results:**

Calibrated Range / Least Count : -20 to 100 °C / 0.1°C

SI No	Set Point	STD Reading (°C)	DUC Reading (°C)	Error Observed (°C)	Measurement Uncertainty ± (°C)	k Factor
1	-20	-19.94	-20.2	-0.26	0.18	2.0
2	0	0.02	-0.1	-0.12	0.18	2.0
3	40	40.06	39.8	-0.26	0.18	2.0
4	80	80.08	79.6	-0.48	0.18	2.0
5	100	100.11	99.4	-0.71	0.18	2.0

**Conclusion/Remarks:-**

1 Measurement uncertainty reported is at 95.45 % confidence level with k=2.

Calibrated By

  
Kiran. R

(Calibration Engineer)

Checked By

  
Umesh.D

(Lab In-Charge)





# VAIDYANATHESHWARA INSTRUMENTS

## CERTIFICATE OF CALIBRATION



COMMITTED TO THE  
CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.  
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Page: 1 of 2

### 1 Name and Address of the Customer

M/s.: **Energon Health.,**  
**No.703, 3rd Cross, HRBR Layout, 1st Block,**  
**Kalyan Nagar, Bangalore, Karnataka - 560 043.**

### 2 Customer Reference

2.1 ULR No. : **CC247321300001842F**  
2.2 Format No. : **VI-FRM-TH-004**  
2.3 SRF.No : **0087**  
2.4 DC No / Date : **--- / ---**  
2.5 Certificate No. : **VI/21-22/0087-02**  
2.6 Date of Issue : **07-04-2021**

### 3 Details Of Device Under Calibration(DUC).

3.1 Nomenclature : **Digital Thermometer**  
3.2 Make / Model : **--- / ---**  
3.3 Sl.No / Id. No : **--- / DTM-02**  
3.4 DUC Condition : **Satisfactory**  
3.5 Calibration Ref. Std. : **SOP-38-04**  
3.6 No.of Pages : **2**  
3.7 Calibration Date : **07-04-2021**  
3.8 Calibration Due : **06-04-2022**  
3.9 Calibration done at : **VI Thermal Lab**  
3.10 Discipline : **Thermal**

### 4 Environmental Condition

Temperature **25.2 °C** Humidity **51 %Rh**

### 5 Standards Used for Temperature Calibration

Sl. No.	Nomenclature	Make / Model	ID.No.	Certificate. No.	Validity
1	Platinum Resistance Thermometer With Indicator	FLUKE / 5609 (Sensor) & 1524 (Indicator)	03520 (Sensor) & 3028237 (Indicator)	CR/NCAL/51263	27-11-2021
2	Dry Block Calibrator is used as source.				

### 6 Note:

- The Calibration Certificate relates only to the above DUC
- Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab.
- Corrections/erasing, invalidate the Calibration Certificate.
- Calibration of the DUC are traceable to National standards/International Standards
- Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- Results Reported are valid at the time of and under the stated conditions of measurements.
- The usage of NABL Symbol is as per NABL guidelines given in NABL-133

Calibrated By

**Kiran. R**

Checked By

**Umesh.D**  
(Lab In-Charge)





# Vaidyanatheshwara Instruments

## CERTIFICATE OF CALIBRATION



COMMITTED TO THE  
CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No. VI/21-22/0087-02

Page: 2 of 2

**Results:**

Calibrated Range / Least Count : -20 to 100 °C / 0.1°C

SI No	Set Point	STD Reading (°C)	DUC Reading (°C)	Error Observed (°C)	Measurement Uncertainty ± (°C)	k Factor
1	-20	-19.94	-19.8	0.14	0.18	2.0
2	0	0.02	0.1	0.08	0.18	2.0
3	40	40.06	40.3	0.24	0.18	2.0
4	80	80.08	80.5	0.42	0.18	2.0
5	100	100.11	100.7	0.59	0.18	2.0

**Conclusion/Remarks:-**

1 Measurement uncertainty reported is at 95.45 % confidence level with k=2.

Calibrated By

Kiran. R

(Calibration Engineer)

Checked By

Umesh.D

(Lab In-Charge)





# Vaidyanatheshwara Instruments

## CERTIFICATE OF CALIBRATION



COMMITTED TO THE  
CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.  
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Page: 1 of 2

### 1 Name and Address of the Customer

M/s.: Energon Health.,  
No.703, 3rd Cross, HRBR Layout, 1st Block,  
Kalyan Nagar, Bangalore, Karnataka - 560 043.

### 2 Customer Reference

2.1 ULR No. : CC247321300001841F  
2.2 Format No. : VI-FRM-TH-004  
2.3 SRF.No : 0087  
2.4 DC No / Date : --- / ---  
2.5 Certificate No. : VI/21-22/0087-01  
2.6 Date of Issue : 07-04-2021

### 3 Details Of Device Under Calibration(DUC).

3.1 Nomenclature : Digital Thermometer  
3.2 Make / Model : --- / ---  
3.3 SI.No / Id. No : --- / DTM-01  
3.4 DUC Condition : Satisfactory  
3.5 Calibration Ref. Std. : SOP-38-04  
3.6 No.of Pages : 2  
3.7 Calibration Date : 07-04-2021  
3.8 Calibration Due : 06-04-2022  
3.9 Calibration done at : VI Thermal Lab  
3.10 Discipline : Thermal

### 4 Environmental Condition

Temperature 25.2 °C Humidity 51 %Rh

### 5 Standards Used for Temperature Calibration

Sl. No.	Nomenclature	Make / Model	ID.No.	Certificate. No.	Validity
1	Platinum Resistance Thermometer With Indicator	FLUKE / 5609 (Sensor) & 1524 (Indicator)	03520 (Sensor) & 3028237 (Indicator)	CR/NCAL/51263	27-11-2021
2	Dry Block Calibrator is used as source.				

### 6 Note:

- The Calibration Certificate relates only to the above DUC
- Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab.
- Corrections/erasing, invalidate the Calibration Certificate.
- Calibration of the DUC are traceable to National standards/International Standards
- Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- Results Reported are valid at the time of and under the stated conditions of measurements.
- The usage of NABL Symbol is as per NABL guidelines given in NABL-133

Calibrated By

Kiran. R

Checked By

Umesh.D

(Lab In-Charge)







COMMITTED TO THE CUSTOMER SINCE - 1996

# Vaidyanatheshwara Instruments

## CERTIFICATE OF CALIBRATION



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No. VI/21-22/0087-01

Page: 2 of 2

### Results:

Calibrated Range / Least Count : -20 to 100 °C / 0.1°C

SI No	Set Point	STD Reading (°C)	DUC Reading (°C)	Error Observed (°C)	Measurement Uncertainty ± (°C)	k Factor
1	-20	-19.94	-19.7	0.24	0.18	2.0
2	0	0.02	0.1	0.08	0.18	2.0
3	40	40.06	40.3	0.24	0.18	2.0
4	80	80.08	80.6	0.52	0.18	2.0
5	100	100.11	100.8	0.69	0.18	2.0

### Conclusion/Remarks:-

1 Measurement uncertainty reported is at 95.45 % confidence level with k=2.

Calibrated By

Kiran. R

(Calibration Engineer)

Checked By

Umesh.D

(Lab In-Charge)

