



VAIDYANATHESHWARA INSTRUMENTS

CERTIFICATE OF CALIBRATION



COMMITTED TO THE CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
 Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

1 Name and Address of the Customer : M/s. DIALOGIX HEALTH SERVICES PVT. LTD.,
 Kalyan Nagar , Bangalore.

2 Customer Reference

2.1 ULR No : CC247321100010077F
 2.2 SRF No : 0125
 2.3 Certificate No. : VI/21-22/0125-01
 2.4 Format No. : VI-FRM-ME-105
 2.5 Receipt Date : 09 - 04 - 2021
 2.6 Date Of Issue : 09 - 04 - 2021

3 Details Of Device Under Calibration(DUC).

3.1 Nomenclature : Pipette
 3.2 Make : Merilette
 3.3 Range : 5 - 50 µl
 3.4 SL No. : 317582
 3.5 DUC Condition : Satisfactory
 3.6 Calibration Procedure No. : SOP-16-71 Based On ISO 8655-6:2002 E
 3.7 No.of Pages : 2
 3.8 Calibration Date : 09-04-2021
 3.9 Calibration Due : 08-04-2022
 3.10 Calibration done at : VI Volumetric Lab
 3.11 Discipline : Mechanical (Mass & volume)

4 Environmental Condition

Temperature 20.2 °C Humidity 51 %Rh

5 Standards Used for calibration

Sl. No.	Nomenclature	Make & Model	Sl. No	Range	Traceable to /Cert. No.	Validity
1	Digital Weighing Balance	RADWAG/MYA5.4Y	544953	0.1mg to 5g	VI/20-21/INT-ME-121	18-09-2021
2	E1 Class Weights	LCGC	VI-E1-ME-001	1mg to 200g	TVCSP1 19/04/339-01	02 - 04 - 2022

6 Note:

- The Calibration Certificate relates only to the above DUC
- Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab..
- Corrections/erasing, invalidate the Calibration Certificate.
- Calibration of the DUC are traceable to National standards/International Standards
- Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- Results Reported are valid at the time of and under the stated conditions of measurements
- The usage of NABL symbol is as per NABL guidelines given in NABL-133.

Calibrated By

 Sameer M S
 (Calibration Engineer)

Checked By

 P. Santhosh Kumar
 (Lab- In-Charge)





VAIDYANATHESHWARA INSTRUMENTS

CERTIFICATE OF CALIBRATION



COMMITTED TO THE CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No: VI/21-22/0125-01

Page 2 of 2

Range: 5 - 50 µl

Results:

Range	Cal Point	Volume observed	Expanded Uncertainty ±
	µl	µl	µl
5 - 50 µl	5.0	5.207	0.02
	20.0	20.426	0.04
	50.0	50.946	0.20

Note:

1. Visual Inspection : Found Well.
2. Triple Distilled water is used to Calibrate the MicroPipette.

Conclusion /Remarks:


1. Ref. standard used are traceable to National/International Standard
2. The Expanded Uncertainty of associated with measurement at approximate 95.45% confidence level with coverage factor k=2

Calibrated By

Sameer M S
(Calibration Engineer)

Checked By

P. Santhosh Kumar
(Lab- In-Charge)

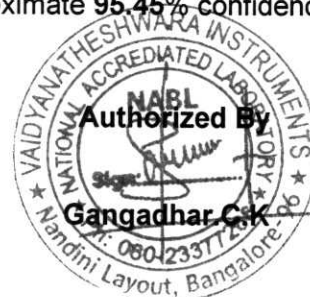

Authorized By

Gangadhar Csk



COMMITTED TO THE
CUSTOMER SINCE - 1996

VAIDYANATHESHWARA INSTRUMENTS

CERTIFICATE OF CALIBRATION



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Page 1 of 2

1 Name and Address of the Customer : M/s. DIALOGIX HEALTH SERVICES PVT. LTD.,
Kalyan Nagar , Bangalore.

2 Customer Reference

2.1 ULR No : CC247321100010078F
2.2 SRF No : 0125
2.3 Certificate No. : VI/21-22/0125-02
2.4 Format No. : VI-FRM-ME-105
2.5 Receipt Date : 09 - 04 - 2021
2.6 Date Of Issue : 09 - 04 - 2021

3 Details Of Device Under Calibration(DUC).

3.1 Nomenclature : Pipette
3.2 Make : Merilette
3.3 Range : 100 - 1000 µl
3.4 SL No. : 317974
3.5 DUC Condition : Satisfactory
3.6 Calibration Procedure No. : SOP-16-71 Based On ISO 8655-6:2002 E
3.7 No.of Pages : 2
3.8 Calibration Date : 09-04-2021
3.9 Calibration Due : 08-04-2022
3.10 Calibration done at : VI Volumetric Lab
3.11 Discipline : Mechanical (Mass & volume)

4 Environmental Condition

Temperature 20.3 °C Humidity 53 %Rh

5 Standards Used for calibration


Sl. No.	Nomenclature	Make & Model	Sl. No	Range	Traceable to /Cert. No.	Validity
1	Digital Weighing Balance	RADWAG/MYA5.4Y	544953	0.1mg to 5g	VI/20-21/INT-ME-121	18-09-2021
2	E1 Class Weights	LCGC	VI-E1-ME-001	1mg to 200g	TVCSPL 19/04/339-01	02 - 04 - 2022

6 Note:

- The Calibration Certificate relates only to the above DUC
- Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab..
- Corrections/erasing, invalidate the Calibration Certificate.
- Calibration of the DUC are traceable to National standards/International Standards
- Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- Results Reported are valid at the time of and under the stated conditions of measurements
- The usage of NABL symbol is as per NABL guidelines given in NABL-133.

Calibrated By
Sameer M S
Sameer M S
(Calibration Engineer)

Checked By
P. Santhosh Kumar
P. Santhosh Kumar
(Lab- In-Charge)

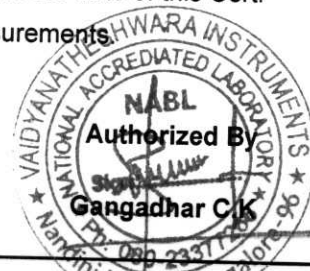



VAIDYANATHESHWARA INSTRUMENTS

CERTIFICATE OF CALIBRATION



COMMITTED TO THE
CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No: VI/21-22/0125-02

Page 2 of 2

Range: 100 - 1000 μ l

Results:

Range	Cal Point	Volume observed	Expanded Uncertainty \pm
	μ l	μ l	μ l
100 - 1000 μ l	100.0	100.328	0.62
	500.0	500.899	3.10
	1000.0	1001.456	6.20

Note:

1. Visual Inspection : Found Well.
2. Tripple Distilled water is used to Calibrate the MicroPipette.

Conclusion /Remarks:

1. Ref. standard used are traceable to National/International Standard
2. The Expanded Uncertainty of associated with measurement at approximate 95.45% confidence level with coverage factor k=2

Calibrated By


Sameer M S

Sameer M S
(Calibration Engineer)

Checked By

P. Santhosh Kumar

P. Santhosh Kumar
(Lab- In-Charge)

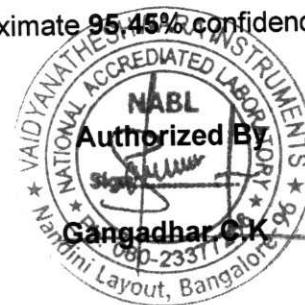

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Page: 1 of 2

1 Name and Address of the Customer

M/s.: **Energon Health ,**
No.703, 3rd Cross Road, HRBR Layout ,
1 st Block, Kalyan Nagar, Bangalore - 560 043.

2 Customer Reference

2.1 ULR No. : CC247321500022900F
2.2 Format No. : VI-FRM-TH-006
2.3 SRF No. : 0032
2.4 Certificate No. : **VI/21-22/0032-01**
2.5 Date of Issue : 07-04-2021

3 Details Of Device Under Calibration(DUC).

3.1 Nomenclature : **Refrigerator**
3.2 Make : LG
3.3 Id.No. : EH/REF/01
3.4 Range / Resolution : 2 to 8 °C / 0.1 °C
3.5 DUC Condition : Satisfactory
3.6 Calibration Procedure No. : SOP-38-06
3.7 No.of Pages : 2
3.8 Calibration Date : **06-04-2021**
3.9 Calibration Due : **05-04-2022**
3.10 Calibration done at : Onsite
3.11 Instrument Location : Sample Storage
3.12 Discipline : Thermal

4 Environmental Condition

Temperature 26.4 °C Humidity 54 %RH

5 Standards Used for Temperature Calibration

Sl. No.	Nomenclature	Make / Model	Sl. No.	Certificate. No.	Validity
1	Precision Thermometer with RTD Sensor	Lutron / TM-917	Q601311	VI/20-21/INT-TH-55	28-08-2021

6 Note:


- 6.1.The Calibration Certificate relates only to the above DUC
- 6.2.Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI.
- 6.3.Corrections/erasing, invalidate the Calibration Certificate.
- 6.4.Calibration of the DUC are traceable to National standards/International Standards
- 6.5.Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6.Results Reported are valid at the time of and under the stated conditions of measurements.
- 6.7.The usage of NABL Symbol is as per NABL guidelines given in NABL-133

Calibrated By

F. Prathi
Madhusudhan
(Calibration Engineer)

Checked By

Umesh D
Umesh D
(Onsite In-Charge)

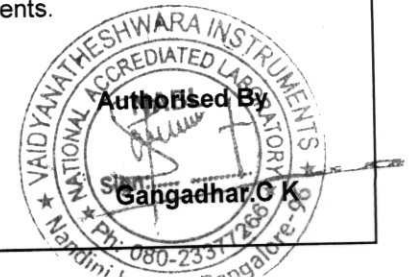



VAIDYANATHESHWARA INSTRUMENTS

CERTIFICATE OF CALIBRATION



COMMITTED TO THE CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
 Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No. VI/21-22/0032-01

Page: 2 of 2


Results:

Range : 2 to 8 °C

Resolution: 0.1 °C

SI No	STD Reading (°C)	DUC Reading (°C)	Error Observed (°C)	Measurement Uncertainty ± (°C)	k Factor
1	2.05	2.0	-0.05	1.6	2.0
2	3.09	3.0	-0.09	1.6	2.0
3	4.13	4.0	-0.13	1.6	2.0
4	6.18	6.0	-0.18	1.6	2.0
5	8.25	8.0	-0.25	1.6	2.0

Pictorial Representation of Sensors Placement

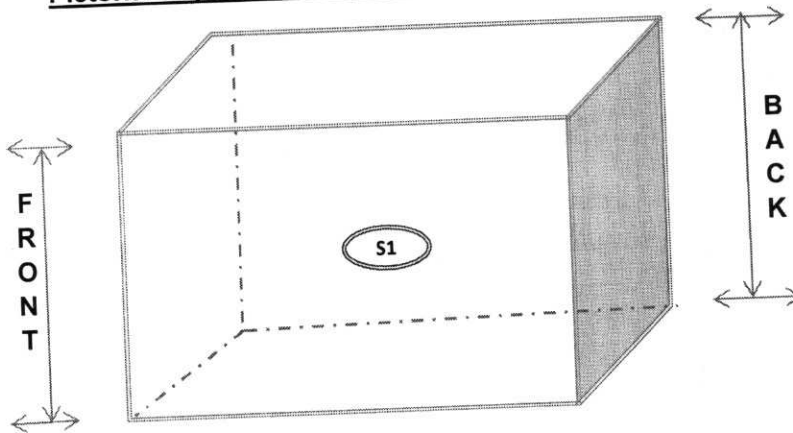

Note :

1. S1 Indicates Placement of Standard Sensor

Conclusion / Remarks:

1 Measurement Uncertainty reported is at 95.45% confidence level with k = 2.

Calibrated By

F. Pruthi
 Madhusudan
 (Calibration Engineer)

Checked By

F. Pruthi
 Umesh D
 (Onsite In-Charge)

Authorised By





VAIDYANATHESHWARA INSTRUMENTS

CERTIFICATE OF CALIBRATION



COMMITTED TO THE CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
 Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Page: 1 of 2

1 Name and Address of the Customer

M/s.: **Energon Health ,**
No.703, 3rd Cross Road, HRBR Layout ,
1 st Block, Kalyan Nagar, Bangalore - 560 043.

2 Customer Reference

- 2.1 ULR No. : CC247321500022901F
- 2.2 Format No. : VI-FRM-TH-006
- 2.3 SRF No. : 0032
- 2.4 Certificate No. : **VI/21-22/0032-02**
- 2.5 Date of Issue : 07-04-2021

3 Details Of Device Under Calibration(DUC).

- 3.1 Nomenclature : **Refrigerator**
- 3.2 Make : Whirlpool
- 3.3 Id.No. : EH/REF/02
- 3.4 Range / Resolution : 2 to 8 °C / 0.1 °C
- 3.5 DUC Condition : Satisfactory
- 3.6 Calibration Procedure No. : SOP-38-06
- 3.7 No.of Pages : 2
- 3.8 Calibration Date : **06-04-2021**
- 3.9 Calibration Due : **05-04-2022**
- 3.10 Calibration done at : Onsite
- 3.11 Instrument Location : Clinical Pathology
- 3.12 Discipline : Thermal

4 Environmental Condition

Temperature 26.4 °C Humidity 54 %RH

5 Standards Used for Temperature Calibration

Sl. No.	Nomenclature	Make / Model	Sl. No.	Certificate. No.	Validity
1	Precision Thermometer with RTD Sensor	Lutron / TM-917	Q601311	VI/20-21/INT-TH-55	28-08-2021

6 Note:

- 6.1.The Calibration Certificate relates only to the above DUC
- 6.2.Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI.
- 6.3.Corrections/erasing, invalidate the Calibration Certificate.
- 6.4.Calibration of the DUC are traceable to National standards/International Standards
- 6.5.Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6.Results Reported are valid at the time of and under the stated conditions of measurements.
- 6.7.The usage of NABL Symbol is as per NABL guidelines given in NABL-133

Calibrated By

F. Pruthi
Madhusudhan
 (Calibration Engineer)

Checked By

F. Pruthi
Umesh D
 (Onsite In-Charge)





VAIDYANATHESHWARA INSTRUMENTS

CERTIFICATE OF CALIBRATION



COMMITTED TO THE
CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No. VI/21-22/0032-02

Page: 2 of 2


Results:

Range : 2 to 8 °C

Resolution: 0.1 °C

SI No	STD Reading (°C)	DUC Reading (°C)	Error Observed (°C)	Measurement Uncertainty ± (°C)	k Factor
1	2.02	2.0	-0.02	1.6	2.0
2	3.05	3.0	-0.05	1.6	2.0
3	4.10	4.0	-0.10	1.6	2.0
4	6.15	6.0	-0.15	1.6	2.0
5	8.20	8.0	-0.20	1.6	2.0

Pictorial Representation of Sensors Placement

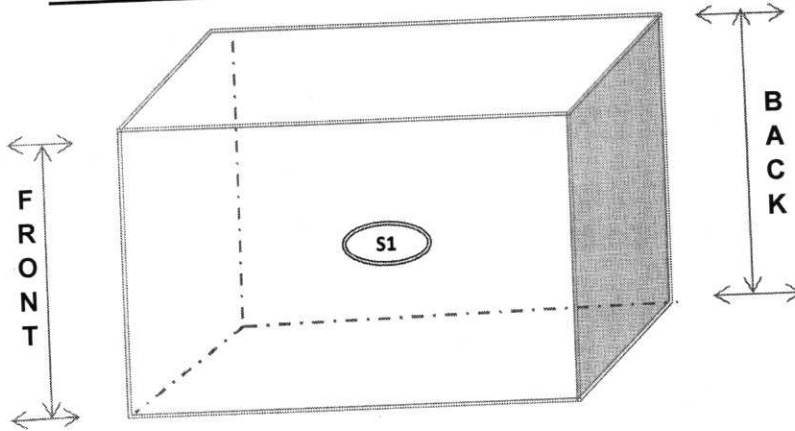

Note :

- S1 Indicates Placement of Standard Sensor

Conclusion / Remarks:

1 Measurement Uncertainty reported is at 95.45% confidence level with k = 2

Calibrated By

F. Jeeithi
Madhusudan
(Calibration Engineer)

Checked By

Umesh D
Umesh D
(Onsite In-Charge)

Authorised By





VAIDYANATHESHWARA INSTRUMENTS

CERTIFICATE OF CALIBRATION



COMMITTED TO THE
CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Page: 1 of 2

1 Name and Address of the Customer

M/s.: **Energon Health ,**
No.703, 3rd Cross Road, HRBR Layout ,
1 st Block, Kalyan Nagar, Bangalore - 560 043.

2 Customer Reference

2.1 ULR No. : CC247321500022902F
2.2 SRF No. : 0032
2.3 Certificate No. : **VI/21-22/0032-03**
2.4 Format No. : VI-FRM-TH-008
2.5 Date of Issue : 07-04-2021

3 Details Of Device Under Calibration(DUC).

3.1 Nomenclature : **Deep Freezer**
3.2 Make : Indicool
3.3 ID.No. : EH/DF/01
3.4 Range / Resolution : -18 to -22 °C / 0.1 °C
3.5 DUC Condition : Satisfactory
3.6 Calibration Procedure No. : SOP-38-08
3.7 No.of Pages : 2
3.8 Calibration Date : **06-04-2021**
3.9 Calibration Due : **05-04-2022**
3.10 Calibration done at : Onsite
3.11 Instrument Location : Clinical Pathology
3.12 Discipline : Thermal

4 Environmental Condition

Temperature 26.8 °C Humidity 56 %RH

5 Standards Used for Temperature Calibration

Sl. No.	Nomenclature	Make / Model	Sl. No.	Certificate. No.	Validity
1	Precision Thermometer with RTD Sensor	Lutron / TM-917	Q601311	VI/20-21/INT-TH-55	28-08-2021

6 Note:

- The Calibration Certificate relates only to the above DUC
- Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI.
- Corrections/erasing, invalidate the Calibration Certificate.
- Calibration of the DUC are traceable to National standards/International Standards
- Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- Results Reported are valid at the time of and under the stated conditions of measurements
- The usage of NABL Symbol is as per NABL guidelines given in NABL-133

Calibrated By
F. Pruthi
Madhusudhan

Checked By
F. Pruthi
Umesh.D
(Onsite In-Charge)





Vaidyanatheshwara Instruments

CERTIFICATE OF CALIBRATION



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
 Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No. VI/21-22/0032-03


Page: 2 of 2

Results:

Range / Resolution : -18 to -22 °C / 0.1 °C

SI No	STD Reading (°C)	DUC Reading (°C)	Error Observed (°C)	Measurement Uncertainty ± (°C)	k Factor
1	-18.07	-18.0	0.07	1.6	2.0
2	-19.09	-19.0	0.09	1.6	2.0
3	-20.11	-20.0	0.11	1.6	2.0
4	-21.13	-21.0	0.13	1.6	2.0
5	-22.15	-22.0	0.15	1.6	2.0

Pictorial Representation of Sensors Placement

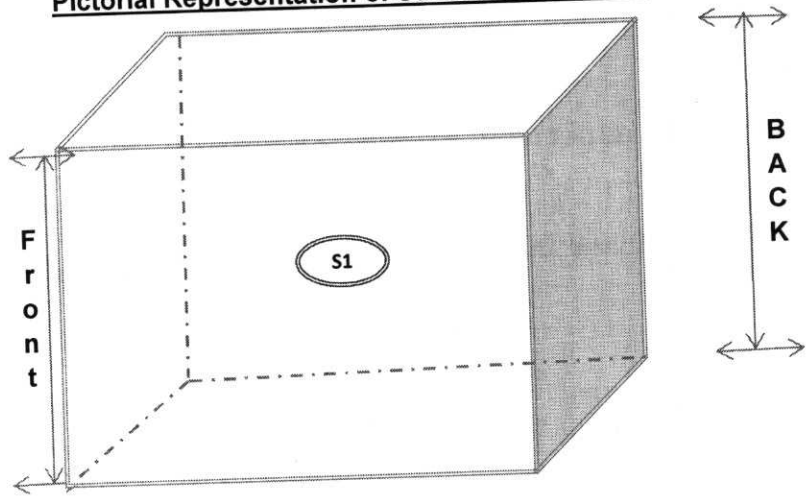

Note :

1. S1 Indicates Placement of Standard Sensor
2. Calibration done in empty condition.

Conclusion / Remarks:

1 Measurement Uncertainty reported is at 95.45% confidence level with k = 2

Calibrated By
F. Jothi
 Madhusudhan
 (Calibration Engineer)

Checked By
F. Jothi
 Umesh.D
 (Onsite In-Charge)





Vaidyanatheshwara Instruments

CERTIFICATE OF CALIBRATION



COMMITTED TO THE
CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Page 1 of 2

1 Name and Address of Customer

M/s.: Energon Health.,
No.703, 3rd Cross, HRBR Layout, 1st Block,
Kalyan Nagar, Bangalore, Karnataka - 560 043.

2 Customer Reference

2.1 ULR No. : CC247321300001845F
2.2 Format No. : VI-FRM-TH-002
2.3 SRF No. : 0087
2.4 DC No / Date : --- / ---
2.5 Certification No. : VI/21-22/0087-05
2.6 Date of Issue : 07-04-2021

3 Details Of Device Under Calibration(DUC).

3.1 Nomenclature : Digital Thermo-Hygrometer
3.2 Make / Model : --- / HTC-1
3.3 SI.No. / ID.No. : --- / DHTM-02
3.4 DUC Condition : Satisfactory
3.5 Calibration Procedure No. : SOP - 38-02
3.6 No.of Pages : 2
3.7 Calibration Date : 07-04-2021
3.8 Calibration Due : 06-04-2022
3.9 Calibration done at : VI Thermal Lab
3.10 Discipline : Thermal

4 Environmental Condition:

Temperature 25.4 °C Humidity 53 %RH

5 Standards Used for calibration:

Sl. No	Nomenclature	Make & Model	SI. No	Certificate No.	Validity
1	Hygropalm With Sensor	Rotronic / HP23	60885044 & 20146871	CR/NCAL/51117	05-08-2021
2	Platinum Resistance Thermometer With Indicator	FLUKE / 5609 (Sensor) & 1524 (Indicator)	03520 (Sensor) & 3028237 (Indicator)	CR/NCAL/51263	27-11-2021
3	Humidity+Temperature Chamber is Used As a Source				

6 Note:


- The Calibration Certificate relates only to the above DUC
- Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab..
- Corrections/erasing, invalidate the Calibration Certificate.
- Calibration of the DUC are traceable to National standards/International Standards
- Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- Results Reported are valid at the time of and under the stated conditions of measurements
- The usage of NABL Symbol is as per NABL guidelines given in NABL-133

Calibrated By

Kiran. R

Checked By

Umesh.D
(Lab In-Charge)

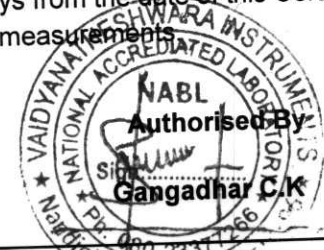



COMMITTED TO THE
CUSTOMER SINCE - 1996

VAIDYANATHESHWARA INSTRUMENTS

CERTIFICATE OF CALIBRATION



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certification No. VI/21-22/0087-05

Page No: 2 of 2

Results:

Range / Resolution : -50 to 70 °C / 0.1 °C

Test Results of Temperature @ 65%RH

SI No	Set Point (°C)	DUC Reading (°C)	STD Reading (°C)	Error Observed (°C)	Measurement Uncertainty ± (°C)	k Factor
1	15	14.7	15.04	-0.34	0.18	2.0
2	30	29.5	30.06	-0.56	0.18	2.0
3	45	44.3	45.08	-0.78	0.18	2.0

Range / Resolution : 10 to 99 % RH / 1% RH

Test Results of Humidity @ 25°C

SI No	Set Point (%RH)	DUC Reading (%RH)	STD Reading (%RH)	Error Observed (%RH)	Measurement Uncertainty ± (%RH)	k Factor
1	30	28	30.07	-2.07	1.48	2.0
2	50	47	50.09	-3.09	1.48	2.0
3	80	77	80.13	-3.13	1.48	2.0

Conclusion / Remarks:

1. Measurement Uncertainty reported is at 95.45% confidence level with k = 2.

Calibrated By

Kiran. R
(Calibration Engineer)

Checked By

Umesh.D
(Lab In-Charge)





VAIDYANATHESHWARA INSTRUMENTS

CERTIFICATE OF CALIBRATION



COMMITTED TO THE
CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Page: 1 of 2

1 Name and Address of the Customer

M/s.: Energon Health.,
No.703, 3rd Cross, HRBR Layout, 1st Block,
Kalyan Nagar, Bangalore, Karnataka - 560 043.

2 Customer Reference

2.1 ULR No. : CC247321300001843F
2.2 Format No. : VI-FRM-TH-004
2.3 SRF.No : 0087
2.4 DC No / Date : --- / ---
2.5 Certificate No. : VI/21-22/0087-03
2.6 Date of Issue : 07-04-2021

3 Details Of Device Under Calibration(DUC).

3.1 Nomenclature : Digital Thermometer
3.2 Make / Model : --- / ---
3.3 SI.No / Id. No : --- / DTM-03
3.4 DUC Condition : Satisfactory
3.5 Calibration Ref. Std. : SOP-38-04
3.6 No.of Pages : 2
3.7 Calibration Date : 07-04-2021
3.8 Calibration Due : 06-04-2022
3.9 Calibration done at : VI Thermal Lab
3.10 Discipline : Thermal

4 Environmental Condition

Temperature 25.2 °C Humidity 51 %Rh

5 Standards Used for Temperature Calibration

Sl. No.	Nomenclature	Make / Model	ID.No.	Certificate. No.	Validity
1	Platinum Resistance Thermometer With Indicator	FLUKE / 5609 (Sensor) & 1524 (Indicator)	03520 (Sensor) & 3028237 (Indicator)	CR/NCAL/51263	27-11-2021
2	Dry Block Calibrator is used as source.				

6 Note:


- The Calibration Certificate relates only to the above DUC
- Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab.
- Corrections/erasing, invalidate the Calibration Certificate.
- Calibration of the DUC are traceable to National standards/International Standards
- Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- Results Reported are valid at the time of and under the stated conditions of measurements.
- The usage of NABL Symbol is as per NABL guidelines given in NABL-133

Calibrated By

K. R. K. Man.

Checked By

Umesh.D.

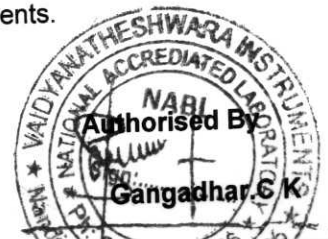



Vaidyanatheshwara INSTRUMENTS

CERTIFICATE OF CALIBRATION



COMMITTED TO THE
CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No. VI/21-22/0087-03

Page: 2 of 2

Results:

Calibrated Range / Least Count : -20 to 100 °C / 0.1°C

SI No	Set Point	STD Reading (°C)	DUC Reading (°C)	Error Observed (°C)	Measurement Uncertainty ± (°C)	k Factor
1	-20	-19.94	-20.2	-0.26	0.18	2.0
2	0	0.02	-0.1	-0.12	0.18	2.0
3	40	40.06	39.8	-0.26	0.18	2.0
4	80	80.08	79.6	-0.48	0.18	2.0
5	100	100.11	99.4	-0.71	0.18	2.0

Conclusion/Remarks:-

1 Measurement uncertainty reported is at 95.45 % confidence level with k=2.

Calibrated By


Kiran. R

(Calibration Engineer)

Checked By


Umesh.D

(Lab In-Charge)





VAIDYANATHESHWARA INSTRUMENTS

CERTIFICATE OF CALIBRATION



COMMITTED TO THE
CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Page: 1 of 2

1 Name and Address of the Customer

M/s.: **Energion Health.,**
No.703, 3rd Cross, HRBR Layout, 1st Block,
Kalyan Nagar, Bangalore, Karnataka - 560 043.

2 Customer Reference

2.1 ULR No. : **CC247321300001842F**
2.2 Format No. : **VI-FRM-TH-004**
2.3 SRF.No : **0087**
2.4 DC No / Date : **--- / ---**
2.5 Certificate No. : **VI/21-22/0087-02**
2.6 Date of Issue : **07-04-2021**

3 Details Of Device Under Calibration(DUC).

3.1 Nomenclature : **Digital Thermometer**
3.2 Make / Model : **--- / ---**
3.3 SI.No / Id. No : **--- / DTM-02**
3.4 DUC Condition : **Satisfactory**
3.5 Calibration Ref. Std. : **SOP-38-04**
3.6 No.of Pages : **2**
3.7 Calibration Date : **07-04-2021**
3.8 Calibration Due : **06-04-2022**
3.9 Calibration done at : **VI Thermal Lab**
3.10 Discipline : **Thermal**

4 Environmental Condition

Temperature **25.2 °C** Humidity **51 %Rh**

5 Standards Used for Temperature Calibration

SI. No.	Nomenclature	Make / Model	ID.No.	Certificate. No.	Validity
1	Platinum Resistance Thermometer With Indicator	FLUKE / 5609 (Sensor) & 1524 (Indicator)	03520 (Sensor) & 3028237 (Indicator)	CR/NCAL/51263	27-11-2021
2	Dry Block Calibrator is used as source.				

6 Note:

- The Calibration Certificate relates only to the above DUC
- Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab.
- Corrections/erasing, invalidate the Calibration Certificate.
- Calibration of the DUC are traceable to National standards/International Standards
- Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- Results Reported are valid at the time of and under the stated conditions of measurements.
- The usage of NABL Symbol is as per NABL guidelines given in NABL-133

Calibrated By

Kiran. R

Checked By

Umesh.D
(Lab In-Charge)





Vaidyanatheshwara Instruments



CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No. VI/21-22/0087-02

Page: 2 of 2

Results:

Calibrated Range / Least Count : -20 to 100 °C / 0.1°C

SI No	Set Point	STD Reading (°C)	DUC Reading (°C)	Error Observed (°C)	Measurement Uncertainty ± (°C)	k Factor
1	-20	-19.94	-19.8	0.14	0.18	2.0
2	0	0.02	0.1	0.08	0.18	2.0
3	40	40.06	40.3	0.24	0.18	2.0
4	80	80.08	80.5	0.42	0.18	2.0
5	100	100.11	100.7	0.59	0.18	2.0

Conclusion/Remarks:-

1 Measurement uncertainty reported is at 95.45 % confidence level with k=2.

Calibrated By

Kiran. R

(Calibration Engineer)

Checked By

Umesh.D

(Lab In-Charge)





Vaidyanatheshwara Instruments



CERTIFICATE OF CALIBRATION

COMMITTED TO THE CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

1 Name and Address of the Customer

M/s.: Energon Health.,
No.703, 3rd Cross, HRBR Layout, 1st Block,
Kalyan Nagar, Bangalore, Karnataka - 560 043.

2 Customer Reference

2.1 ULR No. : CC247321300001841F
2.2 Format No. : VI-FRM-TH-004
2.3 SRF.No : 0087
2.4 DC No / Date : --- / ---
2.5 Certificate No. : VI/21-22/0087-01
2.6 Date of Issue : 07-04-2021

3 Details Of Device Under Calibration(DUC).

3.1 Nomenclature : Digital Thermometer
3.2 Make / Model : --- / ---
3.3 SI.No / Id. No : --- / DTM-01
3.4 DUC Condition : Satisfactory
3.5 Calibration Ref. Std. : SOP-38-04
3.6 No.of Pages : 2
3.7 Calibration Date : 07-04-2021
3.8 Calibration Due : 06-04-2022
3.9 Calibration done at : VI Thermal Lab
3.10 Discipline : Thermal

4 Environmental Condition

Temperature 25.2 °C Humidity 51 %Rh

5 Standards Used for Temperature Calibration

Sl. No.	Nomenclature	Make / Model	ID.No.	Certificate. No.	Validity
1	Platinum Resistance Thermometer With Indicator	FLUKE / 5609 (Sensor) & 1524 (Indicator)	03520 (Sensor) & 3028237 (Indicator)	CR/NCAL/51263	27-11-2021
2	Dry Block Calibrator is used as source.				

6 Note:

- The Calibration Certificate relates only to the above DUC
- Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab.
- Corrections/erasing, invalidate the Calibration Certificate.
- Calibration of the DUC are traceable to National standards/International Standards
- Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- Results Reported are valid at the time of and under the stated conditions of measurements.
- The usage of NABL Symbol is as per NABL guidelines given in NABL-133

Calibrated By

Kiran. R

Checked By

Umesh.D

(Lab In-Charge)





COMMITTED TO THE
CUSTOMER SINCE - 1996

VAIDYANATHESHWARA INSTRUMENTS

CERTIFICATE OF CALIBRATION



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No. VI/21-22/0087-01

Page: 2 of 2

Results:

Calibrated Range / Least Count : -20 to 100 °C / 0.1°C

Sl No	Set Point	STD Reading (°C)	DUC Reading (°C)	Error Observed (°C)	Measurement Uncertainty ± (°C)	k Factor
1	-20	-19.94	-19.7	0.24	0.18	2.0
2	0	0.02	0.1	0.08	0.18	2.0
3	40	40.06	40.3	0.24	0.18	2.0
4	80	80.08	80.6	0.52	0.18	2.0
5	100	100.11	100.8	0.69	0.18	2.0

Conclusion/Remarks:-

1 Measurement uncertainty reported is at 95.45 % confidence level with k=2.

Calibrated By


Kiran. R

(Calibration Engineer)

Checked By


Umesh.D

(Lab In-Charge)





CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

1 Name and Address of the Customer : M/s. DIALOGIX HEALTH SERVICES PVT. LTD.,
Kalyan Nagar , Bangalore.

2 Customer Reference

- 2.1 ULR No : CC247321100009950F
- 2.2 SRF No : 0086
- 2.3 Certificate No. : VI/21-22/0086-01
- 2.4 Format No. : VI-FRM-ME-105
- 2.5 Receipt Date : 07 - 04 - 2021
- 2.6 Date Of Issue : 07 - 04 - 2021

3 Details Of Device Under Calibration(DUC).

- 3.1 Nomenclature : Pipette
- 3.2 Make : DRAGON LAB
- 3.3 Range : 5 - 50 µl
- 3.4 SL No. : YE209AS0035842
- 3.5 DUC Condition : Satisfactory
- 3.6 Calibration Procedure No. : SOP-16-71 Based On ISO 8655-6:2002 E
- 3.7 No.of Pages : 2
- 3.8 Calibration Date : 07-04-2021
- 3.9 Calibration Due : 06-04-2022
- 3.10 Calibration done at : VI Volumetric Lab
- 3.11 Discipline : Mechanical (Mass & volume)

4 Environmental Condition

Temperature 20.4 °C Humidity 52 %Rh

5 Standards Used for calibration

Sl. No.	Nomenclature	Make & Model	Sl. No	Range	Traceable to /Cert. No.	Validity
1	Digital Weighing Balance	RADWAG/MYA5.4Y	544953	0.1mg to 5g	VI/20-21/INT-ME-121	18-09-2021
2	E1 Class Weights	LCGC	VI-E1-ME-001	1mg to 200g	TVCSPL 19/04/339-01	02 - 04 - 2022

6 Note:

- 6.1. The Calibration Certificate relates only to the above DUC
- 6.2. Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab..
- 6.3. Corrections/erasing, invalidate the Calibration Certificate.
- 6.4. Calibration of the DUC are traceable to National standards/International Standards
- 6.5. Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6. Results Reported are valid at the time of and under the stated conditions of measurements
- 6.7. The usage of NABL symbol is as per NABL guidelines given in NABL-133.

Calibrated By
Veda Murthy K.S
Veda Murthy K.S
(Calibration Engineer)

Checked By
P. Santhosh Kumar
P. Santhosh Kumar
(Lab- In-Charge)





Vaidyanatheshwara Instruments



CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No: VI/21-22/0086-01

Page 2 of 2

Range: 5 - 50 µl

Results:

Range	Cal Point	Volume observed	Expanded Uncertainty ±
	µl	µl	µl
5 - 50 µl	5.0	5.014	0.02
	20.0	20.025	0.04
	50.0	50.046	0.20

Note:

1. Visual Inspection : Found Well.
2. Triple Distilled water is used to Calibrate the MicroPipette.

Conclusion /Remarks:

1. Ref. standard used are traceable to National/International Standard
2. The Expanded Uncertainty of associated with measurement at approximate 95.45% confidence level with coverage factor k=2

Calibrated By

Veda Murthy K.S
Veda Murthy K.S
 (Calibration Engineer)

Checked By

P. Santhosh Kumar
P. Santhosh Kumar
 (Lab- In-Charge)





Vaidyanatheshwara Instruments



CERTIFICATE OF CALIBRATION

COMMITTED TO THE CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

1 Name and Address of the Customer : M/s. DIALOGIX HEALTH SERVICES PVT. LTD.,
Kalyan Nagar , Bangalore.

2 Customer Reference

- 2.1 ULR No : CC247321100009951F
- 2.2 SRF No : 0086
- 2.3 Certificate No. : VI/21-22/0086-02
- 2.4 Format No. : VI-FRM-ME-105
- 2.5 Receipt Date : 07 - 04 - 2021
- 2.6 Date Of Issue : 07 - 04 - 2021

3 Details Of Device Under Calibration(DUC).

- 3.1 Nomenclature : Pipette
- 3.2 Make : DRAGON LAB
- 3.3 Range : 100 - 1000 µl
- 3.4 SL No. : YEAA9AD0013272
- 3.5 DUC Condition : Satisfactory
- 3.6 Calibration Procedure No. : SM/WI/M-10 Based On ISO 8655-6:2002 E
- 3.7 No.of Pages : 2
- 3.8 Calibration Date : 07-04-2021
- 3.9 Calibration Due : 06-04-2022
- 3.10 Calibration done at : VI Volumetric Lab
- 3.11 Discipline : Mechanical (Mass & Volume)

4 Environmental Condition

Temperature 20.4 °C Humidity 51 %Rh

5 Standards Used for calibration


Sl. No.	Nomenclature	Make & Model	Sl. No	Range	Traceable to /Cert. No.	Validity
1	Digital Weighing Balance	RADWAG/MYA5.4Y	544953	0.1mg to 5g	VI/20-21/INT-ME-121	18-09-2021
2	E1 Class Weights	LCGC	VI-E1-ME-001	1mg to 200g	TVCSP1 19/04/339-01	02 - 04 - 2022

6 Note:

- 6.1. The Calibration Certificate relates only to the above DUC
- 6.2. Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab..
- 6.3. Corrections/erasing, invalidate the Calibration Certificate.
- 6.4. Calibration of the DUC are traceable to National standards/International Standards
- 6.5. Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6. Results Reported are valid at the time of and under the stated conditions of measurements
- 6.7. The usage of NABL symbol is as per NABL guidelines given in NABL-133.

Calibrated By
Veda Murthy K.S
Veda Murthy K.S
(Calibration Engineer)

Checked By
P Santhosh Kumar
P Santhosh Kumar
(Lab In-Charge)

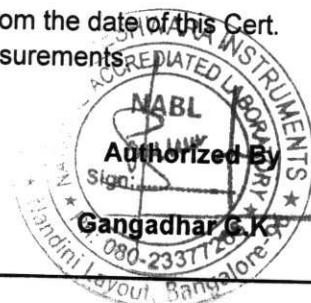



COMMITTED TO THE
CUSTOMER SINCE - 1996

Vaidyanatheshwara INSTRUMENTS

CERTIFICATE OF CALIBRATION



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No: VI/21-22/0086-02

Page 2 of 2

Range: 100 - 1000 μ l

Results:

Range	Cal Point	Volume observed	Expanded Uncertainty \pm
	μ l	μ l	μ l
100 - 1000 μ l	100.0	99.459	0.62
	500.0	498.838	3.10
	1000.0	998.159	6.20

Note:

1. Visual Inspection : Found Well.
2. Tripple Distilled water is used to Calibrate the MicroPipette.

Conclusion /Remarks:


1. Ref. standard used are traceable to National/International Standard
2. The Expanded Uncertainty of associated with measurement at approximate 95.45% confidence level with coverage factor k=2

Calibrated By

Veda Murthy K.S
Veda Murthy K.S
(Calibration Engineer)

Checked By

P Santhosh Kumar
P Santhosh Kumar
(Lab In-Charge)

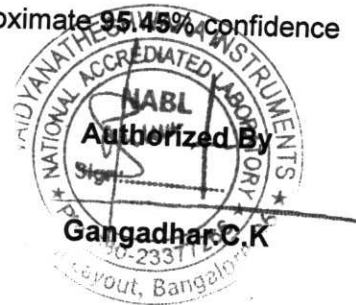



COMMITTED TO THE
CUSTOMER SINCE - 1996

VAIDYANATHESHWARA INSTRUMENTS

CERTIFICATE OF CALIBRATION



CERTIFICATE NO
CC-2473

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Page 1 of 2

1 Name and Address of Customer

M/s.: **Energon Health.,**
No.703, 3rd Cross, HRBR Layout, 1st Block,
Kalyan Nagar, Bangalore, Karnataka - 560 043.

2 Customer Reference

2.1 ULR No. : **CC247321300001844F**
2.2 Format No. : **VI-FRM-TH-002**
2.3 SRF No : **0087**
2.4 DC No / Date : **--- / ---**
2.5 Certification No. : **VI/21-22/0087-04**
2.6 Date of Issue : **07-04-2021**

3 Details Of Device Under Calibration(DUC).

3.1 Nomenclature : **Digital Thermo-Hygrometer**
3.2 Make / Model : **--- / HTC-1**
3.3 SI.No. / ID.No. : **--- / DHTM-01**
3.4 DUC Condition : **Satisfactory**
3.5 Calibration Procedure No. : **SOP - 38-02**
3.6 No.of Pages : **2**
3.7 Calibration Date : **07-04-2021**
3.8 Calibration Due : **06-04-2022**
3.9 Calibration done at : **VI Thermal Lab**
3.10 Discipline : **Thermal**

4 Environmental Condition:

Temperature 25.4 °C Humidity 53 %RH

5 Standards Used for calibration:

Sl. No	Nomenclature	Make & Model	Sl. No	Certificate No.	Validity
1	Hygropalm With Sensor	Rotronic / HP23	60885044 & 20146871	CR/NCAL/51117	05-08-2021
2	Platinum Resistance Thermometer With Indicator	FLUKE / 5609 (Sensor) & 1524 (Indicator)	03520 (Sensor) & 3028237 (Indicator)	CR/NCAL/51263	27-11-2021

3 Humidity+Temperature Chamber is Used As a Source

6 Note:

- 6.1. The Calibration Certificate relates only to the above DUC
- 6.2. Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab..
- 6.3. Corrections/erasing, invalidate the Calibration Certificate.
- 6.4. Calibration of the DUC are traceable to National standards/International Standards
- 6.5. Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6. Results Reported are valid at the time of and under the stated conditions of measurements.
- 6.7. The usage of NABL Symbol is as per NABL guidelines given in NABL-133

Calibrated By

Kiran. R

(Calibration Engineer)

Checked By

Umesh.D

(Lab In-Charge)





COMMITTED TO THE
CUSTOMER SINCE - 1996

Vaidyanatheshwara Instruments

CERTIFICATE OF CALIBRATION



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Contact : 080-23377266, Mob : 9986586789 / 9448080177 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certification No. VI/21-22/0087-04

Page No: 2 of 2

Results:

Range / Resolution : -50 to 70 °C / 0.1 °C

Test Results of Temperature @ 65%RH

SI No	Set Point (°C)	DUC Reading (°C)	STD Reading (°C)	Error Observed (°C)	Measurement Uncertainty ± (°C)	k Factor
1	15	15.3	15.04	0.26	0.18	2.0
2	30	30.5	30.06	0.44	0.18	2.0
3	45	45.7	45.08	0.62	0.18	2.0

Range / Resolution : 10 to 99 % RH / 1% RH

Test Results of Humidity @ 25°C

SI No	Set Point (%RH)	DUC Reading (%RH)	STD Reading (%RH)	Error Observed (%RH)	Measurement Uncertainty ± (%RH)	k Factor
1	30	32	30.07	1.93	1.48	2.0
2	50	53	50.09	2.91	1.48	2.0
3	80	84	80.13	3.87	1.48	2.0

Conclusion / Remarks:


1. Measurement Uncertainty reported is at 95.45% confidence level with k = 2.

Calibrated By


Kiran. R

(Calibration Engineer)

Checked By


Umesh.D
(Lab In-Charge)

