

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021


Biochemistry, Albumin, g/dL

	N	Mean	SD	CV%	Excluded
All Methods	168	3.99	0.47	11.65	4
Bromcresol Green (BCG)	160	4.01	0.46	11.41	4
RANDOX RX daytona	1	--	--	--	--

Your Result	3.60	SDI / z-Score	-0.43
Assigned Value	3.73	Average SDI	-0.43
SDPA	0.294	Uncertainty of AV	0.02
Standard Unit Result Val	3.60	%DEV	-10.13

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

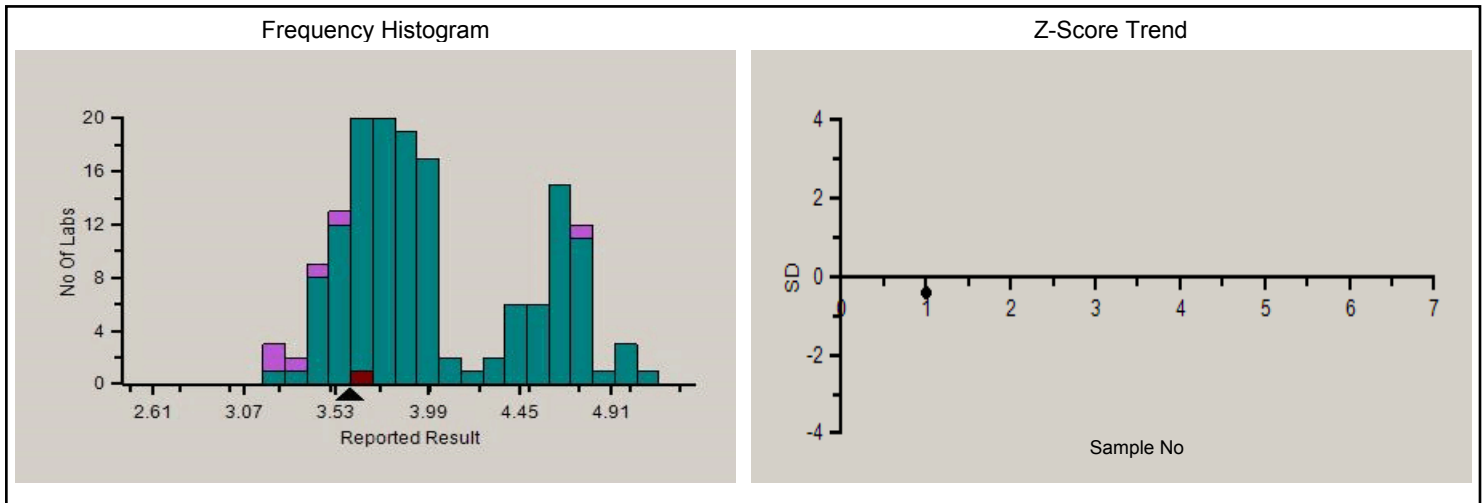

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Biochemistry, Albumin		N	Mean	SD	CV%	Excluded
	All Analyzer	168	3.99	0.47	11.65	4
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	31	4.60	0.20	4.37	--
	Roche cobas c 311	28	3.82	0.13	3.38	--
	Fuji Dri-Chem 4000i	16	4.74	0.20	4.15	--
	Horiba ABX Pentra C200	10	3.55	0.15	4.12	--
	Roche cobas c 111	10	3.91	0.13	3.23	--
	Roche cobas INTEGRA	10	3.80	0.13	3.35	--
	Erba EM 200	8	3.58	0.10	2.71	--
	Roche cobas 6000	8	3.81	0.16	4.20	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, ALP, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	167	87.20	13.87	15.91	18
■ PNPP, AMP Buffer	77	95.05	14.81	15.59	7
■ RANDOX RX daytona	1	--	--	--	1

Your Result	56.00	SDI / z-Score	-1.58
Assigned Value	78.29	Average SDI	-1.16
SDPA	14.091	Uncertainty of AV	0.63
Standard Unit Result Val	56.00	%DEV	-41.09

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

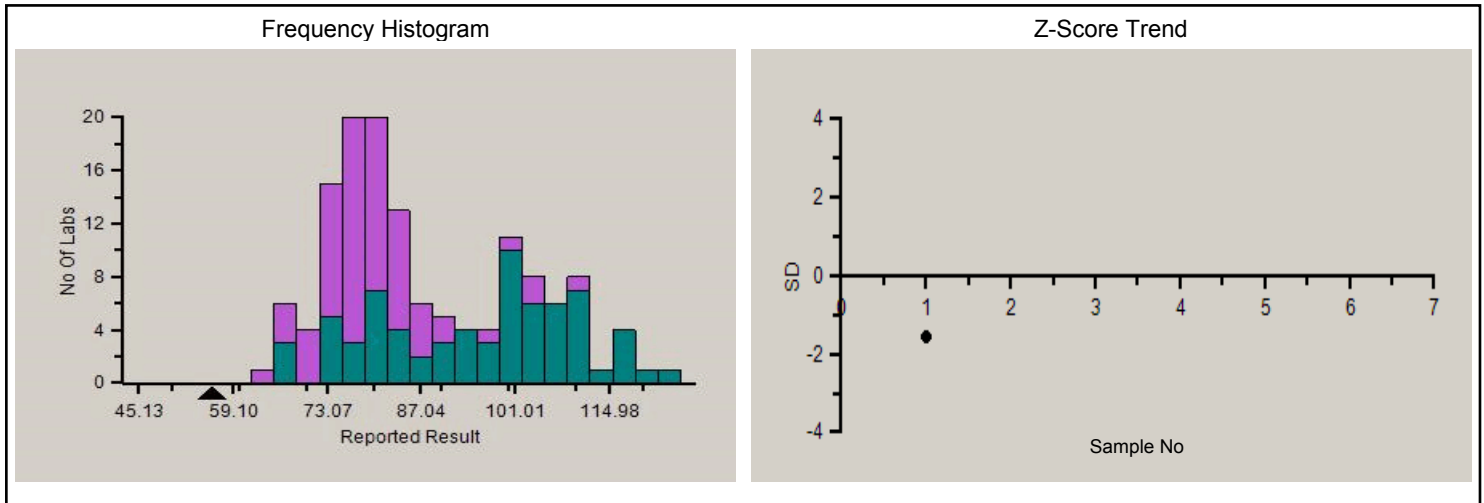

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, ALP		N	Mean	SD	CV%	Excluded
	All Analyzer	167	87.20	13.87	15.91	18
Your Analyzer :	RANDOX RX daytona	1	--	--	--	1
	Fuji Dri-Chem NX500/i	33	106.25	7.85	7.39	1
	Roche cobas c 311	28	78.32	3.62	4.62	--
	Fuji Dri-Chem 4000i	16	102.13	7.54	7.38	1
	Roche cobas c 111	11	76.60	6.07	7.92	--
	Horiba ABX Pentra C200	10	77.41	7.49	9.68	1
	Roche cobas INTEGRA	10	78.53	2.52	3.21	--
	Roche cobas 6000	8	79.38	4.31	5.43	--
	Erba EM 200	6	78.73	10.70	13.60	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, ALT, U/L

	N	Mean	SD	CV%	Excluded
All Methods	168	29.17	29.26	100.33	61
IFCC - UV without P5P	18	13.47	1.89	14.02	8
RANDOX RX daytona	1	--	--	--	--

Your Result	13.00	SDI / z-Score	0.18
Assigned Value	12.56	Average SDI	0.65
SDPA	2.510	Uncertainty of AV	0.21
Standard Unit Result Val	13.00	%DEV	-3.50

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

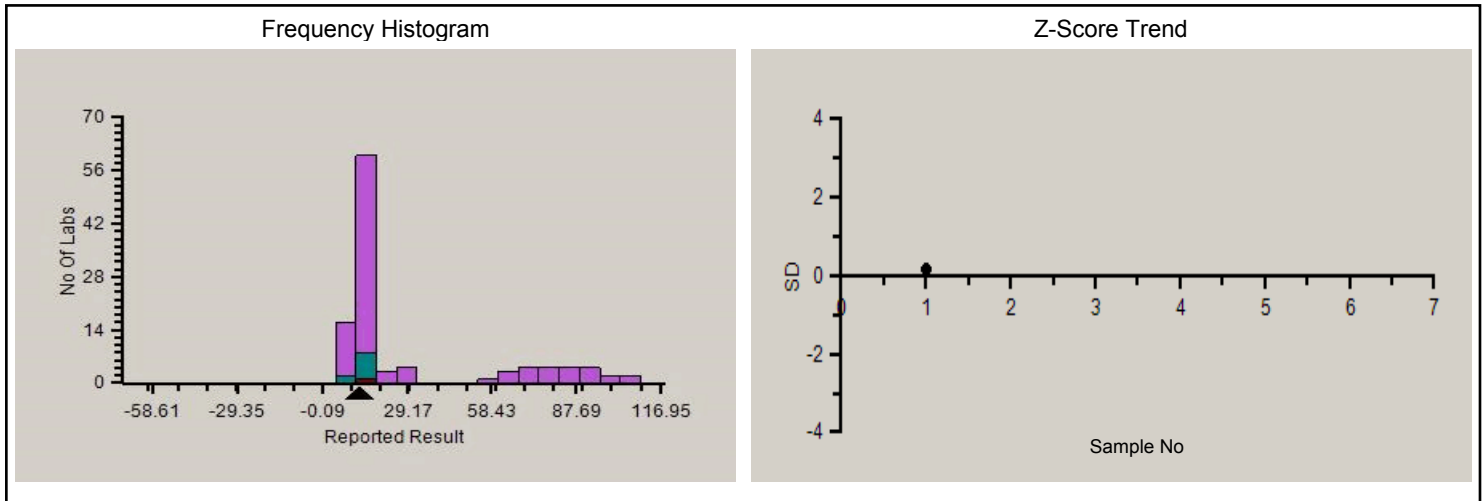

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, ALT		N	Mean	SD	CV%	Excluded
	All Analyzer	168	29.17	29.26	100.33	61
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	30	87.00	12.62	14.51	18
	Roche cobas c 311	28	13.02	1.36	10.46	6
	Fuji Dri-Chem 4000i	16	76.40	14.14	18.50	6
	Horiba ABX Pentra C200	11	12.64	1.59	12.60	--
	Roche cobas c 111	11	13.25	1.65	12.42	1
	Roche cobas INTEGRA	10	11.46	1.39	12.14	--
	Roche cobas 6000	8	12.51	1.41	11.27	--
	Erba EM 200	7	19.73	3.20	16.22	3

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Amylase, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	100	60.30	6.95	11.52	8
■ G7 PNP	66	60.12	6.81	11.33	--
■ RANDOX RX daytona	1	--	--	--	--

Your Result	74.00	SDI / z-Score	1.35
Assigned Value	66.36	Average SDI	1.04
SDPA	5.639	Uncertainty of AV	0.56
Standard Unit Result Val	74.00	%DEV	23.09

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

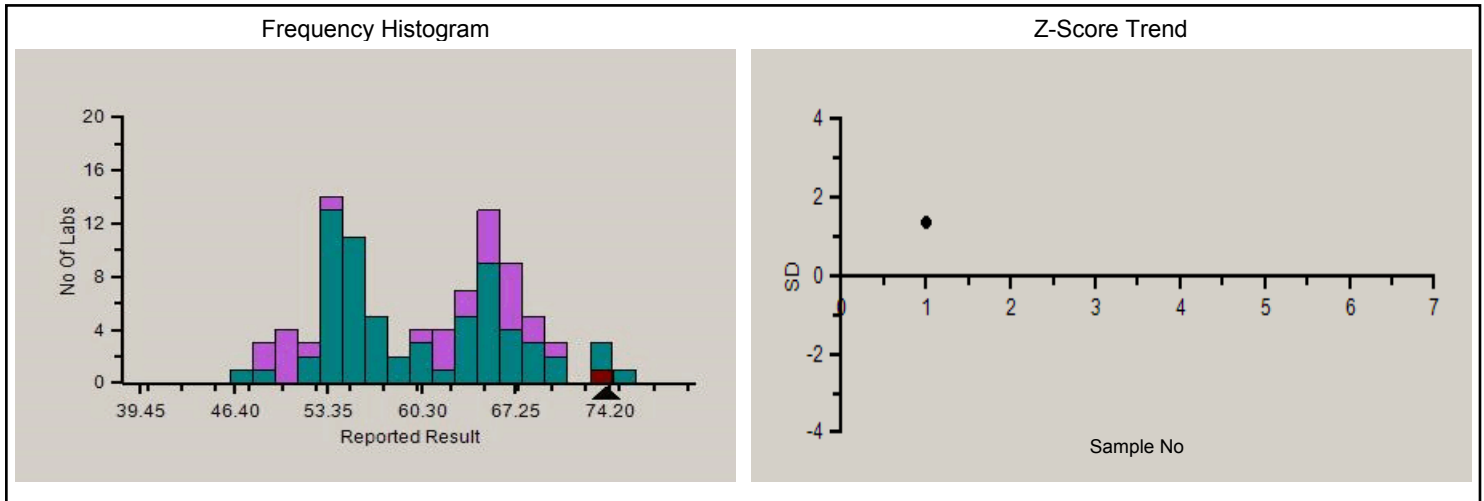

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Amylase		N	Mean	SD	CV%	Excluded
	All Analyzer	100	60.30	6.95	11.52	8
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	23	55.61	3.58	6.43	--
	Roche cobas c 311	15	66.72	3.00	4.49	--
	Fuji Dri-Chem 4000i	14	54.64	1.74	3.18	--
	Roche cobas INTEGRA	7	65.35	3.08	4.72	--
	Roche cobas 6000	6	66.22	1.83	2.77	--
	Roche cobas 8000	4	67.25	2.22	3.30	--
	Roche cobas c 111	3	69.10	5.67	8.20	--
	Star 20	3	62.50	0.00	0.00	2

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, AST, U/L

	N	Mean	SD	CV%	Excluded
All Methods	167	27.28	11.26	41.27	63
IFCC - UV without P5P	16	26.75	11.58	43.29	5
RANDOX RX daytona	1	--	--	--	--

Your Result	17.00	SDI / z-Score	-0.69
Assigned Value	19.73	Average SDI	-0.24
SDPA	3.945	Uncertainty of AV	0.35
Standard Unit Result Val	17.00	%DEV	-36.45

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

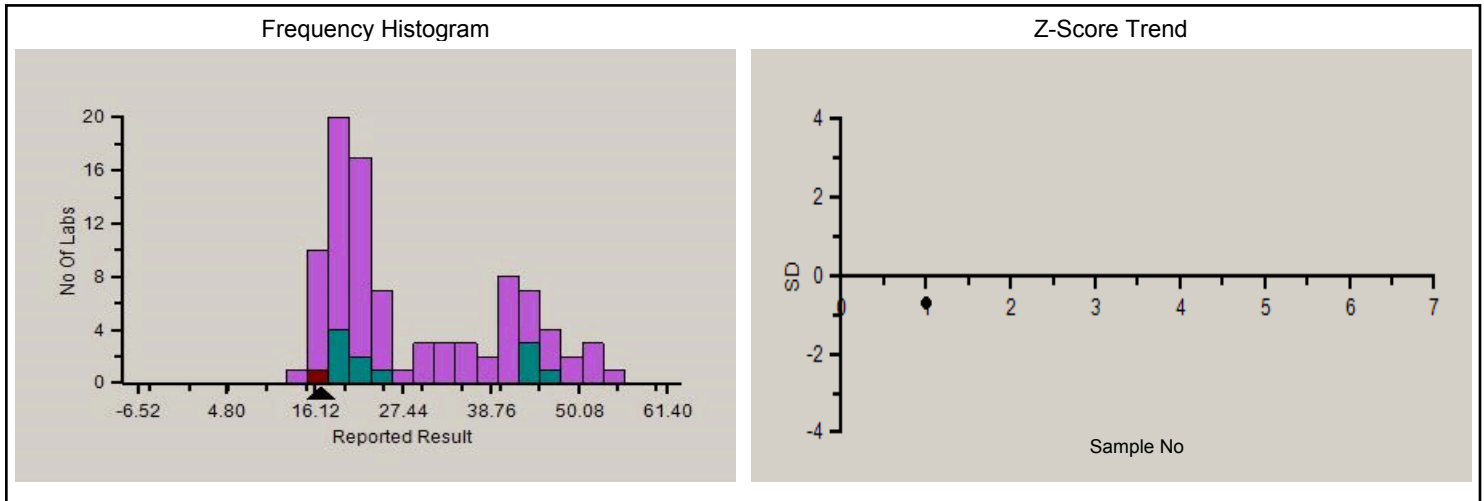

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, AST		N	Mean	SD	CV%	Excluded
	All Analyzer	167	27.28	11.26	41.27	63
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	31	42.36	7.61	17.95	20
	Roche cobas c 311	27	20.46	2.41	11.77	5
	Fuji Dri-Chem 4000i	16	45.89	6.86	14.96	7
	Roche cobas c 111	12	21.67	2.88	13.28	5
	Horiba ABX Pentra C200	10	18.60	0.95	5.13	1
	Roche cobas INTEGRA	10	17.58	1.54	8.74	1
	Roche cobas 6000	8	20.63	2.12	10.27	--
	Erba EM 200	7	41.00	7.95	19.38	3

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Bilirubin Direct, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	166	0.10	0.02	17.00	51
■ DMSO	1	--	--	--	1
■ RANDOX RX daytona	1	--	--	--	1

Your Result	0.19	SDI / z-Score	2.19
Assigned Value	0.10	Average SDI	0.99
SDPA	0.043	Uncertainty of AV	0.01
Standard Unit Result Val	0.19	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

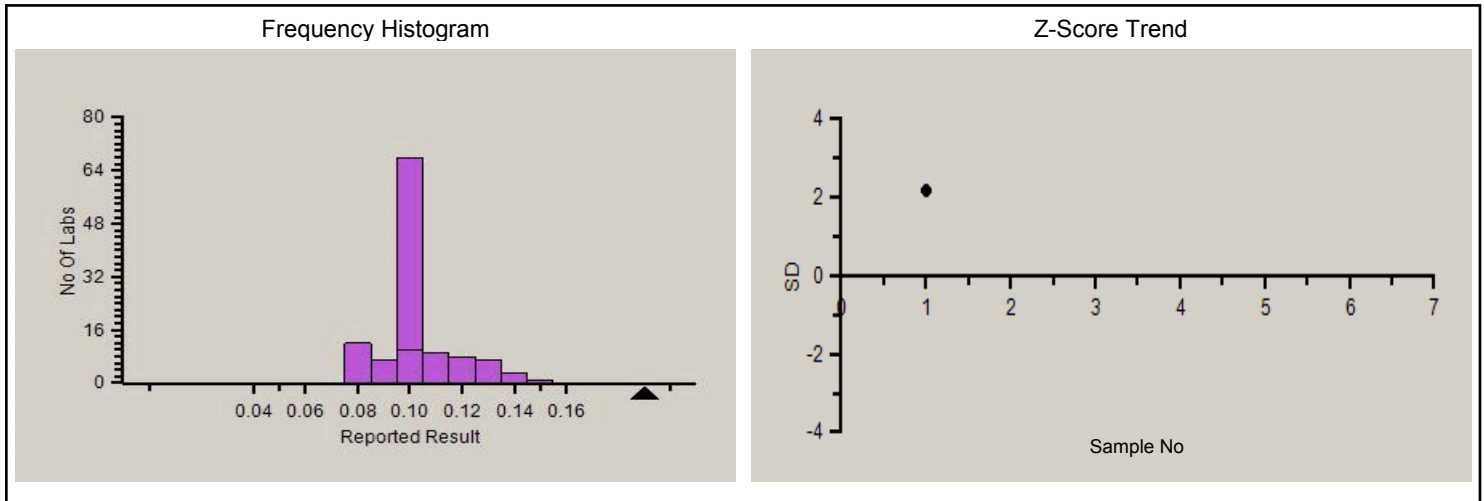

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Bilirubin Direct		N	Mean	SD	CV%	Excluded
	All Analyzer	166	0.10	0.02	17.00	51
Your Analyzer :	RANDOX RX daytona	1	--	--	--	1
	Fuji Dri-Chem NX500/i	28	0.10	0.01	8.08	9
	Roche cobas c 311	27	0.09	0.02	19.15	5
	Fuji Dri-Chem 4000i	16	0.10	0.00	0.00	9
	Horiba ABX Pentra C200	11	0.12	0.02	13.91	--
	Roche cobas c 111	11	0.11	0.01	11.01	4
	Roche cobas INTEGRA	10	0.10	0.01	13.54	--
	Erba EM 200	8	0.12	0.04	34.43	2
	Roche cobas 6000	8	0.10	0.01	9.38	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Bilirubin Total, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	170	0.31	0.14	45.05	49
DMSO	1	--	--	--	1
RANDOX RX daytona	1	--	--	--	1

Your Result	0.56	SDI / z-Score	2.56
Assigned Value	0.32	Average SDI	1.97
SDPA	0.095	Uncertainty of AV	0.02
Standard Unit Result Val	0.56	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

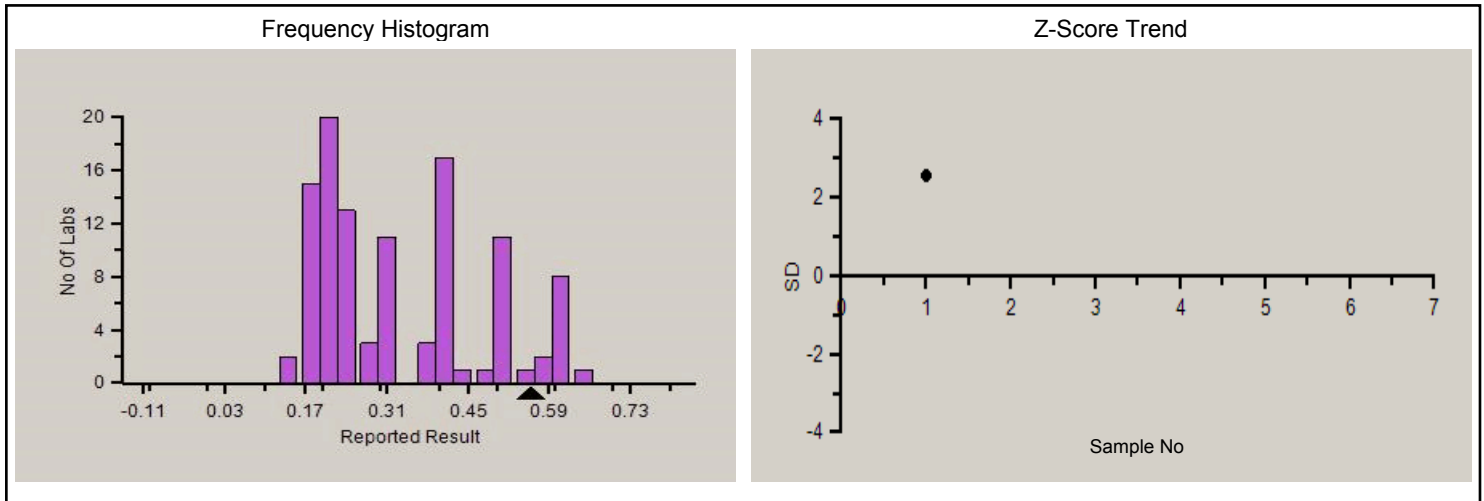

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Bilirubin Total		N	Mean	SD	CV%	Excluded
	All Analyzer	170	0.31	0.14	45.05	49
Your Analyzer :	RANDOX RX daytona	1	--	--	--	1
	Fuji Dri-Chem NX500/i	30	0.47	0.08	16.24	6
	Roche cobas c 311	28	0.20	0.03	14.50	6
	Fuji Dri-Chem 4000i	16	0.51	0.08	16.37	2
	Horiba ABX Pentra C200	11	0.22	0.03	11.26	6
	Roche cobas c 111	10	0.20	0.03	15.76	4
	Roche cobas INTEGRA	10	0.20	0.02	8.08	1
	Erba EM 200	8	0.22	0.03	14.93	1
	Roche cobas 6000	8	0.19	0.02	10.83	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Calcium, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	157	7.64	0.53	6.92	11
Arsenazo III	53	7.85	0.47	6.00	7
RANDOX RX daytona	1	--	--	--	--

Your Result	8.00	SDI / z-Score	-0.19
Assigned Value	8.15	Average SDI	-0.29
SDPA	0.806	Uncertainty of AV	0.41
Standard Unit Result Val	8.00	%DEV	1.91

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

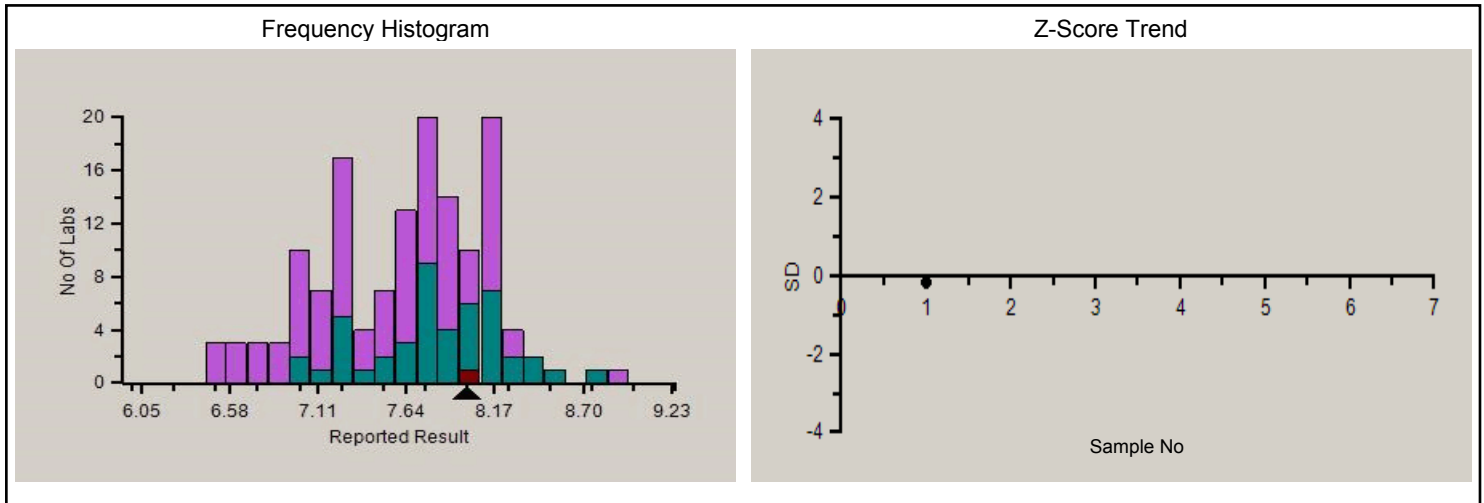

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Calcium		N	Mean	SD	CV%	Excluded
	All Analyzer	157	7.64	0.53	6.92	11
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	28	7.00	0.31	4.43	--
	Roche cobas c 311	25	7.92	0.25	3.18	1
	Fuji Dri-Chem 4000i	16	7.26	0.35	4.80	--
	Roche cobas INTEGRA	11	7.76	0.31	3.99	--
	Roche cobas c 111	10	7.83	0.26	3.27	1
	Roche cobas 6000	7	7.81	0.15	1.97	--
	Erba EM 200	6	8.43	0.62	7.31	--
	Beckman Coulter AU480	5	7.88	0.20	2.51	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Chloride, mEq/L

	N	Mean	SD	CV%	Excluded
■ All Methods	140	105.52	12.39	11.74	15
■ ISE direct	95	0.00	0.00	0.00	9
■ EasyLyte	8	0.00	0.00	0.00	1

Your Result	109.60	SDI / z-Score	-0.54
Assigned Value	113.62	Average SDI	-0.53
SDPA	7.385	Uncertainty of AV	0.47
Standard Unit Result Val	109.60	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

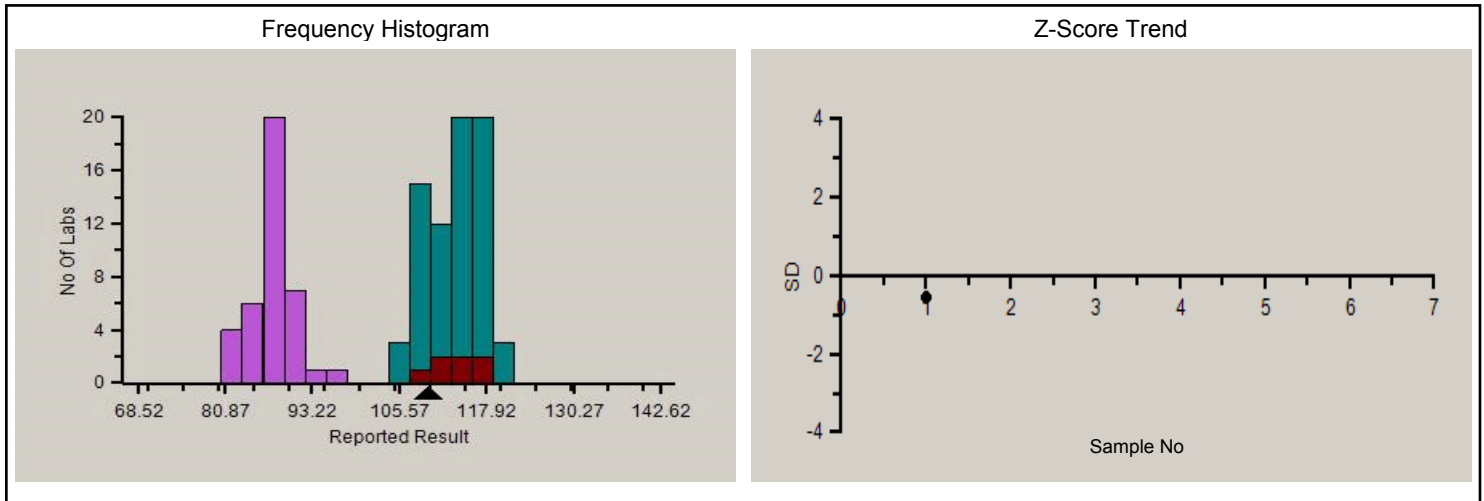

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Chloride		N	Mean	SD	CV%	Excluded
	All Analyzer	140	105.52	12.39	11.74	15
Your Analyzer :	EasyLyte	8	0.00	0.00	0.00	1
	Fuji Dri-Chem NX500/i	32	0.00	0.00	0.00	1
	Fuji Dri-Chem 4000i	17	0.00	0.00	0.00	1
	Roche cobas c 311	16	0.00	0.00	0.00	--
	Roche AVL 9180	11	110.17	1.91	1.74	--
	Roche AVL 9180	10	0.00	0.00	0.00	--
	Roche cobas 6000	8	0.00	0.00	0.00	1
	Roche cobas 8000	4	0.00	0.00	0.00	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, CK, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	76	80.59	15.40	19.11	8
■ Colorimetric	1	--	--	--	--
■ Fuji Nx 700	3	70.67	1.16	1.63	--

Your Result	72.00	SDI / z-Score	0.66
Assigned Value	66.28	Average SDI	0.05
SDPA	8.616	Uncertainty of AV	1.81
Standard Unit Result Val	72.00	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

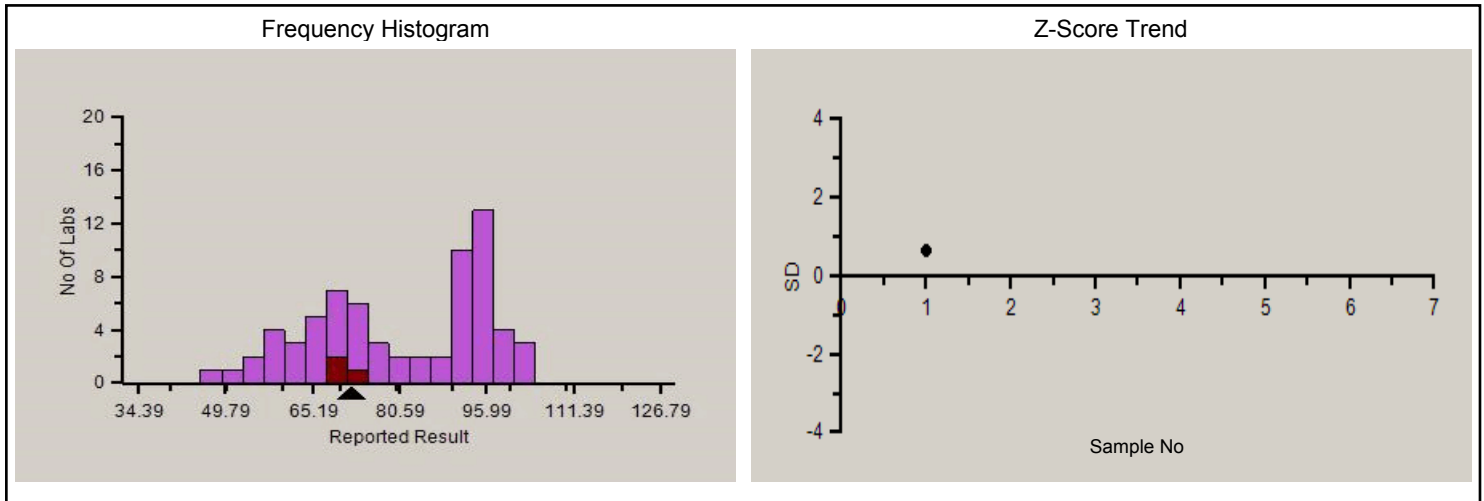

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, CK		N	Mean	SD	CV%	Excluded
	All Analyzer	76	80.59	15.40	19.11	8
Your Analyzer :	Fuji Nx 700	3	70.67	1.16	1.63	--
	Fuji Dri-Chem NX500/i	21	66.12	8.97	13.57	4
	Roche cobas c 311	13	94.52	4.02	4.26	--
	Fuji Dri-Chem 4000i	11	66.00	5.04	7.64	--
	Roche cobas INTEGRA	7	93.04	6.31	6.78	--
	Roche cobas 6000	5	92.20	2.95	3.20	--
	Roche cobas 8000	4	95.25	1.71	1.79	--
	Star 20	2	--	--	--	2

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, GGT, U/L

	N	Mean	SD	CV%	Excluded
All Methods	135	15.80	3.87	24.49	11
IFCC	12	16.84	3.85	22.88	--
RANDOX RX daytona	1	--	--	--	--

Your Result	21.00	SDI / z-Score	0.94
Assigned Value	18.40	Average SDI	0.88
SDPA	2.760	Uncertainty of AV	0.27
Standard Unit Result Val	21.00	%DEV	24.69

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

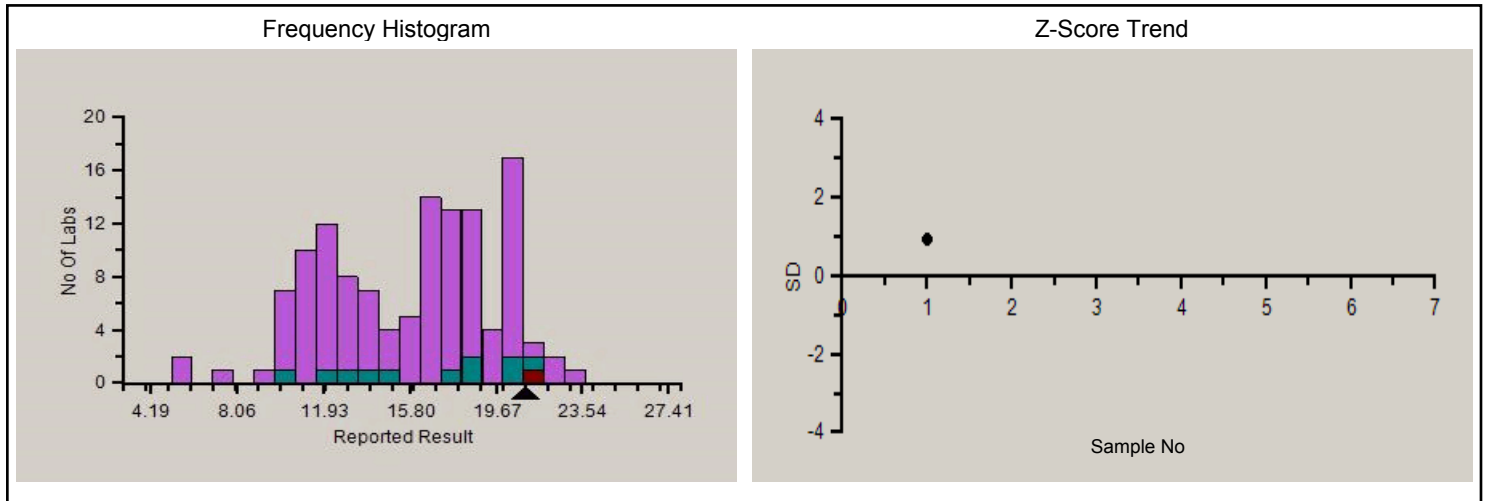

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, GGT		N	Mean	SD	CV%	Excluded
	All Analyzer	135	15.80	3.87	24.49	11
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	32	12.03	1.19	9.88	2
	Roche cobas c 311	24	19.00	1.23	6.50	2
	Fuji Dri-Chem 4000i	12	11.33	1.50	13.21	--
	Roche cobas INTEGRA	11	16.87	1.42	8.43	--
	Roche cobas c 111	10	16.97	1.39	8.18	1
	Horiba ABX Pentra C200	6	18.40	2.30	12.47	--
	Roche cobas 6000	6	18.33	1.51	8.22	--
	Beckman Coulter AU480	5	19.08	1.42	7.43	1

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, LDH, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	93	145.36	59.94	41.23	14
■ L to P - IFCC Ref. Proc., Calibrated	3	121.67	33.50	27.54	--
■ Fuji Nx 700	3	109.00	5.29	4.86	--

Your Result	107.00	SDI / z-Score	0.33
Assigned Value	102.59	Average SDI	-0.67
SDPA	13.360	Uncertainty of AV	1.85
Standard Unit Result Val	107.00	%DEV	-12.06

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

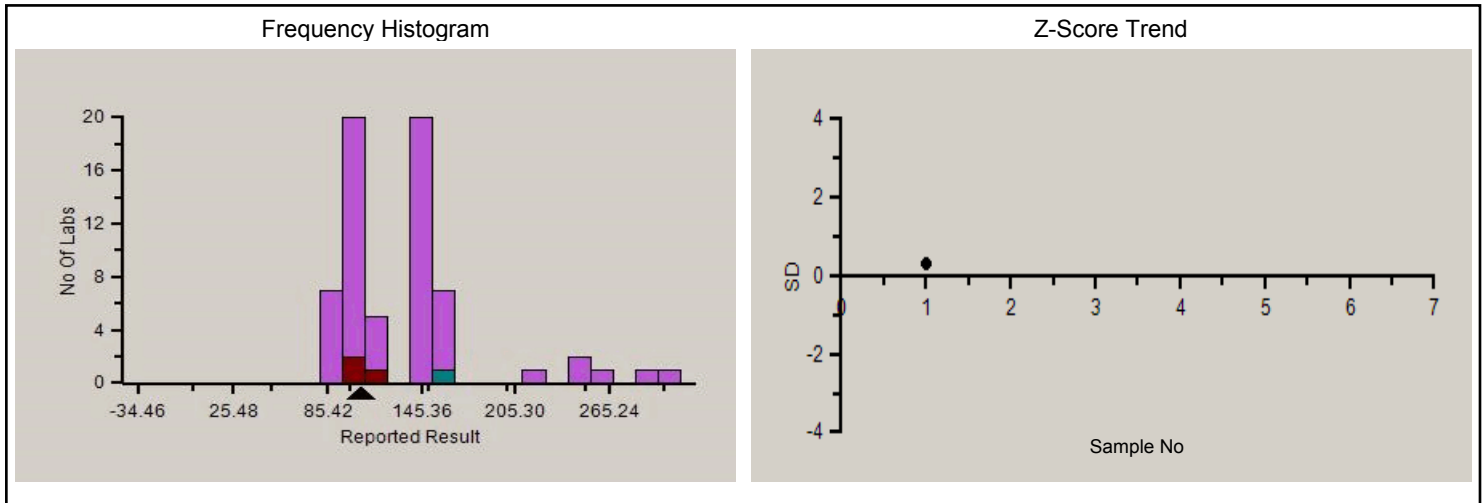

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Biochemistry, LDH		N	Mean	SD	CV%	Excluded
	All Analyzer	93	145.36	59.94	41.23	14
Your Analyzer :	Fuji Nx 700	3	109.00	5.29	4.86	--
	Fuji Dri-Chem NX500/i	25	100.00	8.03	8.03	6
	Fuji Dri-Chem 4000i	12	104.67	9.06	8.66	--
	Roche cobas c 311	11	149.91	5.11	3.41	--
	Roche cobas INTEGRA	7	146.55	2.93	2.00	--
	Roche cobas 6000	6	150.17	5.08	3.38	--
	Beckman Coulter AU480	4	197.00	0.00	0.00	2
	Roche cobas 8000	4	146.75	2.22	1.51	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Lipase, U/L

	N	Mean	SD	CV%	Excluded
All Methods	81	48.90	16.91	34.57	9
Enzymatic colorimetric	14	41.82	14.72	35.21	3
Fuji Nx 700	3	56.67	5.13	9.06	--

Your Result	58.00	SDI / z-Score	-0.25
Assigned Value	59.49	Average SDI	-0.41
SDPA	5.966	Uncertainty of AV	0.80
Standard Unit Result Val	58.00	%DEV	38.71

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

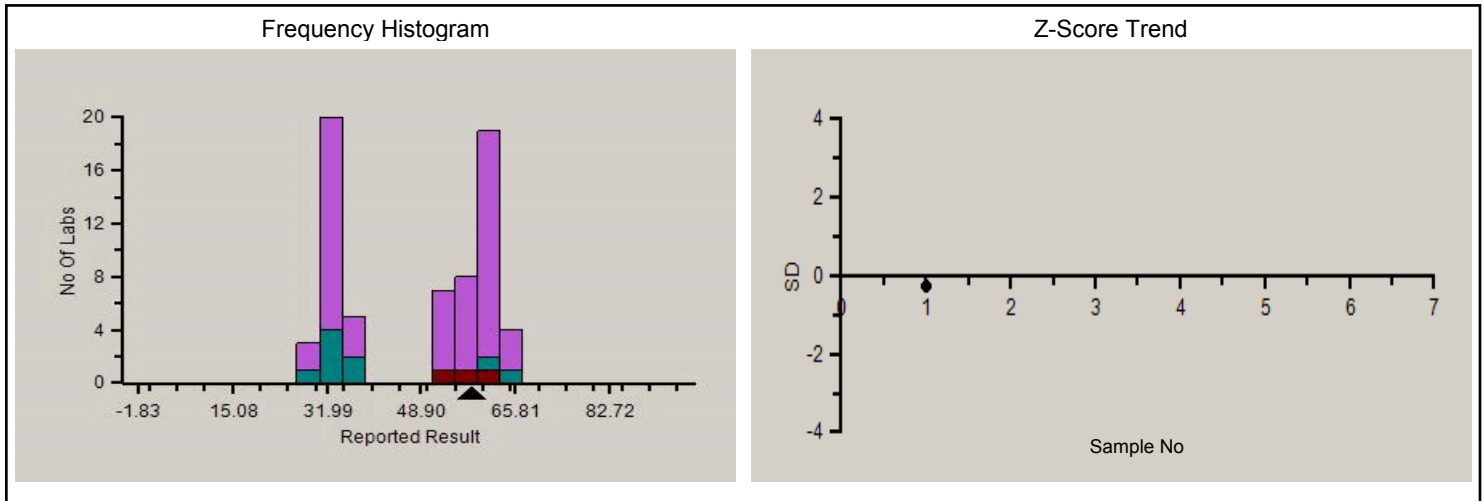

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Lipase		N	Mean	SD	CV%	Excluded
	All Analyzer	81	48.90	16.91	34.57	9
Your Analyzer :	Fuji Nx 700	3	56.67	5.13	9.06	--
	Fuji Dri-Chem NX500/i	22	59.81	4.08	6.83	1
	Fuji Dri-Chem 4000i	14	59.29	3.47	5.86	--
	Roche cobas c 311	12	33.62	1.74	5.16	2
	Roche cobas INTEGRA	6	33.04	2.43	7.36	--
	Roche cobas 6000	5	32.14	1.49	4.65	--
	Roche cobas 8000	3	31.92	3.05	9.55	--
	Star 20	3	69.00	0.00	0.00	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Magnesium, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	55	1.06	0.66	61.79	6
Enzymatic	2	0.50	--	--	1
Fuji Nx 700	2	0.50	--	--	--

Your Result	0.50	SDI / z-Score	0.00
Assigned Value	0.50	Average SDI	-0.15
SDPA	0.065	Uncertainty of AV	0.01
Standard Unit Result Val	0.50	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

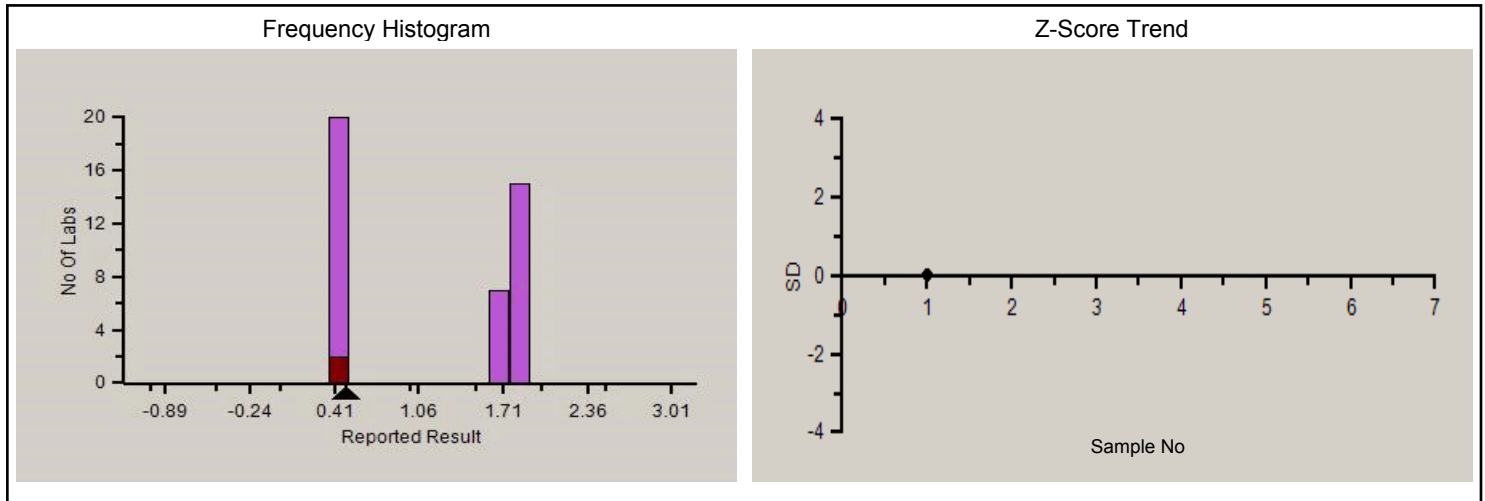

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Magnesium		N	Mean	SD	CV%	Excluded
	All Analyzer	55	1.06	0.66	61.79	6
Your Analyzer :	Fuji Nx 700	2	0.50	--	--	--
	Fuji Dri-Chem NX500/i	17	0.47	0.04	8.16	2
	Fuji Dri-Chem 4000i	10	0.49	0.03	6.53	--
	Roche cobas c 311	7	1.75	0.07	4.18	--
	Roche cobas 6000	6	1.77	0.05	2.83	--
	Roche cobas 8000	4	1.83	0.05	2.96	--
	Roche cobas INTEGRA	2	1.73	--	--	1
	Beckman Coulter AU5800	1	--	--	--	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Potassium, mEq/L

	N	Mean	SD	CV%	Excluded
■ All Methods	151	5.75	0.93	16.17	12
■ ISE direct	105	0.00	0.00	0.00	4
■ EasyLyte	9	0.00	0.00	0.00	--

Your Result	5.71	SDI / z-Score	-1.91
Assigned Value	6.31	Average SDI	-1.85
SDPA	0.316	Uncertainty of AV	0.04
Standard Unit Result Val	5.71	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

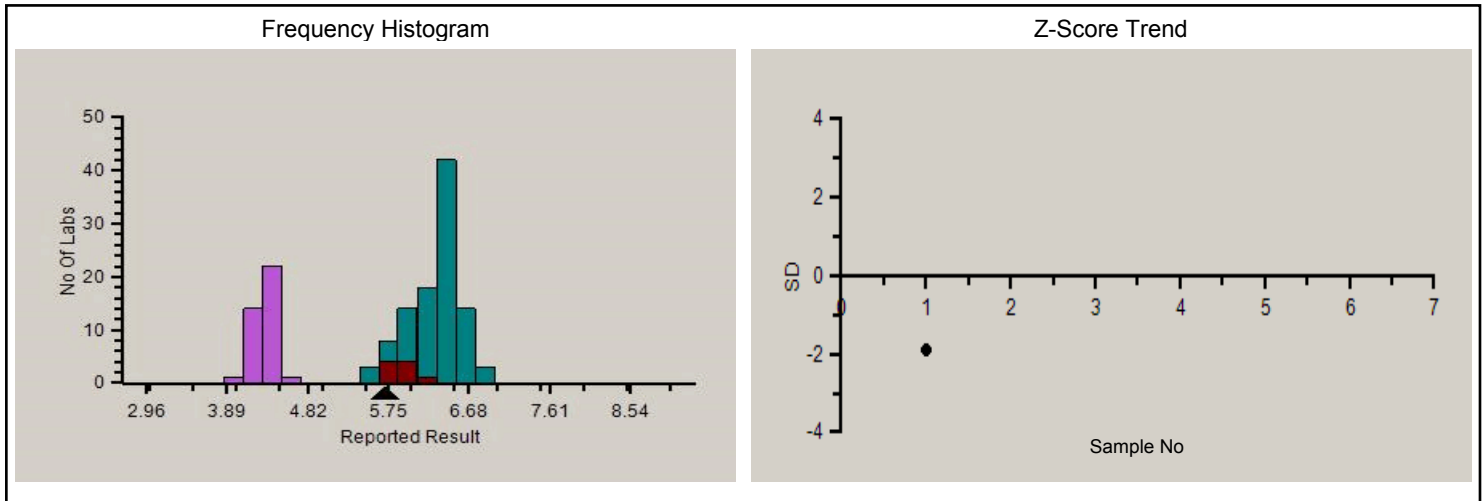

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Potassium		N	Mean	SD	CV%	Excluded
	All Analyzer	151	5.75	0.93	16.17	12
Your Analyzer :	EasyLyte	9	0.00	0.00	0.00	--
	Fuji Dri-Chem NX500/i	33	0.00	0.00	0.00	1
	Fuji Dri-Chem 4000i	19	0.00	0.00	0.00	1
	Roche cobas c 311	16	0.00	0.00	0.00	--
	Roche AVL 9180	13	6.33	0.43	6.81	--
	Roche AVL 9180	12	0.00	0.00	0.00	--
	Roche cobas 6000	8	0.00	0.00	0.00	--
	Sensa Core	5	0.00	0.00	0.00	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Sodium, mEq/L

	N	Mean	SD	CV%	Excluded
All Methods	151	159.57	23.46	14.70	18
ISE direct	105	0.00	0.00	0.00	11
EasyLyte	9	0.00	0.00	0.00	2

Your Result	169.40	SDI / z-Score	-0.58
Assigned Value	174.48	Average SDI	-0.57
SDPA	8.723	Uncertainty of AV	0.48
Standard Unit Result Val	169.40	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

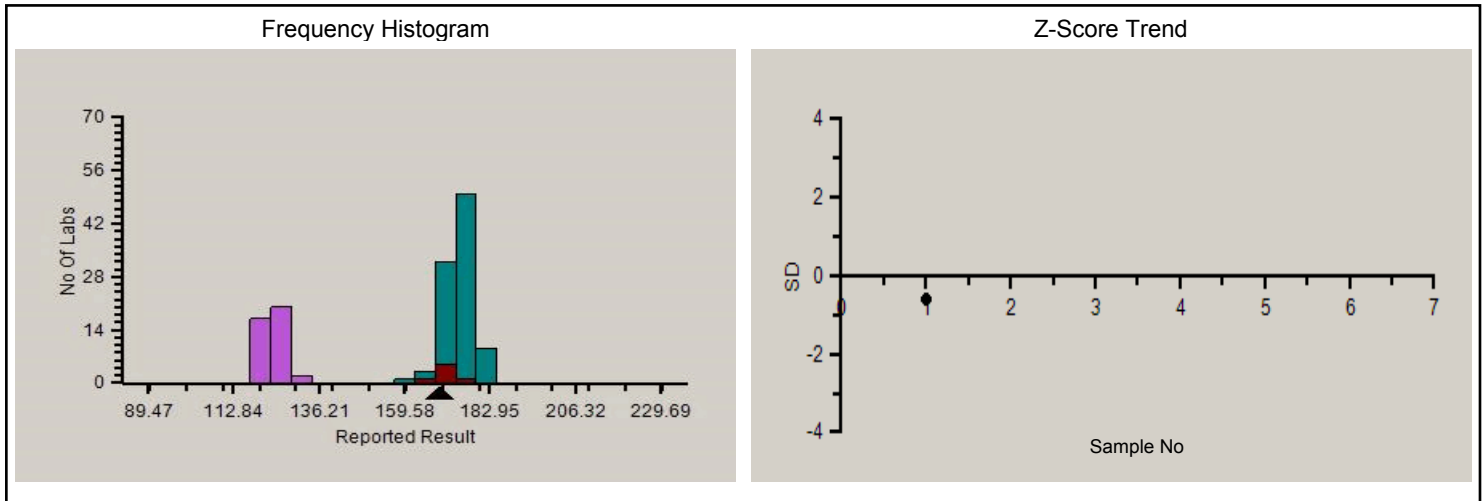

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Sodium		N	Mean	SD	CV%	Excluded
	All Analyzer	151	159.57	23.46	14.70	18
Your Analyzer :	EasyLyte	9	0.00	0.00	0.00	2
	Fuji Dri-Chem NX500/i	34	0.00	0.00	0.00	3
	Fuji Dri-Chem 4000i	18	0.00	0.00	0.00	3
	Roche cobas c 311	16	0.00	0.00	0.00	--
	Roche AVL 9180	13	175.22	5.44	3.11	--
	Roche AVL 9180	12	0.00	0.00	0.00	--
	Roche cobas 6000	8	0.00	0.00	0.00	--
	Sensa Core	5	0.00	0.00	0.00	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Total Protein, g/dL

	N	Mean	SD	CV%	Excluded
■ All Methods	166	6.47	0.32	4.96	3
■ Biuret	163	6.47	0.32	5.00	3
■ RANDOX RX daytona	1	--	--	--	--

Your Result	6.30	SDI / z-Score	-0.29
Assigned Value	6.38	Average SDI	-0.36
SDPA	0.283	Uncertainty of AV	0.03
Standard Unit Result Val	6.30	%DEV	-2.58

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

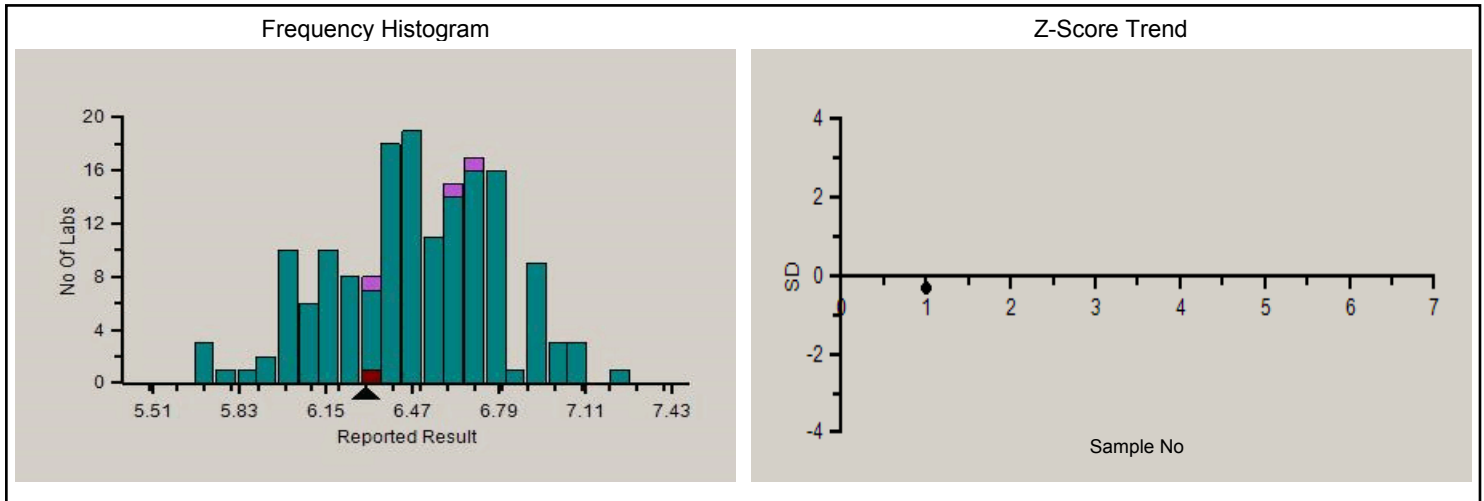

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Total Protein		N	Mean	SD	CV%	Excluded
	All Analyzer	166	6.47	0.32	4.96	3
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	30	6.73	0.17	2.53	--
	Roche cobas c 311	28	6.47	0.21	3.23	--
	Fuji Dri-Chem 4000i	16	6.77	0.15	2.20	--
	Roche cobas c 111	11	6.40	0.33	5.10	--
	Roche cobas INTEGRA	10	6.10	0.24	3.87	--
	Horiba ABX Pentra C200	9	6.42	0.17	2.60	--
	Erba EM 200	8	6.53	0.41	6.34	1
	Roche cobas 6000	8	6.46	0.17	2.59	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Triglycerides, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	166	121.71	8.69	7.14	8
GPO-PAP	15	124.65	10.76	8.63	--
RANDOX RX daytona	1	--	--	--	--

Your Result	128.00	SDI / z-Score	0.16
Assigned Value	125.53	Average SDI	0.41
SDPA	15.189	Uncertainty of AV	0.73
Standard Unit Result Val	128.00	%DEV	2.69

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

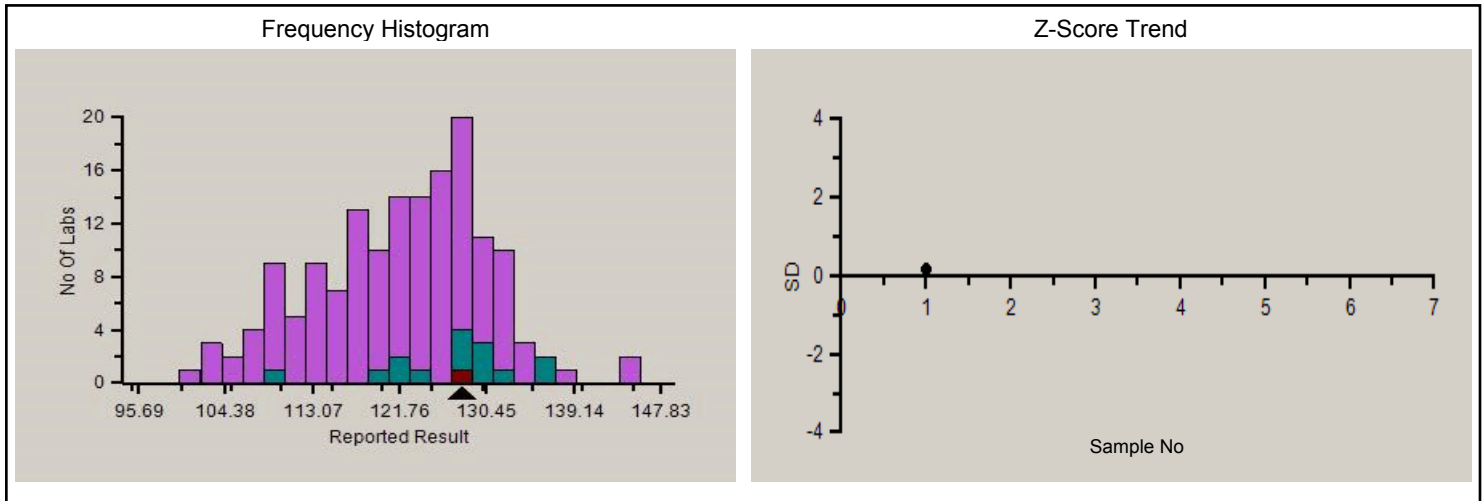

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Triglycerides		N	Mean	SD	CV%	Excluded
	All Analyzer	166	121.71	8.69	7.14	8
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	32	114.44	6.40	5.59	1
	Roche cobas c 311	28	127.01	5.98	4.71	--
	Fuji Dri-Chem 4000i	16	114.19	7.31	6.40	--
	Roche cobas c 111	11	128.25	4.39	3.43	--
	Horiba ABX Pentra C200	10	124.53	4.32	3.47	--
	Roche cobas INTEGRA	10	122.87	4.59	3.73	--
	Roche cobas 6000	8	126.29	1.50	1.19	1
	Erba EM 200	6	121.70	9.86	8.10	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Uric Acid, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	168	4.18	0.35	8.30	10
Uricase	25	4.09	0.39	9.56	5
RANDOX RX daytona	1	--	--	--	1

Your Result	3.30	SDI / z-Score	-2.12
Assigned Value	3.96	Average SDI	-1.92
SDPA	0.313	Uncertainty of AV	0.02
Standard Unit Result Val	3.30	%DEV	-19.32

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

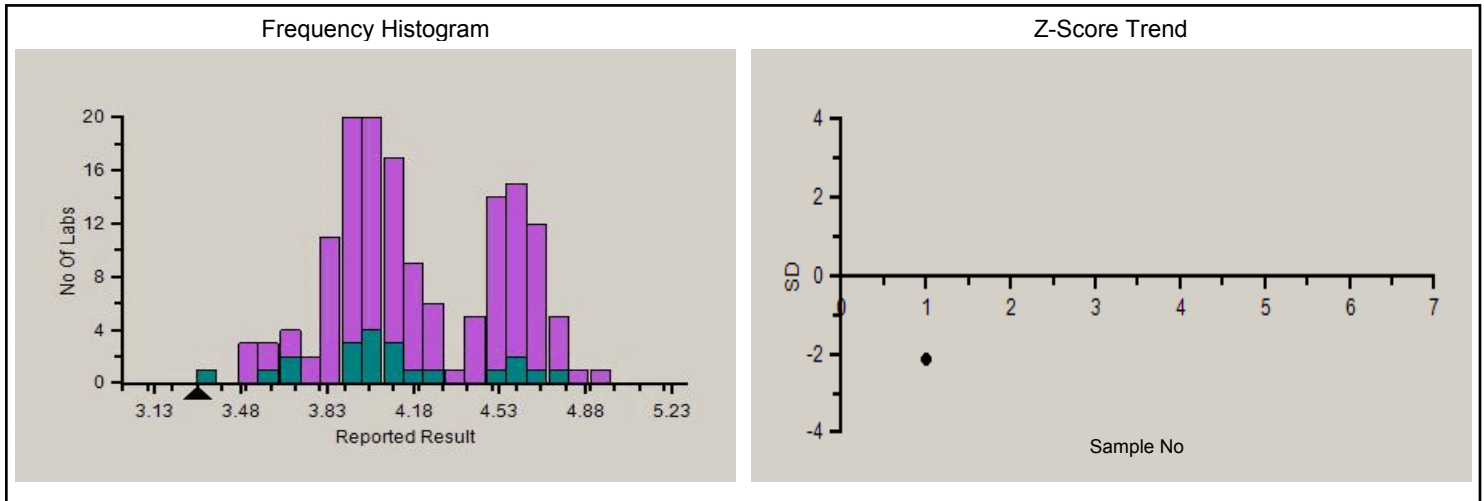

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Biochemistry, Uric Acid		N	Mean	SD	CV%	Excluded
	All Analyzer	168	4.18	0.35	8.30	10
Your Analyzer :	RANDOX RX daytona	1	--	--	--	1
	Fuji Dri-Chem NX500/i	31	4.52	0.20	4.33	1
	Roche cobas c 311	26	3.95	0.17	4.35	1
	Fuji Dri-Chem 4000i	19	4.59	0.20	4.45	1
	Roche cobas c 111	11	4.00	0.17	4.12	--
	Horiba ABX Pentra C200	10	3.96	0.09	2.35	1
	Roche cobas INTEGRA	10	3.97	0.13	3.30	--
	Roche cobas 6000	8	3.94	0.07	1.88	--
	Erba EM 200	6	4.50	0.30	6.64	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
Unit No. 409-416.
Commercial Building - 1A,
Kohinoor Mall, Kirol Road, Kuria (W),
Mumbai - 400070



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021


Biochemistry, Albumin, g/dL

	N	Mean	SD	CV%	Excluded
All Methods	166	3.97	0.46	11.62	6
Bromcresol Green (BCG)	158	3.97	0.46	11.50	5
RANDOX RX daytona	1	--	--	--	--

Your Result	3.60	SDI / z-Score	-0.42
Assigned Value	3.69	Average SDI	-0.43
SDPA	0.213	Uncertainty of AV	0.02
Standard Unit Result Val	3.60	%DEV	-9.41

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

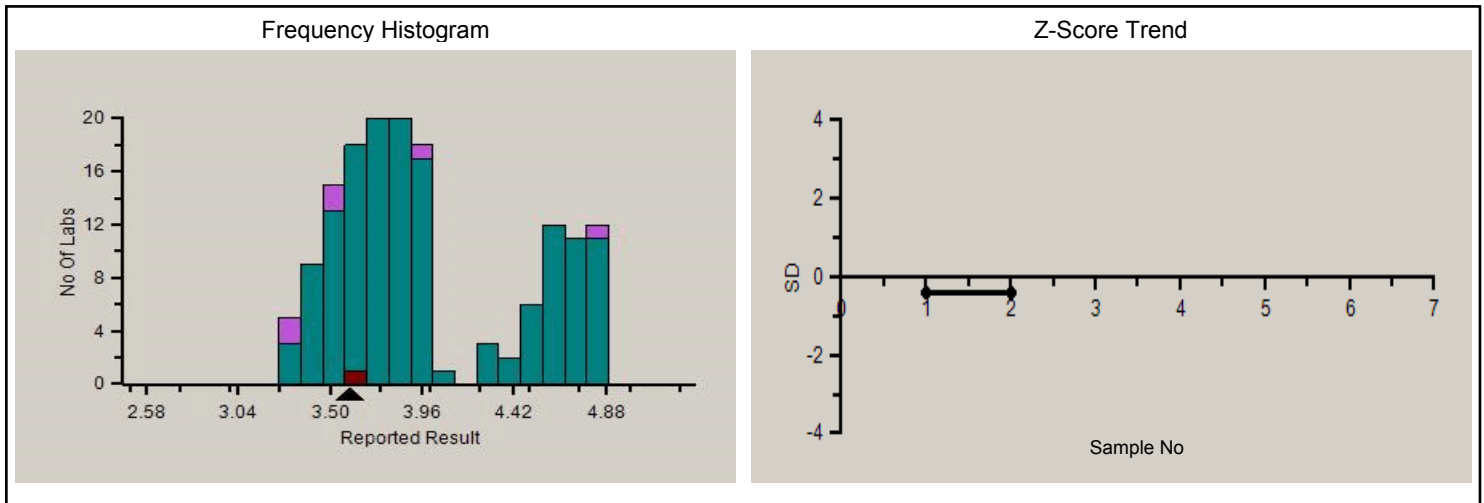

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, Albumin		N	Mean	SD	CV%	Excluded
	All Analyzer	166	3.97	0.46	11.62	6
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	31	4.64	0.14	2.99	--
	Roche cobas c 311	27	3.79	0.11	2.98	--
	Fuji Dri-Chem 4000i	16	4.62	0.16	3.49	1
	Horiba ABX Pentra C200	10	3.51	0.11	3.02	1
	Roche cobas c 111	10	3.87	0.06	1.42	--
	Roche cobas INTEGRA	10	3.76	0.11	2.88	--
	Erba EM 200	8	3.55	0.09	2.45	--
	Roche cobas 6000	8	3.80	0.18	4.60	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, ALP, U/L

	N	Mean	SD	CV%	Excluded
All Methods	165	87.51	15.30	17.48	18
PNPP, AMP Buffer	77	95.81	16.01	16.71	7
RANDOX RX daytona	1	--	--	--	1

Your Result	54.00	SDI / z-Score	-1.68
Assigned Value	77.44	Average SDI	-1.16
SDPA	13.927	Uncertainty of AV	0.61
Standard Unit Result Val	54.00	%DEV	-43.64

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

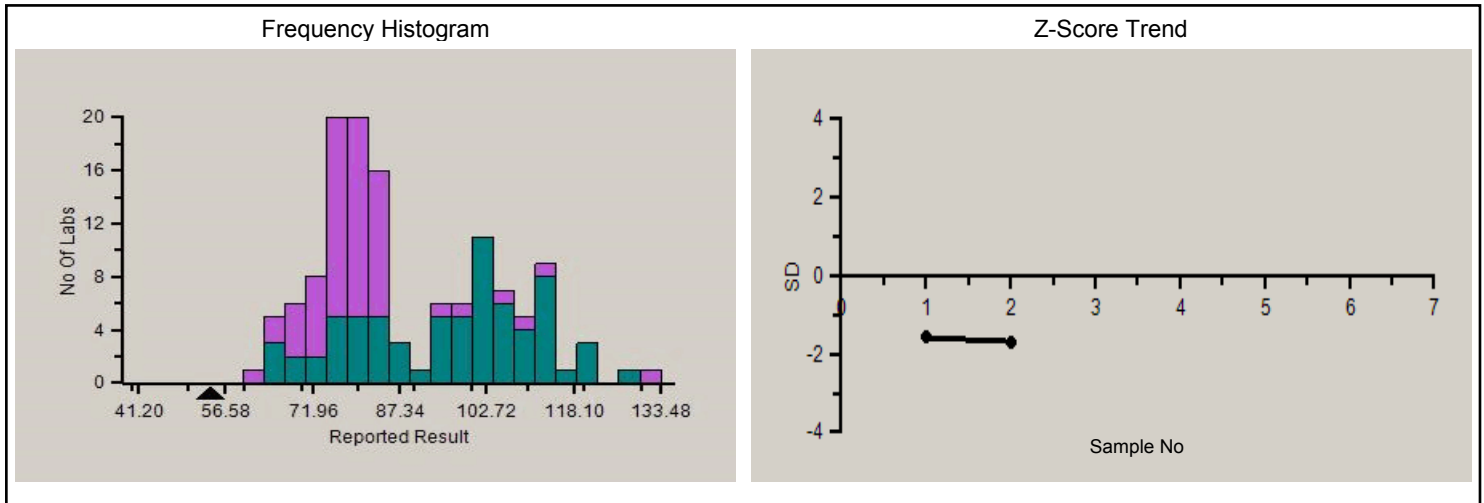

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, ALP		N	Mean	SD	CV%	Excluded
	All Analyzer	165	87.51	15.30	17.48	18
Your Analyzer :	RANDOX RX daytona	1	--	--	--	1
	Fuji Dri-Chem NX500/i	33	108.33	9.10	8.40	--
	Roche cobas c 311	27	77.38	3.66	4.73	--
	Fuji Dri-Chem 4000i	16	104.20	7.87	7.55	1
	Roche cobas c 111	11	75.16	6.85	9.11	--
	Horiba ABX Pentra C200	10	74.69	7.75	10.38	1
	Roche cobas INTEGRA	10	78.48	3.04	3.87	--
	Roche cobas 6000	8	78.38	3.38	4.31	--
	Erba EM 200	6	76.28	9.37	12.28	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, ALT, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	170	14.49	5.73	39.56	35
■ IFCC - UV without P5P	16	11.56	1.26	10.89	6
■ RANDOX RX daytona	1	--	--	--	--

Your Result	11.00	SDI / z-Score	0.10
Assigned Value	10.77	Average SDI	0.65
SDPA	2.261	Uncertainty of AV	0.16
Standard Unit Result Val	11.00	%DEV	-4.84

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

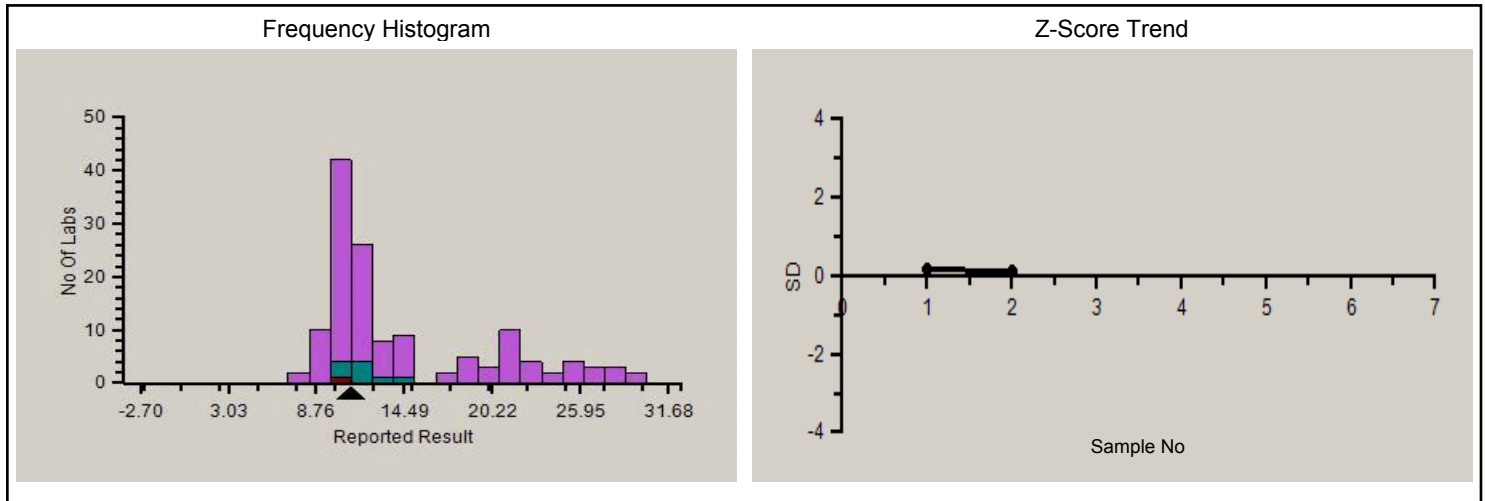

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, ALT		N	Mean	SD	CV%	Excluded
	All Analyzer	170	14.49	5.73	39.56	35
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	32	23.11	3.35	14.49	11
	Roche cobas c 311	27	10.81	1.27	11.77	1
	Fuji Dri-Chem 4000i	16	23.36	2.50	10.71	5
	Horiba ABX Pentra C200	11	11.23	1.29	11.50	1
	Roche cobas c 111	11	10.09	1.24	12.30	2
	Roche cobas INTEGRA	10	10.00	0.92	9.15	1
	Erba EM 200	8	13.41	1.77	13.16	1
	Roche cobas 6000	8	10.74	0.70	6.55	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, Amylase, U/L

	N	Mean	SD	CV%	Excluded
All Methods	99	60.37	7.20	11.93	10
G7 PNP	66	60.94	6.20	10.17	3
RANDOX RX daytona	1	--	--	--	--

Your Result	73.00	SDI / z-Score	0.76
Assigned Value	67.35	Average SDI	1.04
SDPA	7.408	Uncertainty of AV	0.41
Standard Unit Result Val	73.00	%DEV	19.78

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

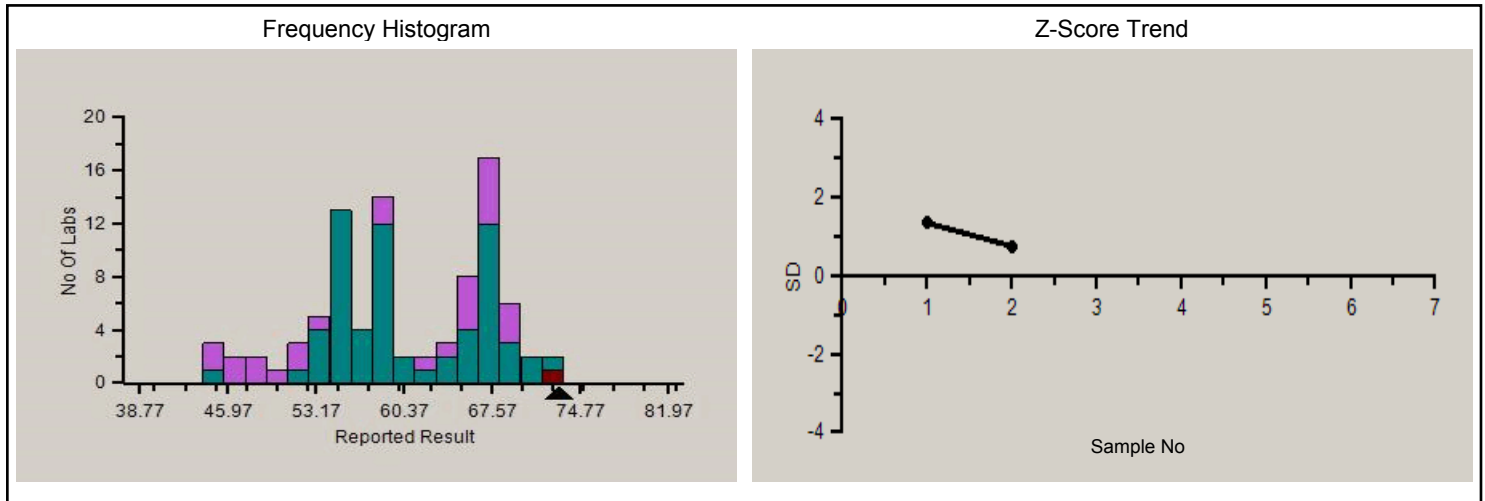

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, Amylase		N	Mean	SD	CV%	Excluded
	All Analyzer	99	60.37	7.20	11.93	10
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	23	57.00	2.56	4.49	--
	Fuji Dri-Chem 4000i	14	56.43	1.91	3.39	--
	Roche cobas c 311	14	67.64	2.26	3.35	--
	Roche cobas INTEGRA	7	66.98	2.53	3.77	--
	Roche cobas 6000	6	67.18	1.46	2.17	--
	Roche cobas 8000	4	67.75	0.96	1.41	--
	Roche cobas c 111	3	66.90	2.97	4.44	1
	Star 20	3	--	--	--	3

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, AST, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	167	19.79	2.98	15.05	22
■ IFCC - UV without P5P	14	18.60	1.39	7.47	5
■ RANDOX RX daytona	1	--	--	--	--

Your Result	18.00	SDI / z-Score	0.03
Assigned Value	17.88	Average SDI	-0.24
SDPA	3.576	Uncertainty of AV	0.22
Standard Unit Result Val	18.00	%DEV	-3.20

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

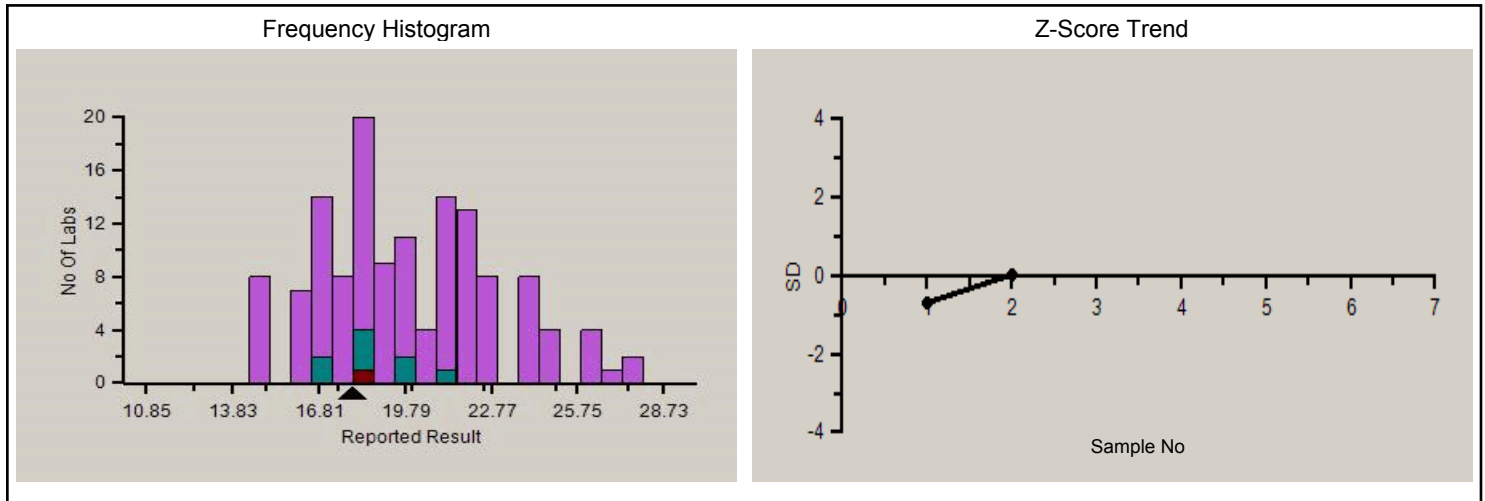

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, AST		N	Mean	SD	CV%	Excluded
	All Analyzer	167	19.79	2.98	15.05	22
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	32	23.35	2.33	9.99	6
	Roche cobas c 311	26	17.90	1.41	7.87	--
	Fuji Dri-Chem 4000i	16	22.19	2.14	9.63	--
	Roche cobas c 111	12	17.81	1.64	9.18	1
	Horiba ABX Pentra C200	10	18.07	1.63	9.01	--
	Roche cobas INTEGRA	10	16.50	1.09	6.57	1
	Erba EM 200	8	19.33	2.97	15.35	4
	Roche cobas 6000	8	17.30	0.78	4.50	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, Bilirubin Direct, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	164	0.10	0.02	15.53	39
■ DMSO	1	--	--	--	1
■ RANDOX RX daytona	1	--	--	--	1

Your Result	0.19	SDI / z-Score	2.09
Assigned Value	0.10	Average SDI	0.99
SDPA	0.044	Uncertainty of AV	0.01
Standard Unit Result Val	0.19	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

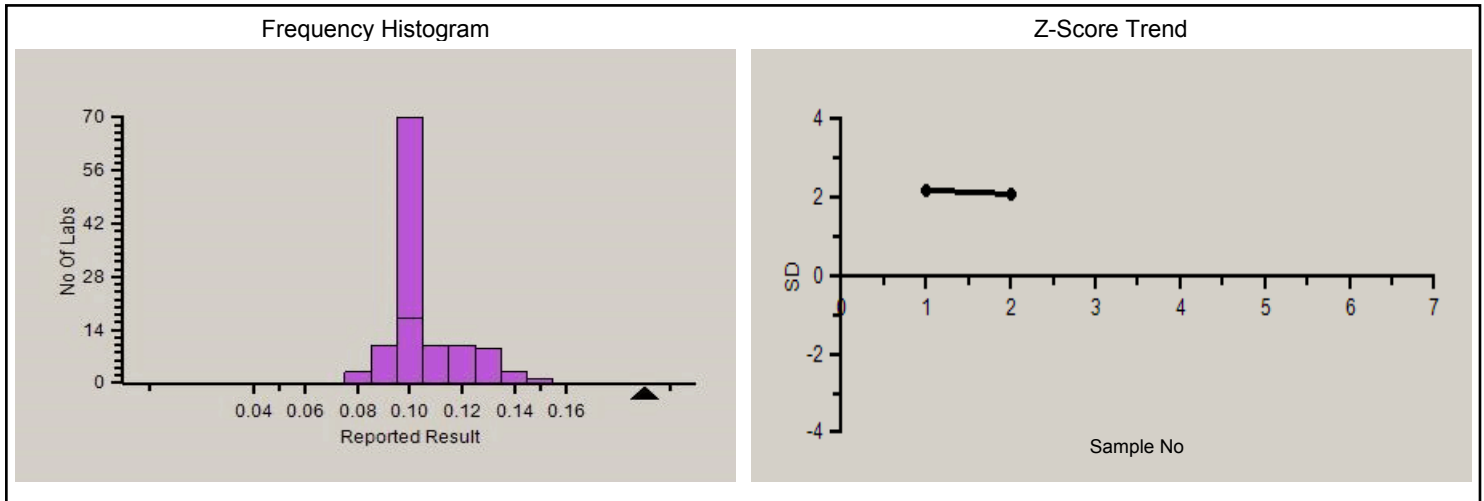

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, Bilirubin Direct		N	Mean	SD	CV%	Excluded
	All Analyzer	164	0.10	0.02	15.53	39
Your Analyzer :	RANDOX RX daytona	1	--	--	--	1
	Fuji Dri-Chem NX500/i	28	0.10	0.00	4.04	8
	Roche cobas c 311	26	0.09	0.01	13.19	3
	Fuji Dri-Chem 4000i	16	0.10	0.00	0.00	6
	Horiba ABX Pentra C200	11	0.12	0.01	10.17	--
	Roche cobas c 111	11	0.11	0.01	12.73	3
	Roche cobas INTEGRA	10	0.10	0.01	7.00	--
	Erba EM 200	8	0.13	0.03	25.56	2
	Roche cobas 6000	8	0.10	0.01	8.42	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, Bilirubin Total, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	167	0.33	0.14	42.81	43
DMSO	1	--	--	--	1
RANDOX RX daytona	1	--	--	--	1

Your Result	0.57	SDI / z-Score	2.42
Assigned Value	0.33	Average SDI	1.97
SDPA	0.099	Uncertainty of AV	0.02
Standard Unit Result Val	0.57	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

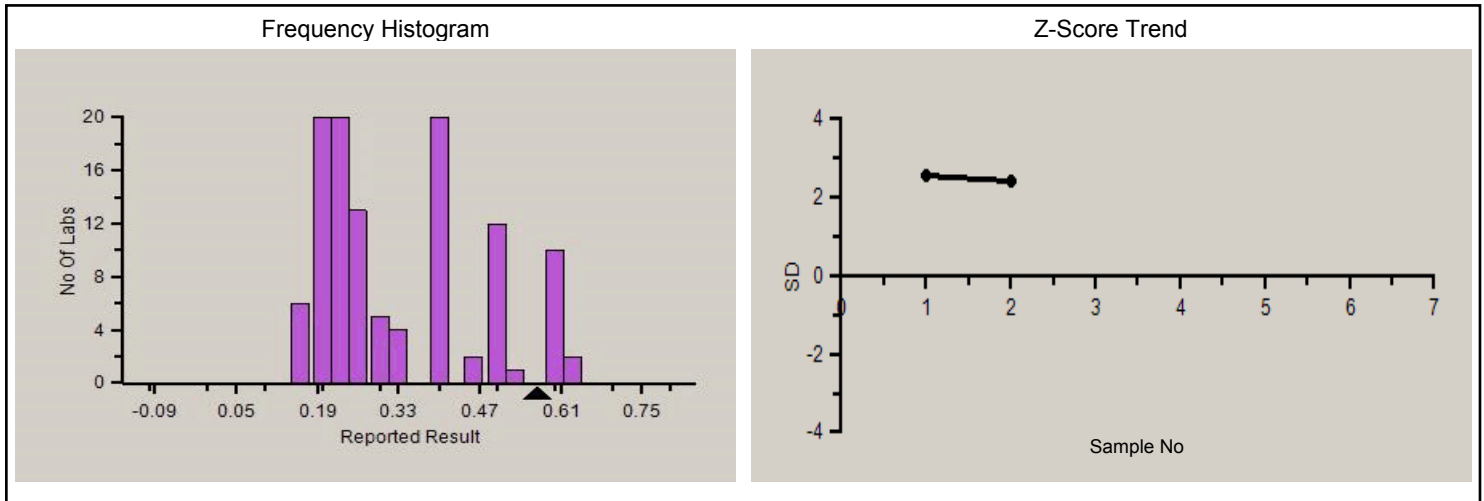

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, Bilirubin Total		N	Mean	SD	CV%	Excluded
	All Analyzer	167	0.33	0.14	42.81	43
Your Analyzer :	RANDOX RX daytona	1	--	--	--	1
	Fuji Dri-Chem NX500/i	30	0.49	0.08	17.11	7
	Roche cobas c 311	26	0.21	0.03	13.53	3
	Fuji Dri-Chem 4000i	16	0.51	0.09	17.36	1
	Horiba ABX Pentra C200	11	0.24	0.02	9.92	6
	Roche cobas c 111	10	0.22	0.04	20.47	4
	Roche cobas INTEGRA	10	0.20	0.02	9.55	1
	Erba EM 200	8	0.24	0.04	16.88	1
	Roche cobas 6000	8	0.19	0.02	12.37	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, Calcium, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	156	7.58	0.57	7.57	8
Arsenazo III	53	7.84	0.49	6.23	5
RANDOX RX daytona	1	--	--	--	--

Your Result	8.00	SDI / z-Score	-0.23
Assigned Value	8.20	Average SDI	-0.29
SDPA	0.887	Uncertainty of AV	0.45
Standard Unit Result Val	8.00	%DEV	2.07

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

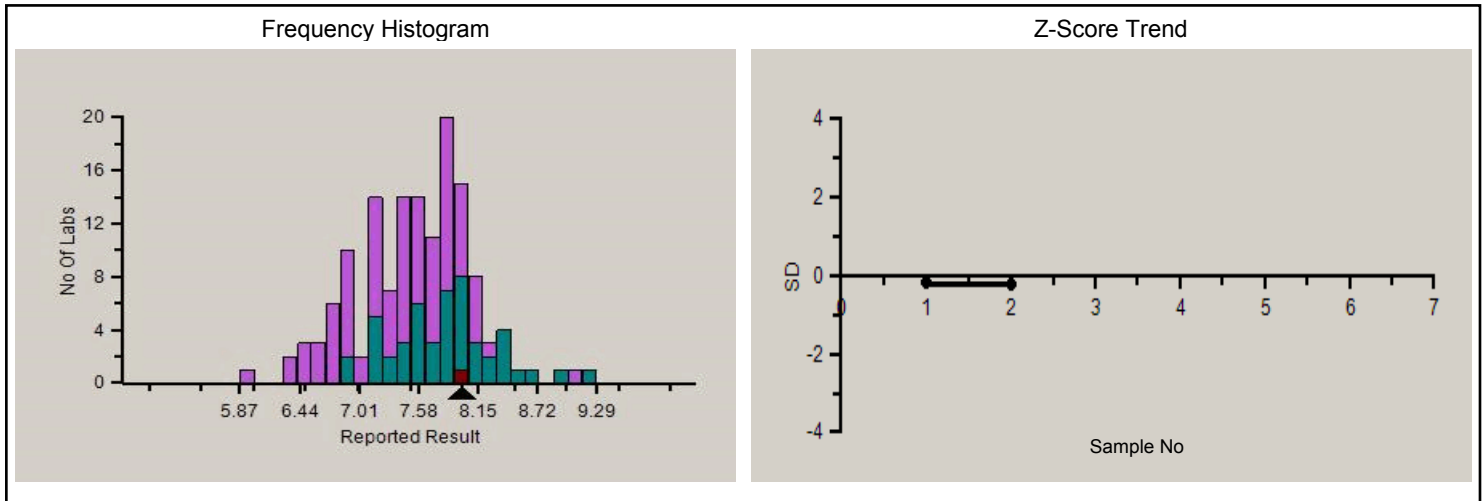

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, Calcium		N	Mean	SD	CV%	Excluded
	All Analyzer	156	7.58	0.57	7.57	8
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	28	6.90	0.32	4.61	--
	Roche cobas c 311	24	7.86	0.22	2.81	--
	Fuji Dri-Chem 4000i	16	7.06	0.48	6.73	--
	Roche cobas INTEGRA	11	7.75	0.28	3.67	--
	Roche cobas c 111	10	7.75	0.21	2.67	--
	Roche cobas 6000	7	7.76	0.14	1.84	1
	Erba EM 200	6	8.43	0.60	7.13	--
	Beckman Coulter AU480	5	7.89	0.19	2.36	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, Chloride, mEq/L

	N	Mean	SD	CV%	Excluded
■ All Methods	138	105.29	12.55	11.92	15
■ ISE direct	94	0.00	0.00	0.00	8
■ EasyLyte	8	0.00	0.00	0.00	1

Your Result	109.50	SDI / z-Score	-0.51
Assigned Value	113.22	Average SDI	-0.53
SDPA	7.350	Uncertainty of AV	0.48
Standard Unit Result Val	109.50	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

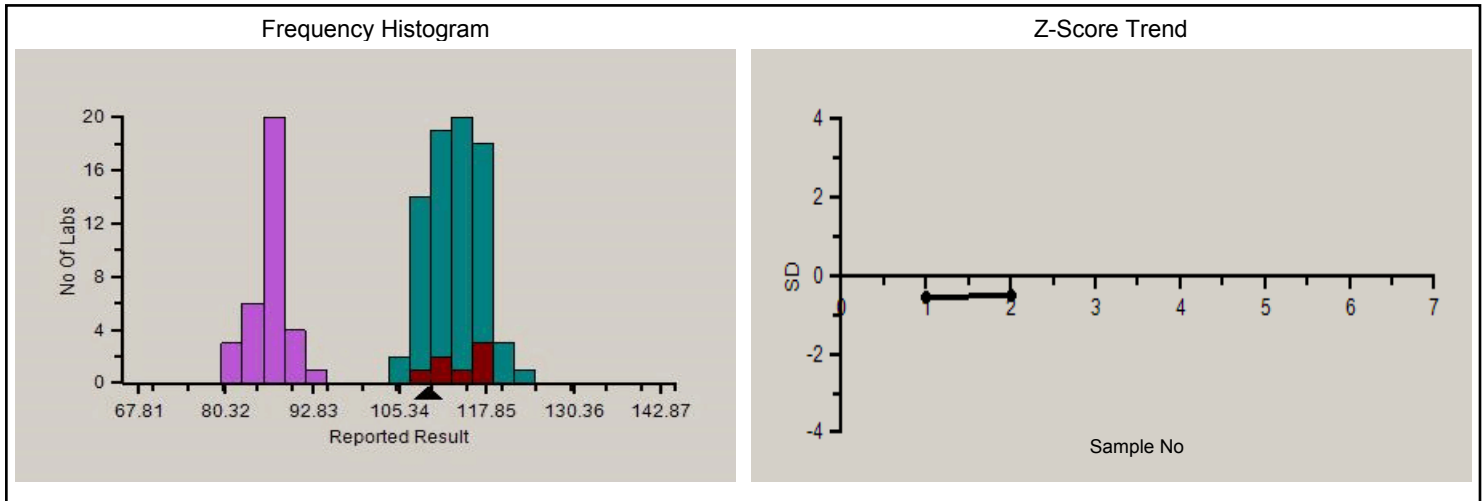

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, Chloride		N	Mean	SD	CV%	Excluded
	All Analyzer	138	105.29	12.55	11.92	15
Your Analyzer :	EasyLyte	8	0.00	0.00	0.00	1
	Fuji Dri-Chem NX500/i	32	0.00	0.00	0.00	1
	Fuji Dri-Chem 4000i	17	0.00	0.00	0.00	1
	Roche cobas c 311	15	0.00	0.00	0.00	--
	Roche AVL 9180	11	108.93	1.85	1.70	--
	Roche AVL 9180	10	0.00	0.00	0.00	--
	Roche cobas 6000	8	0.00	0.00	0.00	1
	Roche cobas 8000	4	0.00	0.00	0.00	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, CK, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	76	85.17	15.66	18.39	5
■ Colorimetric	1	--	--	--	--
■ Fuji Nx 700	3	75.33	2.52	3.34	--

Your Result	78.00	SDI / z-Score	0.75
Assigned Value	71.26	Average SDI	0.05
SDPA	8.998	Uncertainty of AV	1.90
Standard Unit Result Val	78.00	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

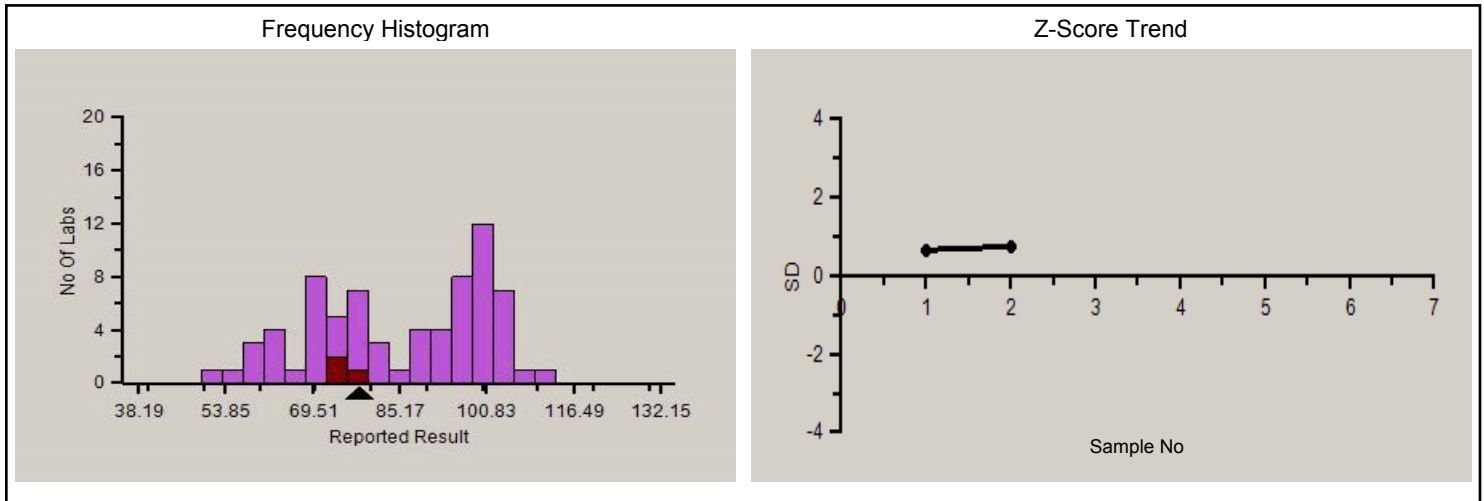

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, CK		N	Mean	SD	CV%	Excluded
	All Analyzer	76	85.17	15.66	18.39	5
Your Analyzer :	Fuji Nx 700	3	75.33	2.52	3.34	--
	Fuji Dri-Chem NX500/i	21	70.55	10.45	14.81	1
	Roche cobas c 311	13	99.33	3.90	3.93	--
	Fuji Dri-Chem 4000i	11	71.73	6.75	9.42	--
	Roche cobas INTEGRA	7	97.87	6.63	6.77	--
	Roche cobas 6000	5	96.82	2.29	2.37	--
	Roche cobas 8000	4	99.75	2.75	2.76	--
	Star 20	2	--	--	--	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, GGT, U/L

	N	Mean	SD	CV%	Excluded
All Methods	135	15.19	4.08	26.87	7
IFCC	12	15.74	3.82	24.27	--
RANDOX RX daytona	1	--	--	--	--

Your Result	20.00	SDI / z-Score	1.17
Assigned Value	17.54	Average SDI	0.88
SDPA	2.104	Uncertainty of AV	0.24
Standard Unit Result Val	20.00	%DEV	27.05

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

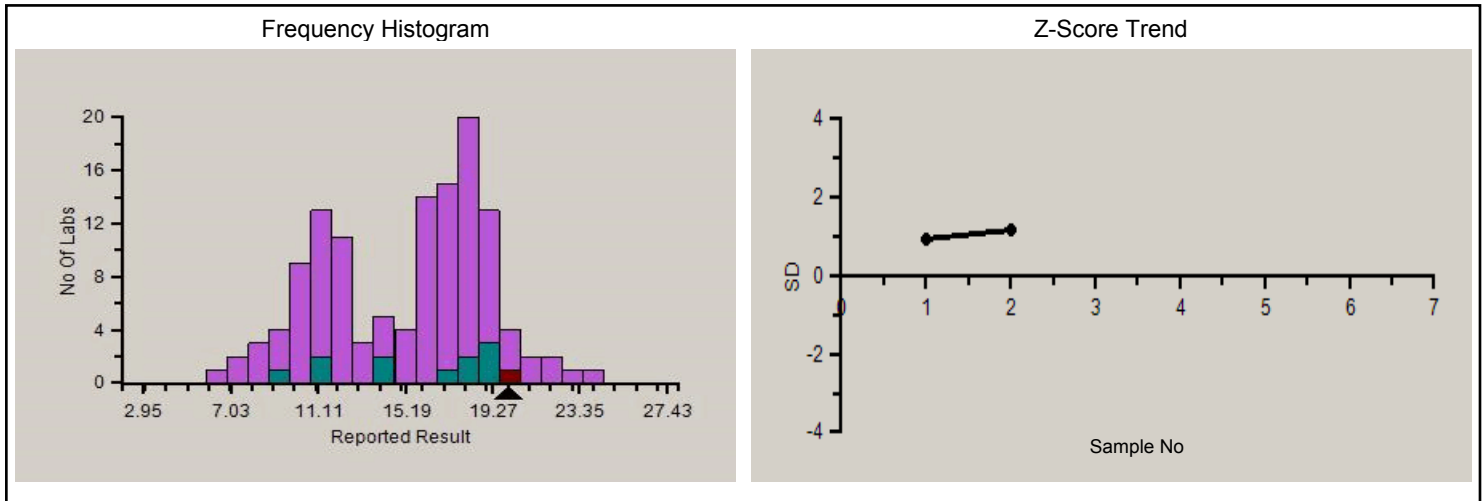

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, GGT		N	Mean	SD	CV%	Excluded
	All Analyzer	135	15.19	4.08	26.87	7
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	32	11.17	1.28	11.49	3
	Roche cobas c 311	24	17.57	1.20	6.83	1
	Fuji Dri-Chem 4000i	12	10.33	1.16	11.18	--
	Roche cobas INTEGRA	11	16.07	1.33	8.25	--
	Roche cobas c 111	10	17.46	3.05	17.48	1
	Horiba ABX Pentra C200	6	16.93	1.82	10.75	--
	Roche cobas 6000	6	17.33	1.37	7.88	--
	Beckman Coulter AU480	5	18.10	0.94	5.18	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, LDH, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	93	144.19	48.59	33.70	7
■ L to P - IFCC Ref. Proc., Calibrated	3	121.33	34.36	28.32	--
■ Fuji Nx 700	3	106.67	4.04	3.79	--

Your Result	102.00	SDI / z-Score	-1.10
Assigned Value	110.86	Average SDI	-0.67
SDPA	8.026	Uncertainty of AV	1.61
Standard Unit Result Val	102.00	%DEV	-15.93

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

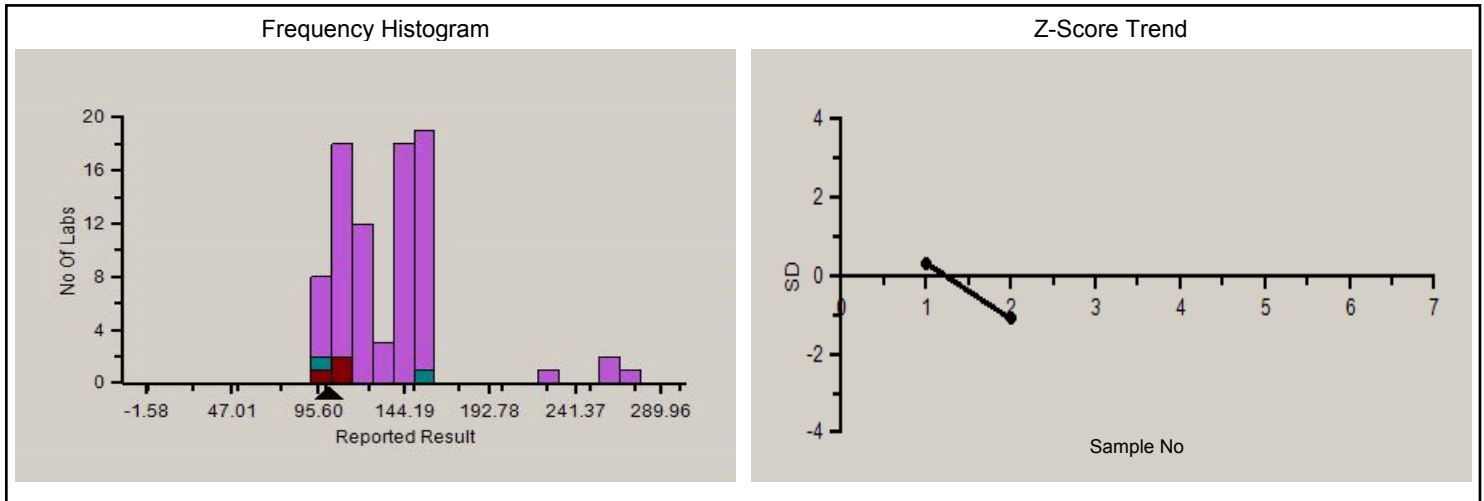

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, LDH		N	Mean	SD	CV%	Excluded
	All Analyzer	93	144.19	48.59	33.70	7
Your Analyzer :	Fuji Nx 700	3	106.67	4.04	3.79	--
	Fuji Dri-Chem NX500/i	24	110.46	7.38	6.68	--
	Fuji Dri-Chem 4000i	12	113.83	8.78	7.71	--
	Roche cobas c 311	11	149.36	5.09	3.40	--
	Roche cobas INTEGRA	7	148.56	3.73	2.51	--
	Roche cobas 6000	6	151.30	4.80	3.17	--
	Beckman Coulter AU480	4	268.20	0.00	0.00	--
	Roche cobas 8000	4	150.25	1.89	1.26	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, Lipase, U/L

	N	Mean	SD	CV%	Excluded
All Methods	80	47.49	14.45	30.42	7
Enzymatic colorimetric	14	44.43	11.50	25.89	3
Fuji Nx 700	3	55.33	7.10	12.82	--

Your Result	54.00	SDI / z-Score	-0.09
Assigned Value	54.41	Average SDI	-0.41
SDPA	4.841	Uncertainty of AV	0.99
Standard Unit Result Val	54.00	%DEV	21.54

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

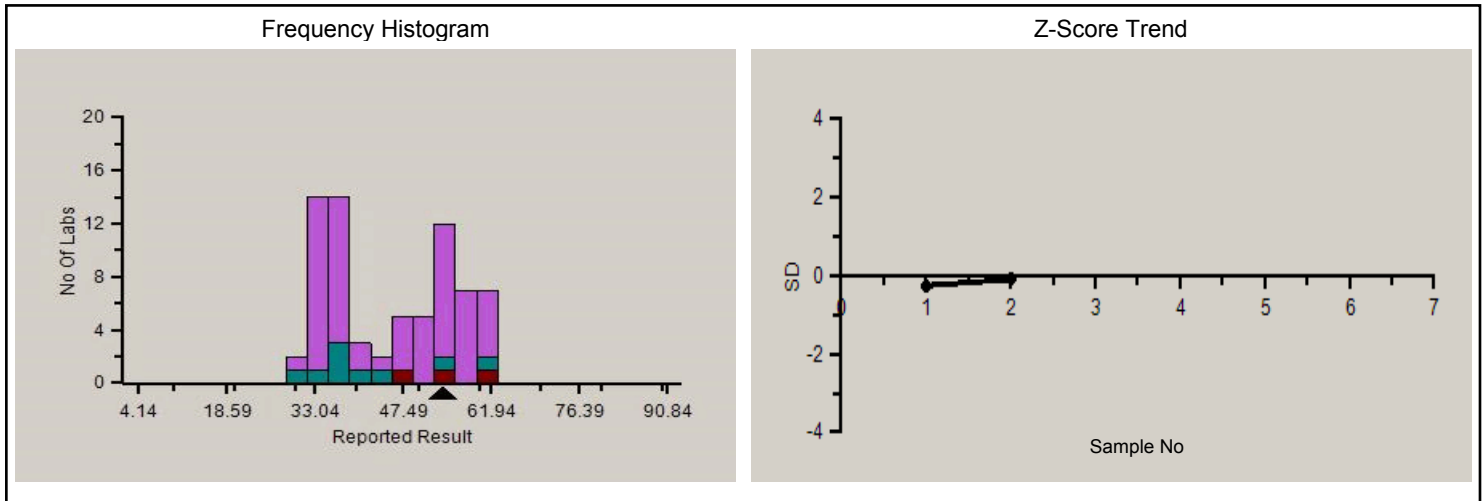

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, Lipase		N	Mean	SD	CV%	Excluded
	All Analyzer	80	47.49	14.45	30.42	7
Your Analyzer :	Fuji Nx 700	3	55.33	7.10	12.82	--
	Fuji Dri-Chem NX500/i	22	53.00	5.18	9.78	2
	Fuji Dri-Chem 4000i	14	55.86	3.30	5.91	--
	Roche cobas c 311	12	36.52	1.50	4.12	--
	Roche cobas INTEGRA	6	35.27	2.43	6.88	--
	Roche cobas 6000	5	35.04	1.29	3.69	--
	Roche cobas 8000	3	34.69	4.73	13.63	--
	Roche cobas c 111	2	36.70	--	--	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, Magnesium, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	55	1.07	0.67	62.72	6
Enzymatic	2	0.50	--	--	1
Fuji Nx 700	2	0.45	--	--	--

Your Result	0.50	SDI / z-Score	0.00
Assigned Value	0.50	Average SDI	-0.15
SDPA	0.070	Uncertainty of AV	0.01
Standard Unit Result Val	0.50	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

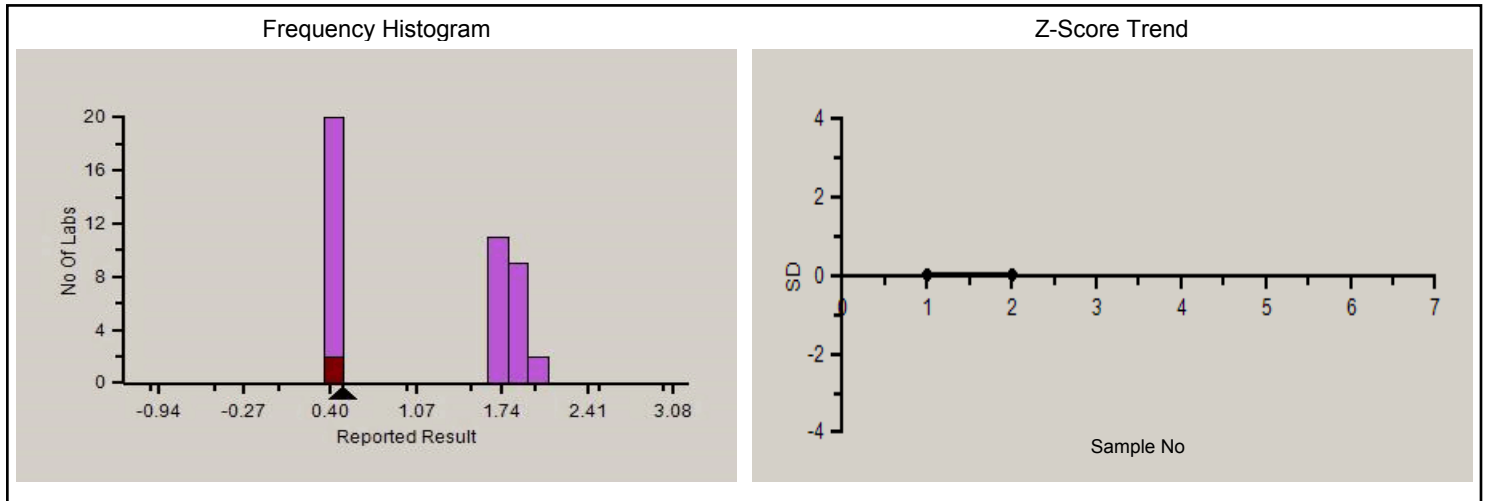

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, Magnesium		N	Mean	SD	CV%	Excluded
	All Analyzer	55	1.07	0.67	62.72	6
Your Analyzer :	Fuji Nx 700	2	0.45	--	--	--
	Fuji Dri-Chem NX500/i	17	0.47	0.03	7.27	2
	Fuji Dri-Chem 4000i	10	0.48	0.04	8.75	--
	Roche cobas c 311	7	1.75	0.04	2.23	--
	Roche cobas 6000	6	1.77	0.08	4.64	--
	Roche cobas 8000	4	1.89	0.09	4.83	--
	Roche cobas INTEGRA	2	1.70	--	--	1
	Beckman Coulter AU5800	1	--	--	--	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, Potassium, mEq/L

	N	Mean	SD	CV%	Excluded
■ All Methods	149	5.70	0.93	16.35	10
■ ISE direct	104	0.00	0.00	0.00	3
■ EasyLyte	9	0.00	0.00	0.00	--

Your Result	5.64	SDI / z-Score	-1.78
Assigned Value	6.25	Average SDI	-1.85
SDPA	0.343	Uncertainty of AV	0.04
Standard Unit Result Val	5.64	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

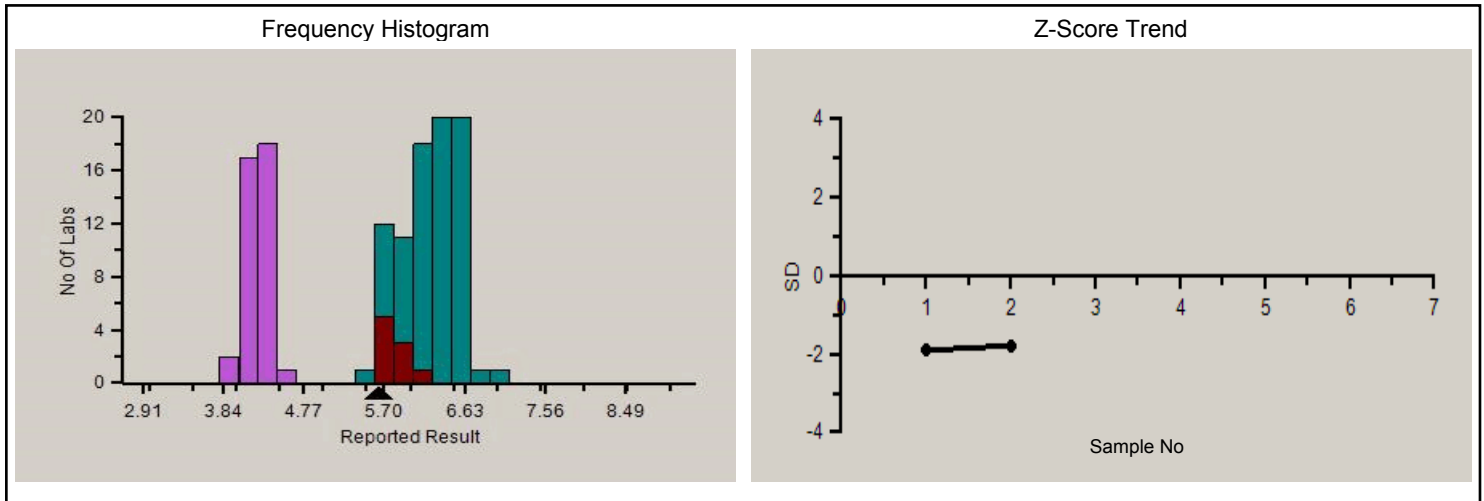

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, Potassium		N	Mean	SD	CV%	Excluded
	All Analyzer	149	5.70	0.93	16.35	10
Your Analyzer :	EasyLyte	9	0.00	0.00	0.00	--
	Fuji Dri-Chem NX500/i	33	0.00	0.00	0.00	1
	Fuji Dri-Chem 4000i	19	0.00	0.00	0.00	1
	Roche cobas c 311	15	0.00	0.00	0.00	--
	Roche AVL 9180	13	6.27	0.37	5.87	--
	Roche AVL 9180	12	0.00	0.00	0.00	--
	Roche cobas 6000	8	0.00	0.00	0.00	--
	Sensa Core	5	0.00	0.00	0.00	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, Sodium, mEq/L

	N	Mean	SD	CV%	Excluded
■ All Methods	149	159.00	23.11	14.54	15
■ ISE direct	104	0.00	0.00	0.00	8
■ EasyLyte	9	0.00	0.00	0.00	2

Your Result	168.50	SDI / z-Score	-0.57
Assigned Value	173.43	Average SDI	-0.57
SDPA	8.671	Uncertainty of AV	0.46
Standard Unit Result Val	168.50	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

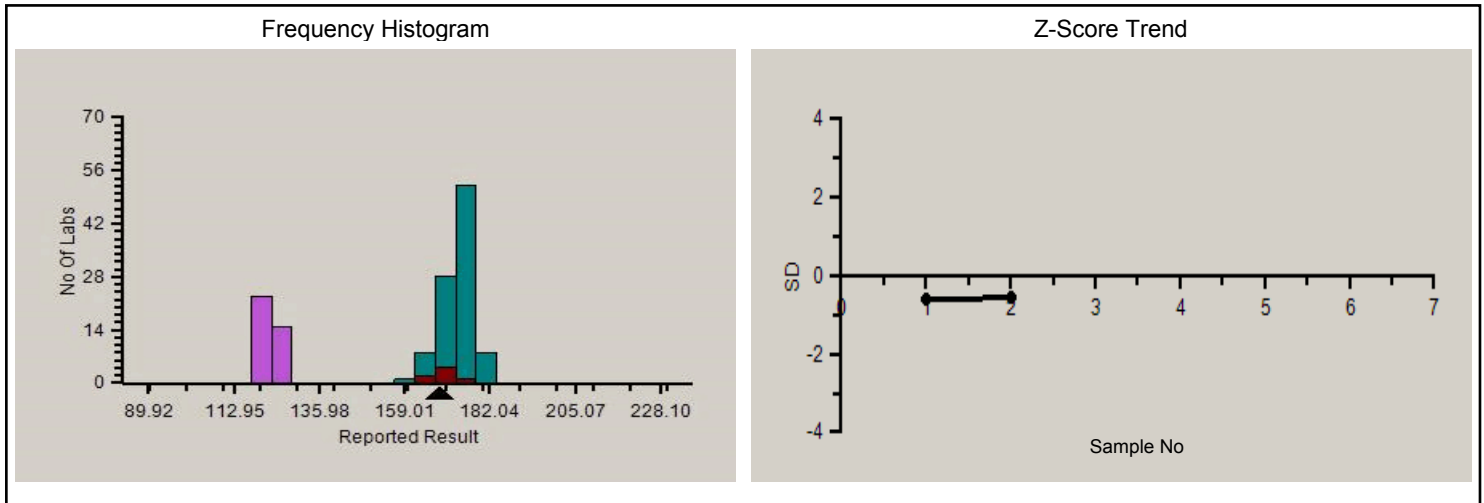

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, Sodium		N	Mean	SD	CV%	Excluded
	All Analyzer	149	159.00	23.11	14.54	15
Your Analyzer :	EasyLyte	9	0.00	0.00	0.00	2
	Fuji Dri-Chem NX500/i	34	0.00	0.00	0.00	3
	Fuji Dri-Chem 4000i	18	0.00	0.00	0.00	2
	Roche cobas c 311	15	0.00	0.00	0.00	--
	Roche AVL 9180	13	174.85	6.33	3.62	--
	Roche AVL 9180	12	0.00	0.00	0.00	--
	Roche cobas 6000	8	0.00	0.00	0.00	--
	Sensa Core	5	0.00	0.00	0.00	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, Total Protein, g/dL

	N	Mean	SD	CV%	Excluded
■ All Methods	164	6.40	0.32	5.03	4
■ Biuret	161	6.40	0.32	5.03	4
■ RANDOX RX daytona	1	--	--	--	--

Your Result	6.20	SDI / z-Score	-0.42
Assigned Value	6.31	Average SDI	-0.36
SDPA	0.252	Uncertainty of AV	0.03
Standard Unit Result Val	6.20	%DEV	-3.14

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

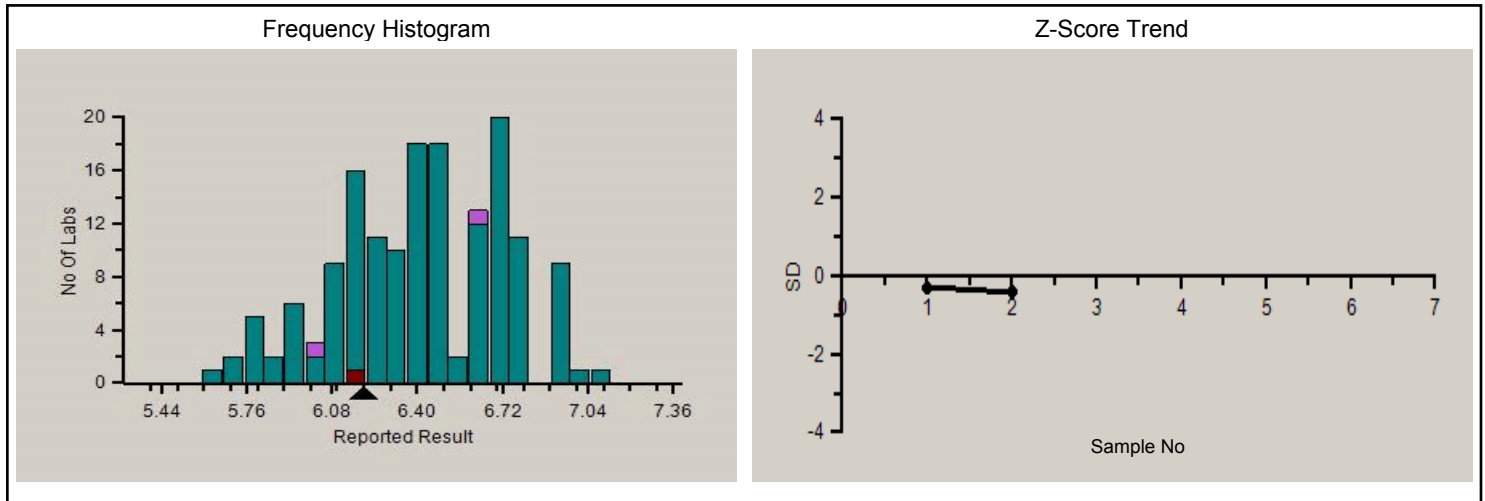

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, Total Protein		N	Mean	SD	CV%	Excluded
	All Analyzer	164	6.40	0.32	5.03	4
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	30	6.73	0.16	2.32	--
	Roche cobas c 311	27	6.37	0.19	3.04	--
	Fuji Dri-Chem 4000i	16	6.69	0.17	2.47	--
	Roche cobas c 111	11	6.27	0.29	4.69	--
	Roche cobas INTEGRA	10	6.12	0.26	4.23	--
	Horiba ABX Pentra C200	9	6.32	0.30	4.67	--
	Erba EM 200	8	6.31	0.29	4.52	1
	Roche cobas 6000	8	6.42	0.14	2.21	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, Triglycerides, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	164	110.59	9.47	8.56	10
■ GPO-PAP	14	116.69	7.08	6.07	1
■ RANDOX RX daytona	1	--	--	--	--

Your Result	124.00	SDI / z-Score	0.65
Assigned Value	115.00	Average SDI	0.41
SDPA	13.799	Uncertainty of AV	0.84
Standard Unit Result Val	124.00	%DEV	6.27

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

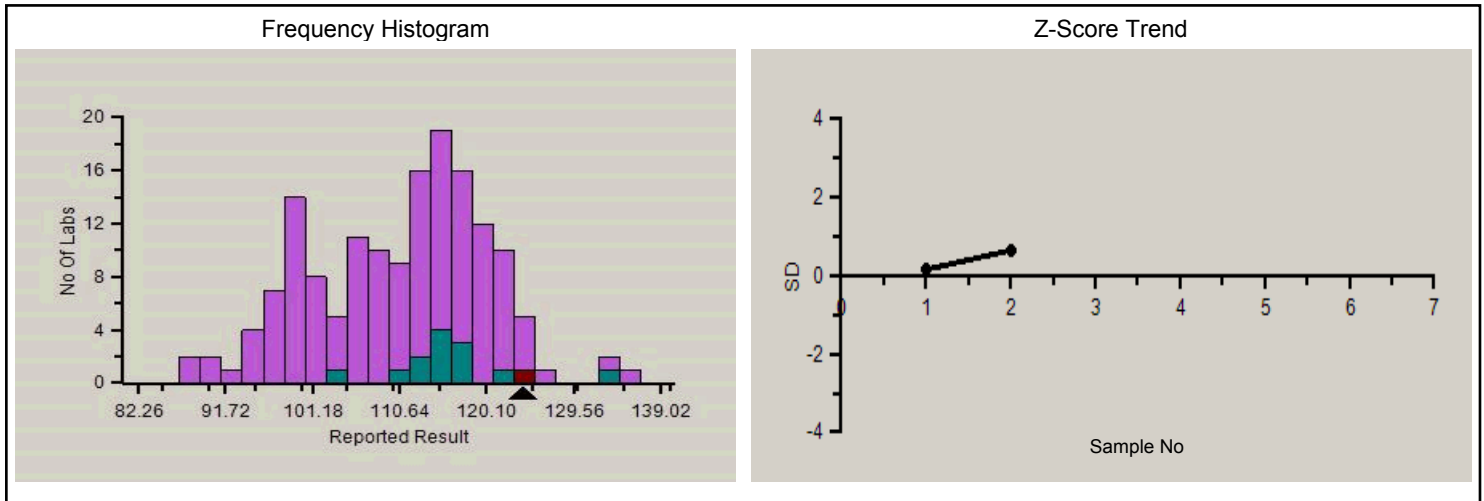

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, Triglycerides		N	Mean	SD	CV%	Excluded
	All Analyzer	164	110.59	9.47	8.56	10
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	32	101.86	7.47	7.33	--
	Roche cobas c 311	27	116.34	7.35	6.32	2
	Fuji Dri-Chem 4000i	16	100.07	6.91	6.91	1
	Roche cobas c 111	11	115.74	4.07	3.51	--
	Horiba ABX Pentra C200	10	116.05	3.63	3.13	1
	Roche cobas INTEGRA	10	114.28	5.62	4.92	--
	Roche cobas 6000	8	117.43	3.98	3.39	--
	Erba EM 200	6	112.98	7.08	6.27	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021


Biochemistry, Uric Acid, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	166	4.18	0.34	8.11	10
Uricase	25	4.11	0.32	7.86	3
RANDOX RX daytona	1	--	--	--	1

Your Result	3.40	SDI / z-Score	-1.72
Assigned Value	3.94	Average SDI	-1.92
SDPA	0.315	Uncertainty of AV	0.02
Standard Unit Result Val	3.40	%DEV	-17.27

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

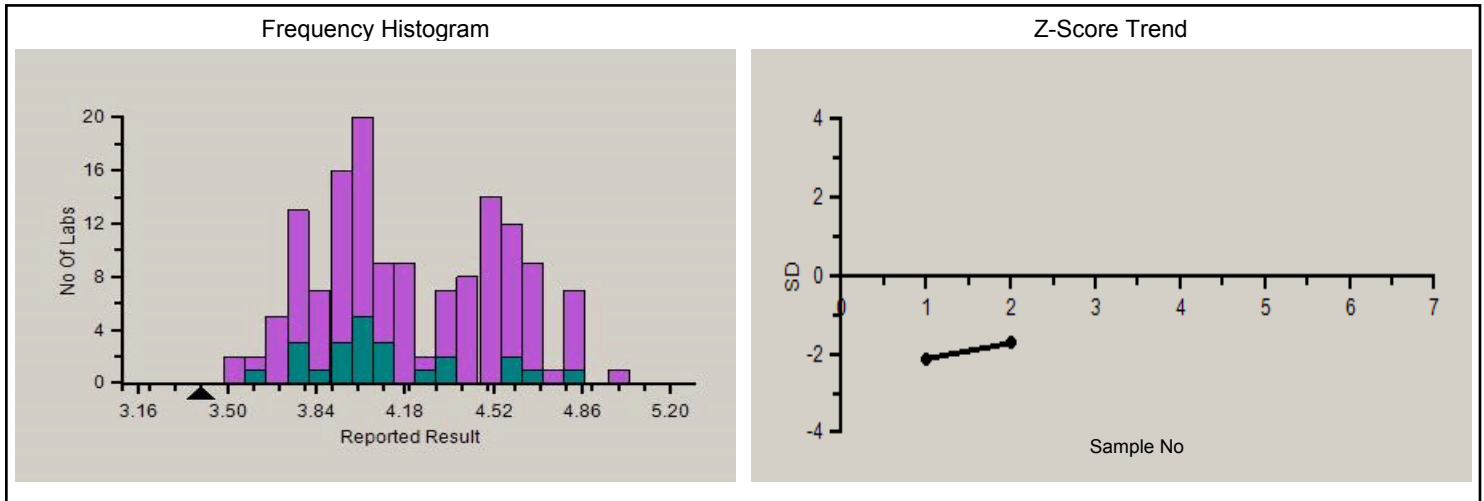

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021

Biochemistry, Uric Acid		N	Mean	SD	CV%	Excluded
	All Analyzer	166	4.18	0.34	8.11	10
Your Analyzer :	RANDOX RX daytona	1	--	--	--	1
	Fuji Dri-Chem NX500/i	31	4.49	0.18	4.05	1
	Roche cobas c 311	25	3.94	0.13	3.20	1
	Fuji Dri-Chem 4000i	19	4.53	0.23	5.07	1
	Roche cobas c 111	11	3.95	0.18	4.58	--
	Horiba ABX Pentra C200	10	3.91	0.15	3.79	--
	Roche cobas INTEGRA	10	3.96	0.11	2.68	--
	Roche cobas 6000	8	3.90	0.11	2.74	--
	Erba EM 200	6	4.54	0.42	9.26	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS

Unit No. 409-416.
Commercial Building - 1A,
Kohinoor Mall, Kirool Road, Kuria (W),
Mumbai - 400070



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 3
Sample Date : 03-03-2021


Biochemistry, Cholesterol, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	163	149.43	8.19	5.48	6
Cholesterol oxidase, esterase, peroxidase	111	149.05	8.25	5.53	2
RANDOX RX daytona	1	--	--	--	--

Your Result	162.00	SDI / z-Score	0.83
Assigned Value	148.50	Average SDI	0.82
SDPA	16.335	Uncertainty of AV	5.00
Standard Unit Result Val	162.00	%DEV	8.69

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

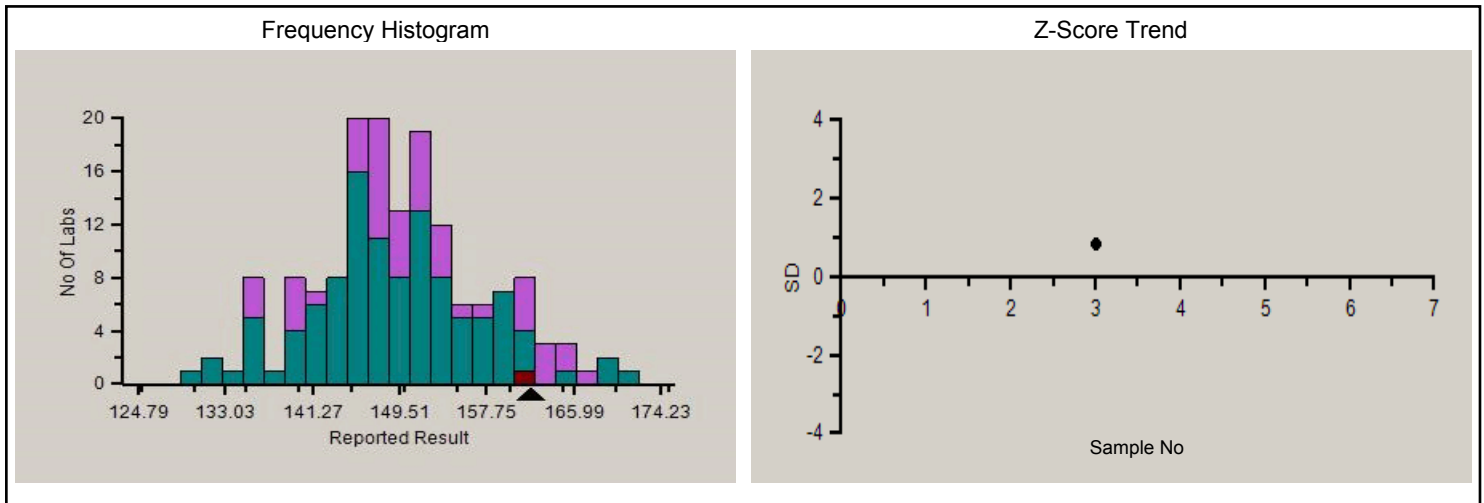

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 3
 Sample Date : 03-03-2021

Biochemistry, Cholesterol		N	Mean	SD	CV%	Excluded
	All Analyzer	163	149.43	8.19	5.48	6
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	30	143.06	6.14	4.29	2
	Roche cobas c 311	28	150.00	4.46	2.97	--
	Fuji Dri-Chem 4000i	16	143.93	8.00	5.56	--
	Roche cobas c 111	12	150.37	4.83	3.22	--
	Roche cobas c 111	11	150.68	4.95	3.28	--
	Roche cobas INTEGRA	10	147.94	3.88	2.62	--
	Horiba ABX Pentra C200	9	159.25	7.22	4.54	1
	Roche cobas 6000	8	150.00	3.12	2.08	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 3
Sample Date : 03-03-2021


Biochemistry, Creatinine, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	167	0.71	0.21	29.07	11
Ammonia Concentration Measurement - color change of BPB	44	0.48	0.13	26.04	4
Fuji Nx 700	1	--	--	--	--

Your Result	0.57	SDI / z-Score	2.12
Assigned Value	0.45	Average SDI	1.23
SDPA	0.059	Uncertainty of AV	0.01
Standard Unit Result Val	0.57	%DEV	18.75

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

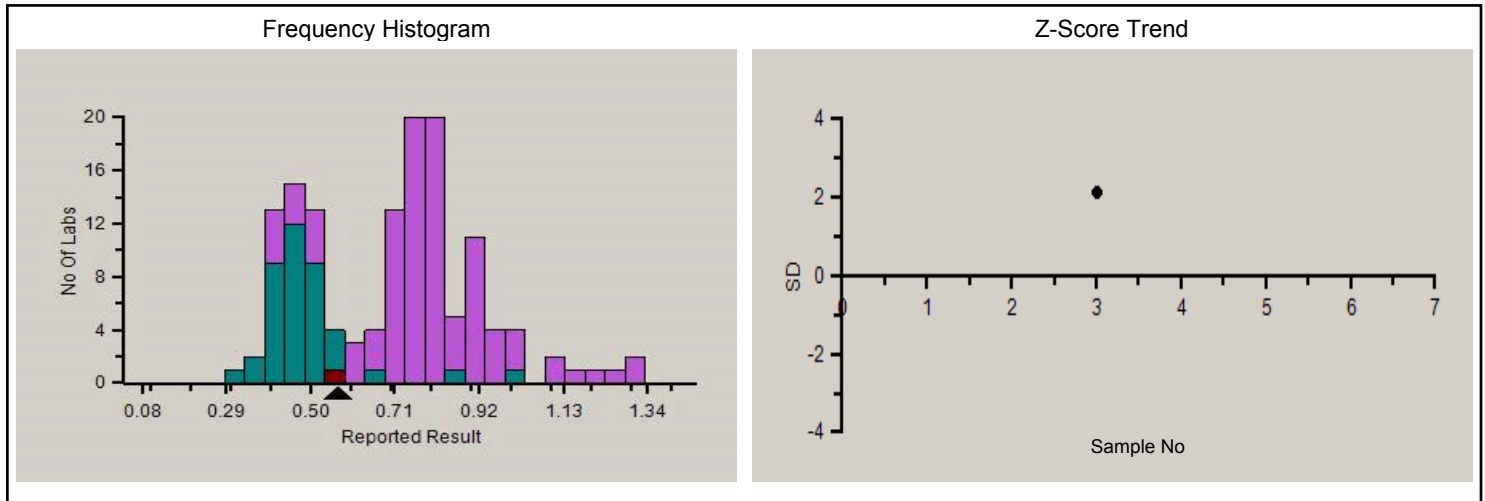

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 3
 Sample Date : 03-03-2021

Biochemistry, Creatinine		N	Mean	SD	CV%	Excluded
	All Analyzer	167	0.71	0.21	29.07	11
Your Analyzer :	Fuji Nx 700	1	--	--	--	--
	Fuji Dri-Chem NX500/i	29	0.43	0.05	11.48	2
	Roche cobas c 311	28	0.78	0.05	6.31	--
	Fuji Dri-Chem 4000i	16	0.47	0.05	10.62	2
	Roche cobas c 111	12	0.79	0.07	9.25	--
	Horiba ABX Pentra C200	11	0.89	0.10	10.86	1
	Roche cobas c 111	11	0.81	0.05	6.46	--
	Roche cobas INTEGRA	10	0.75	0.06	7.31	1
	Roche cobas 6000	8	0.79	0.06	7.01	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 3
Sample Date : 03-03-2021


Biochemistry, Glucose, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	171	73.92	3.52	4.76	10
■ GOD-PAP	7	75.87	2.31	3.05	--
■ RANDOX RX daytona	1	--	--	--	--

Your Result	74.00	SDI / z-Score	-0.23
Assigned Value	75.28	Average SDI	0.10
SDPA	5.646	Uncertainty of AV	0.32
Standard Unit Result Val	74.00	%DEV	-2.47

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

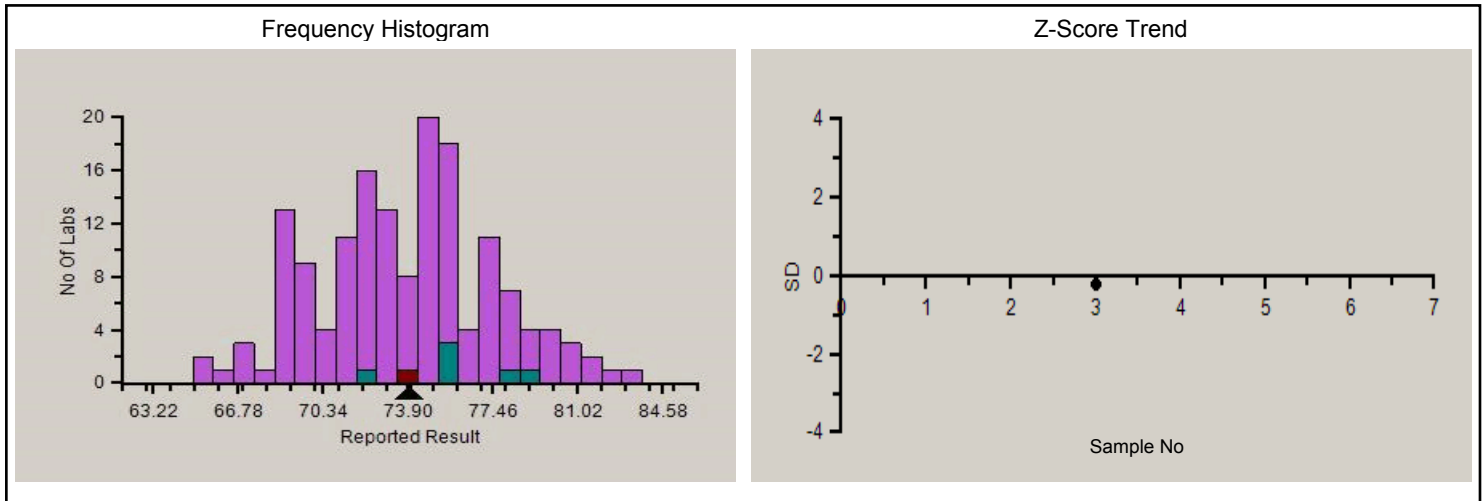

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 3
 Sample Date : 03-03-2021

Biochemistry, Glucose		N	Mean	SD	CV%	Excluded
	All Analyzer	171	73.92	3.52	4.76	10
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	31	70.97	2.50	3.52	--
	Roche cobas c 311	29	75.76	2.54	3.36	--
	Fuji Dri-Chem 4000i	16	70.87	1.81	2.55	1
	Horiba ABX Pentra C200	12	74.11	2.92	3.94	--
	Roche cobas c 111	11	75.64	1.35	1.79	2
	Roche cobas c 111	10	75.27	0.82	1.09	2
	Roche cobas INTEGRA	10	74.81	1.74	2.33	--
	Roche cobas 6000	8	75.75	1.83	2.42	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 3
Sample Date : 03-03-2021


Biochemistry, HDL, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	152	35.32	3.95	11.18	3
■ Direct Clearance	2	34.00	--	--	--
■ RANDOX RX daytona	2	33.00	--	--	--

Your Result	34.00	SDI / z-Score	-0.02
Assigned Value	34.07	Average SDI	0.07
SDPA	3.583	Uncertainty of AV	0.47
Standard Unit Result Val	34.00	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

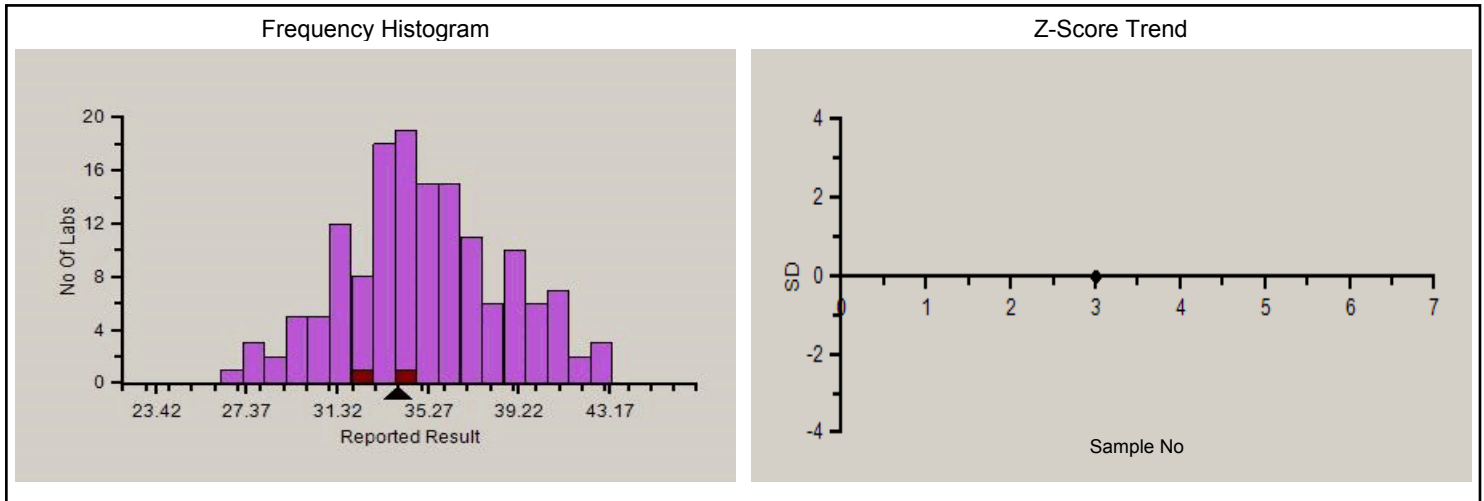

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 3
 Sample Date : 03-03-2021

Biochemistry, HDL		N	Mean	SD	CV%	Excluded
	All Analyzer	152	35.32	3.95	11.18	3
Your Analyzer :	RANDOX RX daytona	2	33.00	--	--	--
	Fuji Dri-Chem NX500/i	31	36.00	2.14	5.96	--
	Roche cobas c 311	27	32.84	2.10	6.40	--
	Fuji Dri-Chem 4000i	15	35.93	2.79	7.76	--
	Roche cobas c 111	12	31.11	2.08	6.70	--
	Roche cobas c 111	11	30.95	2.10	6.80	--
	Horiba ABX Pentra C200	9	39.99	1.65	4.14	--
	Roche cobas INTEGRA	9	31.93	2.37	7.43	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 3
Sample Date : 03-03-2021


Biochemistry, LDL, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	60	97.67	7.31	7.48	5
■ Direct Measurement	7	96.40	10.45	10.84	--
■ RANDOX RX daytona	1	--	--	--	--

Your Result	89.00	SDI / z-Score	0.29
Assigned Value	85.87	Average SDI	0.29
SDPA	10.826	Uncertainty of AV	5.52
Standard Unit Result Val	89.00	%DEV	-7.68

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

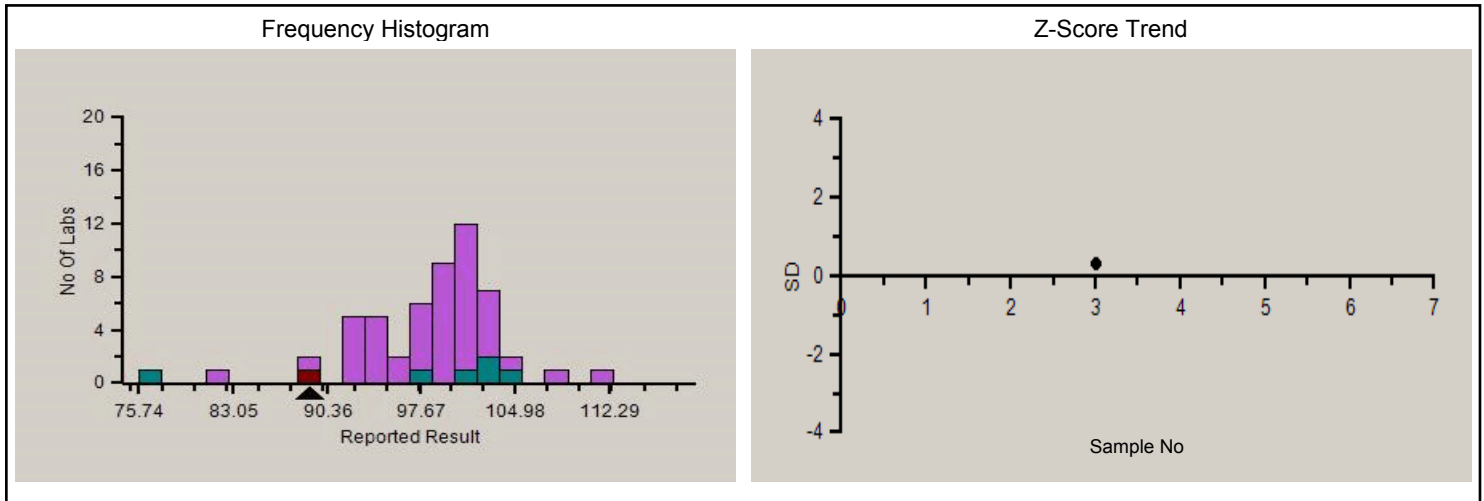

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 3
 Sample Date : 03-03-2021

Biochemistry, LDL		N	Mean	SD	CV%	Excluded
	All Analyzer	60	97.67	7.31	7.48	5
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Roche cobas c 311	21	99.32	4.63	4.66	--
	Roche cobas 6000	7	101.24	2.27	2.24	--
	Roche cobas INTEGRA	6	100.00	3.27	3.27	--
	Horiba ABX Pentra C200	4	85.64	7.97	9.30	--
	Roche cobas c 111	4	99.24	6.44	6.49	1
	Erba EM 360	3	92.40	0.00	0.00	2
	Roche cobas 8000	3	100.93	3.32	3.29	--
	Beckman Coulter AU480	2	101.15	--	--	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 3
Sample Date : 03-03-2021


Biochemistry, Phosphorous Inorganic, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	125	3.40	0.16	4.76	6
Phosphomolybdate method	62	3.38	0.14	3.99	1
RANDOX RX daytona	1	--	--	--	--

Your Result	3.50	SDI / z-Score	0.30
Assigned Value	3.39	Average SDI	0.17
SDPA	0.373	Uncertainty of AV	0.02
Standard Unit Result Val	3.50	%DEV	3.52

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

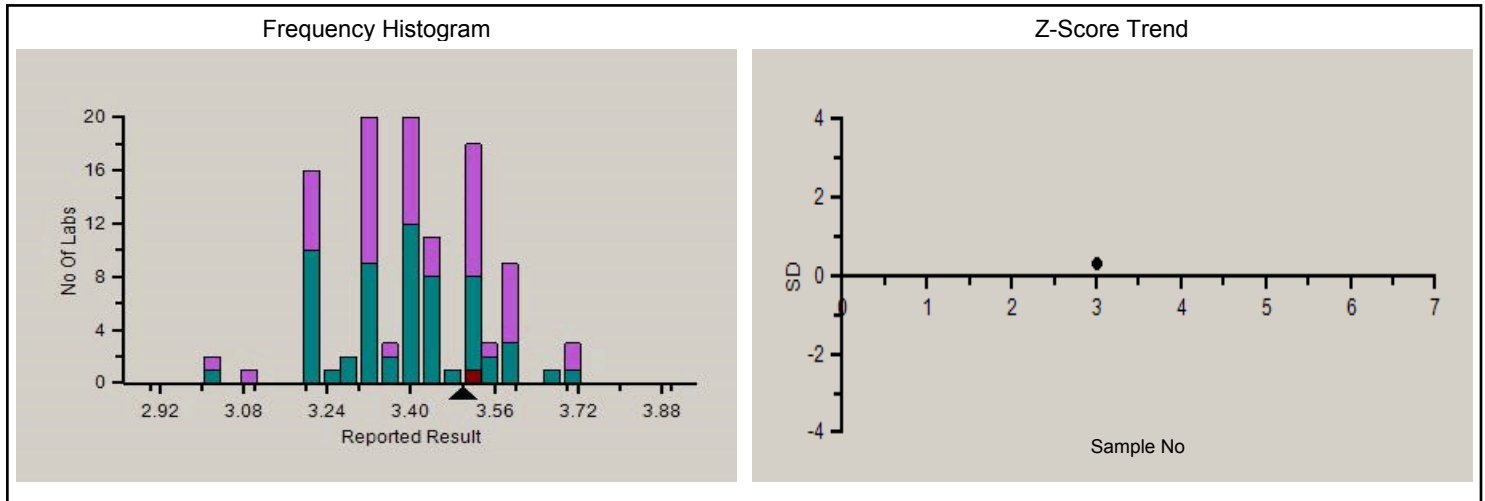

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 3
 Sample Date : 03-03-2021

Biochemistry, Phosphorous Inorganic		N	Mean	SD	CV%	Excluded
	All Analyzer	125	3.40	0.16	4.76	6
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	29	3.36	0.13	3.99	--
	Roche cobas c 311	23	3.39	0.12	3.42	--
	Fuji Dri-Chem 4000i	13	3.39	0.16	4.75	--
	Roche cobas 6000	8	3.31	0.10	3.03	--
	Roche cobas INTEGRA	8	3.43	0.08	2.19	--
	Roche cobas c 111	5	3.54	0.10	2.71	--
	Roche cobas 8000	4	3.38	0.10	2.84	--
	Beckman Coulter AU480	3	3.50	0.11	3.26	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 3
Sample Date : 03-03-2021


Biochemistry, Urea, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	163	23.67	3.40	14.37	18
Urease, GLDH	28	25.90	2.25	8.70	4
RANDOX RX daytona	1	--	--	--	--

Your Result	28.00	SDI / z-Score	0.85
Assigned Value	25.50	Average SDI	1.07
SDPA	2.932	Uncertainty of AV	0.18
Standard Unit Result Val	28.00	%DEV	8.10

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

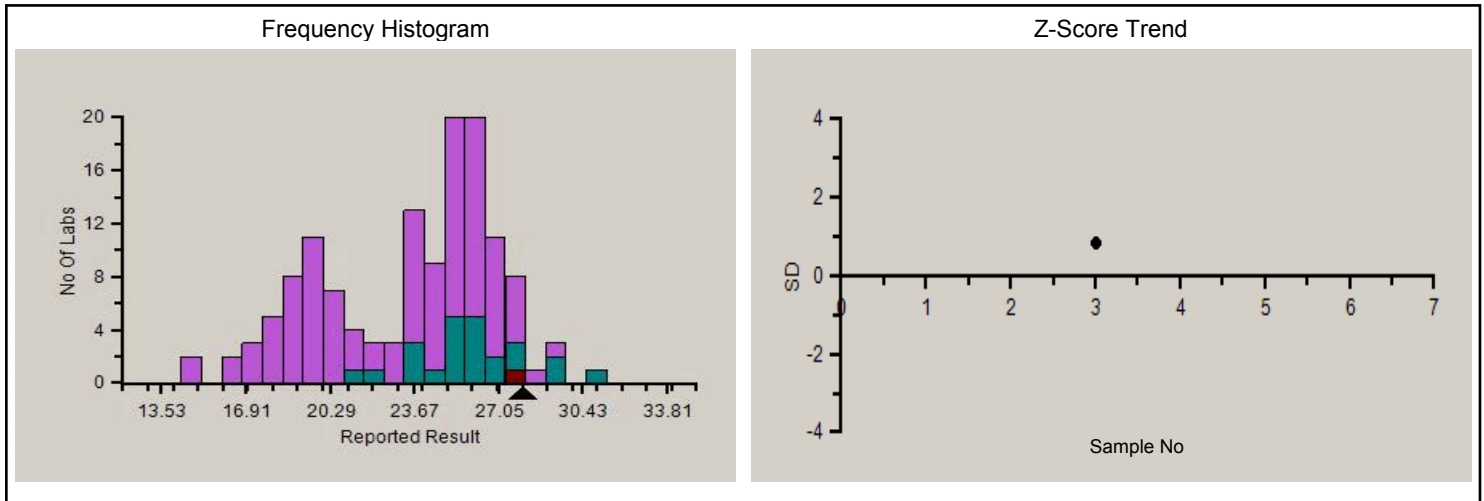

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 3
Sample Date : 03-03-2021

Biochemistry, Urea		N	Mean	SD	CV%	Excluded
	All Analyzer	163	23.67	3.40	14.37	18
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Roche cobas c 311	28	25.81	1.18	4.59	--
	Fuji Dri-Chem NX500/i	25	19.04	1.41	7.41	4
	Fuji Dri-Chem 4000i	16	19.53	0.65	3.34	2
	Horiba ABX Pentra C200	12	27.13	0.88	3.25	3
	Roche cobas c 111	12	24.84	0.73	2.92	--
	Roche cobas c 111	11	24.81	0.76	3.04	--
	Roche cobas INTEGRA	10	24.20	1.12	4.62	--
	Roche cobas 6000	8	25.76	0.99	3.83	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS

Unit No. 409-416.
Commercial Building - 1A,
Kohinoor Mall, Kirool Road, Kuria (W),
Mumbai - 400070



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 4
Sample Date : 03-03-2021


Biochemistry, Cholesterol, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	162	148.57	7.99	5.38	6
Cholesterol oxidase, esterase, peroxidase	112	147.88	7.77	5.25	2
RANDOX RX daytona	1	--	--	--	--

Your Result	160.00	SDI / z-Score	0.80
Assigned Value	151.00	Average SDI	0.82
SDPA	11.284	Uncertainty of AV	4.70
Standard Unit Result Val	160.00	%DEV	8.20

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

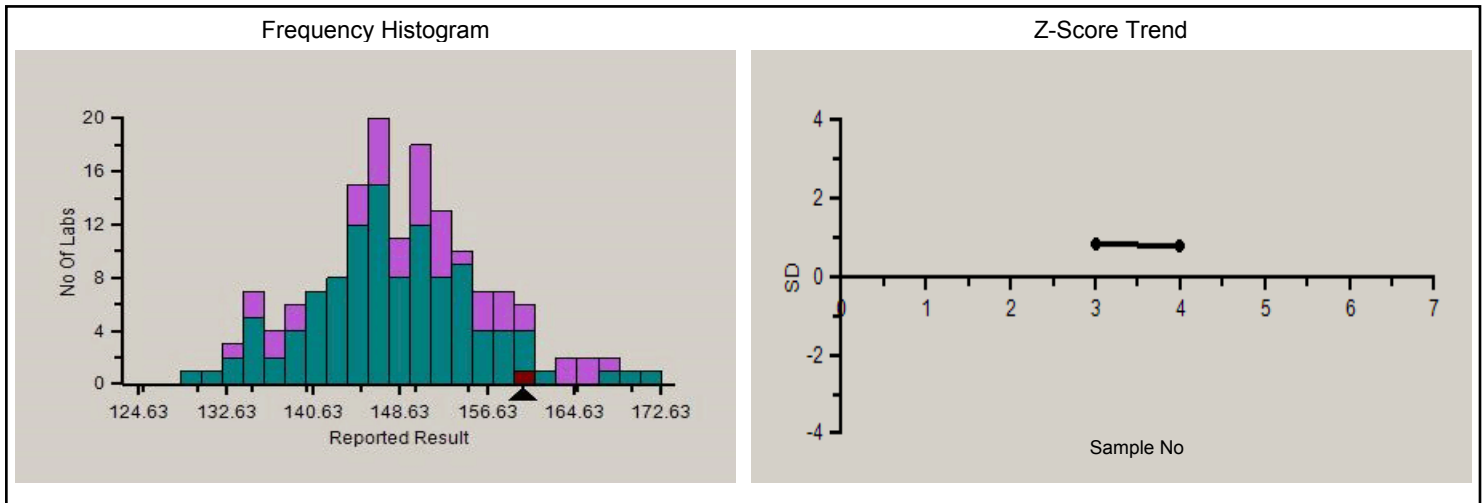

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 4
 Sample Date : 03-03-2021

Biochemistry, Cholesterol		N	Mean	SD	CV%	Excluded
	All Analyzer	162	148.57	7.99	5.38	6
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	31	141.82	5.36	3.78	2
	Roche cobas c 311	27	149.61	4.15	2.78	--
	Fuji Dri-Chem 4000i	16	142.96	6.31	4.41	--
	Roche cobas c 111	12	149.17	6.24	4.18	1
	Roche cobas c 111	11	149.38	6.53	4.37	1
	Roche cobas INTEGRA	10	147.16	3.78	2.57	--
	Horiba ABX Pentra C200	9	157.23	9.04	5.75	--
	Roche cobas 6000	8	148.88	3.72	2.50	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 4
Sample Date : 03-03-2021


Biochemistry, Creatinine, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	165	0.59	0.17	28.43	17
Ammonia Concentration Measurement - color change of BPB	44	0.39	0.07	18.96	4
Fuji Nx 700	1	--	--	--	1

Your Result	0.52	SDI / z-Score	2.41
Assigned Value	0.37	Average SDI	1.23
SDPA	0.063	Uncertainty of AV	0.01
Standard Unit Result Val	0.52	%DEV	35.06

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

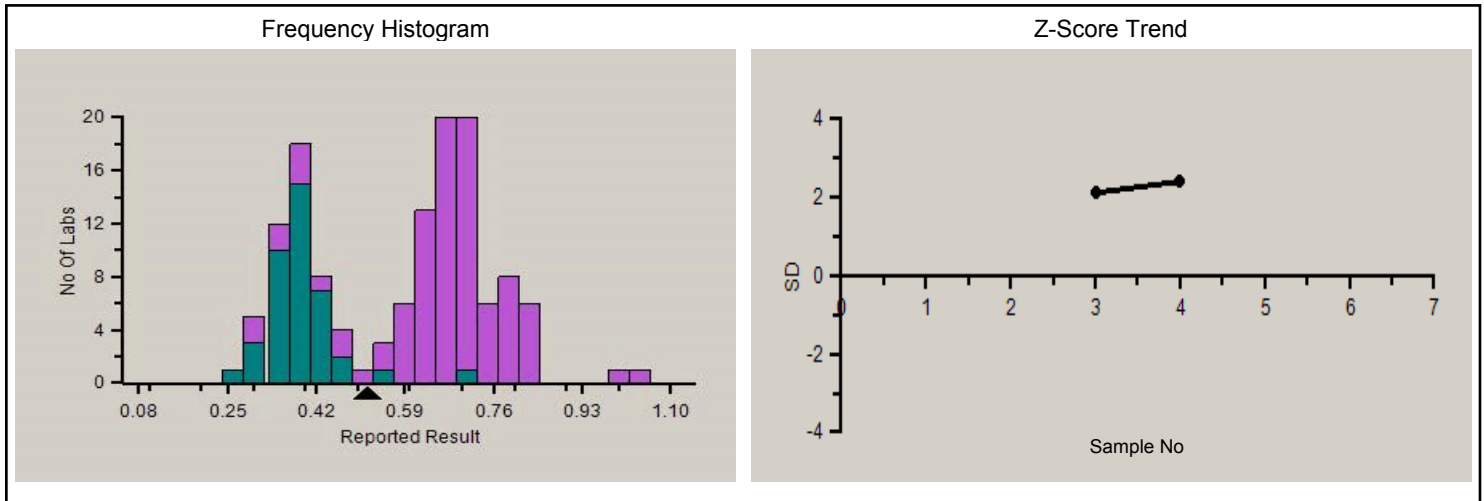

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 4
 Sample Date : 03-03-2021

Biochemistry, Creatinine		N	Mean	SD	CV%	Excluded
	All Analyzer	165	0.59	0.17	28.43	17
Your Analyzer :	Fuji Nx 700	1	--	--	--	1
	Fuji Dri-Chem NX500/i	29	0.36	0.05	13.65	2
	Roche cobas c 311	27	0.67	0.05	6.86	--
	Fuji Dri-Chem 4000i	16	0.38	0.04	10.94	--
	Roche cobas c 111	12	0.69	0.07	10.15	--
	Horiba ABX Pentra C200	11	0.76	0.06	8.33	4
	Roche cobas c 111	11	0.70	0.07	10.22	--
	Roche cobas INTEGRA	10	0.64	0.06	8.54	1
	Roche cobas 6000	8	0.69	0.03	4.63	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 4
Sample Date : 03-03-2021


Biochemistry, Glucose, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	169	76.08	3.72	4.89	10
GOD-PAP	7	76.93	2.62	3.41	--
RANDOX RX daytona	1	--	--	--	--

Your Result	77.00	SDI / z-Score	-0.09
Assigned Value	77.56	Average SDI	0.10
SDPA	5.971	Uncertainty of AV	0.31
Standard Unit Result Val	77.00	%DEV	0.09

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

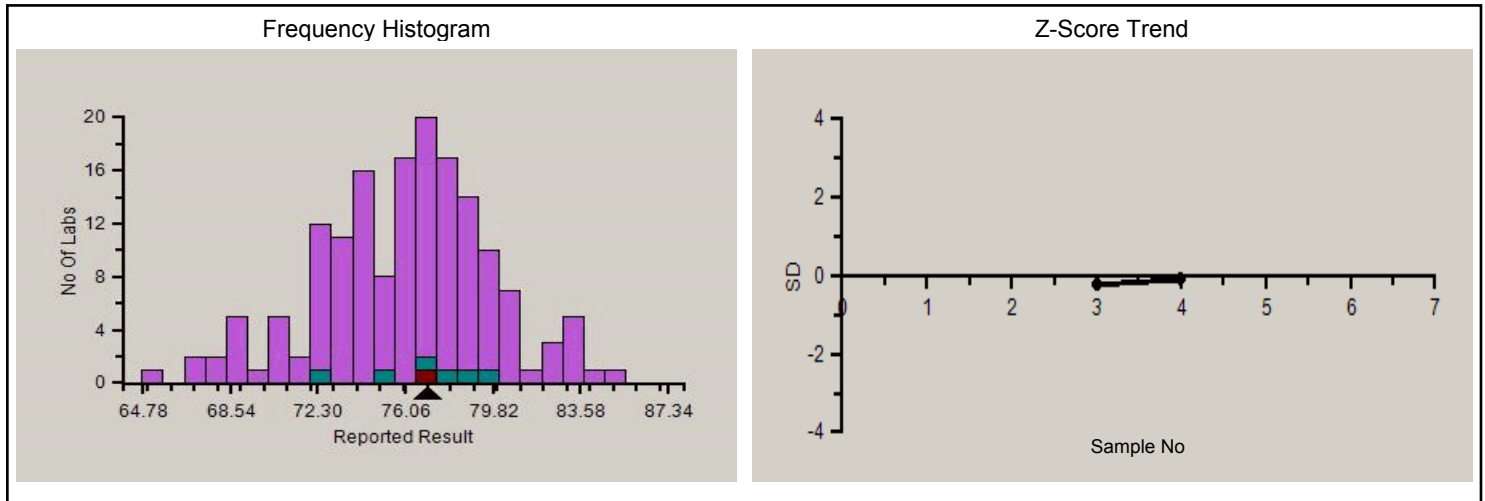

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 4
 Sample Date : 03-03-2021

Biochemistry, Glucose		N	Mean	SD	CV%	Excluded
	All Analyzer	169	76.08	3.72	4.89	10
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	31	72.88	2.81	3.86	--
	Roche cobas c 311	28	77.76	2.48	3.18	--
	Fuji Dri-Chem 4000i	16	73.27	1.67	2.28	1
	Horiba ABX Pentra C200	12	76.63	3.10	4.05	--
	Roche cobas c 111	11	78.13	1.94	2.49	3
	Roche cobas c 111	10	77.75	1.75	2.25	3
	Roche cobas INTEGRA	10	76.98	1.38	1.79	--
	Roche cobas 6000	8	77.88	2.23	2.87	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 4
Sample Date : 03-03-2021


Biochemistry, HDL, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	151	35.67	3.78	10.61	6
Direct Clearance	2	35.00	--	--	--
RANDOX RX daytona	2	36.50	--	--	--

Your Result	35.00	SDI / z-Score	0.15
Assigned Value	34.44	Average SDI	0.07
SDPA	3.671	Uncertainty of AV	0.48
Standard Unit Result Val	35.00	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

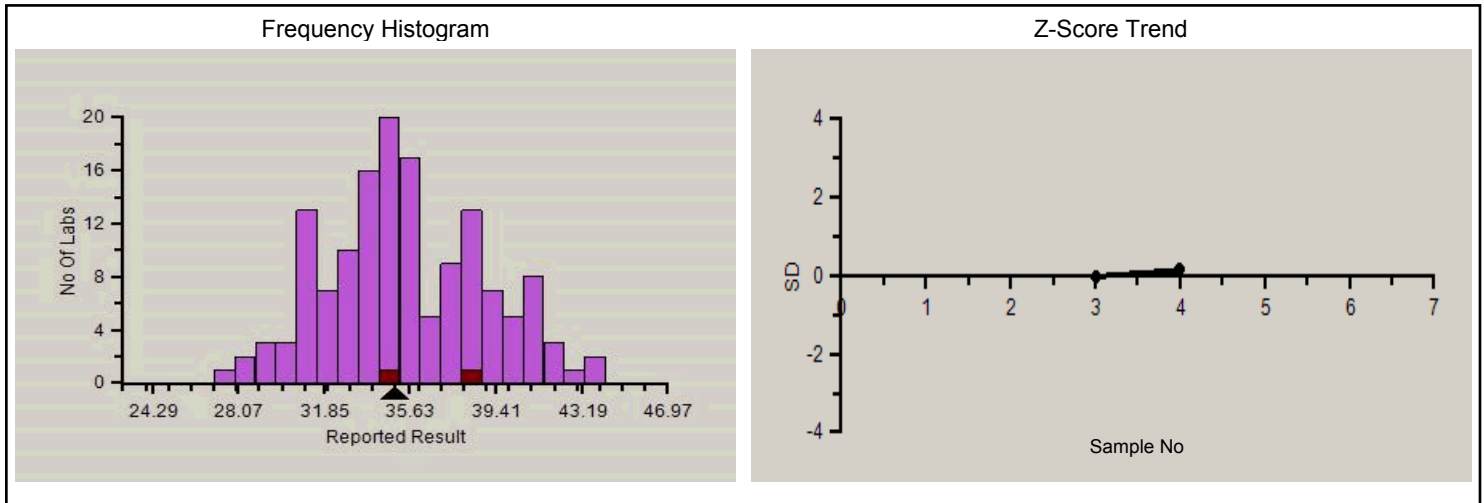

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 4
 Sample Date : 03-03-2021

Biochemistry, HDL		N	Mean	SD	CV%	Excluded
	All Analyzer	151	35.67	3.78	10.61	6
Your Analyzer :	RANDOX RX daytona	2	36.50	--	--	--
	Fuji Dri-Chem NX500/i	30	36.22	1.84	5.07	--
	Roche cobas c 311	27	33.19	2.02	6.07	--
	Fuji Dri-Chem 4000i	15	36.86	2.03	5.52	1
	Roche cobas c 111	12	31.24	2.12	6.80	--
	Roche cobas c 111	11	30.96	1.99	6.41	--
	Horiba ABX Pentra C200	9	40.50	1.79	4.42	--
	Roche cobas INTEGRA	9	32.24	2.25	6.98	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 4
Sample Date : 03-03-2021


Biochemistry, LDL, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	59	96.14	6.18	6.43	5
Direct Measurement	7	95.02	10.01	10.54	--
RANDOX RX daytona	1	--	--	--	--

Your Result	89.00	SDI / z-Score	0.28
Assigned Value	86.65	Average SDI	0.29
SDPA	8.342	Uncertainty of AV	4.26
Standard Unit Result Val	89.00	%DEV	-6.33

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

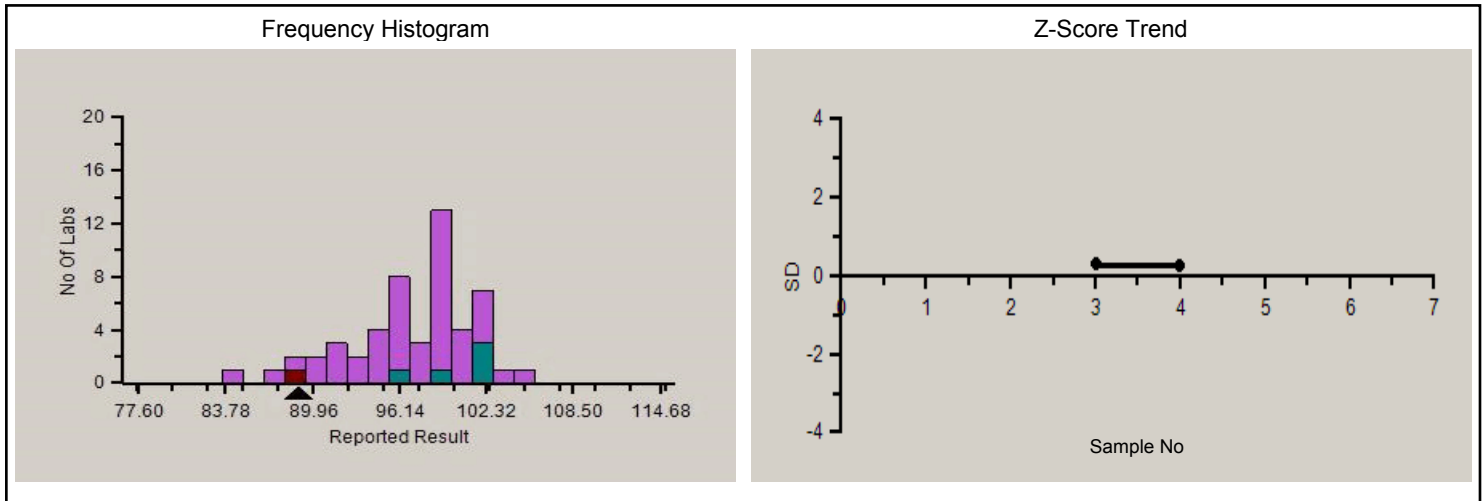

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 4
 Sample Date : 03-03-2021

Biochemistry, LDL		N	Mean	SD	CV%	Excluded
	All Analyzer	59	96.14	6.18	6.43	5
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Roche cobas c 311	21	97.30	3.93	4.04	1
	Roche cobas 6000	7	99.50	1.98	1.99	--
	Roche cobas INTEGRA	6	98.36	3.00	3.05	--
	Horiba ABX Pentra C200	4	85.80	8.09	9.42	--
	Roche cobas c 111	4	96.67	6.71	6.94	1
	Roche cobas 8000	3	99.27	2.48	2.50	--
	Beckman Coulter AU480	2	101.30	--	--	--
	Erba EM 360	2	90.90	--	--	1

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 4
Sample Date : 03-03-2021


Biochemistry, Phosphorous Inorganic, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	124	3.34	0.16	4.89	7
Phosphomolybdate method	62	3.32	0.13	3.97	1
RANDOX RX daytona	1	--	--	--	--

Your Result	3.50	SDI / z-Score	0.54
Assigned Value	3.32	Average SDI	0.17
SDPA	0.332	Uncertainty of AV	0.02
Standard Unit Result Val	3.50	%DEV	5.36

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

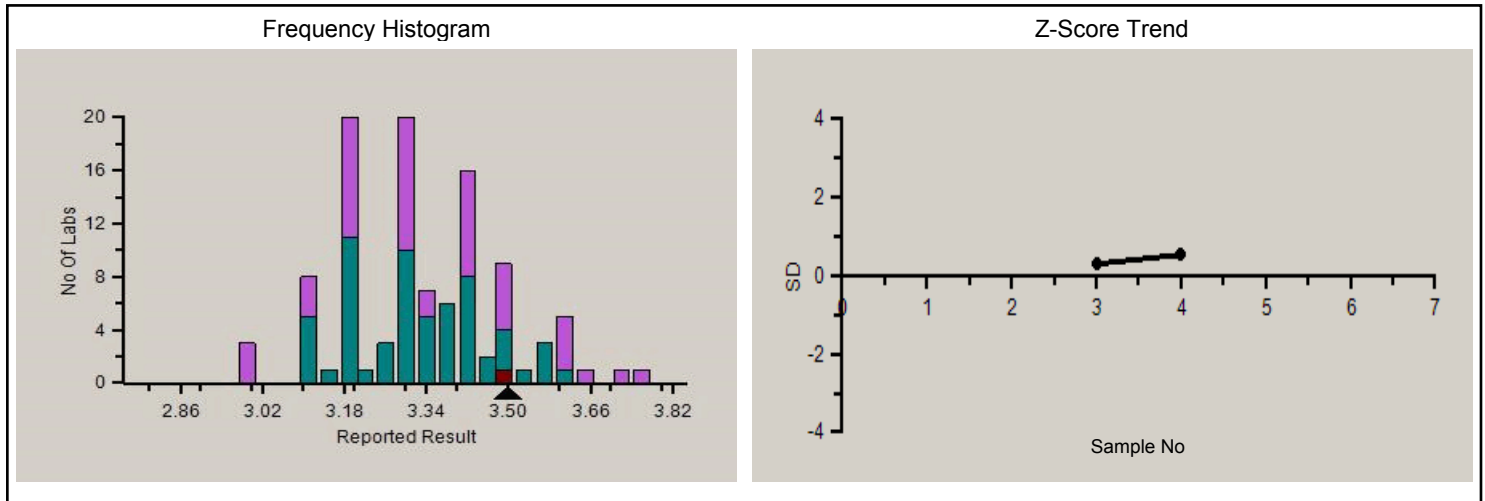

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 4
 Sample Date : 03-03-2021

Biochemistry, Phosphorous Inorganic						
	N	Mean	SD	CV%	Excluded	
All Analyzer	124	3.34	0.16	4.89	7	
Your Analyzer : RANDOX RX daytona	1	--	--	--	--	
Fuji Dri-Chem NX500/i	29	3.32	0.14	4.07	1	
Roche cobas c 311	22	3.33	0.14	4.17	--	
Fuji Dri-Chem 4000i	13	3.29	0.16	4.78	--	
Roche cobas 6000	8	3.24	0.11	3.25	--	
Roche cobas INTEGRA	8	3.34	0.06	1.86	--	
Roche cobas c 111	5	3.53	0.03	0.94	1	
Roche cobas 8000	4	3.28	0.07	2.26	--	
Beckman Coulter AU480	3	3.36	0.06	1.82	--	

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 4
Sample Date : 03-03-2021


Biochemistry, Urea, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	161	21.74	3.45	15.88	13
Urease, GLDH	26	23.62	2.63	11.14	3
RANDOX RX daytona	1	--	--	--	--

Your Result	27.00	SDI / z-Score	1.59
Assigned Value	23.31	Average SDI	1.07
SDPA	2.331	Uncertainty of AV	0.19
Standard Unit Result Val	27.00	%DEV	14.31

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

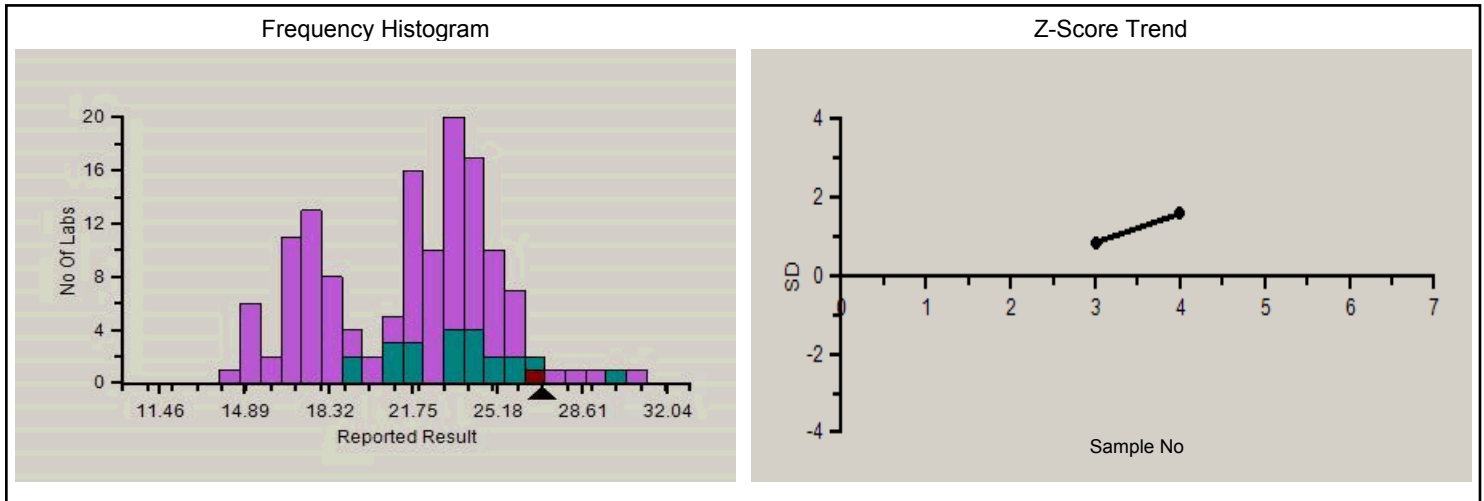

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 4
 Sample Date : 03-03-2021

Biochemistry, Urea		N	Mean	SD	CV%	Excluded
	All Analyzer	161	21.74	3.45	15.88	13
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Roche cobas c 311	27	23.59	0.99	4.21	--
	Fuji Dri-Chem NX500/i	25	17.02	1.36	8.00	3
	Fuji Dri-Chem 4000i	16	17.75	0.47	2.65	2
	Horiba ABX Pentra C200	12	25.44	1.35	5.30	1
	Roche cobas c 111	12	22.57	1.26	5.56	--
	Roche cobas c 111	11	22.49	1.29	5.72	--
	Roche cobas INTEGRA	10	22.03	1.18	5.37	--
	Roche cobas 6000	8	23.30	0.81	3.49	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
 Unit No. 409-416.
 Commercial Building - 1A,
 Kohinoor Mall, Kirool Road, Kuria (W),
 Mumbai - 400070



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, ALP, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	141	193.32	20.55	10.63	10
■ PNPP, AMP Buffer	65	196.76	21.76	11.06	5
■ RANDOX RX daytona	1	--	--	--	--

Your Result	179.00	SDI / z-Score	-0.23
Assigned Value	184.97	Average SDI	-1.16
SDPA	25.896	Uncertainty of AV	2.01
Standard Unit Result Val	179.00	%DEV	-9.03

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

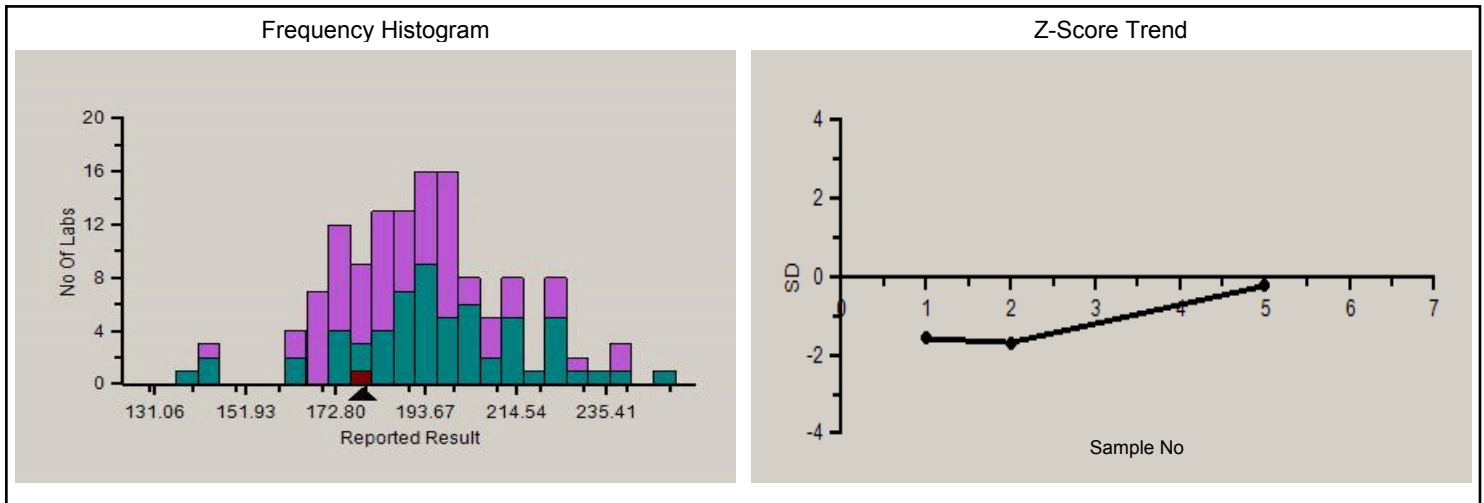

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, ALP		N	Mean	SD	CV%	Excluded
	All Analyzer	141	193.32	20.55	10.63	10
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	32	203.03	15.57	7.67	1
	Roche cobas c 311	27	181.23	9.50	5.24	--
	Fuji Dri-Chem 4000i	15	204.14	16.81	8.24	1
	Roche cobas c 111	11	191.72	21.02	10.96	--
	Horiba ABX Pentra C200	10	193.52	17.60	9.10	1
	Roche cobas c 111	10	186.89	14.35	7.68	--
	Roche cobas INTEGRA	9	190.45	16.85	8.85	--
	Roche cobas 6000	8	186.50	10.06	5.39	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, ALT, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	144	46.97	3.72	7.92	4
■ IFCC - UV without P5P	13	50.02	2.86	5.72	1
■ RANDOX RX daytona	1	--	--	--	--

Your Result	54.00	SDI / z-Score	1.66
Assigned Value	46.33	Average SDI	0.65
SDPA	4.623	Uncertainty of AV	0.38
Standard Unit Result Val	54.00	%DEV	7.95

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

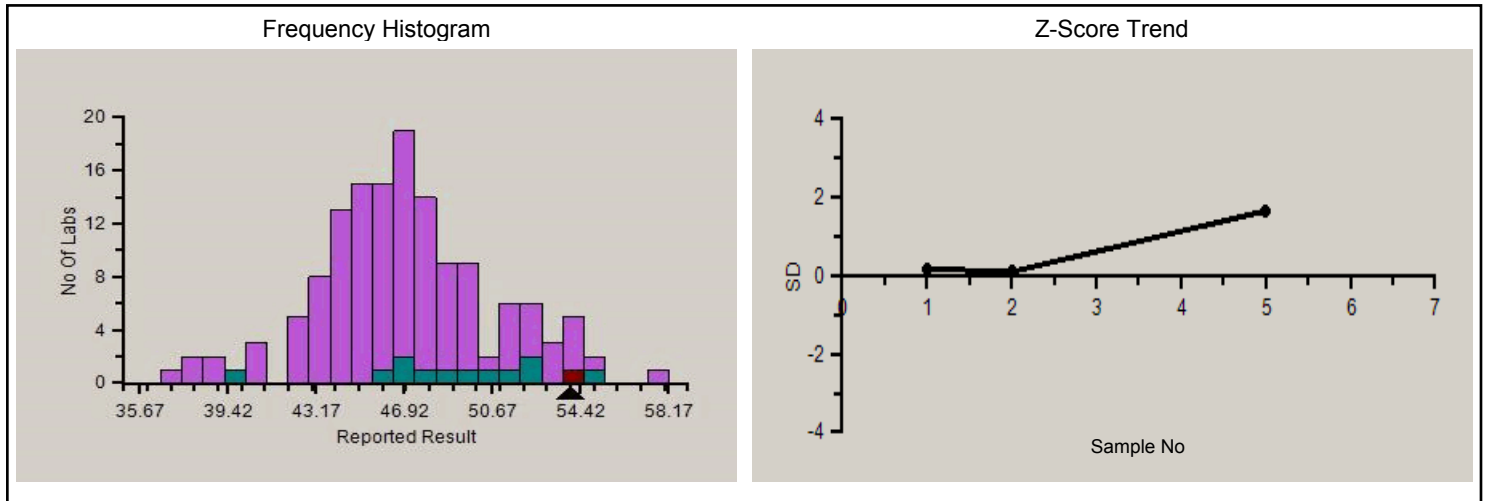

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, ALT		N	Mean	SD	CV%	Excluded
	All Analyzer	144	46.97	3.72	7.92	4
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	31	47.93	3.70	7.73	1
	Roche cobas c 311	27	45.76	2.41	5.27	--
	Fuji Dri-Chem 4000i	15	47.53	3.11	6.55	--
	Horiba ABX Pentra C200	12	49.66	3.01	6.06	--
	Roche cobas c 111	11	44.75	2.27	5.07	--
	Roche cobas c 111	10	45.22	1.72	3.81	--
	Roche cobas INTEGRA	9	45.93	3.95	8.59	--
	Roche cobas 6000	8	45.51	2.15	4.72	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Amylase, U/L

	N	Mean	SD	CV%	Excluded
All Methods	87	180.64	21.14	11.70	3
G7 PNP	64	180.36	11.74	6.51	2
RANDOX RX daytona	1	--	--	--	--

Your Result	194.00	SDI / z-Score	1.02
Assigned Value	176.12	Average SDI	1.04
SDPA	17.612	Uncertainty of AV	1.55
Standard Unit Result Val	194.00	%DEV	7.57

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

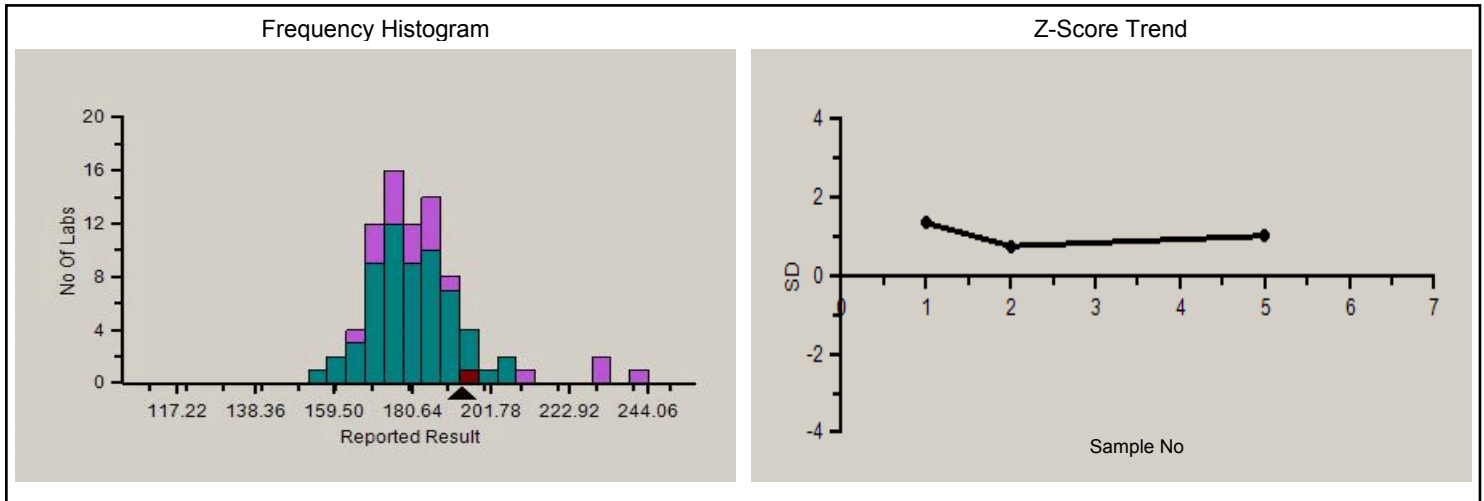

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, Amylase		N	Mean	SD	CV%	Excluded
	All Analyzer	87	180.64	21.14	11.70	3
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	22	182.50	14.55	7.97	1
	Fuji Dri-Chem 4000i	14	184.93	7.03	3.80	--
	Roche cobas c 311	13	174.41	7.72	4.43	--
	Roche cobas INTEGRA	7	178.57	4.78	2.68	--
	Roche cobas 6000	6	171.93	6.53	3.80	--
	Roche cobas 8000	4	168.75	3.95	2.34	--
	Roche cobas c 111	3	184.00	11.39	6.19	--
	Horiba ABX Pentra C200	2	193.15	--	--	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, AST, U/L

	N	Mean	SD	CV%	Excluded
All Methods	143	94.40	5.54	5.87	6
IFCC - UV without P5P	11	98.77	4.93	4.99	--
RANDOX RX daytona	1	--	--	--	--

Your Result	93.00	SDI / z-Score	-0.05
Assigned Value	93.61	Average SDI	-0.24
SDPA	11.233	Uncertainty of AV	0.64
Standard Unit Result Val	93.00	%DEV	-5.84

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

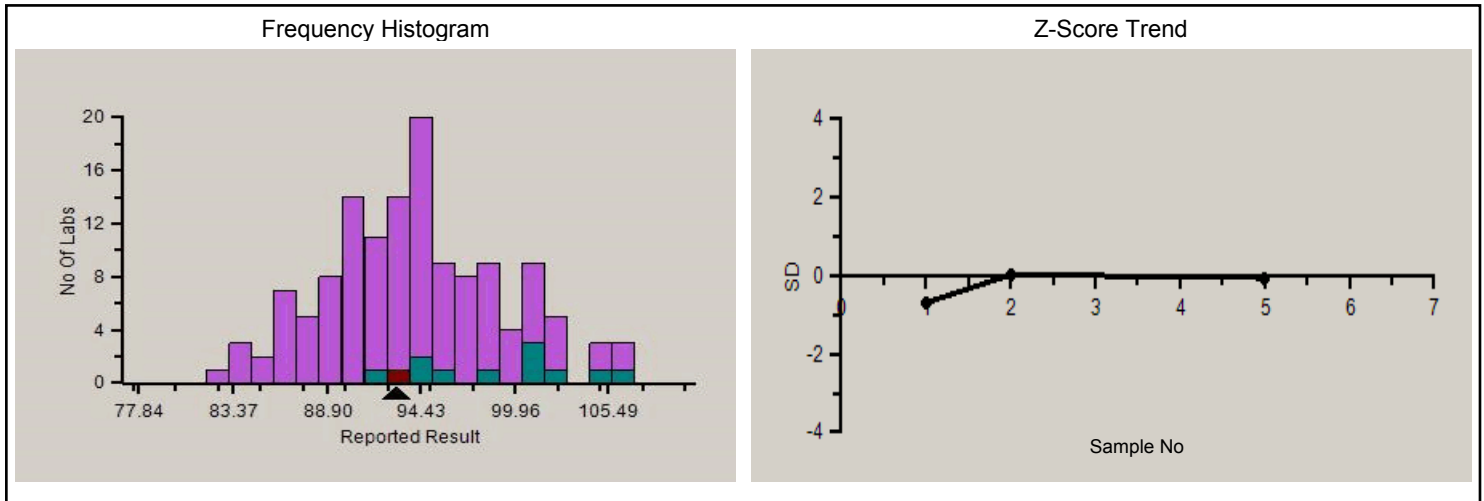

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, AST		N	Mean	SD	CV%	Excluded
	All Analyzer	143	94.40	5.54	5.87	6
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	32	94.40	5.84	6.19	2
	Roche cobas c 311	26	93.50	3.40	3.64	--
	Fuji Dri-Chem 4000i	15	91.53	4.00	4.37	--
	Roche cobas c 111	12	91.63	4.03	4.40	--
	Roche cobas c 111	11	91.04	3.63	3.99	--
	Horiba ABX Pentra C200	10	96.87	5.97	6.17	1
	Roche cobas INTEGRA	9	92.68	3.90	4.21	1
	Roche cobas 6000	8	93.26	4.69	5.03	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Bilirubin Direct, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	139	0.92	0.13	13.64	16
■ DMSO	1	--	--	--	--
■ RANDOX RX daytona	1	--	--	--	--

Your Result	0.69	SDI / z-Score	-1.32
Assigned Value	0.94	Average SDI	0.99
SDPA	0.188	Uncertainty of AV	0.02
Standard Unit Result Val	0.69	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

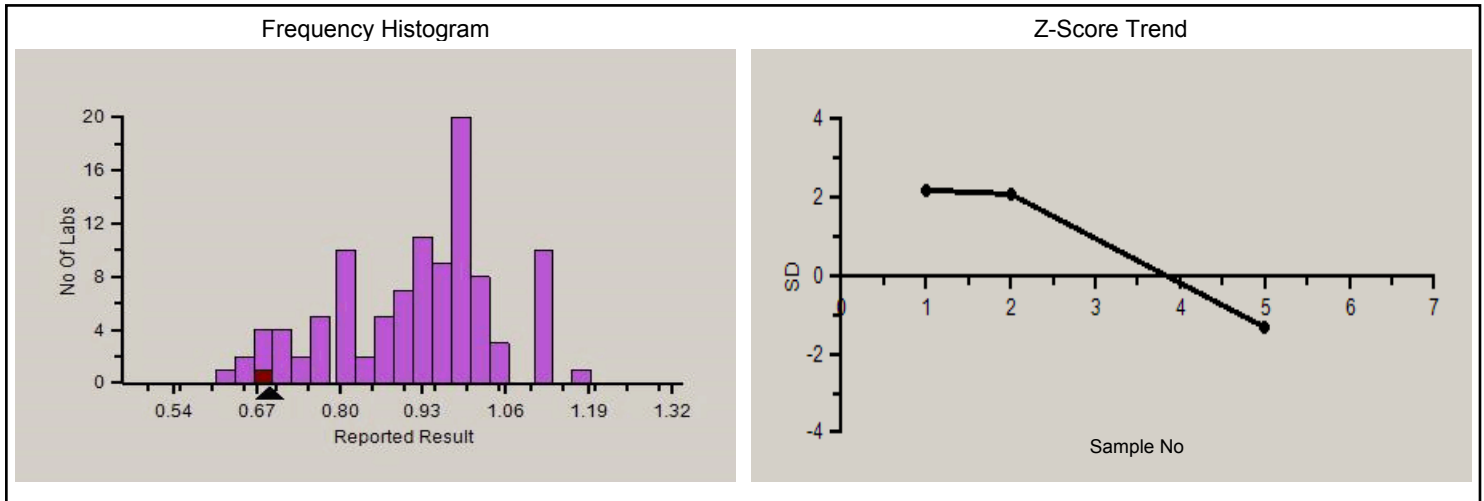

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, Bilirubin Direct		N	Mean	SD	CV%	Excluded
	All Analyzer	139	0.92	0.13	13.64	16
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	28	0.97	0.08	8.56	1
	Roche cobas c 311	26	0.94	0.11	11.24	1
	Fuji Dri-Chem 4000i	15	0.99	0.05	4.63	--
	Horiba ABX Pentra C200	11	0.75	0.07	8.98	1
	Roche cobas c 111	11	1.03	0.09	8.22	2
	Roche cobas c 111	10	1.04	0.09	8.67	2
	Roche cobas INTEGRA	9	0.90	0.08	8.56	--
	Roche cobas 6000	8	0.95	0.07	7.26	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Bilirubin Total, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	142	1.92	0.17	8.66	8
DMSO	1	--	--	--	--
RANDOX RX daytona	1	--	--	--	--

Your Result	2.33	SDI / z-Score	0.93
Assigned Value	2.16	Average SDI	1.97
SDPA	0.182	Uncertainty of AV	0.07
Standard Unit Result Val	2.33	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

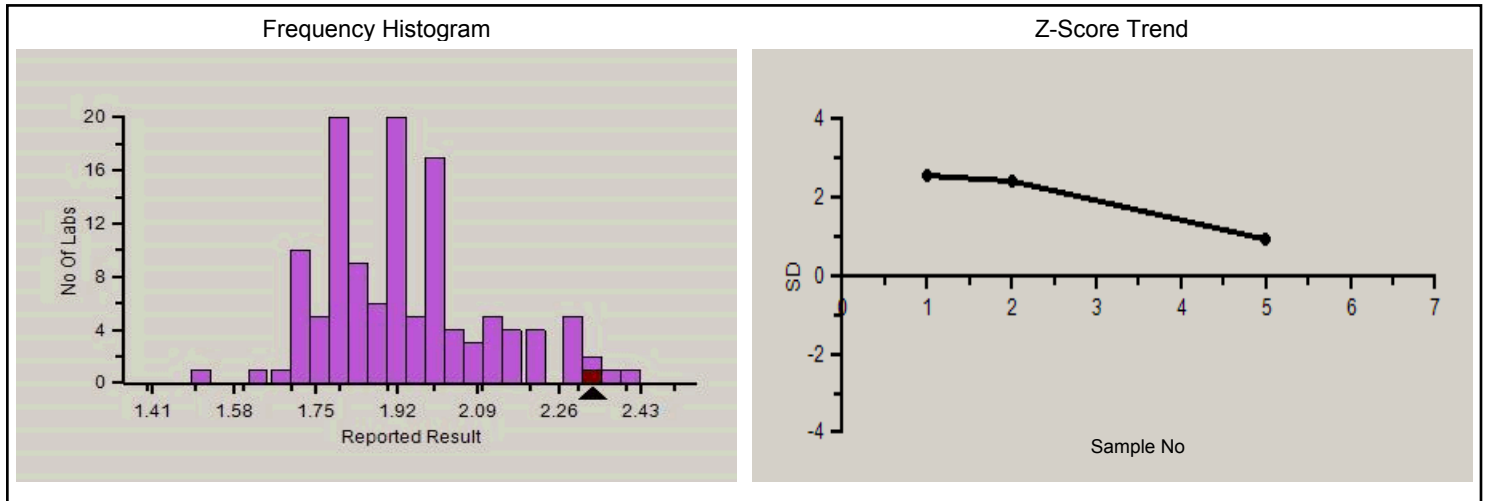

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, Bilirubin Total		N	Mean	SD	CV%	Excluded
	All Analyzer	142	1.92	0.17	8.66	8
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	29	1.83	0.13	7.25	2
	Roche cobas c 311	27	1.87	0.11	6.03	2
	Fuji Dri-Chem 4000i	15	1.87	0.11	5.62	--
	Horiba ABX Pentra C200	11	2.05	0.11	5.32	2
	Roche cobas c 111	10	1.99	0.20	10.20	--
	Roche cobas c 111	9	1.95	0.15	7.81	--
	Roche cobas INTEGRA	9	1.86	0.13	6.72	--
	Roche cobas 6000	8	1.83	0.09	5.08	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Calcium, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	131	5.77	0.34	5.91	10
Arsenazo III	34	5.81	0.41	7.10	6
RANDOX RX daytona	1	--	--	--	--

Your Result	5.60	SDI / z-Score	-0.44
Assigned Value	5.81	Average SDI	-0.29
SDPA	0.464	Uncertainty of AV	0.04
Standard Unit Result Val	5.60	%DEV	-3.55

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

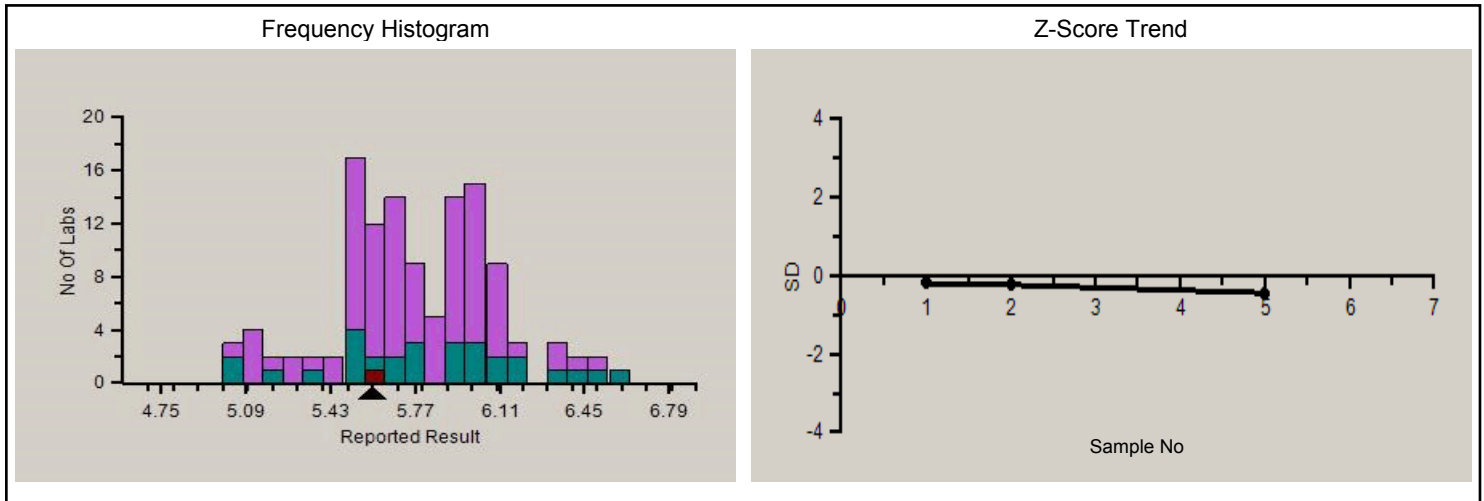

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, Calcium		N	Mean	SD	CV%	Excluded
	All Analyzer	131	5.77	0.34	5.91	10
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	27	5.61	0.34	6.00	2
	Roche cobas c 311	24	5.87	0.23	3.83	--
	Fuji Dri-Chem 4000i	15	5.64	0.29	5.14	--
	Roche cobas c 111	10	5.87	0.30	5.13	--
	Roche cobas INTEGRA	10	5.78	0.35	6.08	--
	Roche cobas c 111	9	5.84	0.31	5.27	--
	Roche cobas 6000	7	5.85	0.15	2.62	--
	Beckman Coulter AU480	5	5.77	0.21	3.55	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, CK, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	70	246.71	39.40	15.97	3
■ Colorimetric	1	--	--	--	--
■ Fuji Nx 700	3	278.00	33.96	12.21	--

Your Result	255.00	SDI / z-Score	-1.26
Assigned Value	282.95	Average SDI	0.05
SDPA	22.154	Uncertainty of AV	4.82
Standard Unit Result Val	255.00	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

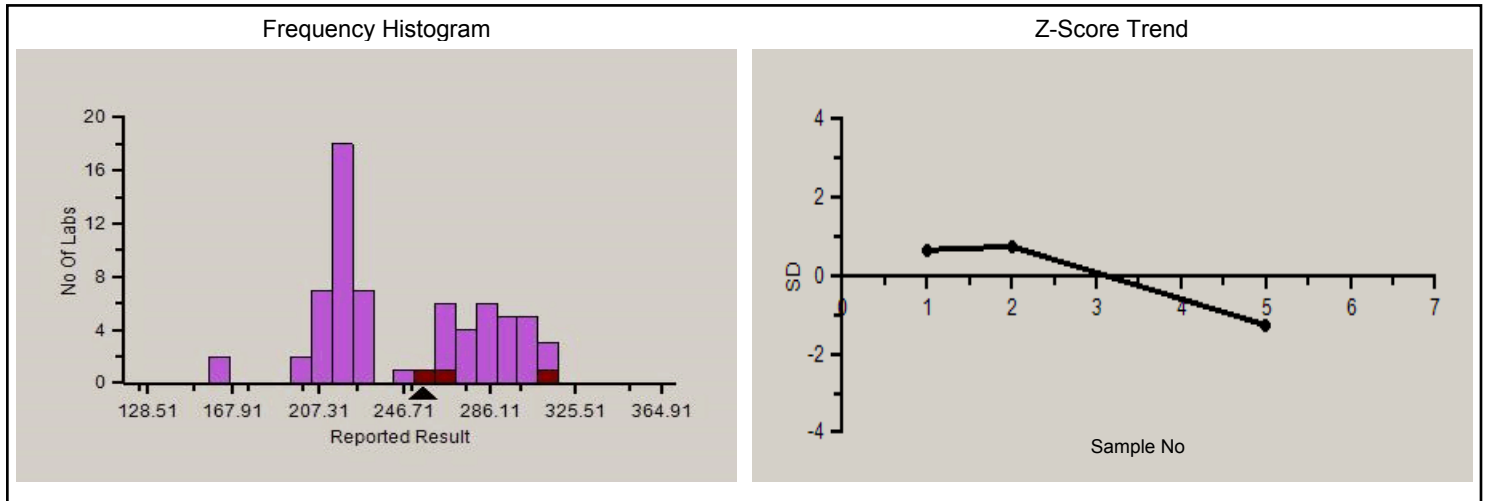

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, CK		N	Mean	SD	CV%	Excluded
	All Analyzer	70	246.71	39.40	15.97	3
Your Analyzer :	Fuji Nx 700	3	278.00	33.96	12.21	--
	Fuji Dri-Chem NX500/i	20	278.05	24.73	8.89	1
	Roche cobas c 311	12	219.54	6.09	2.77	--
	Fuji Dri-Chem 4000i	11	285.36	24.73	8.67	--
	Roche cobas INTEGRA	7	220.34	13.16	5.97	--
	Roche cobas 6000	5	215.44	8.49	3.94	--
	Roche cobas 8000	4	213.75	4.19	1.96	--
	Beckman Coulter AU480	1	--	--	--	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Creatinine, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	140	2.53	0.19	7.52	4
Ammonia Concentration Measurement - color change of BPB	42	2.39	0.12	4.98	2
Fuji Nx 700	1	--	--	--	--

Your Result	2.24	SDI / z-Score	-0.83
Assigned Value	2.38	Average SDI	1.23
SDPA	0.166	Uncertainty of AV	0.02
Standard Unit Result Val	2.24	%DEV	-6.20

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

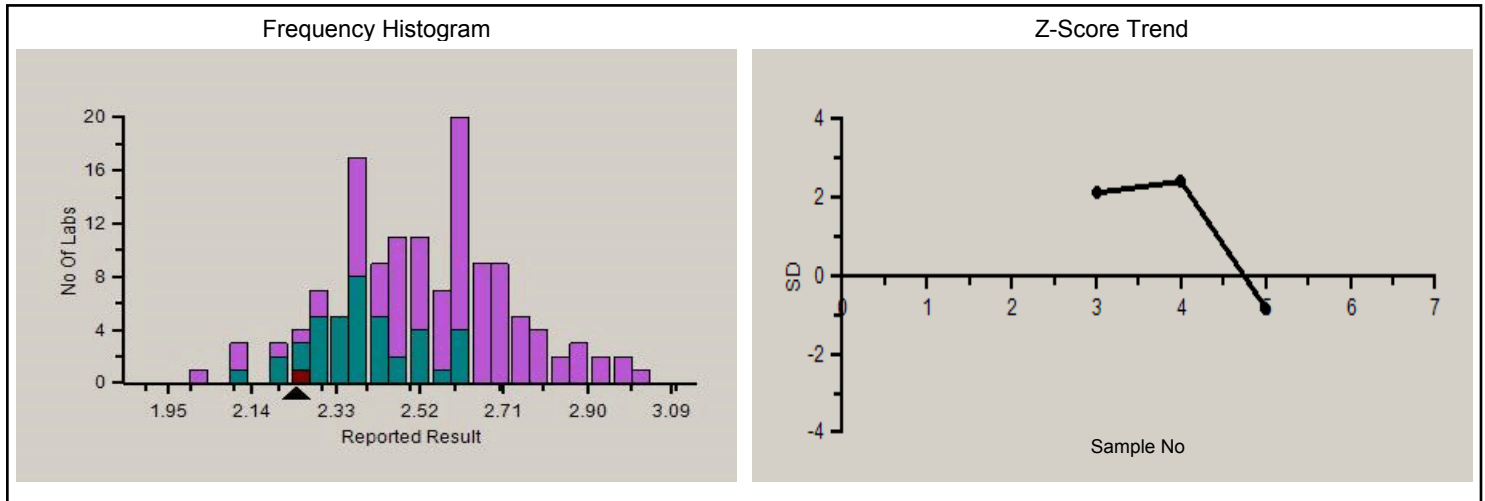

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, Creatinine		N	Mean	SD	CV%	Excluded
	All Analyzer	140	2.53	0.19	7.52	4
Your Analyzer :	Fuji Nx 700	1	--	--	--	--
	Fuji Dri-Chem NX500/i	28	2.38	0.11	4.71	2
	Roche cobas c 311	27	2.62	0.13	4.85	--
	Fuji Dri-Chem 4000i	15	2.39	0.12	5.11	1
	Horiba ABX Pentra C200	11	2.57	0.26	10.05	--
	Roche cobas c 111	11	2.55	0.18	7.03	--
	Roche cobas c 111	10	2.59	0.11	4.09	--
	Roche cobas INTEGRA	9	2.48	0.21	8.31	--
	Roche cobas 6000	8	2.60	0.11	4.38	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, GGT, U/L

	N	Mean	SD	CV%	Excluded
All Methods	123	90.79	16.32	17.97	6
IFCC	11	87.93	12.58	14.31	--
RANDOX RX daytona	1	--	--	--	--

Your Result	84.00	SDI / z-Score	0.53
Assigned Value	78.58	Average SDI	0.88
SDPA	10.215	Uncertainty of AV	0.65
Standard Unit Result Val	84.00	%DEV	-4.47

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

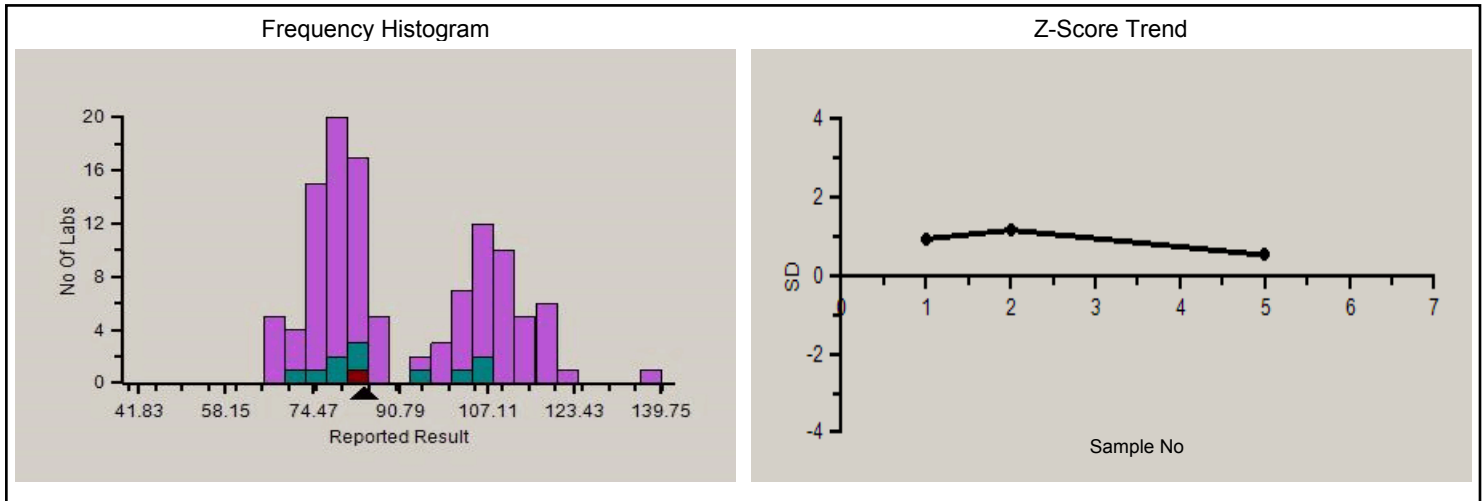

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021

Biochemistry, GGT		N	Mean	SD	CV%	Excluded
	All Analyzer	123	90.79	16.32	17.97	6
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	30	108.66	10.52	9.68	1
	Roche cobas c 311	24	78.70	4.47	5.68	1
	Fuji Dri-Chem 4000i	12	107.67	4.44	4.12	--
	Roche cobas INTEGRA	10	78.46	5.14	6.55	--
	Roche cobas c 111	9	80.35	5.89	7.34	1
	Horiba ABX Pentra C200	6	78.34	4.74	6.05	1
	Roche cobas 6000	6	77.83	3.55	4.56	--
	Beckman Coulter AU480	5	78.10	2.29	2.93	1

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Glucose, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	143	133.24	6.91	5.19	8
GOD-PAP	4	135.25	6.80	5.03	--
RANDOX RX daytona	1	--	--	--	--

Your Result	142.00	SDI / z-Score	0.61
Assigned Value	134.61	Average SDI	0.10
SDPA	12.115	Uncertainty of AV	0.92
Standard Unit Result Val	142.00	%DEV	4.99

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

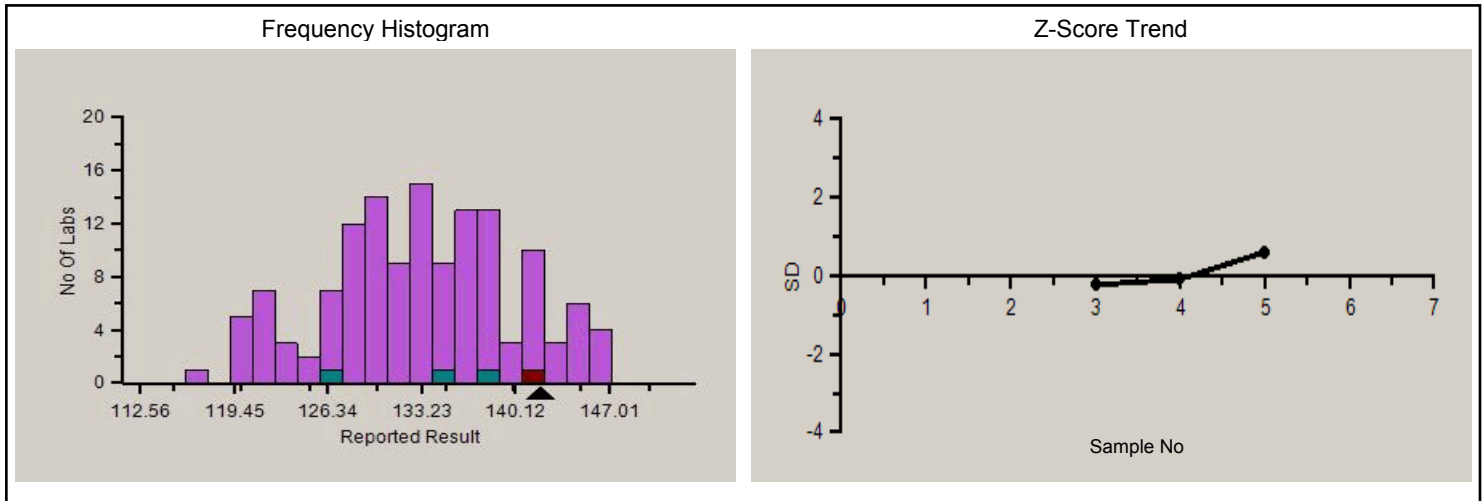

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, Glucose		N	Mean	SD	CV%	Excluded
	All Analyzer	143	133.24	6.91	5.19	8
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	30	131.57	7.66	5.82	2
	Roche cobas c 311	27	133.56	6.08	4.55	3
	Fuji Dri-Chem 4000i	15	130.60	5.72	4.38	--
	Horiba ABX Pentra C200	12	131.57	7.56	5.75	--
	Roche cobas c 111	10	136.47	4.44	3.25	1
	Roche cobas c 111	9	137.03	4.40	3.21	1
	Roche cobas INTEGRA	9	134.88	6.60	4.89	--
	Roche cobas 6000	8	135.25	4.37	3.23	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, LDH, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	81	194.07	49.12	25.31	10
■ L to P - IFCC Ref. Proc., Calibrated	2	139.00	--	--	1
■ Fuji Nx 700	3	156.00	18.68	11.98	--

Your Result	139.00	SDI / z-Score	-1.25
Assigned Value	168.36	Average SDI	-0.67
SDPA	23.570	Uncertainty of AV	2.78
Standard Unit Result Val	139.00	%DEV	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

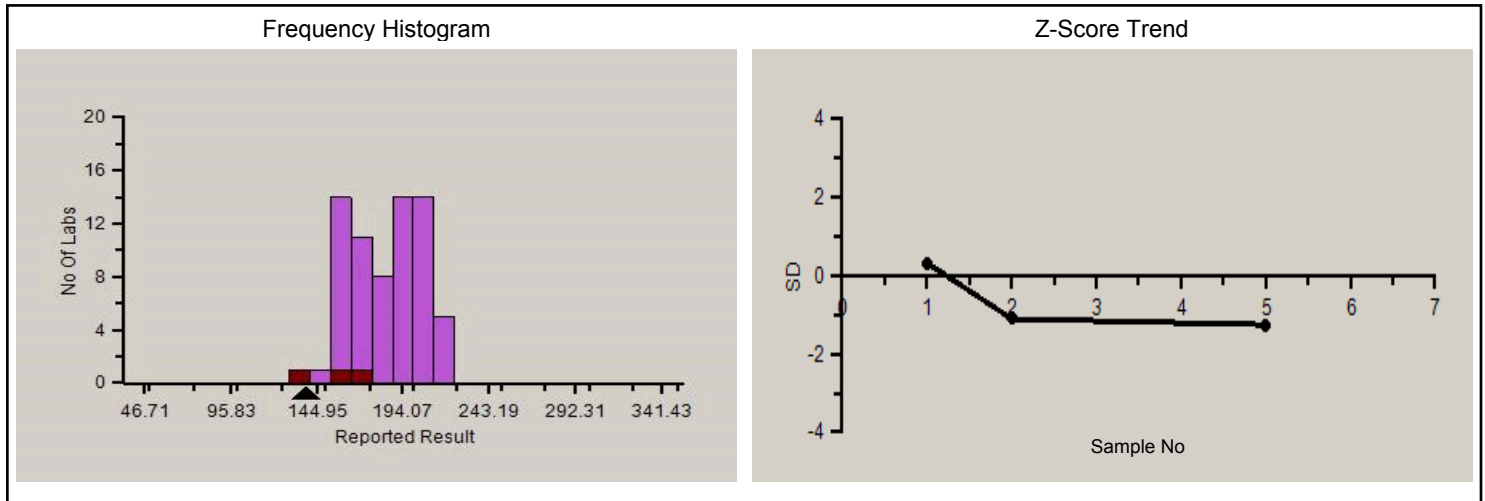

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, LDH		N	Mean	SD	CV%	Excluded
	All Analyzer	81	194.07	49.12	25.31	10
Your Analyzer :	Fuji Nx 700	3	156.00	18.68	11.98	--
	Fuji Dri-Chem NX500/i	22	168.45	10.07	5.98	2
	Fuji Dri-Chem 4000i	12	170.75	13.59	7.96	--
	Roche cobas c 311	10	201.50	6.31	3.13	--
	Roche cobas INTEGRA	7	209.65	9.68	4.62	--
	Roche cobas 6000	6	206.00	9.80	4.76	--
	Roche cobas 8000	4	199.50	6.86	3.44	--
	Beckman Coulter AU480	3	187.60	15.25	8.13	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Lipase, U/L

	N	Mean	SD	CV%	Excluded
All Methods	71	49.91	43.79	87.75	4
Enzymatic colorimetric	12	41.08	12.56	30.57	1
Fuji Nx 700	3	52.33	5.13	9.81	--

Your Result	48.00	SDI / z-Score	-0.88
Assigned Value	54.24	Average SDI	-0.41
SDPA	7.051	Uncertainty of AV	0.75
Standard Unit Result Val	48.00	%DEV	16.84

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

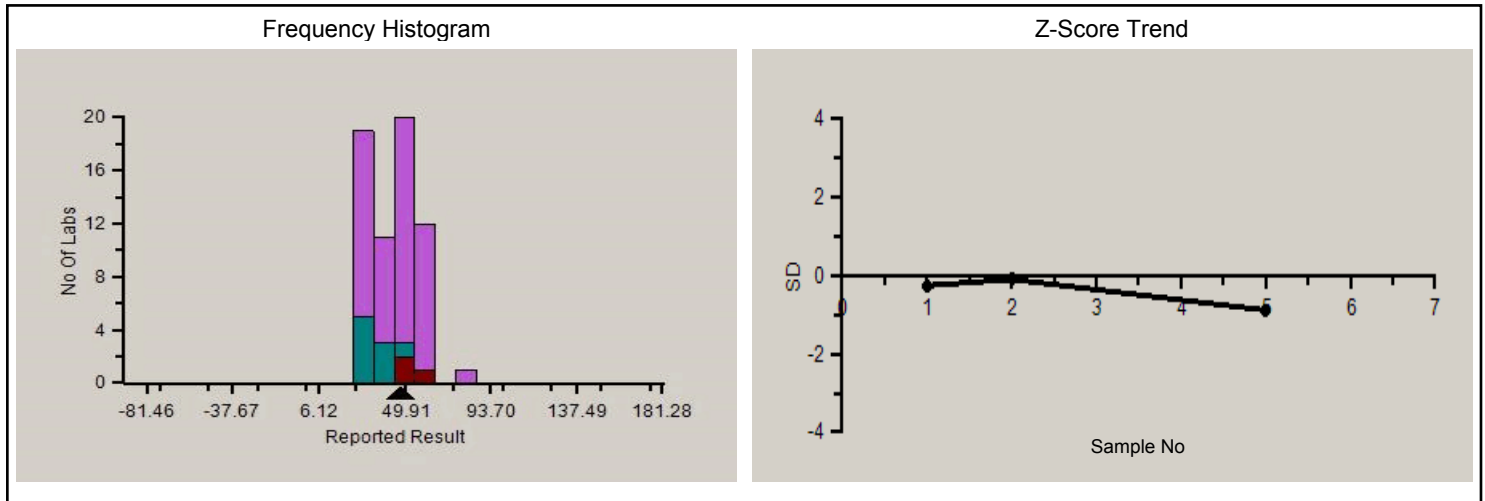

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, Lipase		N	Mean	SD	CV%	Excluded
	All Analyzer	71	49.91	43.79	87.75	4
Your Analyzer :	Fuji Nx 700	3	52.33	5.13	9.81	--
	Fuji Dri-Chem NX500/i	19	54.63	4.81	8.80	1
	Fuji Dri-Chem 4000i	14	54.79	2.26	4.12	--
	Roche cobas c 311	11	33.52	5.45	16.25	1
	Roche cobas INTEGRA	6	32.00	2.93	9.15	1
	Roche cobas 6000	5	33.22	4.10	12.35	--
	Roche cobas 8000	3	32.14	4.54	14.11	--
	Roche cobas c 111	3	32.25	4.60	14.25	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Magnesium, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	53	2.04	0.16	7.73	6
■ Enzymatic	2	1.85	--	--	--
■ Fuji Nx 700	2	1.85	--	--	--

Your Result	1.90	SDI / z-Score	-0.44
Assigned Value	2.01	Average SDI	-0.15
SDPA	0.262	Uncertainty of AV	0.05
Standard Unit Result Val	1.90	%DEV	2.70

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

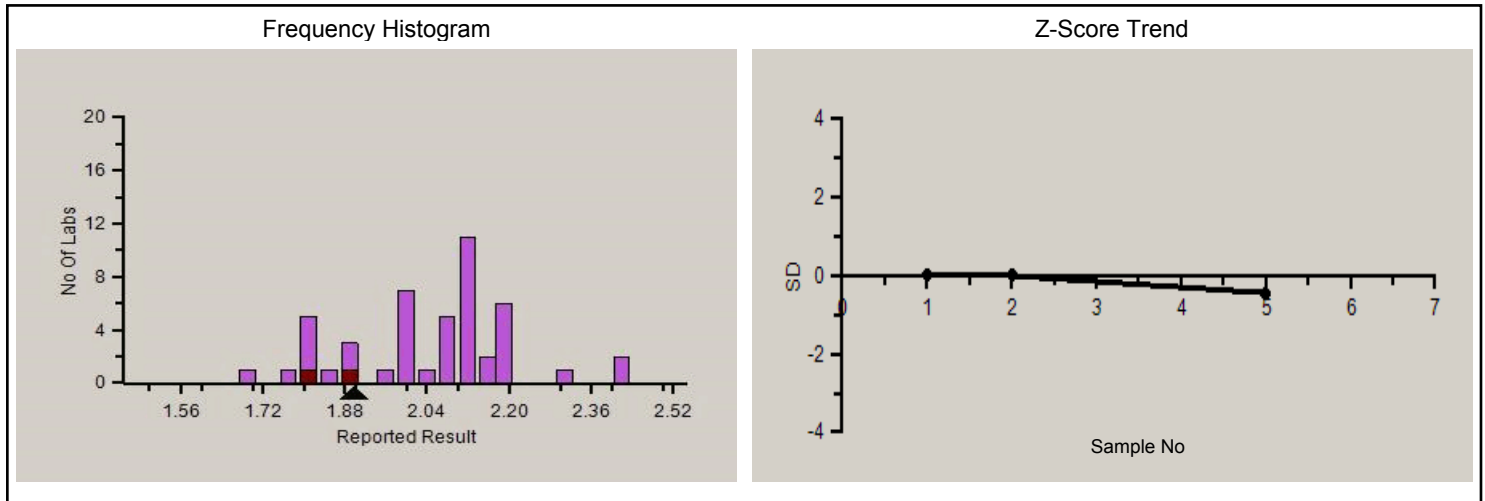

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, Magnesium		N	Mean	SD	CV%	Excluded
	All Analyzer	53	2.04	0.16	7.73	6
Your Analyzer :	Fuji Nx 700	2	1.85	--	--	--
	Fuji Dri-Chem NX500/i	16	2.04	0.20	9.55	2
	Fuji Dri-Chem 4000i	10	2.03	0.18	8.72	--
	Roche cobas c 311	7	2.10	0.08	4.01	--
	Roche cobas 6000	6	2.07	0.08	4.01	1
	Roche cobas 8000	4	2.11	0.08	3.98	--
	Roche cobas INTEGRA	2	2.02	--	--	1
	Beckman Coulter AU5800	1	--	--	--	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Phosphorous Inorganic, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	110	3.88	0.39	10.03	6
Phosphomolybdate method	57	3.63	0.23	6.25	3
RANDOX RX daytona	1	--	--	--	--

Your Result	3.50	SDI / z-Score	-0.33
Assigned Value	3.62	Average SDI	0.17
SDPA	0.362	Uncertainty of AV	0.03
Standard Unit Result Val	3.50	%DEV	-3.66

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

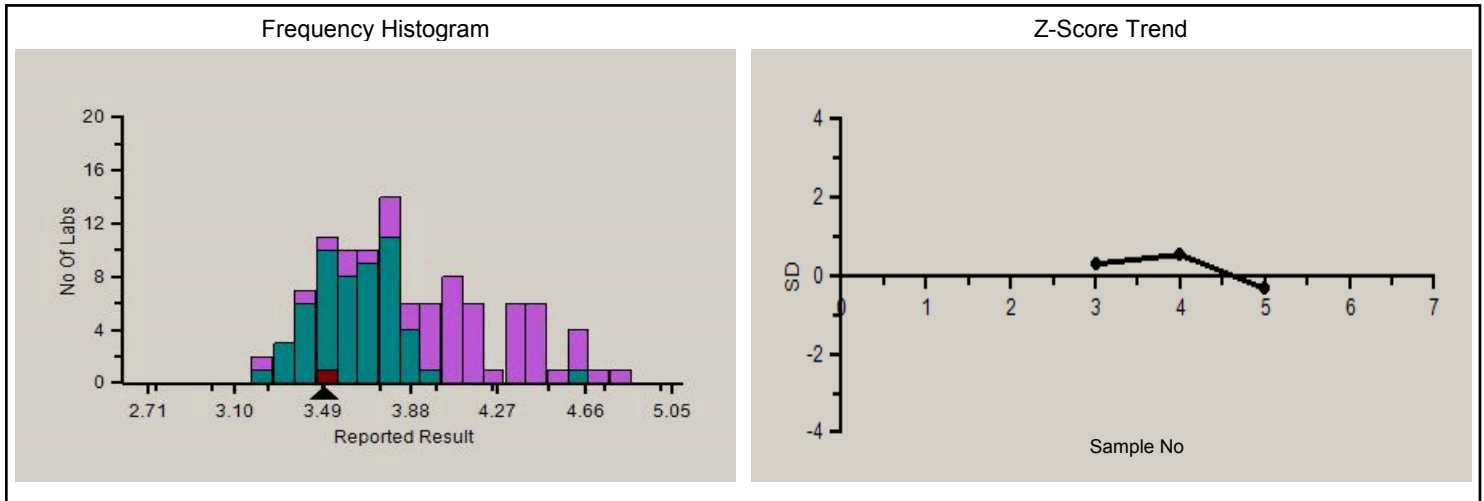

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 5
 Sample Date : 03-03-2021

Biochemistry, Phosphorous Inorganic		N	Mean	SD	CV%	Excluded
	All Analyzer	110	3.88	0.39	10.03	6
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Fuji Dri-Chem NX500/i	26	4.24	0.32	7.55	3
	Roche cobas c 311	22	3.64	0.19	5.19	--
	Fuji Dri-Chem 4000i	13	4.22	0.23	5.39	--
	Roche cobas 6000	8	3.54	0.18	5.00	--
	Roche cobas INTEGRA	7	3.66	0.17	4.72	--
	Roche cobas c 111	6	3.89	0.38	9.69	--
	Roche cobas 8000	4	3.55	0.22	6.11	--
	Beckman Coulter AU480	3	3.59	0.04	0.98	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021


Biochemistry, Urea, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	137	47.62	2.79	5.85	7
Urease, GLDH	16	47.56	4.02	8.45	--
RANDOX RX daytona	1	--	--	--	--

Your Result	50.00	SDI / z-Score	0.76
Assigned Value	47.76	Average SDI	1.07
SDPA	2.952	Uncertainty of AV	0.39
Standard Unit Result Val	50.00	%DEV	5.13

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

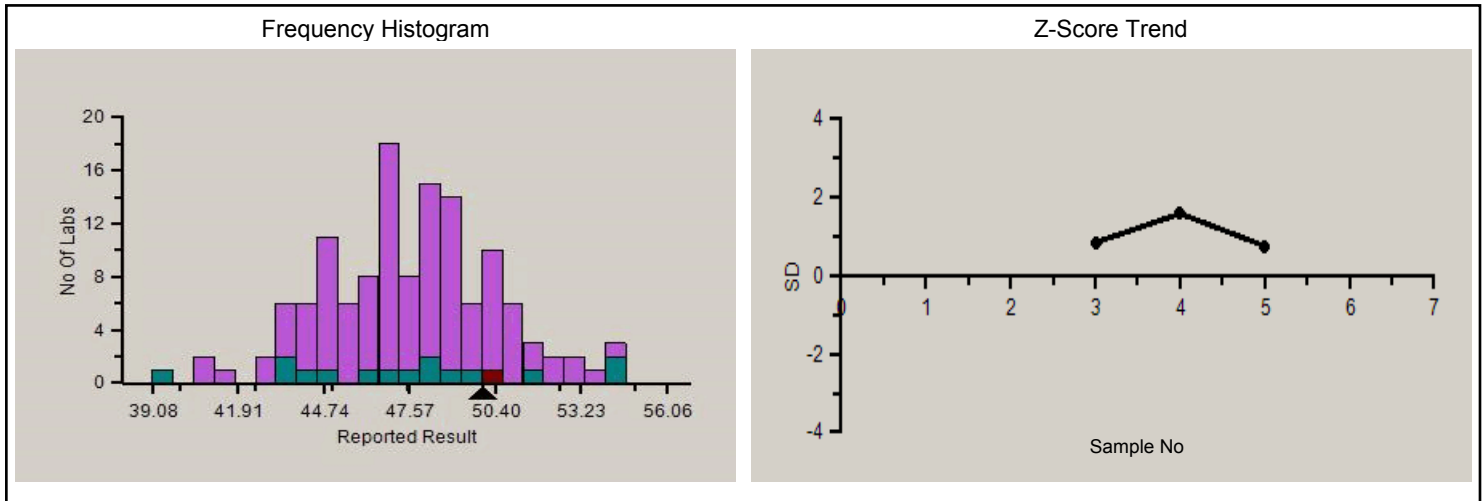

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 5
Sample Date : 03-03-2021

Biochemistry, Urea		N	Mean	SD	CV%	Excluded
	All Analyzer	137	47.62	2.79	5.85	7
Your Analyzer :	RANDOX RX daytona	1	--	--	--	--
	Roche cobas c 311	27	49.40	1.50	3.04	--
	Fuji Dri-Chem NX500/i	25	47.59	2.18	4.57	4
	Fuji Dri-Chem 4000i	15	47.00	2.38	5.06	1
	Horiba ABX Pentra C200	12	45.25	4.30	9.50	--
	Roche cobas c 111	11	46.00	2.40	5.21	--
	Roche cobas c 111	10	46.50	1.83	3.93	--
	Roche cobas INTEGRA	9	45.40	1.39	3.05	--
	Roche cobas 6000	8	48.54	3.03	6.24	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS

Unit No. 409-416.
Commercial Building - 1A,
Kohinoor Mall, Kirool Road, Kuria (W),
Mumbai - 400070



PC-1022

Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021


HbA1C, HbA1c, %

	N	Mean	SD	CV%	Excluded
■ All Methods	48	8.01	0.83	10.35	1
■ Ion Exchange HPLC	30	8.22	0.30	3.65	1
■ Biorad D-10	25	7.92	0.37	4.63	--

Your Result	7.50	SDI / z-Score	-1.27
Assigned Value	7.96	Average SDI	-1.52
SDPA	0.362	Uncertainty of AV	0.09
Standard Unit Result Val	7.50	%DEV	-5.35

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

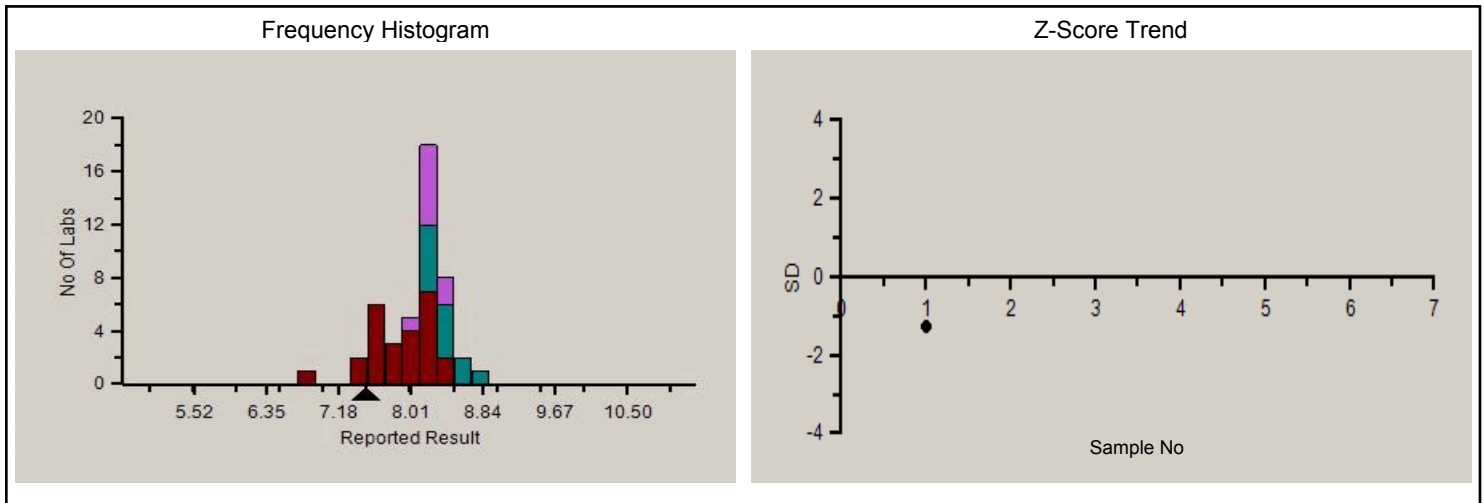

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

HbA1C, HbA1c		N	Mean	SD	CV%	Excluded
	All Analyzer	48	8.01	0.83	10.35	1
Your Analyzer :	Biorad D-10	25	7.92	0.37	4.63	--
	Tosoh G8 Auto HPLC	14	8.40	0.18	2.19	--
	Tosoh HLC 723 GX	7	8.25	0.16	1.99	1
	Mispa i2	1	--	--	--	--
	Biorad VII Turbo 2.0	1	--	--	--	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS

Unit No. 409-416.
 Commercial Building - 1A,
 Kohinoor Mall, Kirol Road, Kuria (W),
 Mumbai - 400070



PC-1022

Analyte Methodwise Result Report

Lab : 427
Lab Name : VINAMRA SWARAJ HOSPITAL
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


HbA1C, HbA1c, %

	N	Mean	SD	CV%	Excluded
All Methods	49	6.12	0.51	8.35	1
Ion Exchange HPLC	31	6.24	0.21	3.38	1
Biorad D-10	25	6.11	0.27	4.42	--

Your Result	5.60	SDI / z-Score	-1.76
Assigned Value	6.12	Average SDI	-1.52
SDPA	0.296	Uncertainty of AV	0.07
Standard Unit Result Val	5.60	%DEV	-8.38

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

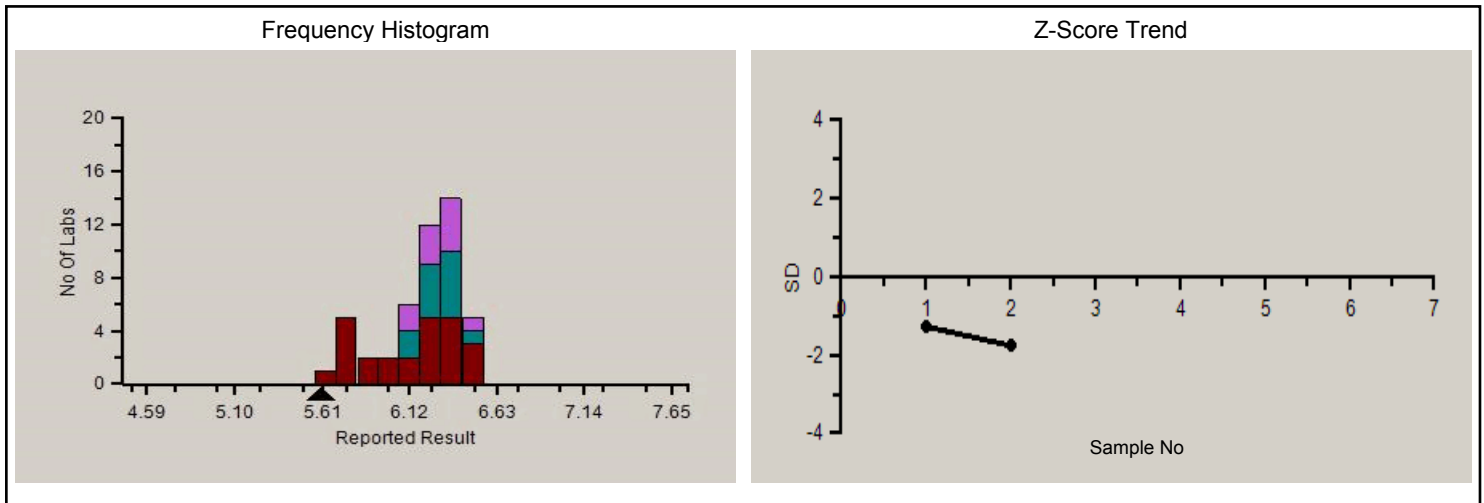

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 427
 Lab Name : VINAMRA SWARAJ HOSPITAL
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

HbA1C, HbA1c		N	Mean	SD	CV%	Excluded
	All Analyzer	49	6.12	0.51	8.35	1
Your Analyzer :	Biorad D-10	25	6.11	0.27	4.42	--
	Tosoh G8 Auto HPLC	14	6.30	0.14	2.24	--
	Tosoh HLC 723 GX	8	6.20	0.06	0.94	1
	Mispa i2	1	--	--	--	--
	Biorad VII Turbo 2.0	1	--	--	--	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS

Unit No. 409-416.
 Commercial Building - 1A,
 Kohinoor Mall, Kirol Road, Kuria (W),
 Mumbai - 400070



PC-1022

Certificate of Participation

Metropolis Healthcare Ltd. EQAS

Cycle 2020 – January to December

VINAMRA SWARAJ HOSPITAL

Lab ID: 427

Has successfully participated in Scheme for

- Clinical Biochemistry
- HbA1c
- Qualitative Immunoassay



Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam

PT Coordinator