

Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, ALT, U/L

	N	Mean	SD	CV%	Excluded
All Methods	168	29.17	29.26	100.33	61
IFCC-Kinetic	7	22.33	4.98	22.29	3
Erba Chem 5/Plus	2	27.23	--	--	1

Your Result	11.85	SDI / z-Score	-2.45
Assigned Value	23.20	Average SDI	2.08
SDPA	4.640	Uncertainty of AV	1.51
Standard Unit Result Val	11.85	%DEV	-46.93

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

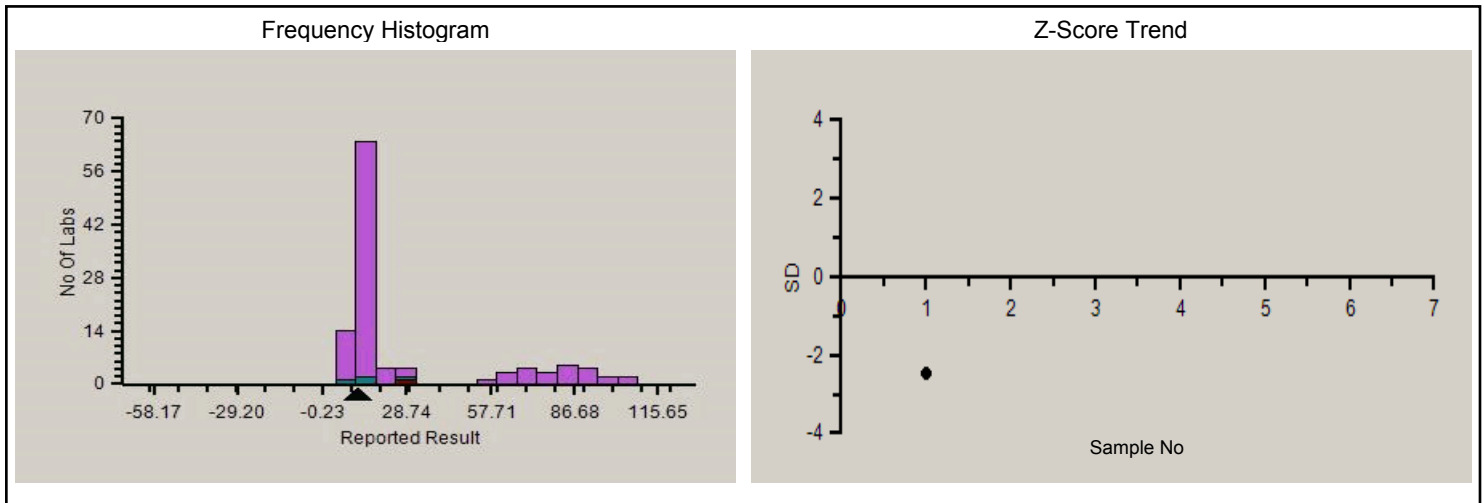

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
 Lab Name : SADBHAVANA PATHOLOGY LAB
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, ALT		N	Mean	SD	CV%	Excluded
	All Analyzer	168	29.17	29.26	100.33	61
Your Analyzer :	Erba Chem 5/Plus	2	27.23	--	--	1
	Fuji Dri-Chem NX500/i	30	87.00	12.62	14.51	18
	Roche cobas c 311	29	13.17	1.52	11.51	6
	Roche cobas c 311	28	13.02	1.36	10.46	6
	Fuji Dri-Chem 4000i	16	76.40	14.14	18.50	6
	Roche cobas c 111	12	13.25	1.65	12.42	1
	Horiba ABX Pentra C200	11	12.64	1.59	12.60	--
	Roche cobas c 111	11	13.25	1.65	12.42	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Bilirubin Direct, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	166	0.10	0.02	17.00	51
Diazotization	134	0.10	0.02	16.33	37
Erba Chem 5/Plus	2	--	--	--	2

Your Result	0.17	SDI / z-Score	1.72
Assigned Value	0.10	Average SDI	1.90
SDPA	0.043	Uncertainty of AV	0.01
Standard Unit Result Val	0.17	%DEV	73.47

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

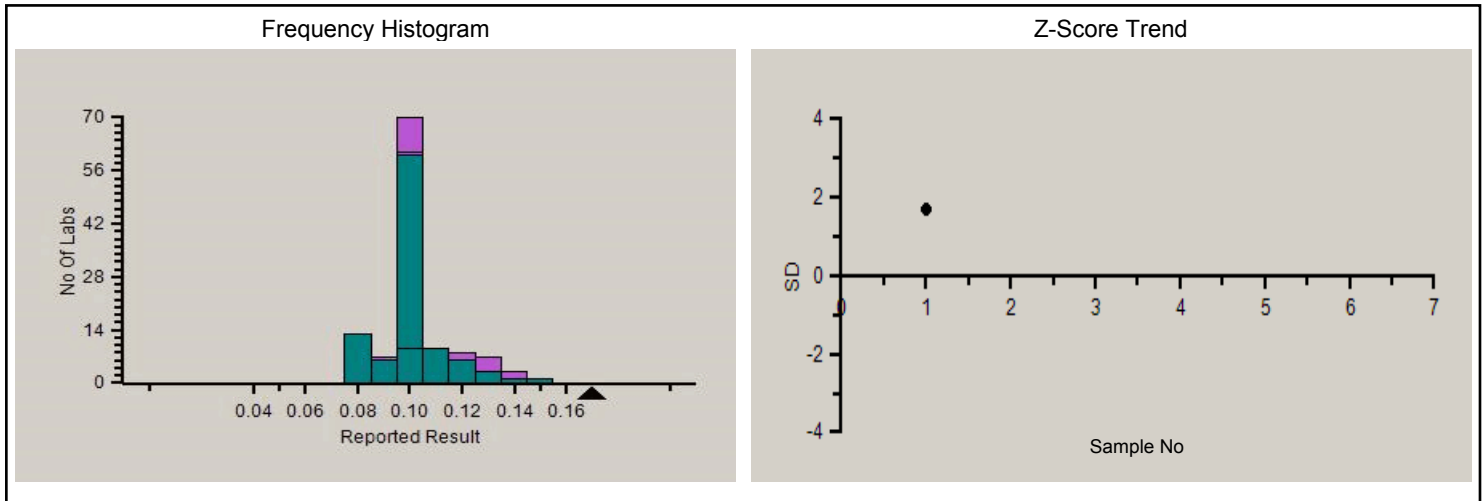

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
 Lab Name : SADBHAVANA PATHOLOGY LAB
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Bilirubin Direct		N	Mean	SD	CV%	Excluded
	All Analyzer	166	0.10	0.02	17.00	51
Your Analyzer :	Erba Chem 5/Plus	2	--	--	--	2
	Fuji Dri-Chem NX500/i	28	0.10	0.01	8.08	9
	Roche cobas c 311	28	0.09	0.02	19.15	5
	Roche cobas c 311	27	0.09	0.02	19.15	5
	Fuji Dri-Chem 4000i	16	0.10	0.00	0.00	9
	Roche cobas c 111	12	0.11	0.01	11.11	4
	Horiba ABX Pentra C200	11	0.12	0.02	13.91	--
	Roche cobas c 111	11	0.11	0.01	11.01	4

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Bilirubin Total, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	170	0.31	0.14	45.05	49
Diazotization	45	0.29	0.14	46.76	13
Erba Chem 5/Plus	2	0.31	--	--	--

Your Result	0.30	SDI / z-Score	-0.18
Assigned Value	0.32	Average SDI	-0.19
SDPA	0.095	Uncertainty of AV	0.02
Standard Unit Result Val	0.30	%DEV	2.39

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

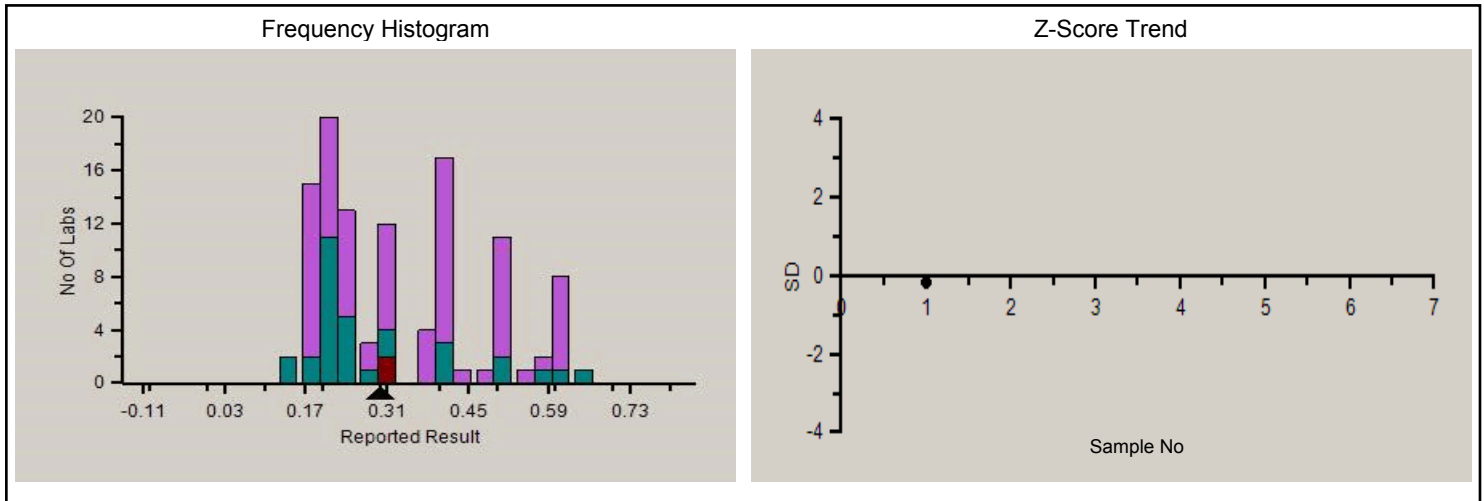

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
 Lab Name : SADBHAVANA PATHOLOGY LAB
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Bilirubin Total		N	Mean	SD	CV%	Excluded
	All Analyzer	170	0.31	0.14	45.05	49
Your Analyzer :	Erba Chem 5/Plus	2	0.31	--	--	--
	Fuji Dri-Chem NX500/i	30	0.47	0.08	16.24	6
	Roche cobas c 311	29	0.20	0.03	14.07	6
	Roche cobas c 311	28	0.20	0.03	14.50	6
	Fuji Dri-Chem 4000i	16	0.51	0.08	16.37	2
	Horiba ABX Pentra C200	11	0.22	0.03	11.26	6
	Roche cobas c 111	11	0.21	0.03	14.56	4
	Roche cobas c 111	10	0.20	0.03	15.76	4

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Calcium, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	157	7.64	0.53	6.92	11
■ Arsenazo III	53	7.85	0.47	6.00	7
■ Erba Chem 5/Plus	2	8.01	--	--	--

Your Result	7.51	SDI / z-Score	-1.09
Assigned Value	8.20	Average SDI	-1.16
SDPA	0.631	Uncertainty of AV	0.23
Standard Unit Result Val	7.51	%DEV	-4.33

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

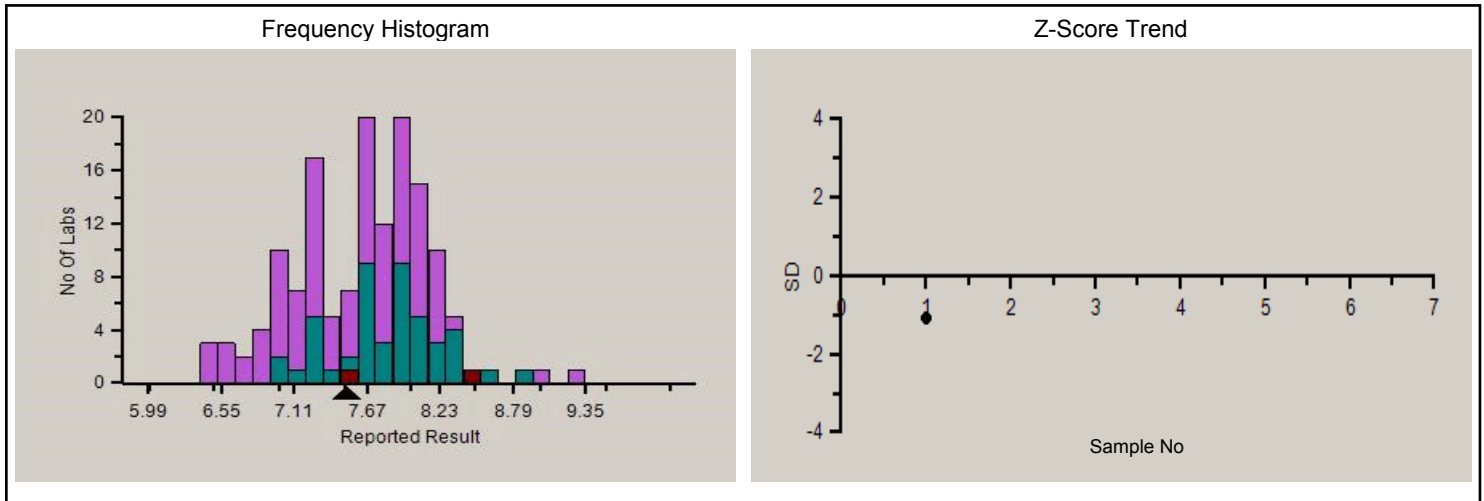

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
 Lab Name : SADBHAVANA PATHOLOGY LAB
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Calcium		N	Mean	SD	CV%	Excluded
	All Analyzer	157	7.64	0.53	6.92	11
Your Analyzer :	Erba Chem 5/Plus	2	8.01	--	--	--
	Fuji Dri-Chem NX500/i	28	7.00	0.31	4.43	--
	Roche cobas c 311	26	7.93	0.25	3.12	1
	Roche cobas c 311	25	7.92	0.25	3.18	1
	Fuji Dri-Chem 4000i	16	7.26	0.35	4.80	--
	Roche cobas c 111	11	7.91	0.34	4.32	1
	Roche cobas INTEGRA	11	7.76	0.31	3.99	--
	Roche cobas c 111	10	7.83	0.26	3.27	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Triglycerides, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	166	121.71	8.69	7.14	8
■ GPO-TOPS	3	122.85	6.01	4.89	1
■ Erba Chem 5/Plus	1	--	--	--	1

Your Result	83.99	SDI / z-Score	-2.84
Assigned Value	119.64	Average SDI	-2.87
SDPA	12.546	Uncertainty of AV	4.05
Standard Unit Result Val	83.99	%DEV	-31.63

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

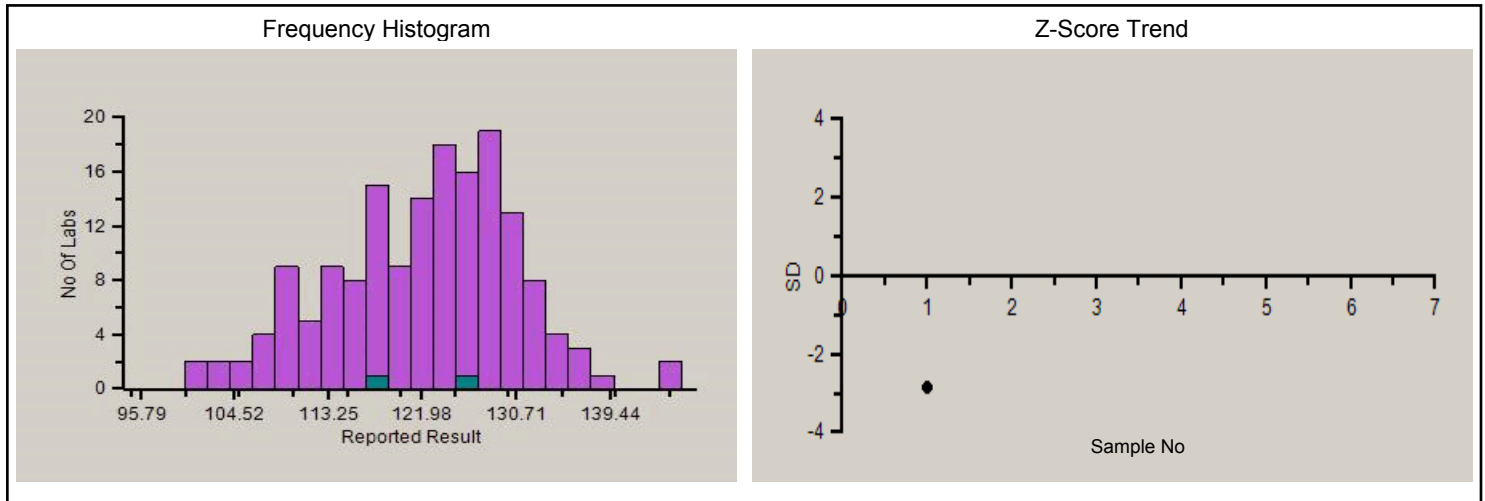

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
 Lab Name : SADBHAVANA PATHOLOGY LAB
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Biochemistry, Triglycerides		N	Mean	SD	CV%	Excluded
	All Analyzer	166	121.71	8.69	7.14	8
Your Analyzer :	Erba Chem 5/Plus	1	--	--	--	1
	Fuji Dri-Chem NX500/i	32	114.44	6.40	5.59	1
	Roche cobas c 311	29	127.35	6.16	4.84	--
	Roche cobas c 311	28	127.01	5.98	4.71	--
	Fuji Dri-Chem 4000i	16	114.19	7.31	6.40	--
	Roche cobas c 111	12	128.81	4.62	3.59	--
	Roche cobas c 111	11	128.25	4.39	3.43	--
	Horiba ABX Pentra C200	10	124.53	4.32	3.47	--
	Roche cobas INTEGRA	10	122.87	4.59	3.73	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Biochemistry, Uric Acid, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	168	4.18	0.35	8.30	10
■ Uricase-TOPS	2	3.77	--	--	--
■ Erba Chem 5/Plus	2	4.01	--	--	--

Your Result	4.00	SDI / z-Score	-0.32
Assigned Value	4.18	Average SDI	-0.63
SDPA	0.553	Uncertainty of AV	0.15
Standard Unit Result Val	4.00	%DEV	6.24

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

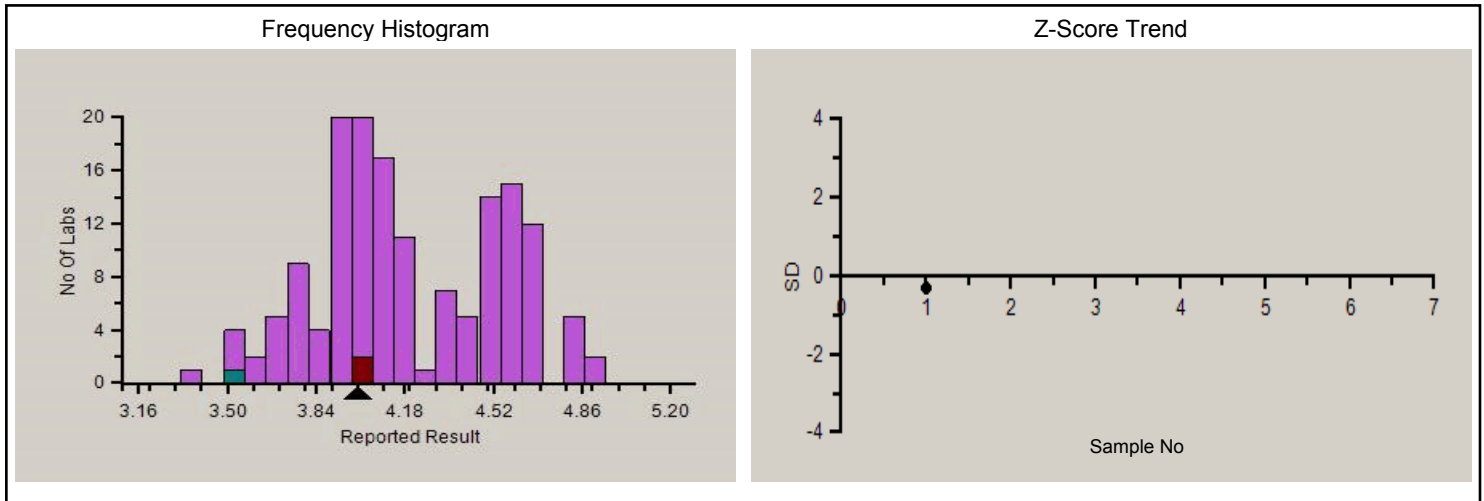

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Biochemistry, Uric Acid		N	Mean	SD	CV%	Excluded
	All Analyzer	168	4.18	0.35	8.30	10
Your Analyzer :	Erba Chem 5/Plus	2	4.01	--	--	--
	Fuji Dri-Chem NX500/i	31	4.52	0.20	4.33	1
	Roche cobas c 311	27	3.96	0.18	4.42	1
	Roche cobas c 311	26	3.95	0.17	4.35	1
	Fuji Dri-Chem 4000i	19	4.59	0.20	4.45	1
	Roche cobas c 111	12	4.02	0.17	4.15	--
	Roche cobas c 111	11	4.00	0.17	4.12	--
	Horiba ABX Pentra C200	10	3.96	0.09	2.35	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
Unit No. 409-416.
Commercial Building - 1A,
Kohinoor Mall, Kirool Road, Kuria (W),
Mumbai - 400070



PC-1022

Analyte Methodwise Result Report

Lab : 446
 Lab Name : SADBHAVANA PATHOLOGY LAB
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021


Biochemistry, ALT, U/L

	N	Mean	SD	CV%	Excluded
■ All Methods	170	14.49	5.73	39.56	35
■ IFCC-Kinetic	7	14.50	3.91	26.98	1
■ Erba Chem 5/Plus	2	13.79	--	--	1

Your Result	30.94	SDI / z-Score	6.61
Assigned Value	12.97	Average SDI	2.08
SDPA	2.720	Uncertainty of AV	0.50
Standard Unit Result Val	30.94	%DEV	113.34

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

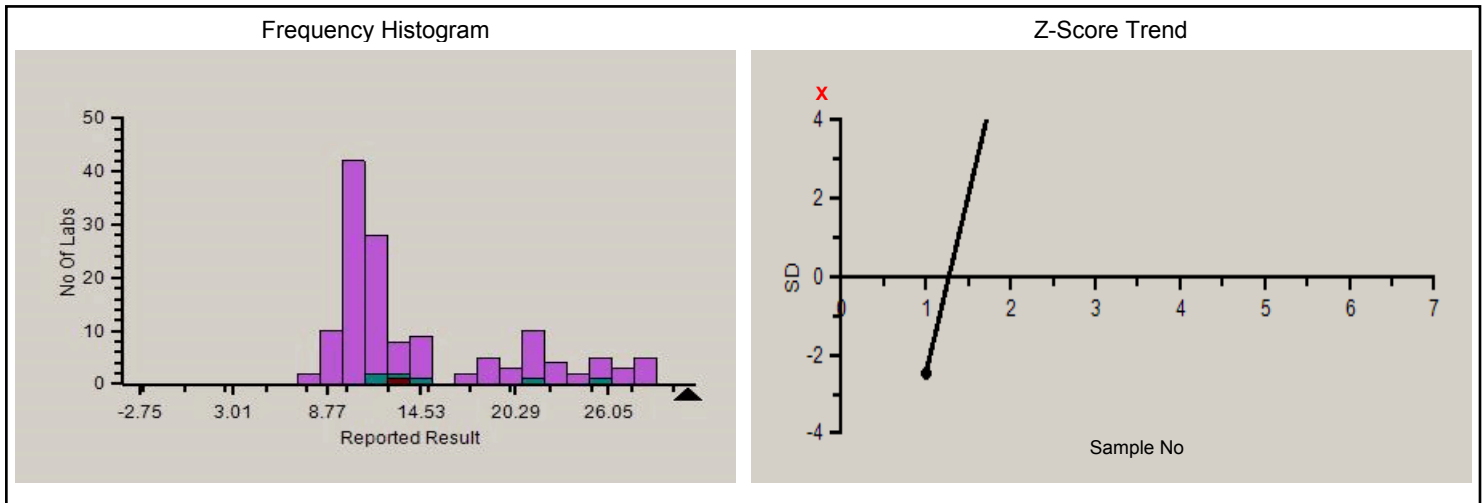

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
 Lab Name : SADBHAVANA PATHOLOGY LAB
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, ALT		N	Mean	SD	CV%	Excluded
	All Analyzer	170	14.49	5.73	39.56	35
Your Analyzer :	Erba Chem 5/Plus	2	13.79	--	--	1
	Fuji Dri-Chem NX500/i	32	23.11	3.35	14.49	11
	Roche cobas c 311	28	10.83	1.25	11.57	1
	Roche cobas c 311	27	10.81	1.27	11.77	1
	Fuji Dri-Chem 4000i	16	23.36	2.50	10.71	5
	Roche cobas c 111	12	10.09	1.24	12.30	2
	Horiba ABX Pentra C200	11	11.23	1.29	11.50	1
	Roche cobas c 111	11	10.09	1.24	12.30	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, Bilirubin Direct, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	164	0.10	0.02	15.53	39
■ Diazotization	132	0.10	0.01	14.00	26
■ Erba Chem 5/Plus	2	0.13	--	--	1

Your Result	0.19	SDI / z-Score	2.09
Assigned Value	0.10	Average SDI	1.90
SDPA	0.044	Uncertainty of AV	0.01
Standard Unit Result Val	0.19	%DEV	90.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

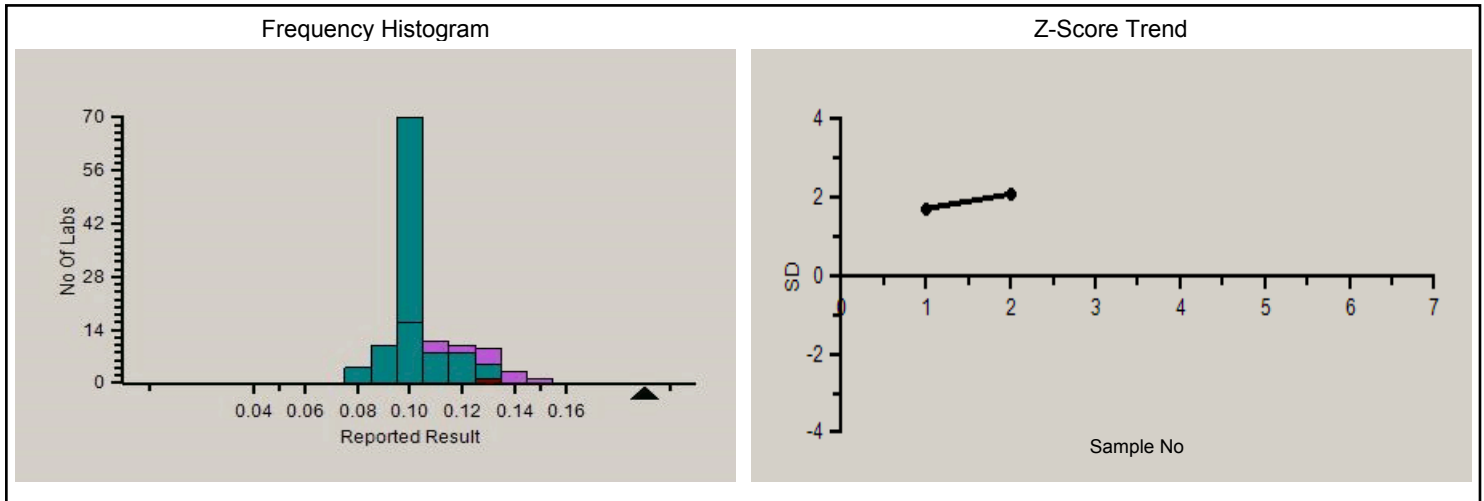

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
 Lab Name : SADBHAVANA PATHOLOGY LAB
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, Bilirubin Direct		N	Mean	SD	CV%	Excluded
	All Analyzer	164	0.10	0.02	15.53	39
Your Analyzer :	Erba Chem 5/Plus	2	0.13	--	--	1
	Fuji Dri-Chem NX500/i	28	0.10	0.00	4.04	8
	Roche cobas c 311	27	0.09	0.01	13.04	3
	Roche cobas c 311	26	0.09	0.01	13.19	3
	Fuji Dri-Chem 4000i	16	0.10	0.00	0.00	6
	Roche cobas c 111	12	0.11	0.01	11.82	3
	Horiba ABX Pentra C200	11	0.12	0.01	10.17	--
	Roche cobas c 111	11	0.11	0.01	12.73	3

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, Bilirubin Total, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	167	0.33	0.14	42.81	43
■ Diazotization	43	0.31	0.13	41.69	10
■ Erba Chem 5/Plus	2	0.33	--	--	--

Your Result	0.31	SDI / z-Score	-0.20
Assigned Value	0.33	Average SDI	-0.19
SDPA	0.099	Uncertainty of AV	0.02
Standard Unit Result Val	0.31	%DEV	0.98

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

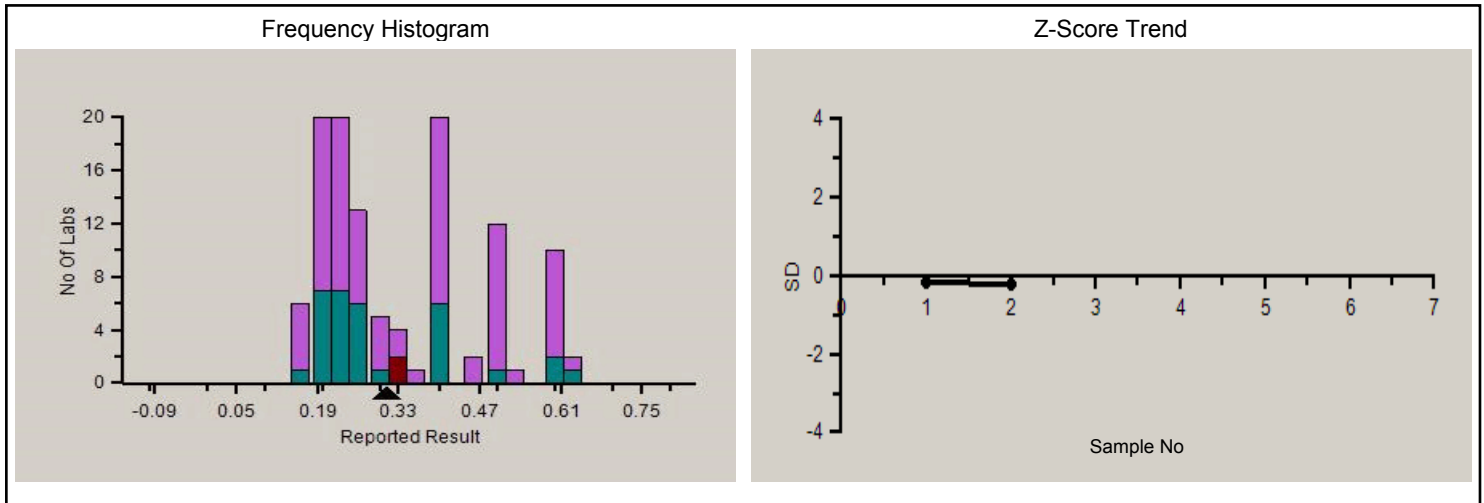

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
 Lab Name : SADBHAVANA PATHOLOGY LAB
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, Bilirubin Total		N	Mean	SD	CV%	Excluded
	All Analyzer	167	0.33	0.14	42.81	43
Your Analyzer :	Erba Chem 5/Plus	2	0.33	--	--	--
	Fuji Dri-Chem NX500/i	30	0.49	0.08	17.11	7
	Roche cobas c 311	27	0.21	0.03	13.46	3
	Roche cobas c 311	26	0.21	0.03	13.53	3
	Fuji Dri-Chem 4000i	16	0.51	0.09	17.36	1
	Horiba ABX Pentra C200	11	0.24	0.02	9.92	6
	Roche cobas c 111	11	0.22	0.04	18.72	4
	Roche cobas c 111	10	0.22	0.04	20.47	4

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, Calcium, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	156	7.58	0.57	7.57	8
■ Arsenazo III	53	7.84	0.49	6.23	5
■ Erba Chem 5/Plus	2	7.38	--	--	--

Your Result	7.45	SDI / z-Score	-1.23
Assigned Value	8.20	Average SDI	-1.16
SDPA	0.611	Uncertainty of AV	0.24
Standard Unit Result Val	7.45	%DEV	-4.95

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

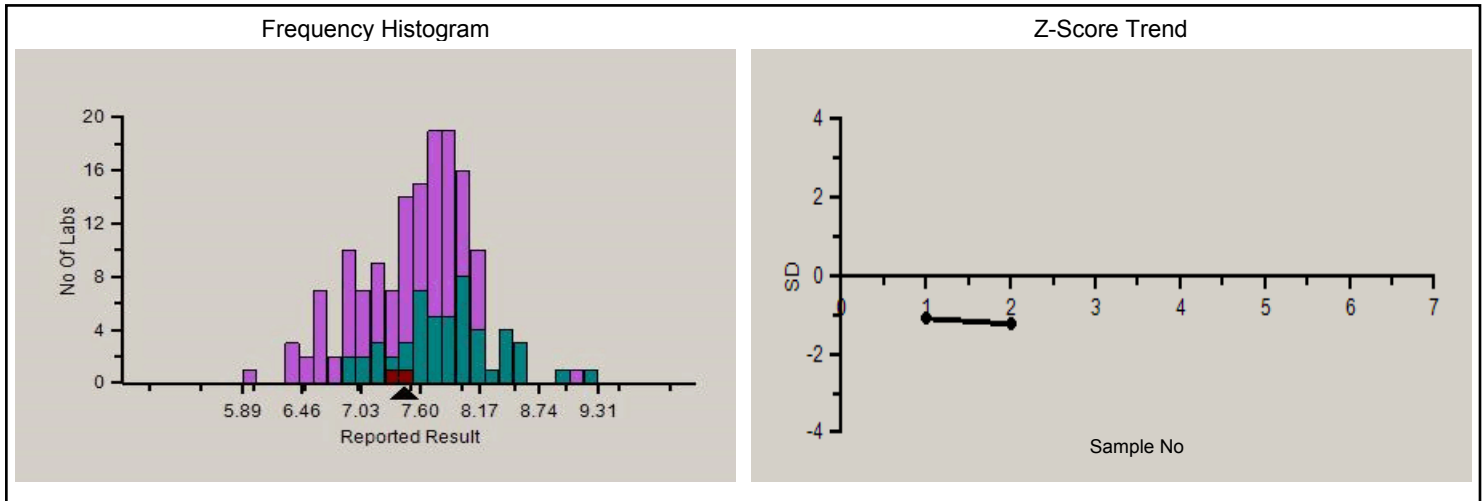

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
 Lab Name : SADBHAVANA PATHOLOGY LAB
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, Calcium		N	Mean	SD	CV%	Excluded
	All Analyzer	156	7.58	0.57	7.57	8
Your Analyzer :	Erba Chem 5/Plus	2	7.38	--	--	--
	Fuji Dri-Chem NX500/i	28	6.90	0.32	4.61	--
	Roche cobas c 311	25	7.87	0.22	2.80	--
	Roche cobas c 311	24	7.86	0.22	2.81	--
	Fuji Dri-Chem 4000i	16	7.06	0.48	6.73	--
	Roche cobas c 111	11	7.83	0.32	4.13	--
	Roche cobas INTEGRA	11	7.75	0.28	3.67	--
	Roche cobas c 111	10	7.75	0.21	2.67	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, Triglycerides, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	164	110.59	9.47	8.56	10
■ GPO-TOPS	3	108.10	2.55	2.36	1
■ Erba Chem 5/Plus	1	--	--	--	1

Your Result	72.75	SDI / z-Score	-2.89
Assigned Value	111.45	Average SDI	-2.87
SDPA	13.374	Uncertainty of AV	2.81
Standard Unit Result Val	72.75	%DEV	-32.70

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

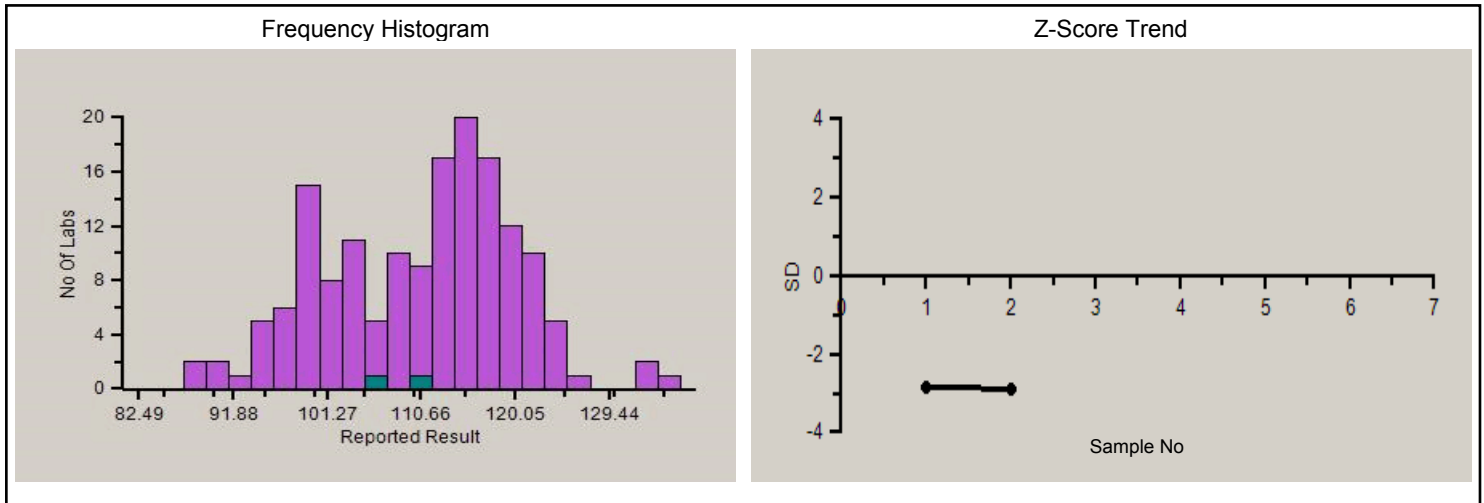

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
 Lab Name : SADBHAVANA PATHOLOGY LAB
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Biochemistry, Triglycerides		N	Mean	SD	CV%	Excluded
	All Analyzer	164	110.59	9.47	8.56	10
Your Analyzer :	Erba Chem 5/Plus	1	--	--	--	1
	Fuji Dri-Chem NX500/i	32	101.86	7.47	7.33	--
	Roche cobas c 311	27	116.34	7.35	6.32	2
	Fuji Dri-Chem 4000i	16	100.07	6.91	6.91	1
	Roche cobas c 111	12	115.59	3.91	3.38	--
	Roche cobas c 111	11	115.74	4.07	3.51	--
	Horiba ABX Pentra C200	10	116.05	3.63	3.13	1
	Roche cobas INTEGRA	10	114.28	5.62	4.92	--
	Roche cobas 6000	8	117.43	3.98	3.39	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021


Biochemistry, Uric Acid, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	166	4.18	0.34	8.11	10
■ Uricase-TOPS	2	3.74	--	--	--
■ Erba Chem 5/Plus	2	4.19	--	--	--

Your Result	3.85	SDI / z-Score	-0.94
Assigned Value	4.33	Average SDI	-0.63
SDPA	0.510	Uncertainty of AV	0.14
Standard Unit Result Val	3.85	%DEV	3.08

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

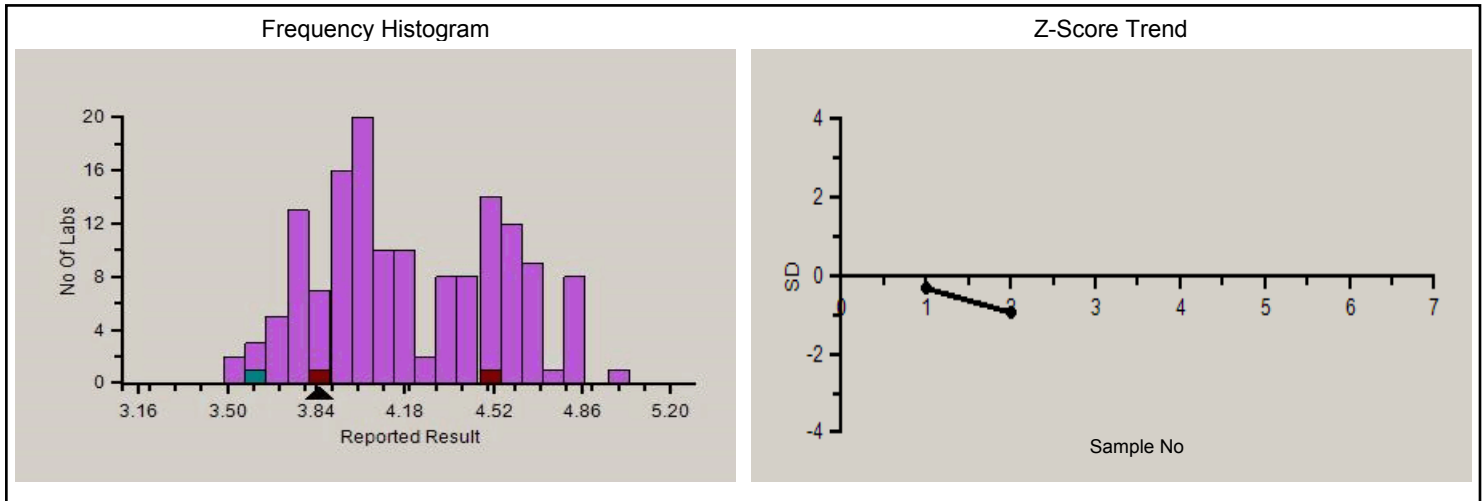

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021

Biochemistry, Uric Acid		N	Mean	SD	CV%	Excluded
	All Analyzer	166	4.18	0.34	8.11	10
Your Analyzer :	Erba Chem 5/Plus	2	4.19	--	--	--
	Fuji Dri-Chem NX500/i	31	4.49	0.18	4.05	1
	Roche cobas c 311	26	3.95	0.13	3.24	1
	Roche cobas c 311	25	3.94	0.13	3.20	1
	Fuji Dri-Chem 4000i	19	4.53	0.23	5.07	1
	Roche cobas c 111	12	3.98	0.20	5.03	--
	Roche cobas c 111	11	3.95	0.18	4.58	--
	Horiba ABX Pentra C200	10	3.91	0.15	3.79	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS

Unit No. 409-416.
Commercial Building - 1A,
Kohinoor Mall, Kirool Road, Kuria (W),
Mumbai - 400070



PC-1022

Analyte Methodwise Result Report

Lab : 446
 Lab Name : SADBHAVANA PATHOLOGY LAB
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 3
 Sample Date : 03-03-2021


Biochemistry, Cholesterol, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	163	149.43	8.19	5.48	6
CHOD-PAP	30	150.59	8.57	5.69	3
Erba Chem 5/Plus	1	--	--	--	--

Your Result	135.40	SDI / z-Score	-0.80
Assigned Value	148.50	Average SDI	-0.97
SDPA	16.335	Uncertainty of AV	5.00
Standard Unit Result Val	135.40	%DEV	-10.09

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

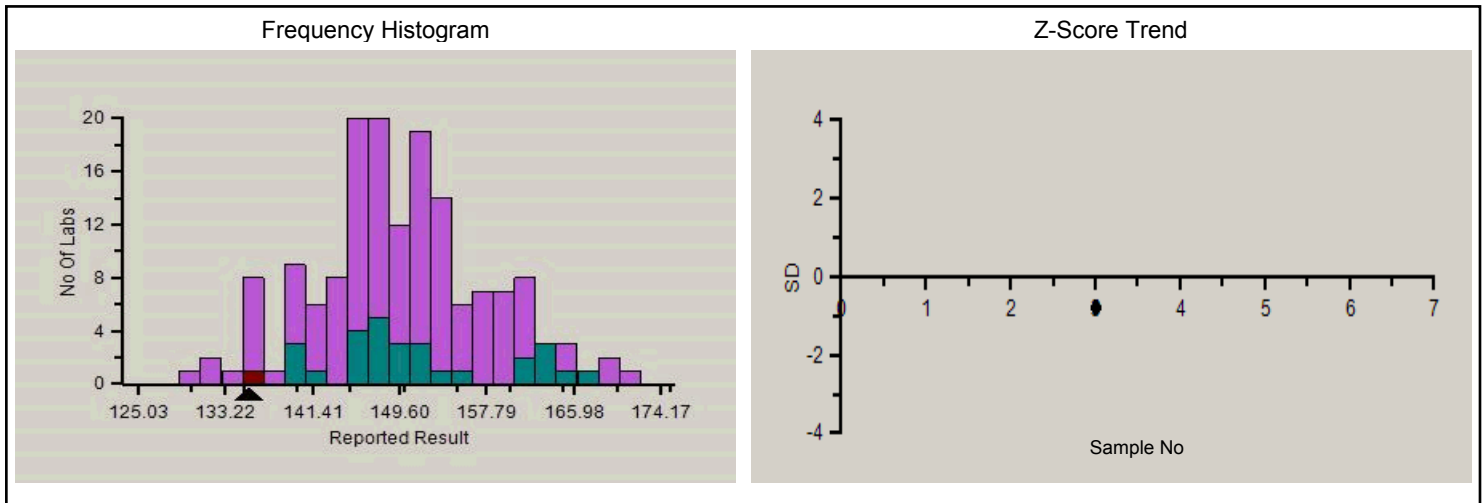

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
 Lab Name : SADBHAVANA PATHOLOGY LAB
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 3
 Sample Date : 03-03-2021

Biochemistry, Cholesterol		N	Mean	SD	CV%	Excluded
	All Analyzer	163	149.43	8.19	5.48	6
Your Analyzer :	Erba Chem 5/Plus	1	--	--	--	--
	Fuji Dri-Chem NX500/i	30	143.06	6.14	4.29	2
	Roche cobas c 311	29	150.10	4.42	2.94	--
	Roche cobas c 311	28	150.00	4.46	2.97	--
	Fuji Dri-Chem 4000i	16	143.93	8.00	5.56	--
	Roche cobas c 111	12	150.37	4.83	3.22	--
	Roche cobas c 111	11	150.68	4.95	3.28	--
	Roche cobas INTEGRA	10	147.94	3.88	2.62	--
	Horiba ABX Pentra C200	9	159.25	7.22	4.54	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 3
Sample Date : 03-03-2021


Biochemistry, Creatinine, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	167	0.71	0.21	29.07	11
■ Modified Jaffe	14	0.97	0.15	15.54	2
■ Erba Chem 5/Plus	2	1.12	--	--	--

Your Result	1.11	SDI / z-Score	-0.14
Assigned Value	1.13	Average SDI	0.83
SDPA	0.146	Uncertainty of AV	0.06
Standard Unit Result Val	1.11	%DEV	14.20

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

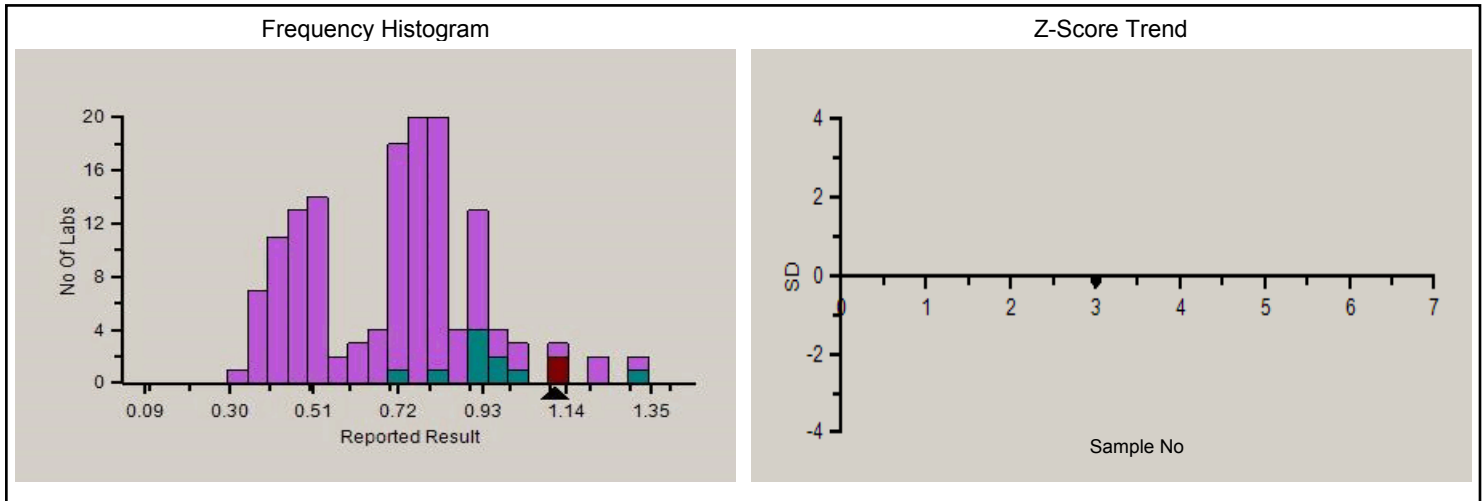

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
 Lab Name : SADBHAVANA PATHOLOGY LAB
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 3
 Sample Date : 03-03-2021

Biochemistry, Creatinine		N	Mean	SD	CV%	Excluded
	All Analyzer	167	0.71	0.21	29.07	11
Your Analyzer :	Erba Chem 5/Plus	2	1.12	--	--	--
	Fuji Dri-Chem NX500/i	29	0.43	0.05	11.48	2
	Roche cobas c 311	29	0.78	0.05	6.42	--
	Roche cobas c 311	28	0.78	0.05	6.31	--
	Fuji Dri-Chem 4000i	16	0.47	0.05	10.62	2
	Roche cobas c 111	12	0.79	0.07	9.25	--
	Horiba ABX Pentra C200	11	0.89	0.10	10.86	1
	Roche cobas c 111	11	0.81	0.05	6.46	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 3
Sample Date : 03-03-2021


Biochemistry, Glucose, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	171	73.92	3.52	4.76	10
■ GPO-POD	15	74.15	4.95	6.67	1
■ Erba Chem 5/Plus	2	77.98	--	--	--

Your Result	72.56	SDI / z-Score	0.20
Assigned Value	71.42	Average SDI	0.90
SDPA	5.714	Uncertainty of AV	2.10
Standard Unit Result Val	72.56	%DEV	-2.14

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

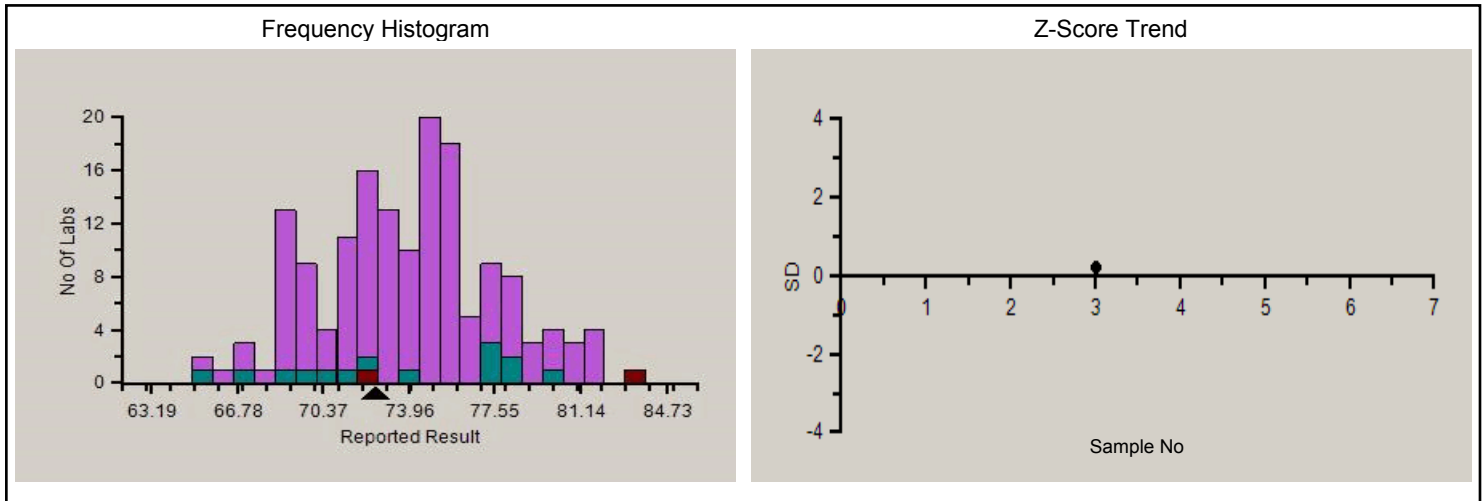

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 3
Sample Date : 03-03-2021

Biochemistry, Glucose		N	Mean	SD	CV%	Excluded
	All Analyzer	171	73.92	3.52	4.76	10
Your Analyzer :	Erba Chem 5/Plus	2	77.98	--	--	--
	Fuji Dri-Chem NX500/i	31	70.97	2.50	3.52	--
	Roche cobas c 311	29	75.76	2.54	3.36	--
	Fuji Dri-Chem 4000i	17	71.13	2.03	2.85	1
	Fuji Dri-Chem 4000i	16	70.87	1.81	2.55	1
	Horiba ABX Pentra C200	12	74.11	2.92	3.94	--
	Roche cobas c 111	11	75.64	1.35	1.79	2
	Roche cobas c 111	10	75.27	0.82	1.09	2

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 3
Sample Date : 03-03-2021


Biochemistry, Urea, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	163	23.67	3.40	14.37	18
■ Urease, GLDH	28	25.90	2.25	8.70	4
■ Erba Chem 5/Plus	2	27.59	--	--	--

Your Result	29.18	SDI / z-Score	1.26
Assigned Value	25.50	Average SDI	2.12
SDPA	2.932	Uncertainty of AV	0.18
Standard Unit Result Val	29.18	%DEV	12.65

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

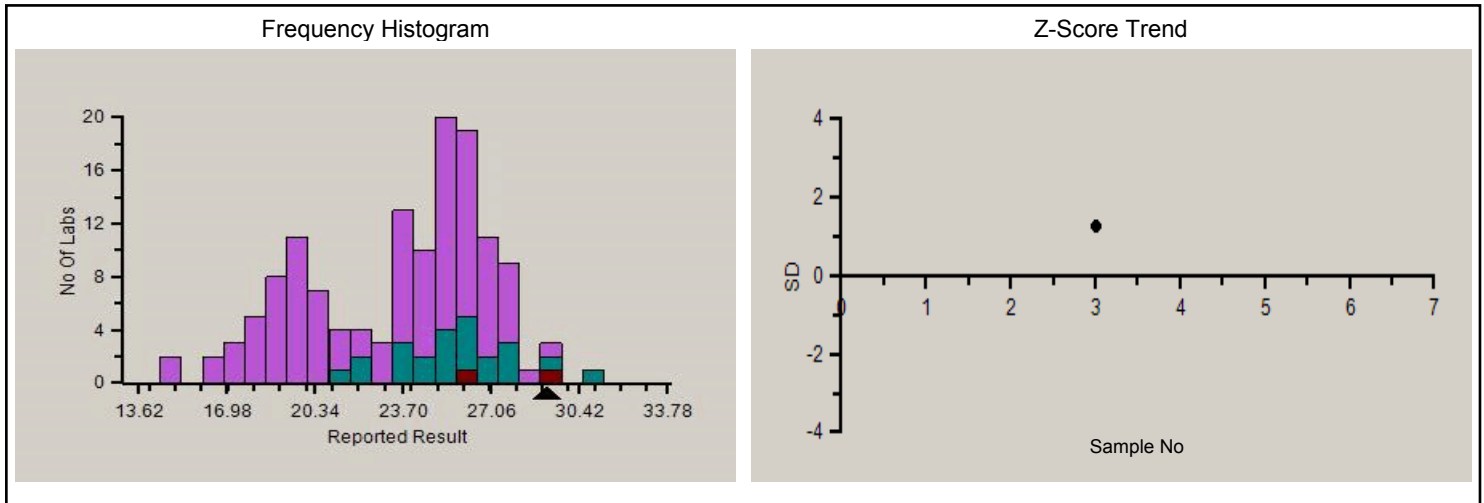

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
 Lab Name : SADBHAVANA PATHOLOGY LAB
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 3
 Sample Date : 03-03-2021

Biochemistry, Urea		N	Mean	SD	CV%	Excluded
	All Analyzer	163	23.67	3.40	14.37	18
Your Analyzer :	Erba Chem 5/Plus	2	27.59	--	--	--
	Roche cobas c 311	29	25.78	1.17	4.54	--
	Roche cobas c 311	28	25.81	1.18	4.59	--
	Fuji Dri-Chem NX500/i	25	19.04	1.41	7.41	4
	Fuji Dri-Chem 4000i	16	19.53	0.65	3.34	2
	Horiba ABX Pentra C200	12	27.13	0.88	3.25	3
	Roche cobas c 111	12	24.84	0.73	2.92	--
	Roche cobas c 111	11	24.81	0.76	3.04	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
 Unit No. 409-416.
 Commercial Building - 1A,
 Kohinoor Mall, Kirool Road, Kuria (W),
 Mumbai - 400070



PC-1022

Analyte Methodwise Result Report

Lab : 446
 Lab Name : SADBHAVANA PATHOLOGY LAB
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 4
 Sample Date : 03-03-2021


Biochemistry, Cholesterol, mg/dl

	N	Mean	SD	CV%	Excluded
All Methods	162	148.57	7.99	5.38	6
CHOD-PAP	29	150.17	8.79	5.85	3
Erba Chem 5/Plus	1	--	--	--	--

Your Result	138.30	SDI / z-Score	-1.13
Assigned Value	151.00	Average SDI	-0.97
SDPA	11.284	Uncertainty of AV	4.70
Standard Unit Result Val	138.30	%DEV	-7.90

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

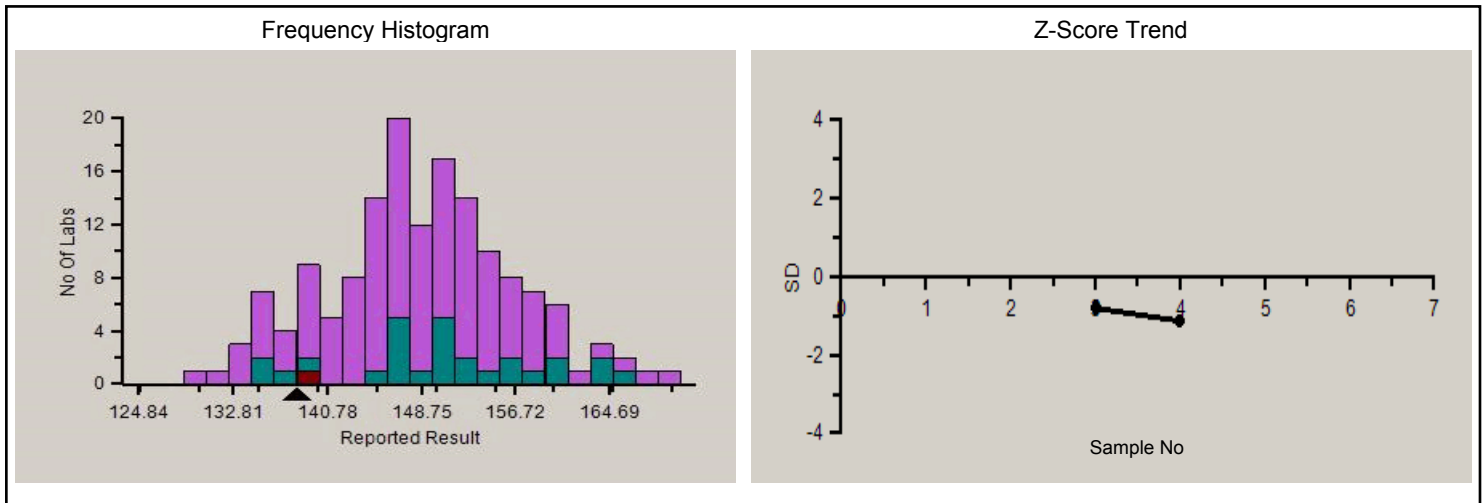

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
 Lab Name : SADBHAVANA PATHOLOGY LAB
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 4
 Sample Date : 03-03-2021

Biochemistry, Cholesterol		N	Mean	SD	CV%	Excluded
	All Analyzer	162	148.57	7.99	5.38	6
Your Analyzer :	Erba Chem 5/Plus	1	--	--	--	--
	Fuji Dri-Chem NX500/i	31	141.82	5.36	3.78	2
	Roche cobas c 311	28	149.70	4.10	2.74	--
	Roche cobas c 311	27	149.61	4.15	2.78	--
	Fuji Dri-Chem 4000i	16	142.96	6.31	4.41	--
	Roche cobas c 111	12	149.17	6.24	4.18	1
	Roche cobas c 111	11	149.38	6.53	4.37	1
	Roche cobas INTEGRA	10	147.16	3.78	2.57	--
	Horiba ABX Pentra C200	9	157.23	9.04	5.75	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 4
Sample Date : 03-03-2021


Biochemistry, Creatinine, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	165	0.59	0.17	28.43	17
■ Modified Jaffe	13	0.83	0.12	14.56	5
■ Erba Chem 5/Plus	2	1.01	--	--	--

Your Result	1.03	SDI / z-Score	1.79
Assigned Value	0.79	Average SDI	0.83
SDPA	0.134	Uncertainty of AV	0.06
Standard Unit Result Val	1.03	%DEV	23.95

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

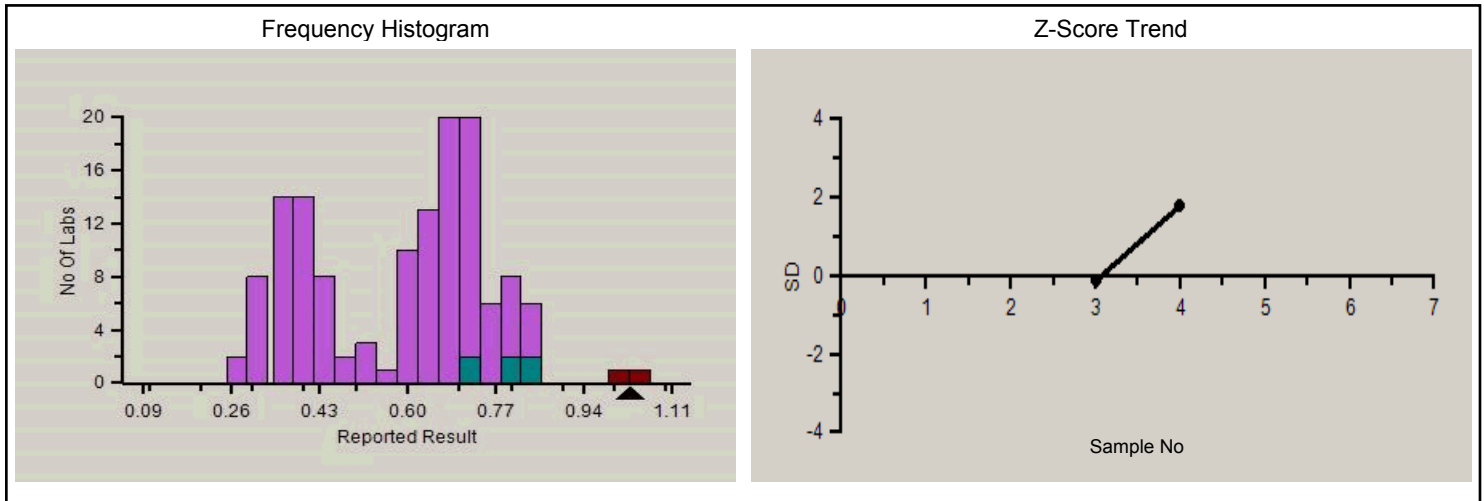

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
 Lab Name : SADBHAVANA PATHOLOGY LAB
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 4
 Sample Date : 03-03-2021

Biochemistry, Creatinine		N	Mean	SD	CV%	Excluded
	All Analyzer	165	0.59	0.17	28.43	17
Your Analyzer :	Erba Chem 5/Plus	2	1.01	--	--	--
	Fuji Dri-Chem NX500/i	29	0.36	0.05	13.65	2
	Roche cobas c 311	28	0.67	0.05	6.98	--
	Roche cobas c 311	27	0.67	0.05	6.86	--
	Fuji Dri-Chem 4000i	16	0.38	0.04	10.94	--
	Roche cobas c 111	12	0.69	0.07	10.15	--
	Horiba ABX Pentra C200	11	0.76	0.06	8.33	4
	Roche cobas c 111	11	0.70	0.07	10.22	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 4
Sample Date : 03-03-2021


Biochemistry, Glucose, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	169	76.08	3.72	4.89	10
■ GPO-POD	15	77.56	5.03	6.49	2
■ Erba Chem 5/Plus	2	83.93	--	--	--

Your Result	85.09	SDI / z-Score	1.60
Assigned Value	74.00	Average SDI	0.90
SDPA	6.951	Uncertainty of AV	2.90
Standard Unit Result Val	85.09	%DEV	9.72

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

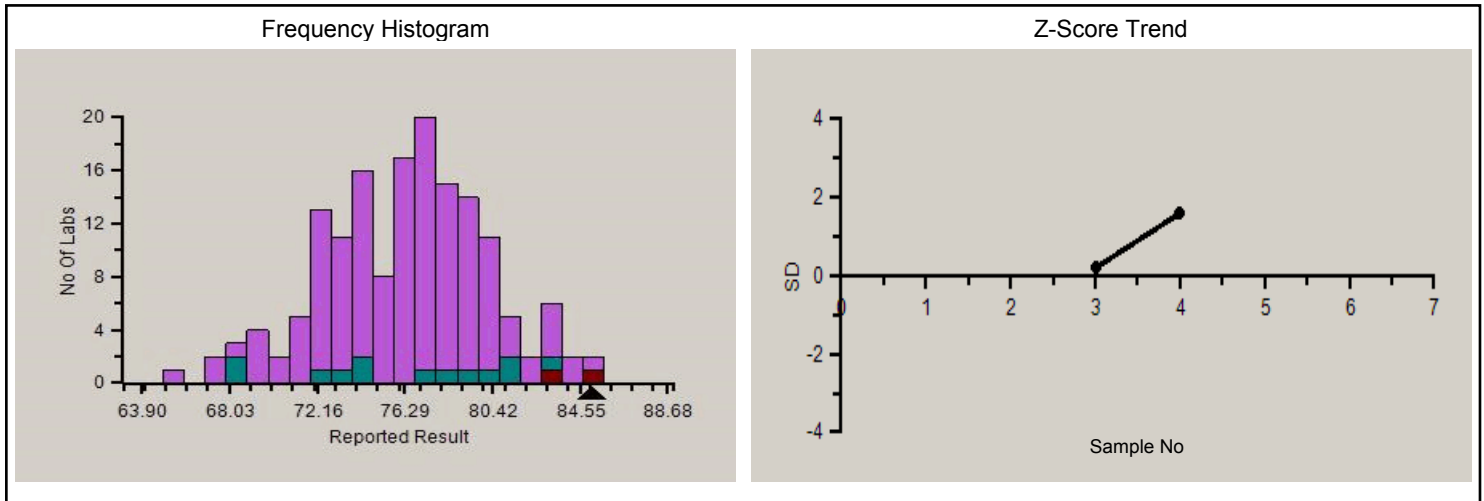

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
 Lab Name : SADBHAVANA PATHOLOGY LAB
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 4
 Sample Date : 03-03-2021

Biochemistry, Glucose		N	Mean	SD	CV%	Excluded
	All Analyzer	169	76.08	3.72	4.89	10
Your Analyzer :	Erba Chem 5/Plus	2	83.93	--	--	--
	Fuji Dri-Chem NX500/i	31	72.88	2.81	3.86	--
	Roche cobas c 311	28	77.76	2.48	3.18	--
	Fuji Dri-Chem 4000i	17	73.53	1.91	2.60	1
	Fuji Dri-Chem 4000i	16	73.27	1.67	2.28	1
	Horiba ABX Pentra C200	12	76.63	3.10	4.05	--
	Roche cobas c 111	11	78.13	1.94	2.49	3
	Roche cobas c 111	10	77.75	1.75	2.25	3

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 4
Sample Date : 03-03-2021


Biochemistry, Urea, mg/dl

	N	Mean	SD	CV%	Excluded
■ All Methods	161	21.74	3.45	15.88	13
■ Urease, GLDH	26	23.62	2.63	11.14	3
■ Erba Chem 5/Plus	2	24.00	--	--	1

Your Result	30.22	SDI / z-Score	2.97
Assigned Value	23.31	Average SDI	2.12
SDPA	2.331	Uncertainty of AV	0.19
Standard Unit Result Val	30.22	%DEV	27.95

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

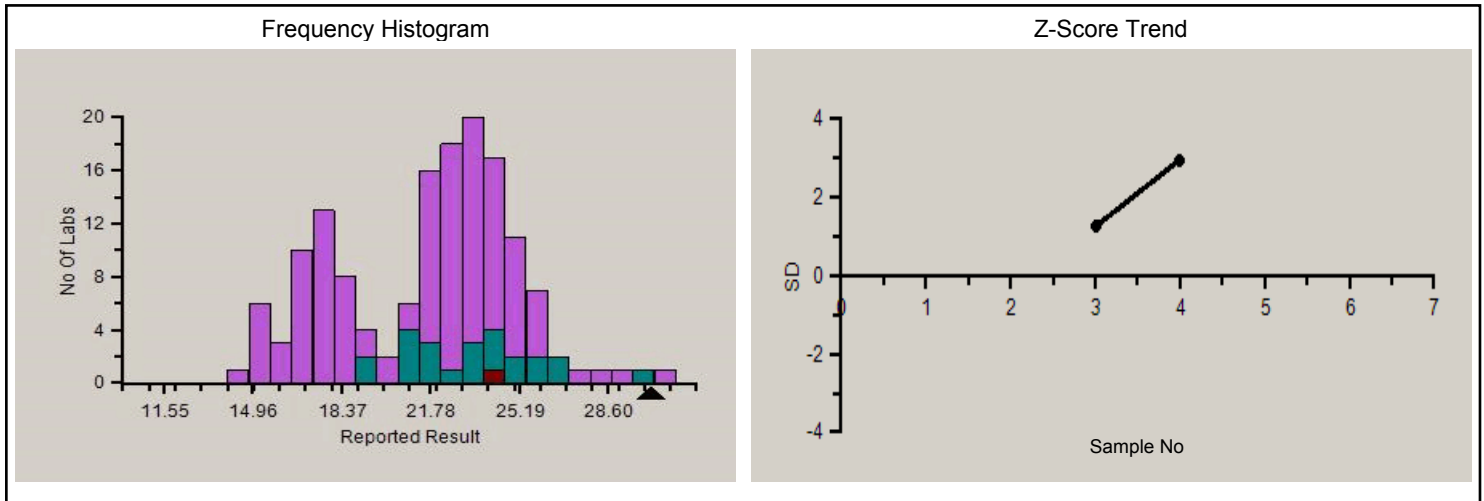

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 446
Lab Name : SADBHAVANA PATHOLOGY LAB
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 4
Sample Date : 03-03-2021

Biochemistry, Urea		N	Mean	SD	CV%	Excluded
	All Analyzer	161	21.74	3.45	15.88	13
Your Analyzer :	Erba Chem 5/Plus	2	24.00	--	--	1
	Roche cobas c 311	28	23.56	0.99	4.20	--
	Roche cobas c 311	27	23.59	0.99	4.21	--
	Fuji Dri-Chem NX500/i	25	17.02	1.36	8.00	3
	Fuji Dri-Chem 4000i	16	17.75	0.47	2.65	2
	Horiba ABX Pentra C200	12	25.44	1.35	5.30	1
	Roche cobas c 111	12	22.57	1.26	5.56	--
	Roche cobas c 111	11	22.49	1.29	5.72	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
Unit No. 409-416.
Commercial Building - 1A,
Kohinoor Mall, Kirol Road, Kuria (W),
Mumbai - 400070



PC-1022