

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 1  
Sample Date : 03-03-2021


**Biochemistry, Albumin, g/dL**

	N	Mean	SD	CV%	Excluded
All Methods	168	3.99	0.47	11.65	4
Bromcresol Green (BCG)	160	4.01	0.46	11.41	4
Erba EM 200	7	3.55	0.07	2.06	--

<b>Your Result</b>	3.51	<b>SDI / z-Score</b>	-0.73
<b>Assigned Value</b>	3.73	<b>Average SDI</b>	-0.53
<b>SDPA</b>	0.294	<b>Uncertainty of AV</b>	0.02
<b>Standard Unit Result Val</b>	3.51	<b>%DEV</b>	-1.21

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

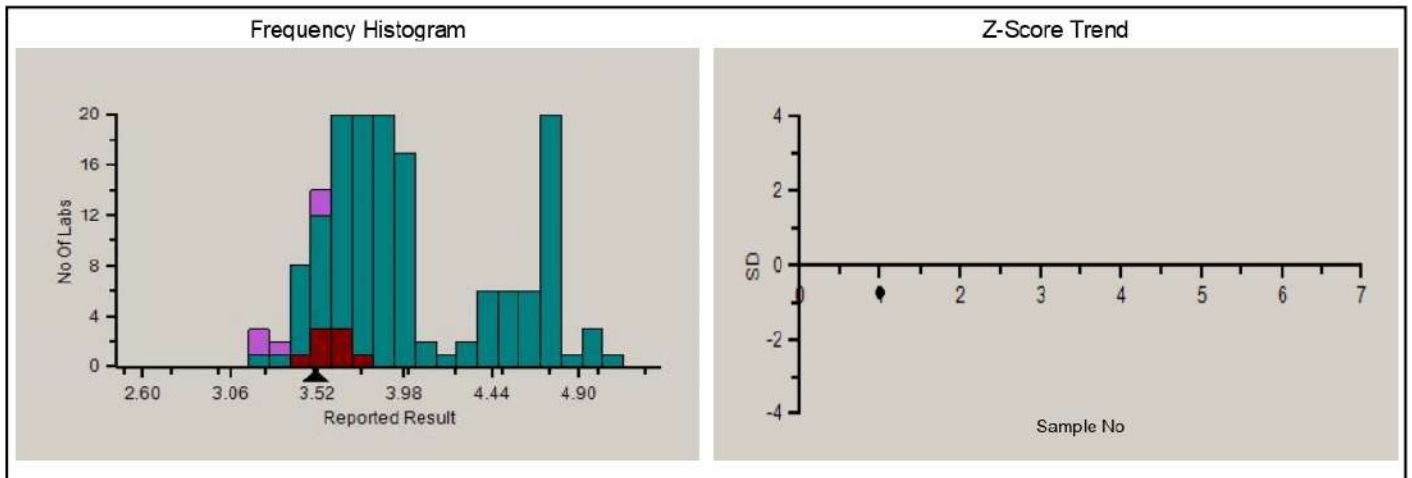

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 1  
 Sample Date : 03-03-2021

<b>Biochemistry, Albumin</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	168	3.99	0.47	11.65	4
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>7</b>	<b>3.55</b>	<b>0.07</b>	<b>2.06</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	31	4.60	0.20	4.37	--
	Roche cobas c 311	29	3.82	0.13	3.41	--
	Roche cobas c 311	28	3.82	0.13	3.38	--
	Fuji Dri-Chem 4000i	16	4.74	0.20	4.15	--
	Roche cobas c 111	11	3.86	0.19	5.03	--
	Horiba ABX Pentra C200	10	3.55	0.15	4.12	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 1  
Sample Date : 03-03-2021


**Biochemistry, ALP, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	167	87.20	13.87	15.91	18
IFCC	20	76.99	7.17	9.32	4
Erba EM 200	5	83.98	2.62	3.12	2

<b>Your Result</b>	85.93	<b>SDI / z-Score</b>	0.54
<b>Assigned Value</b>	78.29	<b>Average SDI</b>	-0.18
<b>SDPA</b>	14.091	<b>Uncertainty of AV</b>	0.63
<b>Standard Unit Result Val</b>	85.93	<b>%DEV</b>	2.33

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

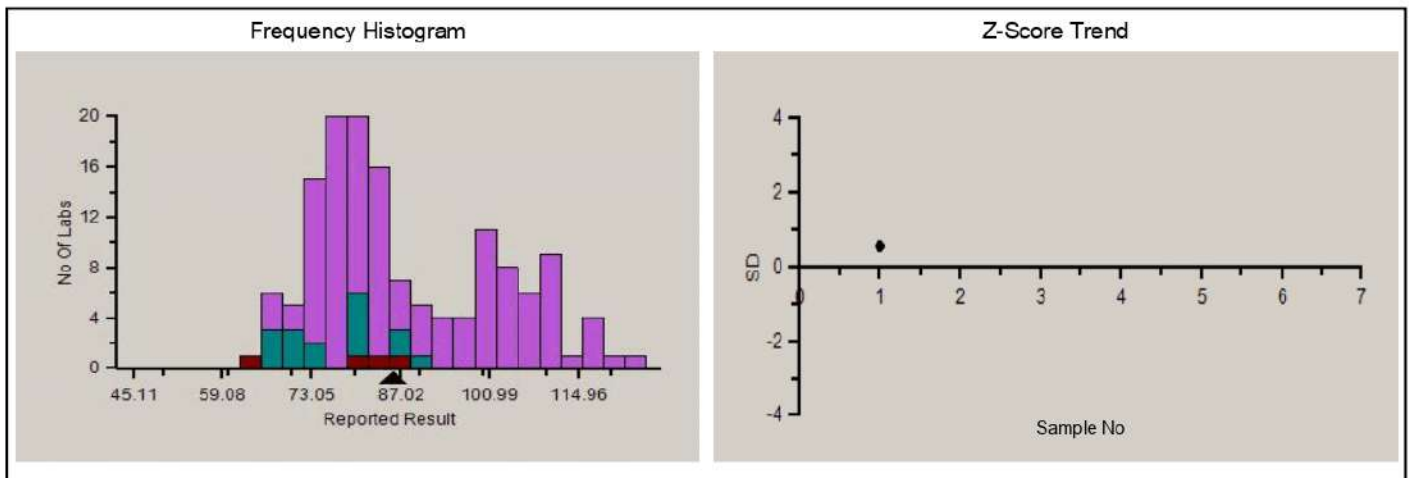

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

**Lab :** 429  
**Lab Name :** NEYVELI DIAGNOSTIC CENTRE  
**Report Date :** 19/03/2021

**Cycle No :** 210103  
**Sample No :** 1  
**Sample Date :** 03-03-2021

<b>Biochemistry, ALP</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	167	87.20	13.87	15.91	18
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>5</b>	<b>83.98</b>	<b>2.62</b>	<b>3.12</b>	<b>2</b>
	Fuji Dri-Chem NX500/i	33	106.25	7.85	7.39	1
	Roche cobas c 311	29	78.31	3.55	4.54	—
	Roche cobas c 311	28	78.32	3.62	4.62	—
	Fuji Dri-Chem 4000i	16	102.13	7.54	7.38	1
	Roche cobas c 111	12	77.55	6.66	8.59	—
	Roche cobas c 111	11	76.60	6.07	7.92	—

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 1  
Sample Date : 03-03-2021


**Biochemistry, ALT, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	168	29.17	29.26	100.33	61
IFCC	17	11.68	1.31	11.20	13
Erba EM 200	6	19.73	3.20	16.22	3

<b>Your Result</b>	13.81	<b>SDI / z-Score</b>	-2.02
<b>Assigned Value</b>	23.20	<b>Average SDI</b>	1.03
<b>SDPA</b>	4.640	<b>Uncertainty of AV</b>	1.51
<b>Standard Unit Result Val</b>	13.81	<b>%DEV</b>	-30.02

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

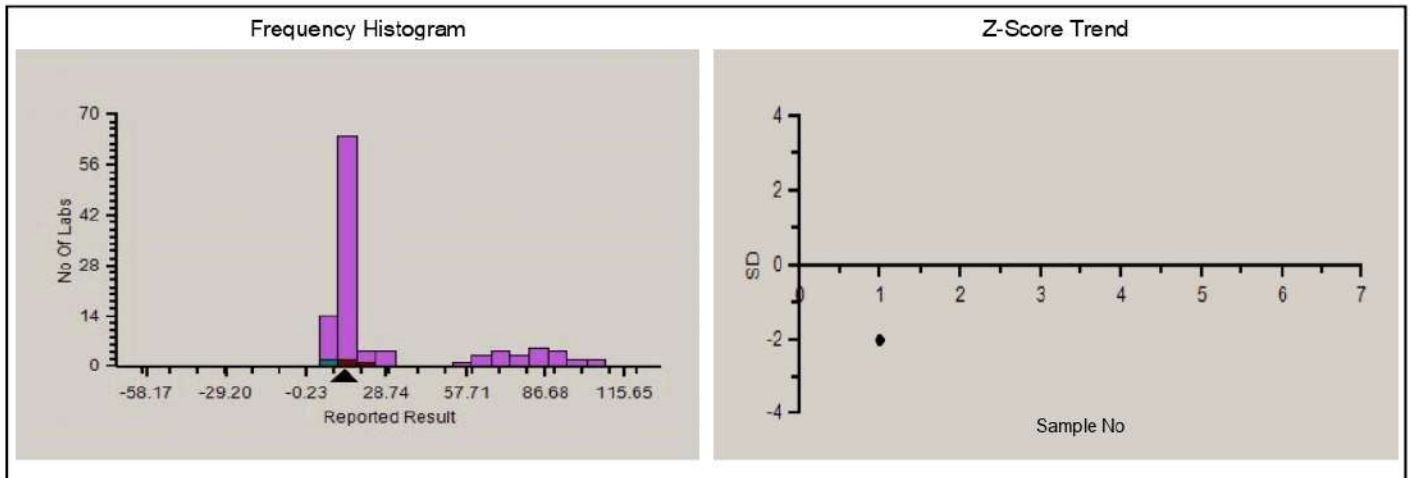

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

**Lab :** 429  
**Lab Name :** NEYVELI DIAGNOSTIC CENTRE  
**Report Date :** 19/03/2021

**Cycle No :** 210103  
**Sample No :** 1  
**Sample Date :** 03-03-2021

<b>Biochemistry, ALT</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	168	29.17	29.26	100.33	61
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>6</b>	<b>19.73</b>	<b>3.20</b>	<b>16.22</b>	<b>3</b>
	Fuji Dri-Chem NX500/i	30	87.00	12.62	14.51	18
	Roche cobas c 311	29	13.17	1.52	11.51	6
	Roche cobas c 311	28	13.02	1.36	10.46	6
	Fuji Dri-Chem 4000i	16	76.40	14.14	18.50	6
	Roche cobas c 111	12	13.25	1.65	12.42	1
	Horiba ABX Pentra C200	11	12.64	1.59	12.60	—

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 1  
Sample Date : 03-03-2021


**Biochemistry, Amylase, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	100	60.30	6.95	11.52	8
CNP-triose/CNPG3	14	58.00	7.96	13.73	5
Erba EM 200	1	--	--	--	1

<b>Your Result</b>	67.00	<b>SDI / z-Score</b>	2.29
<b>Assigned Value</b>	54.30	<b>Average SDI</b>	0.55
<b>SDPA</b>	5.539	<b>Uncertainty of AV</b>	0.65
<b>Standard Unit Result Val</b>	67.00	<b>%DEV</b>	15.52

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

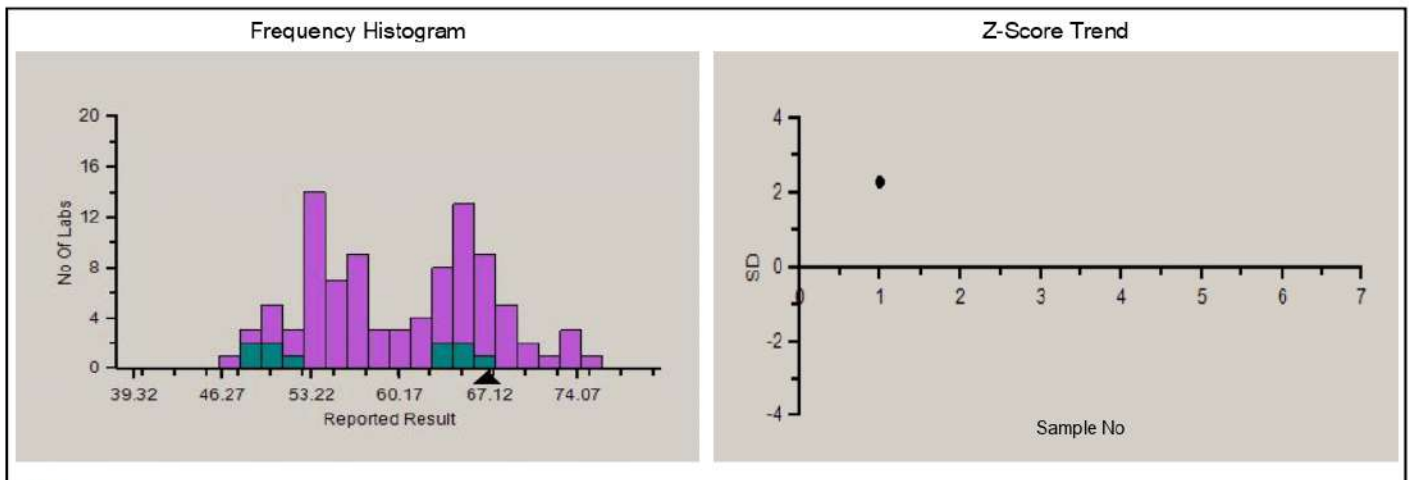

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 1  
 Sample Date : 03-03-2021

<b>Biochemistry, Amylase</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	100	60.30	6.95	11.52	8
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	23	55.61	3.58	6.43	--
	Fuji Dri-Chem 4000i	15	54.87	1.89	3.44	--
	Roche cobas c 311	15	66.72	3.00	4.49	--
	Fuji Dri-Chem 4000i	14	54.64	1.74	3.18	--
	Roche cobas INTEGRA	7	65.35	3.08	4.72	--
	Roche cobas 6000	6	66.22	1.83	2.77	--
	Roche cobas 8000	4	67.25	2.22	3.30	--
	Roche cobas c 111	3	69.10	5.67	8.20	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022



**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 1  
Sample Date : 03-03-2021


**Biochemistry, AST, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	167	27.28	11.26	41.27	63
IFCC	18	26.37	9.67	36.68	9
Erba EM 200	6	40.00	9.42	23.55	3

<b>Your Result</b>	29.50	<b>SDI / z-Score</b>	-1.09
<b>Assigned Value</b>	37.70	<b>Average SDI</b>	-1.10
<b>SDPA</b>	7.540	<b>Uncertainty of AV</b>	2.32
<b>Standard Unit Result Val</b>	29.50	<b>%DEV</b>	-26.25

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

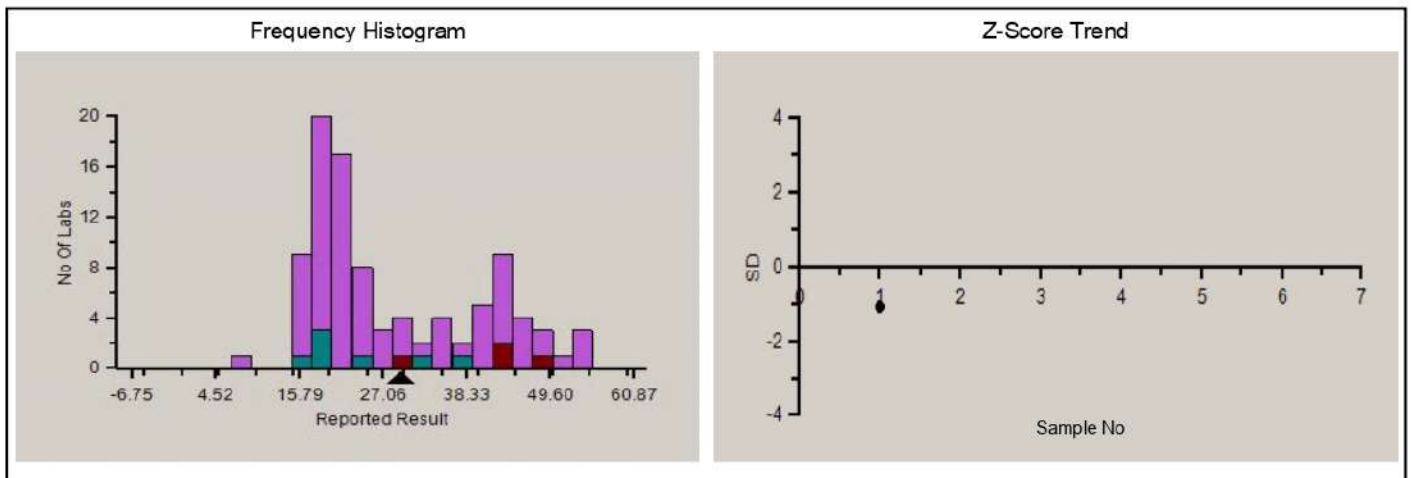

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

**Lab :** 429  
**Lab Name :** NEYVELI DIAGNOSTIC CENTRE  
**Report Date :** 19/03/2021

**Cycle No :** 210103  
**Sample No :** 1  
**Sample Date :** 03-03-2021

<b>Biochemistry, AST</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	167	27.28	11.26	41.27	63
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>6</b>	<b>40.00</b>	<b>9.42</b>	<b>23.55</b>	<b>3</b>
	Fuji Dri-Chem NX500/i	31	42.36	7.61	17.95	20
	Roche cobas c 311	28	20.76	2.77	13.35	5
	Roche cobas c 311	27	20.46	2.41	11.77	5
	Fuji Dri-Chem 4000i	16	45.89	6.86	14.96	7
	Roche cobas c 111	13	21.23	2.95	13.89	5
	Roche cobas c 111	12	21.67	2.88	13.28	5

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 1  
 Sample Date : 03-03-2021


**Biochemistry, Bilirubin Direct, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	166	0.10	0.02	17.00	51
<span style="color: teal;">■</span> Diazotization	134	0.10	0.02	16.33	37
<span style="color: red;">■</span> Erba EM 200	7	0.11	0.03	25.93	2

<b>Your Result</b>	0.07	<b>SDI / z-Score</b>	-0.86
<b>Assigned Value</b>	0.11	<b>Average SDI</b>	-0.94
<b>SDPA</b>	0.051	<b>Uncertainty of AV</b>	0.01
<b>Standard Unit Result Val</b>	0.07	<b>%DEV</b>	-35.19

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

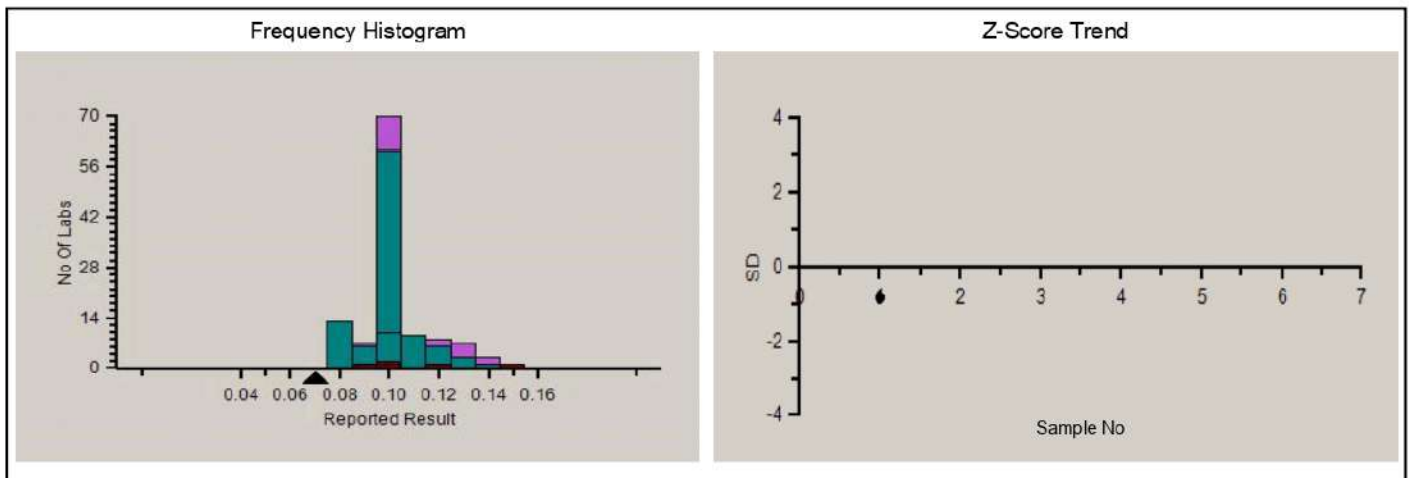

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 1  
 Sample Date : 03-03-2021

<b>Biochemistry, Bilirubin Direct</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	166	0.10	0.02	17.00	51
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>7</b>	<b>0.11</b>	<b>0.03</b>	<b>25.93</b>	<b>2</b>
	Fuji Dri-Chem NX500/i	28	0.10	0.01	8.08	9
	Roche cobas c 311	28	0.09	0.02	19.15	5
	Roche cobas c 311	27	0.09	0.02	19.15	5
	Fuji Dri-Chem 4000i	16	0.10	0.00	0.00	9
	Roche cobas c 111	12	0.11	0.01	11.11	4
	Horiba ABX Pentra C200	11	0.12	0.02	13.91	—

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 1  
Sample Date : 03-03-2021


**Biochemistry, Bilirubin Total, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	170	0.31	0.14	45.05	49
Diazotization	45	0.29	0.14	46.76	13
Erba EM 200	7	0.22	0.03	14.42	1

<b>Your Result</b>	0.20	<b>SDI / z-Score</b>	-0.02
<b>Assigned Value</b>	0.20	<b>Average SDI</b>	-0.11
<b>SDPA</b>	0.060	<b>Uncertainty of AV</b>	0.01
<b>Standard Unit Result Val</b>	0.20	<b>%DEV</b>	-6.98

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

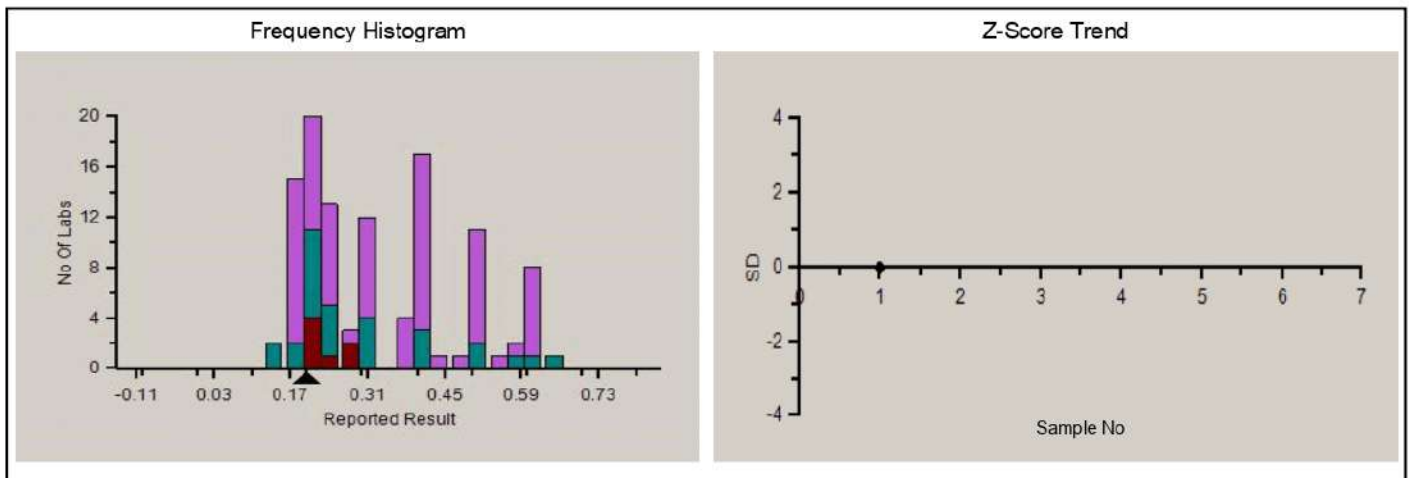

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 1  
 Sample Date : 03-03-2021

<b>Biochemistry, Bilirubin Total</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	170	0.31	0.14	45.05	49
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>7</b>	<b>0.22</b>	<b>0.03</b>	<b>14.42</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	30	0.47	0.08	16.24	6
	Roche cobas c 311	29	0.20	0.03	14.07	6
	Roche cobas c 311	28	0.20	0.03	14.50	6
	Fuji Dri-Chem 4000i	16	0.51	0.08	16.37	2
	Horiba ABX Pentra C200	11	0.22	0.03	11.26	6
	Roche cobas c 111	11	0.21	0.03	14.56	4

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.






PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 1  
Sample Date : 03-03-2021


**Biochemistry, Calcium, mg/dl**

	N	Mean	SD	CV%	Excluded
 All Methods	157	7.64	0.53	6.92	11
 Arsenazo I	3	7.79	1.13	14.47	--
 Erba EM 200	5	8.51	0.65	7.62	--

<b>Your Result</b>	8.95	<b>SDI / z-Score</b>	1.19
<b>Assigned Value</b>	8.20	<b>Average SDI</b>	1.01
<b>SDPA</b>	0.631	<b>Uncertainty of AV</b>	0.23
<b>Standard Unit Result Val</b>	8.95	<b>%DEV</b>	5.17

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

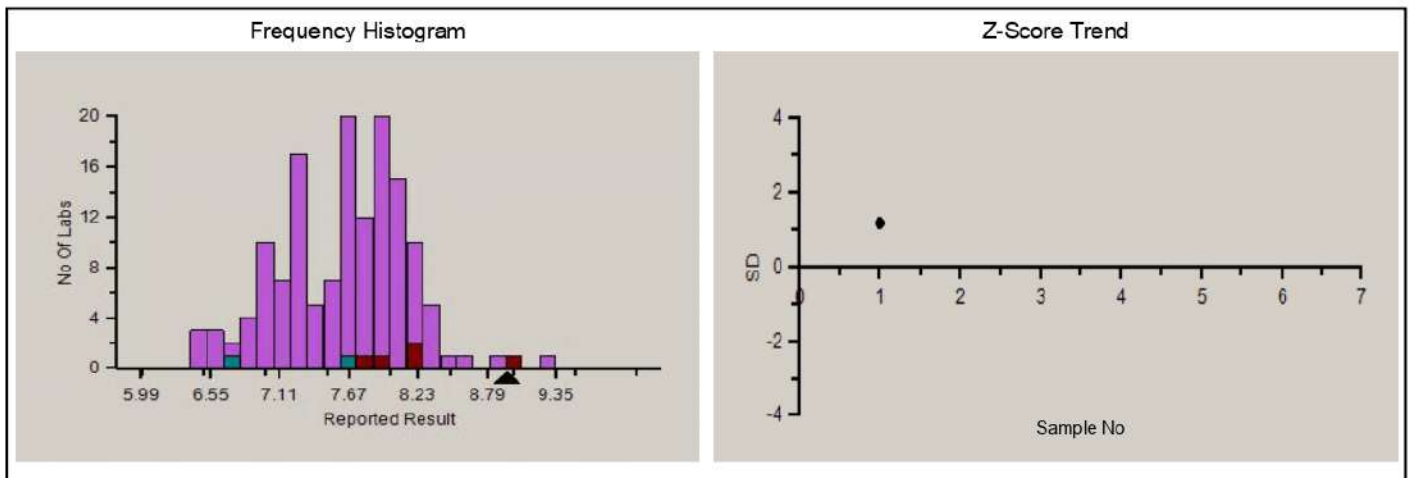

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 1  
 Sample Date : 03-03-2021

Biochemistry, Calcium		N	Mean	SD	CV%	Excluded
	All Analyzer	157	7.64	0.53	6.92	11
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>5</b>	<b>8.51</b>	<b>0.65</b>	<b>7.62</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	28	7.00	0.31	4.43	--
	Roche cobas c 311	26	7.93	0.25	3.12	1
	Roche cobas c 311	25	7.92	0.25	3.18	1
	Fuji Dri-Chem 4000i	16	7.26	0.35	4.80	--
	Roche cobas c 111	11	7.91	0.34	4.32	1
	Roche cobas INTEGRA	11	7.76	0.31	3.99	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022



**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 1  
 Sample Date : 03-03-2021


**Biochemistry, Chloride, mEq/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	140	105.52	12.39	11.74	15
<span style="color: teal;">■</span> Mercuric thiocyanate, ferric ion	2	0.00	--	--	--
<span style="color: red;">■</span> Erba Chem 7	1	--	--	--	--

<b>Your Result</b>	80.92	<b>SDI / z-Score</b>	-1.21
<b>Assigned Value</b>	87.86	<b>Average SDI</b>	-1.03
<b>SDPA</b>	5.710	<b>Uncertainty of AV</b>	0.52
<b>Standard Unit Result Val</b>	80.92	<b>%DEV</b>	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

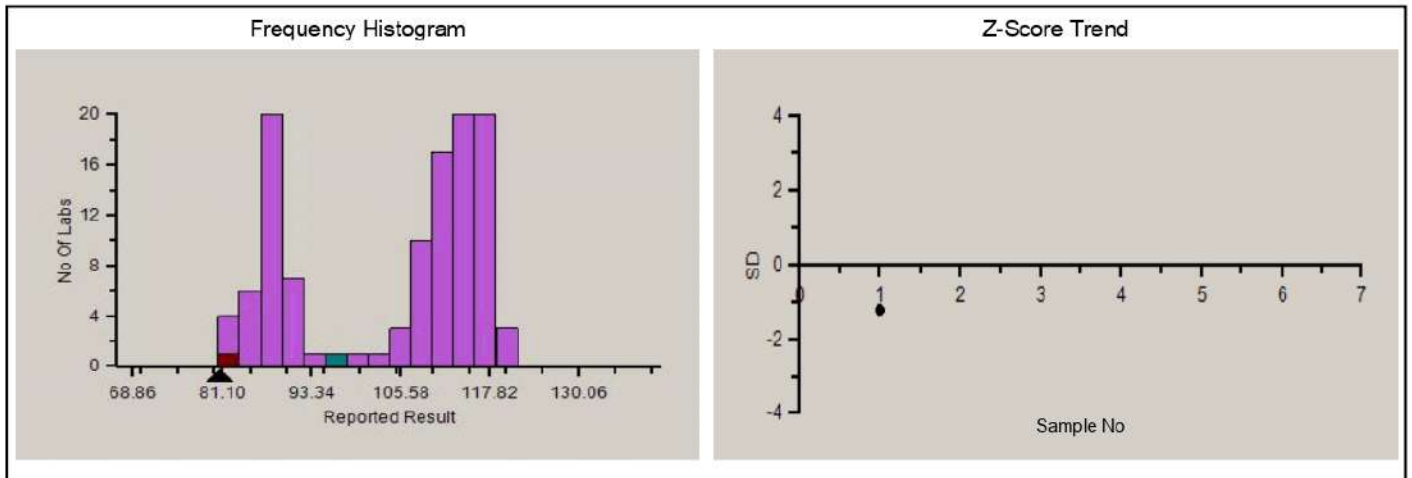

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 1  
 Sample Date : 03-03-2021

<b>Biochemistry, Chloride</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	140	105.52	12.39	11.74	15
<b>Your Analyzer :</b>	<b>Erba Chem 7</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	32	0.00	0.00	0.00	1
	Fuji Dri-Chem 4000i	17	0.00	0.00	0.00	1
	Roche cobas c 311	16	0.00	0.00	0.00	--
	Roche AVL 9180	12	110.49	2.13	1.93	--
	Roche AVL 9180	11	110.17	1.91	1.74	--
	Roche AVL 9180	10	0.00	0.00	0.00	--
	EasyLyte	9	112.26	4.60	4.10	1
	Roche cobas 6000	8	0.00	0.00	0.00	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 1  
 Sample Date : 03-03-2021


**Biochemistry, GGT, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	135	15.80	3.87	24.49	11
SZASZ IFCC standardized	3	20.00	0.00	0.00	2
Erba EM 200	3	18.45	2.62	14.18	1

<b>Your Result</b>	26.10	<b>SDI / z-Score</b>	2.79
<b>Assigned Value</b>	18.40	<b>Average SDI</b>	1.23
<b>SDPA</b>	2.760	<b>Uncertainty of AV</b>	0.27
<b>Standard Unit Result Val</b>	26.10	<b>%DEV</b>	30.50

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

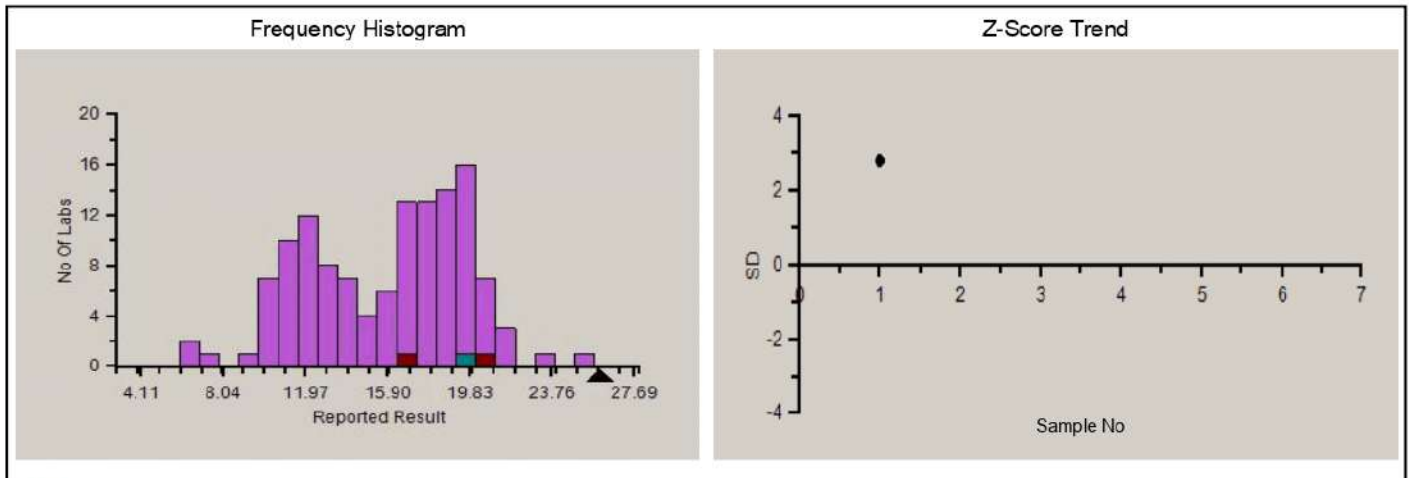

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 1  
 Sample Date : 03-03-2021

<b>Biochemistry, GGT</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	135	15.80	3.87	24.49	11
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>3</b>	<b>18.45</b>	<b>2.62</b>	<b>14.18</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	32	12.03	1.19	9.88	2
	Roche cobas c 311	25	19.26	1.74	9.02	2
	Roche cobas c 311	24	19.00	1.23	6.50	2
	Fuji Dri-Chem 4000i	12	11.33	1.50	13.21	—
	Roche cobas INTEGRA	11	16.87	1.42	8.43	—
	Roche cobas c 111	10	16.97	1.39	8.18	1
	Beckman Coulter AU480	6	19.20	1.35	7.03	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 1  
Sample Date : 03-03-2021


**Biochemistry, Potassium, mEq/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	151	5.75	0.93	16.17	12
<span style="color: teal;">■</span> Colorimetric	2	--	--	--	2
<span style="color: red;">■</span> Erba Chem 7	1	--	--	--	1

<b>Your Result</b>	3.84	<b>SDI / z-Score</b>	-2.14
<b>Assigned Value</b>	4.30	<b>Average SDI</b>	-1.83
<b>SDPA</b>	0.215	<b>Uncertainty of AV</b>	0.02
<b>Standard Unit Result Val</b>	3.84	<b>%DEV</b>	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

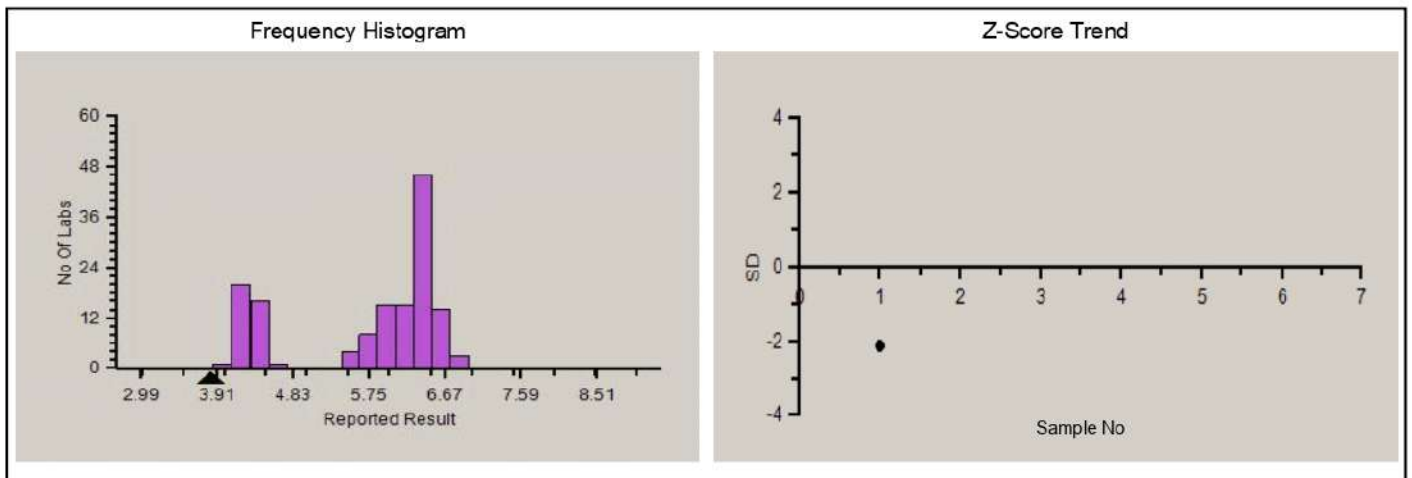

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 1  
 Sample Date : 03-03-2021

<b>Biochemistry, Potassium</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	151	5.75	0.93	16.17	12
<b>Your Analyzer :</b>	<b>Erba Chem 7</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	33	0.00	0.00	0.00	1
	Fuji Dri-Chem 4000i	19	0.00	0.00	0.00	1
	Roche cobas c 311	16	0.00	0.00	0.00	--
	Roche AVL 9180	14	6.27	0.46	7.28	--
	Roche AVL 9180	13	6.33	0.43	6.81	--
	Roche AVL 9180	12	0.00	0.00	0.00	--
	EasyLyte	10	5.86	0.14	2.35	--
	EasyLyte	9	0.00	0.00	0.00	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.






PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 1  
 Sample Date : 03-03-2021


**Biochemistry, Sodium, mEq/L**

	N	Mean	SD	CV%	Excluded
 All Methods	151	159.57	23.46	14.70	18
 Colorimetric	2	0.00	--	--	1
 Erba EM 200	2	0.00	--	--	--

<b>Your Result</b>	123.90	<b>SDI / z-Score</b>	0.05
<b>Assigned Value</b>	123.57	<b>Average SDI</b>	-0.19
<b>SDPA</b>	6.178	<b>Uncertainty of AV</b>	0.44
<b>Standard Unit Result Val</b>	123.90	<b>%DEV</b>	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

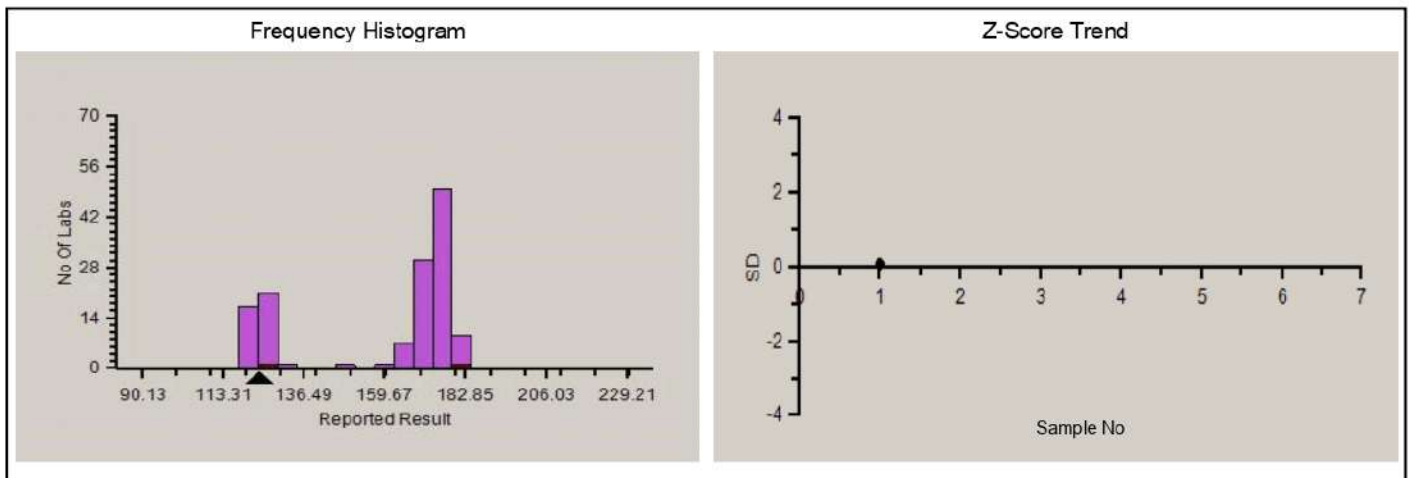

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 1  
 Sample Date : 03-03-2021

<b>Biochemistry, Sodium</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	151	159.57	23.46	14.70	18
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>2</b>	<b>0.00</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	34	0.00	0.00	0.00	3
	Fuji Dri-Chem 4000i	18	0.00	0.00	0.00	3
	Roche cobas c 311	16	0.00	0.00	0.00	--
	Roche AVL 9180	14	173.21	9.18	5.30	--
	Roche AVL 9180	13	175.22	5.44	3.11	--
	Roche AVL 9180	12	0.00	0.00	0.00	--
	EasyLyte	10	170.00	3.04	1.79	2

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.

*Dr. Nigam*

**Dr Puneet Kumar Nigam**  
**PT coordinator & Technical Manager, MHL EQAS**  
 Unit No. 409-416,  
 Commercial Building - 1A,  
 Koinoor Mall, Kiroi Road, Kurla (W),  
 Mumbai - 400070



PC-1022



**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, Albumin, g/dL**

	N	Mean	SD	CV%	Excluded
All Methods	166	3.97	0.46	11.62	6
Bromcresol Green (BCG)	158	3.97	0.46	11.50	5
Erba EM 200	7	3.54	0.08	2.29	--

<b>Your Result</b>	3.62	<b>SDI / z-Score</b>	-0.32
<b>Assigned Value</b>	3.69	<b>Average SDI</b>	-0.53
<b>SDPA</b>	0.213	<b>Uncertainty of AV</b>	0.02
<b>Standard Unit Result Val</b>	3.62	<b>%DEV</b>	2.38

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

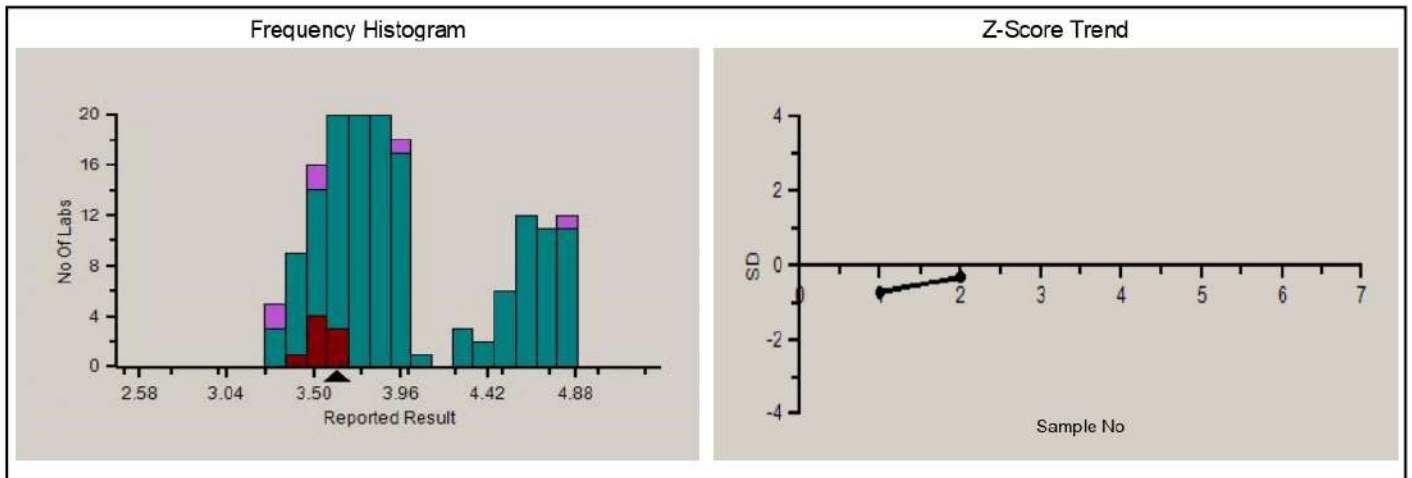

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

**Lab :** 429  
**Lab Name :** NEYVELI DIAGNOSTIC CENTRE  
**Report Date :** 19/03/2021

**Cycle No :** 210103  
**Sample No :** 2  
**Sample Date :** 03-03-2021

<b>Biochemistry, Albumin</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	166	3.97	0.46	11.62	6
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>7</b>	<b>3.54</b>	<b>0.08</b>	<b>2.29</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	31	4.64	0.14	2.99	--
	Roche cobas c 311	28	3.78	0.11	3.01	--
	Roche cobas c 311	27	3.79	0.11	2.98	--
	Fuji Dri-Chem 4000i	16	4.62	0.16	3.49	1
	Roche cobas c 111	11	3.85	0.10	2.50	--
	Horiba ABX Pentra C200	10	3.51	0.11	3.02	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, ALP, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	165	87.51	15.30	17.48	18
IFCC	18	79.40	15.45	19.46	4
Erba EM 200	5	80.70	3.75	4.64	2

<b>Your Result</b>	78.11	<b>SDI / z-Score</b>	0.05
<b>Assigned Value</b>	77.44	<b>Average SDI</b>	-0.18
<b>SDPA</b>	13.927	<b>Uncertainty of AV</b>	0.61
<b>Standard Unit Result Val</b>	78.11	<b>%DEV</b>	-3.21

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

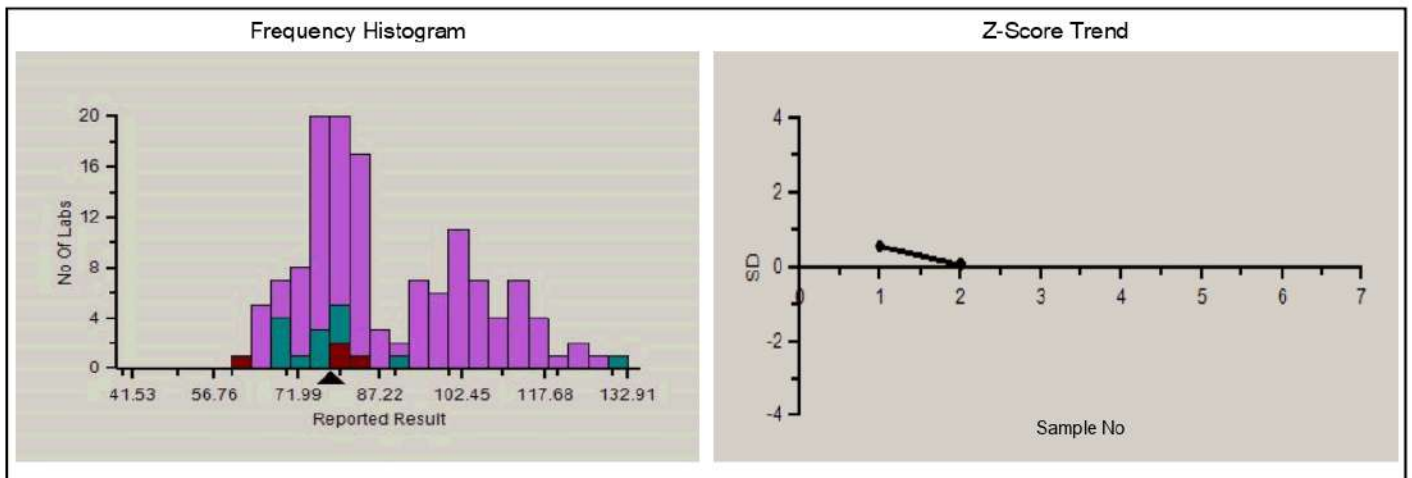

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

<b>Biochemistry, ALP</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	165	87.51	15.30	17.48	18
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>5</b>	<b>80.70</b>	<b>3.75</b>	<b>4.64</b>	<b>2</b>
	Fuji Dri-Chem NX500/i	33	108.33	9.10	8.40	—
	Roche cobas c 311	28	77.40	3.59	4.64	—
	Roche cobas c 311	27	77.38	3.66	4.73	—
	Fuji Dri-Chem 4000i	16	104.20	7.87	7.55	1
	Roche cobas c 111	12	76.56	8.14	10.63	—
	Roche cobas c 111	11	75.16	6.85	9.11	—

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.






PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021


**Biochemistry, ALT, U/L**

	N	Mean	SD	CV%	Excluded
 All Methods	170	14.49	5.73	39.56	35
 IFCC	17	11.75	1.96	16.69	2
 Erba EM 200	7	13.41	1.77	13.16	1

<b>Your Result</b>	11.55	<b>SDI / z-Score</b>	-0.52
<b>Assigned Value</b>	12.97	<b>Average SDI</b>	1.03
<b>SDPA</b>	2.720	<b>Uncertainty of AV</b>	0.50
<b>Standard Unit Result Val</b>	11.55	<b>%DEV</b>	-13.86

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

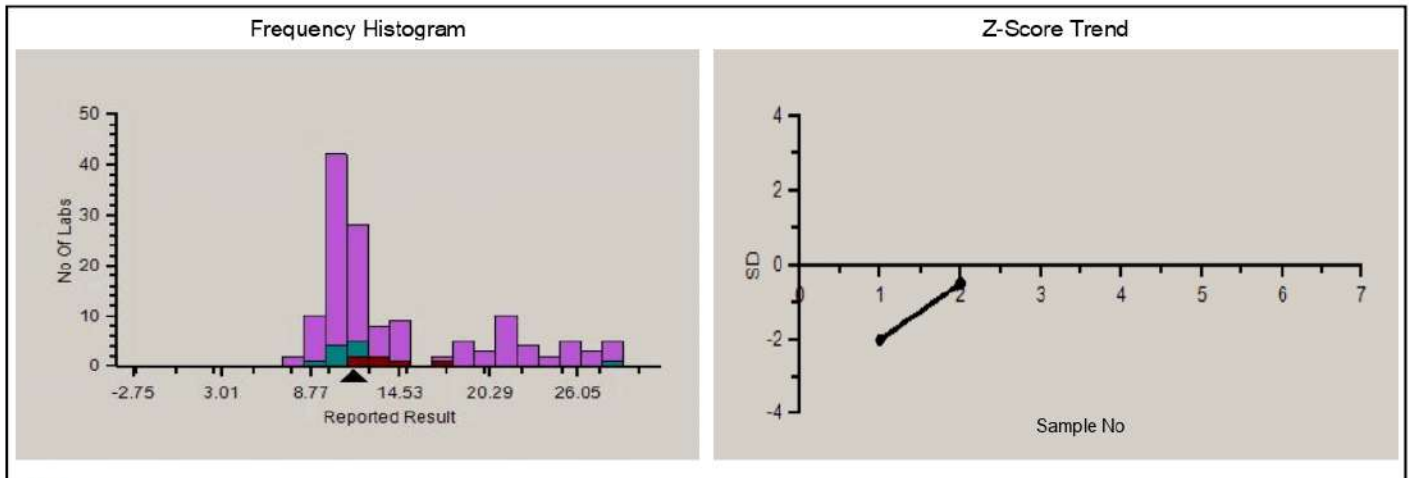

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

Biochemistry, ALT		N	Mean	SD	CV%	Excluded
All Analyzer		170	14.49	5.73	39.56	35
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>7</b>	<b>13.41</b>	<b>1.77</b>	<b>13.16</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	32	23.11	3.35	14.49	11
	Roche cobas c 311	28	10.83	1.25	11.57	1
	Roche cobas c 311	27	10.81	1.27	11.77	1
	Fuji Dri-Chem 4000i	16	23.36	2.50	10.71	5
	Roche cobas c 111	12	10.09	1.24	12.30	2
	Horiba ABX Pentra C200	11	11.23	1.29	11.50	1

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, Amylase, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	99	60.37	7.20	11.93	10
CNP-triose/CNPG3	14	54.89	9.83	17.91	3
Erba EM 200	1	--	--	--	--

<b>Your Result</b>	46.00	<b>SDI / z-Score</b>	-1.55
<b>Assigned Value</b>	55.48	<b>Average SDI</b>	0.55
<b>SDPA</b>	6.103	<b>Uncertainty of AV</b>	0.68
<b>Standard Unit Result Val</b>	46.00	<b>%DEV</b>	-16.20

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

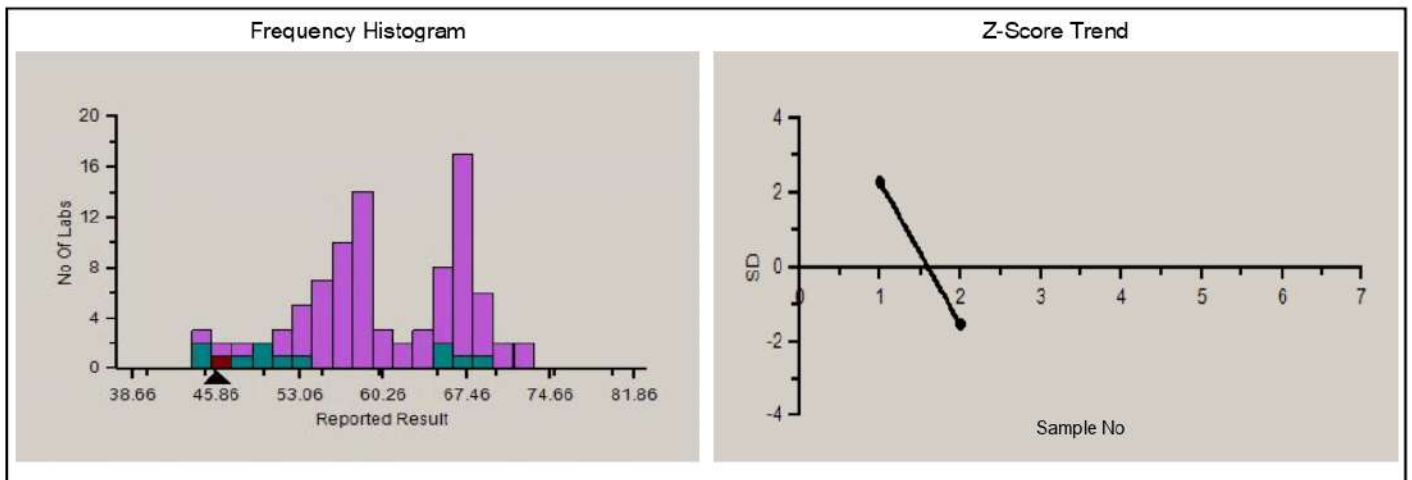

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

<b>Biochemistry, Amylase</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	99	60.37	7.20	11.93	10
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	23	57.00	2.56	4.49	--
	Fuji Dri-Chem 4000i	15	56.67	2.06	3.63	--
	Fuji Dri-Chem 4000i	14	56.43	1.91	3.39	--
	Roche cobas c 311	14	67.64	2.26	3.35	--
	Roche cobas INTEGRA	7	66.98	2.53	3.77	--
	Roche cobas 6000	6	67.18	1.46	2.17	--
	Roche cobas 8000	4	67.75	0.96	1.41	--
	Roche cobas c 111	3	66.90	2.97	4.44	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022



**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, AST, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	167	19.79	2.98	15.05	22
IFCC	18	18.91	2.58	13.61	4
Erba EM 200	7	19.33	2.97	15.35	4

<b>Your Result</b>	18.20	<b>SDI / z-Score</b>	-0.43
<b>Assigned Value</b>	19.92	<b>Average SDI</b>	-1.10
<b>SDPA</b>	3.983	<b>Uncertainty of AV</b>	0.81
<b>Standard Unit Result Val</b>	18.20	<b>%DEV</b>	-5.86

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

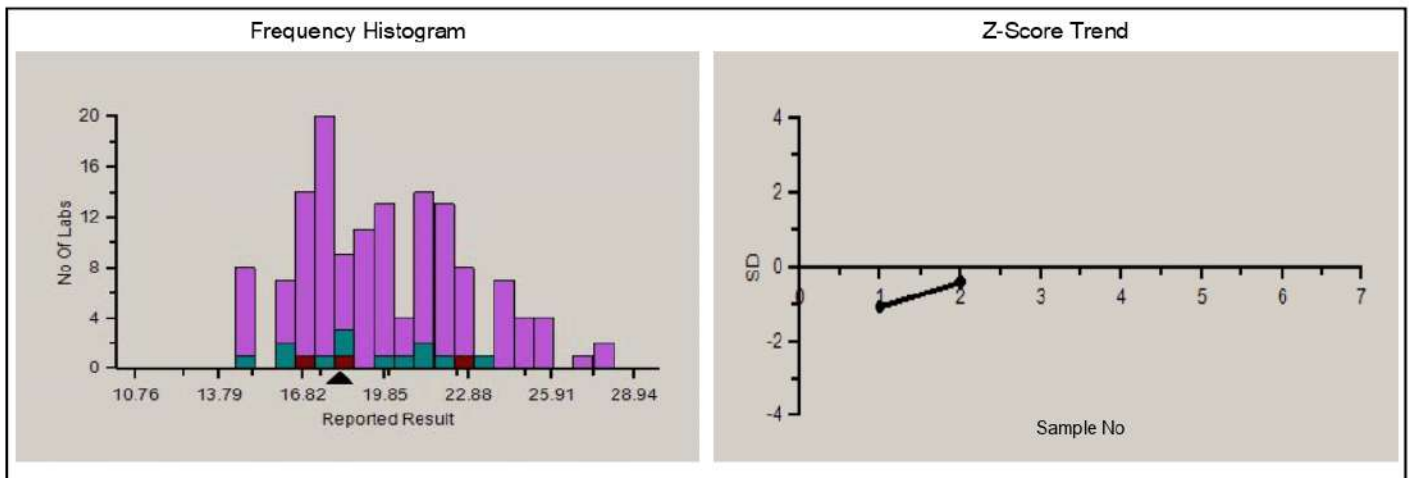

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

Biochemistry, AST		N	Mean	SD	CV%	Excluded
All Analyzer		167	19.79	2.98	15.05	22
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>7</b>	<b>19.33</b>	<b>2.97</b>	<b>15.35</b>	<b>4</b>
	Fuji Dri-Chem NX500/i	32	23.35	2.33	9.99	6
	Roche cobas c 311	27	17.93	1.39	7.77	—
	Roche cobas c 311	26	17.90	1.41	7.87	—
	Fuji Dri-Chem 4000i	16	22.19	2.14	9.63	—
	Roche cobas c 111	13	17.99	1.68	9.35	1
	Roche cobas c 111	12	17.81	1.64	9.18	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, Bilirubin Direct, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	164	0.10	0.02	15.53	39
Diazotization	132	0.10	0.01	14.00	26
Erba EM 200	7	0.12	0.03	23.39	2

<b>Your Result</b>	0.05	<b>SDI / z-Score</b>	-1.30
<b>Assigned Value</b>	0.12	<b>Average SDI</b>	-0.94
<b>SDPA</b>	0.054	<b>Uncertainty of AV</b>	0.01
<b>Standard Unit Result Val</b>	0.05	<b>%DEV</b>	-59.68

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

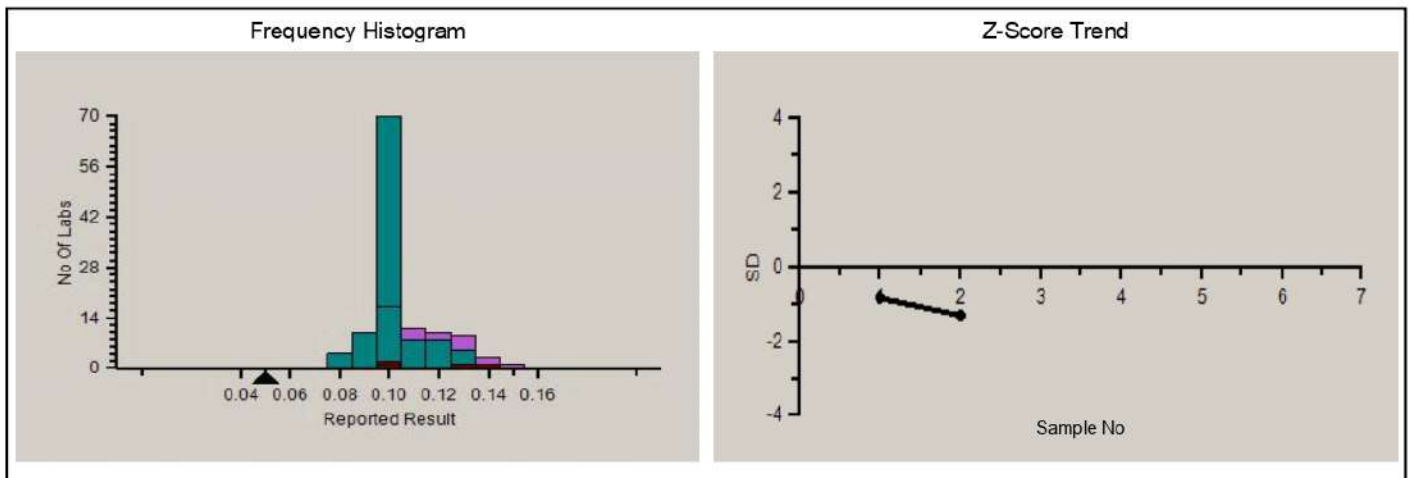

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

**Lab :** 429  
**Lab Name :** NEYVELI DIAGNOSTIC CENTRE  
**Report Date :** 19/03/2021

**Cycle No :** 210103  
**Sample No :** 2  
**Sample Date :** 03-03-2021

<b>Biochemistry, Bilirubin Direct</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	164	0.10	0.02	15.53	39
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>7</b>	<b>0.12</b>	<b>0.03</b>	<b>23.39</b>	<b>2</b>
	Fuji Dri-Chem NX500/i	28	0.10	0.00	4.04	8
	Roche cobas c 311	27	0.09	0.01	13.04	3
	Roche cobas c 311	26	0.09	0.01	13.19	3
	Fuji Dri-Chem 4000i	16	0.10	0.00	0.00	6
	Roche cobas c 111	12	0.11	0.01	11.82	3
	Horiba ABX Pentra C200	11	0.12	0.01	10.17	—

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, Bilirubin Total, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	167	0.33	0.14	42.81	43
Diazotization	43	0.31	0.13	41.69	10
Erba EM 200	7	0.23	0.04	15.35	1

<b>Your Result</b>	0.20	<b>SDI / z-Score</b>	-0.17
<b>Assigned Value</b>	0.21	<b>Average SDI</b>	-0.11
<b>SDPA</b>	0.063	<b>Uncertainty of AV</b>	0.01
<b>Standard Unit Result Val</b>	0.20	<b>%DEV</b>	-12.28

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

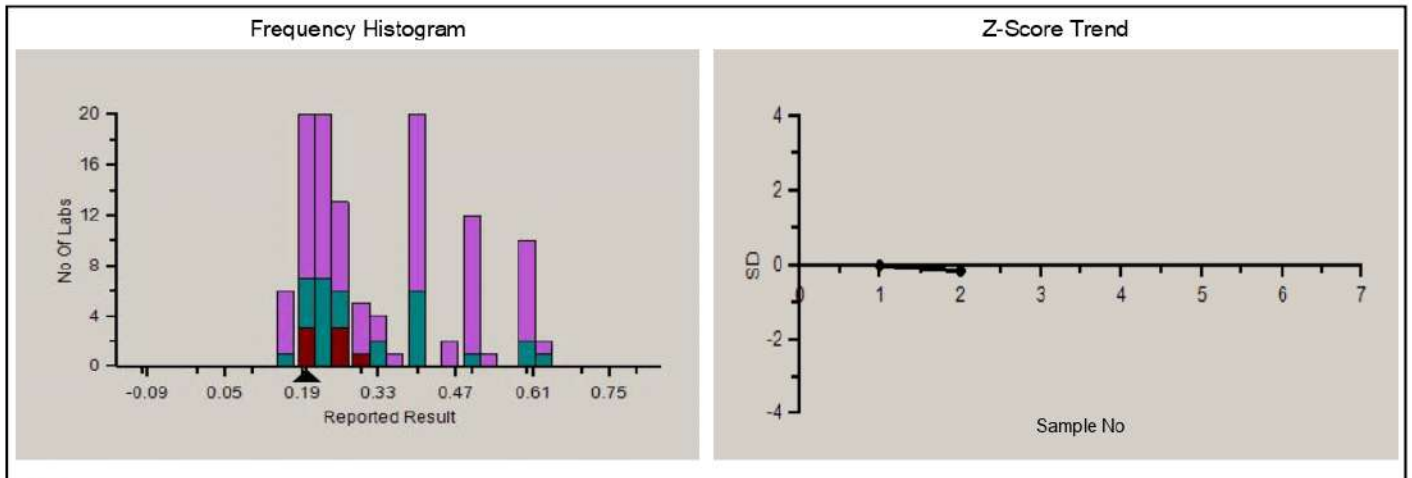

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

<b>Biochemistry, Bilirubin Total</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	167	0.33	0.14	42.81	43
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>7</b>	<b>0.23</b>	<b>0.04</b>	<b>15.35</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	30	0.49	0.08	17.11	7
	Roche cobas c 311	27	0.21	0.03	13.46	3
	Roche cobas c 311	26	0.21	0.03	13.53	3
	Fuji Dri-Chem 4000i	16	0.51	0.09	17.36	1
	Horiba ABX Pentra C200	11	0.24	0.02	9.92	6
	Roche cobas c 111	11	0.22	0.04	18.72	4

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021


**Biochemistry, Calcium, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	156	7.58	0.57	7.57	8
<span style="color: teal;">■</span> Arsenazo I	3	7.78	1.23	15.77	--
<span style="color: red;">■</span> Erba EM 200	5	8.57	0.54	6.34	--

<b>Your Result</b>	9.05	<b>SDI / z-Score</b>	1.39
<b>Assigned Value</b>	8.20	<b>Average SDI</b>	1.01
<b>SDPA</b>	0.611	<b>Uncertainty of AV</b>	0.24
<b>Standard Unit Result Val</b>	9.05	<b>%DEV</b>	5.60

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

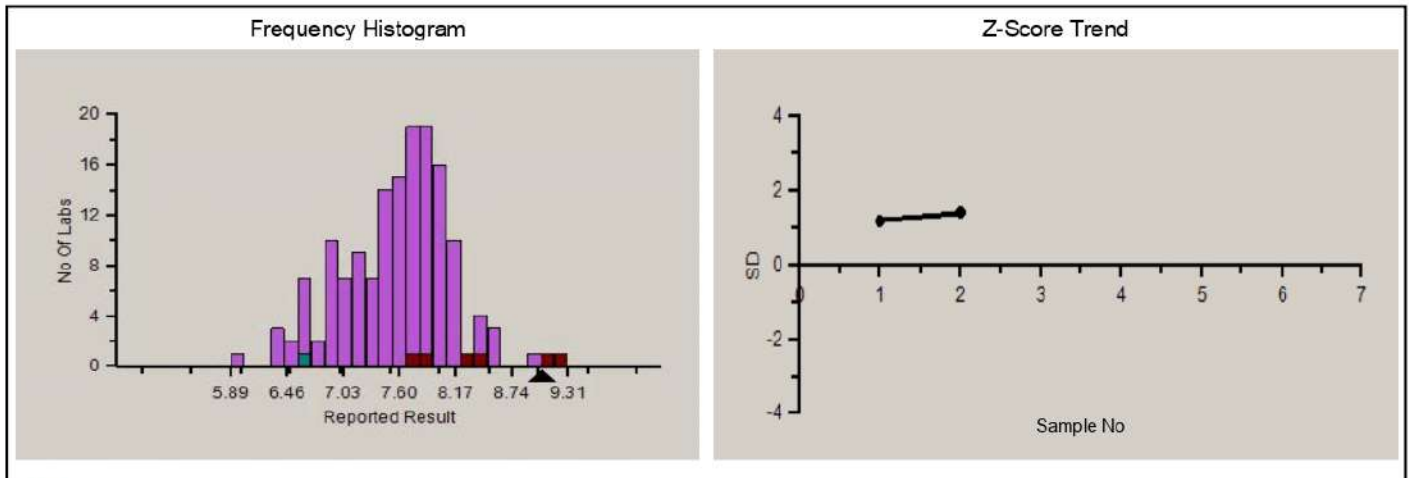

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

Biochemistry, Calcium		N	Mean	SD	CV%	Excluded
	All Analyzer	156	7.58	0.57	7.57	8
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>5</b>	<b>8.57</b>	<b>0.54</b>	<b>6.34</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	28	6.90	0.32	4.61	--
	Roche cobas c 311	25	7.87	0.22	2.80	--
	Roche cobas c 311	24	7.86	0.22	2.81	--
	Fuji Dri-Chem 4000i	16	7.06	0.48	6.73	--
	Roche cobas c 111	11	7.83	0.32	4.13	--
	Roche cobas INTEGRA	11	7.75	0.28	3.67	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022



**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021


**Biochemistry, Chloride, mEq/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	138	105.29	12.55	11.92	15
<span style="color: teal;">■</span> Mercuric thiocyanate, ferric ion	2	0.00	--	--	1
<span style="color: red;">■</span> Erba Chem 7	1	--	--	--	--

<b>Your Result</b>	82.11	<b>SDI / z-Score</b>	-0.86
<b>Assigned Value</b>	86.96	<b>Average SDI</b>	-1.03
<b>SDPA</b>	5.650	<b>Uncertainty of AV</b>	0.44
<b>Standard Unit Result Val</b>	82.11	<b>%DEV</b>	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

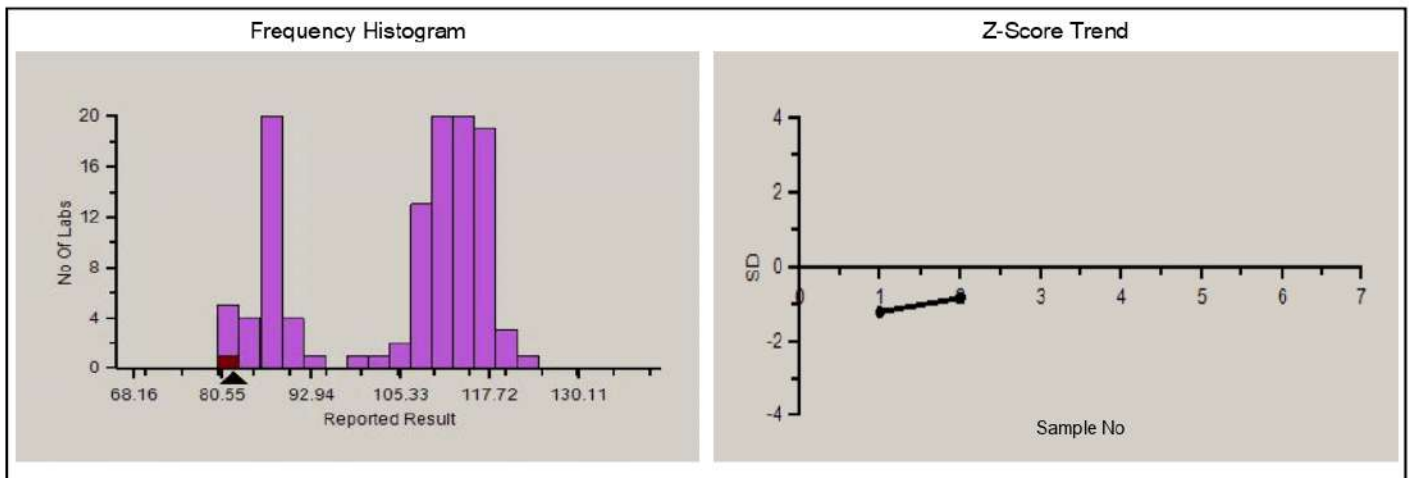

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

<b>Biochemistry, Chloride</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	138	105.29	12.55	11.92	15
<b>Your Analyzer :</b>	<b>Erba Chem 7</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	32	0.00	0.00	0.00	1
	Fuji Dri-Chem 4000i	17	0.00	0.00	0.00	1
	Roche cobas c 311	15	0.00	0.00	0.00	--
	Roche AVL 9180	12	109.27	2.12	1.94	--
	Roche AVL 9180	11	108.93	1.85	1.70	--
	Roche AVL 9180	10	0.00	0.00	0.00	--
	EasyLyte	9	112.61	5.27	4.68	1
	Roche cobas 6000	8	0.00	0.00	0.00	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021


**Biochemistry, GGT, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	135	15.19	4.08	26.87	7
SZASZ IFCC standardized	3	20.38	2.11	10.33	--
Erba EM 200	3	19.05	2.77	14.56	--

<b>Your Result</b>	21.14	<b>SDI / z-Score</b>	1.71
<b>Assigned Value</b>	17.54	<b>Average SDI</b>	1.23
<b>SDPA</b>	2.104	<b>Uncertainty of AV</b>	0.24
<b>Standard Unit Result Val</b>	21.14	<b>%DEV</b>	3.73

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

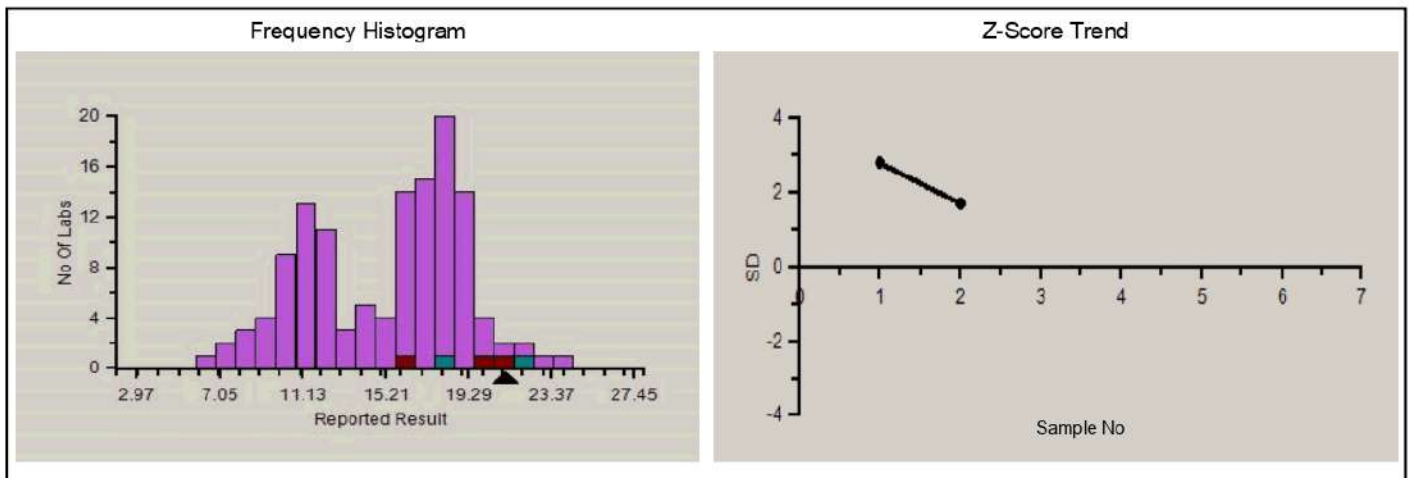

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

**Lab :** 429  
**Lab Name :** NEYVELI DIAGNOSTIC CENTRE  
**Report Date :** 19/03/2021

**Cycle No :** 210103  
**Sample No :** 2  
**Sample Date :** 03-03-2021

<b>Biochemistry, GGT</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	135	15.19	4.08	26.87	7
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>3</b>	<b>19.05</b>	<b>2.77</b>	<b>14.56</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	32	11.17	1.28	11.49	3
	Roche cobas c 311	25	17.57	1.20	6.83	1
	Roche cobas c 311	24	17.57	1.20	6.83	1
	Fuji Dri-Chem 4000i	12	10.33	1.16	11.18	--
	Roche cobas INTEGRA	11	16.07	1.33	8.25	--
	Roche cobas c 111	10	17.46	3.05	17.48	1
	Beckman Coulter AU480	6	18.38	0.88	4.81	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.






PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, Potassium, mEq/L**

	N	Mean	SD	CV%	Excluded
 All Methods	149	5.70	0.93	16.35	10
 Colorimetric	2	0.00	--	--	1
 Erba Chem 7	1	--	--	--	--

<b>Your Result</b>	3.92	<b>SDI / z-Score</b>	-1.51
<b>Assigned Value</b>	4.24	<b>Average SDI</b>	-1.83
<b>SDPA</b>	0.212	<b>Uncertainty of AV</b>	0.02
<b>Standard Unit Result Val</b>	3.92	<b>%DEV</b>	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

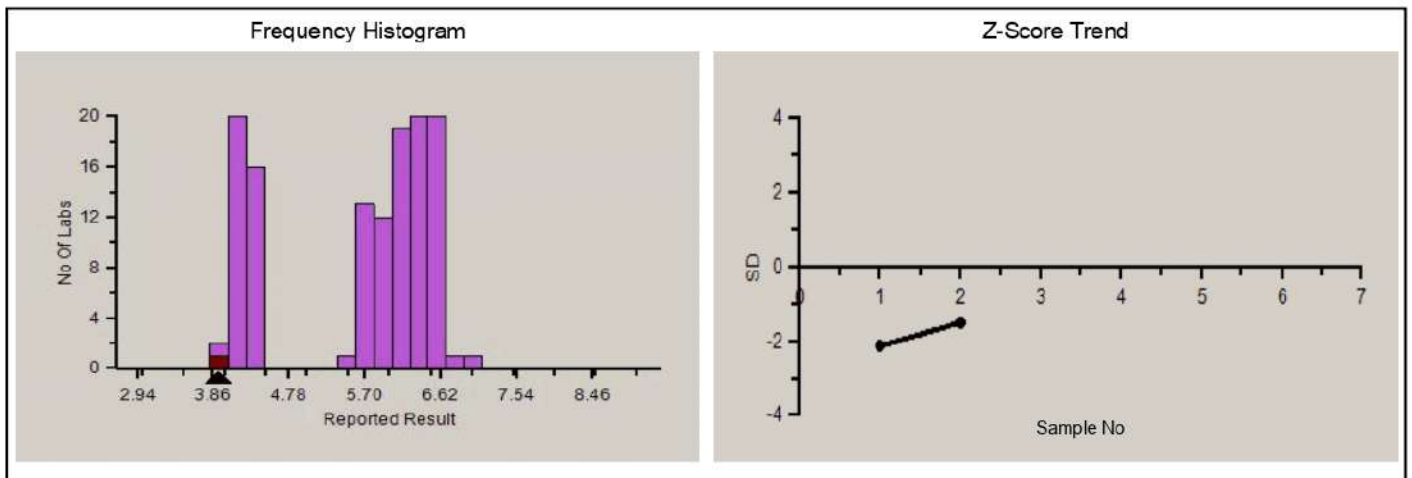

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

<b>Biochemistry, Potassium</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	149	5.70	0.93	16.35	10
<b>Your Analyzer :</b>	<b>Erba Chem 7</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	33	0.00	0.00	0.00	1
	Fuji Dri-Chem 4000i	19	0.00	0.00	0.00	1
	Roche cobas c 311	15	0.00	0.00	0.00	--
	Roche AVL 9180	14	6.23	0.38	6.17	--
	Roche AVL 9180	13	6.27	0.37	5.87	--
	Roche AVL 9180	12	0.00	0.00	0.00	--
	EasyLyte	10	5.83	0.14	2.42	--
	EasyLyte	9	0.00	0.00	0.00	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.






PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 2  
Sample Date : 03-03-2021


**Biochemistry, Sodium, mEq/L**

	N	Mean	SD	CV%	Excluded
 All Methods	149	159.00	23.11	14.54	15
 Colorimetric	2	0.00	--	--	1
 Erba EM 200	2	0.00	--	--	--

<b>Your Result</b>	120.10	<b>SDI / z-Score</b>	-0.43
<b>Assigned Value</b>	122.77	<b>Average SDI</b>	-0.19
<b>SDPA</b>	6.130	<b>Uncertainty of AV</b>	0.43
<b>Standard Unit Result Val</b>	120.10	<b>%DEV</b>	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

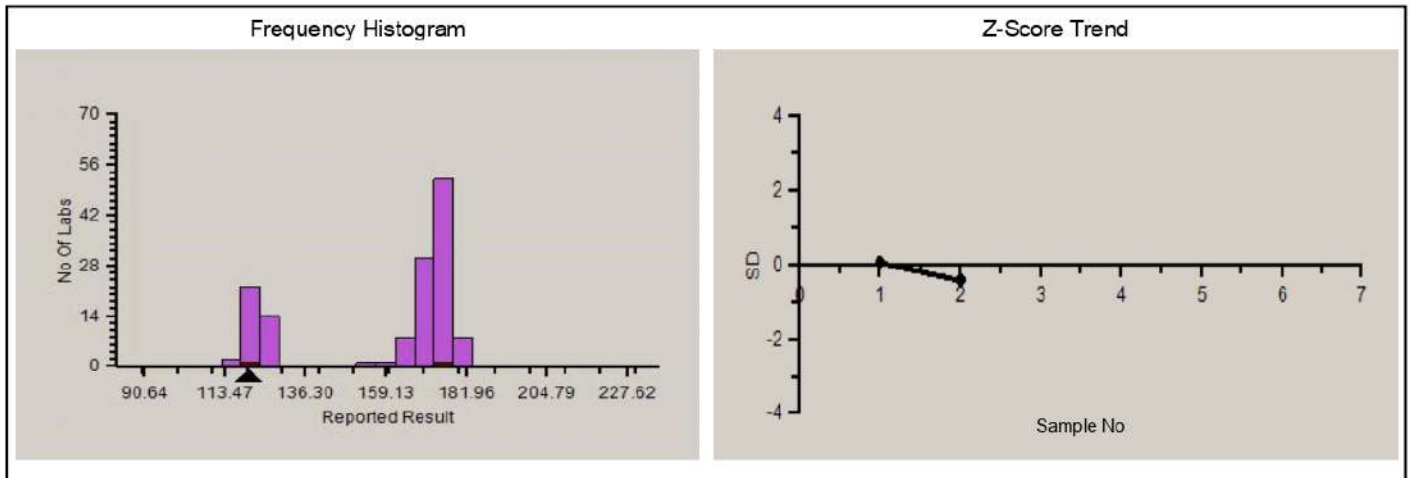

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 2  
 Sample Date : 03-03-2021

<b>Biochemistry, Sodium</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	149	159.00	23.11	14.54	15
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>2</b>	<b>0.00</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	34	0.00	0.00	0.00	3
	Fuji Dri-Chem 4000i	18	0.00	0.00	0.00	2
	Roche cobas c 311	15	0.00	0.00	0.00	--
	Roche AVL 9180	14	173.15	8.81	5.09	--
	Roche AVL 9180	13	174.85	6.33	3.62	--
	Roche AVL 9180	12	0.00	0.00	0.00	--
	EasyLyte	10	170.03	3.27	1.92	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.

*Dr. Nigam*

**Dr Puneet Kumar Nigam**  
**PT coordinator & Technical Manager, MHL EQAS**  
 Unit No. 409-416,  
 Commercial Building - 1A,  
 Kohinoor Mall, Kiroli Road, Kurla (W),  
 Mumbai - 400070



PC-1022



**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 3  
Sample Date : 03-03-2021


**Biochemistry, Cholesterol, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	163	149.43	8.19	5.48	6
CHOD-POD	15	148.39	7.83	5.28	--
Erba EM 200	5	153.84	6.76	4.39	--

<b>Your Result</b>	148.20	<b>SDI / z-Score</b>	-0.45
<b>Assigned Value</b>	151.05	<b>Average SDI</b>	-0.50
<b>SDPA</b>	6.392	<b>Uncertainty of AV</b>	0.80
<b>Standard Unit Result Val</b>	148.20	<b>%DEV</b>	-3.67

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

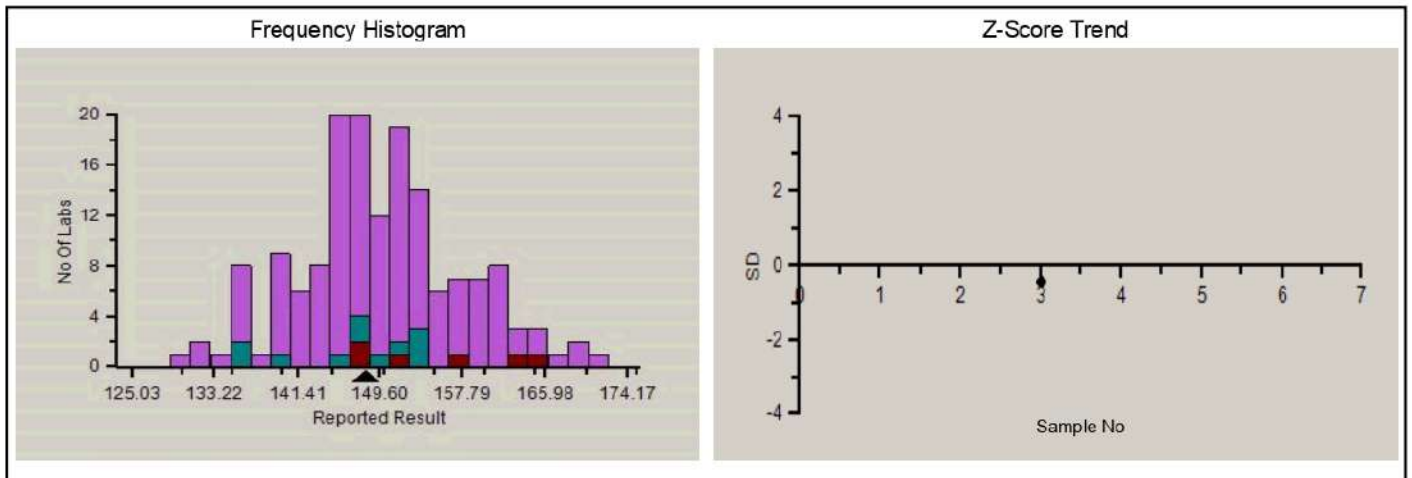

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 3  
 Sample Date : 03-03-2021

<b>Biochemistry, Cholesterol</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	163	149.43	8.19	5.48	6
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>5</b>	<b>153.84</b>	<b>6.76</b>	<b>4.39</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	30	143.06	6.14	4.29	2
	Roche cobas c 311	29	150.10	4.42	2.94	--
	Roche cobas c 311	28	150.00	4.46	2.97	--
	Fuji Dri-Chem 4000i	16	143.93	8.00	5.56	--
	Roche cobas c 111	12	150.37	4.83	3.22	--
	Roche cobas c 111	11	150.68	4.95	3.28	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.






PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 3  
Sample Date : 03-03-2021


**Biochemistry, Creatinine, mg/dl**

	N	Mean	SD	CV%	Excluded
 All Methods	167	0.71	0.21	29.07	11
 Jaffe's Kinetic	2	0.67	--	--	--
 Erba EM 200	6	0.75	0.10	13.02	--

<b>Your Result</b>	0.62	<b>SDI / z-Score</b>	-0.19
<b>Assigned Value</b>	0.80	<b>Average SDI</b>	-0.83
<b>SDPA</b>	0.954	<b>Uncertainty of AV</b>	0.01
<b>Standard Unit Result Val</b>	0.62	<b>%DEV</b>	-17.66

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

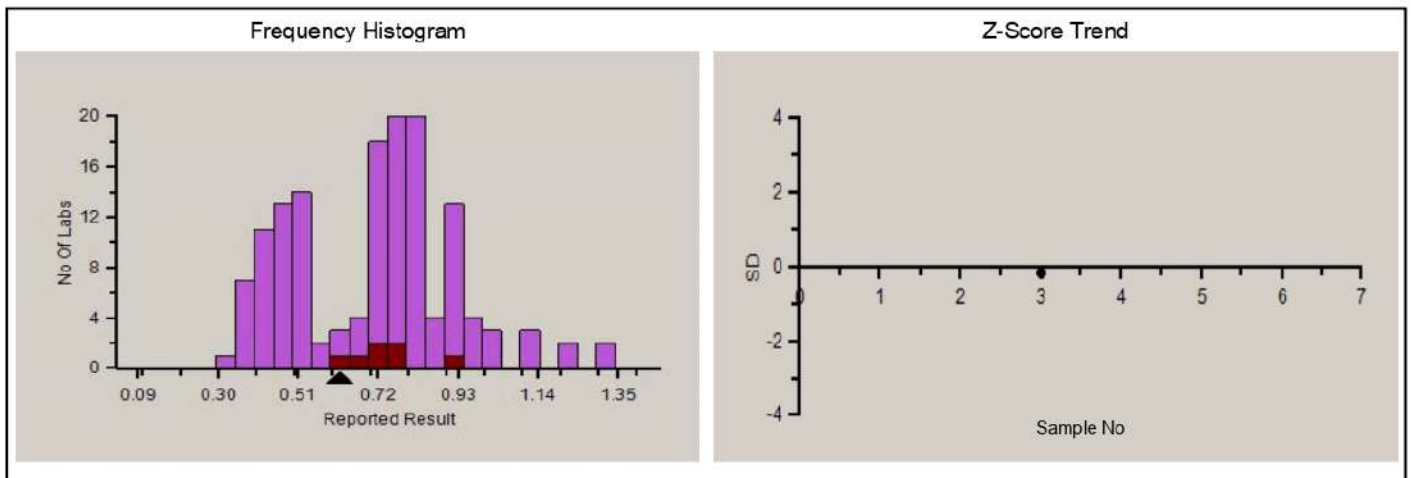

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 3  
 Sample Date : 03-03-2021

<b>Biochemistry, Creatinine</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	167	0.71	0.21	29.07	11
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>6</b>	<b>0.75</b>	<b>0.10</b>	<b>13.02</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	29	0.43	0.05	11.48	2
	Roche cobas c 311	29	0.78	0.05	6.42	--
	Roche cobas c 311	28	0.78	0.05	6.31	--
	Fuji Dri-Chem 4000i	16	0.47	0.05	10.62	2
	Roche cobas c 111	12	0.79	0.07	9.25	--
	Horiba ABX Pentra C200	11	0.89	0.10	10.86	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.






PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 3  
Sample Date : 03-03-2021


**Biochemistry, Glucose, mg/dl**

	N	Mean	SD	CV%	Excluded
 All Methods	171	73.92	3.52	4.76	10
 GPO-POD	15	74.15	4.95	6.67	1
 Erba EM 200	5	79.30	2.26	2.85	1

<b>Your Result</b>	80.01	<b>SDI / z-Score</b>	0.84
<b>Assigned Value</b>	75.28	<b>Average SDI</b>	0.33
<b>SDPA</b>	5.646	<b>Uncertainty of AV</b>	0.32
<b>Standard Unit Result Val</b>	80.01	<b>%DEV</b>	0.89

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

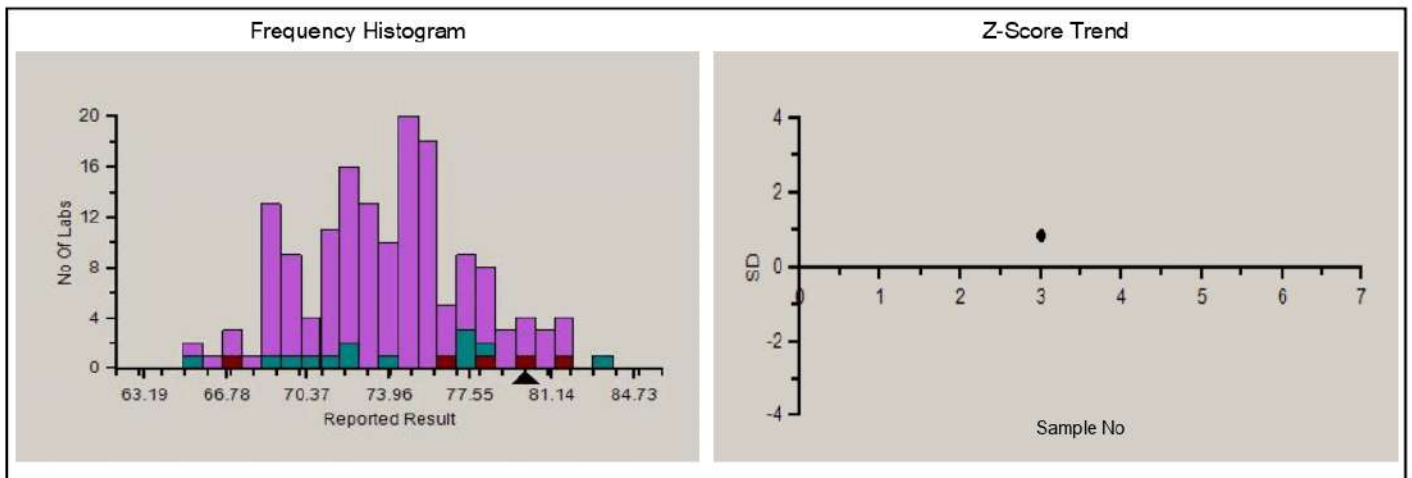

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

**Lab :** 429  
**Lab Name :** NEYVELI DIAGNOSTIC CENTRE  
**Report Date :** 19/03/2021

**Cycle No :** 210103  
**Sample No :** 3  
**Sample Date :** 03-03-2021

<b>Biochemistry, Glucose</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	171	73.92	3.52	4.76	10
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>5</b>	<b>79.30</b>	<b>2.26</b>	<b>2.85</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	31	70.97	2.50	3.52	—
	Roche cobas c 311	29	75.76	2.54	3.36	—
	Fuji Dri-Chem 4000i	17	71.13	2.03	2.85	1
	Fuji Dri-Chem 4000i	16	70.87	1.81	2.55	1
	Horiba ABX Pentra C200	12	74.11	2.92	3.94	—
	Roche cobas c 111	11	75.64	1.35	1.79	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 3  
Sample Date : 03-03-2021


**Biochemistry, HDL, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	152	35.32	3.95	11.18	3
<span style="color: teal;">■</span> Direct measure-PEG	22	36.43	3.61	9.91	2
<span style="color: red;">■</span> Erba EM 200	5	38.08	5.66	14.86	2

<b>Your Result</b>	31.55	<b>SDI / z-Score</b>	-1.43
<b>Assigned Value</b>	41.35	<b>Average SDI</b>	-1.48
<b>SDPA</b>	6.834	<b>Uncertainty of AV</b>	3.49
<b>Standard Unit Result Val</b>	31.55	<b>%DEV</b>	-17.15

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

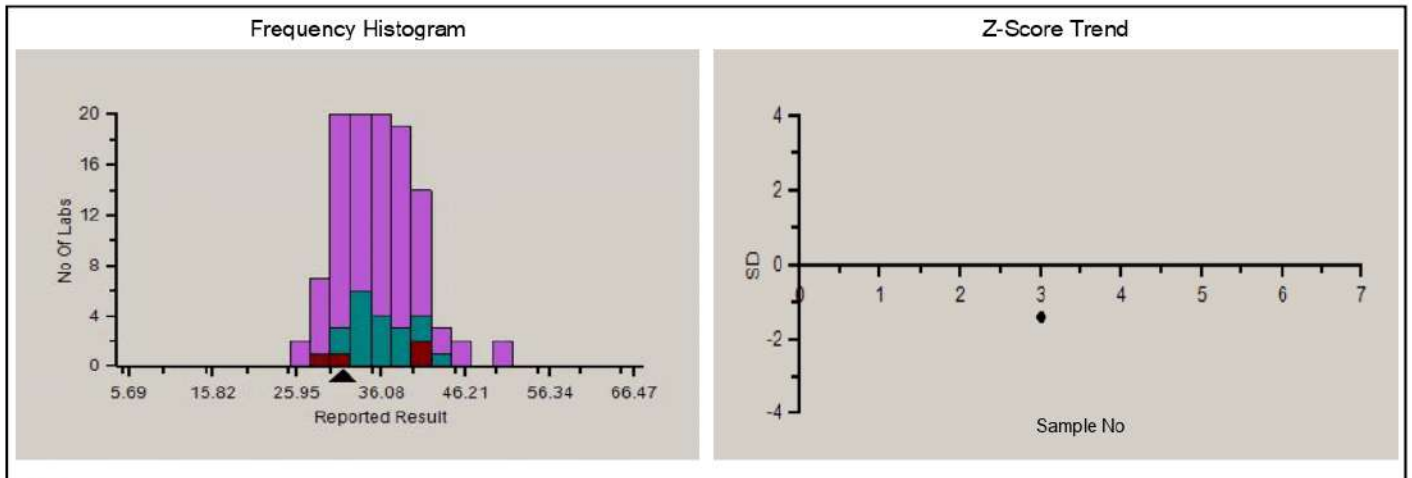

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 3  
 Sample Date : 03-03-2021

Biochemistry, HDL		N	Mean	SD	CV%	Excluded
All Analyzer		152	35.32	3.95	11.18	3
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>5</b>	<b>38.08</b>	<b>5.66</b>	<b>14.86</b>	<b>2</b>
	Fuji Dri-Chem NX500/i	31	36.00	2.14	5.96	—
	Roche cobas c 311	28	32.76	2.10	6.42	—
	Roche cobas c 311	27	32.84	2.10	6.40	—
	Fuji Dri-Chem 4000i	15	35.93	2.79	7.76	—
	Roche cobas c 111	12	31.11	2.08	6.70	—
	Roche cobas c 111	11	30.95	2.10	6.80	—

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022



**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 3  
Sample Date : 03-03-2021


**Biochemistry, LDL, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	60	97.67	7.31	7.48	5
Direct measure	21	97.22	9.55	9.82	2
Erba EM 200	1	--	--	--	--

<b>Your Result</b>	97.02	<b>SDI / z-Score</b>	-0.26
<b>Assigned Value</b>	99.32	<b>Average SDI</b>	-0.26
<b>SDPA</b>	8.939	<b>Uncertainty of AV</b>	0.71
<b>Standard Unit Result Val</b>	97.02	<b>%DEV</b>	-0.21

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

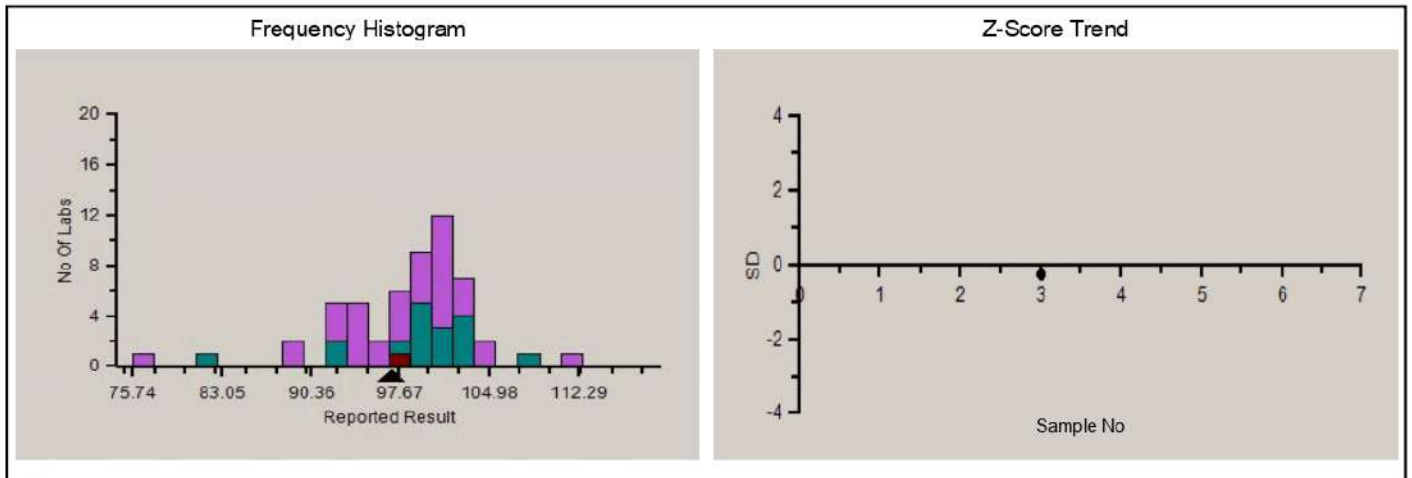

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

**Lab :** 429  
**Lab Name :** NEYVELI DIAGNOSTIC CENTRE  
**Report Date :** 19/03/2021

**Cycle No :** 210103  
**Sample No :** 3  
**Sample Date :** 03-03-2021

<b>Biochemistry, LDL</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	60	97.67	7.31	7.48	5
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Roche cobas c 311	21	99.32	4.63	4.66	--
	Roche cobas 6000	7	101.24	2.27	2.24	--
	Roche cobas INTEGRA	6	100.00	3.27	3.27	--
	Horiba ABX Pentra C200	4	85.64	7.97	9.30	--
	Roche cobas c 111	4	99.24	6.44	6.49	1
	Erba EM 360	3	92.40	0.00	0.00	2
	Roche cobas 8000	3	100.93	3.32	3.29	--
	Beckman Coulter AU480	2	101.15	--	--	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 3  
Sample Date : 03-03-2021


**Biochemistry, Urea, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	163	23.67	3.40	14.37	18
Urease, GLDH	28	25.90	2.25	8.70	4
Erba EM 200	5	25.88	1.19	4.59	1

<b>Your Result</b>	21.15	<b>SDI / z-Score</b>	-1.48
<b>Assigned Value</b>	25.50	<b>Average SDI</b>	-1.13
<b>SDPA</b>	2.932	<b>Uncertainty of AV</b>	0.18
<b>Standard Unit Result Val</b>	21.15	<b>%DEV</b>	-18.26

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

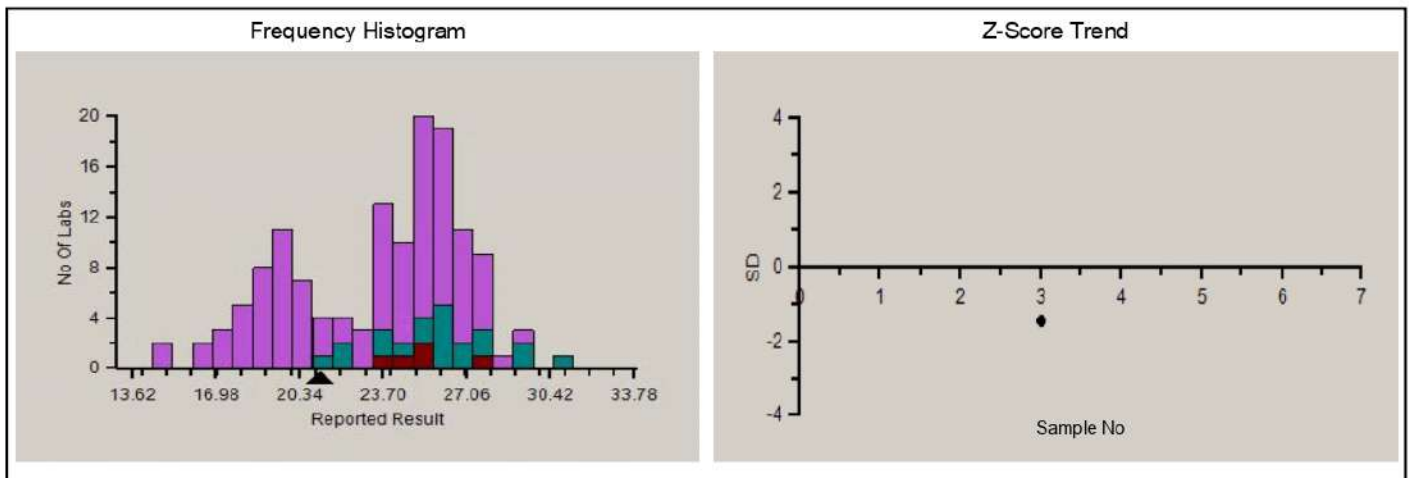

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 3  
 Sample Date : 03-03-2021

Biochemistry, Urea		N	Mean	SD	CV%	Excluded
All Analyzer		163	23.67	3.40	14.37	18
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>5</b>	<b>25.88</b>	<b>1.19</b>	<b>4.59</b>	<b>1</b>
	Roche cobas c 311	29	25.78	1.17	4.54	—
	Roche cobas c 311	28	25.81	1.18	4.59	—
	Fuji Dri-Chem NX500/i	25	19.04	1.41	7.41	4
	Fuji Dri-Chem 4000i	16	19.53	0.65	3.34	2
	Horiba ABX Pentra C200	12	27.13	0.88	3.25	3
	Roche cobas c 111	12	24.84	0.73	2.92	—

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.

*Dr. Puneet Kumar Nigam*

**Dr Puneet Kumar Nigam**  
**PT coordinator & Technical Manager, MHL EQAS**  
 Unit No. 409-416,  
 Commercial Building - 1A,  
 Kohinoor Mall, Kiroli Road, Kurla (W),  
 Mumbai - 400070



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 4  
Sample Date : 03-03-2021


**Biochemistry, Cholesterol, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	162	148.57	7.99	5.38	6
CHOD-POD	14	148.69	8.01	5.39	1
Erba EM 200	5	152.84	8.13	5.32	--

<b>Your Result</b>	146.20	<b>SDI / z-Score</b>	-0.55
<b>Assigned Value</b>	150.36	<b>Average SDI</b>	-0.50
<b>SDPA</b>	7.518	<b>Uncertainty of AV</b>	0.74
<b>Standard Unit Result Val</b>	146.20	<b>%DEV</b>	-4.34

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

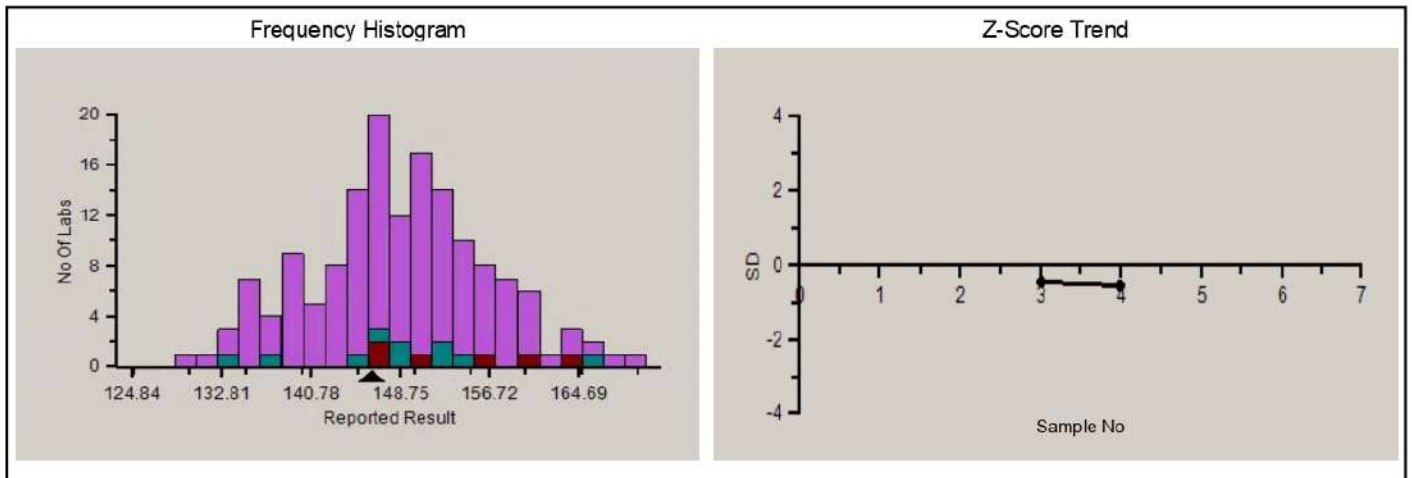

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

**Lab :** 429  
**Lab Name :** NEYVELI DIAGNOSTIC CENTRE  
**Report Date :** 19/03/2021

**Cycle No :** 210103  
**Sample No :** 4  
**Sample Date :** 03-03-2021

<b>Biochemistry, Cholesterol</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	162	148.57	7.99	5.38	6
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>5</b>	<b>152.84</b>	<b>8.13</b>	<b>5.32</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	31	141.82	5.36	3.78	2
	Roche cobas c 311	28	149.70	4.10	2.74	--
	Roche cobas c 311	27	149.61	4.15	2.78	--
	Fuji Dri-Chem 4000i	16	142.96	6.31	4.41	--
	Roche cobas c 111	12	149.17	6.24	4.18	1
	Roche cobas c 111	11	149.38	6.53	4.37	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.






PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 4  
Sample Date : 03-03-2021


**Biochemistry, Creatinine, mg/dl**

	N	Mean	SD	CV%	Excluded
 All Methods	165	0.59	0.17	28.43	17
 Jaffe's Kinetic	2	0.61	--	--	1
 Erba EM 200	6	0.69	0.08	12.17	1

<b>Your Result</b>	0.50	<b>SDI / z-Score</b>	-2.26
<b>Assigned Value</b>	0.69	<b>Average SDI</b>	-0.83
<b>SDPA</b>	0.082	<b>Uncertainty of AV</b>	0.01
<b>Standard Unit Result Val</b>	0.50	<b>%DEV</b>	-27.54

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

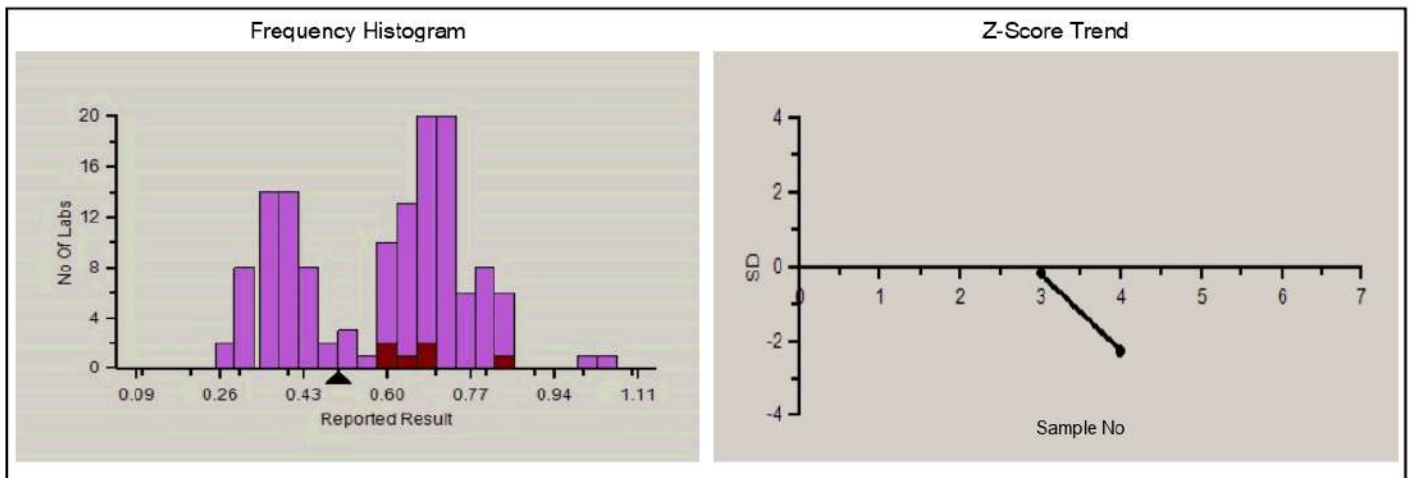

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 4  
 Sample Date : 03-03-2021

<b>Biochemistry, Creatinine</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	165	0.59	0.17	28.43	17
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>6</b>	<b>0.69</b>	<b>0.08</b>	<b>12.17</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	29	0.36	0.05	13.65	2
	Roche cobas c 311	28	0.67	0.05	6.98	—
	Roche cobas c 311	27	0.67	0.05	6.86	—
	Fuji Dri-Chem 4000i	16	0.38	0.04	10.94	—
	Roche cobas c 111	12	0.69	0.07	10.15	—
	Horiba ABX Pentra C200	11	0.76	0.06	8.33	4

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022



**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 4  
Sample Date : 03-03-2021


**Biochemistry, Glucose, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	169	76.08	3.72	4.89	10
<span style="color: teal;">■</span> GPO-POD	15	77.56	5.03	6.49	2
<span style="color: red;">■</span> Erba EM 200	5	80.54	2.24	2.78	1

<b>Your Result</b>	78.25	<b>SDI / z-Score</b>	0.12
<b>Assigned Value</b>	77.56	<b>Average SDI</b>	0.33
<b>SDPA</b>	5.971	<b>Uncertainty of AV</b>	0.31
<b>Standard Unit Result Val</b>	78.25	<b>%DEV</b>	-2.84

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

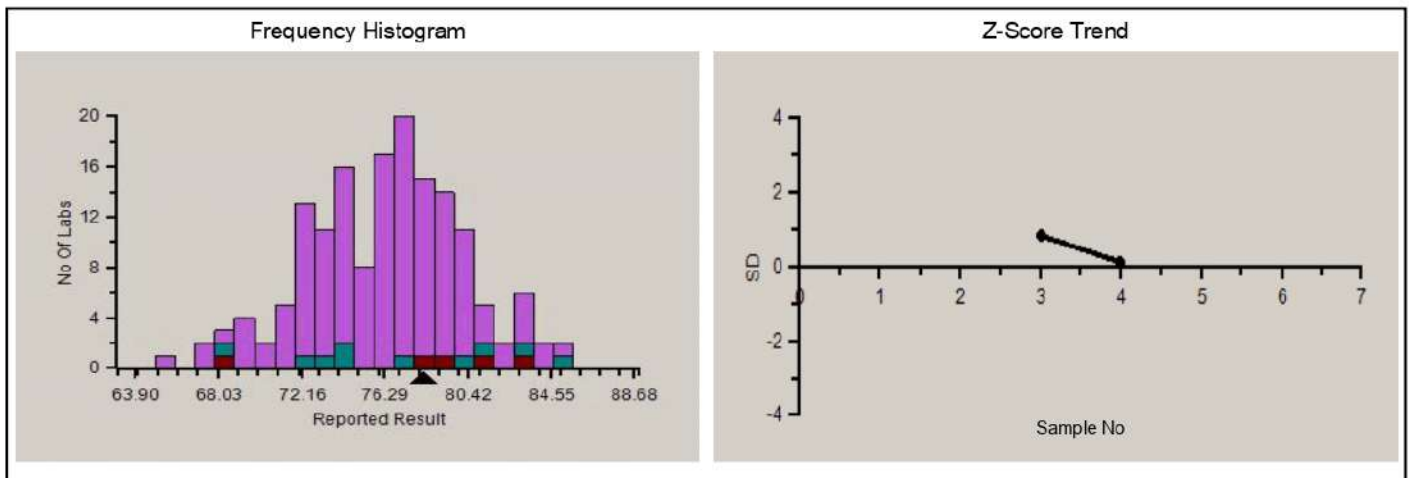

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 4  
 Sample Date : 03-03-2021

<b>Biochemistry, Glucose</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	169	76.08	3.72	4.89	10
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>5</b>	<b>80.54</b>	<b>2.24</b>	<b>2.78</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	31	72.88	2.81	3.86	—
	Roche cobas c 311	28	77.76	2.48	3.18	—
	Fuji Dri-Chem 4000i	17	73.53	1.91	2.60	1
	Fuji Dri-Chem 4000i	16	73.27	1.67	2.28	1
	Horiba ABX Pentra C200	12	76.63	3.10	4.05	—
	Roche cobas c 111	11	78.13	1.94	2.49	3

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 4  
Sample Date : 03-03-2021


**Biochemistry, HDL, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	151	35.67	3.78	10.61	6
Direct measure-PEG	22	37.19	3.30	8.87	2
Erba EM 200	5	38.65	5.65	14.61	2

<b>Your Result</b>	32.16	<b>SDI / z-Score</b>	-1.54
<b>Assigned Value</b>	41.40	<b>Average SDI</b>	-1.48
<b>SDPA</b>	6.012	<b>Uncertainty of AV</b>	3.36
<b>Standard Unit Result Val</b>	32.16	<b>%DEV</b>	-16.80

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

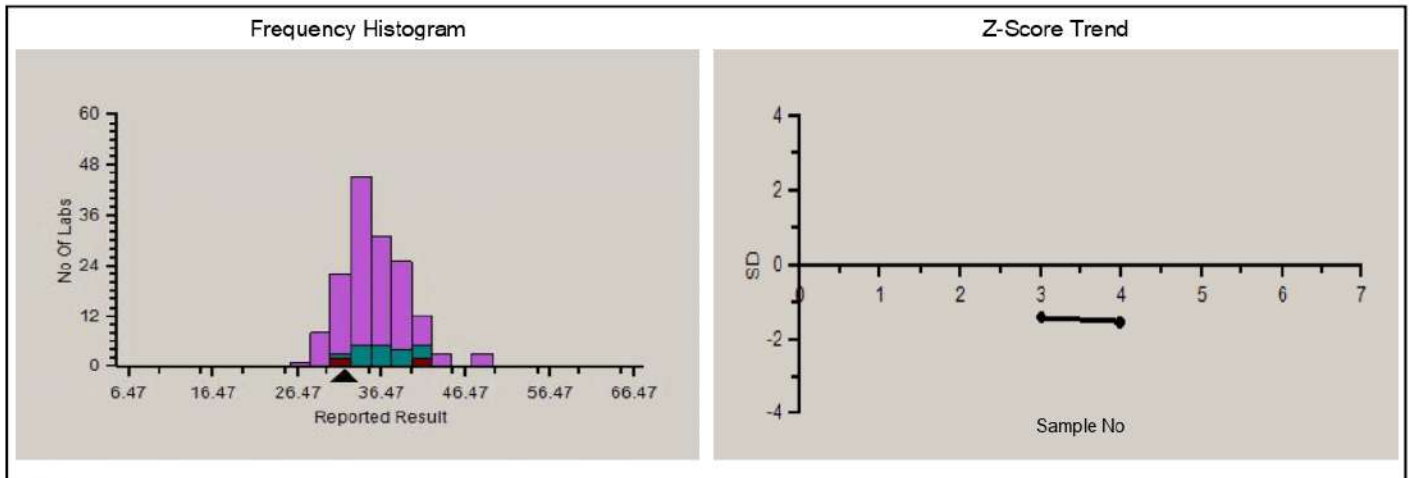

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 4  
 Sample Date : 03-03-2021

<b>Biochemistry, HDL</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	151	35.67	3.78	10.61	6
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>5</b>	<b>38.65</b>	<b>5.65</b>	<b>14.61</b>	<b>2</b>
	Fuji Dri-Chem NX500/i	30	36.22	1.84	5.07	—
	Roche cobas c 311	28	33.15	1.99	5.99	—
	Roche cobas c 311	27	33.19	2.02	6.07	—
	Fuji Dri-Chem 4000i	15	36.86	2.03	5.52	1
	Roche cobas c 111	12	31.24	2.12	6.80	—
	Roche cobas c 111	11	30.96	1.99	6.41	—

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.






PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 4  
 Sample Date : 03-03-2021


**Biochemistry, LDL, mg/dl**

	N	Mean	SD	CV%	Excluded
 All Methods	59	96.14	6.18	6.43	5
 Direct measure	20	96.23	7.49	7.78	1
 Erba EM 200	1	--	--	--	--

<b>Your Result</b>	96.02	<b>SDI / z-Score</b>	-0.25
<b>Assigned Value</b>	97.99	<b>Average SDI</b>	-0.26
<b>SDPA</b>	7.838	<b>Uncertainty of AV</b>	0.69
<b>Standard Unit Result Val</b>	96.02	<b>%DEV</b>	-0.22

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

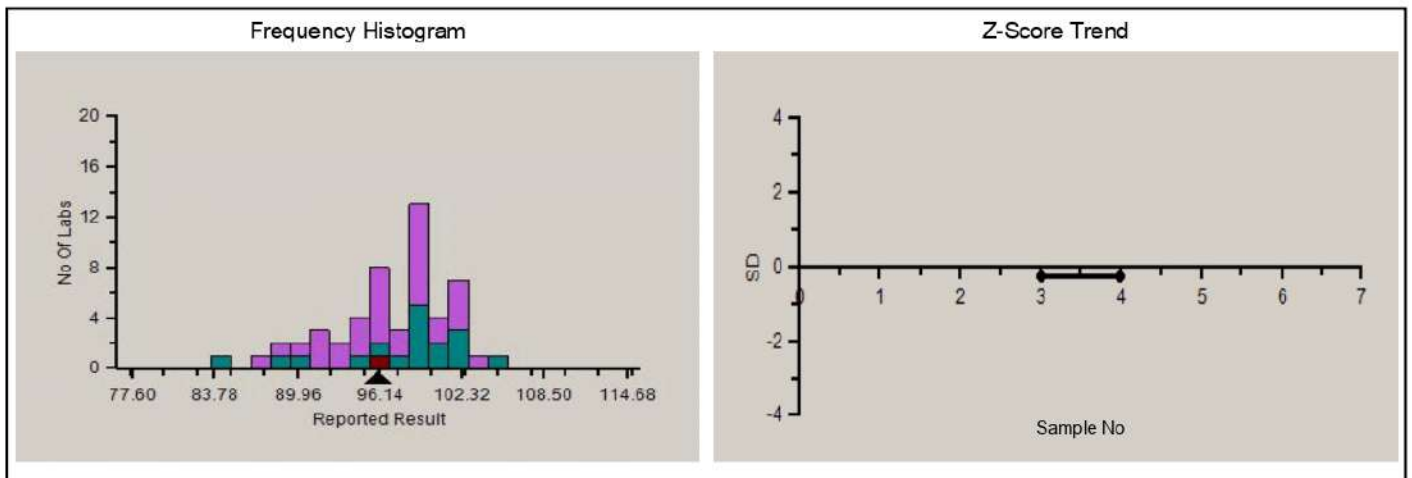

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 4  
 Sample Date : 03-03-2021

<b>Biochemistry, LDL</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	59	96.14	6.18	6.43	5
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Roche cobas c 311	21	97.30	3.93	4.04	1
	Roche cobas 6000	7	99.50	1.98	1.99	--
	Roche cobas INTEGRA	6	98.36	3.00	3.05	--
	Horiba ABX Pentra C200	4	85.80	8.09	9.42	--
	Roche cobas c 111	4	96.67	6.71	6.94	1
	Roche cobas 8000	3	99.27	2.48	2.50	--
	Beckman Coulter AU480	2	101.30	--	--	--
	Erba EM 360	2	90.90	--	--	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 4  
Sample Date : 03-03-2021


**Biochemistry, Urea, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	161	21.74	3.45	15.88	13
Urease, GLDH	26	23.62	2.63	11.14	3
Erba EM 200	5	22.52	2.25	9.98	--

<b>Your Result</b>	19.22	<b>SDI / z-Score</b>	-1.75
<b>Assigned Value</b>	23.31	<b>Average SDI</b>	-1.13
<b>SDPA</b>	2.331	<b>Uncertainty of AV</b>	0.19
<b>Standard Unit Result Val</b>	19.22	<b>%DEV</b>	-14.67

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

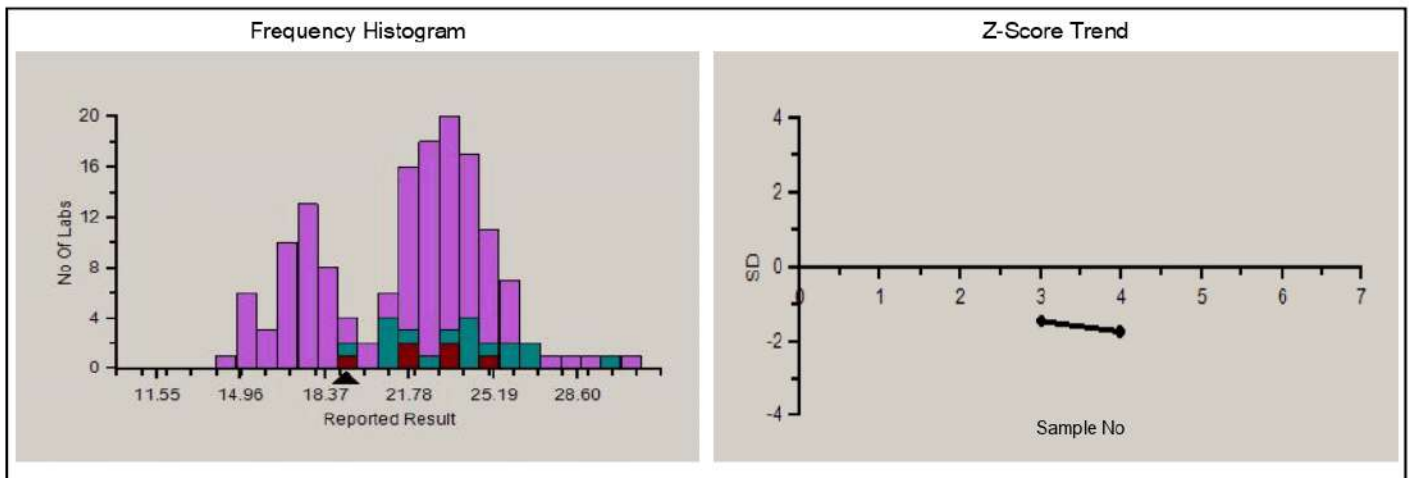

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 4  
 Sample Date : 03-03-2021

Biochemistry, Urea		N	Mean	SD	CV%	Excluded
	All Analyzer	161	21.74	3.45	15.88	13
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>5</b>	<b>22.52</b>	<b>2.25</b>	<b>9.98</b>	<b>--</b>
	Roche cobas c 311	28	23.56	0.99	4.20	--
	Roche cobas c 311	27	23.59	0.99	4.21	--
	Fuji Dri-Chem NX500/i	25	17.02	1.36	8.00	3
	Fuji Dri-Chem 4000i	16	17.75	0.47	2.65	2
	Horiba ABX Pentra C200	12	25.44	1.35	5.30	1
	Roche cobas c 111	12	22.57	1.26	5.56	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.

*Dr. Puneet Kumar Nigam*

**Dr Puneet Kumar Nigam**  
**PT coordinator & Technical Manager, MHL EQAS**  
 Unit No. 409-416,  
 Commercial Building - 1A,  
 Kohinoor Mall, Kiroi Road, Kurla (W),  
 Mumbai - 400070



PC-1022



**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 5  
Sample Date : 03-03-2021


**Biochemistry, ALP, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	141	193.32	20.55	10.63	10
IFCC	13	205.31	18.30	8.92	3
Erba EM 200	3	190.30	0.00	0.00	2

<b>Your Result</b>	190.30	<b>SDI / z-Score</b>	-1.13
<b>Assigned Value</b>	226.15	<b>Average SDI</b>	-0.18
<b>SDPA</b>	31.661	<b>Uncertainty of AV</b>	9.40
<b>Standard Unit Result Val</b>	190.30	<b>%DEV</b>	-7.31

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

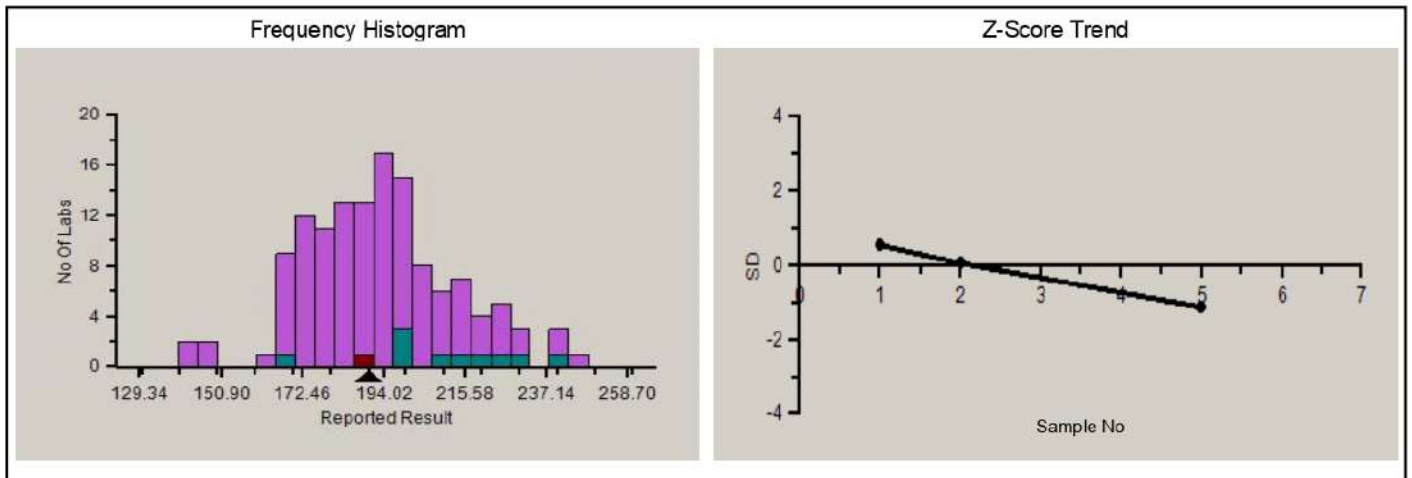

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 5  
 Sample Date : 03-03-2021

<b>Biochemistry, ALP</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	141	193.32	20.55	10.63	10
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>3</b>	<b>190.30</b>	<b>0.00</b>	<b>0.00</b>	<b>2</b>
	Fuji Dri-Chem NX500/i	32	203.03	15.57	7.67	1
	Roche cobas c 311	28	180.97	9.42	5.21	—
	Roche cobas c 311	27	181.23	9.50	5.24	—
	Fuji Dri-Chem 4000i	15	204.14	16.81	8.24	1
	Roche cobas c 111	11	191.72	21.02	10.96	—
	Horiba ABX Pentra C200	10	193.52	17.60	9.10	1
	Roche cobas c 111	10	186.89	14.35	7.68	—

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.






PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 5  
Sample Date : 03-03-2021


**Biochemistry, ALT, U/L**

	N	Mean	SD	CV%	Excluded
 All Methods	144	46.97	3.72	7.92	4
 IFCC	11	48.25	3.35	6.94	1
 Erba EM 200	3	49.80	6.79	13.63	1

<b>Your Result</b>	88.17	<b>SDI / z-Score</b>	5.62
<b>Assigned Value</b>	47.85	<b>Average SDI</b>	1.03
<b>SDPA</b>	7.178	<b>Uncertainty of AV</b>	1.82
<b>Standard Unit Result Val</b>	88.17	<b>%DEV</b>	82.74

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

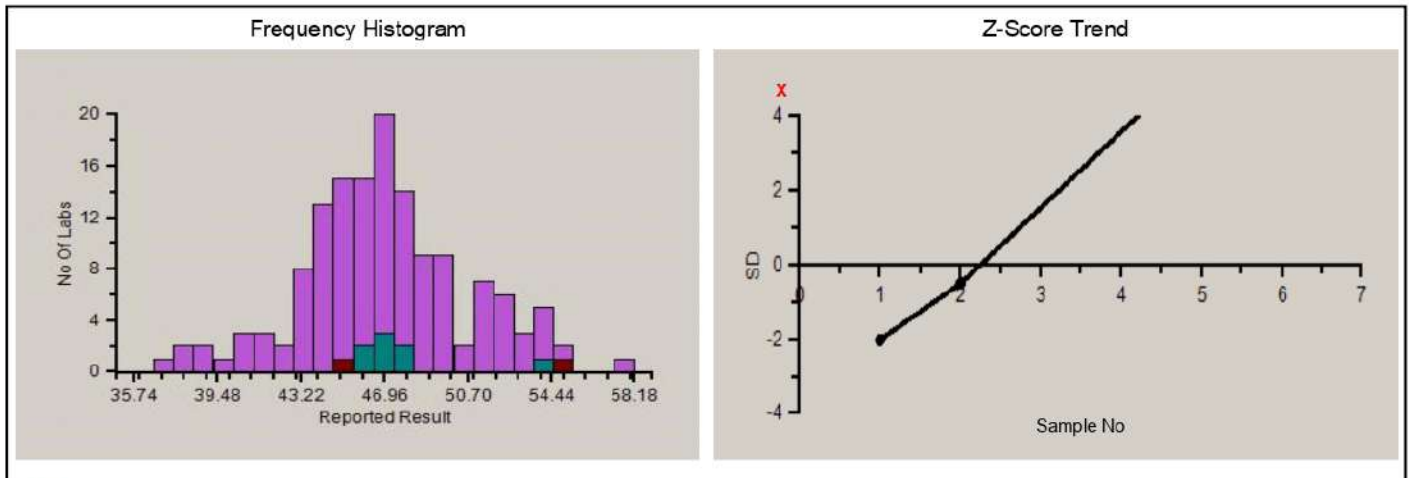

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 5  
 Sample Date : 03-03-2021

<b>Biochemistry, ALT</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	144	46.97	3.72	7.92	4
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>3</b>	<b>49.80</b>	<b>6.79</b>	<b>13.63</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	31	47.93	3.70	7.73	1
	Roche cobas c 311	28	45.80	2.37	5.18	—
	Roche cobas c 311	27	45.76	2.41	5.27	—
	Fuji Dri-Chem 4000i	15	47.53	3.11	6.55	—
	Horiba ABX Pentra C200	12	49.66	3.01	6.06	—
	Roche cobas c 111	11	44.75	2.27	5.07	—
	Roche cobas c 111	10	45.22	1.72	3.81	—

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 5  
 Sample Date : 03-03-2021


**Biochemistry, Amylase, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	87	180.64	21.14	11.70	3
CNP-triose/CNPG3	9	177.78	10.36	5.83	1
Erba EM 200	1	--	--	--	--

<b>Your Result</b>	116.00	<b>SDI / z-Score</b>	0.91
<b>Assigned Value</b>	111.00	<b>Average SDI</b>	0.55
<b>SDPA</b>	5.508	<b>Uncertainty of AV</b>	3.98
<b>Standard Unit Result Val</b>	116.00	<b>%DEV</b>	-34.75

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

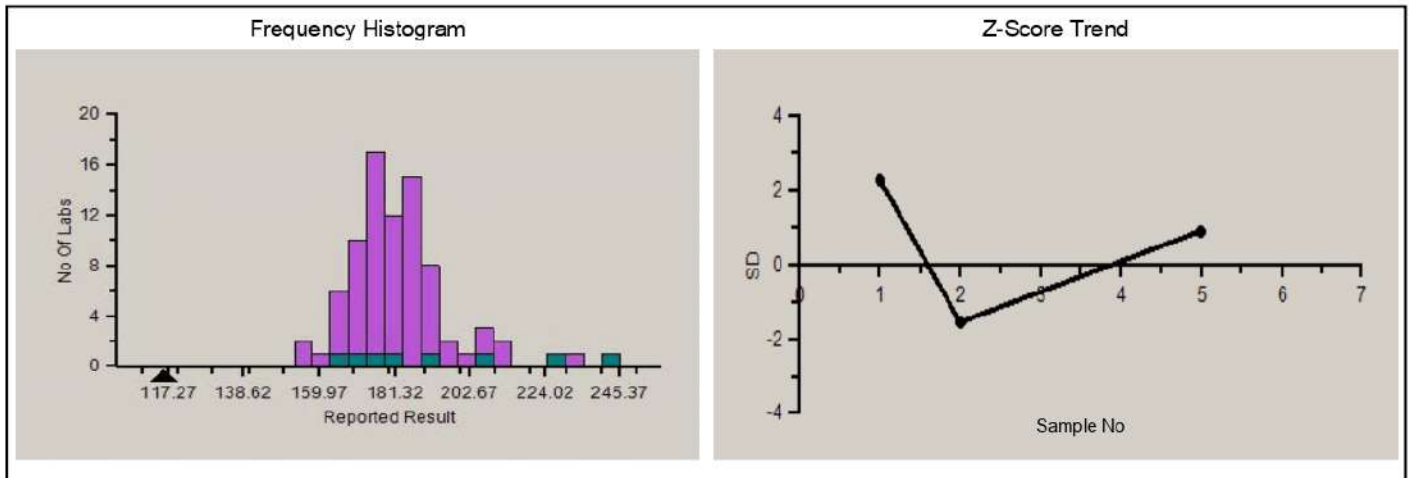

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 5  
 Sample Date : 03-03-2021

Biochemistry, Amylase		N	Mean	SD	CV%	Excluded
All Analyzer		87	180.64	21.14	11.70	3
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	22	182.50	14.55	7.97	1
	Fuji Dri-Chem 4000i	15	186.67	9.55	5.12	--
	Fuji Dri-Chem 4000i	14	184.93	7.03	3.80	--
	Roche cobas c 311	13	174.41	7.72	4.43	--
	Roche cobas INTEGRA	7	178.57	4.78	2.68	--
	Roche cobas 6000	6	171.93	6.53	3.80	--
	Roche cobas 8000	4	168.75	3.95	2.34	--
	Roche cobas c 111	3	184.00	11.39	6.19	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 5  
Sample Date : 03-03-2021


**Biochemistry, AST, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	143	94.40	5.54	5.87	6
IFCC	11	92.73	5.10	5.50	1
Erba EM 200	4	95.17	5.75	6.04	--

<b>Your Result</b>	88.17	<b>SDI / z-Score</b>	-1.79
<b>Assigned Value</b>	99.00	<b>Average SDI</b>	-1.10
<b>SDPA</b>	6.048	<b>Uncertainty of AV</b>	2.18
<b>Standard Unit Result Val</b>	88.17	<b>%DEV</b>	-4.91

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

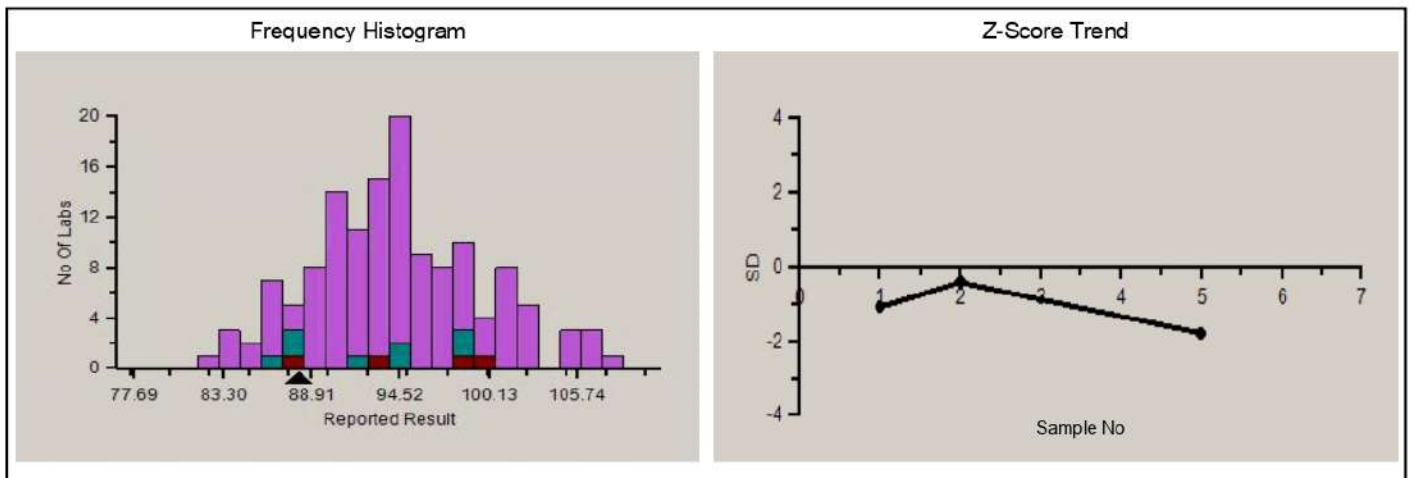

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

**Lab :** 429  
**Lab Name :** NEYVELI DIAGNOSTIC CENTRE  
**Report Date :** 19/03/2021

**Cycle No :** 210103  
**Sample No :** 5  
**Sample Date :** 03-03-2021

<b>Biochemistry, AST</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	143	94.40	5.54	5.87	6
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>4</b>	<b>95.17</b>	<b>5.75</b>	<b>6.04</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	32	94.40	5.84	6.19	2
	Roche cobas c 311	27	93.46	3.34	3.58	--
	Roche cobas c 311	26	93.50	3.40	3.64	--
	Fuji Dri-Chem 4000i	15	91.53	4.00	4.37	--
	Roche cobas c 111	12	91.63	4.03	4.40	--
	Roche cobas c 111	11	91.04	3.63	3.99	--
	Horiba ABX Pentra C200	10	96.87	5.97	6.17	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022






**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 5  
Sample Date : 03-03-2021


**Biochemistry, Bilirubin Direct, mg/dl**

	N	Mean	SD	CV%	Excluded
 All Methods	139	0.92	0.13	13.64	16
 Diazotization	118	0.95	0.11	11.71	10
 Erba EM 200	4	0.62	0.00	0.00	3

<b>Your Result</b>	0.62	<b>SDI / z-Score</b>	-0.67
<b>Assigned Value</b>	0.72	<b>Average SDI</b>	-0.94
<b>SDPA</b>	0.143	<b>Uncertainty of AV</b>	0.03
<b>Standard Unit Result Val</b>	0.62	<b>%DEV</b>	-34.60

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

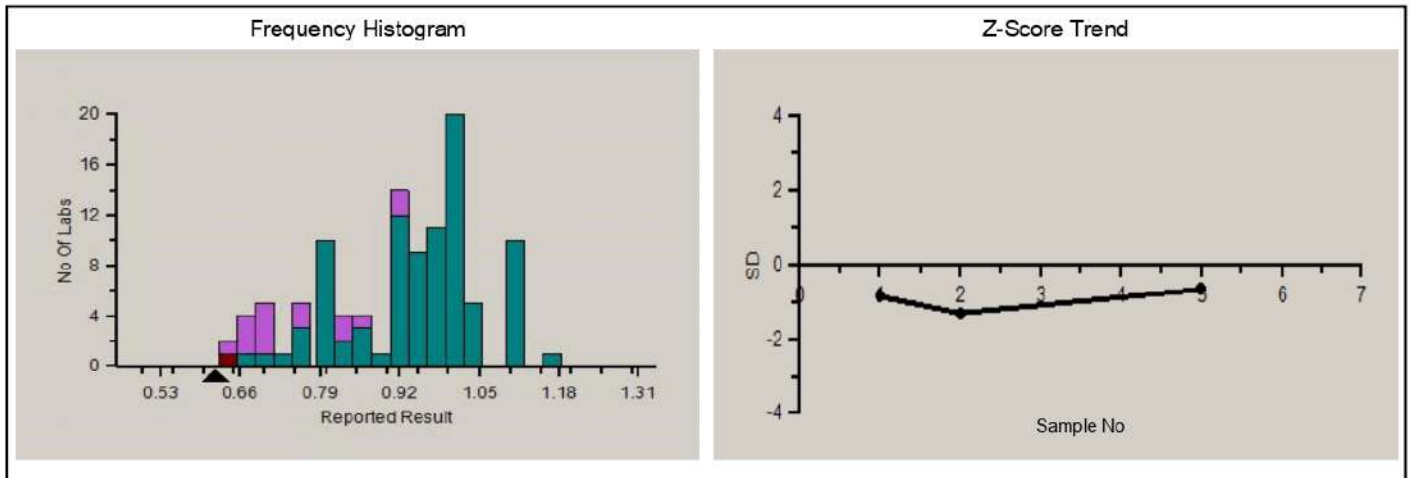

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 5  
 Sample Date : 03-03-2021

<b>Biochemistry, Bilirubin Direct</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	139	0.92	0.13	13.64	16
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>4</b>	<b>0.62</b>	<b>0.00</b>	<b>0.00</b>	<b>3</b>
	Fuji Dri-Chem NX500/i	28	0.97	0.08	8.56	1
	Roche cobas c 311	27	0.94	0.11	11.63	1
	Roche cobas c 311	26	0.94	0.11	11.24	1
	Fuji Dri-Chem 4000i	15	0.99	0.05	4.63	–
	Horiba ABX Pentra C200	11	0.75	0.07	8.98	1
	Roche cobas c 111	11	1.03	0.09	8.22	2
	Roche cobas c 111	10	1.04	0.09	8.67	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 5  
 Sample Date : 03-03-2021


**Biochemistry, Bilirubin Total, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	142	1.92	0.17	8.66	8
Diazotization	35	1.88	0.18	9.29	3
Erba EM 200	4	2.05	0.21	10.42	--

<b>Your Result</b>	1.85	<b>SDI / z-Score</b>	-0.14
<b>Assigned Value</b>	1.91	<b>Average SDI</b>	-0.11
<b>SDPA</b>	0.381	<b>Uncertainty of AV</b>	0.02
<b>Standard Unit Result Val</b>	1.85	<b>%DEV</b>	-1.80

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

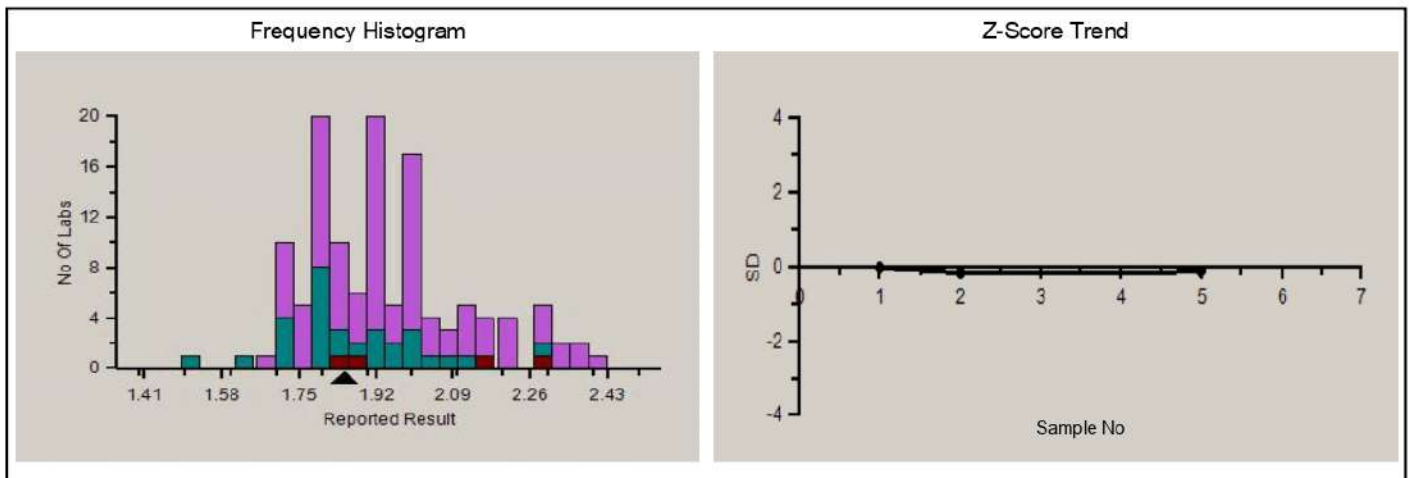

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 5  
 Sample Date : 03-03-2021

<b>Biochemistry, Bilirubin Total</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	142	1.92	0.17	8.66	8
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>4</b>	<b>2.05</b>	<b>0.21</b>	<b>10.42</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	29	1.83	0.13	7.25	2
	Roche cobas c 311	28	1.87	0.11	5.93	2
	Roche cobas c 311	27	1.87	0.11	6.03	2
	Fuji Dri-Chem 4000i	15	1.87	0.11	5.62	--
	Horiba ABX Pentra C200	11	2.05	0.11	5.32	2
	Roche cobas c 111	10	1.99	0.20	10.20	--
	Roche cobas c 111	9	1.95	0.15	7.81	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.






PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 5  
 Sample Date : 03-03-2021


**Biochemistry, Calcium, mg/dl**

	N	Mean	SD	CV%	Excluded
 All Methods	131	5.77	0.34	5.91	10
 Arsenazo I	3	5.93	0.90	15.20	--
 Erba EM 200	4	6.43	0.35	5.46	1

<b>Your Result</b>	6.80	<b>SDI / z-Score</b>	0.46
<b>Assigned Value</b>	6.60	<b>Average SDI</b>	1.01
<b>SDPA</b>	0.435	<b>Uncertainty of AV</b>	0.21
<b>Standard Unit Result Val</b>	6.80	<b>%DEV</b>	14.61

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

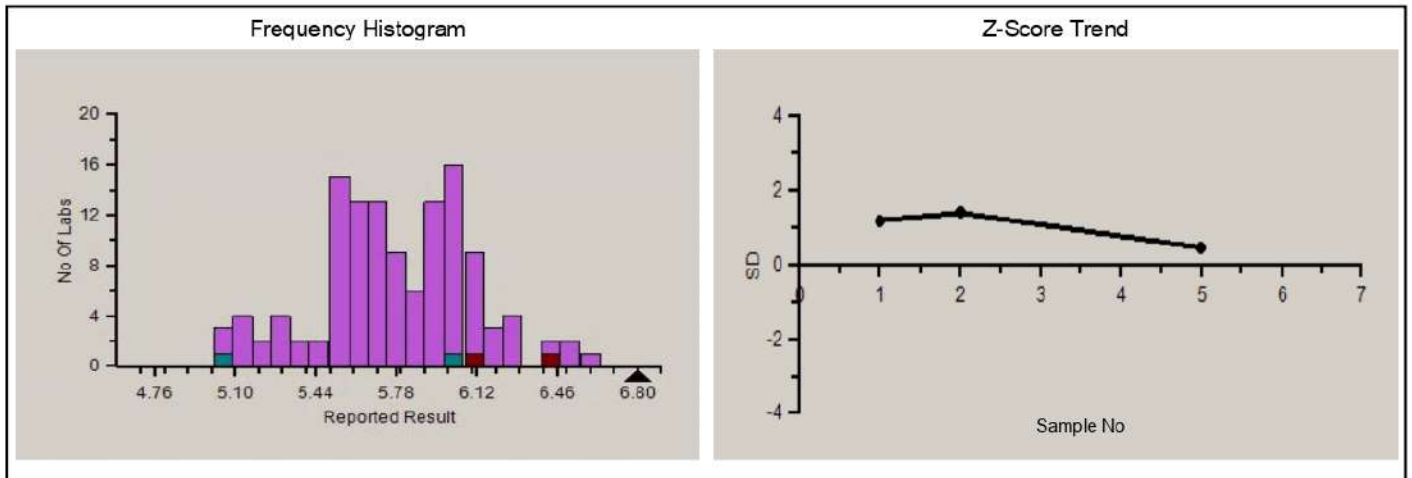

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 5  
 Sample Date : 03-03-2021

Biochemistry, Calcium		N	Mean	SD	CV%	Excluded
	All Analyzer	131	5.77	0.34	5.91	10
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>4</b>	<b>6.43</b>	<b>0.35</b>	<b>5.46</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	27	5.61	0.34	6.00	2
	Roche cobas c 311	25	5.87	0.22	3.76	—
	Roche cobas c 311	24	5.87	0.23	3.83	—
	Fuji Dri-Chem 4000i	15	5.64	0.29	5.14	—
	Roche cobas c 111	10	5.87	0.30	5.13	—
	Roche cobas INTEGRA	10	5.78	0.35	6.08	—
	Roche cobas c 111	9	5.84	0.31	5.27	—

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.






PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 5  
 Sample Date : 03-03-2021


**Biochemistry, Creatinine, mg/dl**

	N	Mean	SD	CV%	Excluded
 All Methods	140	2.53	0.19	7.52	4
 Jaffe's Kinetic	2	2.48	--	--	--
 Erba EM 200	4	2.51	0.11	4.35	--

<b>Your Result</b>	2.59	<b>SDI / z-Score</b>	-0.05
<b>Assigned Value</b>	2.60	<b>Average SDI</b>	-0.83
<b>SDPA</b>	0.208	<b>Uncertainty of AV</b>	0.02
<b>Standard Unit Result Val</b>	2.59	<b>%DEV</b>	4.65

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

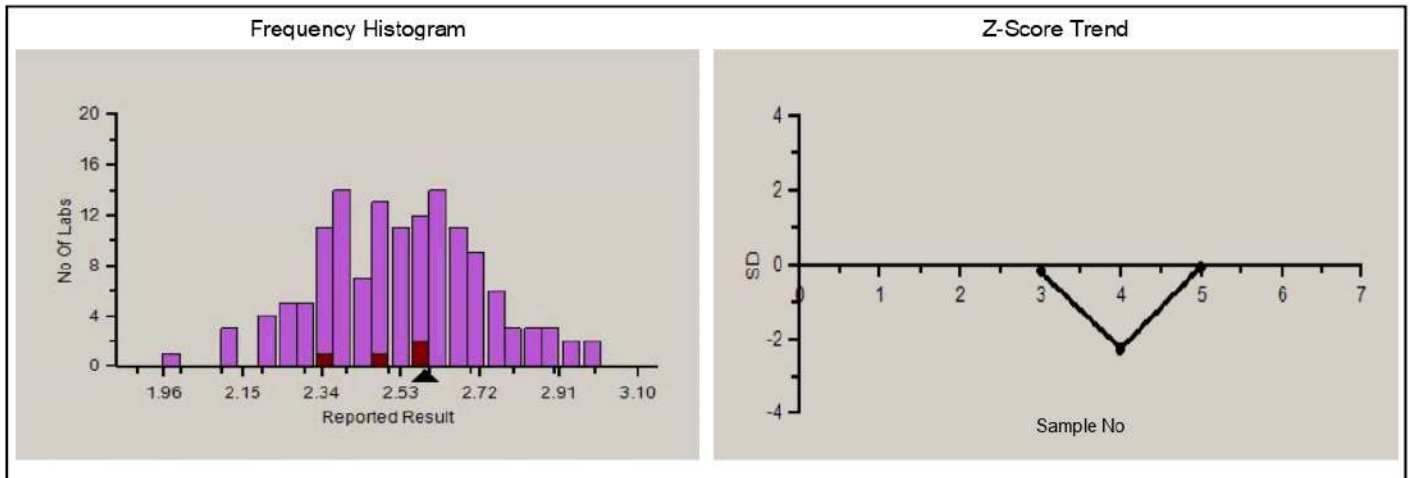

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 5  
 Sample Date : 03-03-2021

<b>Biochemistry, Creatinine</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	140	2.53	0.19	7.52	4
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>4</b>	<b>2.51</b>	<b>0.11</b>	<b>4.35</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	28	2.38	0.11	4.71	2
	Roche cobas c 311	28	2.62	0.13	4.92	--
	Roche cobas c 311	27	2.62	0.13	4.85	--
	Fuji Dri-Chem 4000i	15	2.39	0.12	5.11	1
	Horiba ABX Pentra C200	11	2.57	0.26	10.05	--
	Roche cobas c 111	11	2.55	0.18	7.03	--
	Roche cobas c 111	10	2.59	0.11	4.09	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022



**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 5  
Sample Date : 03-03-2021


**Biochemistry, GGT, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	123	90.79	16.32	17.97	6
SZASZ IFCC standardized	2	74.09	--	--	--
Erba EM 200	2	71.64	--	--	--

<b>Your Result</b>	70.17	<b>SDI / z-Score</b>	-0.82
<b>Assigned Value</b>	78.58	<b>Average SDI</b>	1.23
<b>SDPA</b>	10.215	<b>Uncertainty of AV</b>	0.65
<b>Standard Unit Result Val</b>	70.17	<b>%DEV</b>	-5.28

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

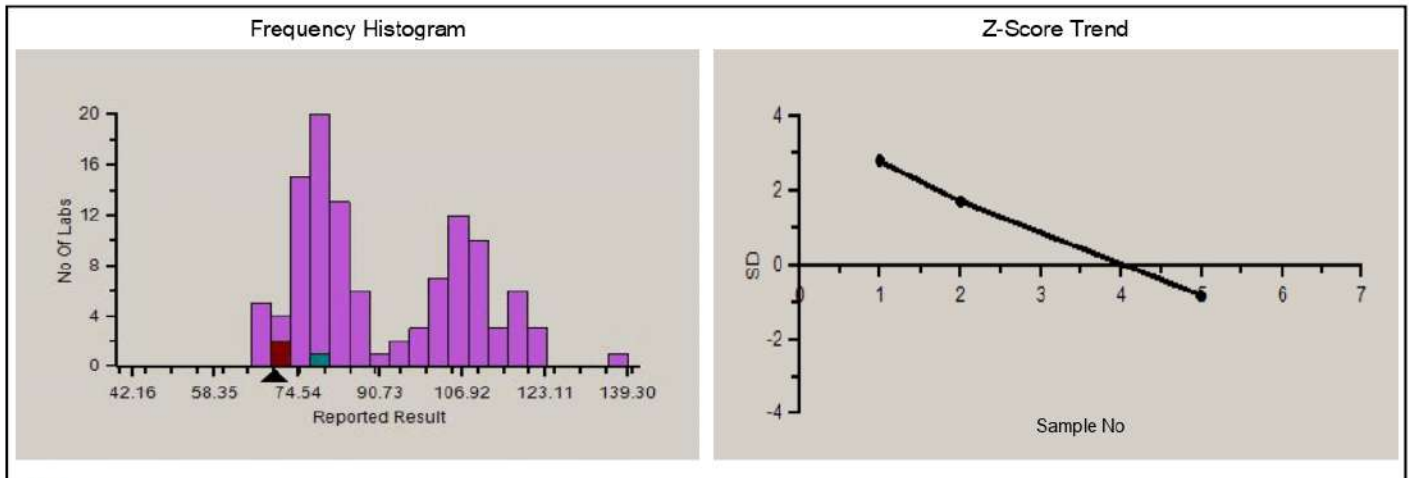

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

**Lab :** 429  
**Lab Name :** NEYVELI DIAGNOSTIC CENTRE  
**Report Date :** 19/03/2021

**Cycle No :** 210103  
**Sample No :** 5  
**Sample Date :** 03-03-2021

<b>Biochemistry, GGT</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	123	90.79	16.32	17.97	6
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>2</b>	<b>71.64</b>	--	--	--
	Fuji Dri-Chem NX500/i	30	108.66	10.52	9.68	1
	Roche cobas c 311	25	79.21	5.04	6.36	1
	Roche cobas c 311	24	78.70	4.47	5.68	1
	Fuji Dri-Chem 4000i	12	107.67	4.44	4.12	--
	Roche cobas INTEGRA	10	78.46	5.14	6.55	--
	Roche cobas c 111	9	80.35	5.89	7.34	1
	Beckman Coulter AU480	6	79.04	2.89	3.66	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 5  
Sample Date : 03-03-2021


**Biochemistry, Glucose, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	143	133.24	6.91	5.19	8
GPO-POD	8	138.41	7.19	5.20	1
Erba EM 200	3	134.40	3.21	2.39	--

<b>Your Result</b>	135.10	<b>SDI / z-Score</b>	0.04
<b>Assigned Value</b>	134.61	<b>Average SDI</b>	0.33
<b>SDPA</b>	12.115	<b>Uncertainty of AV</b>	0.92
<b>Standard Unit Result Val</b>	135.10	<b>%DEV</b>	-2.39

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

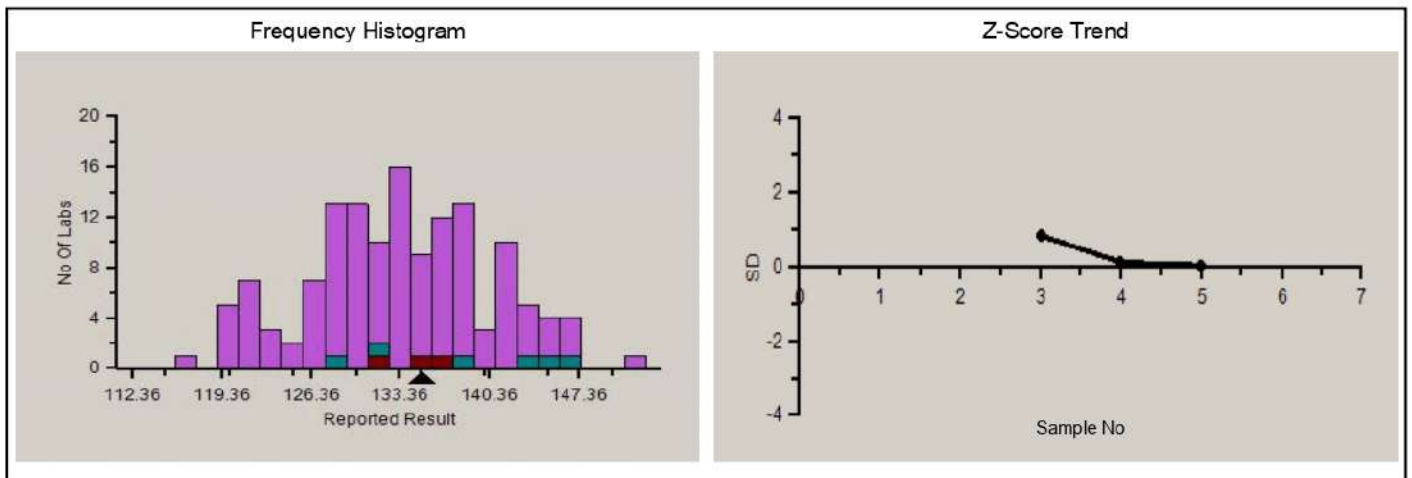

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

**Lab :** 429  
**Lab Name :** NEYVELI DIAGNOSTIC CENTRE  
**Report Date :** 19/03/2021

**Cycle No :** 210103  
**Sample No :** 5  
**Sample Date :** 03-03-2021

<b>Biochemistry, Glucose</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	143	133.24	6.91	5.19	8
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>3</b>	<b>134.40</b>	<b>3.21</b>	<b>2.39</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	30	131.57	7.66	5.82	2
	Roche cobas c 311	27	133.56	6.08	4.55	3
	Fuji Dri-Chem 4000i	16	130.79	5.57	4.26	—
	Fuji Dri-Chem 4000i	15	130.60	5.72	4.38	—
	Horiba ABX Pentra C200	12	131.57	7.56	5.75	—
	Roche cobas c 111	10	136.47	4.44	3.25	1
	Roche cobas c 111	9	137.03	4.40	3.21	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
Lab Name : NEYVELI DIAGNOSTIC CENTRE  
Report Date : 19/03/2021

Cycle No : 210103  
Sample No : 5  
Sample Date : 03-03-2021


**Biochemistry, Urea, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	137	47.62	2.79	5.85	7
Urease, GLDH	16	47.56	4.02	8.45	--
Erba EM 200	3	47.47	2.55	5.38	--

<b>Your Result</b>	47.30	<b>SDI / z-Score</b>	-0.15
<b>Assigned Value</b>	47.76	<b>Average SDI</b>	-1.13
<b>SDPA</b>	2.952	<b>Uncertainty of AV</b>	0.39
<b>Standard Unit Result Val</b>	47.30	<b>%DEV</b>	-0.54

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

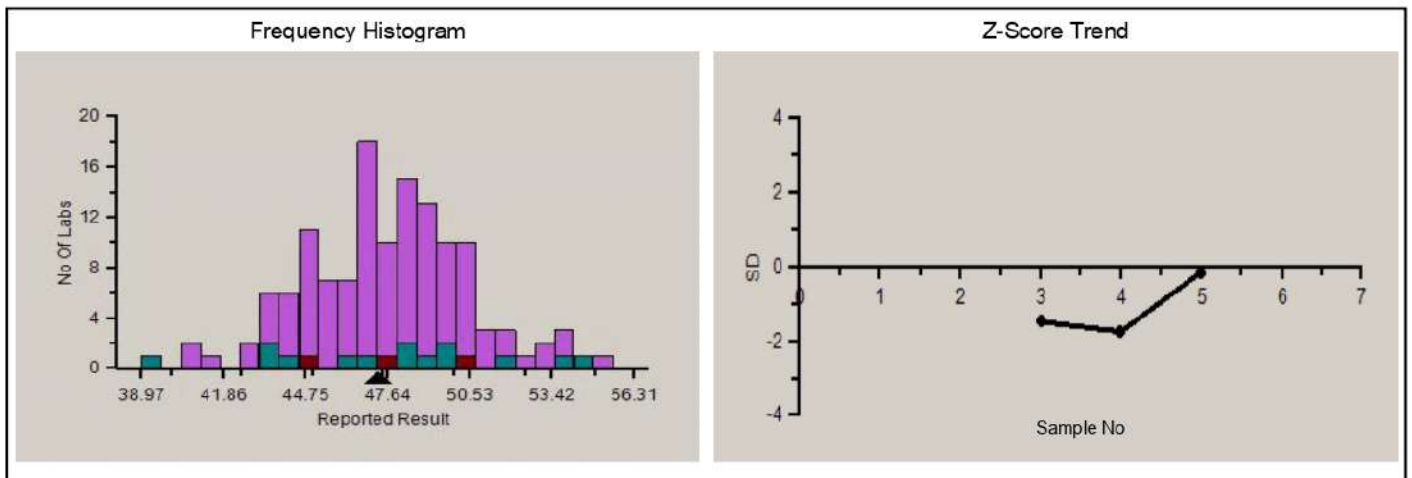

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 429  
 Lab Name : NEYVELI DIAGNOSTIC CENTRE  
 Report Date : 19/03/2021

Cycle No : 210103  
 Sample No : 5  
 Sample Date : 03-03-2021

Biochemistry, Urea		N	Mean	SD	CV%	Excluded
	All Analyzer	137	47.62	2.79	5.85	7
<b>Your Analyzer :</b>	<b>Erba EM 200</b>	<b>3</b>	<b>47.47</b>	<b>2.55</b>	<b>5.38</b>	<b>--</b>
	Roche cobas c 311	28	49.41	1.48	2.99	--
	Roche cobas c 311	27	49.40	1.50	3.04	--
	Fuji Dri-Chem NX500/i	25	47.59	2.18	4.57	4
	Fuji Dri-Chem 4000i	15	47.00	2.38	5.06	1
	Horiba ABX Pentra C200	12	45.25	4.30	9.50	--
	Roche cobas c 111	11	46.00	2.40	5.21	--
	Roche cobas c 111	10	46.50	1.83	3.93	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.

*Dr. Puneet Kumar Nigam*

**Dr Puneet Kumar Nigam**  
**PT coordinator & Technical Manager, MHL EQAS**  
 Unit No. 409-416,  
 Commercial Building - 1A,  
 Kohinoor Mall, Kiroli Road, Kurla (W),  
 Mumbai - 400070



PC-1022