

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 1  
Sample Date : 01-07-2021


**Biochemistry, Albumin, g/dL**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	235	3.98	0.46	11.54	16
<span style="color: teal;">■</span> Bromcresol Green (BCG)	229	3.99	0.47	11.66	16
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	3.59	<b>SDI / z-Score</b>	0.11
<b>Assigned Value</b>	3.57	<b>Average SDI</b>	-0.08
<b>SDPA</b>	0.192	<b>Uncertainty of AV</b>	0.03
<b>Standard Unit Result Val</b>	3.59	<b>%DEV</b>	-9.96

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

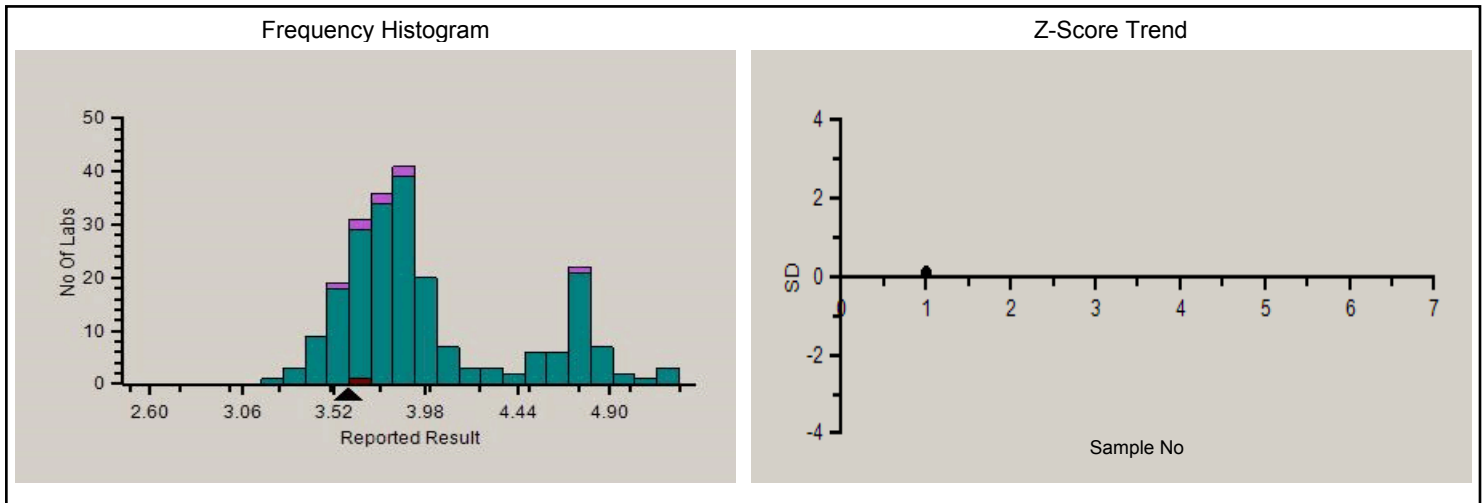

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 1  
 Sample Date : 01-07-2021

Biochemistry, Albumin		N	Mean	SD	CV%	Excluded
	All Analyzer	235	3.98	0.46	11.54	16
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	1	--	--	--	--
	Fuji Dri-Chem NX500/i	37	4.74	0.21	4.49	1
	Fuji Dri-Chem NX500/i	37	4.74	0.21	4.49	1
	Roche cobas c 311	29	3.88	0.09	2.30	1
	Biosystems A15	22	3.89	0.31	7.86	3
	Biosystems A15	22	3.89	0.31	7.86	3
	Erba EM 200	19	3.54	0.19	5.32	1
	Erba EM 200	18	3.51	0.16	4.42	1
	ERBA XL-640	18	3.57	0.14	3.98	2

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 1  
Sample Date : 01-07-2021


**Biochemistry, ALP, U/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	233	84.69	18.97	22.40	15
<span style="color: teal;">■</span> IFCC	26	78.49	22.34	28.46	1
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	72.00	<b>SDI / z-Score</b>	-0.36
<b>Assigned Value</b>	75.87	<b>Average SDI</b>	-0.20
<b>SDPA</b>	10.622	<b>Uncertainty of AV</b>	0.65
<b>Standard Unit Result Val</b>	72.00	<b>%DEV</b>	-8.27

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

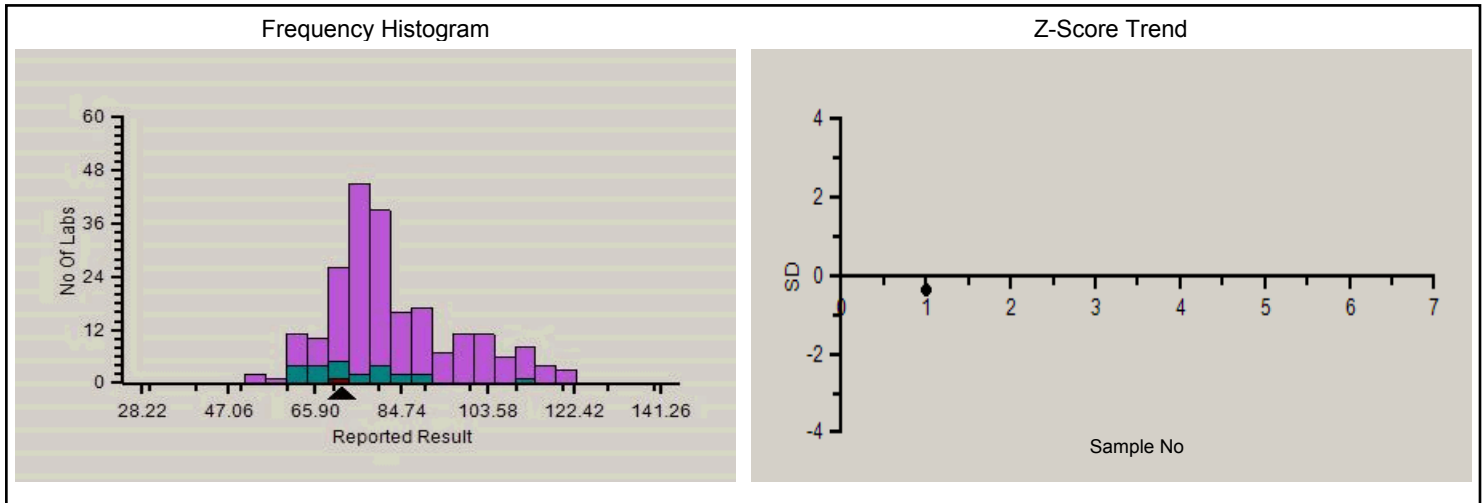

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 1  
 Sample Date : 01-07-2021

Biochemistry, ALP		N	Mean	SD	CV%	Excluded
	All Analyzer	233	84.69	18.97	22.40	15
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	36	104.31	9.88	9.47	--
	Fuji Dri-Chem NX500/i	36	104.31	9.88	9.47	--
	Roche cobas c 311	29	77.82	4.25	5.46	--
	Biosystems A15	22	83.03	8.79	10.58	2
	Biosystems A15	22	83.03	8.79	10.58	2
	Erba EM 200	17	74.01	7.35	9.93	2
	ERBA XL-640	17	74.35	9.25	12.44	--
	ERBA XL-640	17	74.35	9.25	12.44	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 1  
Sample Date : 01-07-2021


**Biochemistry, ALT, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	237	21.54	15.81	73.40	65
IFCC	33	19.62	9.32	47.48	12
Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	20.20	<b>SDI / z-Score</b>	-0.12
<b>Assigned Value</b>	20.62	<b>Average SDI</b>	-0.12
<b>SDPA</b>	3.500	<b>Uncertainty of AV</b>	0.76
<b>Standard Unit Result Val</b>	20.20	<b>%DEV</b>	2.94

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

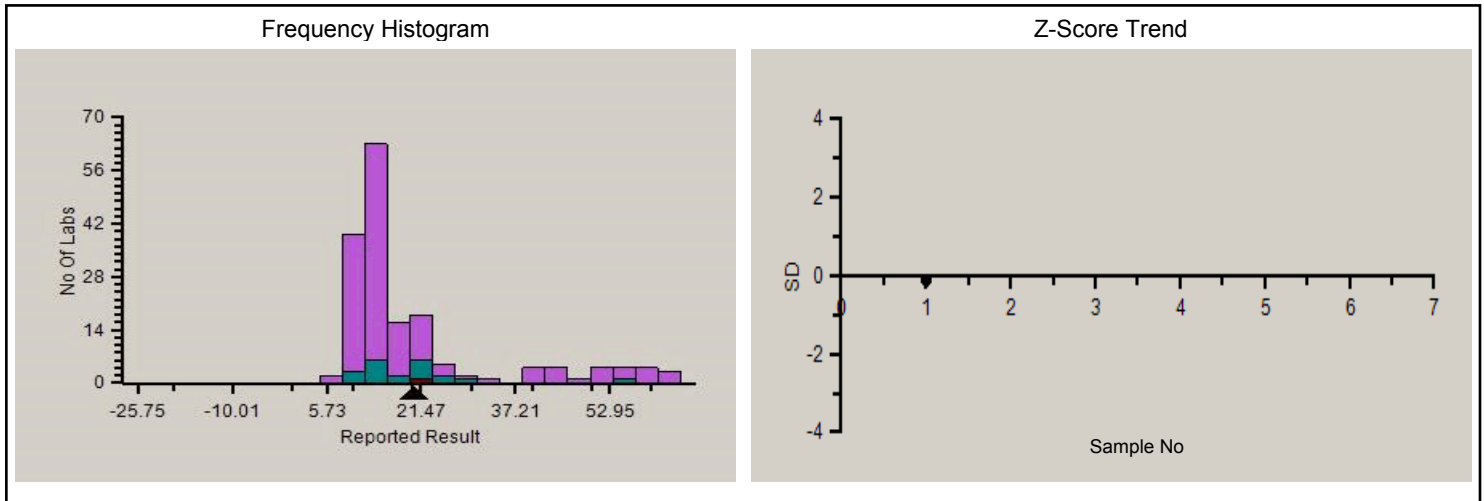

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 1  
 Sample Date : 01-07-2021

Biochemistry, ALT		N	Mean	SD	CV%	Excluded
	All Analyzer	237	21.54	15.81	73.40	65
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	35	52.95	9.67	18.26	15
	Fuji Dri-Chem NX500/i	35	52.95	9.67	18.26	15
	Roche cobas c 311	29	13.30	1.59	11.99	--
	Biosystems A15	22	13.03	1.97	15.12	7
	Biosystems A15	22	13.03	1.97	15.12	7
	Erba EM 200	19	19.16	3.98	20.77	9
	Erba EM 200	18	19.96	3.27	16.39	9
	ERBA XL-640	18	20.97	2.75	13.13	4

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 1  
Sample Date : 01-07-2021


**Biochemistry, AST, U/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	233	28.18	9.02	32.01	54
<span style="color: teal;">■</span> IFCC	31	30.41	8.52	28.01	10
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	30.60	<b>SDI / z-Score</b>	-0.94
<b>Assigned Value</b>	37.35	<b>Average SDI</b>	-0.79
<b>SDPA</b>	7.170	<b>Uncertainty of AV</b>	1.79
<b>Standard Unit Result Val</b>	30.60	<b>%DEV</b>	0.64

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

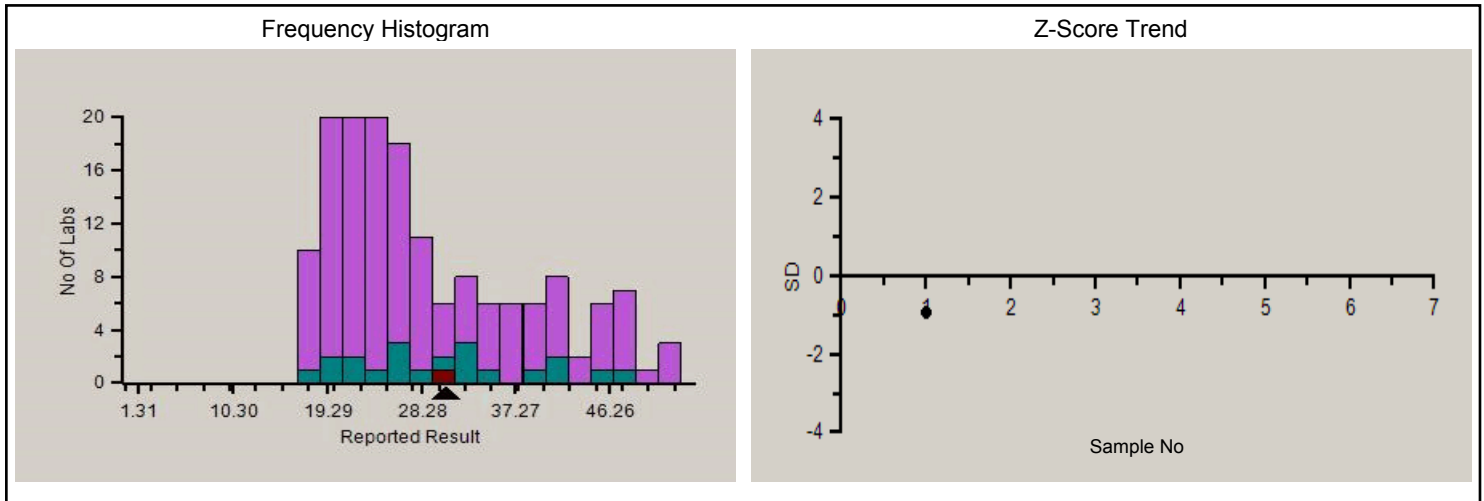

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 1  
 Sample Date : 01-07-2021

Biochemistry, AST		N	Mean	SD	CV%	Excluded
	All Analyzer	233	28.18	9.02	32.01	54
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	36	40.29	6.99	17.36	12
	Fuji Dri-Chem NX500/i	36	40.29	6.99	17.36	12
	Roche cobas c 311	28	23.54	2.22	9.41	--
	Biosystems A15	21	23.98	3.23	13.46	3
	Biosystems A15	21	23.98	3.23	13.46	3
	Erba EM 200	19	33.40	5.71	17.09	10
	Erba EM 200	18	32.74	5.72	17.48	10
	ERBA XL-640	18	37.71	5.84	15.47	4

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 1  
Sample Date : 01-07-2021


**Biochemistry, Bilirubin Direct, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	229	0.10	0.02	23.08	88
<span style="color: teal;">■</span> Jendrassik Grof	6	0.10	0.00	0.00	4
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	1

<b>Your Result</b>	0.04	<b>SDI / z-Score</b>	-2.09
<b>Assigned Value</b>	0.11	<b>Average SDI</b>	-1.88
<b>SDPA</b>	0.032	<b>Uncertainty of AV</b>	0.01
<b>Standard Unit Result Val</b>	0.04	<b>%DEV</b>	-60.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

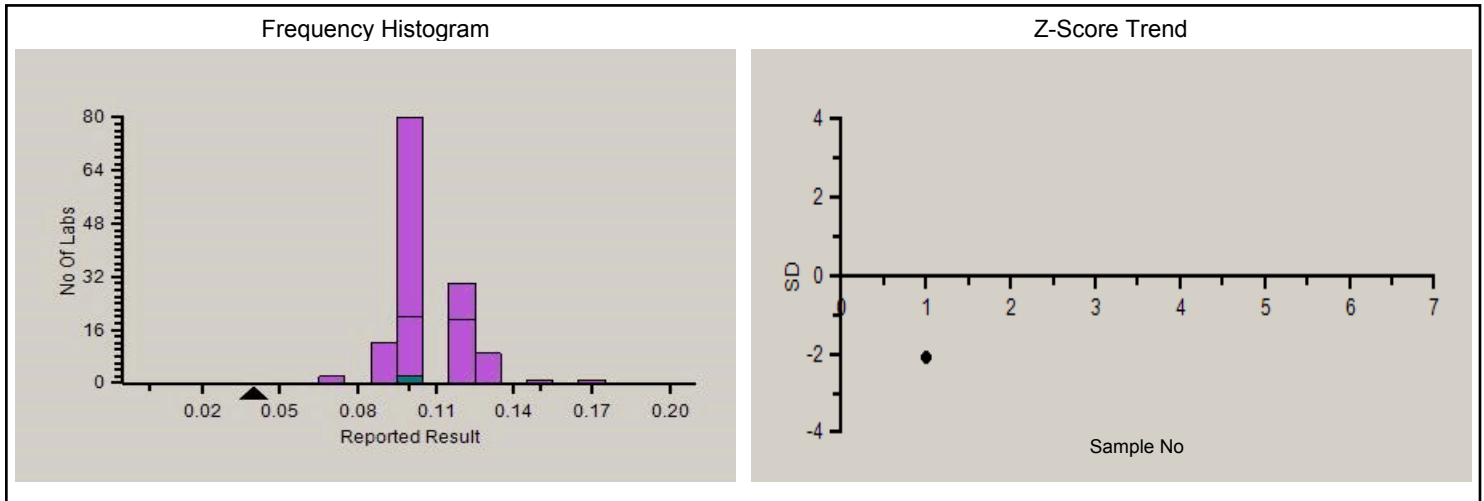

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 1  
 Sample Date : 01-07-2021

Biochemistry, Bilirubin Direct		N	Mean	SD	CV%	Excluded
	All Analyzer	229	0.10	0.02	23.08	88
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	36	0.10	0.00	4.04	10
	Fuji Dri-Chem NX500/i	36	0.10	0.00	4.04	10
	Roche cobas c 311	27	0.10	0.01	14.74	6
	Biosystems A15	21	0.20	0.14	67.49	18
	Biosystems A15	21	0.20	0.14	67.49	18
	Erba EM 200	19	0.11	0.02	19.44	10
	Erba EM 200	18	0.10	0.01	7.92	10
	ERBA XL-640	17	0.11	0.01	12.96	8

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 1  
Sample Date : 01-07-2021


**Biochemistry, Bilirubin Total, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	230	0.31	0.15	47.10	62
<span style="color: teal;">■</span> Jendrassik Grof	12	0.35	0.12	35.13	3
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	1

<b>Your Result</b>	0.09	<b>SDI / z-Score</b>	-1.87
<b>Assigned Value</b>	0.21	<b>Average SDI</b>	-0.84
<b>SDPA</b>	0.062	<b>Uncertainty of AV</b>	0.01
<b>Standard Unit Result Val</b>	0.09	<b>%DEV</b>	-74.50

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

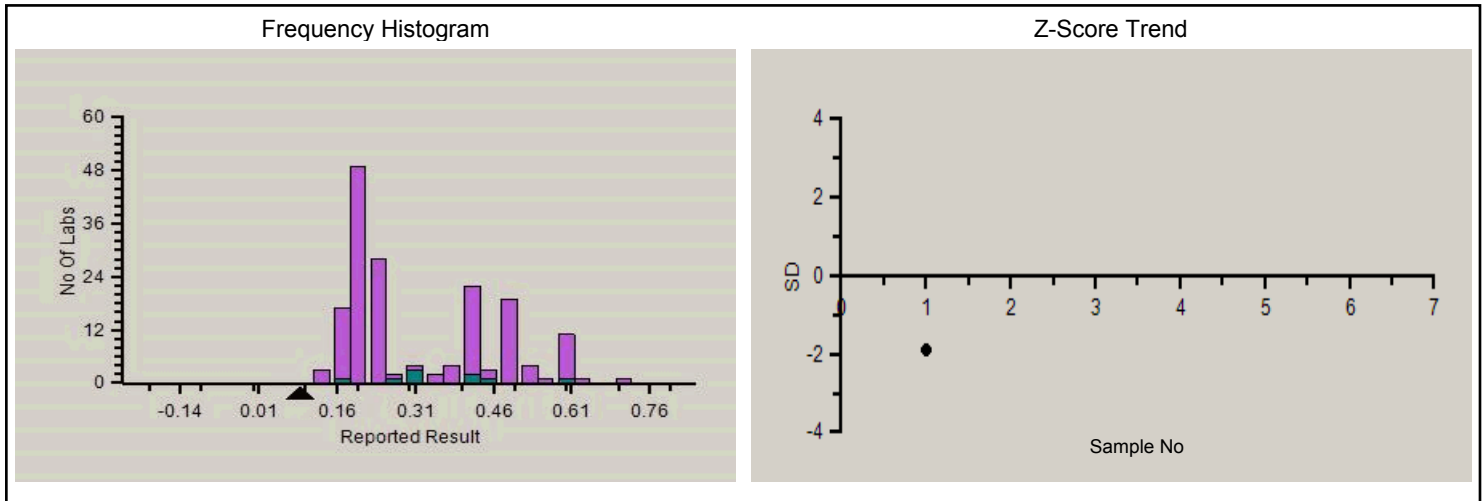

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 1  
 Sample Date : 01-07-2021

<b>Biochemistry, Bilirubin Total</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	230	0.31	0.15	47.10	62
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	36	0.47	0.07	14.68	6
	Fuji Dri-Chem NX500/i	36	0.47	0.07	14.68	6
	Roche cobas c 311	28	0.19	0.03	17.20	3
	Erba EM 200	19	0.21	0.03	15.64	5
	Erba EM 200	18	0.21	0.03	13.17	5
	ERBA XL-640	18	0.21	0.02	10.68	2
	Biosystems A15	17	0.55	0.08	14.91	6
	Biosystems A15	17	0.55	0.08	14.91	6

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 1  
Sample Date : 01-07-2021


**Biochemistry, Calcium, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	177	7.34	0.58	7.89	4
<span style="color: teal;">■</span> Arsenazo III	62	7.63	0.47	6.12	4
<span style="color: darkred;">■</span> Erba Chem 5/Plus	2	8.50	--	--	1

<b>Your Result</b>	8.50	<b>SDI / z-Score</b>	0.55
<b>Assigned Value</b>	8.07	<b>Average SDI</b>	1.81
<b>SDPA</b>	0.785	<b>Uncertainty of AV</b>	0.27
<b>Standard Unit Result Val</b>	8.50	<b>%DEV</b>	11.39

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

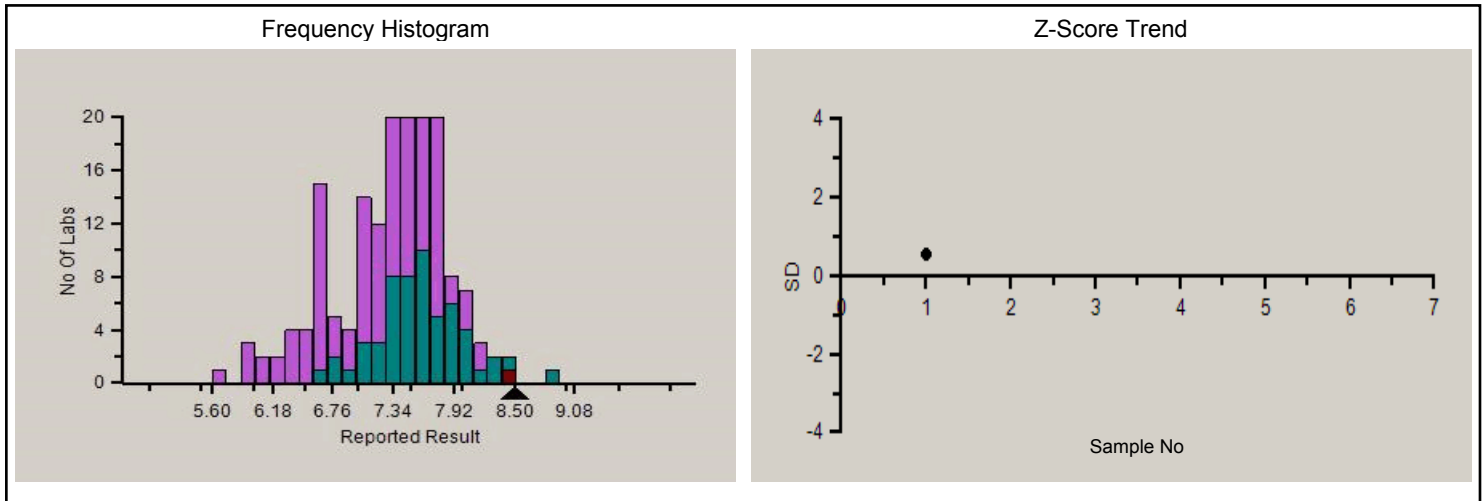

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 1  
 Sample Date : 01-07-2021

Biochemistry, Calcium		N	Mean	SD	CV%	Excluded
	All Analyzer	177	7.34	0.58	7.89	4
<b>Your Analyzer :</b>	<b>Erba Chem 5/Plus</b>	<b>2</b>	<b>8.50</b>	--	--	<b>1</b>
	Fuji Dri-Chem NX500/i	33	6.69	0.43	6.40	--
	Fuji Dri-Chem NX500/i	33	6.69	0.43	6.40	--
	Roche cobas c 311	27	7.54	0.21	2.83	--
	Fuji Dri-Chem 4000i	16	6.65	0.42	6.29	--
	Roche cobas c 111	13	7.65	0.40	5.21	--
	Roche cobas INTEGRA	11	7.37	0.15	2.06	--
	Horiba ABX Pentra C200	9	7.58	0.24	3.14	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 1  
Sample Date : 01-07-2021


**Biochemistry, Chloride, mEq/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	154	107.64	13.00	12.08	21
<span style="color: teal;">■</span> ISE direct	108	115.38	4.51	3.91	9
<span style="color: darkred;">■</span> EasyLyte	8	113.05	3.45	3.05	2

<b>Your Result</b>	134.10	<b>SDI / z-Score</b>	2.13
<b>Assigned Value</b>	115.64	<b>Average SDI</b>	1.84
<b>SDPA</b>	8.672	<b>Uncertainty of AV</b>	0.59
<b>Standard Unit Result Val</b>	134.10	<b>%DEV</b>	18.62

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

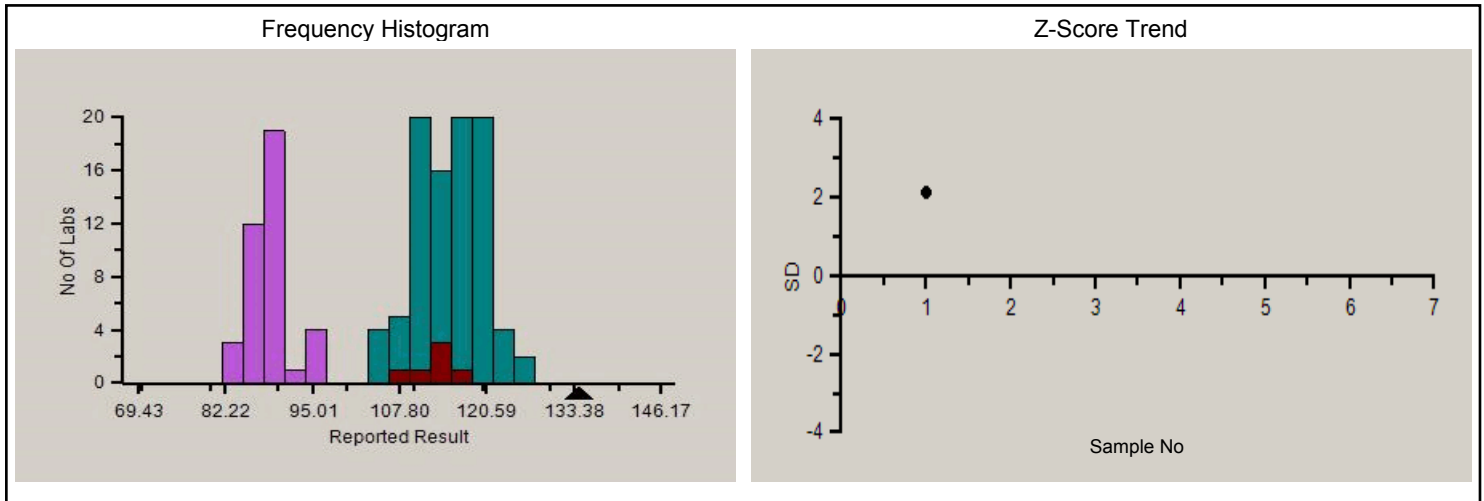

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 1  
 Sample Date : 01-07-2021

Biochemistry, Chloride		N	Mean	SD	CV%	Excluded
	All Analyzer	154	107.64	13.00	12.08	21
<b>Your Analyzer :</b>	<b>EasyLyte</b>	<b>8</b>	<b>113.05</b>	<b>3.45</b>	<b>3.05</b>	<b>2</b>
	Fuji Dri-Chem NX500/i	37	117.58	3.64	3.09	1
	Fuji Dri-Chem NX500/i	37	117.58	3.64	3.09	1
	Roche cobas c 311	16	89.37	7.39	8.26	--
	Fuji Dri-Chem 4000i	15	119.50	3.03	2.54	1
	Roche AVL 9180	11	111.50	1.83	1.64	--
	Roche cobas 6000	8	87.37	1.41	1.62	1
	Bene Sphera C73	8	111.20	1.91	1.72	4

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 1  
Sample Date : 01-07-2021


**Biochemistry, GGT, U/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	146	19.37	4.23	21.86	9
<span style="color: teal;">■</span> SZAZ Carboxylated Substrate	8	21.58	2.57	11.92	3
<span style="color: darkred;">■</span> Erba Chem 5/Plus	1	--	--	--	1

<b>Your Result</b>	14.20	<b>SDI / z-Score</b>	-2.92
<b>Assigned Value</b>	21.82	<b>Average SDI</b>	-3.50
<b>SDPA</b>	2.610	<b>Uncertainty of AV</b>	0.28
<b>Standard Unit Result Val</b>	14.20	<b>%DEV</b>	-34.19

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

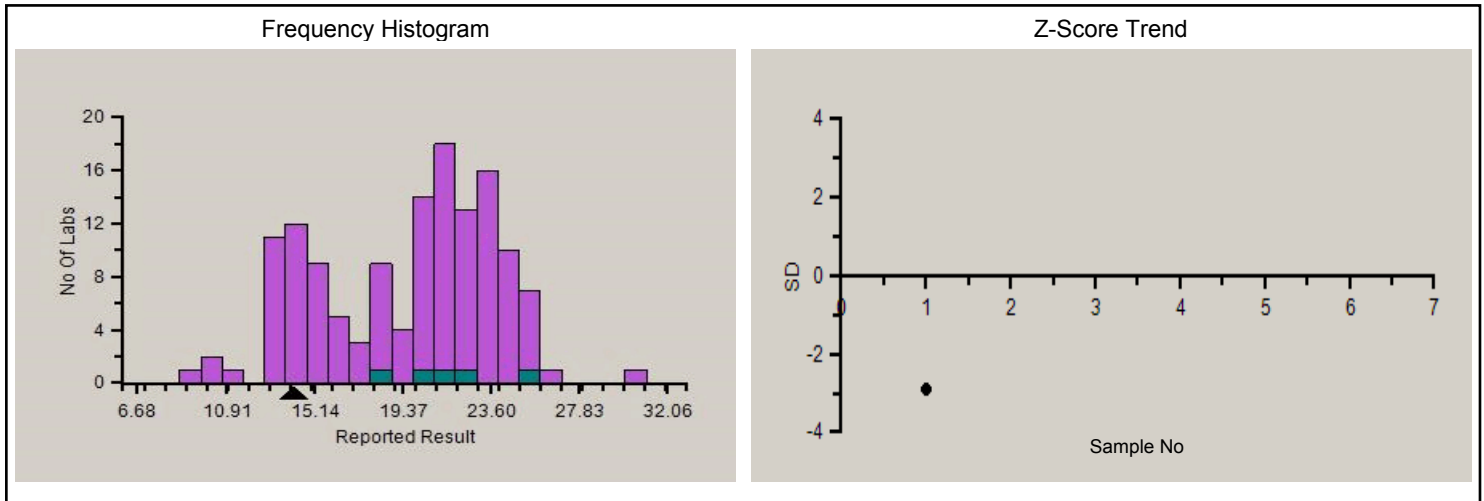

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 1  
 Sample Date : 01-07-2021

Biochemistry, GGT		N	Mean	SD	CV%	Excluded
	All Analyzer	146	19.37	4.23	21.86	9
<b>Your Analyzer :</b>	<b>Erba Chem 5/Plus</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	33	14.39	1.73	12.03	--
	Fuji Dri-Chem NX500/i	33	14.39	1.73	12.03	--
	Roche cobas c 311	26	22.15	1.59	7.19	--
	Roche cobas c 111	12	20.15	1.41	7.00	1
	Fuji Dri-Chem 4000i	11	14.20	1.55	10.91	1
	Roche cobas INTEGRA	11	20.61	1.34	6.50	--
	Horiba ABX Pentra C200	7	21.35	2.47	11.58	1
	Roche cobas 6000	7	22.29	2.22	9.94	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 1  
Sample Date : 01-07-2021


**Biochemistry, LDH, U/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	106	146.81	54.09	36.85	5
<span style="color: teal;">■</span> Kinetic UV optimized DGKC	5	210.46	68.82	32.70	--
<span style="color: darkred;">■</span> Erba Chem 5/Plus	2	249.60	--	--	--

<b>Your Result</b>	241.20	<b>SDI / z-Score</b>	-1.17
<b>Assigned Value</b>	272.00	<b>Average SDI</b>	-1.68
<b>SDPA</b>	26.357	<b>Uncertainty of AV</b>	10.98
<b>Standard Unit Result Val</b>	241.20	<b>%DEV</b>	14.61

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

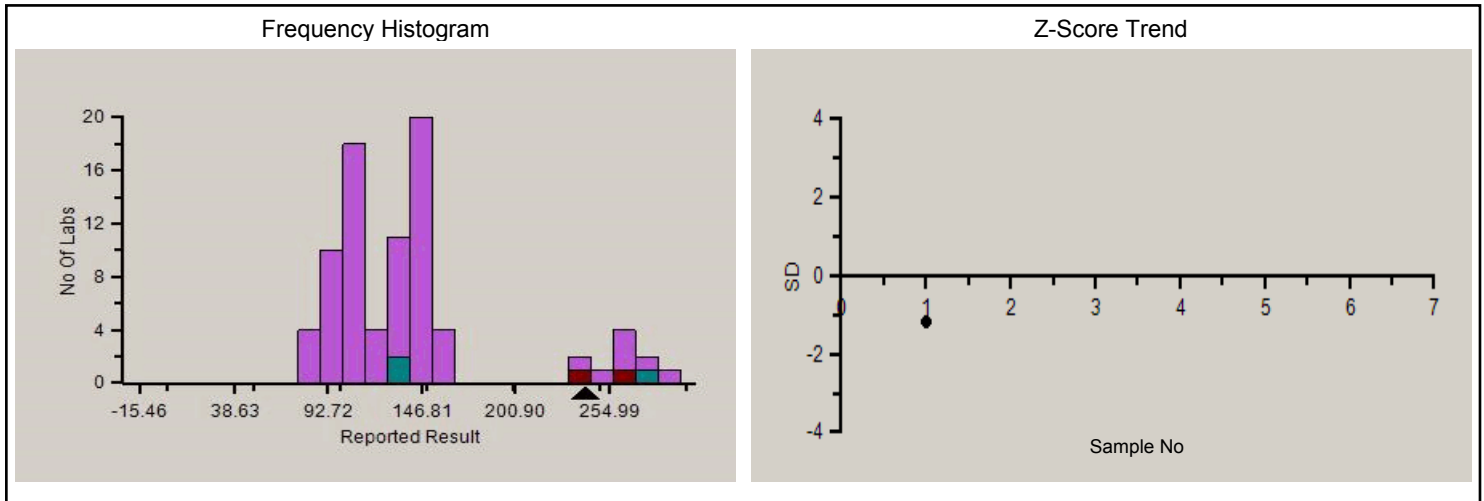

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 1  
 Sample Date : 01-07-2021

Biochemistry, LDH		N	Mean	SD	CV%	Excluded
	All Analyzer	106	146.81	54.09	36.85	5
<b>Your Analyzer :</b>	<b>Erba Chem 5/Plus</b>	<b>2</b>	<b>249.60</b>	--	--	--
	Fuji Dri-Chem NX500/i	26	101.87	9.74	9.56	3
	Roche cobas c 311	17	147.21	6.06	4.11	1
	Fuji Dri-Chem 4000i	10	103.56	6.88	6.64	1
	Roche cobas INTEGRA	8	143.98	5.96	4.14	--
	Roche cobas 6000	6	151.50	2.59	1.71	--
	Beckman Coulter AU480	4	139.73	11.23	8.04	--
	Erba EM 200	4	291.50	25.57	8.77	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 1  
Sample Date : 01-07-2021


**Biochemistry, Magnesium, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	53	1.06	0.67	63.54	3
<span style="color: teal;">■</span> Calmagite	2	1.98	--	--	--
<span style="color: darkred;">■</span> Erba Chem 5/Plus	1	--	--	--	--

<b>Your Result</b>	2.10	<b>SDI / z-Score</b>	1.24
<b>Assigned Value</b>	1.80	<b>Average SDI</b>	0.87
<b>SDPA</b>	0.242	<b>Uncertainty of AV</b>	0.03
<b>Standard Unit Result Val</b>	2.10	<b>%DEV</b>	6.06

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

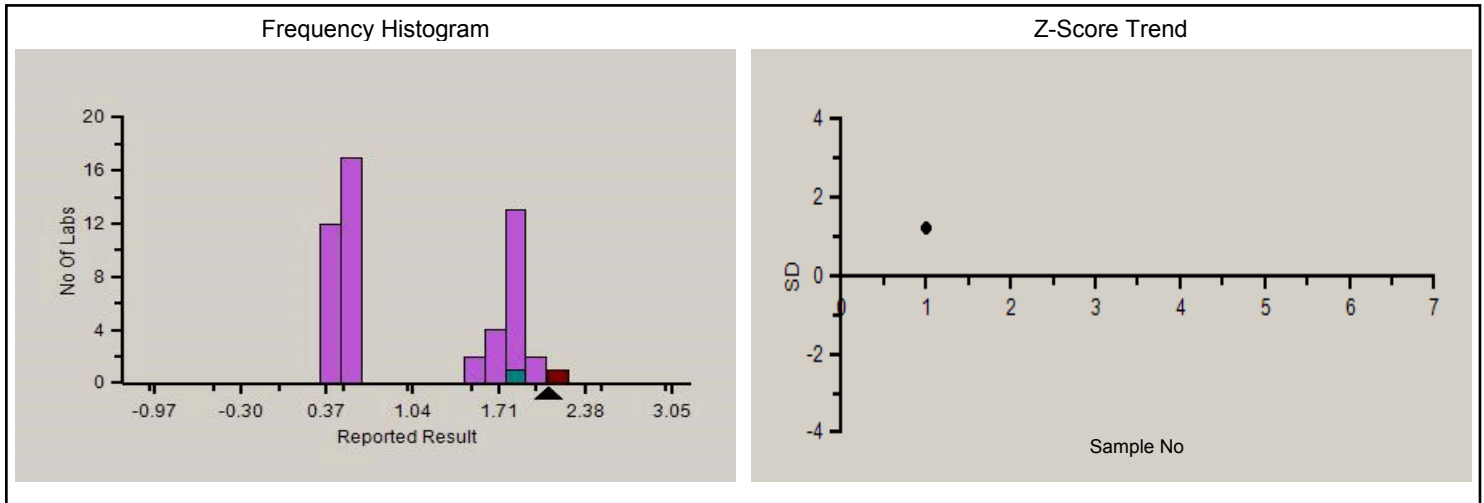

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 1  
 Sample Date : 01-07-2021

Biochemistry, Magnesium		N	Mean	SD	CV%	Excluded
	All Analyzer	53	1.06	0.67	63.54	3
<b>Your Analyzer :</b>	<b>Erba Chem 5/Plus</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	17	0.46	0.04	8.30	--
	Fuji Dri-Chem NX500/i	17	0.46	0.04	8.30	--
	Fuji Dri-Chem 4000i	10	0.49	0.03	6.53	--
	Roche cobas c 311	7	1.76	0.13	7.22	--
	Roche cobas 6000	6	1.78	0.04	2.25	--
	Roche cobas 8000	4	1.82	0.18	9.65	--
	Roche cobas INTEGRA	2	1.78	--	--	--
	Fuji Nx 700	2	0.50	--	--	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 1  
Sample Date : 01-07-2021


**Biochemistry, Potassium, mEq/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	166	5.74	0.93	16.14	14
<span style="color: teal;">■</span> ISE direct	117	6.26	0.30	4.80	1
<span style="color: darkred;">■</span> EasyLyte	9	5.82	0.20	3.51	--

<b>Your Result</b>	6.09	<b>SDI / z-Score</b>	-0.62
<b>Assigned Value</b>	6.27	<b>Average SDI</b>	-0.65
<b>SDPA</b>	0.296	<b>Uncertainty of AV</b>	0.03
<b>Standard Unit Result Val</b>	6.09	<b>%DEV</b>	4.62

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

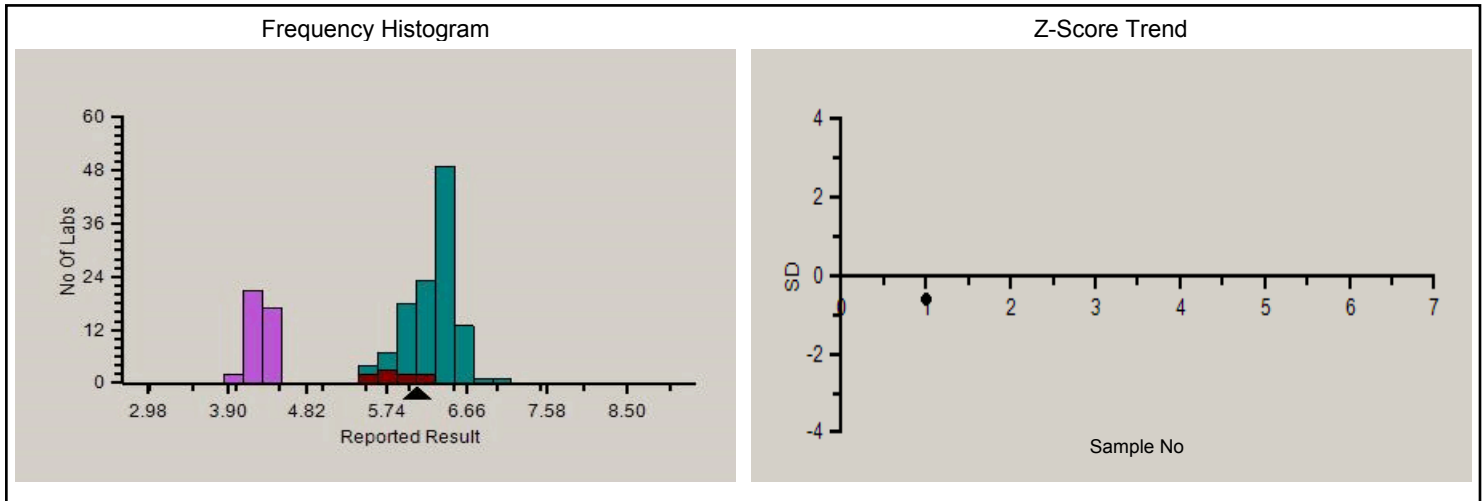

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 1  
 Sample Date : 01-07-2021

<b>Biochemistry, Potassium</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	166	5.74	0.93	16.14	14
<b>Your Analyzer :</b>	<b>EasyLyte</b>	<b>9</b>	<b>5.82</b>	<b>0.20</b>	<b>3.51</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	39	6.37	0.24	3.70	2
	Fuji Dri-Chem NX500/i	39	6.37	0.24	3.70	2
	Fuji Dri-Chem 4000i	17	6.35	0.14	2.22	1
	Roche cobas c 311	17	4.35	0.41	9.43	--
	Roche AVL 9180	13	6.57	0.17	2.59	--
	Roche cobas 6000	8	4.29	0.05	1.07	--
	Bene Sphera C73	8	5.91	0.30	5.03	4

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 1  
Sample Date : 01-07-2021


**Biochemistry, Sodium, mEq/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	165	161.97	22.60	13.96	14
<span style="color: teal;">■</span> ISE direct	118	174.94	5.88	3.36	2
<span style="color: darkred;">■</span> EasyLyte	10	168.95	5.89	3.49	--

<b>Your Result</b>	172.50	<b>SDI / z-Score</b>	-0.29
<b>Assigned Value</b>	175.51	<b>Average SDI</b>	-0.38
<b>SDPA</b>	10.530	<b>Uncertainty of AV</b>	0.64
<b>Standard Unit Result Val</b>	172.50	<b>%DEV</b>	2.10

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

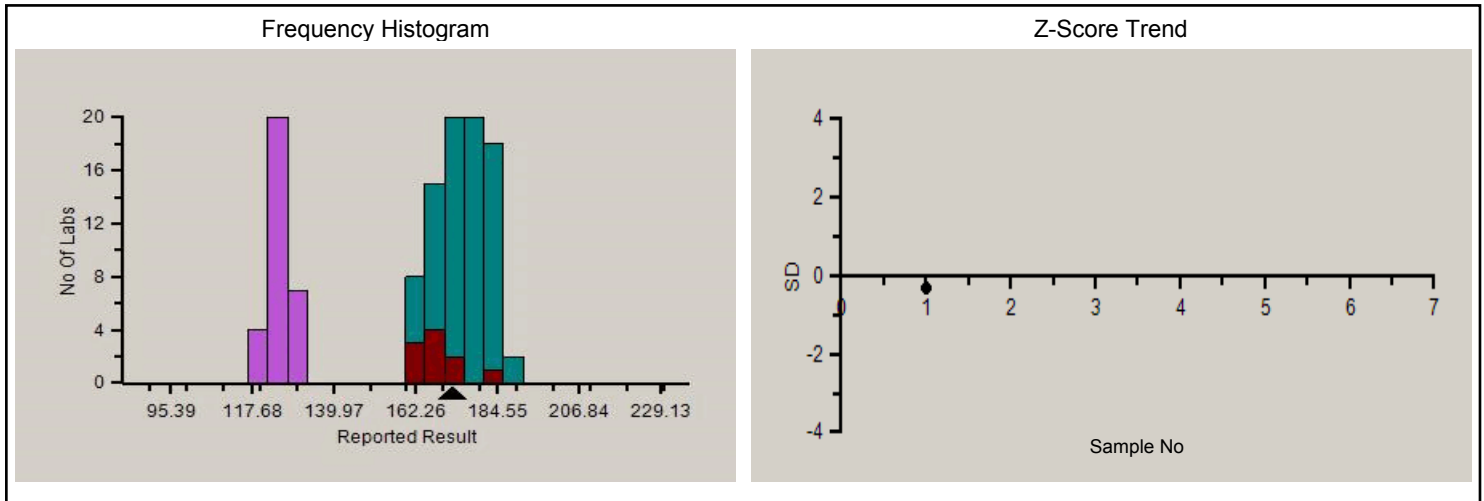

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 1  
 Sample Date : 01-07-2021

Biochemistry, Sodium		N	Mean	SD	CV%	Excluded
	All Analyzer	165	161.97	22.60	13.96	14
<b>Your Analyzer :</b>	<b>EasyLyte</b>	<b>10</b>	<b>168.95</b>	<b>5.89</b>	<b>3.49</b>	--
	Fuji Dri-Chem NX500/i	40	173.81	5.94	3.42	3
	Fuji Dri-Chem NX500/i	40	173.81	5.94	3.42	3
	Roche cobas c 311	17	128.12	14.08	10.99	--
	Fuji Dri-Chem 4000i	16	175.80	1.90	1.08	1
	Roche AVL 9180	13	180.20	2.88	1.60	--
	Roche cobas 6000	8	125.63	1.77	1.41	--
	Bene Sphera C73	8	170.95	2.84	1.66	4

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 1  
Sample Date : 01-07-2021


**Biochemistry, Total Protein, g/dL**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	231	6.46	0.33	5.11	13
<span style="color: teal;">■</span> Biuret	227	6.47	0.33	5.06	12
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	2	6.23	--	--	--

<b>Your Result</b>	6.31	<b>SDI / z-Score</b>	-0.16
<b>Assigned Value</b>	6.37	<b>Average SDI</b>	-0.27
<b>SDPA</b>	0.350	<b>Uncertainty of AV</b>	0.06
<b>Standard Unit Result Val</b>	6.31	<b>%DEV</b>	-2.46

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

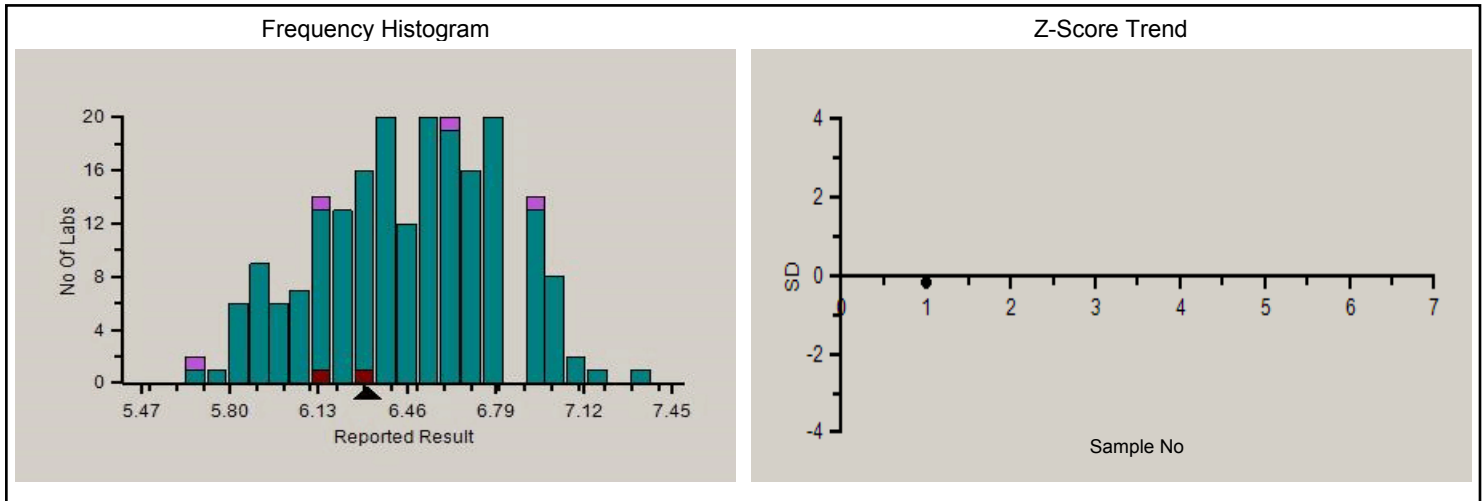

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 1  
 Sample Date : 01-07-2021

<b>Biochemistry, Total Protein</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	231	6.46	0.33	5.11	13
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>2</b>	<b>6.23</b>	--	--	--
	Fuji Dri-Chem NX500/i	37	6.81	0.20	2.86	1
	Fuji Dri-Chem NX500/i	37	6.81	0.20	2.86	1
	Roche cobas c 311	29	6.50	0.18	2.80	--
	Biosystems A15	22	6.44	0.31	4.88	2
	Biosystems A15	22	6.44	0.31	4.88	2
	Erba EM 200	19	6.30	0.32	5.03	3
	Erba EM 200	18	6.32	0.32	5.10	3

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 1  
Sample Date : 01-07-2021


**Biochemistry, Triglycerides, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	228	147.84	14.49	9.80	11
GPO - Peroxidase	18	142.48	14.74	10.35	2
Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	158.50	<b>SDI / z-Score</b>	0.12
<b>Assigned Value</b>	156.13	<b>Average SDI</b>	-0.15
<b>SDPA</b>	20.042	<b>Uncertainty of AV</b>	4.23
<b>Standard Unit Result Val</b>	158.50	<b>%DEV</b>	11.25

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

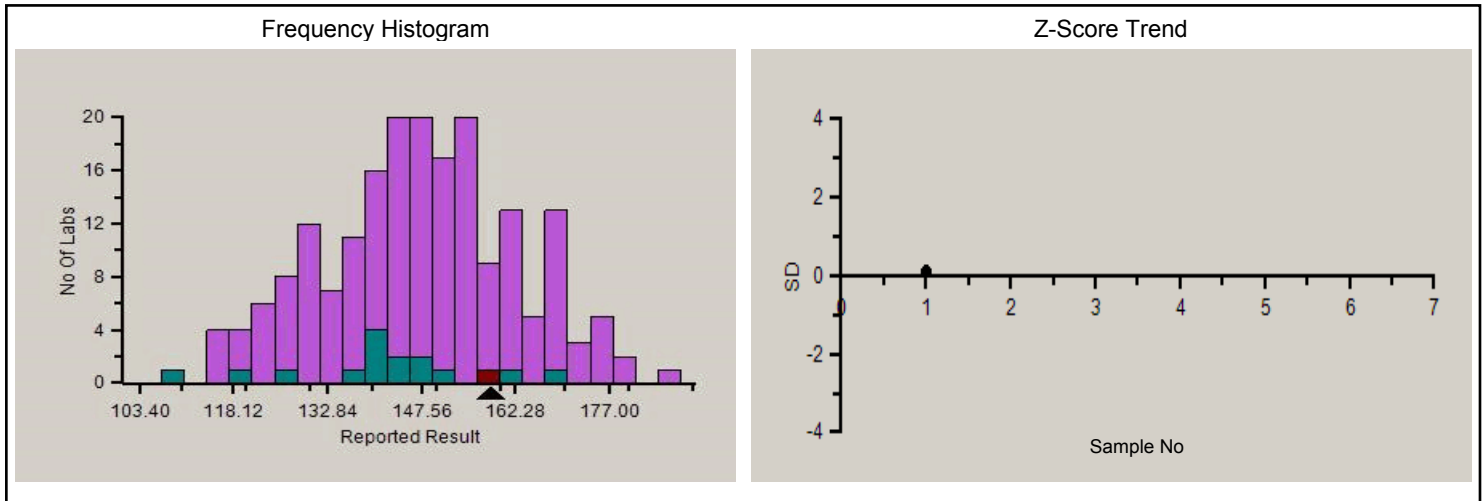

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 1  
 Sample Date : 01-07-2021

<b>Biochemistry, Triglycerides</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	228	147.84	14.49	9.80	11
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	34	140.44	9.30	6.63	--
	Roche cobas c 311	29	155.13	9.99	6.44	1
	Biosystems A15	22	134.29	16.03	11.94	3
	Biosystems A15	22	134.29	16.03	11.94	3
	ERBA XL-640	17	166.14	15.68	9.44	2
	Erba EM 200	15	147.55	17.74	12.03	3
	Fuji Dri-Chem 4000i	15	138.87	10.78	7.77	--
	Erba EM 200	14	149.64	17.00	11.36	3

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 1  
Sample Date : 01-07-2021


**Biochemistry, Uric Acid, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	230	4.50	0.39	8.72	10
<span style="color: teal;">■</span> Uricase	38	4.47	0.34	7.54	2
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	4.57	<b>SDI / z-Score</b>	-0.78
<b>Assigned Value</b>	4.88	<b>Average SDI</b>	-0.82
<b>SDPA</b>	0.392	<b>Uncertainty of AV</b>	0.08
<b>Standard Unit Result Val</b>	4.57	<b>%DEV</b>	2.24

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

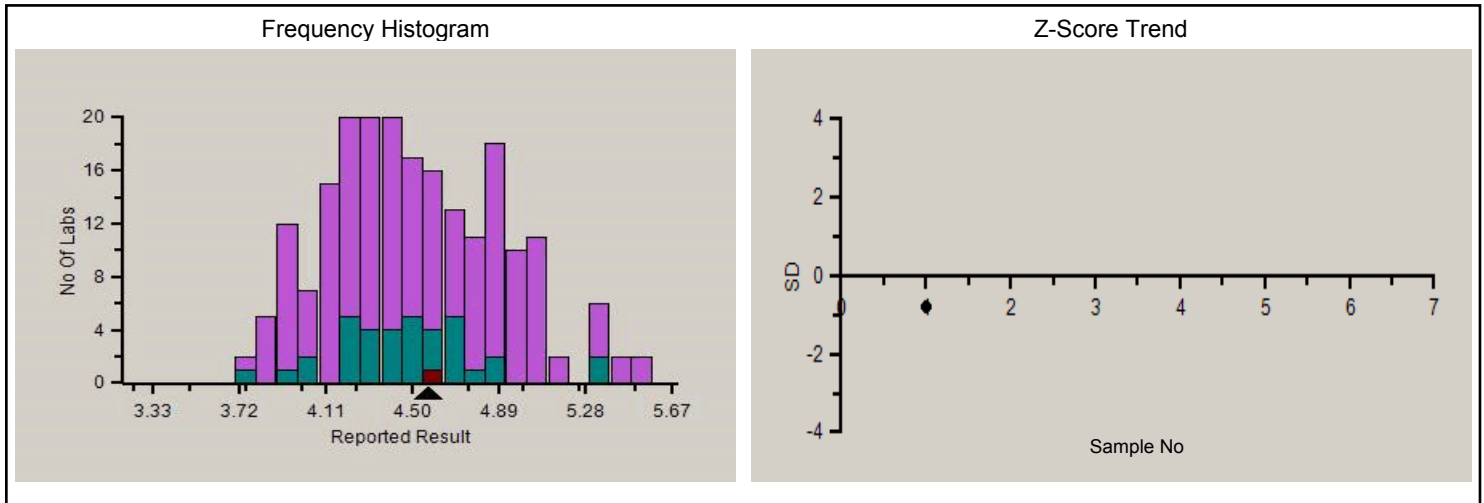

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 1  
Sample Date : 01-07-2021

Biochemistry, Uric Acid		N	Mean	SD	CV%	Excluded
	All Analyzer	230	4.50	0.39	8.72	10
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	35	4.83	0.21	4.41	1
	Fuji Dri-Chem NX500/i	35	4.83	0.21	4.41	1
	Roche cobas c 311	27	4.23	0.23	5.35	--
	Biosystems A15	21	4.14	0.24	5.70	6
	Biosystems A15	21	4.14	0.24	5.70	6
	Erba EM 200	18	4.80	0.35	7.27	--
	ERBA XL-640	18	5.03	0.30	5.87	--
	ERBA XL-640	18	5.03	0.30	5.87	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.

*Dr Puneet Kumar Nigam*

**Dr Puneet Kumar Nigam**  
**PT coordinator & Technical Manager, MHL EQAS**  
Unit No. 409-416.  
Commercial Building - 1A,  
Kohinoor Mall, Kiroi Road, Kuria (W),  
Mumbai - 400070



PC-1022



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 2  
Sample Date : 02-07-2021


**Biochemistry, Albumin, g/dL**

	N	Mean	SD	CV%	Excluded
All Methods	234	3.94	0.46	11.55	15
Bromcresol Green (BCG)	228	3.95	0.46	11.58	15
Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	3.45	<b>SDI / z-Score</b>	-0.26
<b>Assigned Value</b>	3.52	<b>Average SDI</b>	-0.08
<b>SDPA</b>	0.246	<b>Uncertainty of AV</b>	0.04
<b>Standard Unit Result Val</b>	3.45	<b>%DEV</b>	-12.57

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

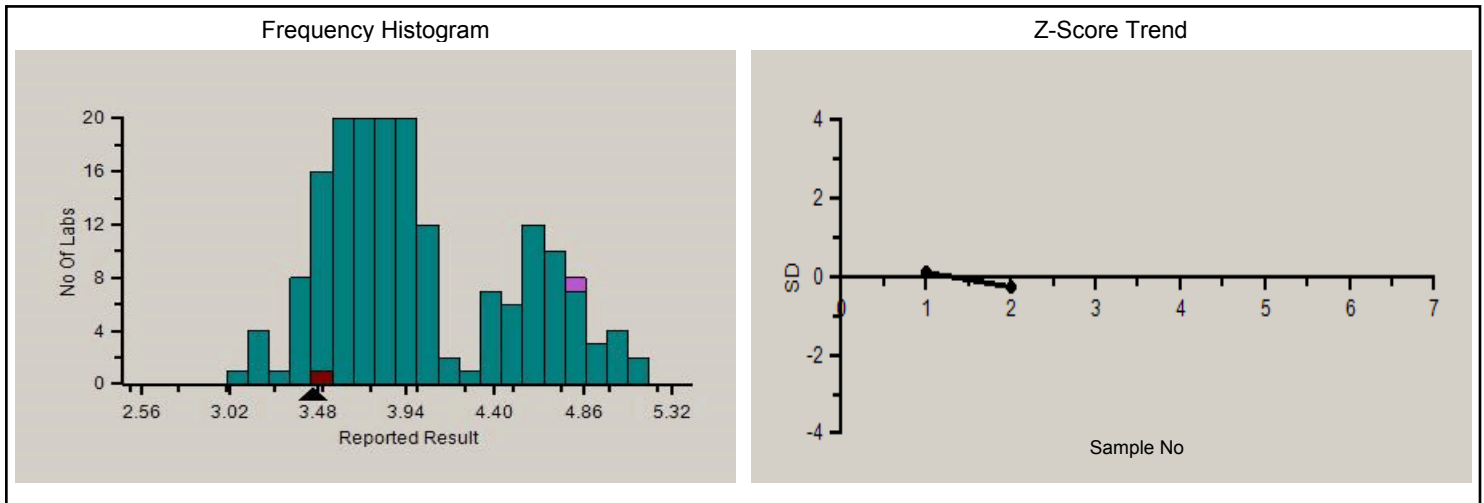

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 2  
 Sample Date : 02-07-2021

Biochemistry, Albumin		N	Mean	SD	CV%	Excluded
	All Analyzer	234	3.94	0.46	11.55	15
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	1	--	--	--	--
	Fuji Dri-Chem NX500/i	37	4.66	0.19	4.10	1
	Fuji Dri-Chem NX500/i	36	4.67	0.19	4.11	1
	Roche cobas c 311	28	3.85	0.09	2.42	--
	Biosystems A15	22	3.90	0.32	8.08	2
	Biosystems A15	22	3.90	0.32	8.08	2
	Erba EM 200	19	3.53	0.22	6.29	2
	Erba EM 200	19	3.53	0.22	6.29	2
	ERBA XL-640	18	3.45	0.20	5.86	1

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 2  
Sample Date : 02-07-2021


**Biochemistry, ALP, U/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	232	84.51	17.89	21.17	18
<span style="color: teal;">■</span> IFCC	25	80.05	24.73	30.90	2
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	76.00	<b>SDI / z-Score</b>	-0.05
<b>Assigned Value</b>	76.54	<b>Average SDI</b>	-0.20
<b>SDPA</b>	10.715	<b>Uncertainty of AV</b>	0.70
<b>Standard Unit Result Val</b>	76.00	<b>%DEV</b>	-5.06

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

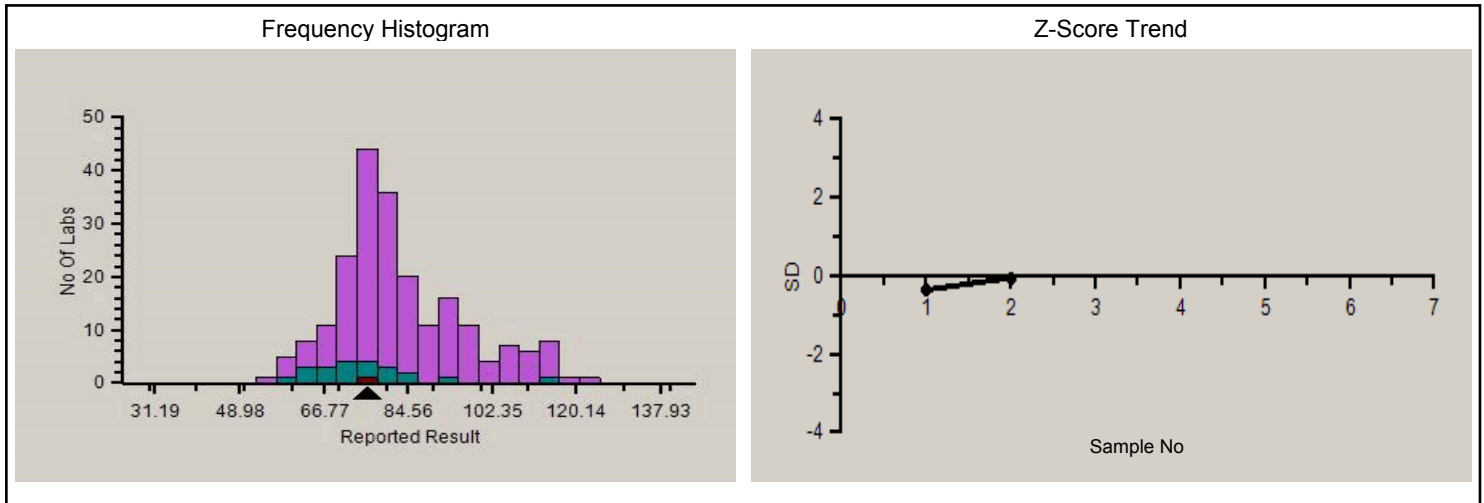

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 2  
 Sample Date : 02-07-2021

Biochemistry, ALP		N	Mean	SD	CV%	Excluded
	All Analyzer	232	84.51	17.89	21.17	18
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	36	103.11	10.04	9.74	--
	Fuji Dri-Chem NX500/i	35	103.31	10.11	9.79	--
	Roche cobas c 311	28	78.57	4.48	5.70	--
	Biosystems A15	22	81.09	9.38	11.57	2
	Biosystems A15	22	81.09	9.38	11.57	2
	Erba EM 200	17	73.01	6.66	9.12	2
	Erba EM 200	17	73.01	6.66	9.12	2
	ERBA XL-640	17	75.24	8.87	11.79	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 2  
Sample Date : 02-07-2021


**Biochemistry, ALT, U/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	237	21.76	18.14	83.35	66
<span style="color: teal;">■</span> IFCC	33	16.92	5.66	33.48	14
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	1

<b>Your Result</b>	12.50	<b>SDI / z-Score</b>	-2.11
<b>Assigned Value</b>	20.10	<b>Average SDI</b>	-0.12
<b>SDPA</b>	3.610	<b>Uncertainty of AV</b>	0.74
<b>Standard Unit Result Val</b>	12.50	<b>%DEV</b>	-26.11

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

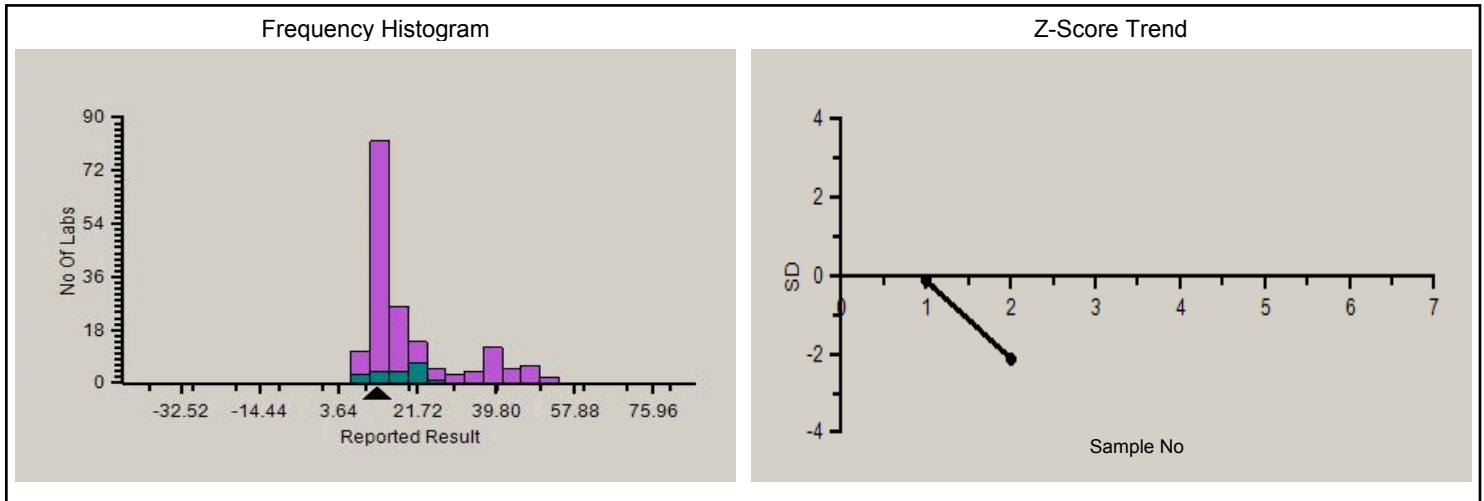

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 2  
 Sample Date : 02-07-2021

Biochemistry, ALT		N	Mean	SD	CV%	Excluded
	All Analyzer	237	21.76	18.14	83.35	66
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	36	41.33	5.91	14.30	15
	Fuji Dri-Chem NX500/i	35	41.90	5.45	13.00	15
	Roche cobas c 311	28	14.53	1.52	10.44	--
	Biosystems A15	22	11.29	2.11	18.65	6
	Biosystems A15	22	11.29	2.11	18.65	6
	Erba EM 200	19	20.01	2.19	10.92	11
	Erba EM 200	19	20.01	2.19	10.92	11
	ERBA XL-640	18	19.91	2.81	14.10	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 2  
Sample Date : 02-07-2021


**Biochemistry, AST, U/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	234	26.67	8.36	31.35	48
<span style="color: teal;">■</span> IFCC	31	29.31	8.65	29.52	10
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	27.00	<b>SDI / z-Score</b>	-1.31
<b>Assigned Value</b>	35.73	<b>Average SDI</b>	-0.79
<b>SDPA</b>	6.690	<b>Uncertainty of AV</b>	1.64
<b>Standard Unit Result Val</b>	27.00	<b>%DEV</b>	-7.89

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

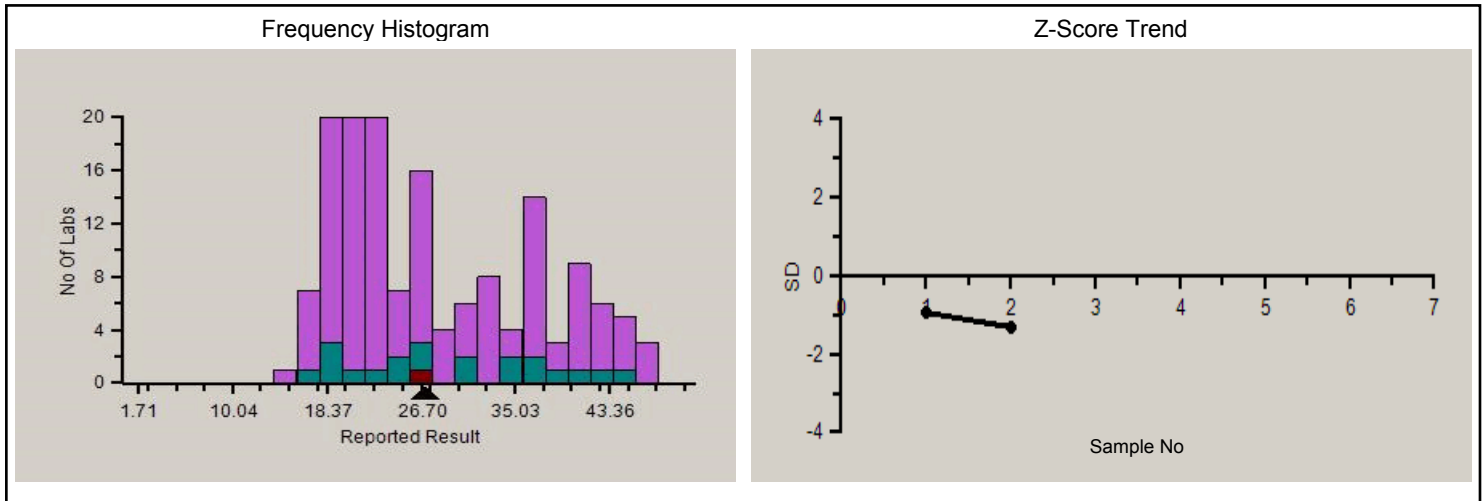

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 2  
 Sample Date : 02-07-2021

Biochemistry, AST		N	Mean	SD	CV%	Excluded
	All Analyzer	234	26.67	8.36	31.35	48
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	37	36.85	5.68	15.42	10
	Fuji Dri-Chem NX500/i	36	37.00	5.74	15.52	10
	Roche cobas c 311	27	22.43	2.12	9.45	1
	Biosystems A15	21	20.52	2.82	13.76	4
	Biosystems A15	21	20.52	2.82	13.76	4
	Erba EM 200	19	32.86	6.61	20.13	8
	Erba EM 200	19	32.86	6.61	20.13	8
	ERBA XL-640	18	37.13	5.52	14.87	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 2  
Sample Date : 02-07-2021


**Biochemistry, Bilirubin Direct, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	228	0.11	0.02	17.76	83
<span style="color: teal;">■</span> Jendrassik Grof	6	--	--	--	6
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	1

<b>Your Result</b>	0.02	<b>SDI / z-Score</b>	-2.49
<b>Assigned Value</b>	0.11	<b>Average SDI</b>	-1.88
<b>SDPA</b>	0.035	<b>Uncertainty of AV</b>	0.01
<b>Standard Unit Result Val</b>	0.02	<b>%DEV</b>	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

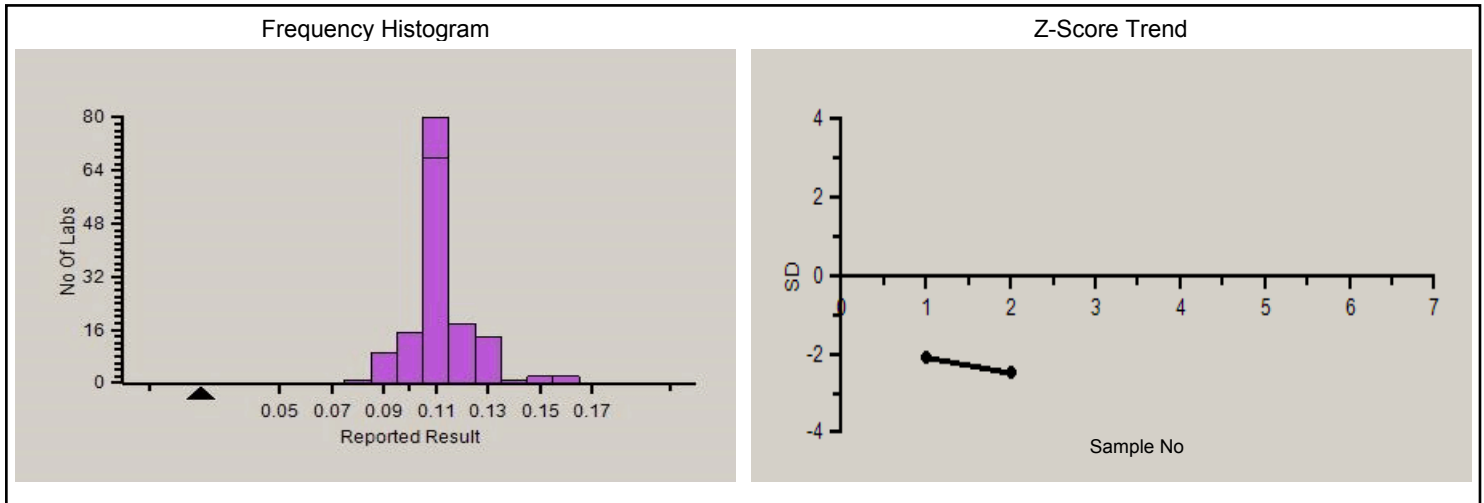

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 2  
 Sample Date : 02-07-2021

<b>Biochemistry, Bilirubin Direct</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	228	0.11	0.02	17.76	83
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	36	0.10	0.01	9.80	13
	Fuji Dri-Chem NX500/i	35	0.10	0.01	6.00	13
	Roche cobas c 311	26	0.10	0.01	14.14	6
	Biosystems A15	21	0.15	0.04	24.67	14
	Biosystems A15	21	0.15	0.04	24.67	14
	Erba EM 200	19	0.11	0.02	17.76	10
	Erba EM 200	19	0.11	0.02	17.76	10
	ERBA XL-640	17	0.11	0.01	10.71	4

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 2  
Sample Date : 02-07-2021


**Biochemistry, Bilirubin Total, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	229	0.35	0.15	41.60	91
<span style="color: teal;">■</span> Jendrassik Grof	12	0.32	0.13	41.69	4
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	1

<b>Your Result</b>	0.18	<b>SDI / z-Score</b>	-0.60
<b>Assigned Value</b>	0.22	<b>Average SDI</b>	-0.84
<b>SDPA</b>	0.058	<b>Uncertainty of AV</b>	0.01
<b>Standard Unit Result Val</b>	0.18	<b>%DEV</b>	-43.57

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

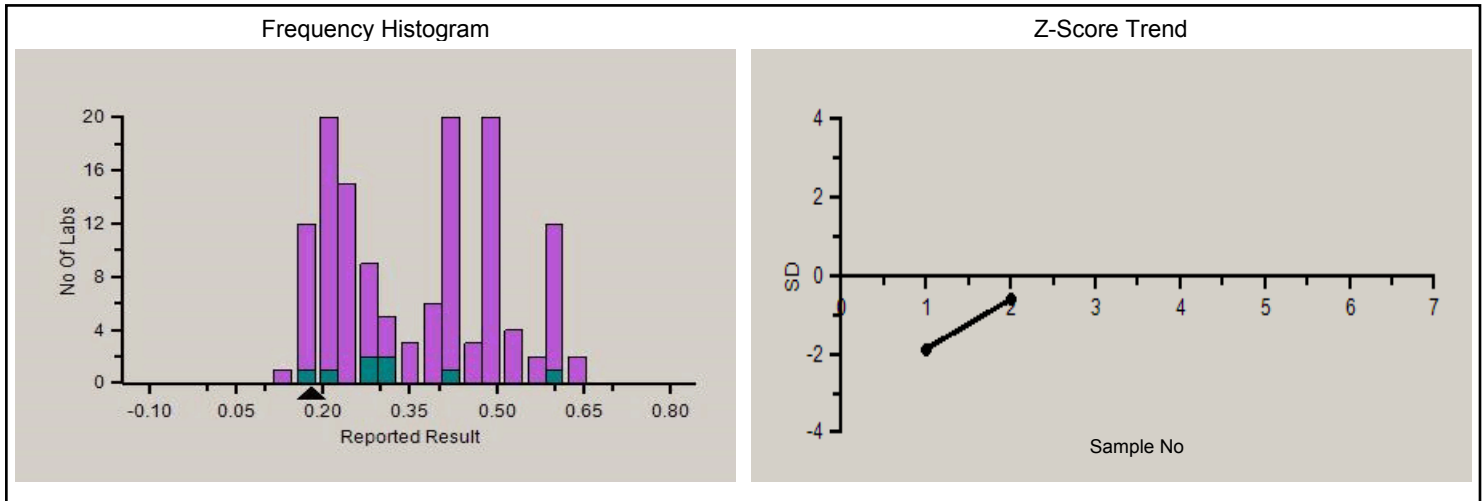

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 2  
 Sample Date : 02-07-2021

<b>Biochemistry, Bilirubin Total</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	229	0.35	0.15	41.60	91
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	36	0.48	0.07	14.70	7
	Fuji Dri-Chem NX500/i	35	0.48	0.07	15.08	7
	Roche cobas c 311	27	0.21	0.03	13.66	5
	Erba EM 200	19	0.00	0.00	0.00	18
	Erba EM 200	19	0.00	0.00	0.00	18
	ERBA XL-640	18	--	--	--	18
	Biosystems A15	17	0.51	0.06	12.67	6
	Biosystems A15	17	0.51	0.06	12.67	6

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 2  
Sample Date : 02-07-2021


**Biochemistry, Chloride, mEq/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	152	106.46	11.99	11.27	20
<span style="color: teal;">■</span> ISE direct	108	113.27	4.25	3.75	8
<span style="color: red;">■</span> EasyLyte	8	111.75	3.37	3.02	2

<b>Your Result</b>	127.60	<b>SDI / z-Score</b>	1.55
<b>Assigned Value</b>	113.49	<b>Average SDI</b>	1.84
<b>SDPA</b>	9.079	<b>Uncertainty of AV</b>	0.54
<b>Standard Unit Result Val</b>	127.60	<b>%DEV</b>	14.18

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

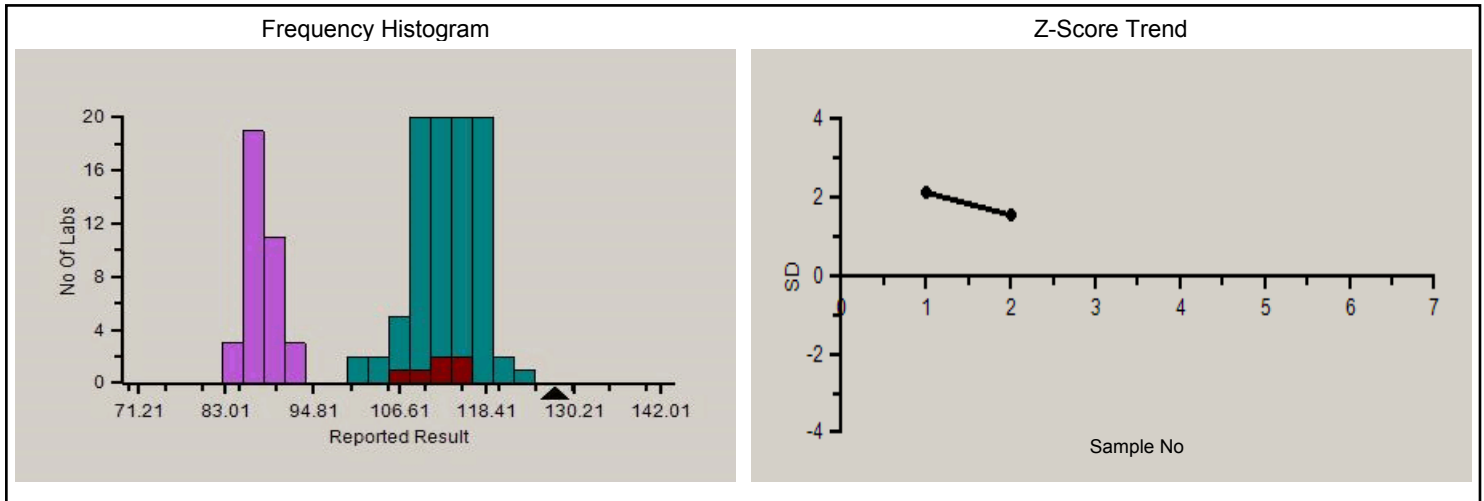

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 2  
 Sample Date : 02-07-2021

Biochemistry, Chloride		N	Mean	SD	CV%	Excluded
	All Analyzer	152	106.46	11.99	11.27	20
<b>Your Analyzer :</b>	<b>EasyLyte</b>	<b>8</b>	<b>111.75</b>	<b>3.37</b>	<b>3.02</b>	<b>2</b>
	Fuji Dri-Chem NX500/i	37	115.19	3.85	3.35	1
	Fuji Dri-Chem NX500/i	36	115.29	3.87	3.36	1
	Fuji Dri-Chem 4000i	15	115.93	3.34	2.88	1
	Roche cobas c 311	15	89.19	7.37	8.26	1
	Roche AVL 9180	11	110.27	2.15	1.95	--
	Roche cobas 6000	8	87.20	1.52	1.74	1
	Bene Sphera C73	8	110.04	1.45	1.31	3

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 2  
Sample Date : 02-07-2021


**Biochemistry, LDH, U/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	106	161.41	56.21	34.83	3
<span style="color: teal;">■</span> Kinetic UV optimized DGKC	6	243.27	62.69	25.77	--
<span style="color: darkred;">■</span> Erba Chem 5/Plus	1	--	--	--	--

<b>Your Result</b>	246.90	<b>SDI / z-Score</b>	-2.28
<b>Assigned Value</b>	306.00	<b>Average SDI</b>	-1.68
<b>SDPA</b>	25.874	<b>Uncertainty of AV</b>	10.78
<b>Standard Unit Result Val</b>	246.90	<b>%DEV</b>	1.49

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

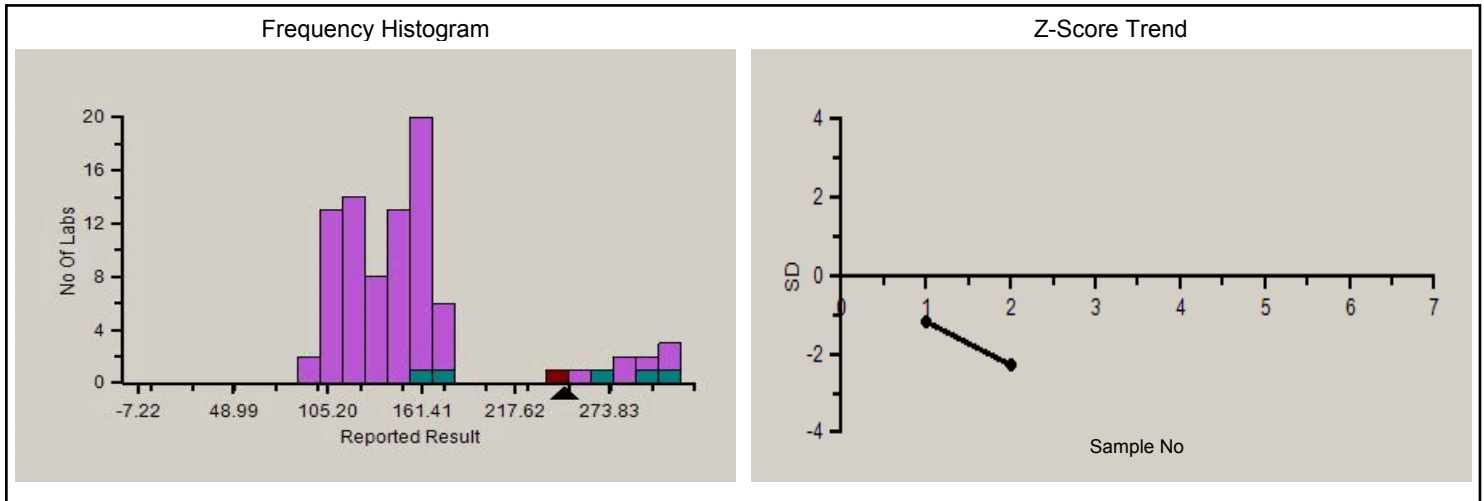

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 2  
 Sample Date : 02-07-2021

Biochemistry, LDH		N	Mean	SD	CV%	Excluded
	All Analyzer	106	161.41	56.21	34.83	3
<b>Your Analyzer :</b>	<b>Erba Chem 5/Plus</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	26	115.50	10.46	9.05	2
	Roche cobas c 311	18	161.39	5.81	3.60	1
	Fuji Dri-Chem 4000i	9	120.11	8.68	7.23	--
	Roche cobas INTEGRA	8	157.84	6.21	3.93	--
	Roche cobas 6000	6	164.73	4.24	2.57	--
	Beckman Coulter AU480	4	152.03	9.81	6.45	--
	Erba EM 200	4	314.33	21.23	6.76	--
	Horiba ABX Pentra C200	4	153.75	5.44	3.54	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 2  
Sample Date : 02-07-2021


**Biochemistry, Lipase, U/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	111	49.04	15.52	31.66	14
<span style="color: teal;">■</span> Turbidimetric	2	--	--	--	2
<span style="color: darkred;">■</span> Erba Chem 5/Plus	1	--	--	--	1

<b>Your Result</b>	94.90	<b>SDI / z-Score</b>	1.88
<b>Assigned Value</b>	67.20	<b>Average SDI</b>	16.48
<b>SDPA</b>	14.724	<b>Uncertainty of AV</b>	8.23
<b>Standard Unit Result Val</b>	94.90	<b>%DEV</b>	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

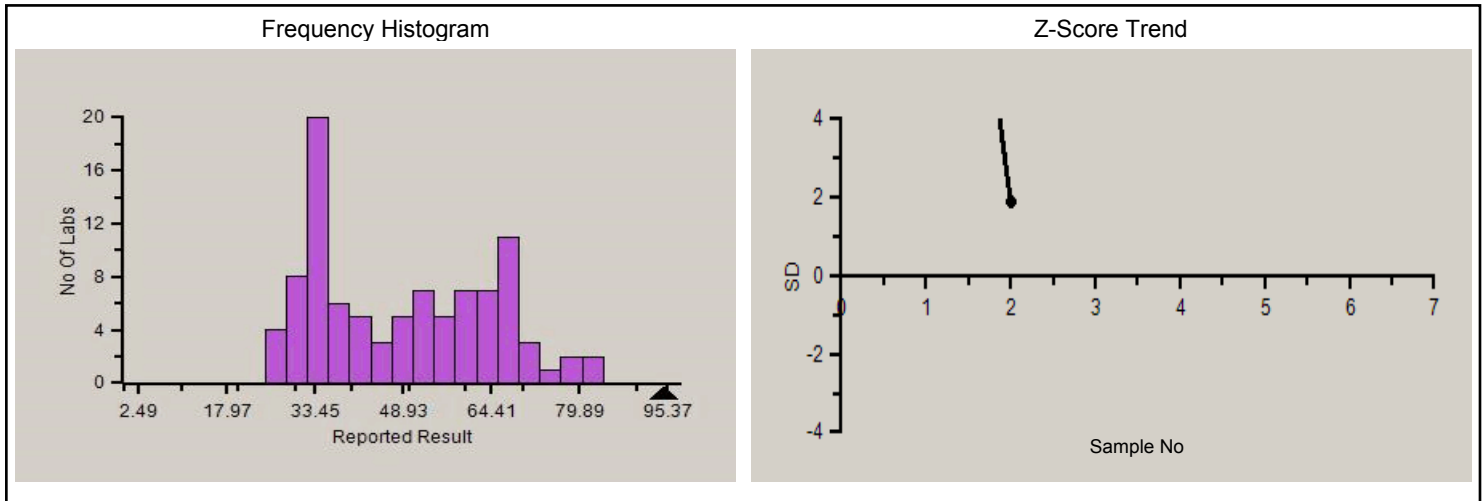

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 2  
 Sample Date : 02-07-2021

<b>Biochemistry, Lipase</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	111	49.04	15.52	31.66	14
<b>Your Analyzer :</b>	<b>Erba Chem 5/Plus</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	24	62.92	7.95	12.63	--
	Biosystems A15	18	42.19	7.24	17.17	5
	Biosystems A15	18	42.19	7.24	17.17	5
	Fuji Dri-Chem 4000i	14	61.86	5.70	9.21	--
	Roche cobas c 311	11	35.06	2.52	7.19	--
	ERBA XL-640	6	69.12	14.72	21.30	1
	Roche cobas INTEGRA	6	33.20	1.76	5.29	--
	Roche cobas 6000	5	32.44	2.33	7.20	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 2  
Sample Date : 02-07-2021


**Biochemistry, Magnesium, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	53	1.08	0.68	63.17	2
<span style="color: teal;">■</span> Calmagite	2	1.97	--	--	--
<span style="color: darkred;">■</span> Erba Chem 5/Plus	1	--	--	--	--

<b>Your Result</b>	2.10	<b>SDI / z-Score</b>	1.21
<b>Assigned Value</b>	1.82	<b>Average SDI</b>	0.87
<b>SDPA</b>	0.235	<b>Uncertainty of AV</b>	0.03
<b>Standard Unit Result Val</b>	2.10	<b>%DEV</b>	6.60

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

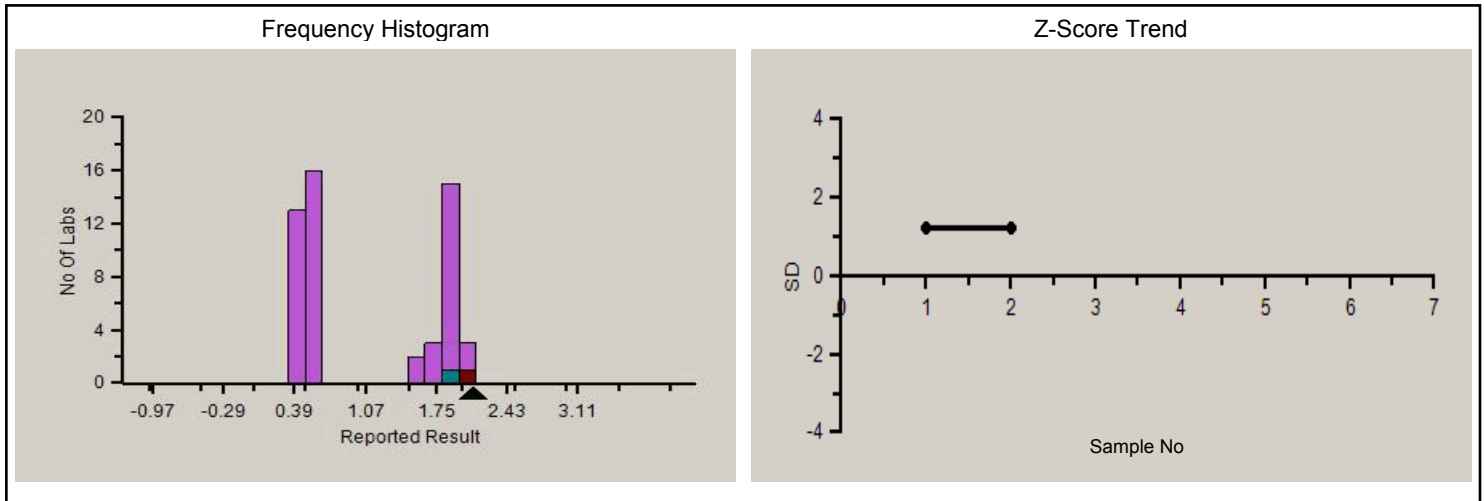

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 2  
 Sample Date : 02-07-2021

<b>Biochemistry, Magnesium</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	53	1.08	0.68	63.17	2
<b>Your Analyzer :</b>	<b>Erba Chem 5/Plus</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	17	0.46	0.04	8.23	--
	Fuji Dri-Chem NX500/i	16	0.46	0.04	8.21	--
	Fuji Dri-Chem 4000i	10	0.48	0.04	8.75	--
	Roche cobas c 311	7	1.78	0.11	6.39	--
	Roche cobas 6000	6	1.79	0.04	2.35	--
	Roche cobas 8000	4	1.81	0.16	9.05	--
	Roche cobas INTEGRA	2	1.80	--	--	--
	Fuji Nx 700	2	0.50	--	--	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 2  
Sample Date : 02-07-2021


**Biochemistry, Potassium, mEq/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	165	5.62	0.87	15.55	14
<span style="color: teal;">■</span> ISE direct	118	6.09	0.29	4.71	1
<span style="color: darkred;">■</span> EasyLyte	9	5.71	0.18	3.22	--

<b>Your Result</b>	5.91	<b>SDI / z-Score</b>	-0.67
<b>Assigned Value</b>	6.10	<b>Average SDI</b>	-0.65
<b>SDPA</b>	0.287	<b>Uncertainty of AV</b>	0.03
<b>Standard Unit Result Val</b>	5.91	<b>%DEV</b>	3.48

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

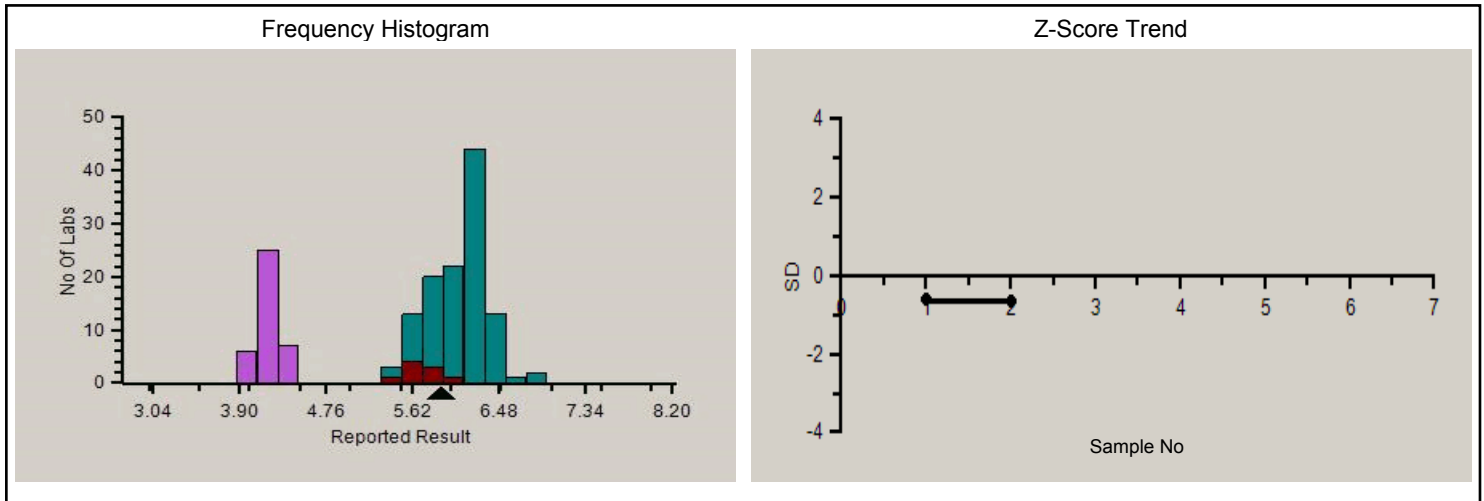

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 2  
 Sample Date : 02-07-2021

Biochemistry, Potassium		N	Mean	SD	CV%	Excluded
	All Analyzer	165	5.62	0.87	15.55	14
<b>Your Analyzer :</b>	<b>EasyLyte</b>	<b>9</b>	<b>5.71</b>	<b>0.18</b>	<b>3.22</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	39	6.21	0.21	3.41	2
	Fuji Dri-Chem NX500/i	38	6.22	0.21	3.41	2
	Fuji Dri-Chem 4000i	17	6.16	0.15	2.50	1
	Roche cobas c 311	16	4.28	0.39	9.02	--
	Roche AVL 9180	13	6.40	0.17	2.63	--
	Bene Sphera C73	9	5.80	0.19	3.19	4
	Bene Sphera C73	9	5.80	0.19	3.19	4

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 2  
Sample Date : 02-07-2021


**Biochemistry, Sodium, mEq/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	164	160.57	21.93	13.66	12
<span style="color: teal;">■</span> ISE direct	118	173.23	5.19	3.00	2
<span style="color: darkred;">■</span> EasyLyte	10	168.89	5.34	3.16	--

<b>Your Result</b>	171.40	<b>SDI / z-Score</b>	-0.47
<b>Assigned Value</b>	173.61	<b>Average SDI</b>	-0.38
<b>SDPA</b>	4.681	<b>Uncertainty of AV</b>	0.55
<b>Standard Unit Result Val</b>	171.40	<b>%DEV</b>	1.49

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

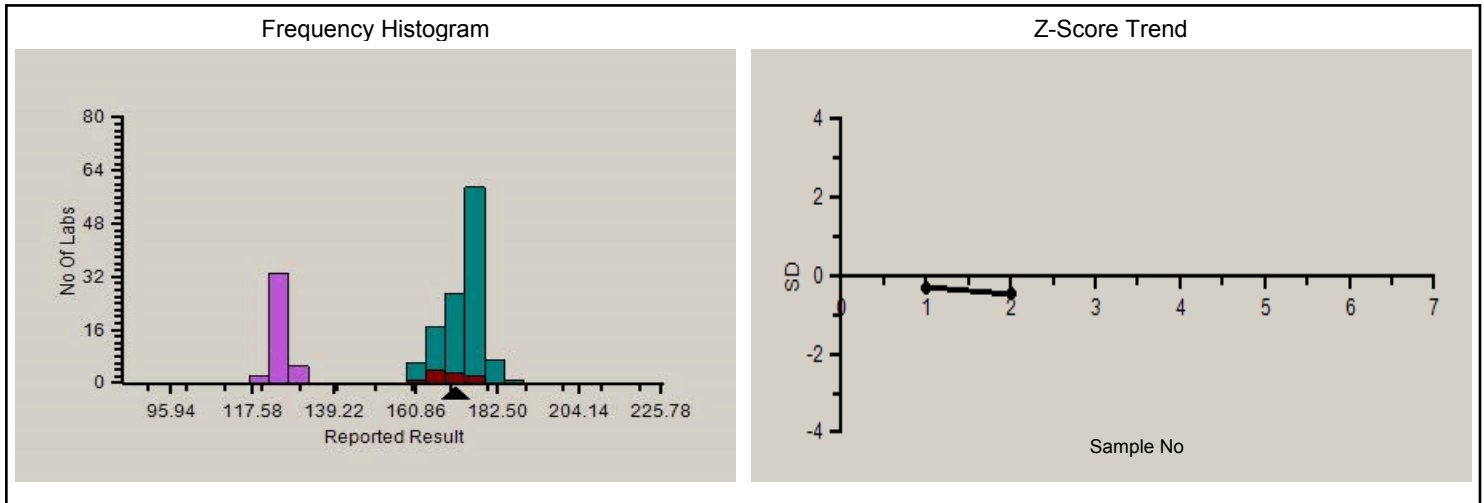

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 2  
 Sample Date : 02-07-2021

Biochemistry, Sodium		N	Mean	SD	CV%	Excluded
	All Analyzer	164	160.57	21.93	13.66	12
<b>Your Analyzer :</b>	<b>EasyLyte</b>	<b>10</b>	<b>168.89</b>	<b>5.34</b>	<b>3.16</b>	--
	Fuji Dri-Chem NX500/i	40	172.68	5.32	3.08	3
	Fuji Dri-Chem NX500/i	39	172.81	5.34	3.09	3
	Fuji Dri-Chem 4000i	16	173.53	2.45	1.41	1
	Roche cobas c 311	16	127.56	13.08	10.25	--
	Roche AVL 9180	13	177.49	2.55	1.44	--
	Bene Sphera C73	9	169.97	2.49	1.46	4
	Bene Sphera C73	9	169.97	2.49	1.46	4

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 2  
Sample Date : 02-07-2021


**Biochemistry, Total Protein, g/dL**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	231	6.42	0.35	5.41	8
<span style="color: teal;">■</span> Biuret	227	6.42	0.34	5.34	8
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	2	6.12	--	--	--

<b>Your Result</b>	6.10	<b>SDI / z-Score</b>	-0.38
<b>Assigned Value</b>	6.28	<b>Average SDI</b>	-0.27
<b>SDPA</b>	0.471	<b>Uncertainty of AV</b>	0.06
<b>Standard Unit Result Val</b>	6.10	<b>%DEV</b>	-5.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

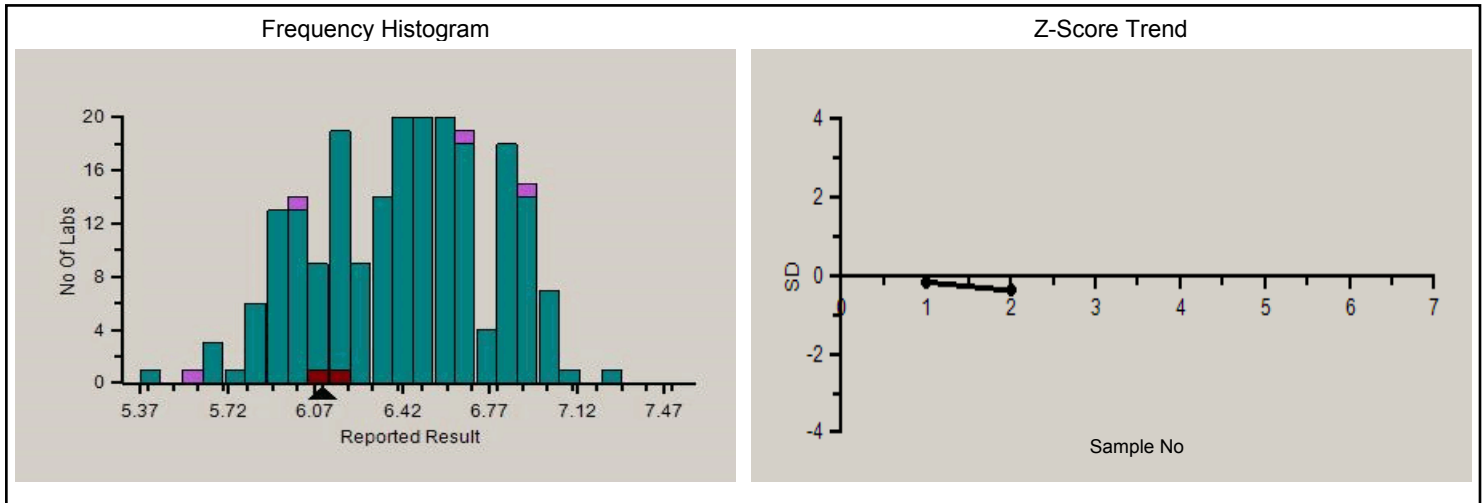

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 2  
 Sample Date : 02-07-2021

Biochemistry, Total Protein		N	Mean	SD	CV%	Excluded
	All Analyzer	231	6.42	0.35	5.41	8
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>2</b>	<b>6.12</b>	--	--	--
	Fuji Dri-Chem NX500/i	37	6.78	0.16	2.33	1
	Fuji Dri-Chem NX500/i	36	6.78	0.16	2.35	1
	Roche cobas c 311	28	6.46	0.17	2.63	--
	Biosystems A15	22	6.41	0.35	5.52	1
	Biosystems A15	22	6.41	0.35	5.52	1
	Erba EM 200	19	6.18	0.38	6.09	2
	Erba EM 200	19	6.18	0.38	6.09	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 2  
Sample Date : 02-07-2021


**Biochemistry, Triglycerides, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	226	141.90	14.92	10.52	5
<span style="color: teal;">■</span> GPO - Peroxidase	18	137.30	13.19	9.61	1
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	138.20	<b>SDI / z-Score</b>	-0.42
<b>Assigned Value</b>	144.78	<b>Average SDI</b>	-0.15
<b>SDPA</b>	15.483	<b>Uncertainty of AV</b>	3.18
<b>Standard Unit Result Val</b>	138.20	<b>%DEV</b>	0.66

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

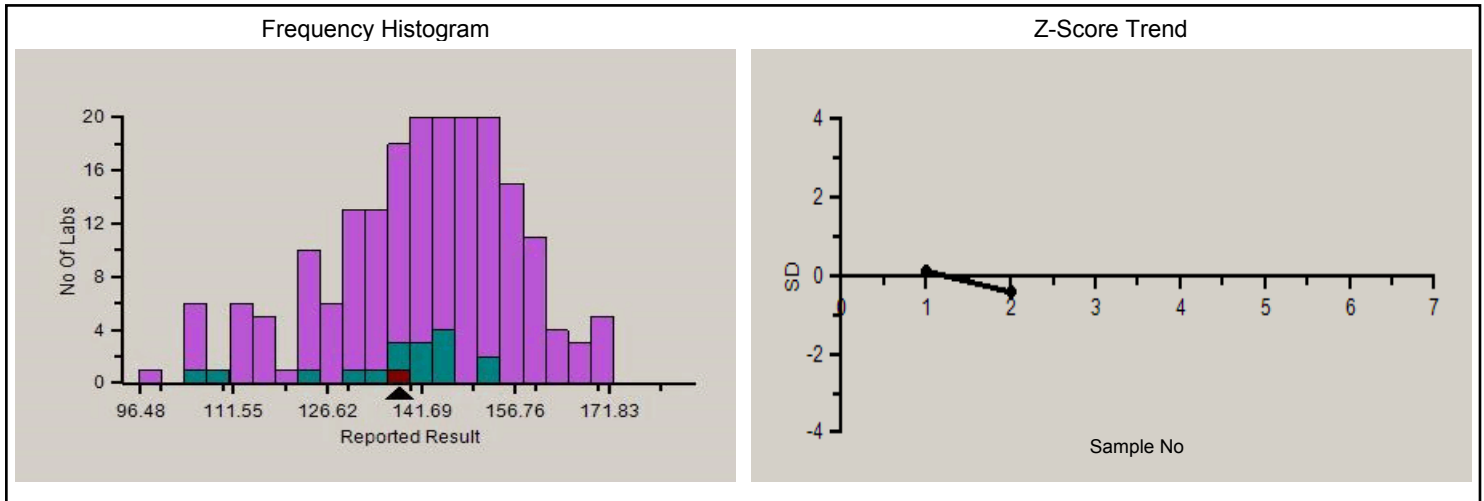

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 2  
 Sample Date : 02-07-2021

<b>Biochemistry, Triglycerides</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	226	141.90	14.92	10.52	5
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	33	138.21	7.89	5.71	--
	Roche cobas c 311	27	150.89	8.57	5.68	--
	Biosystems A15	22	117.71	14.07	11.95	--
	Biosystems A15	22	117.71	14.07	11.95	--
	ERBA XL-640	17	146.13	14.22	9.73	--
	Erba EM 200	15	142.21	12.64	8.89	1
	Erba EM 200	15	142.21	12.64	8.89	1
	Fuji Dri-Chem 4000i	15	135.47	9.25	6.83	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 2  
Sample Date : 02-07-2021


**Biochemistry, Uric Acid, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	229	4.29	0.38	8.75	11
<span style="color: teal;">■</span> Uricase	38	4.31	0.35	8.17	2
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	4.23	<b>SDI / z-Score</b>	-0.86
<b>Assigned Value</b>	4.63	<b>Average SDI</b>	-0.82
<b>SDPA</b>	0.463	<b>Uncertainty of AV</b>	0.07
<b>Standard Unit Result Val</b>	4.23	<b>%DEV</b>	-1.79

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

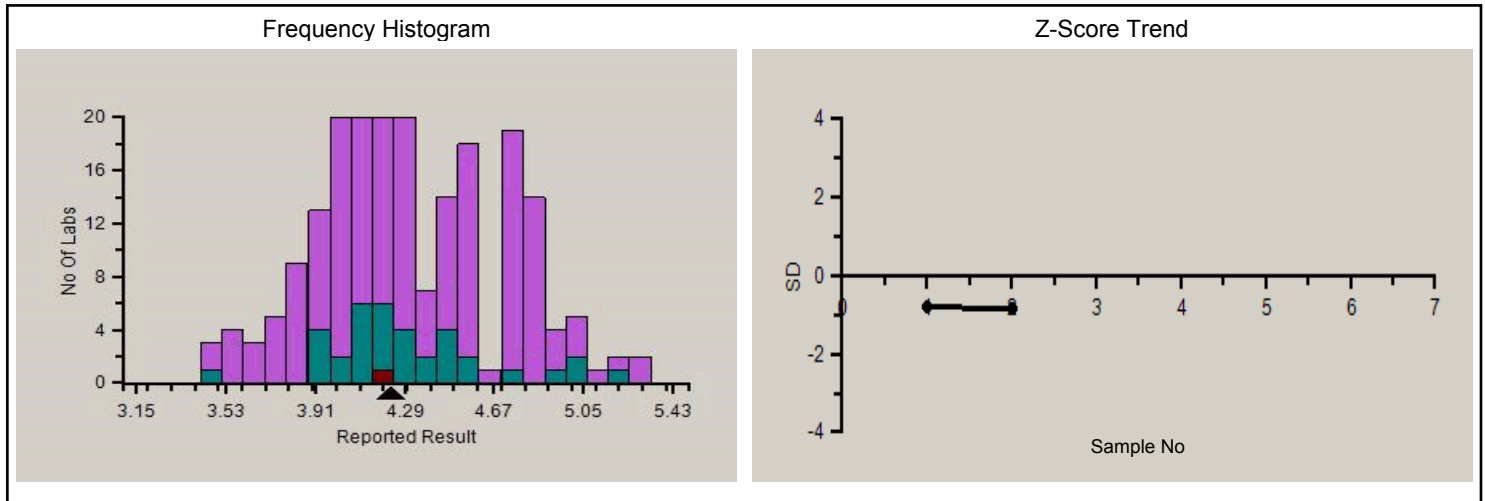

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 2  
Sample Date : 02-07-2021

Biochemistry, Uric Acid		N	Mean	SD	CV%	Excluded
	All Analyzer	229	4.29	0.38	8.75	11
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	35	4.62	0.21	4.59	--
	Fuji Dri-Chem NX500/i	34	4.61	0.21	4.57	--
	Roche cobas c 311	26	4.05	0.21	5.26	--
	Biosystems A15	21	3.91	0.30	7.55	6
	Biosystems A15	21	3.91	0.30	7.55	6
	Erba EM 200	18	4.56	0.34	7.35	1
	Erba EM 200	18	4.56	0.34	7.35	1
	ERBA XL-640	18	4.80	0.27	5.71	--

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.

*Dr Puneet Kumar Nigam*

**Dr Puneet Kumar Nigam**  
**PT coordinator & Technical Manager, MHL EQAS**  
Unit No. 409-416.  
Commercial Building - 1A,  
Kohinoor Mall, Kirool Road, Kuria (W),  
Mumbai - 400070



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 3  
 Sample Date : 02-07-2021


**Biochemistry, Cholesterol, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	229	154.49	8.48	5.49	16
CHOD-PAP	46	156.55	7.83	5.00	7
Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	146.00	<b>SDI / z-Score</b>	-0.99
<b>Assigned Value</b>	156.76	<b>Average SDI</b>	-1.05
<b>SDPA</b>	10.900	<b>Uncertainty of AV</b>	1.55
<b>Standard Unit Result Val</b>	146.00	<b>%DEV</b>	-6.74

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

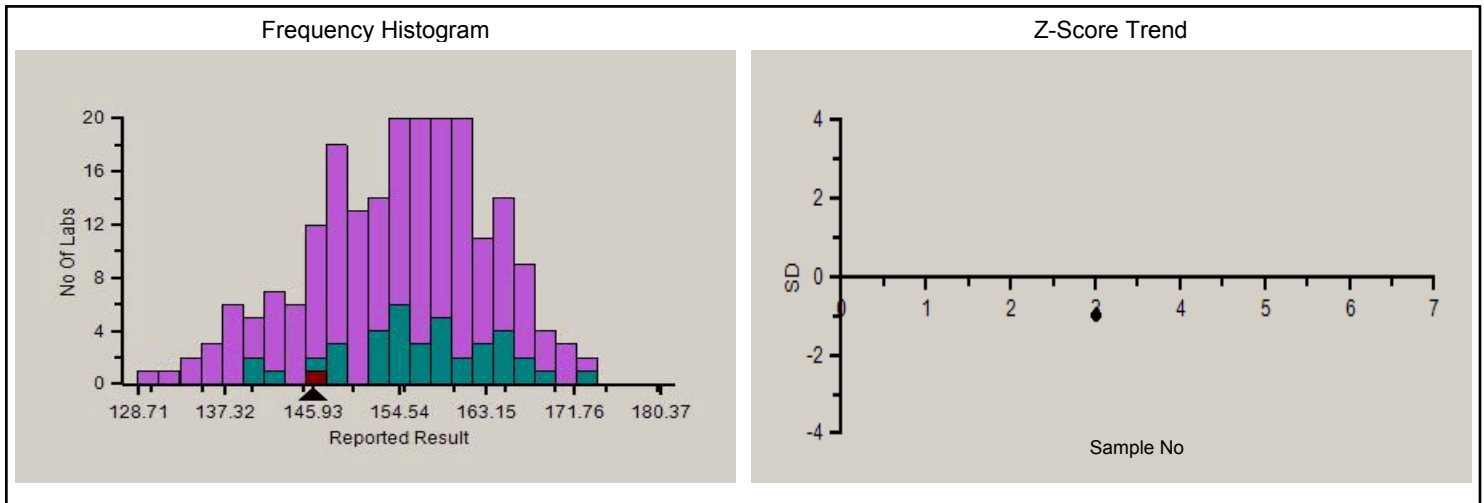

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 3  
 Sample Date : 02-07-2021

<b>Biochemistry, Cholesterol</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	229	154.49	8.48	5.49	16
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	34	146.06	8.39	5.75	3
	Fuji Dri-Chem NX500/i	33	146.04	8.54	5.85	3
	Roche cobas c 311	29	157.26	4.87	3.09	--
	Biosystems A15	23	155.63	9.66	6.21	3
	Biosystems A15	22	155.40	9.87	6.35	3
	Biosystems A15	21	154.85	9.85	6.36	3
	Biosystems A15	21	154.85	9.85	6.36	3
	Erba EM 200	17	156.63	6.11	3.90	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.





**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 3  
Sample Date : 02-07-2021


**Biochemistry, Creatinine, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	237	0.73	0.22	30.77	21
<span style="color: teal;">■</span> Enzymatic	30	0.87	0.19	22.31	4
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	1

<b>Your Result</b>	0.57	<b>SDI / z-Score</b>	-2.04
<b>Assigned Value</b>	0.91	<b>Average SDI</b>	-1.79
<b>SDPA</b>	0.168	<b>Uncertainty of AV</b>	0.04
<b>Standard Unit Result Val</b>	0.57	<b>%DEV</b>	-34.10

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

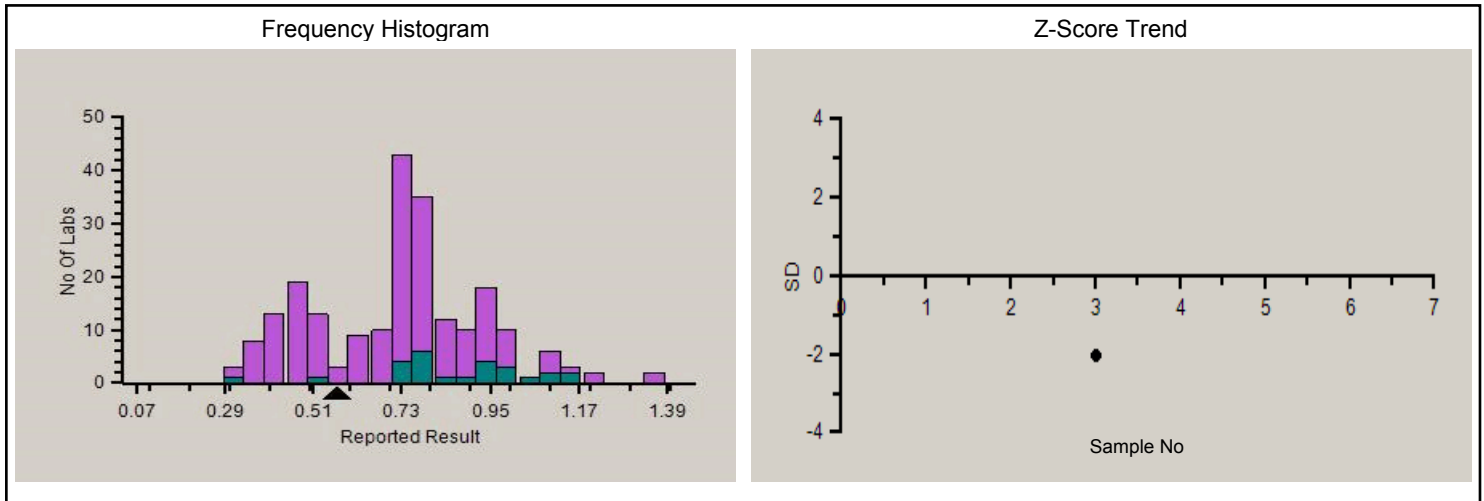

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 3  
 Sample Date : 02-07-2021

Biochemistry, Creatinine		N	Mean	SD	CV%	Excluded
	All Analyzer	237	0.73	0.22	30.77	21
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	36	0.44	0.05	12.41	--
	Fuji Dri-Chem NX500/i	35	0.44	0.06	12.64	--
	Roche cobas c 311	29	0.74	0.05	6.48	--
	Biosystems A15	24	0.74	0.14	19.43	5
	Biosystems A15	23	0.74	0.15	19.70	5
	Biosystems A15	22	0.76	0.13	17.31	5
	Biosystems A15	22	0.76	0.13	17.31	5
	Erba EM 200	18	0.84	0.14	16.73	4

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 3  
Sample Date : 02-07-2021


**Biochemistry, Glucose, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	236	62.24	4.02	6.45	11
<span style="color: teal;">■</span> GOD POD reflectometric analysis	23	61.50	4.76	7.74	2
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	2	65.60	--	--	--

<b>Your Result</b>	67.20	<b>SDI / z-Score</b>	0.24
<b>Assigned Value</b>	65.79	<b>Average SDI</b>	0.11
<b>SDPA</b>	5.920	<b>Uncertainty of AV</b>	1.00
<b>Standard Unit Result Val</b>	67.20	<b>%DEV</b>	9.26

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

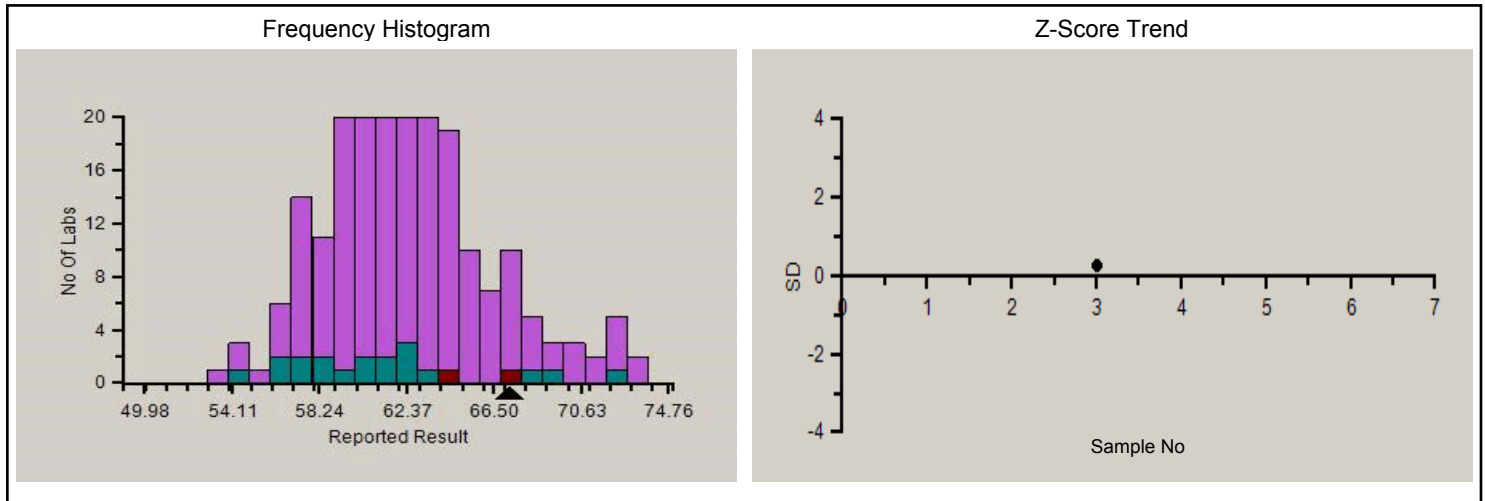

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 3  
 Sample Date : 02-07-2021

Biochemistry, Glucose		N	Mean	SD	CV%	Excluded
	All Analyzer	236	62.24	4.02	6.45	11
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>2</b>	<b>65.60</b>	--	--	--
	Fuji Dri-Chem NX500/i	36	58.99	2.45	4.15	1
	Fuji Dri-Chem NX500/i	35	59.01	2.48	4.20	1
	Roche cobas c 311	29	62.21	2.30	3.70	--
	Biosystems A15	24	62.52	5.07	8.10	1
	Biosystems A15	23	62.18	4.91	7.90	1
	Biosystems A15	22	61.97	4.93	7.95	1
	Biosystems A15	22	61.97	4.93	7.95	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 3  
Sample Date : 02-07-2021


**Biochemistry, HDL, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	219	35.60	4.26	11.98	5
Direct measure-PEG	57	35.63	4.97	13.96	1
Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	34.90	<b>SDI / z-Score</b>	0.09
<b>Assigned Value</b>	34.50	<b>Average SDI</b>	0.11
<b>SDPA</b>	4.480	<b>Uncertainty of AV</b>	0.48
<b>Standard Unit Result Val</b>	34.90	<b>%DEV</b>	-2.06

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

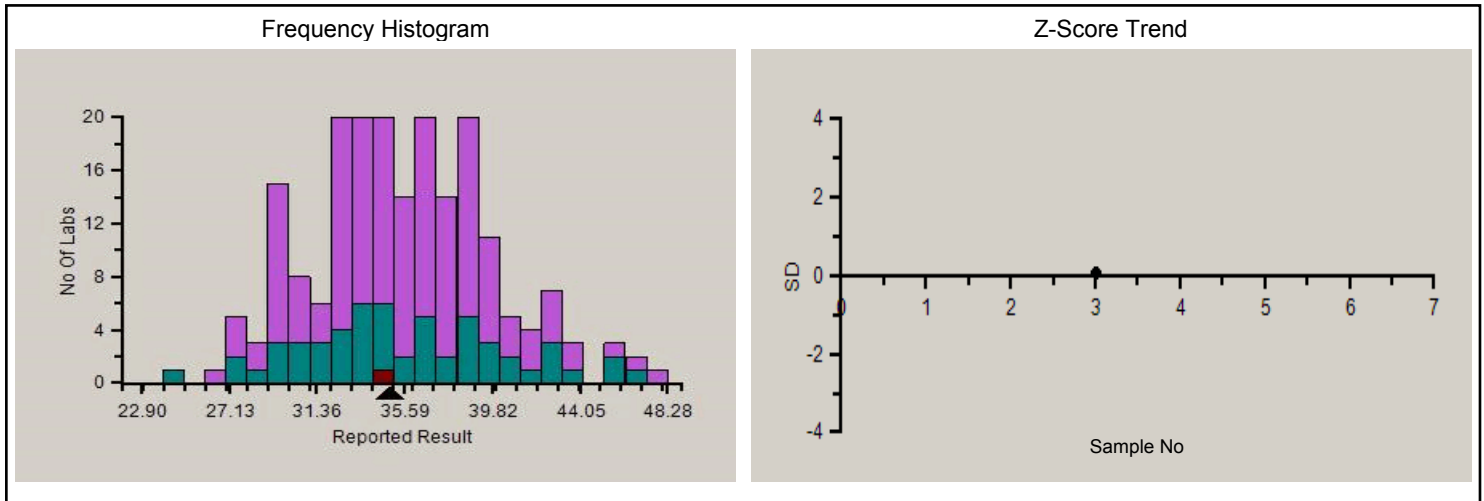

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 3  
 Sample Date : 02-07-2021

Biochemistry, HDL		N	Mean	SD	CV%	Excluded
	All Analyzer	219	35.60	4.26	11.98	5
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	32	36.47	2.16	5.91	--
	Fuji Dri-Chem NX500/i	31	36.50	2.19	5.99	--
	Roche cobas c 311	29	32.77	2.46	7.50	1
	Biosystems A15	23	36.22	4.49	12.41	2
	Biosystems A15	22	36.03	4.52	12.55	2
	Biosystems A15	21	36.22	4.56	12.60	2
	Biosystems A15	21	36.22	4.56	12.60	2
	Erba EM 200	17	36.52	5.88	16.10	1

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 3  
Sample Date : 02-07-2021


**Biochemistry, Phosphorous Inorganic, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	133	3.75	0.22	5.81	4
<span style="color: teal;">■</span> UV Molybdate colorimetric	16	3.89	0.29	7.33	2
<span style="color: darkred;">■</span> Erba Chem 5/Plus	2	3.89	--	--	--

<b>Your Result</b>	4.30	<b>SDI / z-Score</b>	1.61
<b>Assigned Value</b>	3.80	<b>Average SDI</b>	1.23
<b>SDPA</b>	0.310	<b>Uncertainty of AV</b>	0.07
<b>Standard Unit Result Val</b>	4.30	<b>%DEV</b>	10.54

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

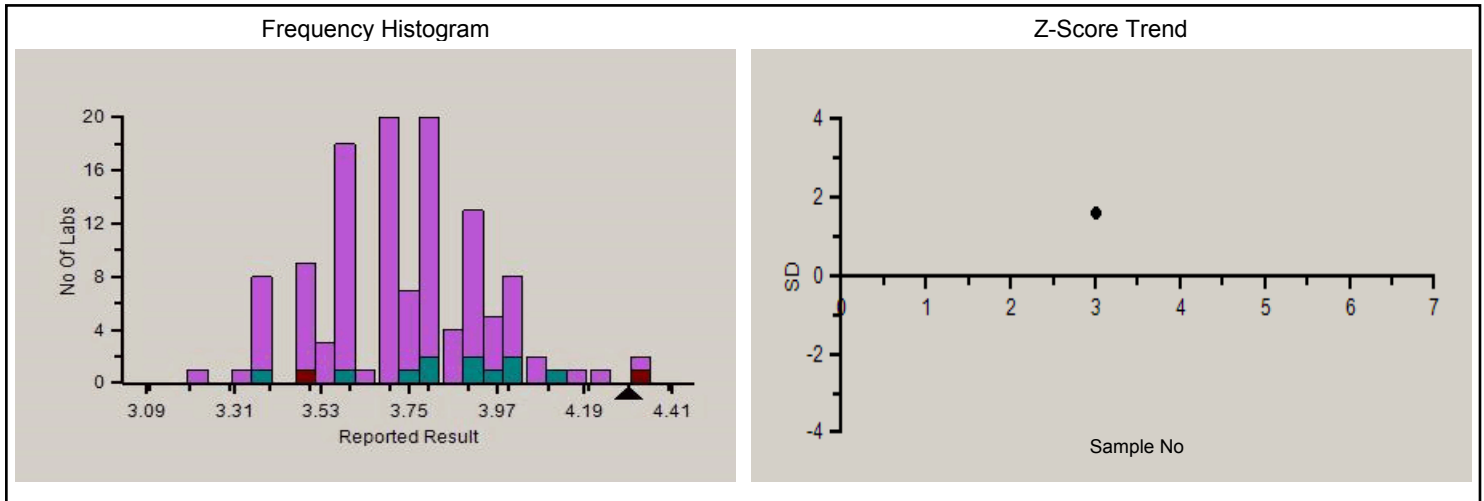

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 3  
 Sample Date : 02-07-2021

Biochemistry, Phosphorous Inorganic		N	Mean	SD	CV%	Excluded
	All Analyzer	133	3.75	0.22	5.81	4
<b>Your Analyzer :</b>	<b>Erba Chem 5/Plus</b>	<b>2</b>	<b>3.89</b>	--	--	--
	Fuji Dri-Chem NX500/i	29	3.70	0.18	4.79	--
	Fuji Dri-Chem NX500/i	28	3.69	0.18	4.85	--
	Roche cobas c 311	24	3.75	0.16	4.29	1
	Fuji Dri-Chem 4000i	14	3.64	0.19	5.25	--
	Roche cobas INTEGRA	9	3.81	0.11	2.84	--
	Roche cobas 6000	8	3.69	0.17	4.47	--
	Horiba ABX Pentra C200	6	4.01	0.30	7.41	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.

*Dr Puneet Kumar Nigam*

**Dr Puneet Kumar Nigam**  
**PT coordinator & Technical Manager, MHL EQAS**  
 Unit No. 409-416.  
 Commercial Building - 1A,  
 Kohinoor Mall, Kirool Road, Kuria (W),  
 Mumbai - 400070



PC-1022



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 5  
Sample Date : 02-07-2021


**Biochemistry, ALP, U/L**

	N	Mean	SD	CV%	Excluded
All Methods	208	204.82	26.56	12.97	18
IFCC	21	201.47	27.09	13.45	1
Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	196.00	<b>SDI / z-Score</b>	-0.19
<b>Assigned Value</b>	200.76	<b>Average SDI</b>	-0.20
<b>SDPA</b>	24.621	<b>Uncertainty of AV</b>	3.19
<b>Standard Unit Result Val</b>	196.00	<b>%DEV</b>	-2.72

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

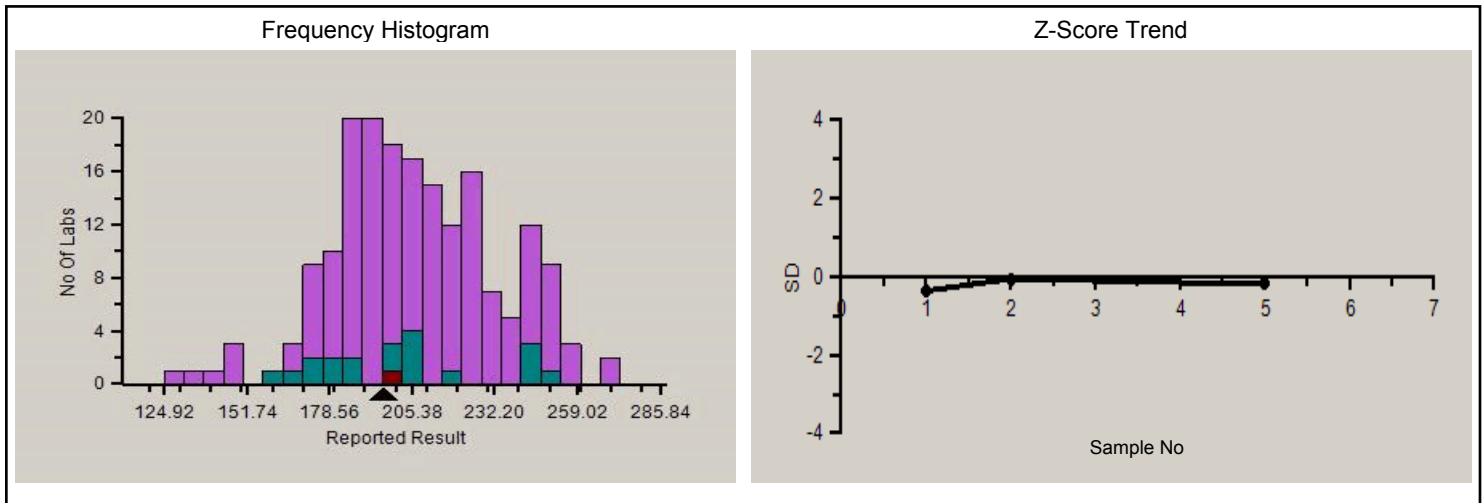

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 5  
 Sample Date : 02-07-2021

<b>Biochemistry, ALP</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	208	204.82	26.56	12.97	18
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	35	213.25	18.76	8.80	3
	Fuji Dri-Chem NX500/i	34	213.81	18.79	8.79	3
	Roche cobas c 311	28	185.68	12.21	6.58	--
	Biosystems A15	23	221.16	23.15	10.47	3
	Biosystems A15	22	220.78	23.76	10.76	3
	Biosystems A15	22	220.78	23.76	10.76	3
	ERBA XL-640	17	230.91	15.31	6.63	5
	ERBA XL-640	17	230.91	15.31	6.63	5

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 5  
Sample Date : 02-07-2021


**Biochemistry, ALT, U/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	210	45.56	4.70	10.31	11
<span style="color: teal;">■</span> IFCC	30	46.02	4.07	8.84	2
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	52.60	<b>SDI / z-Score</b>	1.86
<b>Assigned Value</b>	45.39	<b>Average SDI</b>	-0.12
<b>SDPA</b>	3.879	<b>Uncertainty of AV</b>	0.86
<b>Standard Unit Result Val</b>	52.60	<b>%DEV</b>	14.29

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

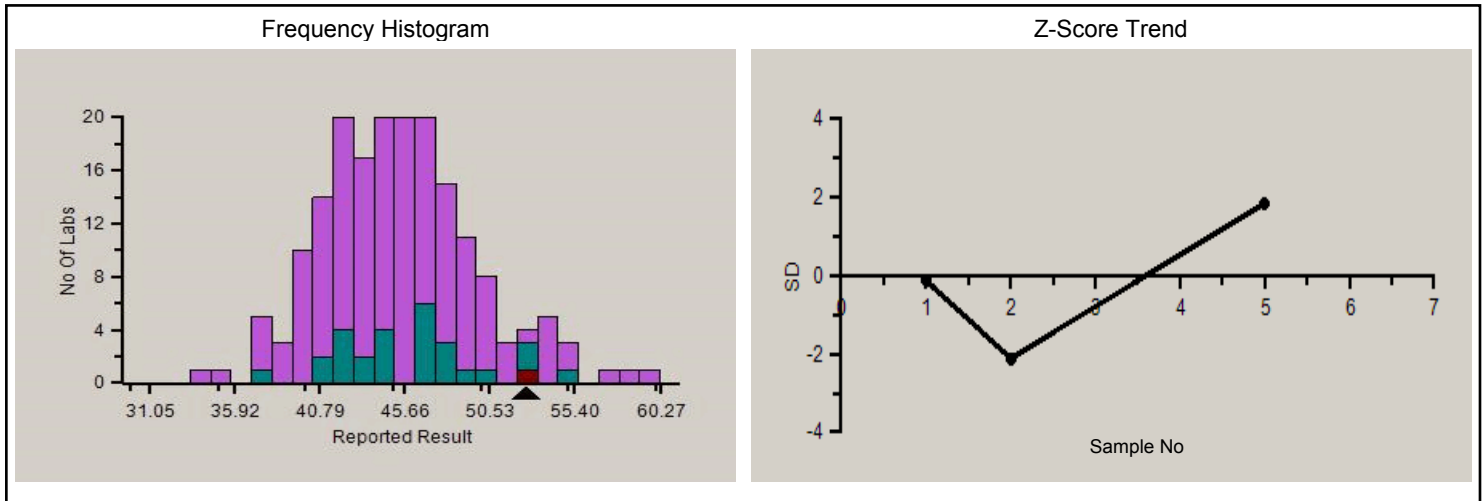

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 5  
 Sample Date : 02-07-2021

Biochemistry, ALT		N	Mean	SD	CV%	Excluded
	All Analyzer	210	45.56	4.70	10.31	11
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	34	45.97	3.46	7.53	2
	Fuji Dri-Chem NX500/i	33	45.97	3.52	7.65	2
	Roche cobas c 311	28	43.19	2.57	5.94	--
	Biosystems A15	23	52.10	6.51	12.49	1
	Biosystems A15	22	52.43	6.47	12.34	1
	Biosystems A15	22	52.43	6.47	12.34	1
	ERBA XL-640	18	46.08	3.48	7.56	--
	Fuji Dri-Chem 4000i	14	46.29	2.09	4.52	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 5  
Sample Date : 02-07-2021


**Biochemistry, Amylase, U/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	126	190.77	17.28	9.06	12
<span style="color: teal;">■</span> Direct Substrate	6	202.48	22.30	11.01	--
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	207.60	<b>SDI / z-Score</b>	0.31
<b>Assigned Value</b>	199.50	<b>Average SDI</b>	4.24
<b>SDPA</b>	25.930	<b>Uncertainty of AV</b>	3.71
<b>Standard Unit Result Val</b>	207.60	<b>%DEV</b>	2.53

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

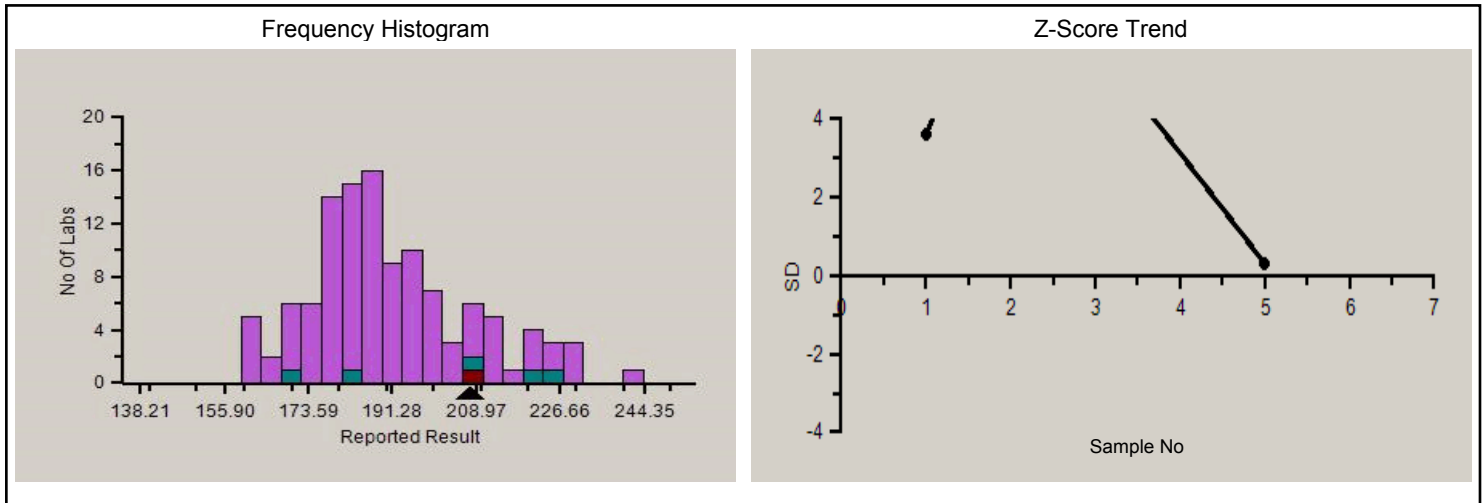

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 5  
 Sample Date : 02-07-2021

Biochemistry, Amylase		N	Mean	SD	CV%	Excluded
	All Analyzer	126	190.77	17.28	9.06	12
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	23	192.24	13.45	7.00	2
	ERBA XL-640	15	195.00	10.38	5.32	--
	ERBA XL-640	15	195.00	10.38	5.32	--
	Fuji Dri-Chem 4000i	15	187.21	13.17	7.03	1
	Roche cobas c 311	14	175.17	7.76	4.43	--
	Biosystems A15	13	215.33	23.41	10.87	--
	Biosystems A15	12	214.00	24.07	11.25	--
	Biosystems A15	12	214.00	24.07	11.25	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 5  
Sample Date : 02-07-2021


**Biochemistry, AST, U/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	209	95.94	8.63	8.99	8
<span style="color: teal;">■</span> IFCC	28	97.29	6.43	6.61	2
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	95.70	<b>SDI / z-Score</b>	-0.12
<b>Assigned Value</b>	96.54	<b>Average SDI</b>	-0.79
<b>SDPA</b>	6.962	<b>Uncertainty of AV</b>	1.51
<b>Standard Unit Result Val</b>	95.70	<b>%DEV</b>	-1.64

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

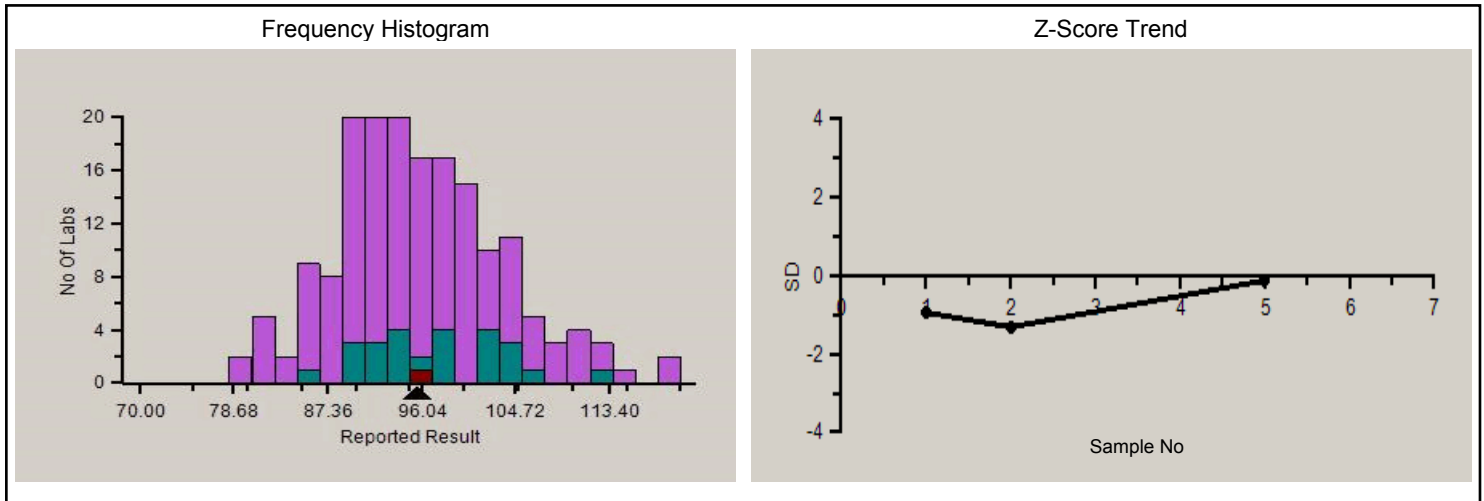

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 5  
 Sample Date : 02-07-2021

Biochemistry, AST		N	Mean	SD	CV%	Excluded
	All Analyzer	209	95.94	8.63	8.99	8
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	36	93.49	5.47	5.85	3
	Fuji Dri-Chem NX500/i	35	93.59	5.52	5.90	3
	Roche cobas c 311	27	92.56	4.43	4.78	--
	Biosystems A15	22	109.37	7.81	7.14	1
	Biosystems A15	21	109.34	8.02	7.34	1
	Biosystems A15	21	109.34	8.02	7.34	1
	ERBA XL-640	18	98.61	6.78	6.88	--
	Roche cobas c 111	15	88.68	5.32	6.00	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.





**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 5  
Sample Date : 02-07-2021


**Biochemistry, Bilirubin Direct, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	205	0.78	0.22	28.04	33
<span style="color: teal;">■</span> Jendrassik Grof	3	0.30	0.00	0.00	2
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	0.30	<b>SDI / z-Score</b>	-1.07
<b>Assigned Value</b>	0.41	<b>Average SDI</b>	-1.88
<b>SDPA</b>	0.102	<b>Uncertainty of AV</b>	0.01
<b>Standard Unit Result Val</b>	0.30	<b>%DEV</b>	0.00

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

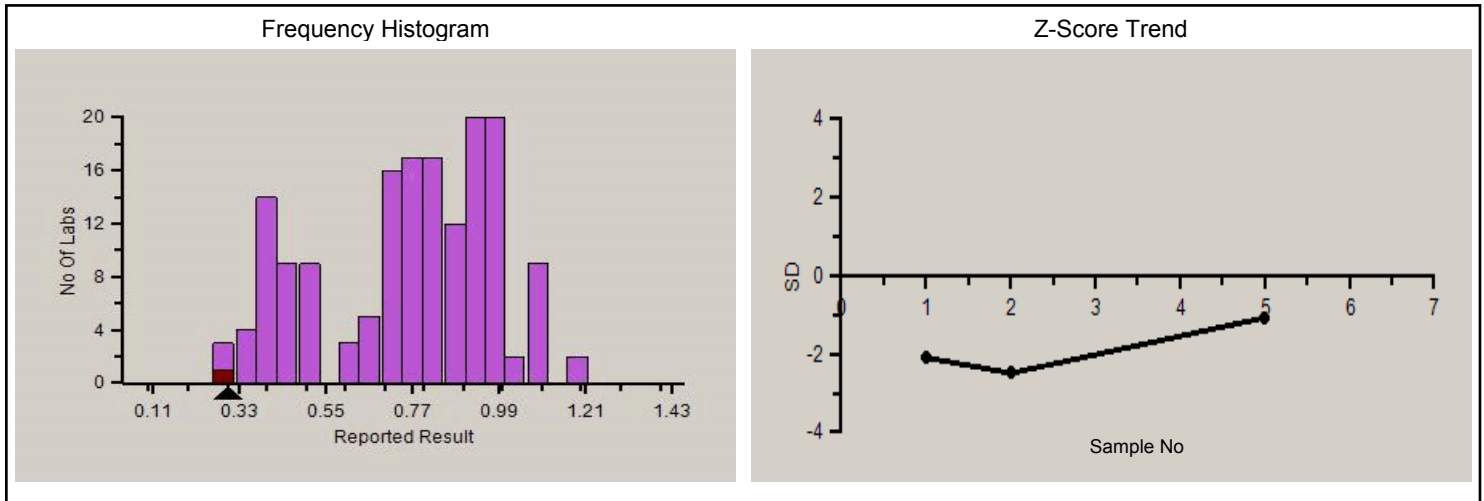

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 5  
 Sample Date : 02-07-2021

<b>Biochemistry, Bilirubin Direct</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	205	0.78	0.22	28.04	33
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	35	0.97	0.11	11.02	3
	Fuji Dri-Chem NX500/i	34	0.97	0.11	11.25	3
	Roche cobas c 311	27	0.85	0.10	12.22	1
	Biosystems A15	22	0.59	0.14	24.27	9
	Biosystems A15	21	0.61	0.13	21.32	9
	Biosystems A15	21	0.61	0.13	21.32	9
	ERBA XL-640	17	0.42	0.06	13.22	--
	Erba EM 200	14	0.39	0.06	15.42	4

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 5  
Sample Date : 02-07-2021


**Biochemistry, Bilirubin Total, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	205	2.12	0.20	9.51	15
<span style="color: teal;">■</span> Jendrassik Grof	7	2.18	0.11	5.10	2
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	2.20	<b>SDI / z-Score</b>	-0.05
<b>Assigned Value</b>	2.21	<b>Average SDI</b>	-0.84
<b>SDPA</b>	0.309	<b>Uncertainty of AV</b>	0.03
<b>Standard Unit Result Val</b>	2.20	<b>%DEV</b>	1.10

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

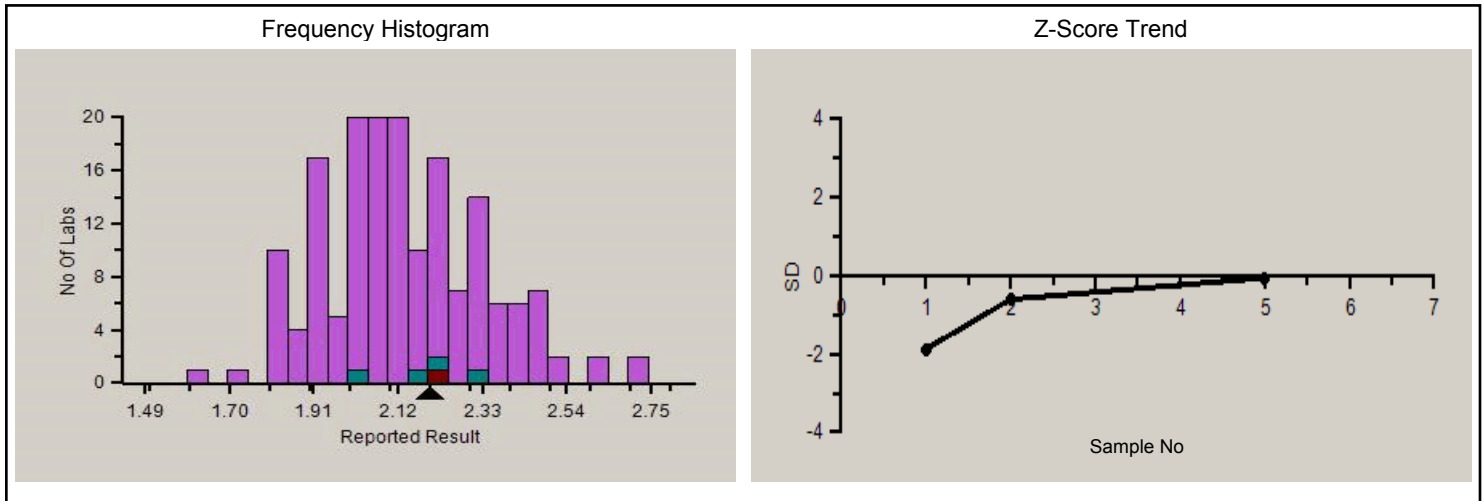

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 5  
 Sample Date : 02-07-2021

<b>Biochemistry, Bilirubin Total</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	205	2.12	0.20	9.51	15
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	35	2.04	0.13	6.43	4
	Fuji Dri-Chem NX500/i	34	2.04	0.13	6.52	4
	Roche cobas c 311	28	2.03	0.10	5.12	--
	Biosystems A15	18	2.04	0.33	16.38	2
	ERBA XL-640	18	2.25	0.16	6.97	1
	Biosystems A15	17	2.09	0.28	13.36	2
	Biosystems A15	17	2.09	0.28	13.36	2
	Erba EM 200	14	2.15	0.19	8.69	3

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 5  
Sample Date : 02-07-2021


**Biochemistry, Creatinine, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	210	2.73	0.26	9.41	10
<span style="color: teal;">■</span> Enzymatic	23	2.91	0.28	9.58	3
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	2.49	<b>SDI / z-Score</b>	-1.10
<b>Assigned Value</b>	2.90	<b>Average SDI</b>	-1.79
<b>SDPA</b>	0.377	<b>Uncertainty of AV</b>	0.06
<b>Standard Unit Result Val</b>	2.49	<b>%DEV</b>	-14.52

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

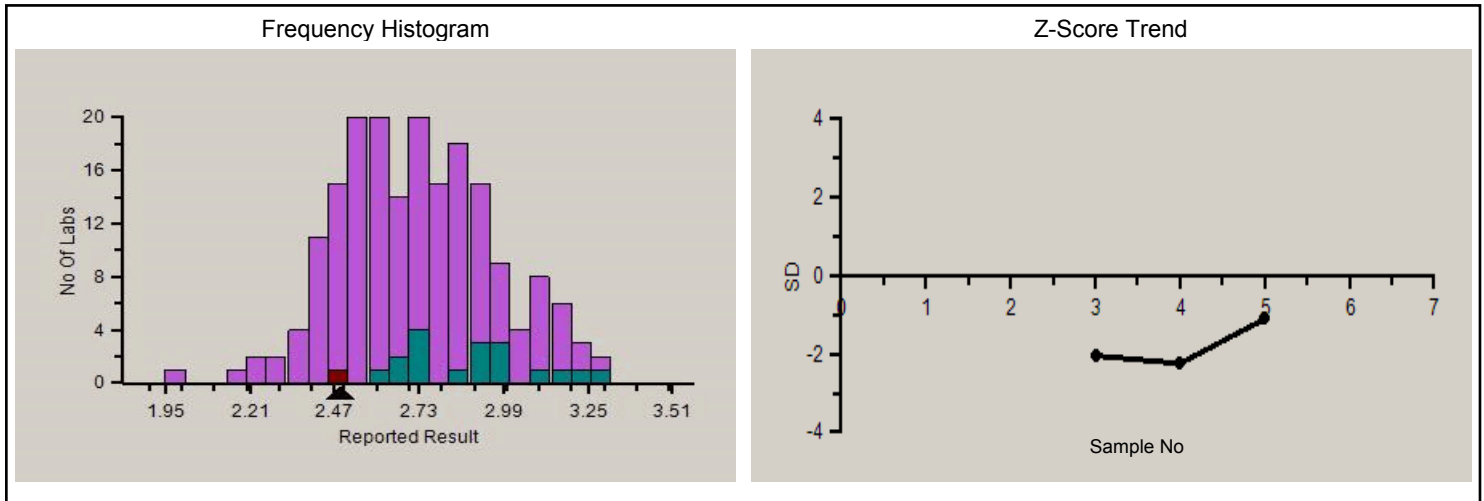

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 5  
 Sample Date : 02-07-2021

<b>Biochemistry, Creatinine</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	210	2.73	0.26	9.41	10
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	34	2.54	0.14	5.55	1
	Fuji Dri-Chem NX500/i	33	2.54	0.14	5.62	1
	Roche cobas c 311	28	2.75	0.14	5.24	--
	Biosystems A15	23	2.82	0.40	14.09	2
	Biosystems A15	22	2.84	0.40	13.91	2
	Biosystems A15	22	2.84	0.40	13.91	2
	ERBA XL-640	18	3.03	0.25	8.16	1
	Fuji Dri-Chem 4000i	15	2.55	0.14	5.54	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 5  
Sample Date : 02-07-2021


**Biochemistry, Glucose, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	210	136.86	8.58	6.27	12
GOD POD reflectometric analysis	20	137.32	9.42	6.86	3
Erba EM Destiny 180/XL-180	2	146.20	--	--	--

<b>Your Result</b>	146.00	<b>SDI / z-Score</b>	0.16
<b>Assigned Value</b>	143.26	<b>Average SDI</b>	0.11
<b>SDPA</b>	17.190	<b>Uncertainty of AV</b>	1.92
<b>Standard Unit Result Val</b>	146.00	<b>%DEV</b>	6.32

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

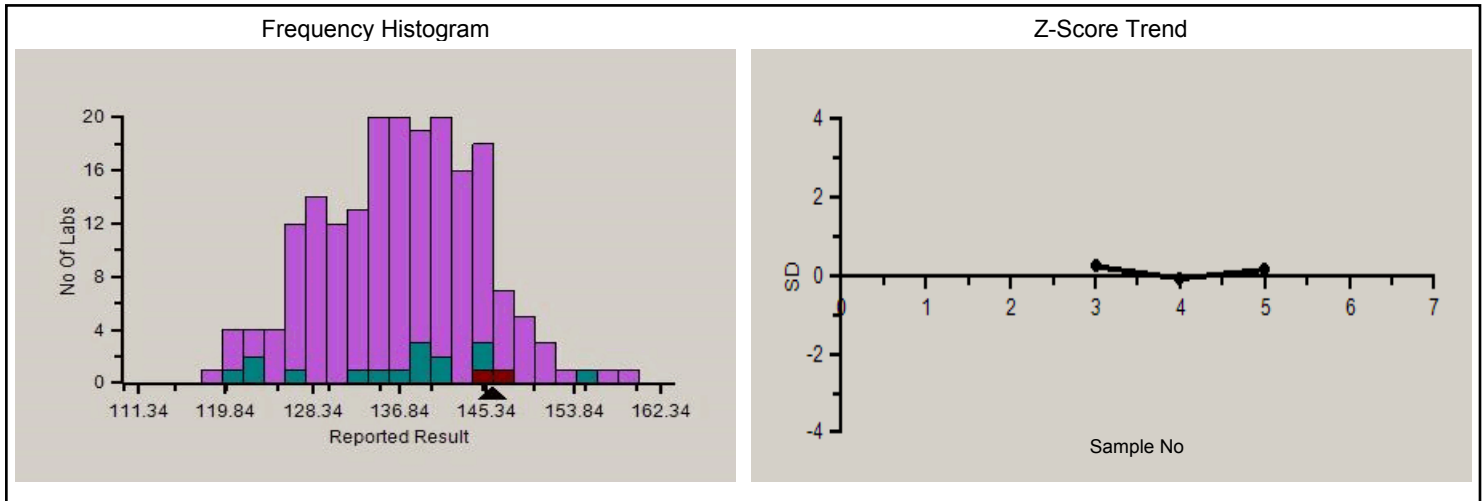

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 5  
 Sample Date : 02-07-2021

Biochemistry, Glucose		N	Mean	SD	CV%	Excluded
	All Analyzer	210	136.86	8.58	6.27	12
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>2</b>	<b>146.20</b>	--	--	--
	Fuji Dri-Chem NX500/i	35	134.87	9.42	6.98	2
	Fuji Dri-Chem NX500/i	34	134.88	9.57	7.09	2
	Roche cobas c 311	28	136.26	4.97	3.64	--
	Biosystems A15	23	131.44	9.69	7.37	1
	Biosystems A15	22	131.26	9.91	7.55	1
	Biosystems A15	22	131.26	9.91	7.55	1
	ERBA XL-640	18	144.67	10.97	7.59	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 5  
Sample Date : 02-07-2021


**Biochemistry, LDH, U/L**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	96	202.38	67.87	33.54	11
<span style="color: teal;">■</span> Kinetic UV optimized DGKC	5	295.28	126.65	42.89	1
<span style="color: darkred;">■</span> Erba Chem 5/Plus	1	--	--	--	--

<b>Your Result</b>	372.20	<b>SDI / z-Score</b>	-1.59
<b>Assigned Value</b>	442.50	<b>Average SDI</b>	-1.68
<b>SDPA</b>	44.250	<b>Uncertainty of AV</b>	17.31
<b>Standard Unit Result Val</b>	372.20	<b>%DEV</b>	26.05

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

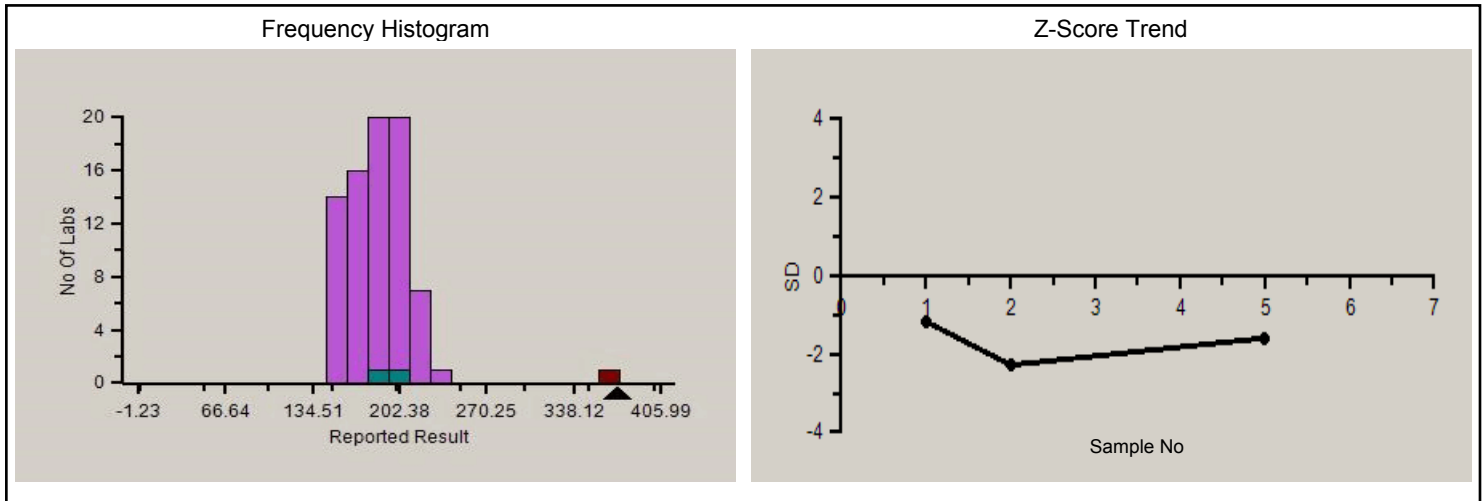

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 5  
 Sample Date : 02-07-2021

Biochemistry, LDH		N	Mean	SD	CV%	Excluded
	All Analyzer	96	202.38	67.87	33.54	11
<b>Your Analyzer :</b>	<b>Erba Chem 5/Plus</b>	1	--	--	--	--
	Fuji Dri-Chem NX500/i	25	164.33	11.29	6.87	4
	Roche cobas c 311	17	198.06	7.99	4.03	1
	Fuji Dri-Chem 4000i	9	167.11	13.13	7.86	--
	Roche cobas INTEGRA	8	202.08	11.64	5.76	--
	Roche cobas 6000	6	203.93	11.41	5.59	--
	Beckman Coulter AU480	4	183.05	7.91	4.32	--
	Horiba ABX Pentra C200	4	206.33	27.68	13.42	1
	Roche cobas 8000	4	203.25	7.59	3.73	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 5  
 Sample Date : 02-07-2021


**Biochemistry, Magnesium, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	50	2.08	0.16	7.84	2
<span style="color: teal;">■</span> Calmagite	2	2.24	--	--	--
<span style="color: darkred;">■</span> Erba Chem 5/Plus	1	--	--	--	--

<b>Your Result</b>	2.20	<b>SDI / z-Score</b>	0.15
<b>Assigned Value</b>	2.16	<b>Average SDI</b>	0.87
<b>SDPA</b>	0.259	<b>Uncertainty of AV</b>	0.03
<b>Standard Unit Result Val</b>	2.20	<b>%DEV</b>	-1.57

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

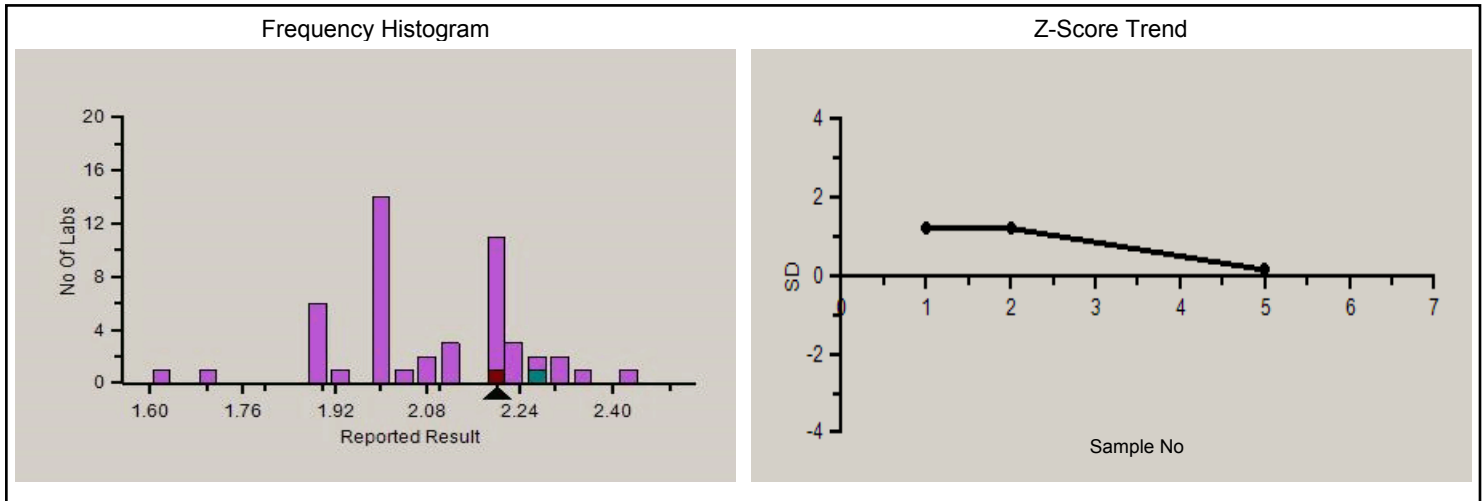

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 5  
 Sample Date : 02-07-2021

<b>Biochemistry, Magnesium</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	50	2.08	0.16	7.84	2
<b>Your Analyzer :</b>	<b>Erba Chem 5/Plus</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	17	2.04	0.21	10.51	--
	Fuji Dri-Chem NX500/i	16	2.04	0.22	10.84	--
	Fuji Dri-Chem 4000i	10	2.01	0.09	4.38	--
	Roche cobas c 311	7	2.16	0.10	4.59	1
	Roche cobas 6000	6	2.13	0.12	5.73	--
	Roche cobas 8000	4	2.17	0.20	8.99	--
	Roche cobas INTEGRA	2	2.16	--	--	--
	Fuji Nx 700	2	2.00	--	--	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 5  
Sample Date : 02-07-2021


**Biochemistry, Phosphorous Inorganic, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	120	3.96	0.42	10.51	4
UV Molybdate colorimetric	12	3.83	0.17	4.52	1
Erba Chem 5/Plus	2	3.95	--	--	--

<b>Your Result</b>	4.10	<b>SDI / z-Score</b>	0.96
<b>Assigned Value</b>	3.75	<b>Average SDI</b>	1.23
<b>SDPA</b>	0.366	<b>Uncertainty of AV</b>	0.10
<b>Standard Unit Result Val</b>	4.10	<b>%DEV</b>	7.11

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

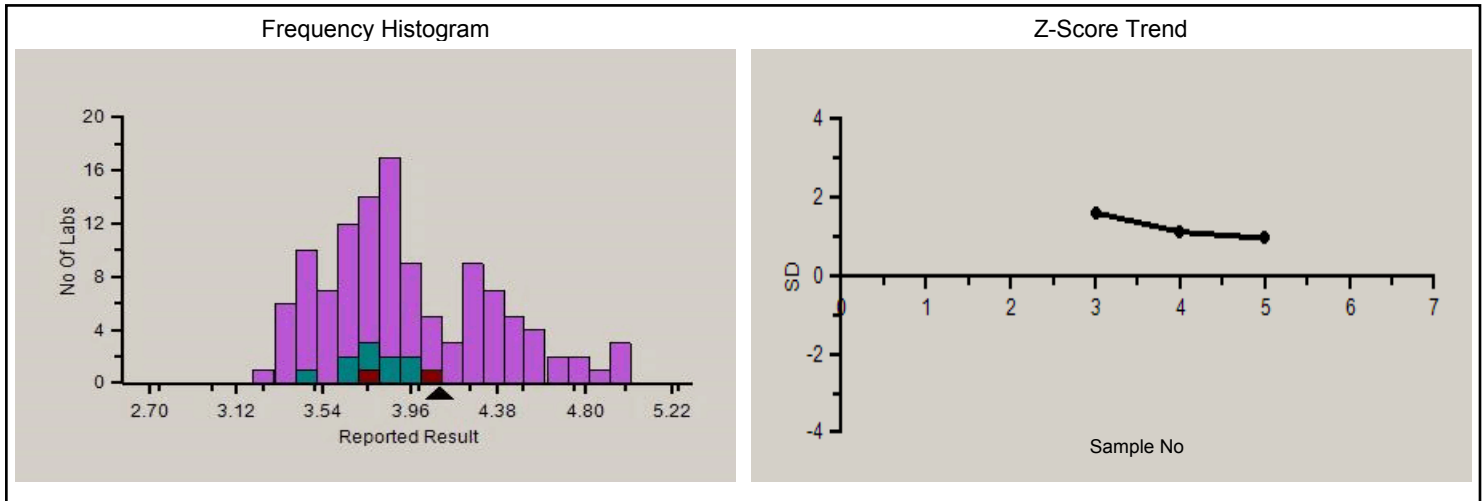

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 5  
 Sample Date : 02-07-2021

<b>Biochemistry, Phosphorous Inorganic</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	120	3.96	0.42	10.51	4
<b>Your Analyzer :</b>	<b>Erba Chem 5/Plus</b>	<b>2</b>	<b>3.95</b>	--	--	--
	Fuji Dri-Chem NX500/i	28	4.40	0.36	8.12	1
	Fuji Dri-Chem NX500/i	27	4.40	0.36	8.27	1
	Roche cobas c 311	23	3.70	0.18	4.92	--
	Fuji Dri-Chem 4000i	14	4.35	0.27	6.23	--
	Roche cobas INTEGRA	9	3.81	0.13	3.34	--
	Roche cobas 6000	8	3.61	0.17	4.60	--
	Horiba ABX Pentra C200	6	4.08	0.30	7.31	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 5  
Sample Date : 02-07-2021


**Biochemistry, Urea, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	209	47.79	3.53	7.38	17
Urease, GLDH	30	48.16	5.34	11.10	3
Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	48.80	<b>SDI / z-Score</b>	-0.11
<b>Assigned Value</b>	49.61	<b>Average SDI</b>	-3.33
<b>SDPA</b>	7.440	<b>Uncertainty of AV</b>	0.99
<b>Standard Unit Result Val</b>	48.80	<b>%DEV</b>	1.34

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

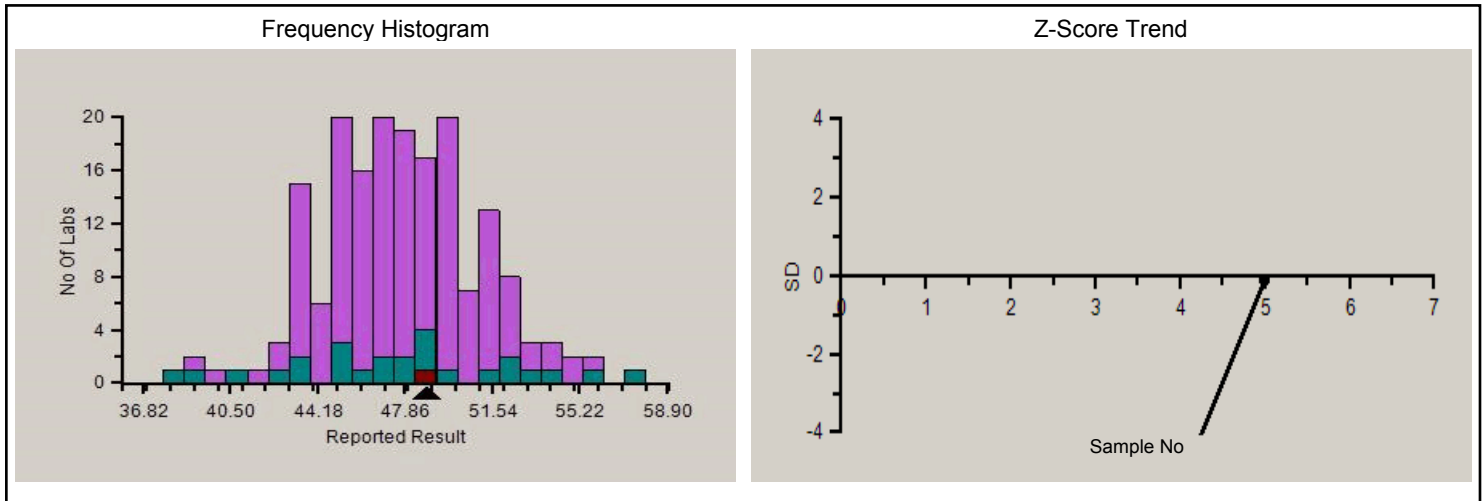

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 5  
Sample Date : 02-07-2021

Biochemistry, Urea		N	Mean	SD	CV%	Excluded
	All Analyzer	209	47.79	3.53	7.38	17
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	36	47.57	3.08	6.47	6
	Fuji Dri-Chem NX500/i	35	47.56	3.13	6.58	6
	Roche cobas c 311	28	48.46	2.50	5.15	1
	Biosystems A15	23	47.54	4.54	9.55	2
	Biosystems A15	22	47.67	4.62	9.69	2
	Biosystems A15	22	47.67	4.62	9.69	2
	ERBA XL-640	17	50.81	4.77	9.38	--
	Fuji Dri-Chem 4000i	14	47.27	2.62	5.55	1

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.

*Dr Puneet Kumar Nigam*

**Dr Puneet Kumar Nigam**  
**PT coordinator & Technical Manager, MHL EQAS**  
Unit No. 409-416.  
Commercial Building - 1A,  
Kohinoor Mall, Kirool Road, Kuria (W),  
Mumbai - 400070



PC-1022



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 4  
Sample Date : 02-07-2021


**Biochemistry, Cholesterol, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	226	149.79	8.45	5.64	17
CHOD-PAP	45	151.25	8.21	5.43	8
Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	138.00	<b>SDI / z-Score</b>	-1.11
<b>Assigned Value</b>	151.49	<b>Average SDI</b>	-1.05
<b>SDPA</b>	12.110	<b>Uncertainty of AV</b>	1.43
<b>Standard Unit Result Val</b>	138.00	<b>%DEV</b>	-8.76

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

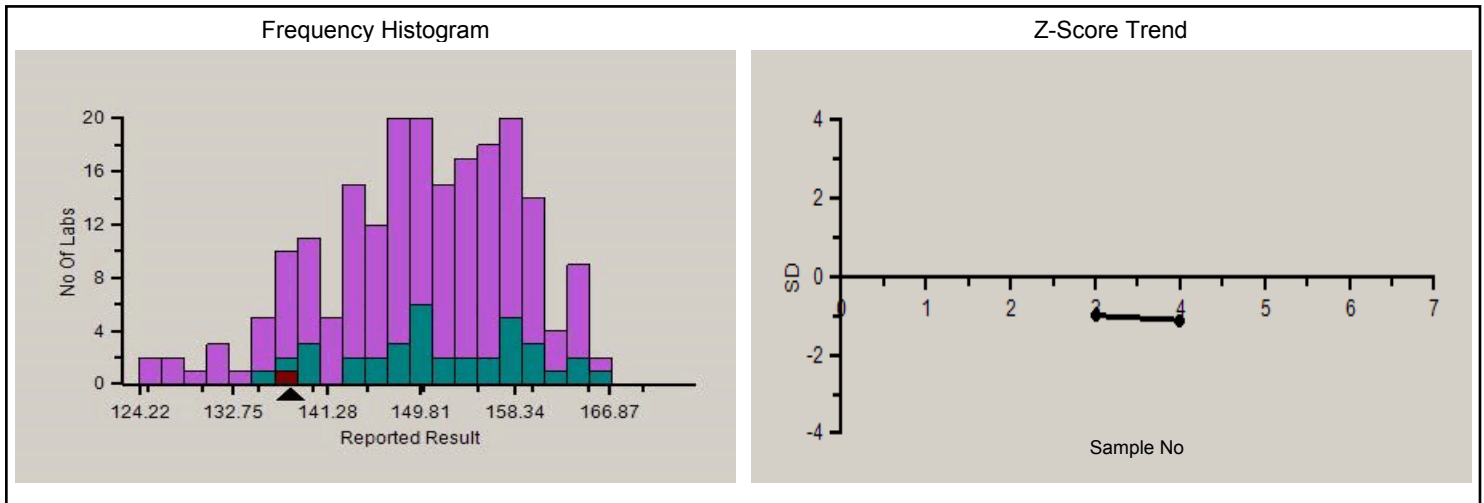

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 4  
 Sample Date : 02-07-2021

<b>Biochemistry, Cholesterol</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	226	149.79	8.45	5.64	17
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	33	141.84	7.46	5.26	3
	Fuji Dri-Chem NX500/i	32	141.90	7.58	5.34	3
	Roche cobas c 311	28	152.40	4.88	3.20	--
	Biosystems A15	23	151.22	9.91	6.55	2
	Biosystems A15	22	151.29	10.16	6.72	2
	Biosystems A15	21	150.83	10.23	6.78	2
	Biosystems A15	21	150.83	10.23	6.78	2
	Erba EM 200	17	150.95	5.96	3.95	2

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 4  
Sample Date : 02-07-2021


**Biochemistry, Creatinine, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	234	0.65	0.21	32.31	19
<span style="color: teal;">■</span> Enzymatic	29	0.82	0.21	24.94	6
<span style="color: darkred;">■</span> Erba EM Destiny 180/XL-180	1	--	--	--	1

<b>Your Result</b>	0.53	<b>SDI / z-Score</b>	-2.24
<b>Assigned Value</b>	0.90	<b>Average SDI</b>	-1.79
<b>SDPA</b>	0.163	<b>Uncertainty of AV</b>	0.03
<b>Standard Unit Result Val</b>	0.53	<b>%DEV</b>	-35.52

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

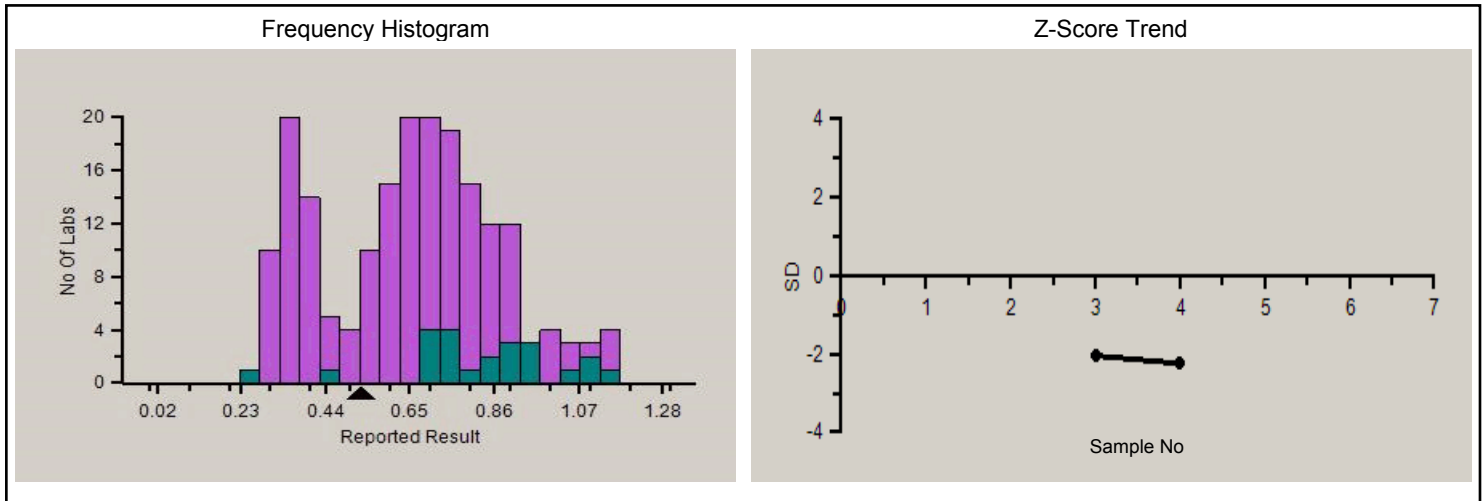

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 4  
 Sample Date : 02-07-2021

<b>Biochemistry, Creatinine</b>		<b>N</b>	<b>Mean</b>	<b>SD</b>	<b>CV%</b>	<b>Excluded</b>
	All Analyzer	234	0.65	0.21	32.31	19
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>1</b>
	Fuji Dri-Chem NX500/i	35	0.35	0.05	14.41	--
	Fuji Dri-Chem NX500/i	34	0.35	0.05	14.69	--
	Roche cobas c 311	28	0.68	0.04	6.43	--
	Biosystems A15	24	0.67	0.13	19.37	4
	Biosystems A15	23	0.68	0.13	19.35	4
	Biosystems A15	22	0.68	0.13	19.35	4
	Biosystems A15	22	0.68	0.13	19.35	4
	Erba EM 200	18	0.82	0.12	14.18	5

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 4  
Sample Date : 02-07-2021


**Biochemistry, Glucose, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	233	67.14	4.38	6.52	14
GOD POD reflectometric analysis	23	68.12	5.11	7.50	3
Erba EM Destiny 180/XL-180	2	70.70	--	--	--

<b>Your Result</b>	70.50	<b>SDI / z-Score</b>	-0.07
<b>Assigned Value</b>	70.92	<b>Average SDI</b>	0.11
<b>SDPA</b>	5.954	<b>Uncertainty of AV</b>	1.11
<b>Standard Unit Result Val</b>	70.50	<b>%DEV</b>	3.50

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

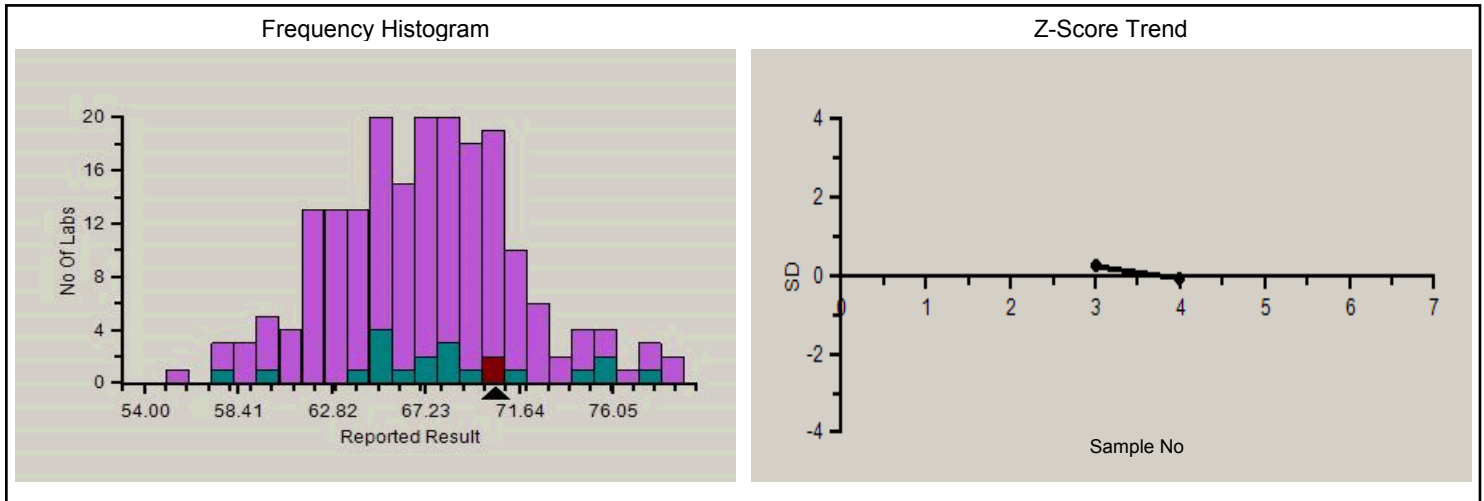

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 4  
 Sample Date : 02-07-2021

Biochemistry, Glucose		N	Mean	SD	CV%	Excluded
	All Analyzer	233	67.14	4.38	6.52	14
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>2</b>	<b>70.70</b>	--	--	--
	Fuji Dri-Chem NX500/i	35	62.75	1.99	3.17	3
	Fuji Dri-Chem NX500/i	34	62.72	2.02	3.21	3
	Roche cobas c 311	28	67.44	1.76	2.61	--
	Biosystems A15	24	67.15	4.14	6.16	1
	Biosystems A15	23	67.02	4.19	6.25	1
	Biosystems A15	22	66.92	4.26	6.37	1
	Biosystems A15	22	66.92	4.26	6.37	1

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 4  
Sample Date : 02-07-2021


**Biochemistry, HDL, mg/dl**

	N	Mean	SD	CV%	Excluded
All Methods	215	33.72	3.96	11.75	11
Direct measure-PEG	56	33.37	4.24	12.72	1
Erba EM Destiny 180/XL-180	1	--	--	--	--

<b>Your Result</b>	33.30	<b>SDI / z-Score</b>	0.12
<b>Assigned Value</b>	32.79	<b>Average SDI</b>	0.11
<b>SDPA</b>	4.166	<b>Uncertainty of AV</b>	0.47
<b>Standard Unit Result Val</b>	33.30	<b>%DEV</b>	-0.20

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

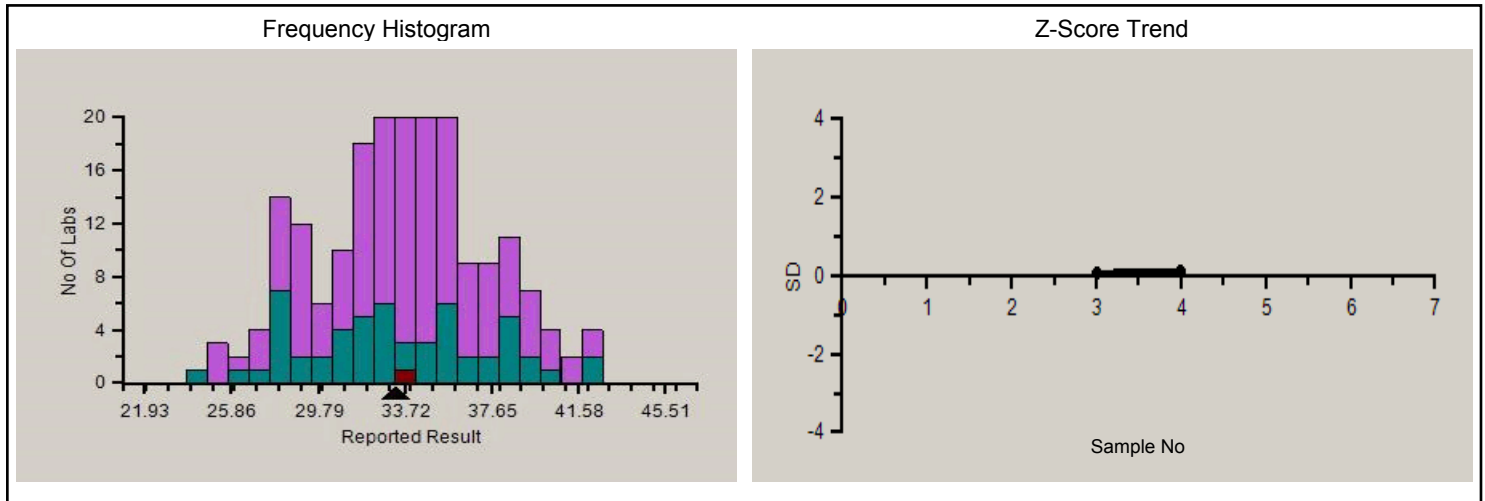

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022

Analyte Methodwise Result Report

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 4  
 Sample Date : 02-07-2021

Biochemistry, HDL		N	Mean	SD	CV%	Excluded
	All Analyzer	215	33.72	3.96	11.75	11
<b>Your Analyzer :</b>	<b>Erba EM Destiny 180/XL-180</b>	<b>1</b>	<b>--</b>	<b>--</b>	<b>--</b>	<b>--</b>
	Fuji Dri-Chem NX500/i	31	34.87	1.45	4.16	2
	Fuji Dri-Chem NX500/i	30	34.87	1.48	4.23	2
	Roche cobas c 311	28	31.51	2.29	7.27	1
	Biosystems A15	23	35.16	4.57	13.00	2
	Biosystems A15	22	34.96	4.59	13.14	2
	Biosystems A15	21	35.13	4.65	13.23	2
	Biosystems A15	21	35.13	4.65	13.23	2
	Erba EM 200	17	33.42	4.87	14.58	1

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



PC-1022



**Analyte Methodwise Result Report**

Lab : 560  
Lab Name : DR SR PATHOLOGY LAB  
Report Date : 19/07/2021

Cycle No : 210207  
Sample No : 4  
Sample Date : 02-07-2021


**Biochemistry, Phosphorous Inorganic, mg/dl**

	N	Mean	SD	CV%	Excluded
<span style="color: purple;">■</span> All Methods	131	3.66	0.21	5.85	4
<span style="color: teal;">■</span> UV Molybdate colorimetric	15	3.79	0.25	6.52	1
<span style="color: darkred;">■</span> Erba Chem 5/Plus	2	3.71	--	--	--

<b>Your Result</b>	4.10	<b>SDI / z-Score</b>	1.12
<b>Assigned Value</b>	3.71	<b>Average SDI</b>	1.23
<b>SDPA</b>	0.348	<b>Uncertainty of AV</b>	0.08
<b>Standard Unit Result Val</b>	4.10	<b>%DEV</b>	8.24

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

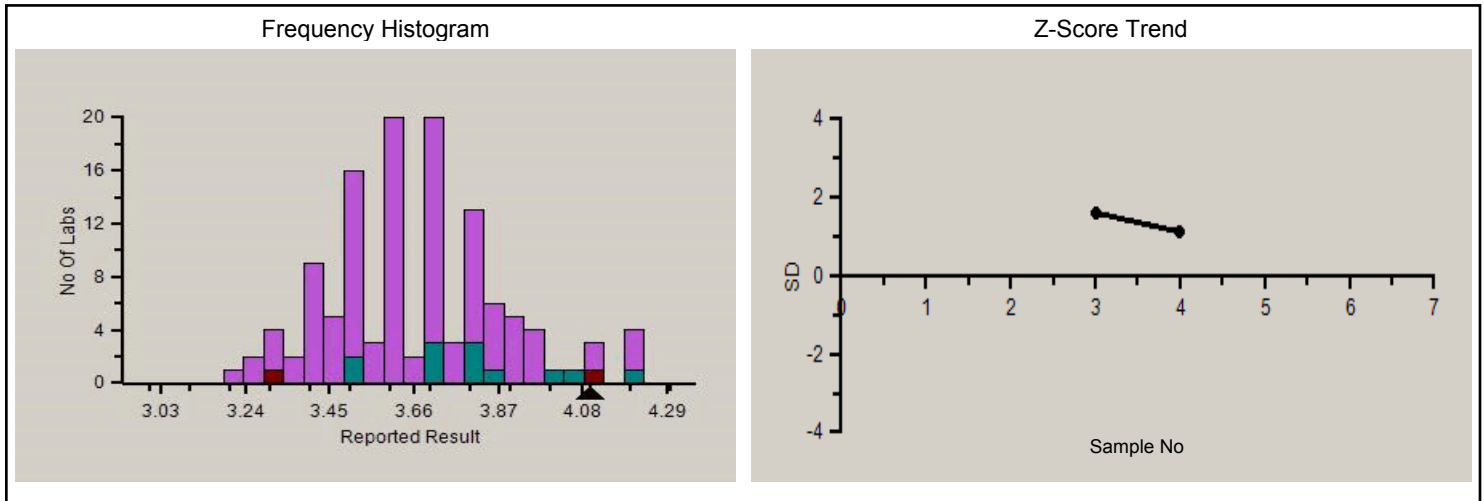

Note : SDI with \* marked are not considered for evaluation.

**Comments :**

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



**Analyte Methodwise Result Report**

Lab : 560  
 Lab Name : DR SR PATHOLOGY LAB  
 Report Date : 19/07/2021

Cycle No : 210207  
 Sample No : 4  
 Sample Date : 02-07-2021

Biochemistry, Phosphorous Inorganic		N	Mean	SD	CV%	Excluded
	All Analyzer	131	3.66	0.21	5.85	4
<b>Your Analyzer :</b>	<b>Erba Chem 5/Plus</b>	<b>2</b>	<b>3.71</b>	--	--	--
	Fuji Dri-Chem NX500/i	28	3.65	0.18	4.85	--
	Fuji Dri-Chem NX500/i	27	3.64	0.18	4.89	--
	Roche cobas c 311	23	3.64	0.17	4.67	--
	Fuji Dri-Chem 4000i	14	3.59	0.18	5.10	--
	Roche cobas INTEGRA	9	3.68	0.12	3.16	--
	Roche cobas 6000	8	3.55	0.12	3.38	--
	Horiba ABX Pentra C200	6	3.92	0.28	7.09	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.

*Dr Puneet Kumar Nigam*

**Dr Puneet Kumar Nigam**  
**PT coordinator & Technical Manager, MHL EQAS**  
 Unit No. 409-416.  
 Commercial Building - 1A,  
 Kohinoor Mall, Kirool Road, Kuria (W),  
 Mumbai - 400070



PC-1022