

Analyte Methodwise Result Report

Lab : 560
 Lab Name : DR SR PATHOLOGY LAB
 Report Date : 19/07/2021

Cycle No : 210207
 Sample No : 2
 Sample Date : 02-07-2021


HbA1C, HbA1c, %

	N	Mean	SD	CV%	Excluded
All Methods	102	5.92	0.30	5.13	5
Nephelometry	10	6.24	0.41	6.55	--
Mispa i2	9	6.26	0.43	6.82	--

Your Result	5.30	SDI / z-Score	-2.58
Assigned Value	6.30	Average SDI	-1.02
SDPA	0.388	Uncertainty of AV	0.15
Standard Unit Result Val	5.30	%DEV	-15.39

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

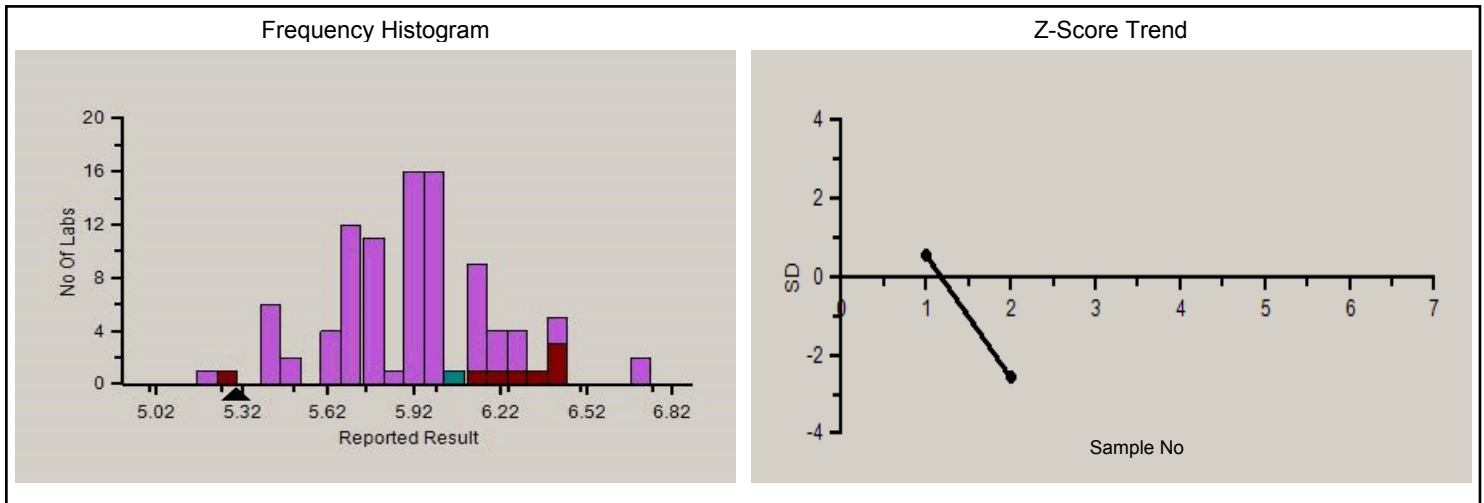

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- If your SDI lies between +/- 2.0 SD then your results are well within limits.
- If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 560
 Lab Name : DR SR PATHOLOGY LAB
 Report Date : 19/07/2021

Cycle No : 210207
 Sample No : 2
 Sample Date : 02-07-2021

HbA1C, HbA1c		N	Mean	SD	CV%	Excluded
	All Analyzer	102	5.92	0.30	5.13	5
Your Analyzer :	Mispa i2	9	6.26	0.43	6.82	--
	Biorad D-10	32	5.88	0.15	2.60	3
	Tosoh G8 Auto HPLC	15	5.96	0.15	2.52	--
	Erba EM 200	12	5.65	0.35	6.15	1
	Transasia XL 640	11	5.89	0.45	7.61	1
	Tosoh HLC 723 GX	7	5.99	0.07	1.15	--
	Roche cobas c 311	6	5.89	0.20	3.45	--
	Roche cobas INTEGRA	3	5.69	0.02	0.40	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
 Unit No. 409-416.
 Commercial Building - 1A,
 Kohinoor Mall, Kirol Road, Kuria (W),
 Mumbai - 400070



PC-1022

Analyte Methodwise Result Report

Lab : 560
 Lab Name : DR SR PATHOLOGY LAB
 Report Date : 19/07/2021

Cycle No : 210207
 Sample No : 1
 Sample Date : 01-07-2021


HbA1C, HbA1c, %

	N	Mean	SD	CV%	Excluded
All Methods	98	5.90	0.36	6.12	7
Nephelometry	10	6.28	0.26	4.19	--
Mispa i2	9	6.31	0.25	3.96	--

Your Result	6.40	SDI / z-Score	0.55
Assigned Value	6.26	Average SDI	-1.02
SDPA	0.255	Uncertainty of AV	0.10
Standard Unit Result Val	6.40	%DEV	1.39

Note : # - Not evaluated / Bimodal distribution

X : SDI more than 4

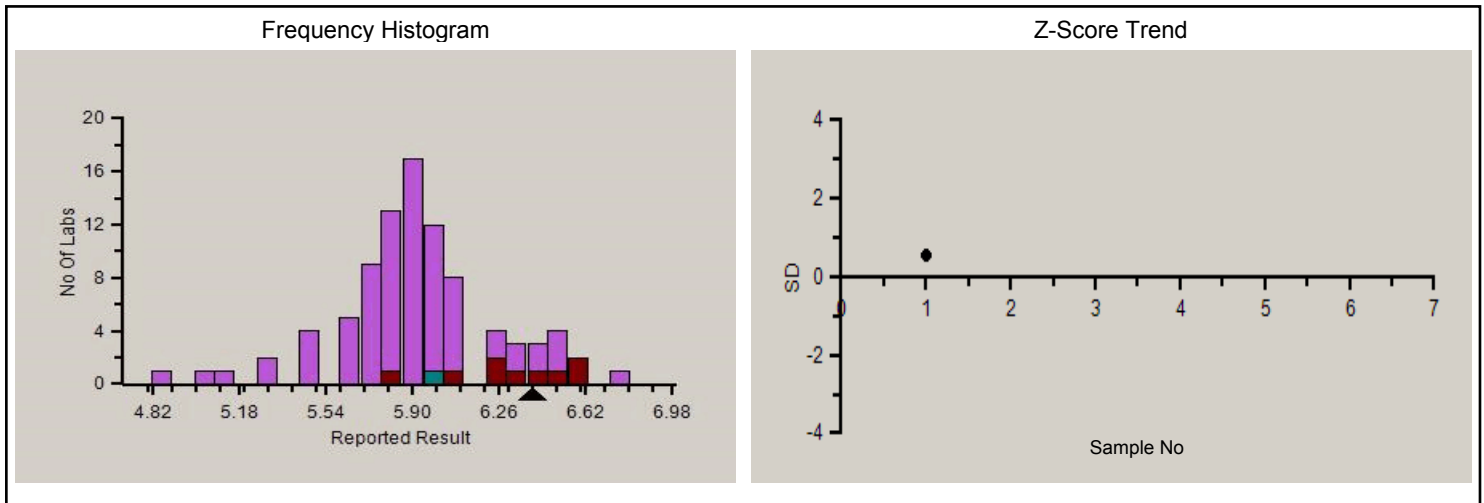

Note : SDI with * marked are not considered for evaluation.

Comments :

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.



Analyte Methodwise Result Report

Lab : 560
 Lab Name : DR SR PATHOLOGY LAB
 Report Date : 19/07/2021

Cycle No : 210207
 Sample No : 1
 Sample Date : 01-07-2021

HbA1C, HbA1c		N	Mean	SD	CV%	Excluded
	All Analyzer	98	5.90	0.36	6.12	7
Your Analyzer :	Mispa i2	9	6.31	0.25	3.96	--
	Biorad D-10	32	5.86	0.16	2.65	4
	Tosoh G8 Auto HPLC	15	5.94	0.19	3.17	--
	Erba EM 200	11	5.54	0.44	7.91	1
	Transasia XL 640	8	5.81	0.81	13.88	1
	Tosoh HLC 723 GX	7	5.97	0.08	1.37	1
	Roche cobas c 311	6	5.98	0.27	4.48	--
	Roche cobas INTEGRA	3	5.62	0.10	1.85	--

Remarks: Interpretation of your reports

- a) If your SDI lies between +/- 2.0 SD then your results are well within limits.
- b) If your SDI lies between +/-2.0 to 2.99 SD then it is a warning alert flag.
- c) If your SDI is +/- 3.0 SD or more then it is an action alert flag.

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
 Unit No. 409-416.
 Commercial Building - 1A,
 Kohinoor Mall, Kirol Road, Kuria (W),
 Mumbai - 400070



PC-1022