

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No : 3/751, 1st Cross Street, Surveyor Colony, K.Pudur, Madurai - 625 007.

Phone : 0452 - 2561691 Mobile : +91 94434 74610



GSTIN: 33AAHCA8053H1ZR • DL No. MDU/4205/20B,MDU/3971/21B • CIN : U33110TN2009PTC072140

CALIBRATION CERTIFICATE



Customer Name & Address:	M/S. Gowtham Diagnostic Centre, 744-B, Uthukuli Main Road, OPP. GH, Kunnathur, Tirupur Dt. - 638 103.	Certificate No:	AMS/LAB/2889723
		Issuing Date:	14/08/2021
		Page No:	1 of 1

Details of Device under Calibration (DUC):

DUC:	Micro Pipette	Id. No:	GDC/LAB/VMP/001
Make:	Dragon Lab	Department:	Laboratory
Model:	Variable	Calibrated On:	13/08/2021
Sl. No:	YE16CAA0129898	Calibration Due Suggested:	12/08/2022
Type:	Variable	DUC Condition on Receipt:	OK
Range & Least Count:	.5 to 50µl		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electronic Weighing Scale	EWC/SF400C	PC/01/21/ATL/0339-01	22/01/2022
2	Thermo Hygrometer	Beetech/088	PC/01/21/ATL/0194-01	22/01/2022

Room Temperature: 25°C±2

Room Humidity: 30-60%

(At the time of Calibration)

Test Results:

SL. No.	DUC Reading (µl)	Standard Reading (µl)		Correction (µl)
		Trial 1	Trial 2	
1	5	4.5	4.5	-0.5
2	10	11.0	11.0	+1.0
3	20	28.0	28.0	+8.0
4	30	35.0	35.0	+5.0
4.	50	45.0	45.0	-5.0

Allowable Tolerance: User Defined

Note:

1. Calibration Points were selected as per customer request.
2. Each reading were taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements



Calibrated By:
(Calibration Engineer)

B. S. S.



Approved by:
(Technical Manager)

B. S. S.

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No : 3/751, 1st Cross Street, Surveyor Colony, K.Pudur, Madurai - 625 007.

Phone : 0452 - 2561691 Mobile : +91 94434 74610



GSTIN. 33AAHCA8053H1ZR • DL No. MDU/4205/20B,MDU/3971/21B • CIN : U33110TN2009PTC072140

CALIBRATION CERTIFICATE



Customer Name & Address:	M/S. Gowtham Diagnostic Centre, 744-B, Uthukuli Main Road, OPP. GH, Kunnathur, Tirupur Dt. - 638 103.	Certificate No:	AMS/LAB/2889724
		Issuing Date:	14/08/2021
		Page No:	1 of 1

Details of Device under Calibration (DUC):

DUC:	Micro Pipette	Id. No:	GDC/LAB/VMP/002
Make:	Bio System	Department:	Laboratory
Model:	Variable	Calibrated On:	13/08/2021
Sl. No:	---	Calibration Due Suggested:	12/08/2022
Type:	Variable	DUC Condition on Receipt:	OK
Range & Least Count:	5 to 50µl		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electronic Weighing Scale	EWC/SF400C	PC/01/21/ATL/0339-01	22/01/2022
2	Thermo Hygrometer	Beetech/088	PC/01/21/ATL/0194-01	22/01/2022

Room Temperature: 25°C±2

Room Humidity: 30-60%

(At the time of Calibration)

Test Results:

SL. No.	DUC Reading (µl)	Standard Reading (µl)		Correction (µl)
		Trial 1	Trial 2	
1	5	5.0	5.0	+0.0
2	10	11.0	11.0	+1.0
3	20	22.0	22.0	+2.0
4	30	31.0	31.0	+1.0
4	50	50.0	50.0	+0.0

Allowable Tolerance: User Defined

Note:

1. Calibration Points were selected as per customer request.
2. Each reading were taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.



Calibrated By:
(Calibration Engineer)

B. S. S.



Approved by:
(Technical Manager)

B. S. S.

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No : 3/751, 1st Cross Street, Surveyor Colony, K.Pudur, Madurai - 625 007.

Phone : 0452 - 2561691 Mobile : +91 94434 74610



GSTIN: 33AAHCA8053H1ZR • DL No. MDU/4205/20B,MDU/3971/21B • CIN : U33110TN2009PTC072140

CALIBRATION CERTIFICATE



Customer Name & Address:	M/S. Gowtham Diagnostic Centre, 744-B, Uthukulj Main Road, OPP. GH, Kunnathur, Tirupur Dt. - 638 103.	Certificate No:	AMS/LAB/2889725
		Issuing Date:	14/08/2021
		Page No:	1 of 1

Details of Device under Calibration (DUC):

DUC:	Micro Pipette	Id. No:	GDC/LAB/VMP/003
Make:	Dragon Lab	Department:	Laboratory
Model:	Variable	Calibrated On:	13/08/2021
Sl. No:	YE173AB0043895	Calibration	
Type:	Variable	Due Suggested:	12/08/2022
Range & Least Count:	100 to 1000µl	DUC Condition on Receipt:	OK

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electronic Weighing Scale	EWC/SF400C	PC/01/21/ATL/0339-01	22/01/2022
2	Thermo Hygrometer	Beetech/088	PC/01/21/ATL/0194-01	22/01/2022

Room Temperature: 25°C±2

Room Humidity: 30-60%

(At the time of Calibration)

Test Results:

SL. No.	DUC Reading (µl)	Standard Reading (µl)		Correction (µl)
		Trial 1	Trial 2	
1	100	90.0	90.0	-10.0
2	200	180.0	180.0	-20.0
3	500	500.0	500.0	+00.0
4	800	800.0	800.0	+00.0
4	1000	1000.0	1000.0	+00.0

Allowable Tolerance: User Defined

Note:

1. Calibration Points were selected as per customer request.
2. Each reading were taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.



Calibrated By:
(Calibration Engineer)

B. S. S.



Approved by:
(Technical Manager)

B. S. S.

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No: 3/751, 1st Cross Street, Surveyor Colony, K.Pudur, Madurai - 625 007.

Phone : 0452 - 2561691 Mobile : +91 94434 74610



GSTIN. 33AAHCA8053H1ZR • DL No. MDU/4205/20B,MDU/3971/21B • CIN : U33110TN2009PTC072140

CALIBRATION CERTIFICATE



Customer Name & Address:	M/S. Gowtham Diagnostic Centre, 744-B, Uthukuli Main Road, OPP. GH, Kunnathur, Tirupur Dt. - 638 103.	Certificate No:	AMS/LAB/2889726
		Issuing Date:	14/08/2021
		Page No:	1 of 1

Details of Device under Calibration (DUC):

DUC:	Micro Pipette	Id. No:	GDC/LAB/VMP/004
Make:	Lab	Department:	Laboratory
Model:	Variable	Calibrated On:	13/08/2021
Sl. No:	---	Calibration Due Suggested:	12/08/2022
Type:	Variable	DUC Condition on Receipt:	OK
Range & Least Count:	100 to 1000µl		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electronic Weighing Scale	EWC/SF400C	PC/01/21/ATL/0339-01	22/01/2022
2	Thermo Hygrometer	Beetech/088	PC/01/21/ATL/0194-01	22/01/2022

Room Temperature: 25°C±2

Room Humidity: 30-60%

(At the time of Calibration)


Test Results:

SL. No.	DUC Reading (µl)	Standard Reading (µl)		Correction (µl)
		Trial 1	Trial 2	
1	100	100.0	100.0	0.0
2	200	200.0	200.0	0.0
3	500	500.0	500.0	0.0
4	800	800.0	800.0	0.0
4	1000	980.0	980.0	-20.0

Allowable Tolerance: User Defined

Note:

1. Calibration Points were selected as per customer request.
2. Each reading were taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

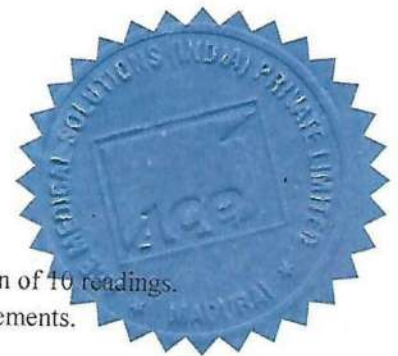

Calibrated By:
(Calibration Engineer)

B. S. S.



Approved by:
(Technical Manager)

B. S. S.

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No : 3/751, 1st Cross Street, Surveyor Colony, K.Pudur, Madurai - 625 007.

Phone : 0452 - 2561691 Mobile : +91 94434 74610



GSTIN. 33AAHCA8053H1ZR • DL No. MDU/4205/20B,MDU/3971/21B • CIN : U33110TN2009PTC072140

CALIBRATION CERTIFICATE



Customer Name & Address:	M/S. Gowtham Diagnostic Centre, 744-B, Uthukuli Main Road, OPP. GH, Kunnathur, Tirupur Dt. - 638 103.	Certificate No:	AMS/LAB/2889727
		Issuing Date:	14/08/2021
		Page No:	1 of 1

Details of Device under Calibration (DUC):

DUC:	Micro Pipette	Id. No:	GDC/LAB/VMP/005
Make:	PATHO PETTE	Department:	Laboratory
Model:	Variable	Calibrated On:	13/08/2021
Sl. No:	---	Calibration Due Suggested:	12/08/2022
Type:	Variable	DUC Condition on Receipt:	OK
Range & Least Count:	100 to 1000µl		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electronic Weighing Scale	EWC/SF400C	PC/01/21/ATL/0339-01	22/01/2022
2	Thermo Hygrometer	Beetech/088	PC/01/21/ATL/0194-01	22/01/2022

Room Temperature: 25°C±2

Room Humidity: 30-60%

(At the time of Calibration)

Test Results:

SL. No.	DUC Reading (µl)	Standard Reading (µl)		Correction (µl)
		Trial 1	Trial 2	
1	100	105.0	105.0	+05.0
2	200	210.0	210.0	+10.0
3	500	480.0	480.0	-20.0
4	800	770.0	770.0	-30.0
4	1000	960.0	960.0	-40.0

Allowable Tolerance: User Defined

Note:

1. Calibration Points were selected as per customer request.
2. Each reading were taken by Repeatability Test (i.e.) each reading in a row is a mean of 40 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

Calibrated By:

(Calibration Engineer)

B. S. S.



Approved by:

(Technical Manager)

B. S. S.