

# CERTIFICATE OF CALIBRATION



CALIBRATION CERTIFICATE NUMBER : 03900003/8/21-22

EQUIPMENT NAME :- MICROPIPETTE			
RECEIVED ON 28.05.2021	CALIBRATED ON 01.06.2021	CALIBRATION DUE DATE RECOMMENDED 01.06.2022	PAGE NO. 1 of 1

**I. Calibrated for :**

PRESTIGE MEDICAL INVESTIGATION, INDORE  
 12/2, NEW AGRAWAL NAGAR, AGRASEN SQUARE  
 Indore, Madhya Pradesh  
 India - 452001

**II. Description and Identification of Instrument :**

Sample Id :	03900003/8
Make :	Not Mentioned
Model :	Not Mentioned
Type :	Not Mentioned
Serial No. :	Not Mentioned

Capacity :	3 µl
Calibrated Range :	3 µl
Least Count :	Not applicable
Condition On Receipt :	Satisfactory
Identification No.:	Not Mentioned

**III. Environment Condition :-**

Temperature :	20 ± 2 °C
Relative Humidity :	50 ± 10 % RH

**IV. Standard/Calibrator and Measuring Equipment Used :**

Nomenclature	Range	Uncertainty	Certificate No.	Traceability	Validity
Weight Box(E1)	1 mg to 200 g	± 0.001 to 0.03 mg	SCW-1120-268	CC-2813	05.11.2023
With Precision Balance, Distilled Water & Digital Thermometer					

**V. Results: (a) Volume**

Serial No.	Scale	UUC #	Standard Average	Correction	Uncertainty (For k=2, 95.45 % C.L.) : ±
1	µl	3.0	0.3071638	-2.692836	0.054

**Note :** 01. UUC # : Unit Under Calibration

02. Certificate shall not be reproduced in full without the written approval of the laboratory

**Other Details**

01. Certificate issue date : 02/06/2021
02. Location of Calibration : Lab
03. Temperature of Distilled water used for calibration is 20.2 °C.
04. The results relate only to the item calibrated

**VI. Inference:**

01. The correction is positive except when indicated other wise It has to be algebraically added to the UUC # reading in order to get the actual reading .

**VII. Reference:**

01. The Calibration is carried out as per the CLL Calibration Procedure No. CLL-IDR-SWP-CAL-000045.
02. All the values have been rounded off as per IS:2-1960.
03. The laboratory is NABL Accredited in the field of Mechanical as per Certificate No. , CC-2089, ULR NO.:CC208921000001238F

**VIII. Details of Adjustment made ( If any)**

Not Done

CALIBRATED BY IDR01183


AUTHORISED SIGNATORY

Signature Not Verified  
 Mitish J. Doshi IDR01183  
 02.06.2021 14:04

**\*\*END OF CALIBRATION CERTIFICATE\*\***

01-Annex.-02

Validative Date: 19

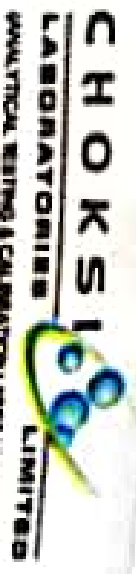

Last Ver 4.0 Dated 01-04-2017

Next Review Due On: 01-04-2022

Equipment ID:

NOT MENTIONED

COC ID:

0890000318/21-3-2

Equipment Name:

MICROPIPE 300

Calibrated On:

(Date of Initiation)

01/05/2021

Calibration Completed on:

(Date of completion)

01/06/2021

Recommended Due Date :

01/06/2022

Valid Calibration Range :

3 μL

Equipment Serial No.:

NOT MENTIONED

Signature:

[Handwritten Signature]

NOTE: Calibration Tag (to be displayed on the instrument after calibration, along with Equipment Tag, CL-MSP-5.5-01-05). Replace after every calibration. Attach the old calibration tags with its corresponding CoC (Certificate of Calibration). Give CoC as follows:

CLL - 3 Character Branch Code - 'Coc' - 3 Character Equipment ID / ddmmYYYY  
(For E.g. IDR-Coc-001/010415 represents calibration tag or Equipment ID '001' at CLL's Indore Branch, on 01 APRIL 2015).

