


Bio-Rad
Laboratories (India) Pvt Ltd
(A wholly owned subsidiary)

"Bio-Rad House", Plot # 86-87 Udyog Vihar Phase - IV Gurgaon-122015, Haryana Phone: 91-124-4029300 Fax: (91)-124-2398115



Website: www.bio-rad.co.in



Calibration Certificate

The **D10 Hemoglobin** system installed at LIKHITHA DIAGNOSTICS, ECIL has been calibrated by checking following procedure.

Hardware Calibration.

Pump flow rate

Actual flow= 2.0 ml/min Measured flow rate=2.0 ml/min

(Flow checked by using volumetric variant sample cups with visible observation)

Column Temperature

Actual Temp = 35 degree C Measured Temp = 34.98 C

(Temp checked by using D10 internal inbuilt temp sensor)

• Optical Detector

Calibrated as per the attached standard test procedure.

Fludic Calibration.

System Calibrated by using NGSP certified Bio-Rad calibrator and performance has been verified by running Quality Control


Date: 26.03.2021

We certify that the **D10 Hemoglobin System** bearing Serial No. DC2A648010 is working as per the specification.

The next calibration due will be on: 25.03.2022

A. Thulasim

Bio-Rad Service

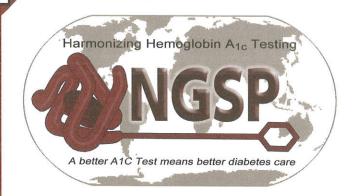

Certificate of Traceability

Manufacturer Certification

This certifies that **Bio-Rad Laboratories, Inc.**, using **D-10 HbA1c**

(12000949) has participated in and successfully completed the NGSP certification for manufacturers and is traceable to the **Diabetes Control and Complications Trial** Reference method. The comparison was performed with: **University of Missouri SRL#9**

The system evaluated was:

Instrument:	Calibrator Lot:	Column Lot #:	
D-10	AA00118, AA00119	R90055B	
Reagent Lot:	Calibrator Assigned Values:		
AA90092, AA90093, AA00142	5.6%, 10.0%		

Randie R Little PhD.

Date of Certification: January 1, 2021

Certification Expires: January 1, 2022

NGSP Steering Committee Chair

NGSP Network Coordinator

SRL director/ supervisor