



CALIBRATION REPORT

Details of the Unit Under Calibration:

Calibration Certificate No: SBS/CL/21-22/09239

Page: 1 of 2

Customer Name:	MEDITECH DIAGNOSTIC CENTRE.	Customer Address:	NEW NO.208,OLD NO.99/1,LAKE VIEW ROAD, WEST MAMBALAM, CHENNAI-33
Location:	LAB	SRF Date:	03-09-2021
Description:	WEIGHT MACHINE	Receipt Date:	03-09-2021
Make & Model:	KRUPS & NA	Date Of calibration:	03-09-2021
Serial No:	80954433	Date Of Due:	02-09-2022
SRF No:	SBS/SRF/21-22/0116-001	Issue Date:	04-09-2021

Traceability Details:

S.No	Standard Used	Make	Model	Serial No	Validity
1	Standard Weights	Sensortron	1Kg	033	08-Aug-2022
2	Standard Weights	Sensortron	2Kg	034	08-Aug-2022
3	Standard Weights	Sensortron	5 Kg	305	31-Mar-2023

Environmental Conditions and Standard Operating Procedure Details:

Temperature	24°C	Calibration Done At	ONSITE
Humidity (40-70% RH)	55%	Calibration Procedure No	SBS/CP/ML/07

REMARKS:

The above mentioned instruments has been calibrated using standard manufacturer recommended protocols, using equipments having traceability to National/International Standards. Partial reproduction of the certificates is not permitted.

Calibrated by:


K.SATHIYAMOORTHY

(Calibration Engineer)

Authorized Signatory:


C. SHANMUGARAJ

(Technical Manager)



Result of Calibration:

QUANTITATIVE TASKS					
S. No	Description	Units	Set Values	Measured Values	Limit/ Tolerance
1.	Weight	Kg	1	1.0	±0.5
2.	Weight	Kg	2	2.0	±0.5
3.	Weight	Kg	3	3.0	±0.5
4.	Weight	Kg	5	5.1	±0.5
5.	Weight	Kg	8	8.2	±0.5

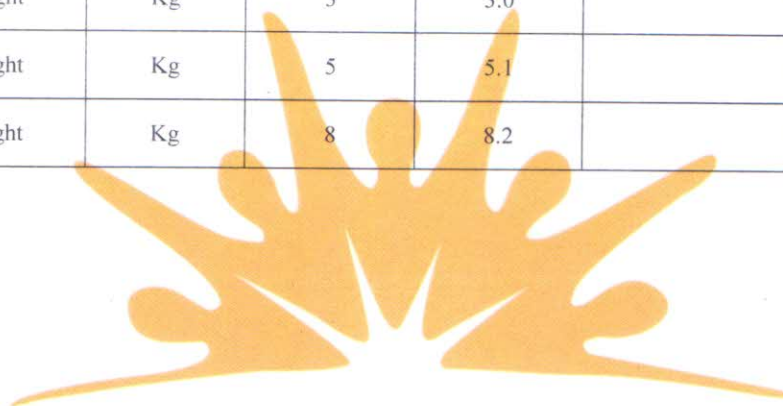

CALIBRATION RESULT:

- Corrective maintenance required
- Removed from use
- Acceptable for use

Calibration Engineer Sign:

K. Sij.

Date: 03-09-2021