

## TECHNICAL SERVICE REPORT

No. 1304316

DATE: 04/09/21

CUSTOMER DETAILS		INSTRUMENT DETAILS		SERVICE STATUS			
NAME: <i>Socia Reveal</i>		MODEL: <i>EM 200</i>		<input checked="" type="checkbox"/> WARRANTY <input type="checkbox"/> R&R <input type="checkbox"/> AMC <input type="checkbox"/> CMC <input type="checkbox"/> CHARGED CALL			
ADDRESS: <i>Jhagdiwadi</i>		SR. NO.: <i>2002286</i>		TYPE OF CALL <input type="checkbox"/> INSTALLATION <input checked="" type="checkbox"/> P.M. VISIT <input type="checkbox"/> I <input type="checkbox"/> II <input type="checkbox"/> III <input type="checkbox"/> IV <input type="checkbox"/> APPLICATION SUPPORT <input checked="" type="checkbox"/> BREAKDOWN			
TEL NO:		JOB COMPLETED		DOWN TIME:			
NAME OF THE OPERATOR:		RESPONSE TIME		COUNTER READING:			
PROBLEM REPORTED: <i>PM + leakage</i>		TRAVEL TIME					
OBSERVATIONS:							
ACTION TAKEN: <i>1) No. of time service done 2) cleared leakage 3) Instrument working ok</i>							
SITE CONDITION: LINE-NEUTRAL VOLT.: <i>229</i> NEUTRAL-EARTH VOLT.: <i>01</i> LINE-EARTH VOLT.: <i>230</i>							
BRAND OF REAGENT USED:				TO BE FILLED IN BY CUSTOMER			
<input type="checkbox"/> FOLLOWING PARTS HAVE BEEN REPLACED <input type="checkbox"/> FOLLOWING PARTS NEED TO BE REPLACED. PLEASE APPROVE				<input checked="" type="checkbox"/> PREVENTIVE MAINTENANCE CARRIED OUT SATISFACTORILY. <input type="checkbox"/> FAULT RECTIFIED & INSTRUMENT IS WORKING SATISFACTORILY. <input type="checkbox"/> WE HEREBY APPROVE RS. _____ FOR PARTS <input type="checkbox"/> COMMENTS (IF ANY):			
NO.	DESCRIPTION	QTY.	COST	TOTAL			
TOTAL Rs.					SEAL	DATE	
					CUSTOMER'S SIGNATURE NAME: <i>Reguher</i>		
INVOICE NO.:				DATE:		BRANCH	H. O.
FOLLOW-UP ACTION (Required if any):				RECEIVED ON:		CHECKED BY:	
ENGINEER'S/PRODUCT SPECIALIST'S SIGNATURE:				JOB CARD NO.:			
TIME:				NAME: <i>M. Anandhan</i>			
NOTE: Parts replaced are chargeable except during warranty Period. Consumables like printer head, lamp, tubing, paper rolls etc. & breakable parts are not covered by warranty and hence are chargeable. Parts replaced due to negligence in operation will also be charged in every case.							
AT TRANSASIA, CUSTOMER SATISFACTION IS OUR PRIME CONCERN. IN CASE YOU HAVE ANY SUGGESTIONS PLEASE CONTACT: GENERAL MANAGER (TECHNICAL SERVICE), MUMBAI. TEL.: 4030 9000 FAX: (022) 4030 9090							

### TRANSASIA BIO-MEDICALS LTD.

Head Office : Transasia House, 8, Chandivali Studio Road, Andheri (E), Mumbai - 400 072. Tel. : (022) 4030 9000 Fax : (022) 2857 3030  
 Mumbai : Toll Free 1800 103 8226  
 Indore : Tel. : (0731) 403 3948    Chennai : Tel. : (044) 2822 7149    Kolkata : Tel. : (033) 2215 7839 Fax : 2215 8035  
 Lucknow : Tel. : (0522) 443 0900    Pune : Tel. : (020) 2616 2658    Dehi : Tel. : (011) 2578 5451/2573 2223  
 Chandigarh : Tel. : (0172) 464 3837    Hyderabad : Tel. : (040) 4430 9000    Ahmedabad : Tel./Fax : (079) 02640 7030/4032 1903  
 Jaipur : Tel. : 93092 63147    Guwahati : Tel. : 91369 50480    Bangalore : Tel./Fax : (080) 2556 8044  
 Patna : Tel. : 77669 00553    Chuttack : Tel. : (0671) 232 4555  
 Kochi : Tel. : (0484) 402 0511    Hubli : Tel. : (0836) 485 0900

DOC NO : SC00-406 / ISS - 5

ISO 13485 & ISO 9001 Certified Co.

www.transasia.co.in

CUSTOMER COPY

**Erba<sup>®</sup>**  
Mannheim

G1] WITHIN RUN PRECISION CHECK

Verified by : Name

SAVED

09/

ERBA PATH: 2004164

2004164

PROV. NO.

05/397

MULTICAL: 2005093

ERBA NORM: 2004163

2004163

ERBA PATH: 2004164

2004164

ITEM	ALB	CHO	GGT	GLU	GPT	PRO	UREA							
RGT lot no.	S102035	S101926	B102053	S102014	B092065	S102009	B102064							
Expiry Date	09/2023	03/2021	09/2022	09/2022	02/2022	09/2023	05/2022							
UNIT	g/dl	mg/dl	IU/L	mg/dl	IU/L	g/dl	mg/dl							
SPECIMEN	NORM	PATH	NORM	PATH	NORM	PATH	NORM	PATH						
1	3.26	4.66	132.00	230.00	40.80	185.70	80.80	246.80	45.90	142.20	5.95	9.17	34.20	93.60
2	3.29	4.62	132.00	231.00	41.70	182.90	80.70	245.60	45.00	144.50	5.89	9.16	34.60	92.80
3	3.27	4.63	129.00	230.00	41.70	179.90	80.60	246.30	44.10	143.00	5.86	9.06	34.60	92.40
4	3.27	4.65	129.00	234.00	41.70	177.80	80.10	246.50	41.20	138.30	5.88	9.13	34.40	91.90
5	3.27	4.66	129.00	231.00	41.90	182.80	80.30	245.80	45.60	142.80	5.88	9.07	34.10	92.40
6	3.26	4.64	133.00	240.00	41.50	185.40	80.00	247.10	44.10	145.70	5.91	9.14	34.60	91.90
7	3.25	4.63	134.00	232.00	42.60	174.00	79.90	247.70	46.20	144.80	5.91	9.14	34.10	91.90
8	3.27	4.64	134.00	232.00	42.40	187.50	79.80	246.50	45.60	145.40	5.89	9.16	34.40	91.90
9	3.26	4.62	131.00	234.00	41.20	180.80	80.20	248.60	46.20	143.30	5.89	9.11	34.40	91.90
10	3.27	4.64	131.00	234.00	42.20	187.00	80.00	246.70	45.30	146.30	5.88	9.11	34.40	91.70
11	3.25	4.62	131.00	232.00	42.10	182.80	80.20	247.40	45.60	145.40	5.90	9.16	34.30	92.50
12	3.26	4.65	130.00	232.00	42.10	184.20	79.60	246.50	44.40	145.10	5.90	9.13	34.50	92.60
13	3.26	4.62	129.00	235.00	42.10	182.60	80.00	246.30	44.70	145.70	5.89	9.12	34.50	92.90
14	3.26	4.62	135.00	229.00	41.50	183.30	80.60	246.90	46.50	146.00	5.86	9.12	34.20	92.60
15	3.26	4.64	134.00	231.00	41.50	182.60	80.90	245.60	45.60	142.80	5.90	9.12	34.50	92.50
16	3.26	4.63	136.00	241.00	39.20	178.40	80.70	246.10	46.20	143.90	5.93	9.15	34.60	92.60
17	3.28	4.64	132.00	237.00	40.50	179.60	80.70	245.60	45.90	142.20	5.89	9.11	34.80	90.80
18	3.26	4.62	132.00	238.00	42.20	180.30	80.70	245.50	45.90	141.60	5.89	9.15	34.40	91.50
19	3.25	4.64	133.00	239.00	42.20	181.50	81.50	248.20	45.00	143.00	5.84	9.12	34.60	92.30
20	3.26	4.64	135.00	239.00	41.20	185.70	82.20	242.80	44.40	144.80	5.87	9.12	34.50	92.20
Mean	3.26	4.64	132.05	234.05	41.62	182.24	80.48	246.43	45.17	143.84	5.89	9.13	34.44	92.25
SD	0.010	0.013	2.188	3.706	0.780	3.338	0.611	1.213	1.188	1.938	0.024	0.028	0.184	0.592
CV(%)	0.30	0.28	1.66	1.58	1.87	1.83	0.76	0.49	2.63	1.35	0.41	0.31	0.54	0.64

Acceptance: Erbanorm < 3.00 % Erbanorm < 3.00 % Erbanorm < 4.99 % Erbanorm < 3.00 % Erbanorm < 3.00 % Erbanorm < 3.00 % Erbanorm < 3.00 % Erbanorm < 3.00 %  
 Erbapath < 3.00 % Erbapath < 3.00 % Erbapath < 3.00 % Erbapath < 3.00 % Erbapath < 3.00 % Erbapath < 3.00 % Erbapath < 3.00 % Erbapath < 3.00 %

## INSTALLATION & TRAINING REPORT

Customer Name : SR Diagnostics Centre, Sewa Ruler, Jhugadia  
 Department : Laboratory  
 Address : Sewa Ruler, Kancherba Hospital, Jhugadia  
 City : Jhugadia Pin : 393110 State : Gujarat  
 Territory : Box-II Zone : WZ-II  
 Telephone & Fax : \_\_\_\_\_ email : sewaruler@gmail.com  
 Contact Person : Mr. Rajendra Mobile No. : 9898516890  
 Instrument Model: EM-200 Sr. No. : 2002286  
 Installation Date : 19/03/21

The above mentioned instrument has been satisfactorily installed by Service Engineer / Product Specialist of Transasia Bio-Medicals Ltd. Operational Training & User Maintenance of the instrument was provided to the following staff members on date (s) : 19/03/21 & 20/03/21

Name (s)	Designation/ Dept.
1. <u>Mr. Rajendra</u>	<u>Lab Incharge</u>
2. _____	_____
3. _____	_____

Test/ Parameters Demonstrated : Calibrate essential parameters. G.C. unit in range

Customer Comments (If any) : \_\_\_\_\_


Engineer / Product Specialist : \_\_\_\_\_ Customer Signature : [Signature]

Signature : [Signature] Customer Name : Dr. Manoj

Name : Manoj Vaja / Siddharth Patel Designation : \_\_\_\_\_

Date : 20/03/21 Customer Seal : \_\_\_\_\_

**Arbitration Clause**  
 All disputes, Differences, controversies and questions directly or indirectly arising at any time under, out of, in connection with or in relation to the payment of this instrument / reagents / service shall be referred to the sole arbitrator to be appointed by Transasia Bio-Medicals Limited under the Arbitration and Conciliation Act 1996. The venue and seat of arbitration shall be at Mumbai. The award rendered by the arbitrator(s) shall be final and binding upon both Parties.

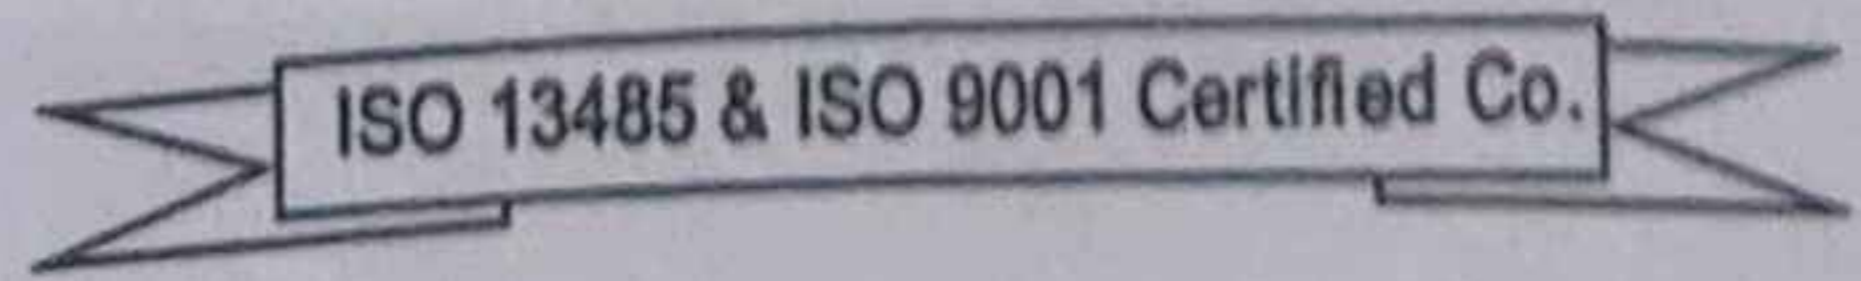

www.transasia.co.in

**TRANSASIA BIO-MEDICALS LTD.**

TRANSASIA HOUSE, 8 CHANDIVALI STUDIO ROAD, ANDHERI (E), MUMBAI - 400 072. TEL : 4030 9000 FAX : (022) 4030 9090 / 2857 3030 Email : transasia@transasia.co.in  
 DELHI (011) 25732223 CHENNAI (044) 28227149 KOLKATA (033) 22157839 BANGALORE (080) 25568044 AHMEDABAD (079) 26407030

Doc No. SCOO-430/ISS-4

CUSTOMER COPY