

Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021


Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Clinical Path - Urine Routine Chemistry, Bilirubin (urine), -

	N
■ All Methods	113
■ Diazonium salt	109
■ Manual	62

Your Result	Negative
Result Expected	Neg

Note : # is an indication that this parameter has not been evaluated

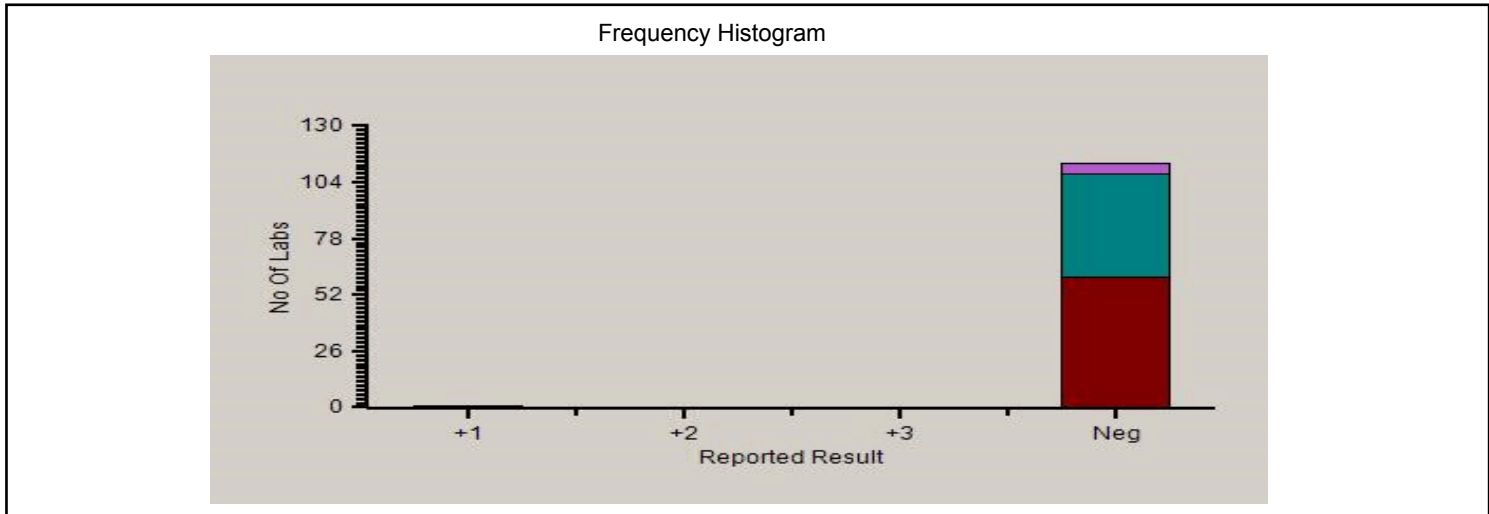

Reported Results Legends :-

+1	: 1+
+2	: 2+
+3	: 3+
Neg	: Negative

Comments :



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 2 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021


Clinical Path - Urine Routine Chemistry,Blood (urine), -

	All Methods	N
	Peroxidase enzyme	118
	Manual	89
		66

Your Result	Negative
Result Expected	Neg

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

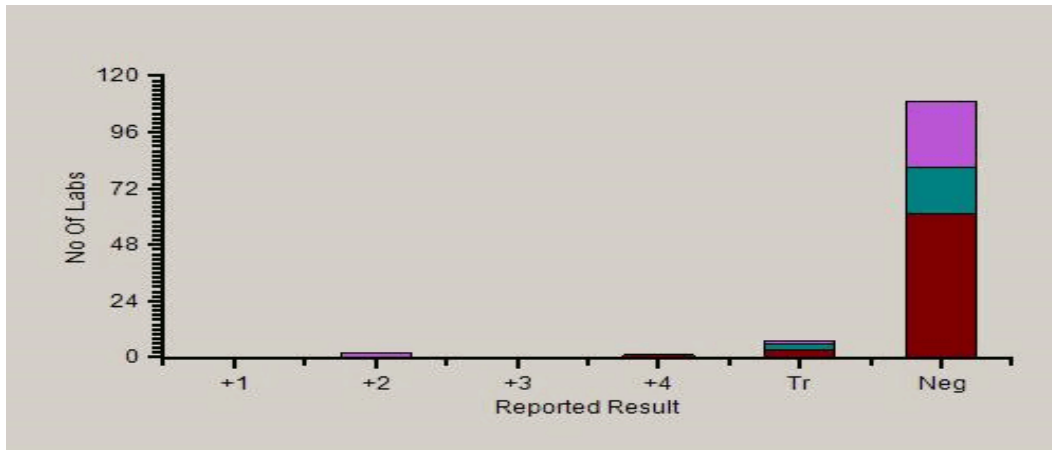

Reported Results Legends :-

+1	: 1+
+2	: 2+
+3	: 3+
+4	: 4+
Tr	: Trace
Neg	: Negative



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021


Clinical Path - Urine Routine Chemistry, Glucose (urine), -

	N
 All Methods	125
 Glucose oxidase peroxidase	103
 Manual	72

Your Result	3+
Result Expected	+2,+3,+4

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

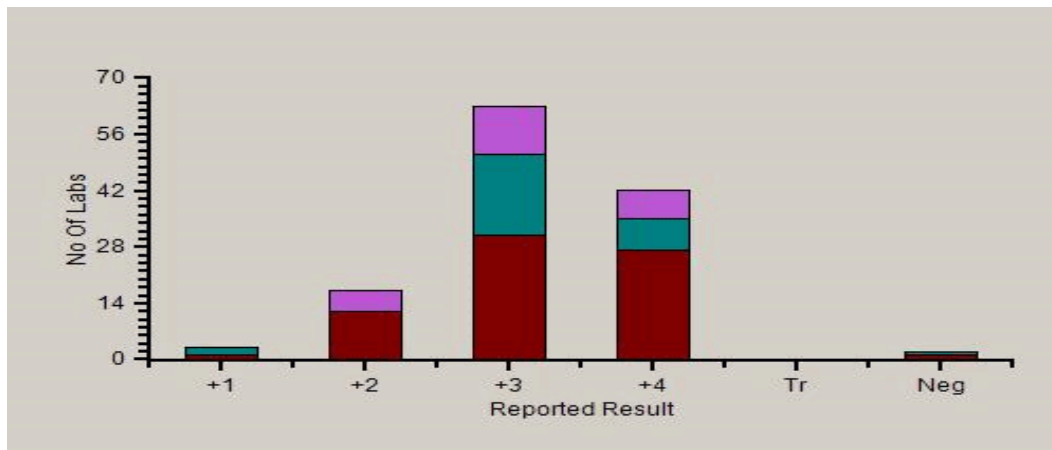

Reported Results Legends :-

+1	: 1+
+2	: 2+
+3	: 3+
+4	: 4+
Tr	: Trace
Neg	: Negative



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021


Clinical Path - Urine Routine Chemistry, Ketone (urine), -

	N
 All Methods	120
 Sodium nitropruside Reflectometric Analysis	88
 Manual	67

Your Result	Negative
Result Expected	Neg

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

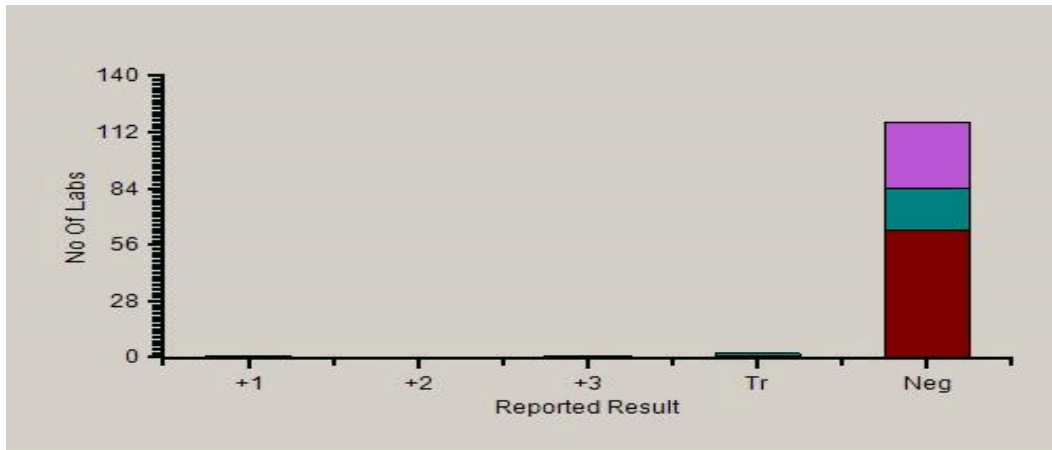

Reported Results Legends :-

+1	: 1+
+2	: 2+
+3	: 3+
Tr	: Trace
Neg	: Negative



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021


Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Clinical Path - Urine Routine Chemistry,Nitrite (urine), -

	N
■ All Methods	119
■ Griess test	33
■ Manual	66

Your Result	Absent
Result Expected	Abs

Note : # is an indication that this parameter has not been evaluated

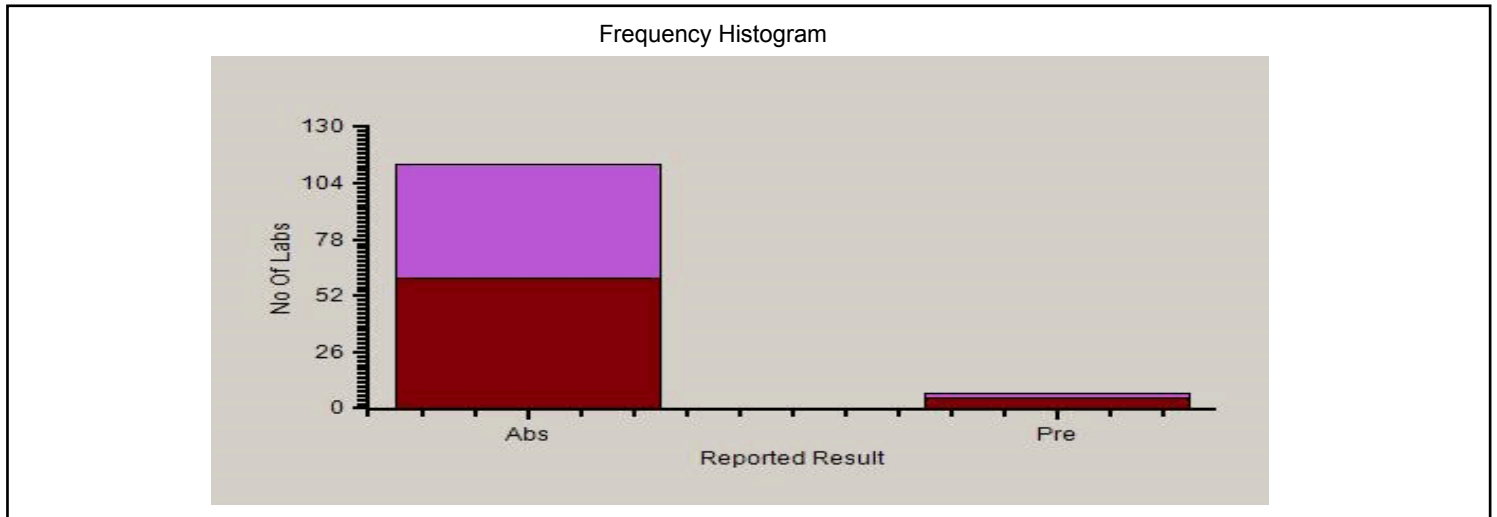

Reported Results Legends :-	
Abs	: Absent
Pre	: Present

Comments :



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021


Clinical Path - Urine Routine Chemistry,pH, -

	N
■ All Methods	120
■ Indicator Principle	122
■ Manual	67

Your Result	6
Result Expected	6,6.5

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

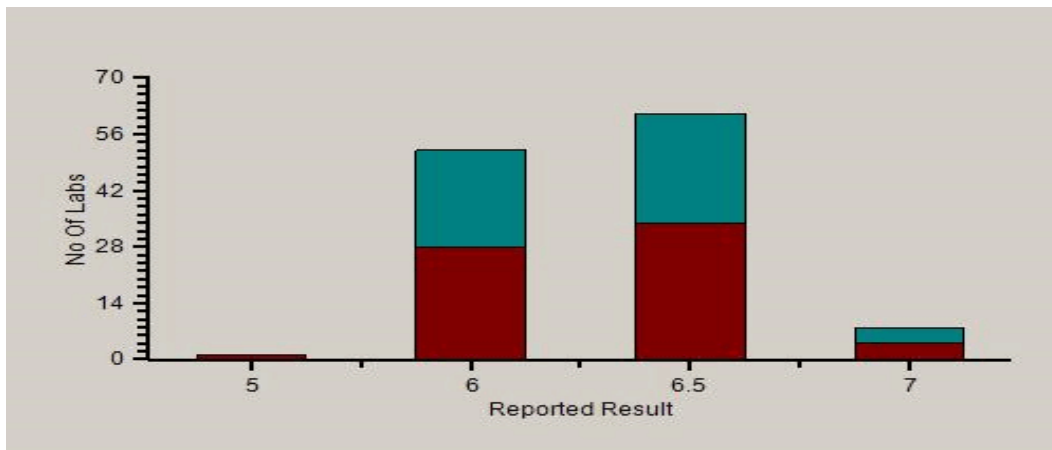

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Reported Results Legends :-	
5	: 5
5.5	: 5.5
6	: 6
6.5	: 6.5
7	: 7
7.5	: 7.5
8	: 8
8.5	: 8.5
9	: 9

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021


Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Clinical Path - Urine Routine Chemistry,Protein (Urine), -

	All Methods	N
	Protein error principle of indicator	125
	Manual	88
		71

Your Result	2+
Result Expected	+1,+2,+3

Note : # is an indication that this parameter has not been evaluated

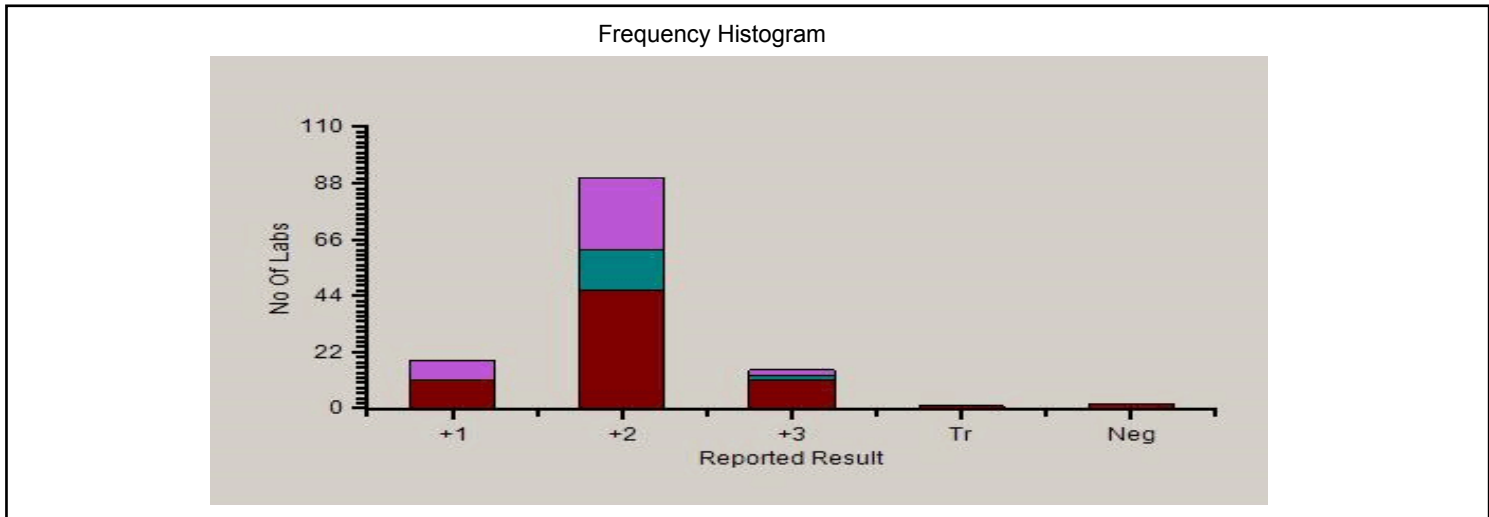

Reported Results Legends :-

+1	: 1+
+2	: 2+
+3	: 3+
Tr	: Trace
Neg	: Negative



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021


Clinical Path - Urine Routine Chemistry, Specific Gravity, -

	All Methods	120
	pH Indicator dye	24
	Manual	67

Your Result	1.020
Result Expected	1.015, 1.020, 1.025

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

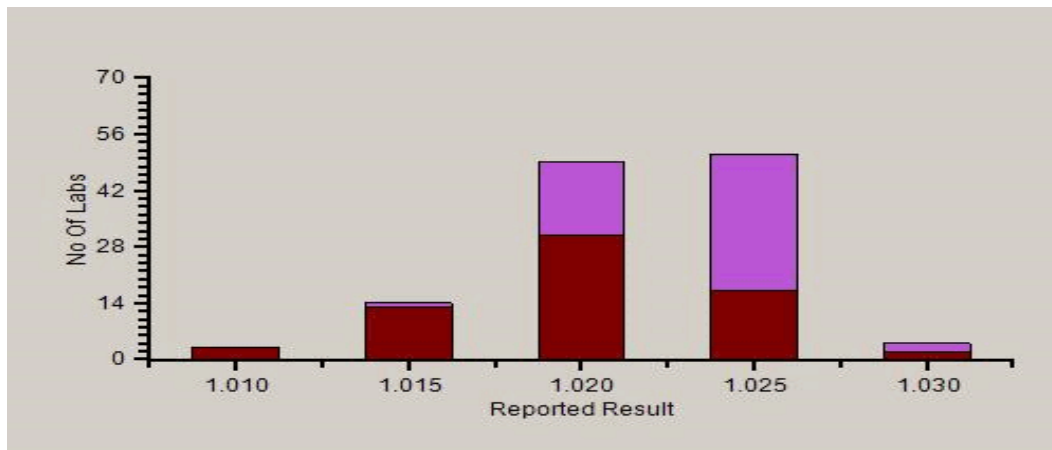

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Reported Results Legends :-	
1.005	: 1.005
1.010	: 1.010
1.015	: 1.015
1.020	: 1.020
1.025	: 1.025
1.030	: 1.030
1.035	: 1.035

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021


Clinical Path - Urine Routine Chemistry,Urine Pregnancy Test, -

	N
 All Methods	78
 Immunochromatography	78
 -	77

Your Result	Negative
Result Expected	Neg

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

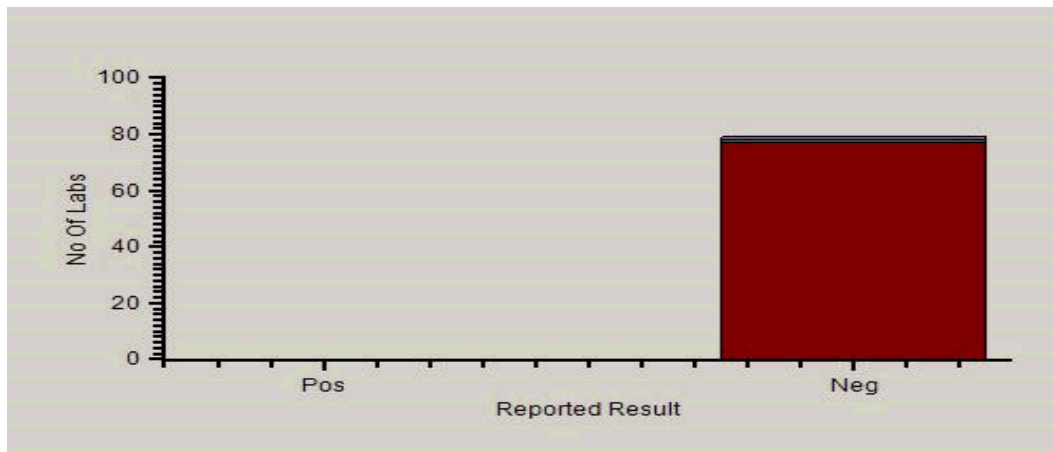

Reported Results Legends :-	
Pos	: Positive
Neg	: Negative

Comments :



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021


Clinical Path - Urine Routine Chemistry,Urobilinogen (urine), -

<p> All Methods</p> <p> Diazonium salt</p> <p> Manual</p>	<p>N</p> <p>115</p> <p>55</p> <p>63</p>
---	---

Your Result	Normal
Result Expected	Nor

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

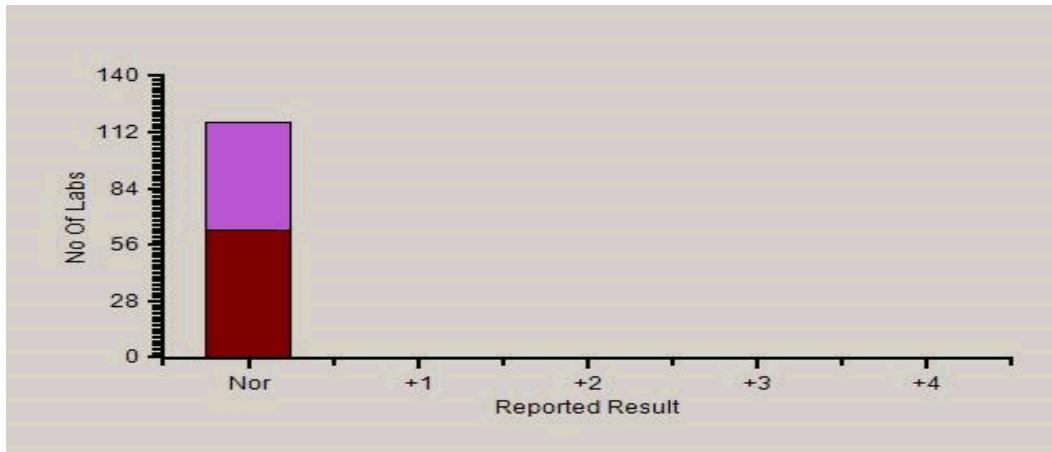

Reported Results Legends :-

Nor	: Normal
+1	: 1+
+2	: 2+
+3	: 3+
+4	: 4+



Analyte Methodwise Qualitative Result Report


Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
Unit No. 409-416,
Commercial Building - 1A,
Kohinoor Mall, Kiroi Road, Kurla (W),
Mumbai - 400070



PC-1022