

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021


Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Qualitative Immunoassay,Dengue NS 1, -

	N
■ All Methods	65
■ Immunochromatography	56
■ Manual	67

Your Result	Negative
Result Expected	Neg

Note : # is an indication that this parameter has not been evaluated

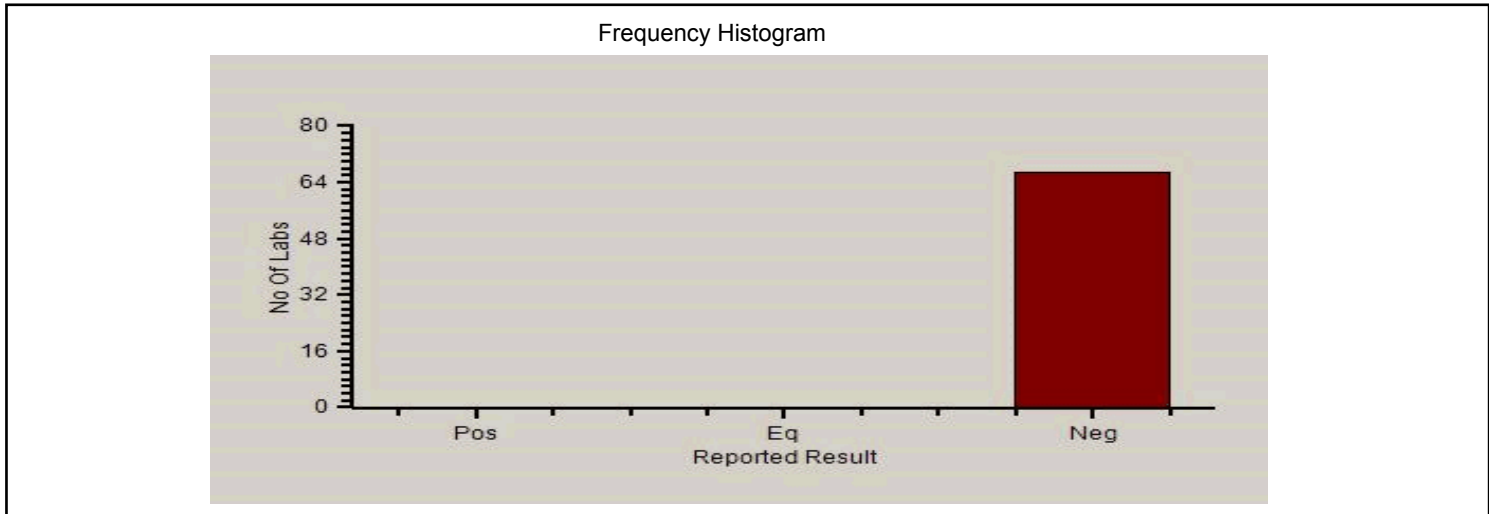

Reported Results Legends :-

Pos	: Positive
Eq	: Equivocal
BL	: Borderline
Neg	: Negative

Comments :



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 2 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021


Qualitative Immunoassay,HBsAg, -

	N
 All Methods	99
 Immunochromatography	60
 Manual	48

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

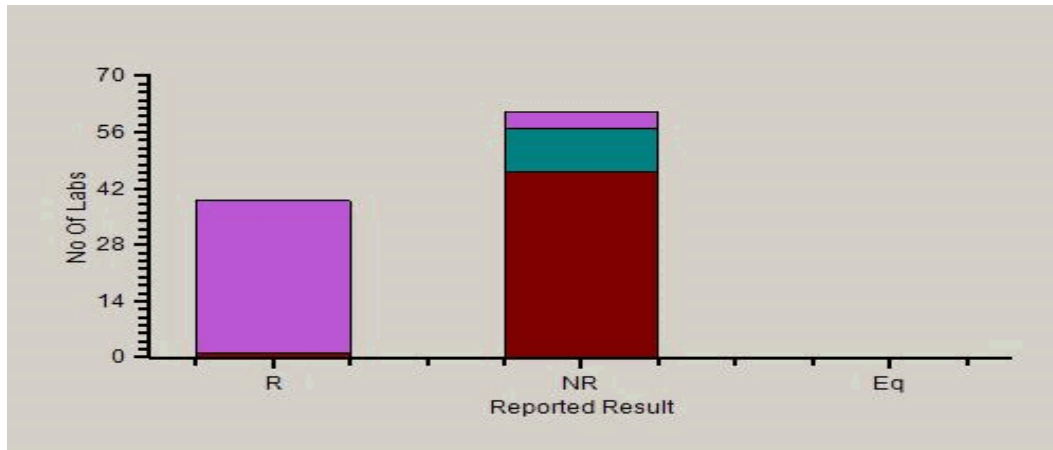

Reported Results Legends :-

R : Reactive
 NR : Non-reactive
 Eq : Equivocal

Comments :



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021


Qualitative Immunoassay,HCV, -

	N
 All Methods	88
 Immunochromatography	52
 Manual	43

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

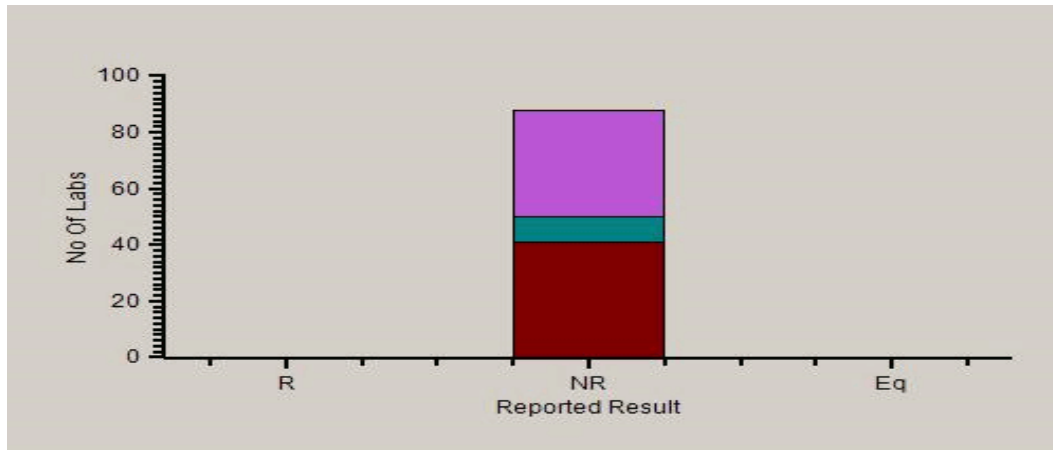

Reported Results Legends :-

R : Reactive
 NR : Non-reactive
 Eq : Equivocal

Comments :



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021


Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Qualitative Immunoassay,HIV Ab, -

	All Methods	N
	Immunochromatography	44
	Manual	42
		38

Your Result	Reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

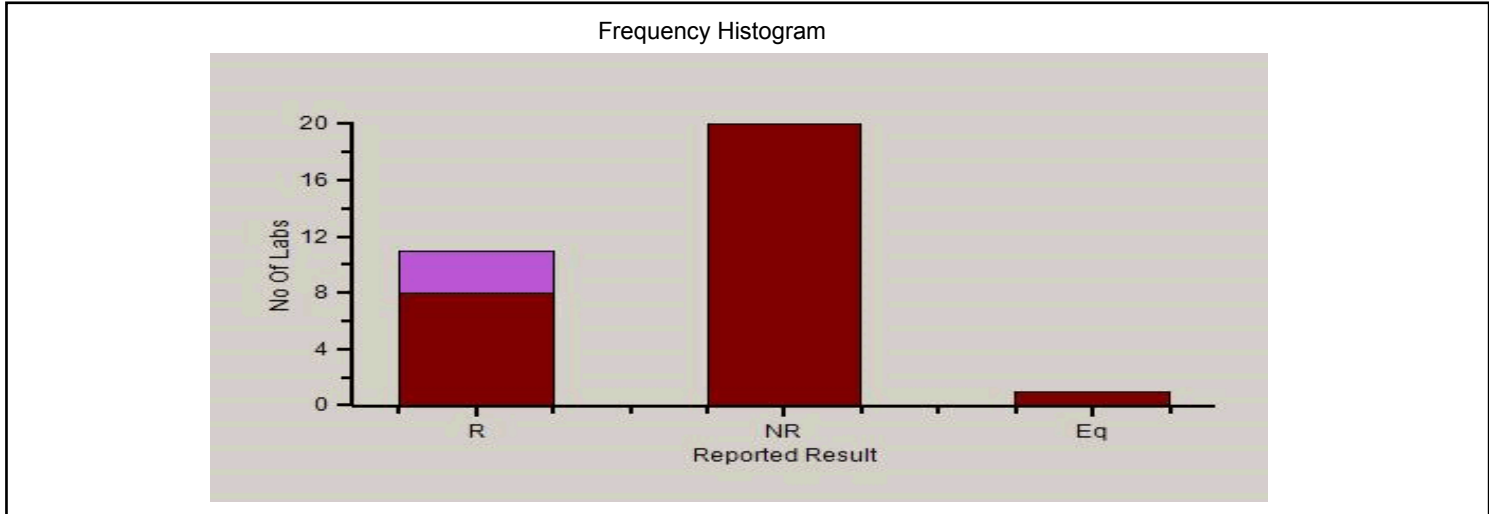

Reported Results Legends :-

R	: Reactive
NR	: Non-reactive
Eq	: Equivocal
Indet	: Indeterminate
HIV-1	: HIV-1 Ab Reactive
HIV-2	: HIV-2 Ab Reactive



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021


Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Qualitative Immunoassay,RPR (Syphilis Serology), -

	N
■ All Methods	75
■ Immunochromatography	28
■ Manual	77

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

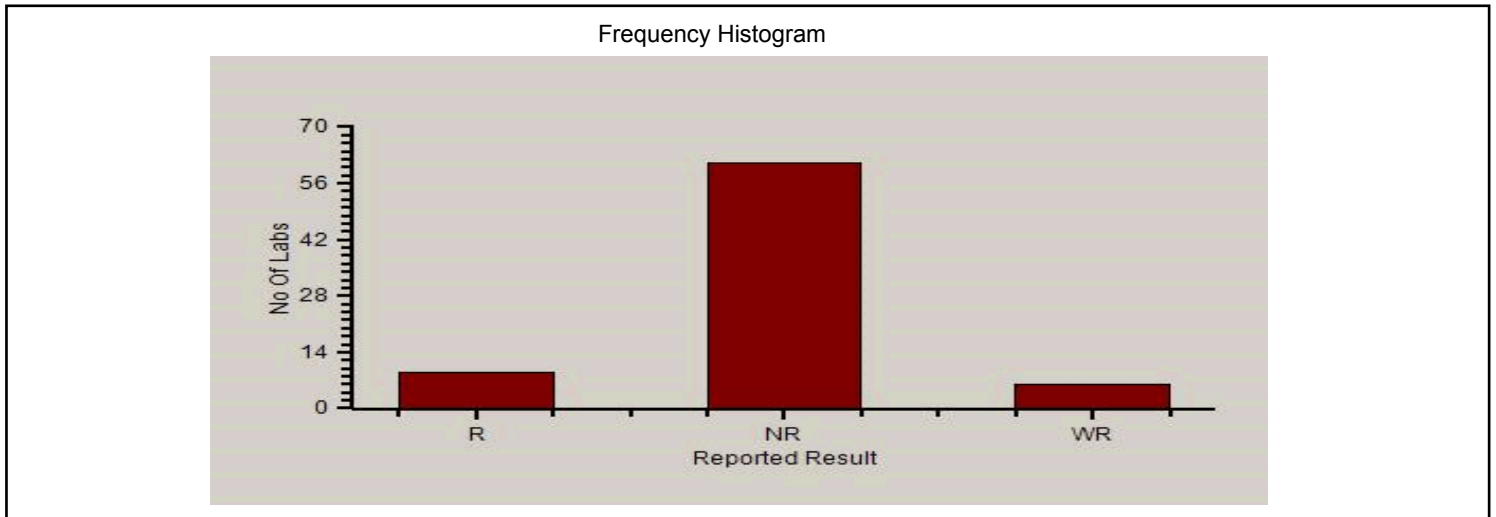

Reported Results Legends :-

R	: Reactive
NR	: Non-reactive
WR	: Weak Reactive

Comments :



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021


Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Qualitative Immunoassay, Typhidot IgM, -

<p> All Methods</p> <p> Immunochromatography</p> <p> Manual</p>	<p>N</p> <p>61</p> <p>63</p> <p>64</p>
---	--

Your Result	Negative
Result Expected	Neg

Note : # is an indication that this parameter has not been evaluated

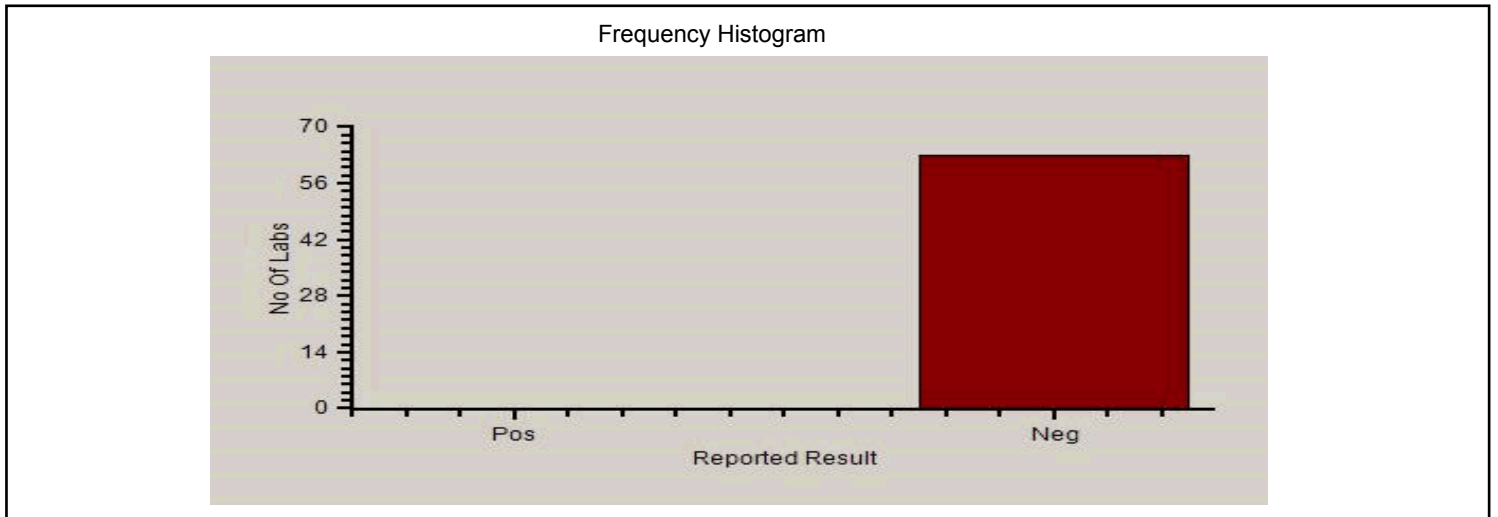

Reported Results Legends :-	
Pos	: Positive
Neg	: Negative

Comments :



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021


Qualitative Immunoassay,Widal test - ParaTyphi A-H antigen (AH), -

	N
 All Methods	76
 Slide Agglutination	54
 Manual	79

Your Result	No Agglutination
Result Expected	NoA

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

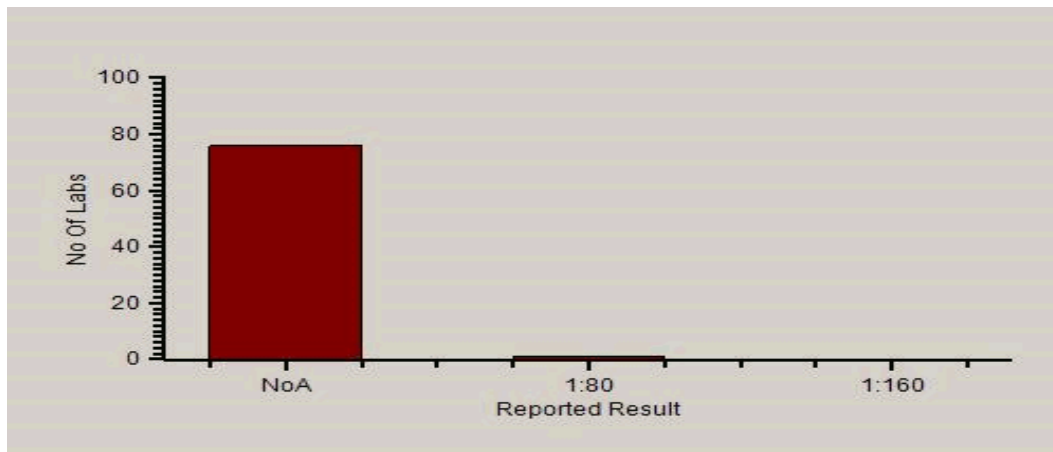

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021


Qualitative Immunoassay,Widal test - ParaTyphi B-H antigen (BH), -

	N
 All Methods	75
 Slide Agglutination	53
 Manual	78

Your Result	No Agglutination
Result Expected	NoA

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

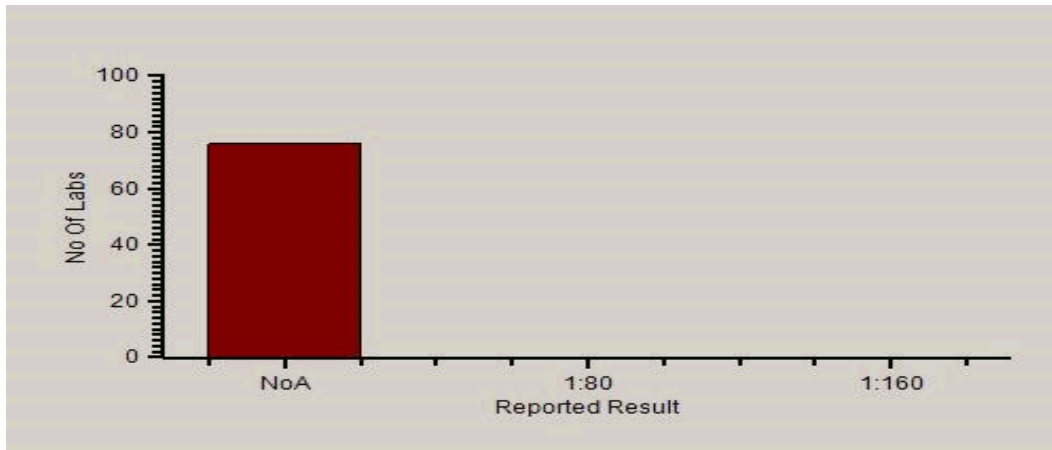

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021


Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021

Qualitative Immunoassay,Widal test - Typhi H antigen (TH), -

<p> All Methods</p> <p> Slide Agglutination</p> <p> Manual</p>	<p>N</p> <p>85</p> <p>60</p> <p>88</p>
--	--

Your Result	No Agglutination
Result Expected	NoA

Note : # is an indication that this parameter has not been evaluated

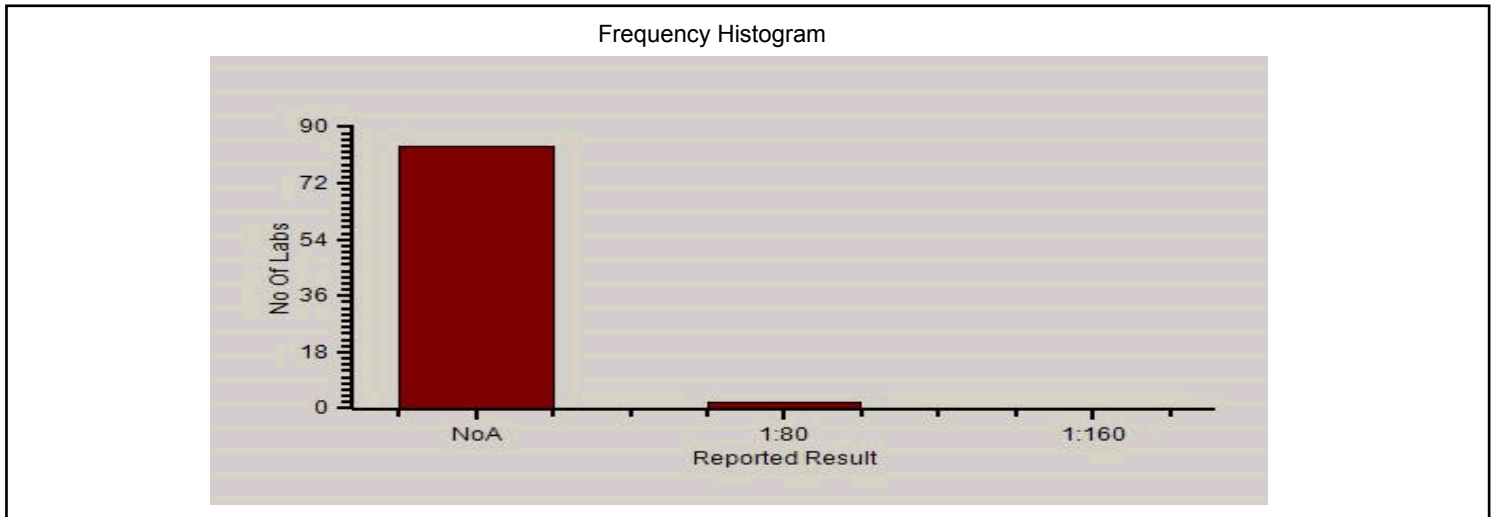

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 1
 Sample Date : 03-03-2021


Qualitative Immunoassay,Widal test - Typhi O antigen (TO), -

	N
 All Methods	86
 Slide Agglutination	61
 Manual	89

Your Result	No Agglutination
Result Expected	NoA

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

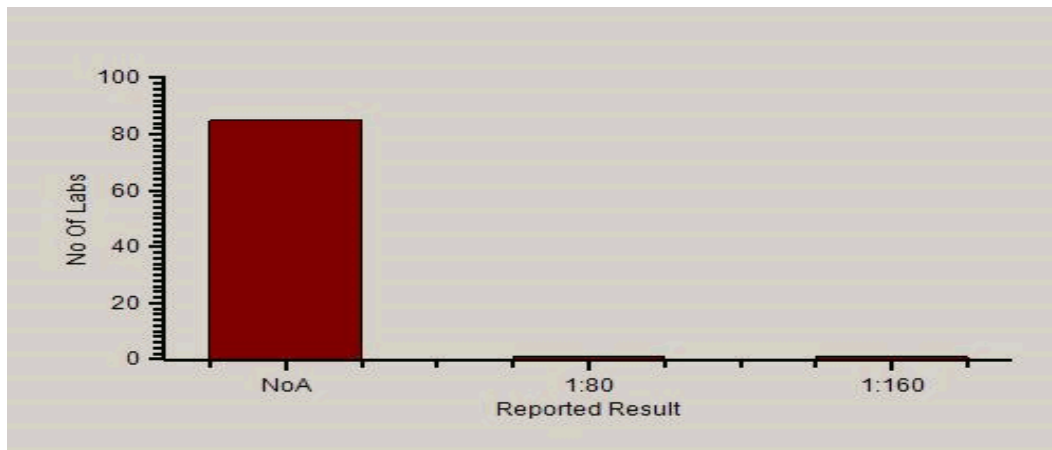

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640



Analyte Methodwise Qualitative Result Report


Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
Unit No. 409-416,
Commercial Building - 1A,
Kohinoor Mall, Kiroi Road, Kurla (W),
Mumbai - 400070



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021


Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021

Qualitative Immunoassay,Dengue NS 1, -

	N
 All Methods	60
 Immunochromatography	51
 Manual	62

Your Result	Negative
Result Expected	Neg

Note : # is an indication that this parameter has not been evaluated

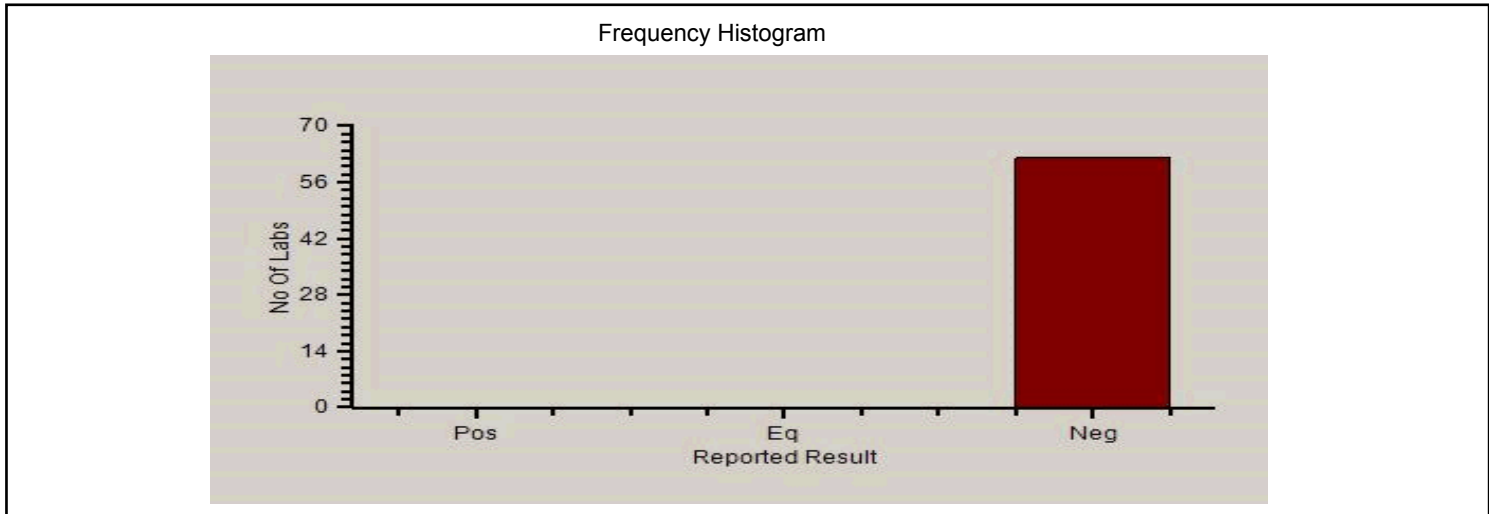

Reported Results Legends :-

Pos	: Positive
Eq	: Equivocal
BL	: Borderline
Neg	: Negative

Comments :



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 2 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021


Qualitative Immunoassay,HBsAg, Nil

	N
 All Methods	92
 Immunochromatography	54
 Manual	43

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

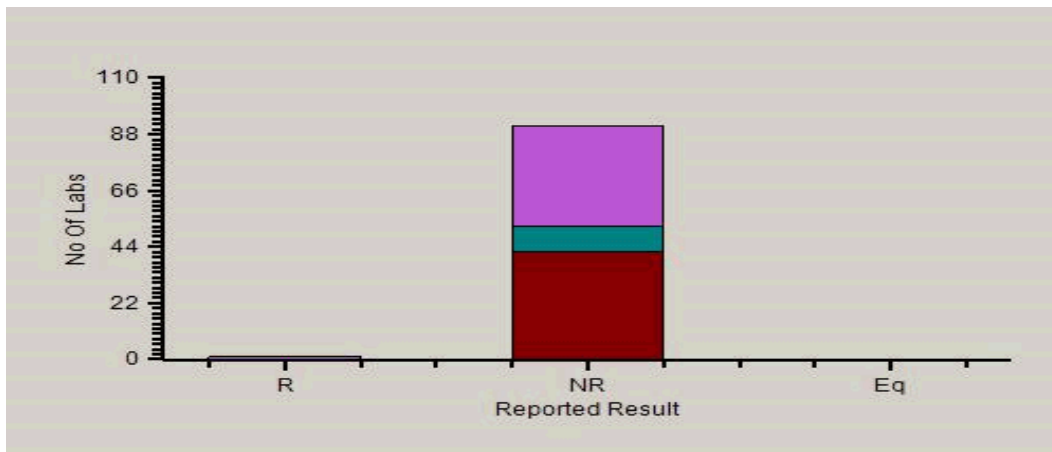

Reported Results Legends :-

- R : Reactive
- NR : Non-reactive
- Eq : Equivocal

Comments :



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021


Qualitative Immunoassay,HCV, -

	All Methods	N
	Immunochromatography	80
	Manual	46
		38

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

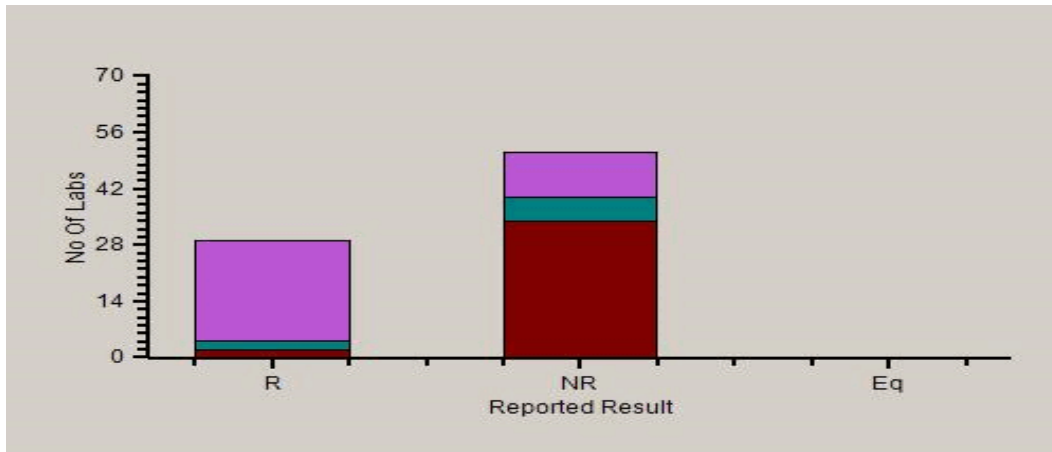

Reported Results Legends :-	
R	: Reactive
NR	: Non-reactive
Eq	: Equivocal

Comments :



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Qualitative Immunoassay,HIV Ab, -


	N
 All Methods	39
 Immunochromatography	37
 Manual	33

Your Result Reactive

Result Expected #

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

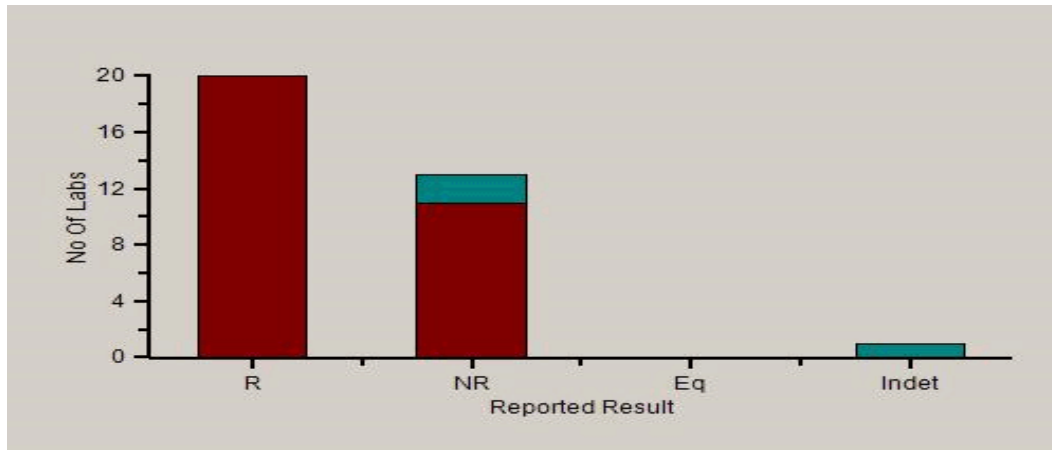

Reported Results Legends :-

- R : Reactive
- NR : Non-reactive
- Eq : Equivocal
- Indet : Indeterminate
- HIV-1 : HIV-1 Ab Reactive
- HIV-2 : HIV-2 Ab Reactive



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021


Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021

Qualitative Immunoassay,RPR (Syphilis Serology), -

	N
 All Methods	72
 Immunochromatography	28
 Manual	74

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

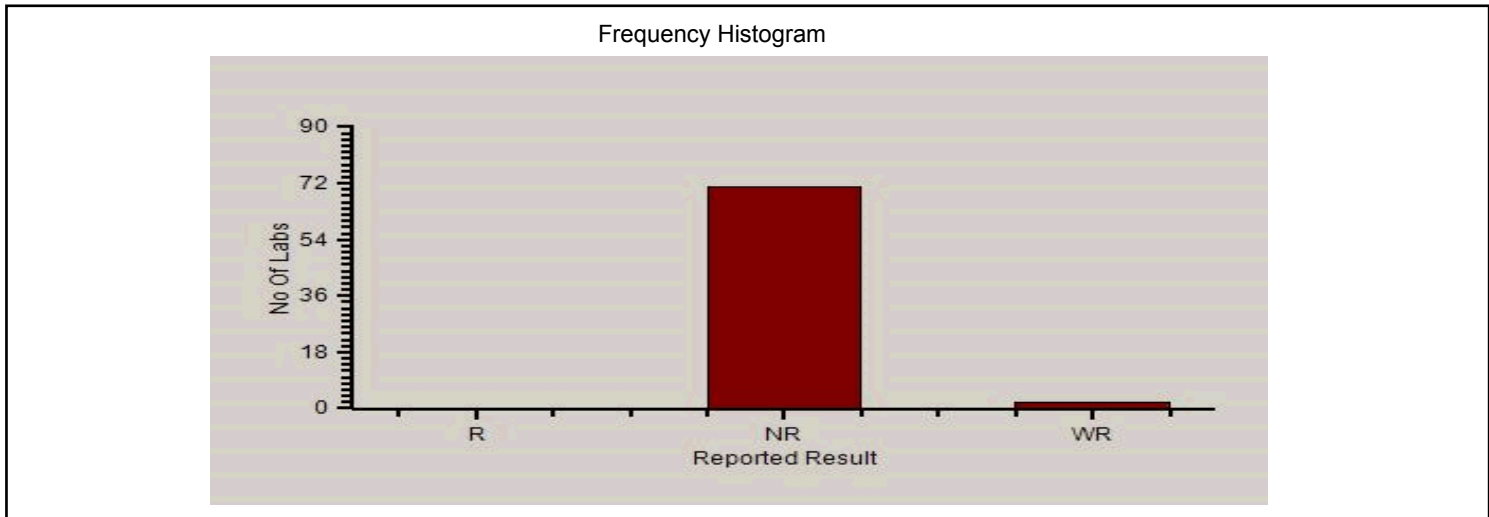

Reported Results Legends :-

R	: Reactive
NR	: Non-reactive
WR	: Weak Reactive

Comments :



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021


Qualitative Immunoassay, Typhidot IgM, -

<p> All Methods</p> <p> Immunochromatography</p> <p> Manual</p>	<p>N</p> <p>58</p> <p>59</p> <p>60</p>
---	--

Your Result	Negative
Result Expected	Neg

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

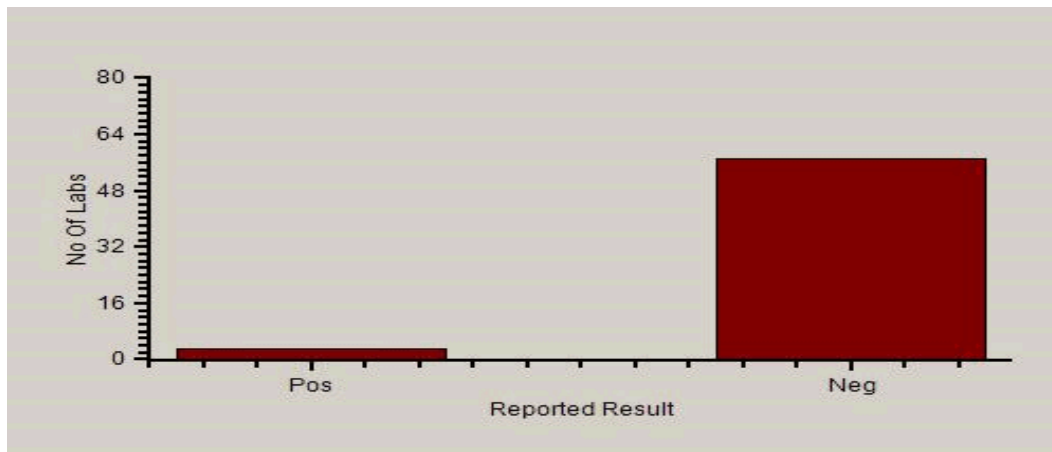

Reported Results Legends :-	
Pos	: Positive
Neg	: Negative

Comments :



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021


Qualitative Immunoassay,Widal test - ParaTyphi A-H antigen (AH), -

	N
 All Methods	71
 Slide Agglutination	49
 Manual	73

Your Result	No Agglutination
Result Expected	NoA

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

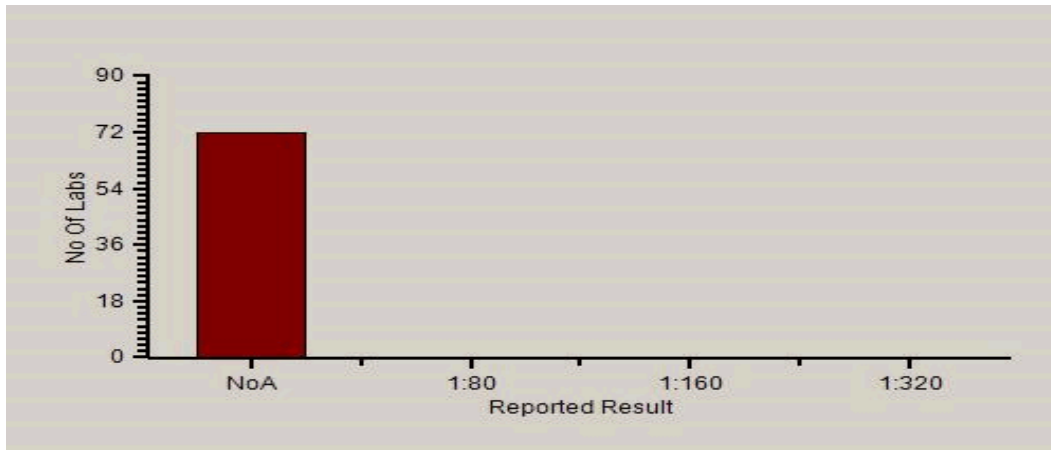

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021


Qualitative Immunoassay,Widal test - ParaTyphi B-H antigen (BH), -

	N
 All Methods	71
 Slide Agglutination	49
 Manual	73

Your Result	No Agglutination
Result Expected	NoA

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

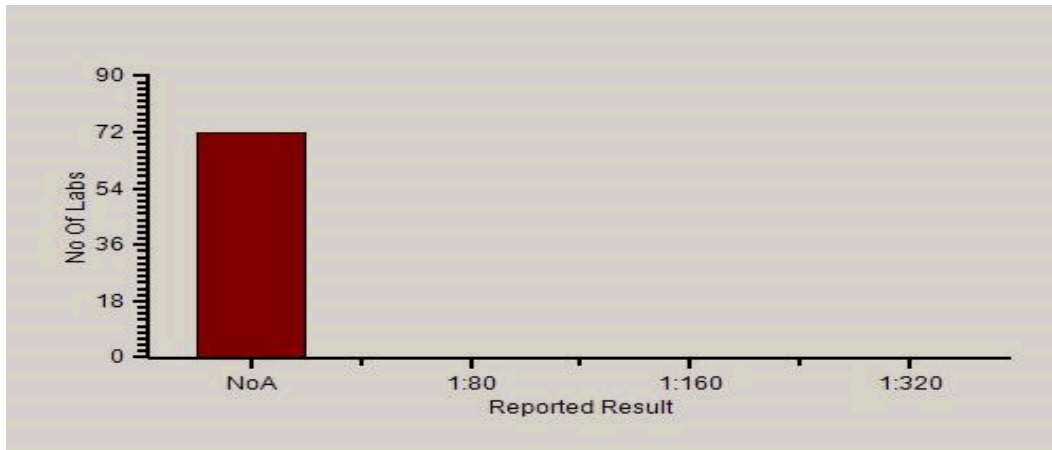

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021


Qualitative Immunoassay,Widal test - Typhi H antigen (TH), -

	N
 All Methods	81
 Slide Agglutination	56
 Manual	83

Your Result	No Agglutination
Result Expected	NoA

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

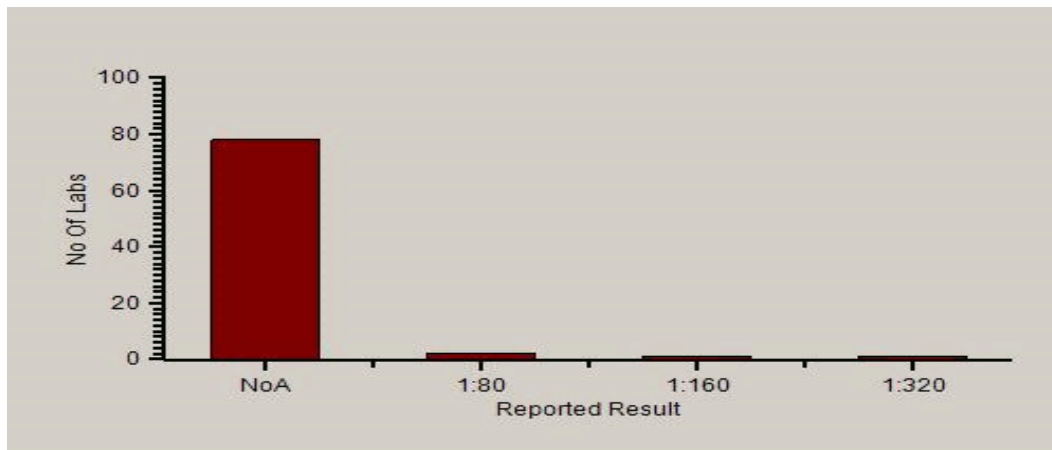

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error

- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 19/03/2021

Cycle No : 210103
 Sample No : 2
 Sample Date : 03-03-2021


Qualitative Immunoassay,Widal test - Typhi O antigen (TO), -

	N
 All Methods	81
 Slide Agglutination	56
 Manual	83

Your Result	No Agglutination
Result Expected	NoA

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

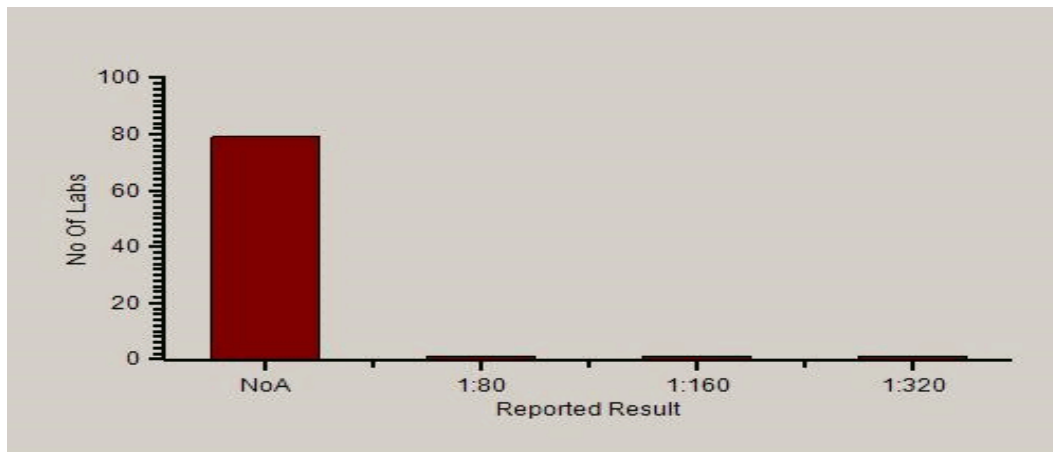

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 2
Sample Date : 03-03-2021

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS

Unit No. 409-416,
Commercial Building - 1A,
Kohinoor Mall, Kiroi Road, Kurla (W),
Mumbai - 400070

