

**TEST & CALIBRATION CERTIFICATE**

UNIT DESCRIPTION: MICRO PIPETTE

COMPANY: VERTEX

RANGE: 100-1000µl

NAME OF CUSTOMER  
& ADDRESS:

ABIRAMI KIDNEY CARE

NO:580, 581, BROUGH ROAD,

NEAR RAVI THEATRE,

ERODE-638 011.

PIPETTE SERVICE: PREVENTIVE MAINTENANCE DONESERVICE: OKCALIBRATION: OKINSTRUMENT WORKING CONDITION: GOOD


CALIBRATION DATE: 25.03.2021

CALIBRATION VALIDITY: 24.03.2022

DATE: 25.03.2021

TEST BY: G. DINESH

APPROVED BY: QA.

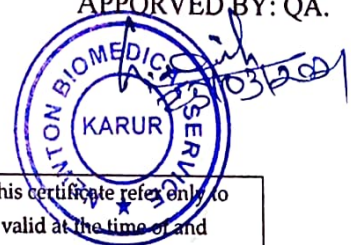

NOTE: 1) Calibration Points & due date is given as per customer request 2) This certificate refer only to particular item submitted for certificate 3) The calibration results reported are valid at the time of and under the stated conditions of the measurements 4) Any error in the certificate should be brought to our lab within 45 days from the date of issue of certificate.

# NEWTON



## BIOMEDICAL SERVICE

GSTIN : 33AAOFN5502A1ZR

CUSTOMER ADDRESS: M/S. ABIRAMI KIDNEY CARE

NO: 580, 581, BROUGH ROAD,

NEAR RAVI THEATRE,

ERODE-638 011.

	DISCIPLINE	:	MECHANICAL CALIBRATION		
NAME OF EQUIPMENT:	MICROPIPETTE	PARAMETER	:	VOLUME	
CERTIFICATE NO	:	NBS210847251	DATE OF ISSUE	:	25-03.2021
RECEIPT NO	:	10136	TEMPERATURE	:	24.5 <sup>0</sup> C
RECEIPT DATE	:	25-03-2021	HUMIDITY	:	53%
JOB CARD NO	:	TPM000	AIR PRESURE	:	959hpa
JOB CARD DATE	:	25-03-2021	MEDIUM OF WEIGHING	:	GRADE III WATER
			DENSITY OF MEDIUM	:	APPROXIMATELY 1
RANGE	:	100-1000µl	DENSITY CORRECTION		
			FACTOR[Z]:	:	1.0037 µl/mg
TIPS USED	:	10-100µl	WEIGHING BALANCE	:	SEMI MICRO BALANCE
SCOPE ACCREDITATION: VOLUME-MICROPIPETTE (1µl-10000µl)					

