



MICROBIOLOGY DEPARTMENT, GRANT MEDICAL COLLEGE
SIR JJ GROUP OF HOSPITALS
BYCULLA, MUMBAI 400008, MAHARASHTRA, INDIA
Ph: 022-23712454/23710234/23735555 Ext: 2359/2276/2350

CERTIFICATE OF CALIBRATION

Date: 11.03.2022

Name of equipment: Refrigerator

Model/Serial No: RT EON 290 P34

Identification No: MDACS/FA/TRAUMA/ICTC/REFRIGERATOR/4(1)

Location: HIV Testing Laboratory

Range: 2-8 °C

Working range: 2-8 °C

Tolerance (if applicable): $\pm 1^{\circ}$ C

Manufacturer: GODREJ

Calibrated on: 11.03.2022

Next Calibration due on: 10.03.2022

Method of Calibration: In-house calibration done using calibrated thermometer (Make: Multi S/N: 2017041148)

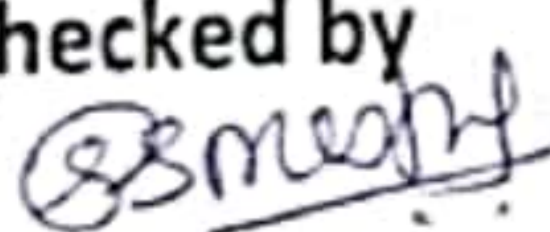
Traceability Certificate No: C2212185/T/11

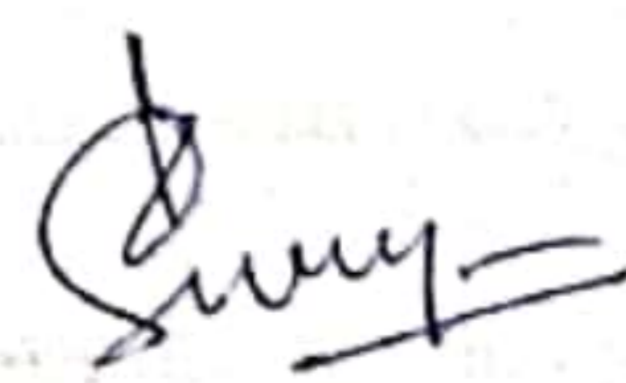
Test Conditions: Temperature: 27°C RH: 60%

Instrument	Readings (°C)					Mean
	1	2	3	4	5	
Master Thermometer	5.0	4.8	4.9	4.5	4.8	4.8
Laboratory Thermometer	5.1	5.0	5.0	4.8	4.9	4.96

Acceptable Variation $\pm 1^{\circ}$ C of the mean master thermometer reading

Remarks: Instrument has passed the acceptance criteria

Checked by

Shivani Mestry
SRL Technical Officer
SRL JJH.


Verified by
Assistant Professor
Department of Microbiology
Grant Government Medical,
College & Sir J. J. Group of
Hospitals, Mumbai - 400 008.



MICROBIOLOGY DEPARTMENT, GRANT MEDICAL COLLEGE
SIR JJ GROUP OF HOSPITALS
BYCULLA, MUMBAI 400008, MAHARASHTRA, INDIA
Ph: 022-23712454/23710234/23735555 Ext: 2359/2270/2350

CERTIFICATE OF CALIBRATION

Date: 11.03.2022

Name of equipment: Refrigerator

Model/Serial No: GL T302RP ZU/ 2020

Identification No: MDACS/FA/TRAUMA/ICTC/REFRIGERATOR/4-(2)

Location: HIV Testing Laboratory

Range: 2-8 °C

Working range: 2-8 °C

Tolerance (if applicable): $\pm 1^{\circ}$ C

Manufacturer: LG

Calibrated on: 11.03.2022

Next Calibration due on: 10.03.2022

Method of Calibration: In-house calibration done using calibrated thermometer (Make: Multi S/N: 2017041148)

Traceability Certificate No: C2212185/T/11

Test Conditions:

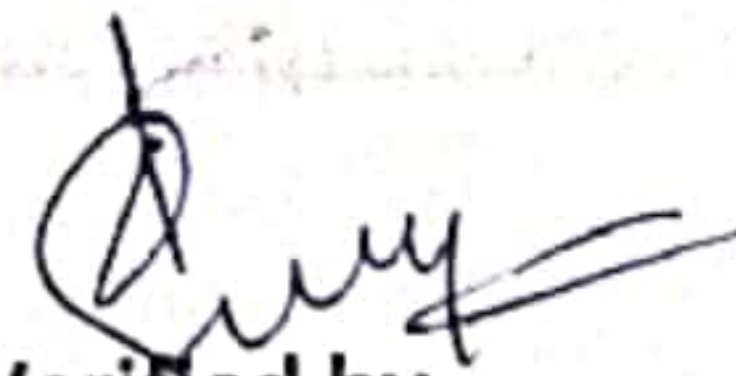
Temperature: 27°C

RH: 60%

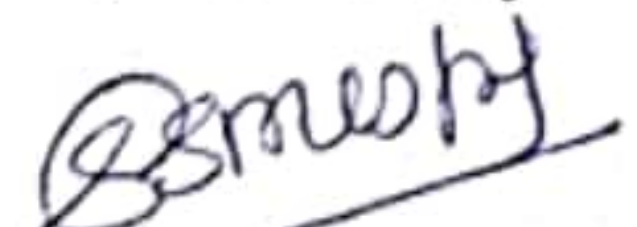
Instrument	Readings (°C)					Mean
	1	2	3	4	5	
Master Thermometer	4.0	4.0	4.0	4.0	5.0	4.2
Laboratory Thermometer	4.5	4.2	4.7	4.1	4.5	4.4

Acceptable Variation $\pm 1^{\circ}$ C of the mean master thermometer reading

Remarks: Instrument has passed the acceptance criteria


Verified by

Checked by



Shivani Mestry
SRL Technical Officer
SRL JJH

Assistant Professor
Department of Microbiology
Grant Government Medical,
College & Sir J. J. Group of
Hospitals, Mumbai - 400 008.



MICROBIOLOGY DEPARTMENT, GRANT MEDICAL COLLEGE
SIR JJ GROUP OF HOSPITALS
BYCULLA, MUMBAI 400008, MAHARASHTRA, INDIA
Ph: 022-23712454/23710234/23735555 Ext: 2359/2276/2350

CERTIFICATE OF CALIBRATION

Date: 11.03.2022

Name of equipment: Refrigerator

Model/Serial No: GC-365/2008

Identification No: MDACS/FA/TRAUMA/ICTC/REFRIGERATOR/4-(3)

Location: HIV Testing Laboratory

Range: 2-8 °C

Working range: 2-8 °C

Tolerance (if applicable): $\pm 1^{\circ}$ C

Manufacturer: LG

Calibrated on: 11.03.2022

Next Calibration due on: 10.03.2022

Method of Calibration: In-house calibration done using calibrated thermometer (Make: Multi S/N: 2017041148)

Traceability Certificate No: C2212185/T/11

Test Conditions:

Temperature: 27°C

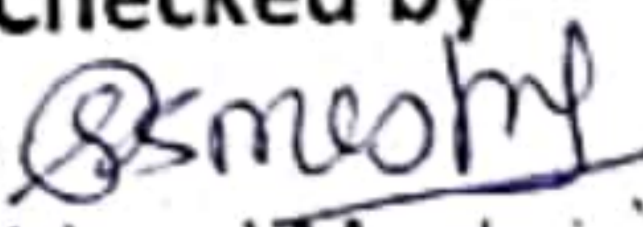
RH: 60%

Instrument	Readings (°C)					Mean
	1	2	3	4	5	
Master Thermometer	4.5	4.2	4.7	4.1	4.5	4.4
Laboratory Thermometer	4.9	4.8	4.9	3.9	4.8	4.66

Acceptable Variation $\pm 1^{\circ}$ C of the mean master thermometer reading

Remarks: Instrument has passed the acceptance criteria

Checked by


Shivani Mestry
SRL Technical Officer
SRL JJH



Verified by

Assistant Professor
Department of Microbiology
Grant Government Medical,
College & Sir J. J. Group of
Hospitals, Mumbai - 400 008.