

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 02/11/2021


Cycle No : 210410
 Sample No : 1
 Sample Date : 05-10-2021

Clinical Path - Urine Sediment Analysis Image,Other findings, -

| | |
|--|--|
| <p>■ All Methods</p> <p>■ -</p> <p>■ -</p> | <p>N</p> <p>38</p> <p>43</p> <p>43</p> |
|--|--|

| | |
|------------------------|--------------------------------|
| Your Result | Renal Tubular Epithelial Cells |
| Result Expected | RTC |

Note : # is an indication that this parameter has not been evaluated

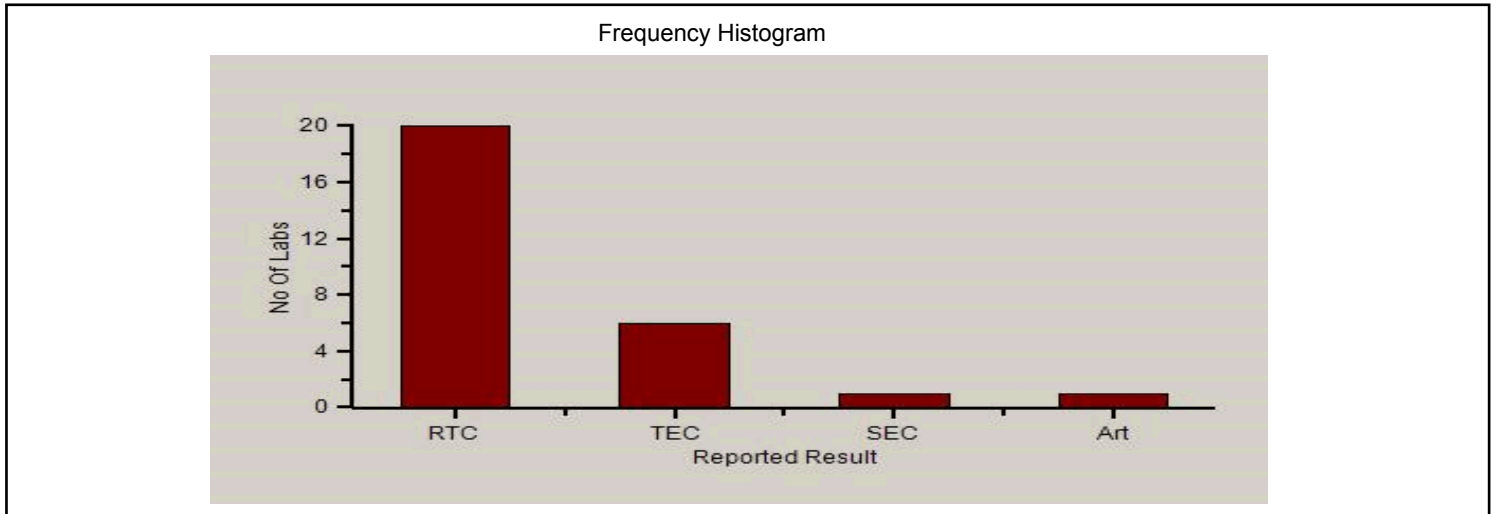

Analyte Methodwise Qualitative Result Report

Lab No.: 596
Lab Name : SYNERGEN DIAGNOSTICS
Report Date : 02/11/2021

Cycle No : 210410
Sample No : 1
Sample Date : 05-10-2021

Reported Results Legends :-

| | |
|------|----------------------------------|
| YC | : Yeast cells |
| RTC | : Renal Tubular Epithelial Cells |
| TEC | : Transitional Epithelial Cells |
| CaOx | : Calcium oxalate crystal |
| SEC | : Squamous Epithelial Cells |
| PC | : Pus cells present |
| RBC | : Red Blood Cells |
| None | : None |
| PC | : Pus cells |
| Art | : Artefact |

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance. Review for systematic error

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS

Unit No. 409-416.
Commercial Building - 1A,
Kohinoor Mall, Kiroli Road, Kurla (W),
Mumbai - 400070

