

Analyte Methodwise Qualitative Result Report

Lab No.: 596
Lab Name : SYNERGEN DIAGNOSTICS
Report Date : 30/12/2021

Cycle No : 210512
Sample No : 1
Sample Date : 11-12-2021


Qualitative Immunoassay, HBsAg, -

	N
All Methods	190
Immunochromatography	142
Manual	123

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

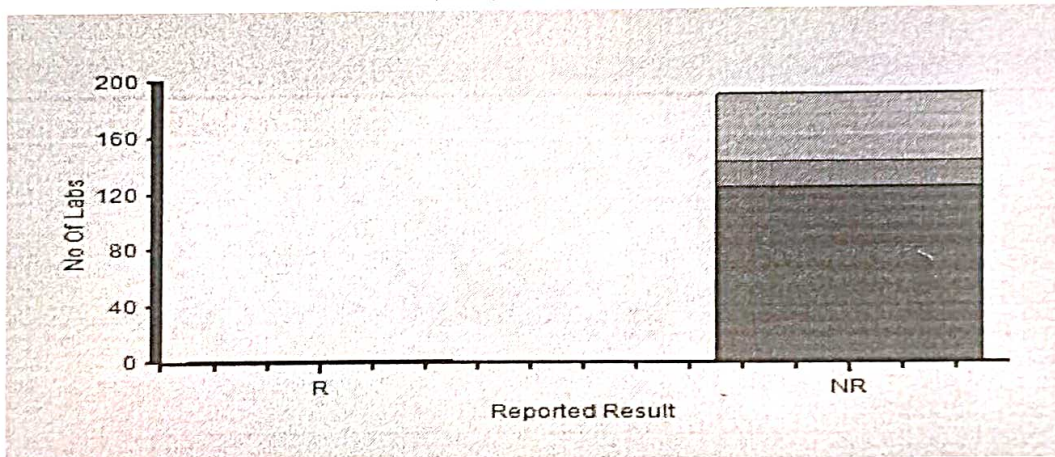

Reported Results Legends :-

R : Reactive
NR : Non-reactive
Eq : Equivocal

Comments :



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
Lab Name : SYNERGEN DIAGNOSTICS
Report Date : 30/12/2021

Cycle No : 210512
Sample No : 1
Sample Date : 11-12-2021

Interpretation when an analyte is reported for multiple samples in a Round.

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021


Qualitative Immunoassay,HCV, -

	N
<input type="checkbox"/> All Methods	148
<input type="checkbox"/> Immunochromatography	103
<input type="checkbox"/> Manual	92

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

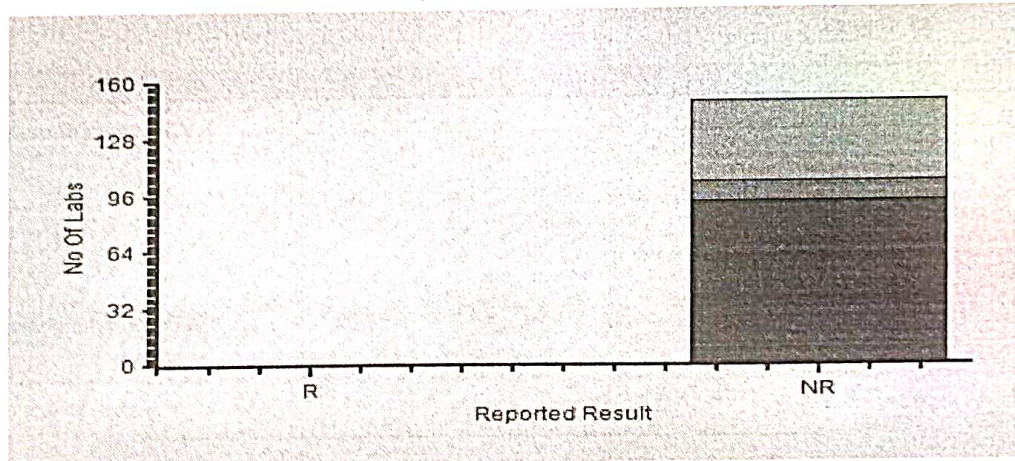

Reported Results Legends :-

R : Reactive
 NR : Non-reactive
 Eq : Equivocal

Comments :



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
Lab Name : SYNERGEN DIAGNOSTICS
Report Date : 30/12/2021

Cycle No : 210512
Sample No : 1
Sample Date : 11-12-2021

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021


Qualitative Immunoassay, HIV Ab, -

	N
All Methods	107
Immunochromatography	100
Manual	93

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

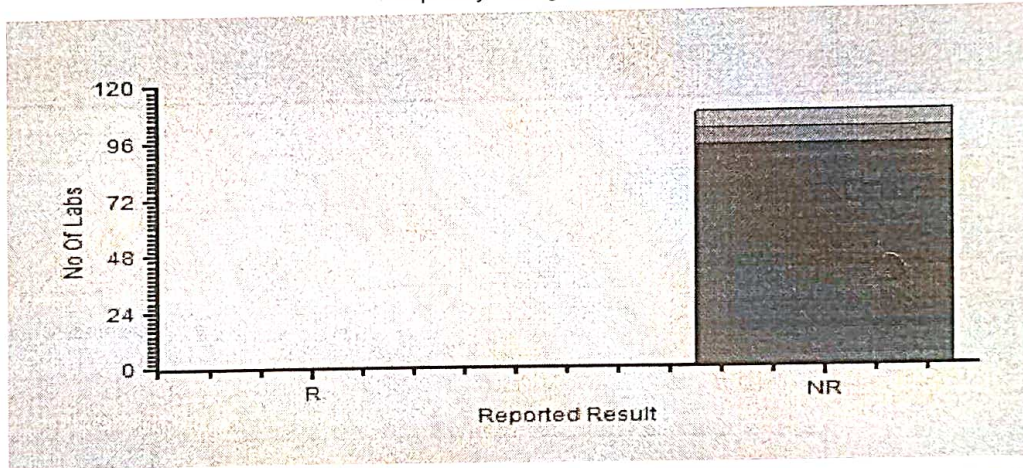

Reported Results Legends :-

- R : Reactive
- NR : Non-reactive
- Eq : Equivocal
- Indet : Indeterminate
- HIV-1 : HIV-1 Ab Reactive
- HIV-2 : HIV-2 Ab Reactive



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
Lab Name : SYNERGEN DIAGNOSTICS
Report Date : 30/12/2021

Cycle No : 210512
Sample No : 1
Sample Date : 11-12-2021

Comments :

Interpretation when an analyte is reported for multiple samples in a Round

- a) Reported on 2 samples
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance. Review for systematic error
- b) Reported on 3 samples
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance. Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021


Qualitative Immunoassay,RPR (Syphilis Serology), -

	N
All Methods	159
Agglutination	65
Manual	159

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

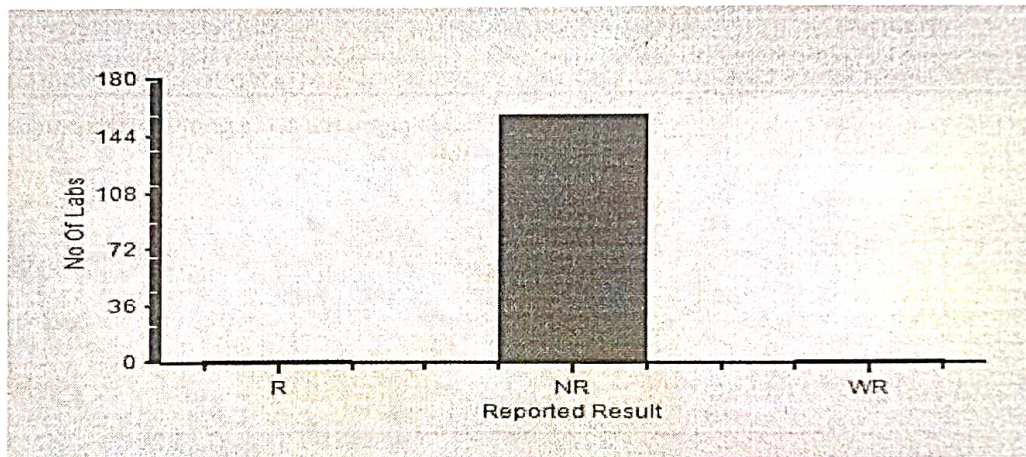

Reported Results Legends :-

- R : Reactive
- NR : Non-reactive
- WR : Weak Reactive

Comments :



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
Lab Name : SYNERGEN DIAGNOSTICS
Report Date : 30/12/2021

Cycle No : 210512
Sample No : 1
Sample Date : 11-12-2021

Interpretation when an analyte is reported for multiple samples in a Round

a) Reported on 2 samples

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance. Review for systematic error

b) Reported on 3 samples

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance. Review for systematic error
- All failed - Unacceptable performance. Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 2
 Sample Date : 11-12-2021


Qualitative Immunoassay,HBsAg, -

	N
All Methods	185
Immunochromatography	137
Manual	119

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

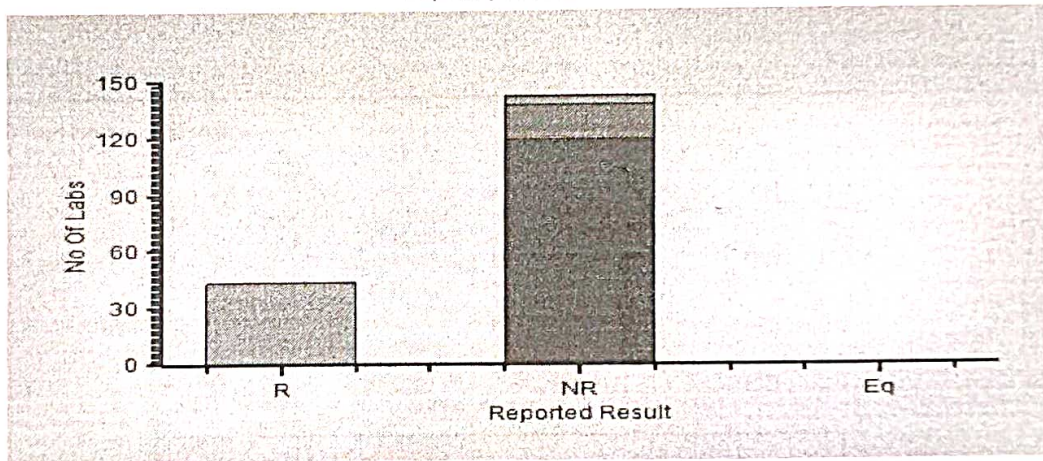

Reported Results Legends :-

R : Reactive
 NR : Non-reactive
 Eq : Equivocal

Comments :



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596

Lab Name : SYNERGEN DIAGNOSTICS

Report Date : 30/12/2021

Cycle No : 210512

Sample No : 2

Sample Date : 11-12-2021

Interpretation when an analyte is reported for multiple samples in a Round

a) Reported on 2 samples

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 2
 Sample Date : 11-12-2021


Qualitative Immunoassay,HCV, -

	N
All Methods	145
Immunochromatography	100
Manual	90

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

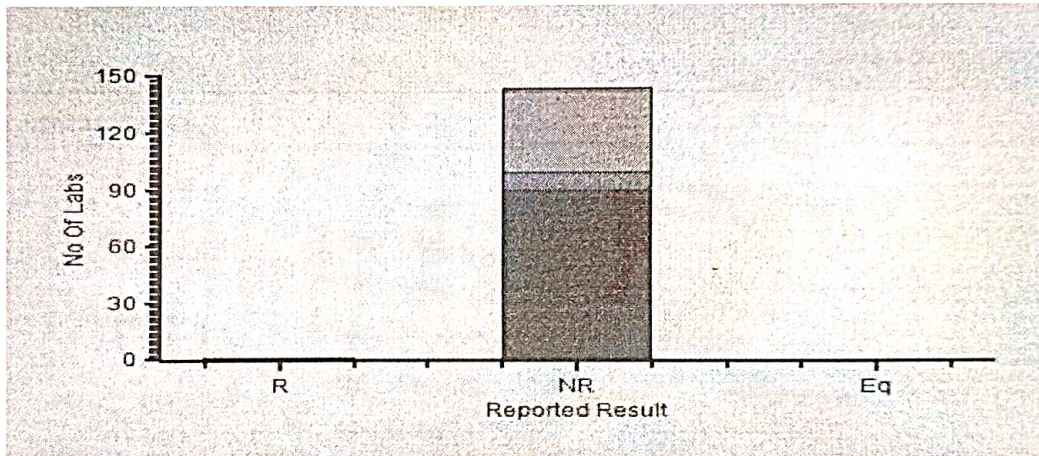

Reported Results Legends :-

R	: Reactive
NR	: Non-reactive
Eq	: Equivocal

Comments :



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
Lab Name : SYNERGEN DIAGNOSTICS
Report Date : 30/12/2021

Cycle No : 210512
Sample No : 2
Sample Date : 11-12-2021

Interpretation when an analyte is reported for multiple samples in a Round

- a) Reported on 2 samples
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance. Review for systematic error
- b) Reported on 3 samples
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance. Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
Lab Name : SYNERGEN DIAGNOSTICS
Report Date : 30/12/2021

Cycle No : 210512
Sample No : 2
Sample Date : 11-12-2021


Qualitative Immunoassay, HIV Ab, -

	N
All Methods	102
Immunochromatography	98
Manual	90

Your Result	HIV-1 Ab Reactive
Result Expected	HIV-1

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

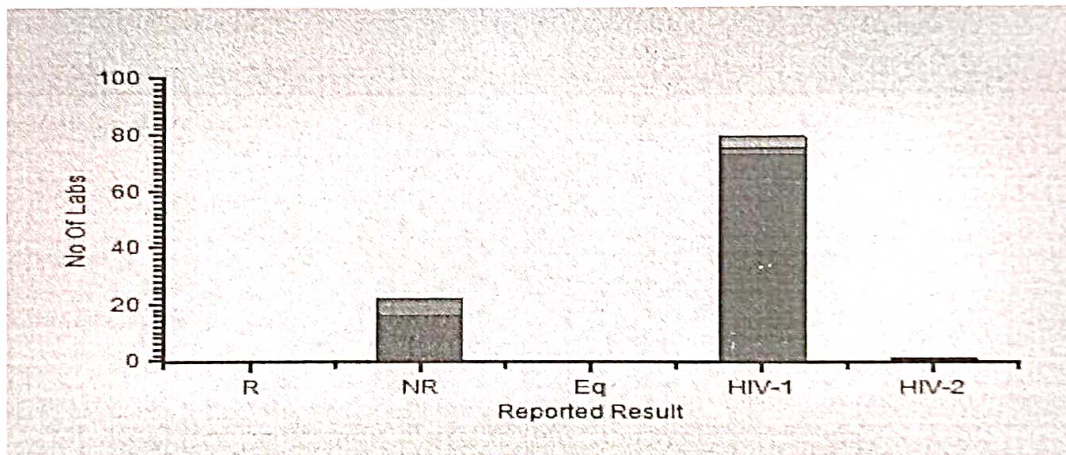

Reported Results Legends :-

R	: Reactive
NR	: Non-reactive
Eq	: Equivocal
Indet	: Indeterminate
HIV-1	: HIV-1 Ab Reactive
HIV-2	: HIV-2 Ab Reactive



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
Lab Name : SYNERGEN DIAGNOSTICS
Report Date : 30/12/2021

Cycle No : 210512
Sample No : 2
Sample Date : 11-12-2021

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 2
 Sample Date : 11-12-2021


Qualitative Immunoassay,RPR (Syphilis Serology), -

	N
■ All Methods	155
■ Agglutination	63
■ Manual	155

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

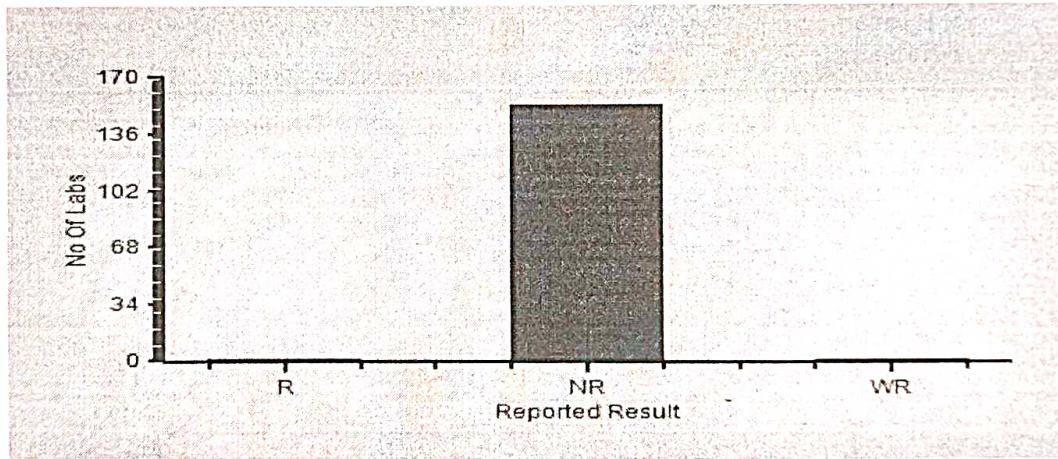

Reported Results Legends :-	
R	: Reactive
NR	: Non-reactive
WR	: Weak Reactive

Comments :



Analyte Methodwise Qualitative Result Report

Lab No.: 596

Lab Name : SYNERGEN DIAGNOSTICS

Report Date : 30/12/2021

Cycle No : 210512

Sample No : 2

Sample Date : 11-12-2021

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance. Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance. Review for systematic error
- All failed - Unacceptable performance. Review for systematic error

