

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 02/11/2021

Cycle No : 210410
 Sample No : 1
 Sample Date : 05-10-2021


Clinical Path - Urine Routine Chemistry,Blood (urine), -

	N
█ All Methods	27
█ Photoelectric colorimetry - (Your Method)	2
█ Urometer 120 - (Your Analyzer)	1

Your Result	3+
Result Expected	+1,+2,+3,+4

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

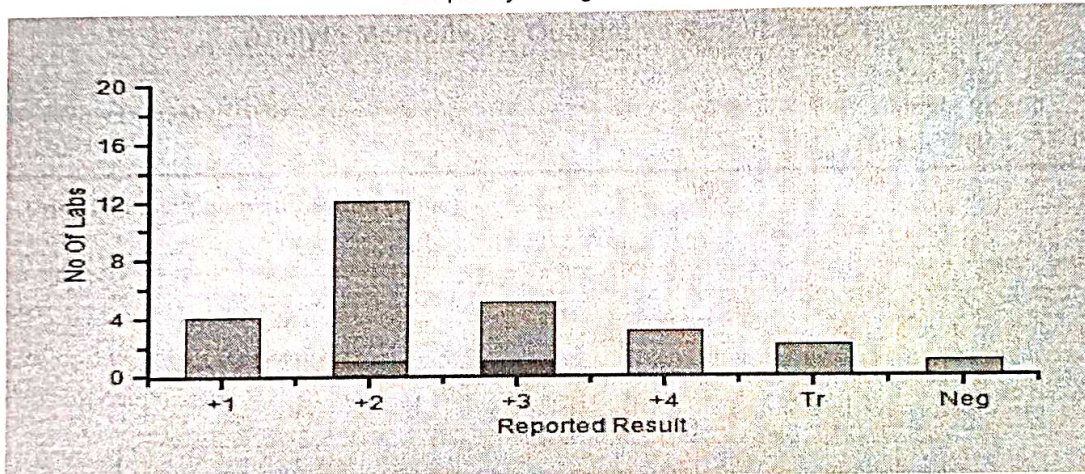

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 02/11/2021

Cycle No : 210410
 Sample No : 1
 Sample Date : 05-10-2021

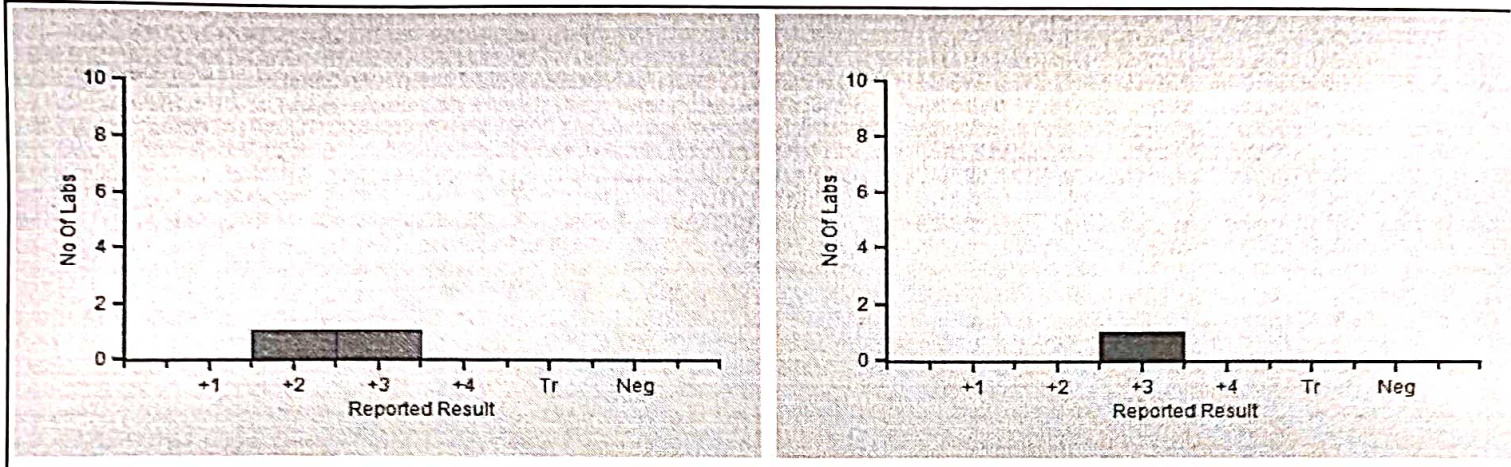

Reported Results Legends :-

+1	: 1+
+2	: 2+
+3	: 3+
+4	: 4+
Tr	: Trace
Neg	: Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 02/11/2021

Cycle No : 210410
 Sample No : 1
 Sample Date : 05-10-2021


Clinical Path - Urine Routine Chemistry,Nitrite (urine), -

■ All Methods	N
■ Photoelectric colorimetry - (Your Method)	28
■ Urometer 120 - (Your Analyzer)	3
	1

Your Result	Absent
Result Expected	Abs

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

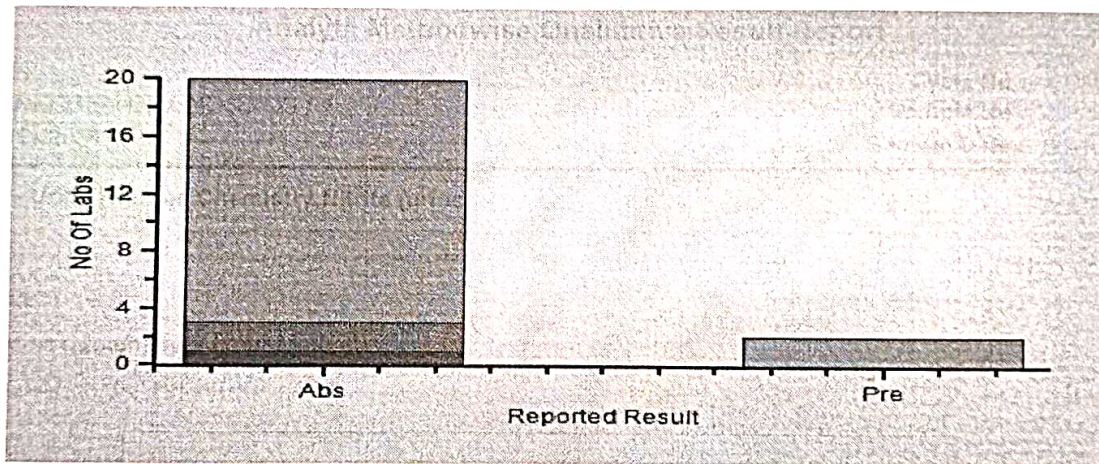

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 02/11/2021

Cycle No : 210410
 Sample No : 1
 Sample Date : 05-10-2021

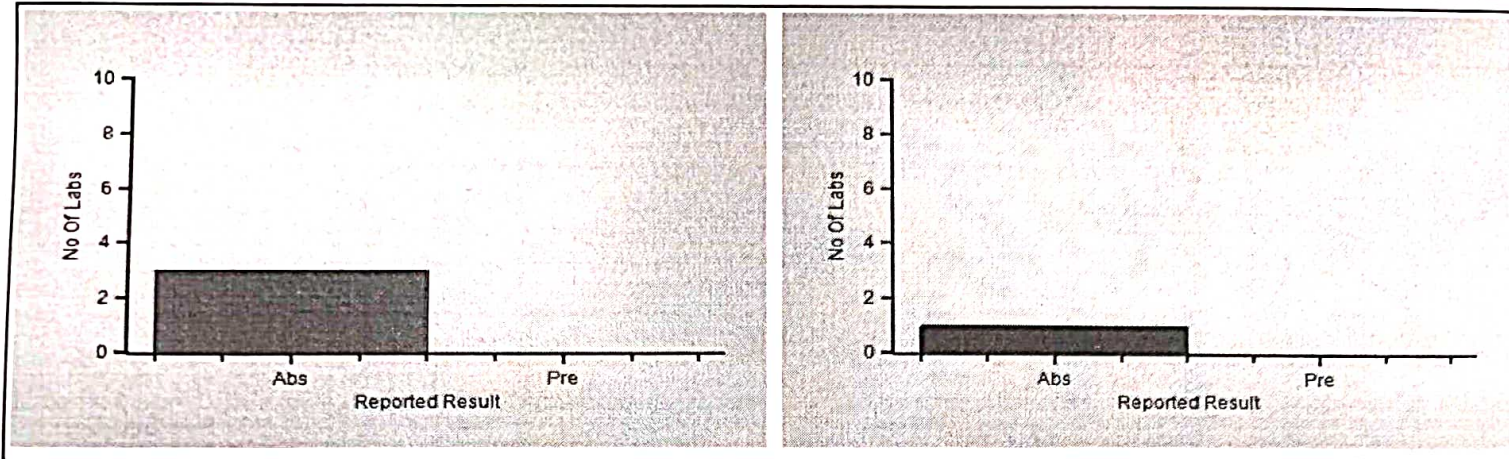

Reported Results Legends :-
 Abs : Absent
 Pre : Present

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



PC-1022