

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021


Clinical Path - Urine Routine Chemistry,Bilirubin (urine), -

| | N |
|---|-----|
| All Methods | 198 |
| Photoelectric colorimetry - (Your Method) | 3 |
| Urometer 120 - (Your Analyzer) | 1 |

| | |
|-----------------|----------|
| Your Result | Negative |
| Result Expected | Neg |

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

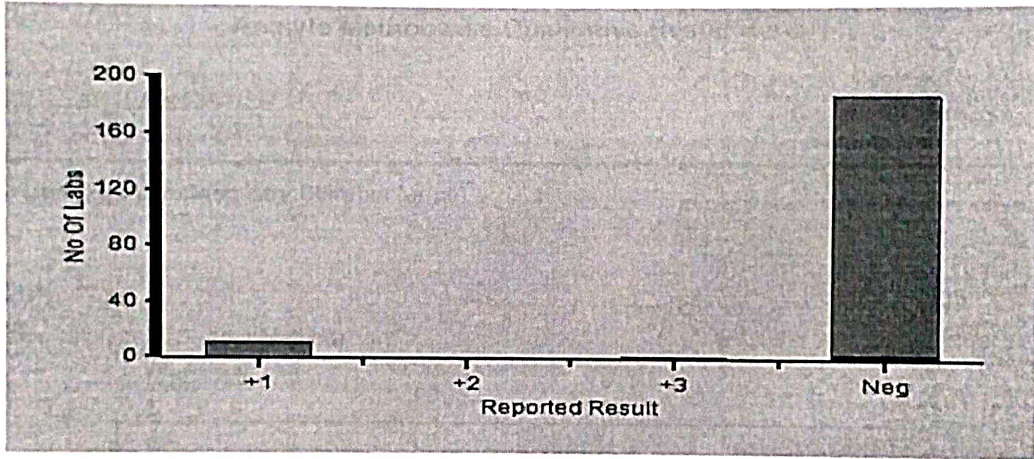


PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
Lab Name : SYNERGEN DIAGNOSTICS
Report Date : 30/12/2021

Cycle No : 210512
Sample No : 1
Sample Date : 11-12-2021

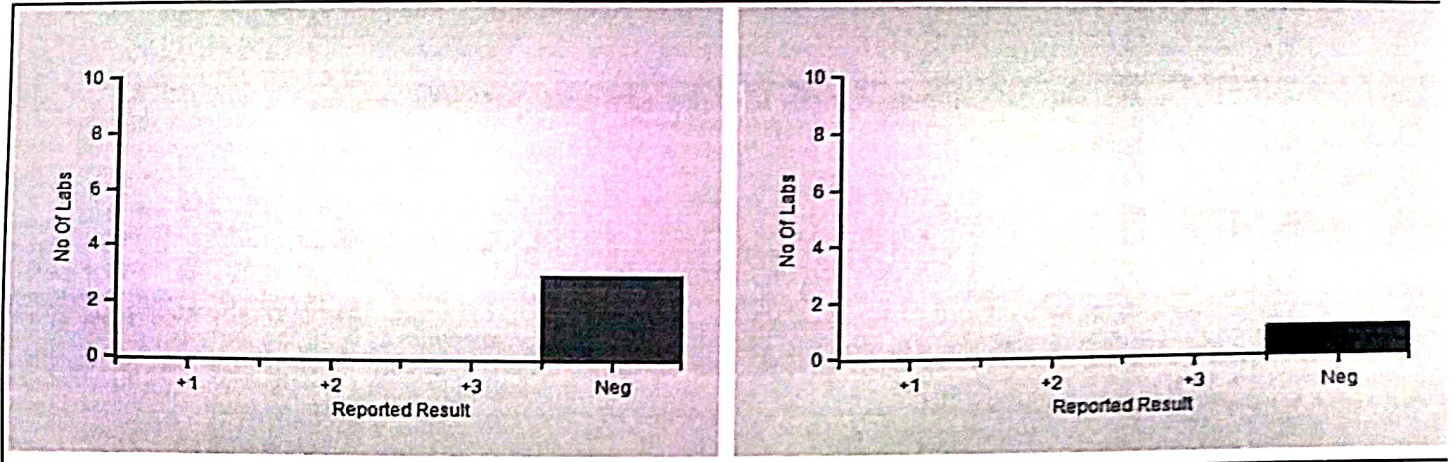

Reported Results Legends :-

| | |
|-----|------------|
| +1 | : 1+ |
| +2 | : 2+ |
| +3 | : 3+ |
| Neg | : Negative |

Comments :

Interpretation when an analyte is reported for multiple samples in a Round

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance. Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance. Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021


Clinical Path - Urine Routine Chemistry,Blood (urine), -

| | |
|---|-----|
| ■ All Methods | N |
| ■ Photoelectric colorimetry - (Your Method) | 199 |
| ■ Urometer 120 - (Your Analyzer) | 3 |
| | 1 |

| | |
|-------------------|----|
| Your Result | 3+ |
| Result Expected # | # |

Note : # is an indication that this parameter has not been evaluated



Frequency Histogram

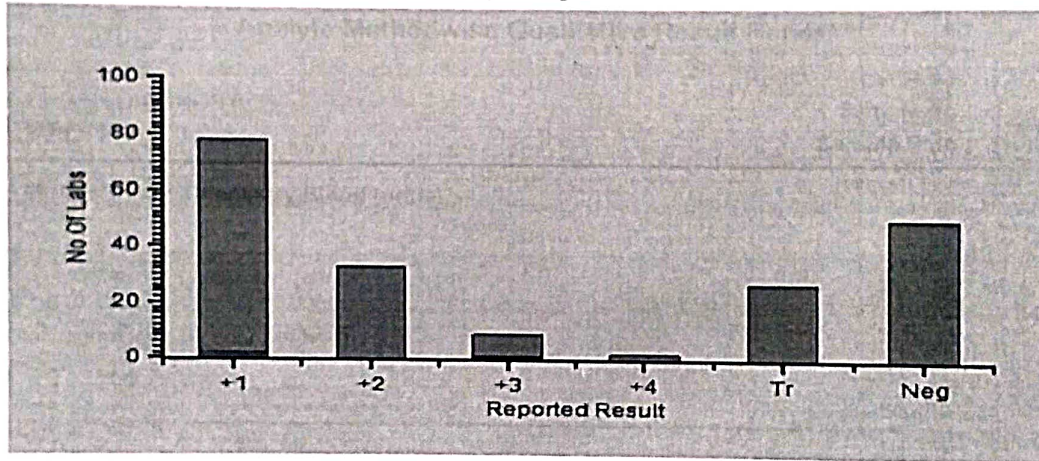

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021

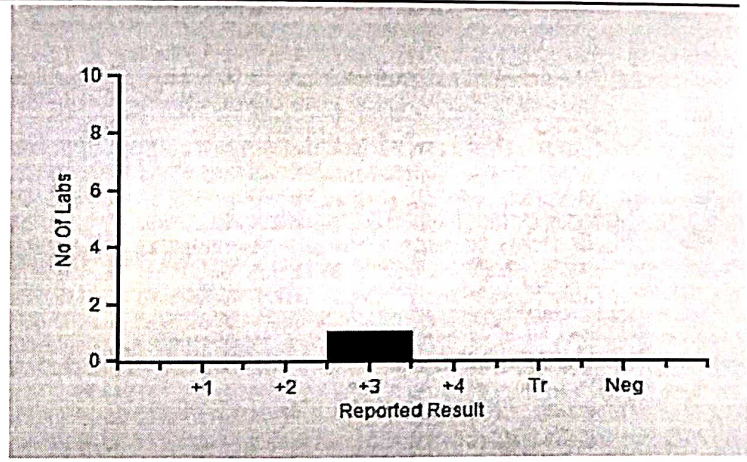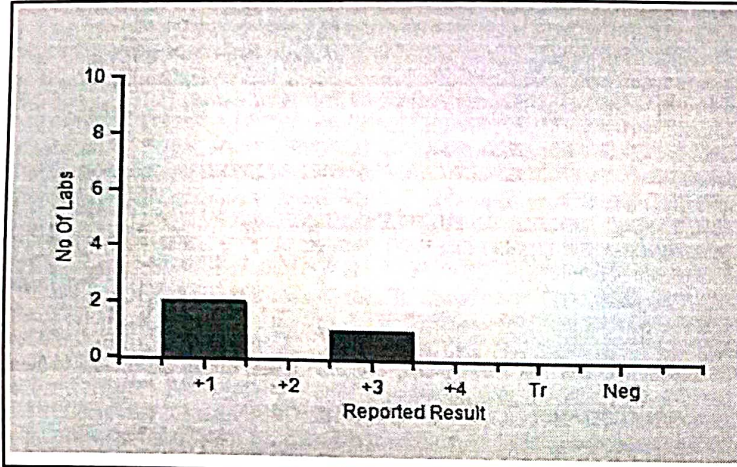

Reported Results Legends :-

| | |
|-----|------------|
| +1 | : 1+ |
| +2 | : 2+ |
| +3 | : 3+ |
| +4 | : 4+ |
| Tr | : Trace |
| Neg | : Negative |

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021


Clinical Path - Urine Routine Chemistry, Glucose (urine), -

| | |
|---|-----|
| ■ All Methods | N |
| ■ Photoelectric colorimetry - (Your Method) | 211 |
| ■ Urometer 120 - (Your Analyzer) | 3 |
| | 1 |

| | |
|-----------------|----------|
| Your Result | 4+ |
| Result Expected | +2,+3,+4 |

Note : # is an indication that this parameter has not been evaluated



Frequency Histogram

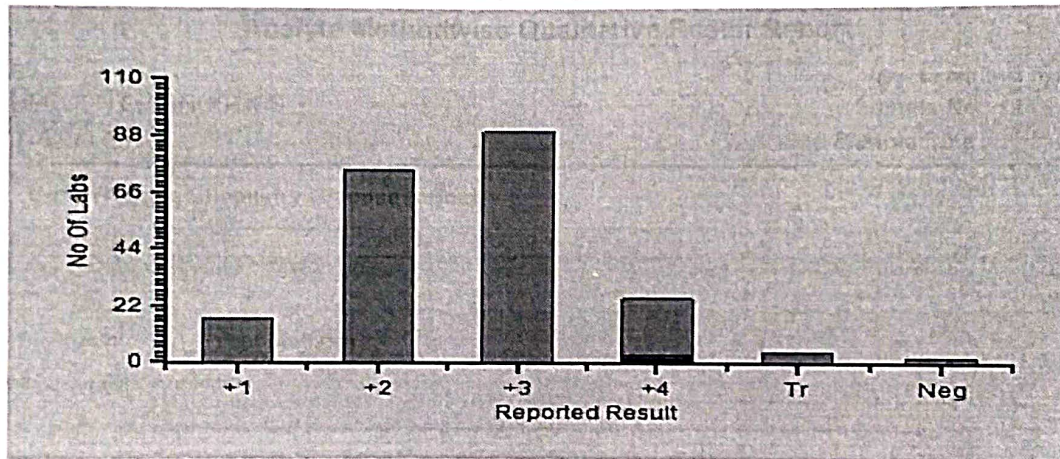

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021

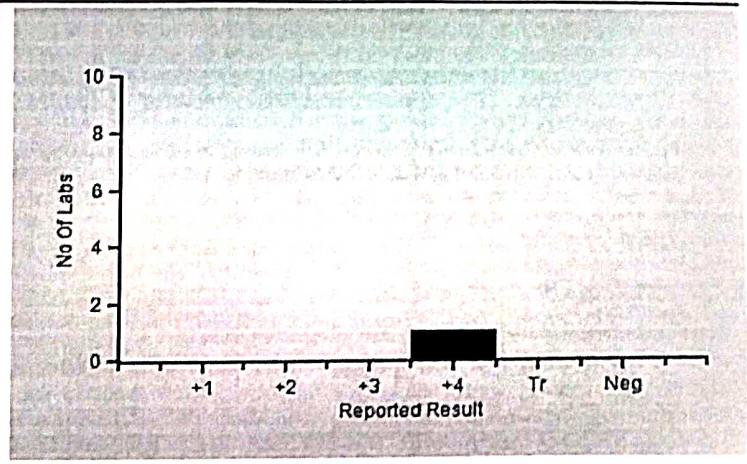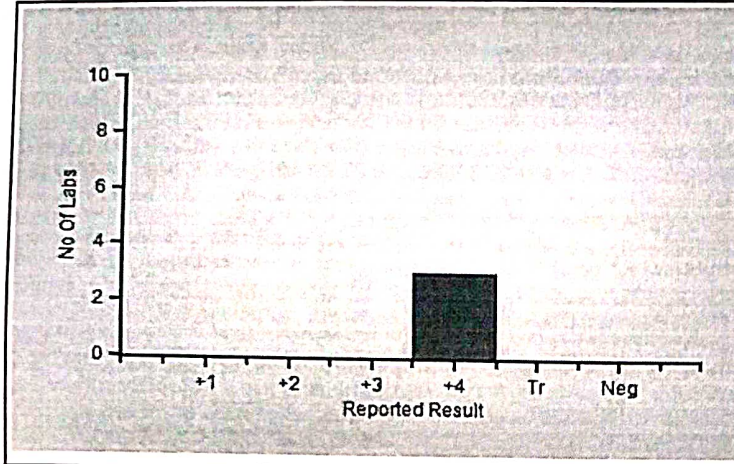

Reported Results Legends :-

| | |
|-----|------------|
| +1 | : 1+ |
| +2 | : 2+ |
| +3 | : 3+ |
| +4 | : 4+ |
| Tr | : Trace |
| Neg | : Negative |

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021


Clinical Path - Urine Routine Chemistry, Ketone (urine), -

| | |
|--|-----|
| <input type="checkbox"/> All Methods | N |
| <input type="checkbox"/> Photoelectric colorimetry - (Your Method) | 203 |
| <input type="checkbox"/> Urometer 120 - (Your Analyzer) | 3 |
| | 1 |

| | |
|------------------------|----------|
| Your Result | Negative |
| Result Expected | Neg |

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram


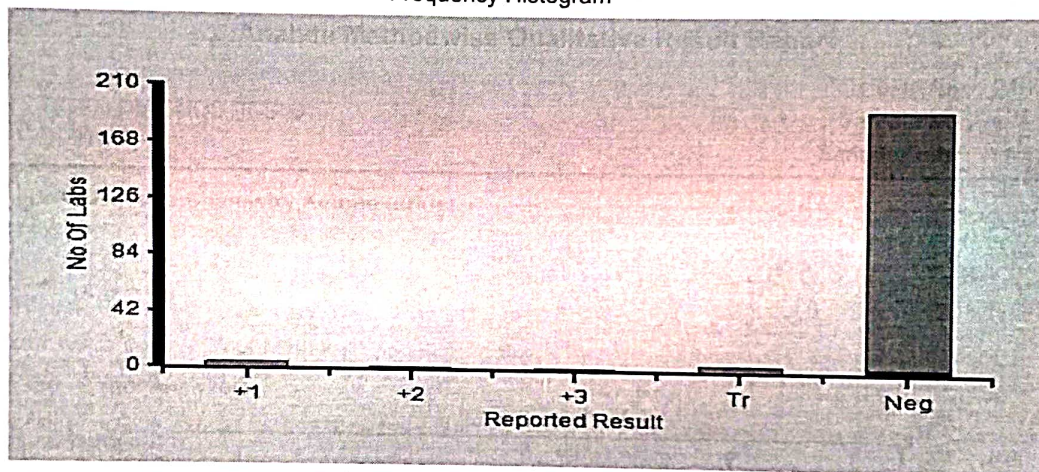


PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021

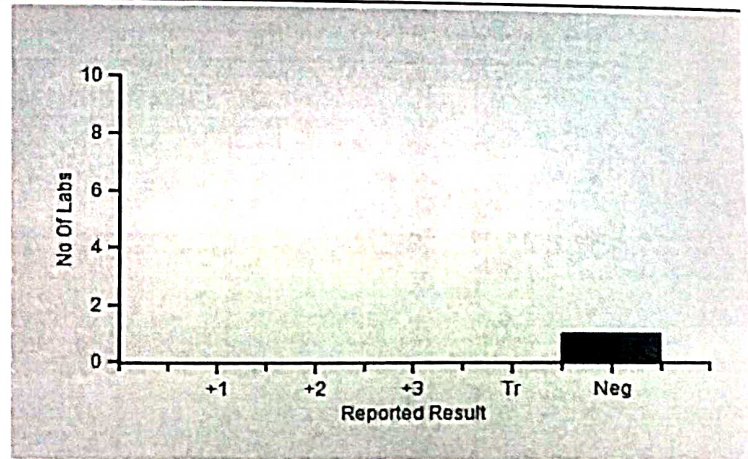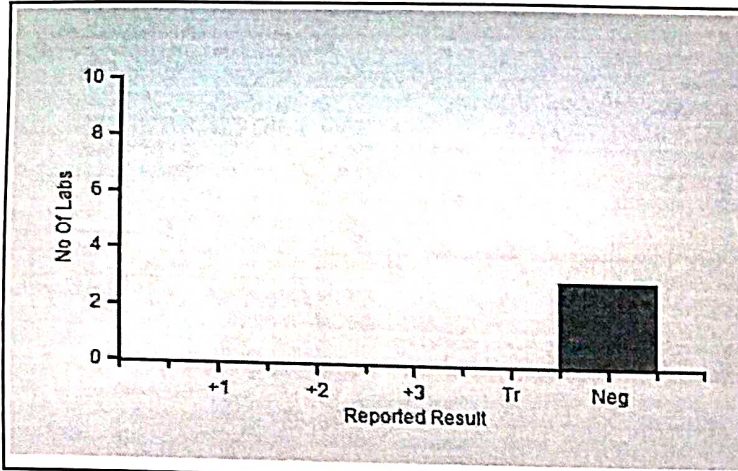

Reported Results Legends :-

| | |
|-----|------------|
| +1 | : 1+ |
| +2 | : 2+ |
| +3 | : 3+ |
| Tr | : Trace |
| Neg | : Negative |

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021


Clinical Path - Urine Routine Chemistry,Nitrite (urine), -

| | |
|---|-----|
| ■ All Methods | N |
| ■ Photoelectric colorimetry - (Your Method) | 199 |
| ■ Urometer 120 - (Your Analyzer) | 6 |
| | 1 |

| | |
|-------------------|---------|
| Your Result | Present |
| Result Expected # | |

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram


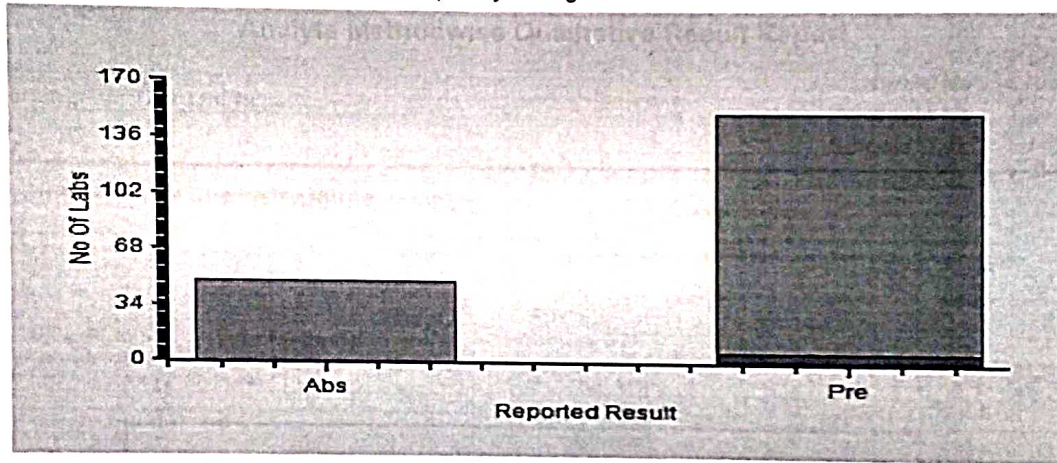


PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021

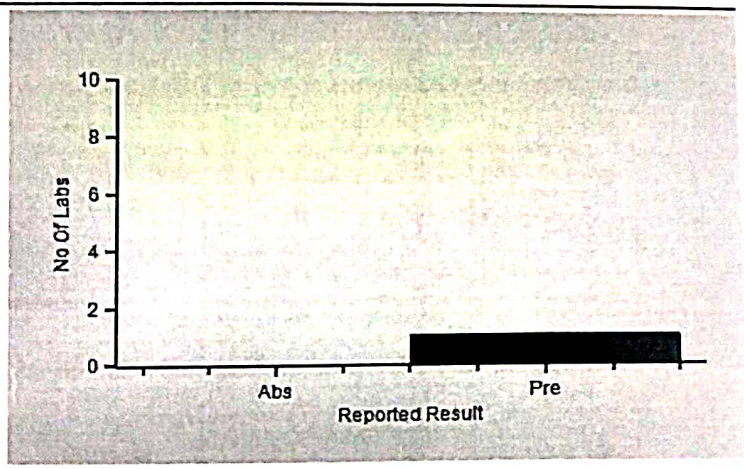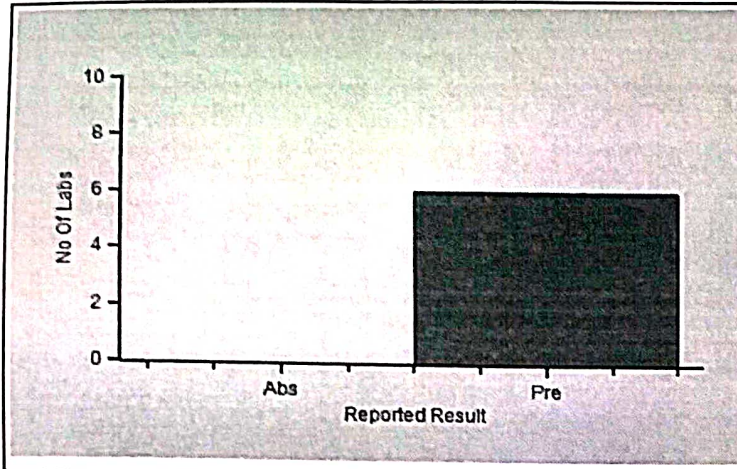

Reported Results Legends :-
 Abs : Absent
 Pre : Present

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



PG-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021


Clinical Path - Urine Routine Chemistry,pH, -

| | |
|---|-----|
| ■ All Methods | N |
| ■ Photoelectric colorimetry - (Your Method) | 207 |
| ■ Urometer 120 - (Your Analyzer) | 5 |
| | 1 |

| | |
|-----------------|-----------|
| Your Result | 6.5 |
| Result Expected | 5.5,6,6.5 |

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram


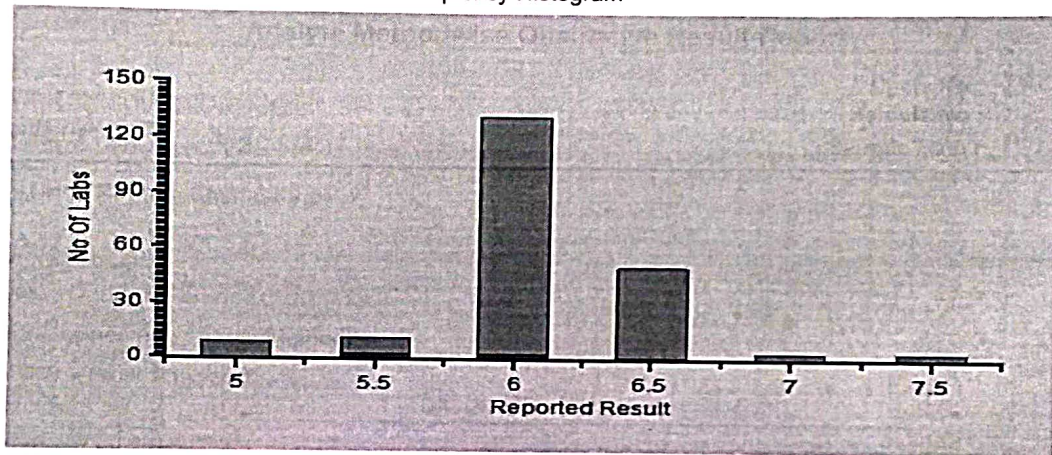


PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021

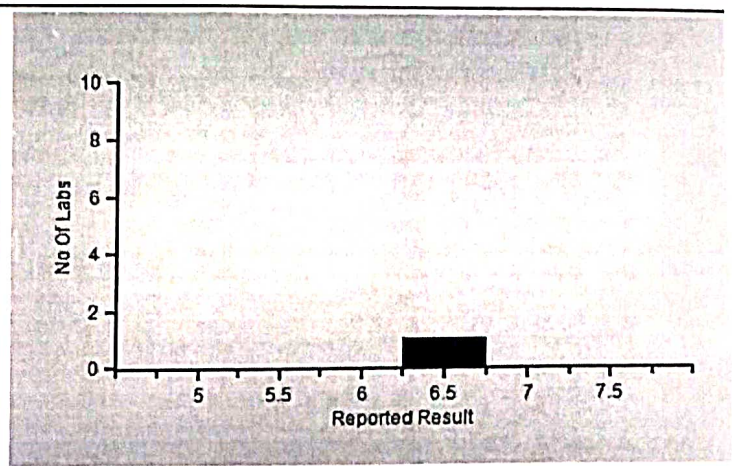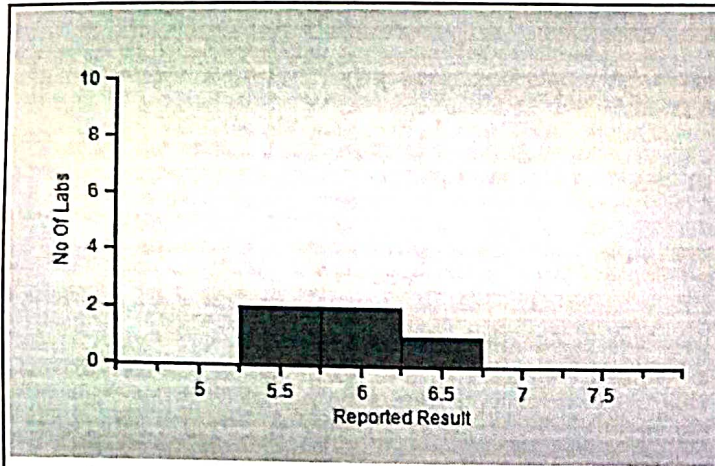

Reported Results Legends :-

| | |
|-----|-------|
| 5 | : 5 |
| 5.5 | : 5.5 |
| 6 | : 6 |
| 6.5 | : 6.5 |
| 7 | : 7 |
| 7.5 | : 7.5 |
| 8 | : 8 |
| 8.5 | : 8.5 |
| 9 | : 9 |

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021


Clinical Path - Urine Routine Chemistry, Protein (Urine), -

| | |
|---|-----|
| ■ All Methods | N |
| ■ Photoelectric colorimetry - (Your Method) | 209 |
| ■ Urometer 120 - (Your Analyzer) | 5 |
| | 1 |

| | |
|-----------------|----------|
| Your Result | Trace |
| Result Expected | +1,+2,Tr |

Note : # is an indication that this parameter has not been evaluated



Frequency Histogram

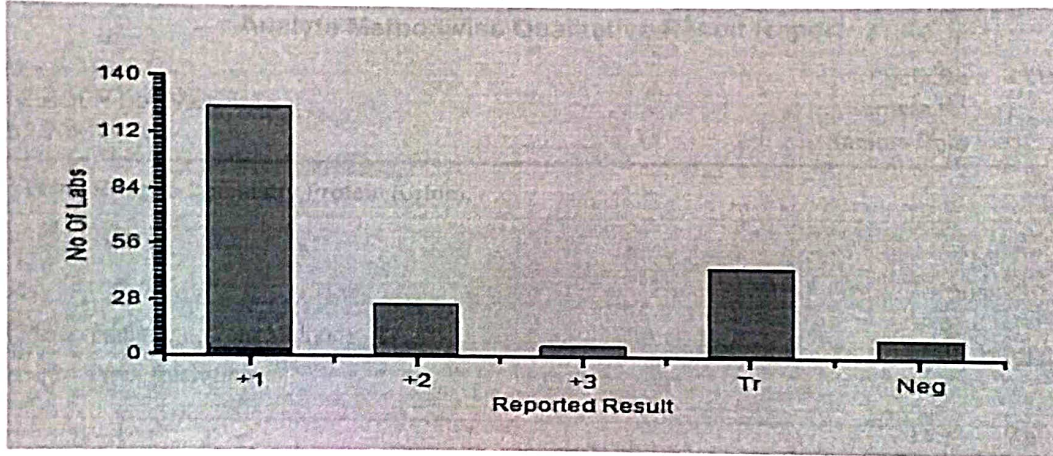

Analyte Methodwise Qualitative Result Report

Lab No.: 596
Lab Name : SYNERGEN DIAGNOSTICS
Report Date : 30/12/2021

Cycle No : 210512
Sample No : 1
Sample Date : 11-12-2021

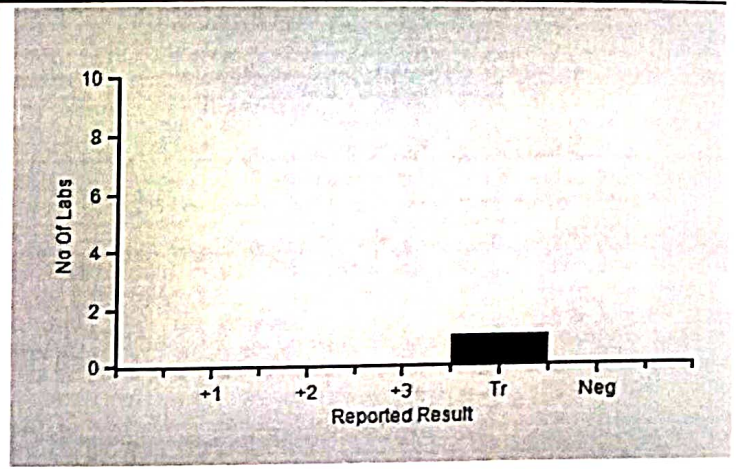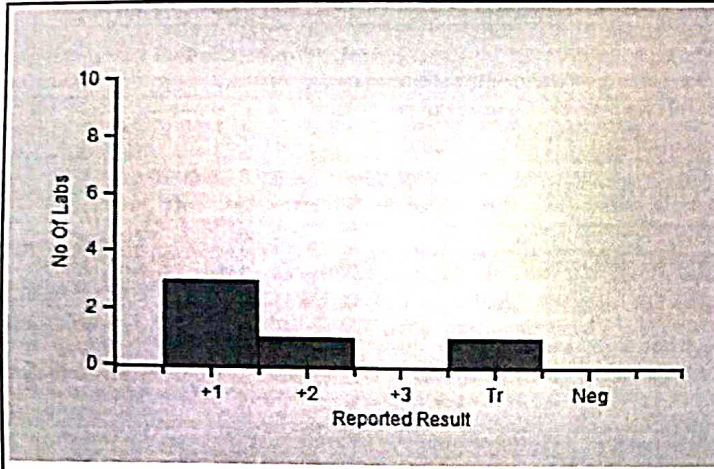

Reported Results Legends :-

| | |
|-----|------------|
| +1 | : 1+ |
| +2 | : 2+ |
| +3 | : 3+ |
| Tr | : Trace |
| Neg | : Negative |

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021


Clinical Path - Urine Routine Chemistry, Specific Gravity, -

| | |
|---|-----|
| ■ All Methods | N |
| ■ Photoelectric colorimetry - (Your Method) | 206 |
| ■ Urometer 120 - (Your Analyzer) | 3 |
| | 1 |

| | |
|-----------------|---------------------|
| Your Result | 1.015 |
| Result Expected | 1.015, 1.020, 1.025 |

Note : # is an indication that this parameter has not been evaluated



Frequency Histogram

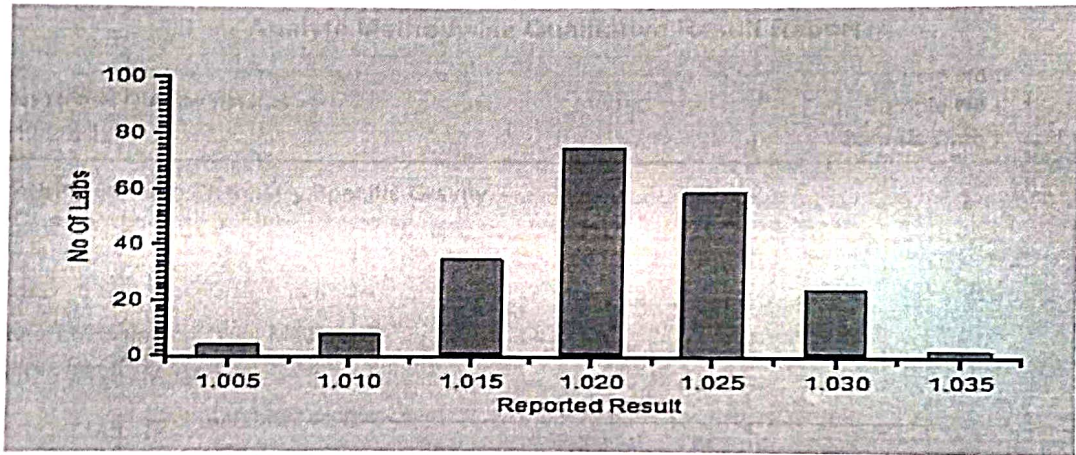

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021

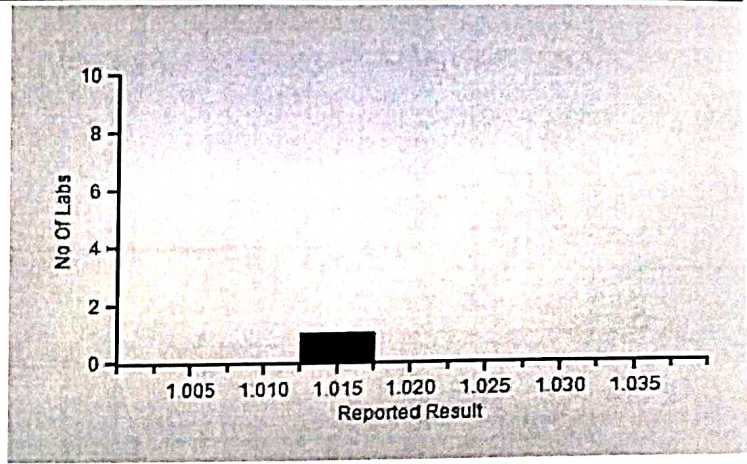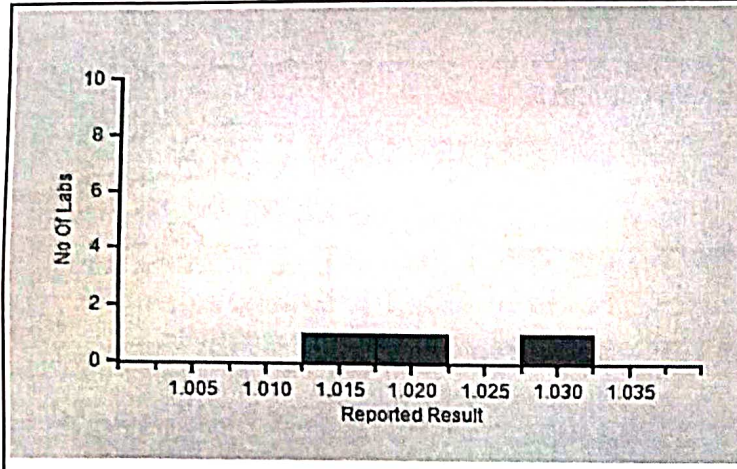

Reported Results Legends :-

| | |
|-------|---------|
| 1.005 | : 1.005 |
| 1.010 | : 1.010 |
| 1.015 | : 1.015 |
| 1.020 | : 1.020 |
| 1.025 | : 1.025 |
| 1.030 | : 1.030 |
| 1.035 | : 1.035 |

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021


Clinical Path - Urine Routine Chemistry,Urine Pregnancy Test, -

| | |
|--|----------|
| | N |
| ■ All Methods | 151 |
| ■ Immunochromatography - (Your Method) | 151 |
| ■ - - (Your Analyzer) | 149 |

| | |
|------------------------|----------|
| Your Result | Negative |
| Result Expected | Pos |

Note : # is an indication that this parameter has not been evaluated



Frequency Histogram

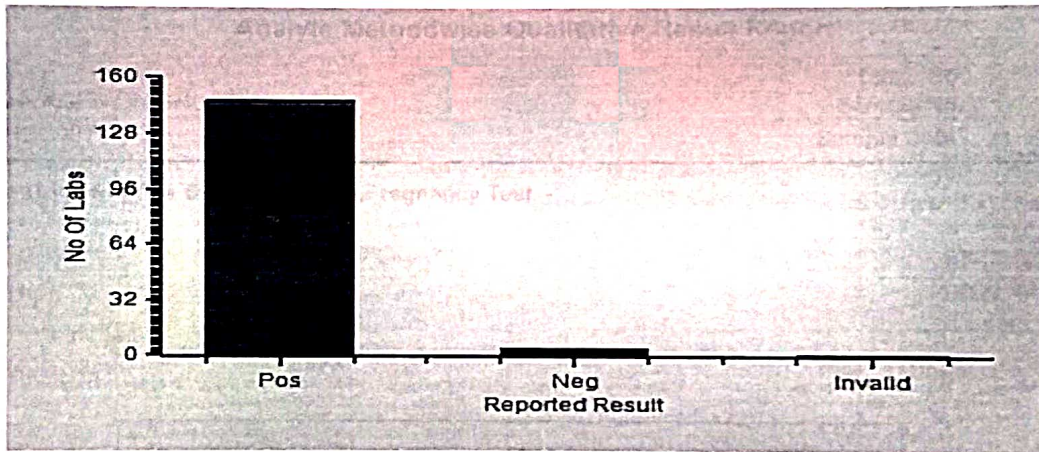

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021

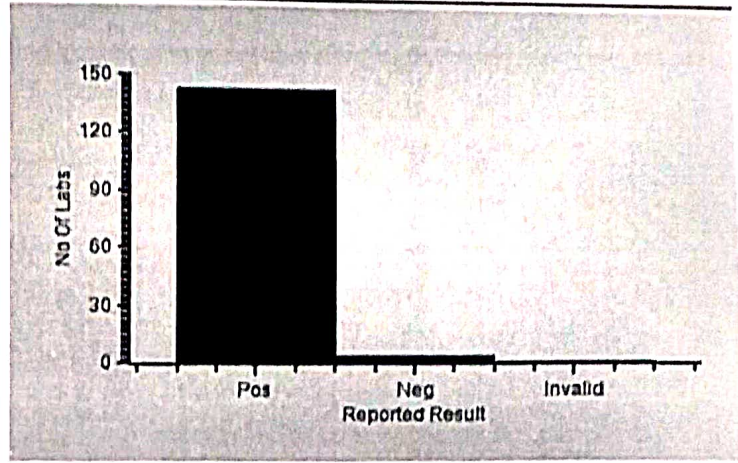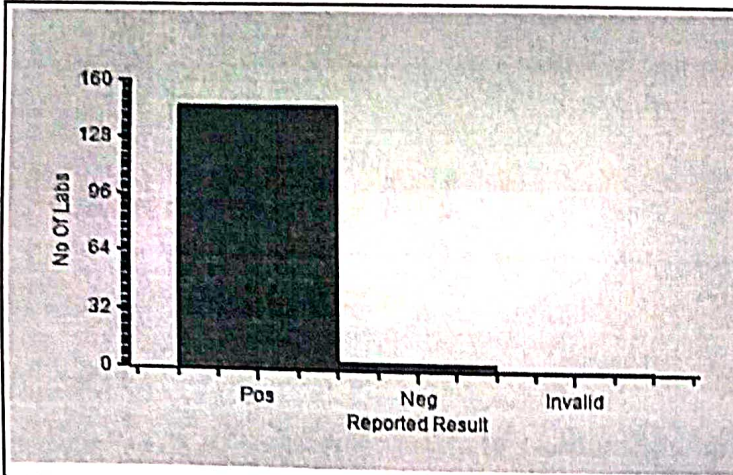

Reported Results Legends :-
 Pos : Positive
 Neg : Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021


Clinical Path - Urine Routine Chemistry,Urobilinogen (urine), -

| | |
|--|-----|
| <input type="checkbox"/> All Methods | N |
| <input type="checkbox"/> Photoelectric colorimetry - (Your Method) | 192 |
| <input type="checkbox"/> Urometer 120 - (Your Analyzer) | 3 |
| | 1 |

| | |
|-----------------|--------|
| Your Result | Normal |
| Result Expected | Nor |

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram


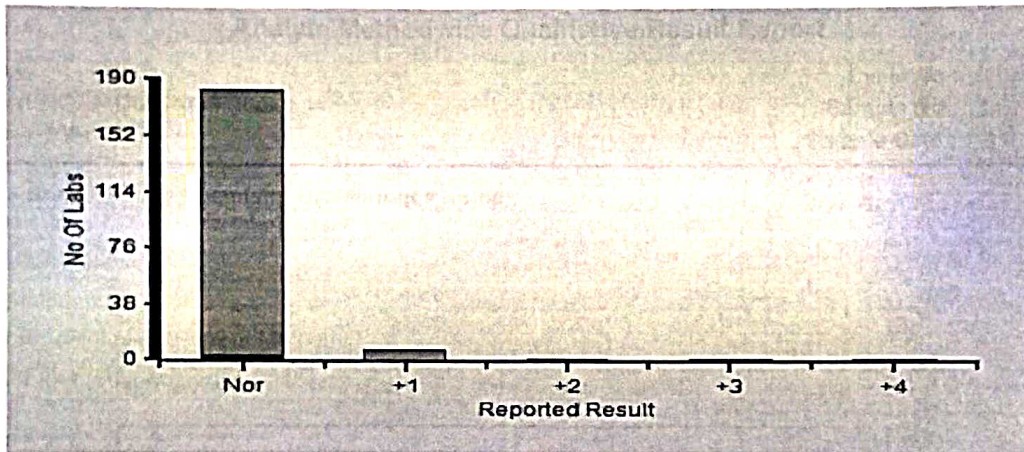


PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
Lab Name : SYNERGEN DIAGNOSTICS
Report Date : 30/12/2021

Cycle No : 210512
Sample No : 1
Sample Date : 11-12-2021

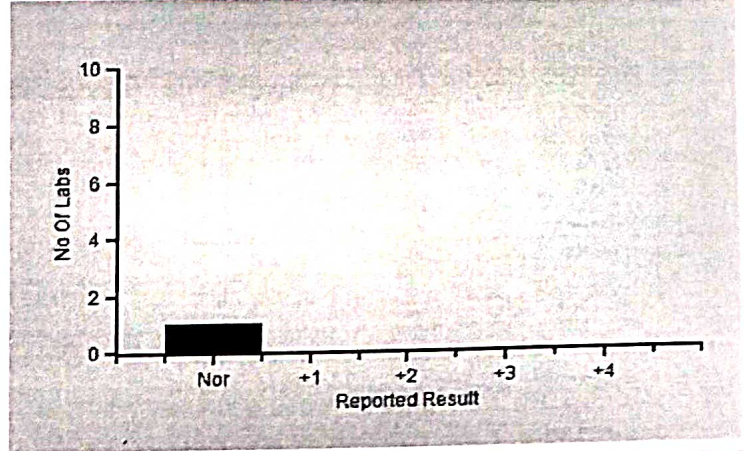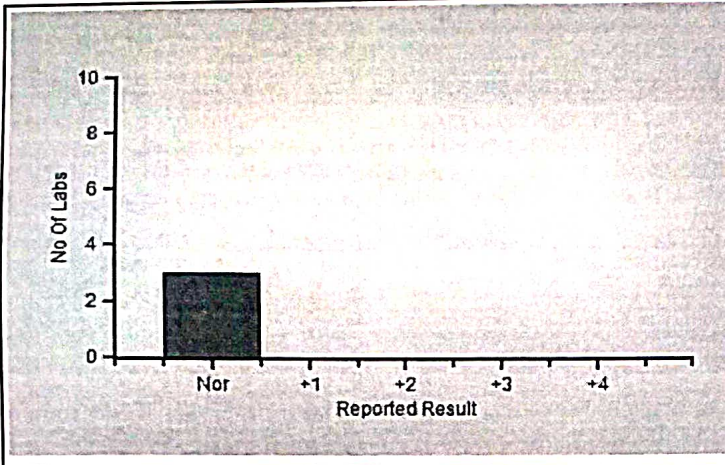

Reported Results Legends :-

| | |
|-----|----------|
| Nor | : Normal |
| +1 | : 1+ |
| +2 | : 2+ |
| +3 | : 3+ |
| +4 | : 4+ |

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error

Dr. Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
Unit No. 409-416,
Commercial Building - 1A,
Kohinoor Mall, Kirod Road, Kurla (W),
Mumbai - 400070



This is a computer generated report hence signature is not required

Cycle NO:- 210410

Sample No:- 1

Sample Date - 05/10/2021

Analyte Methodwise Qualitative Result Report.

- 1) Urine Routine Chemistry, Blood (Urine)
- 2) Urine Routine Chemistry, Nitrite (Urine)

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 02/11/2021

Cycle No : 210410
 Sample No : 1
 Sample Date : 05-10-2021


Clinical Path - Urine Routine Chemistry, Blood (urine), -

| | N |
|---------------------------|----|
| All Methods | 27 |
| Photoelectric colorimetry | 2 |
| Urometer 120 | 1 |

| | |
|-----------------|-------------|
| Your Result | 3+ |
| Result Expected | +1,+2,+3,+4 |

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

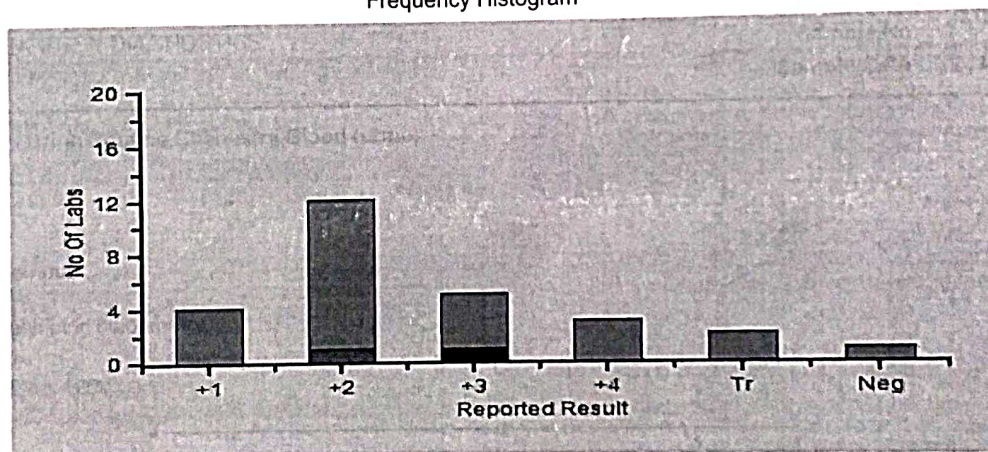

Reported Results Legends :-

| | |
|-----|------------|
| +1 | : 1+ |
| +2 | : 2+ |
| +3 | : 3+ |
| +4 | : 4+ |
| Tr | : Trace |
| Neg | : Negative |



PC-1022

Analyte Methodwise Qualitative Result Report


Lab No.: 596
Lab Name : SYNERGEN DIAGNOSTICS
Report Date : 02/11/2021

Cycle No : 210410
Sample No : 1
Sample Date : 05-10-2021

Comments :

Interpretation when an analyte is reported for multiple samples in a Round

- a) Reported on 2 samples
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance. Review for systematic error
- b) Reported on 3 samples
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance. Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 02/11/2021

Cycle No : 210410
 Sample No : 1
 Sample Date : 05-10-2021


Clinical Path - Urine Routine Chemistry,Nitrite (urine), -

| | N |
|-----------------------------|----|
| ■ All Methods | 28 |
| ■ Photoelectric colorimetry | 3 |
| ■ Urometer 120 | 1 |

| | |
|------------------------|--------|
| Your Result | Absent |
| Result Expected | Abs |

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

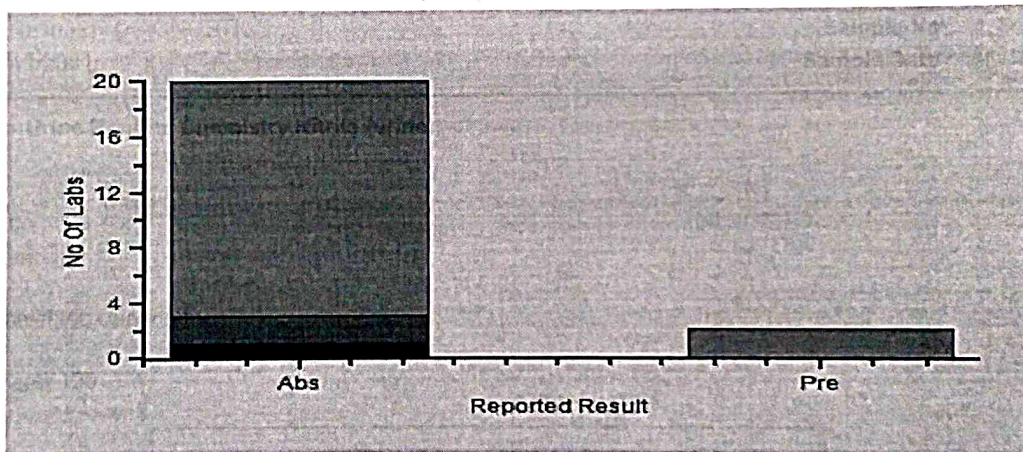

Reported Results Legends :-

Abs : Absent
 Pre : Present

Comments :



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
Lab Name : SYNERGEN DIAGNOSTICS
Report Date : 02/11/2021

Cycle No : 210410
Sample No : 1
Sample Date : 05-10-2021

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance. Review for systematic error



PC-1022