

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021


Immunoassay Extended,HBsAg, -

	N
All Methods	190
Immunochromatography - (Your Method)	146
Manual - (Your Analyzer)	127

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram


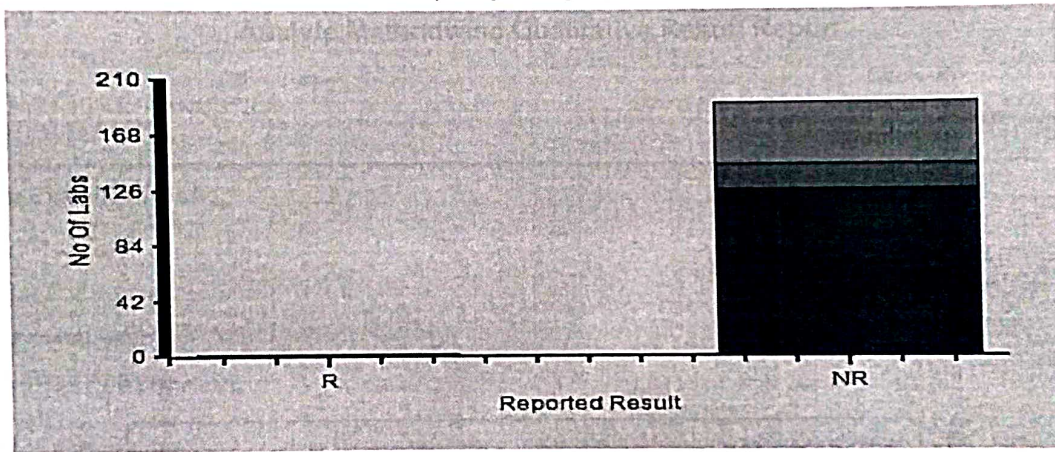


PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021

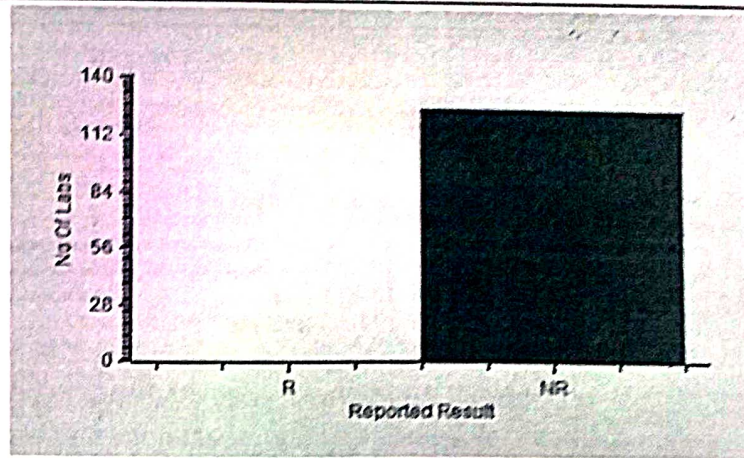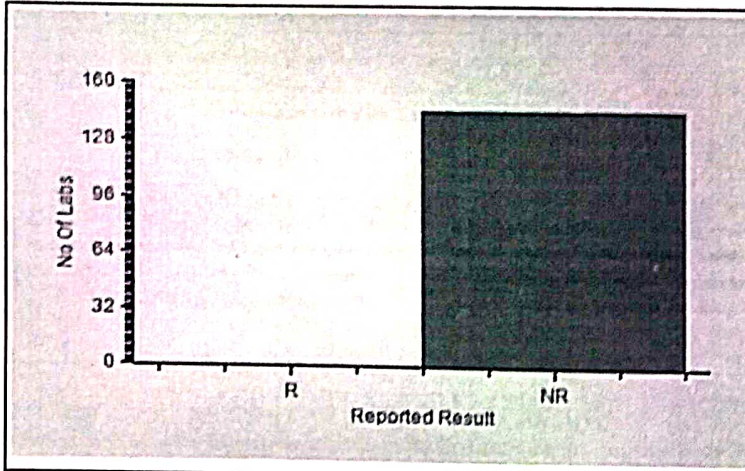

Reported Results Legends :-

R : Reactive
 NR : Non-reactive
 Eq : Equivocal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021


Immunoassay Extended,HCV, -

	N
■ All Methods	148
■ Immunochromatography - (Your Method)	106
■ Manual - (Your Analyzer)	95

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram


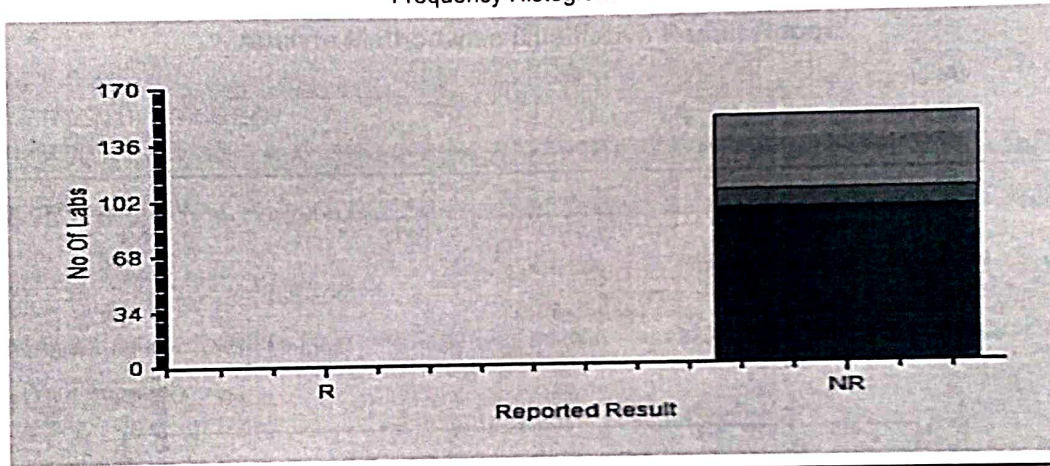


PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021

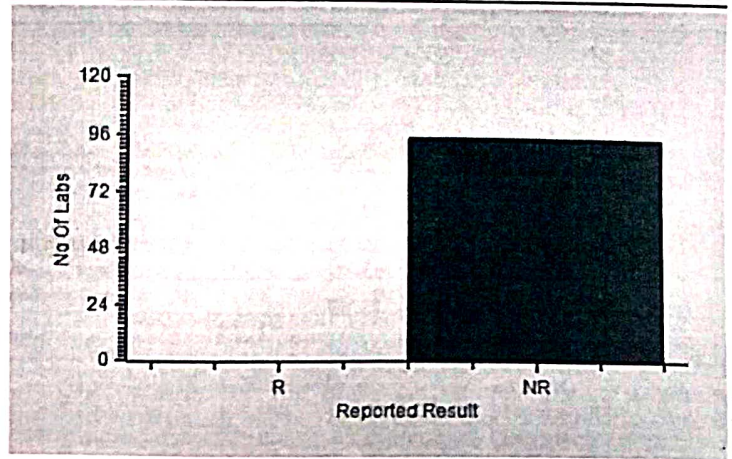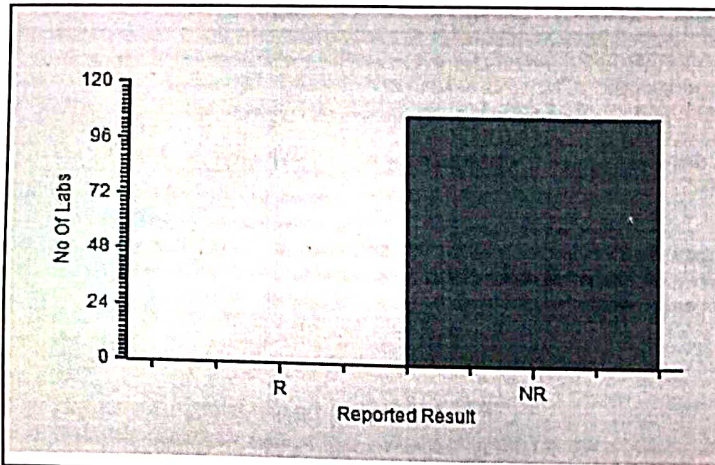

Reported Results Legends :-

R : Reactive
 NR : Non-reactive
 Eq : Equivocal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round.

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021


Immunoassay Extended,HIV Ab, -

<input type="checkbox"/> All Methods	N
<input type="checkbox"/> Immunochromatography - (Your Method)	107
<input type="checkbox"/> Manual - (Your Analyzer)	103
	96

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram


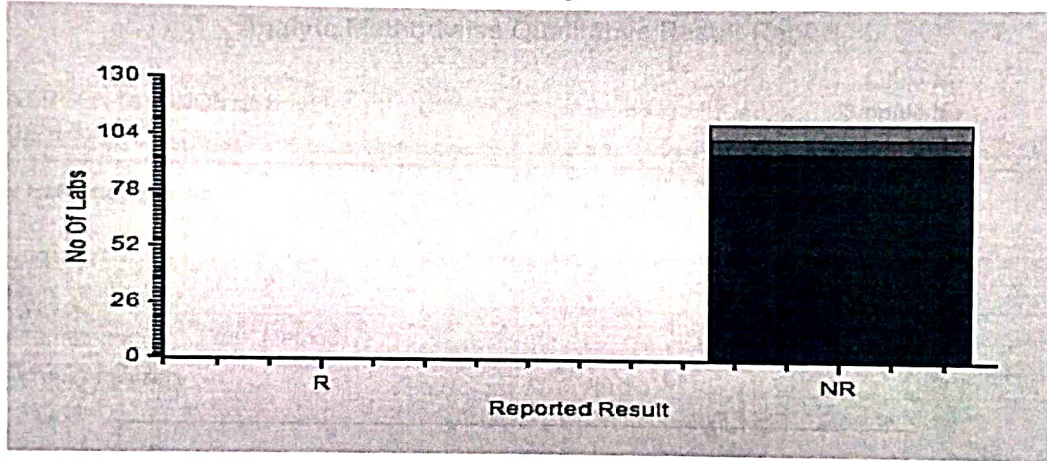


PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021

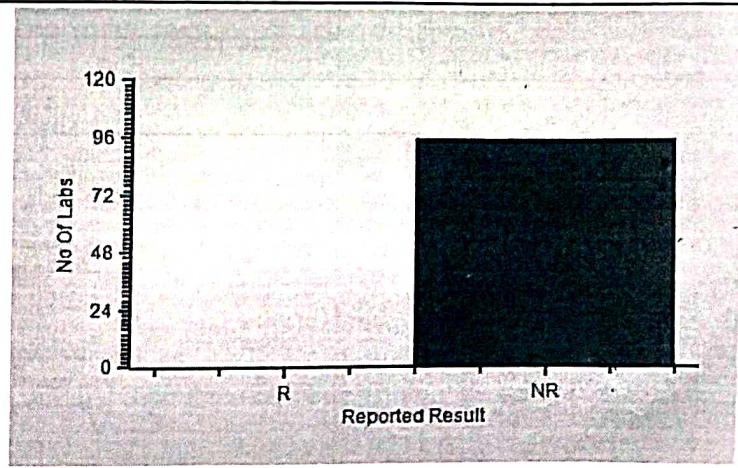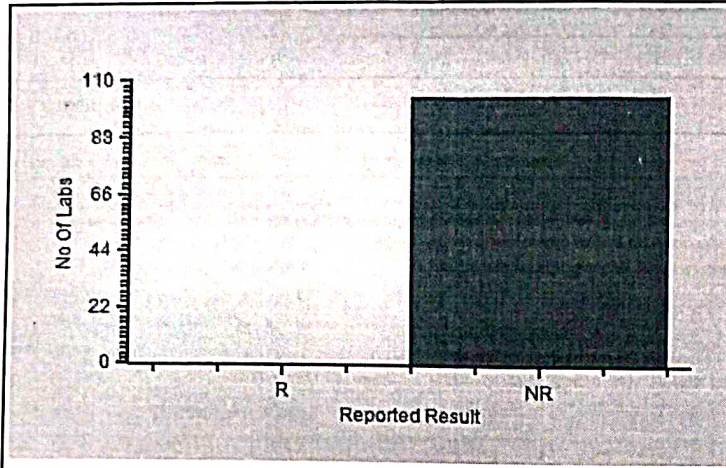

Reported Results Legends :-

R	: Reactive
NR	: Non-reactive
Eq	: Equivocal
Indet	: Indeterminate
HIV-1	: HIV-1 Ab Reactive
HIV-2	: HIV-2 Ab Reactive

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021


Immunoassay Extended,RPR (Syphilis Serology), -

<input type="checkbox"/> All Methods	N
<input type="checkbox"/> Agglutination - (Your Method)	159
<input type="checkbox"/> Manual - (Your Analyzer)	65
	160

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram


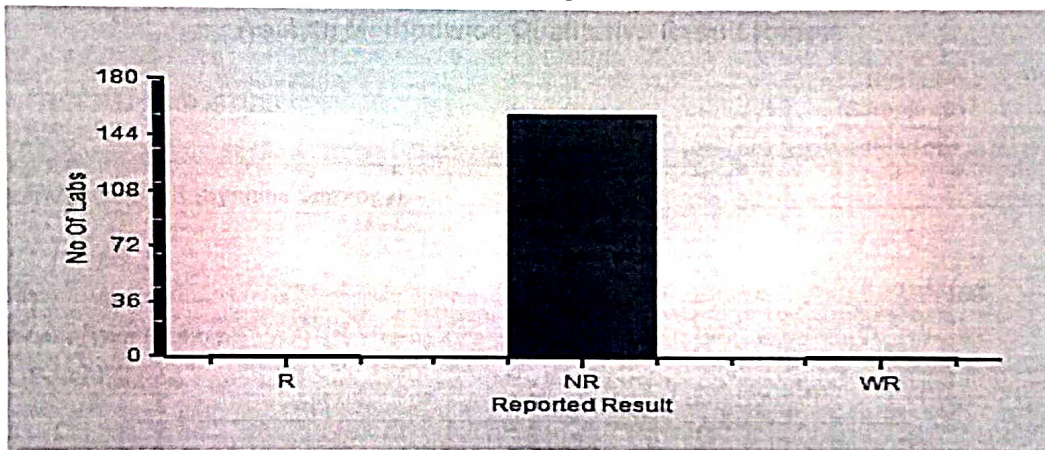


PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 1
 Sample Date : 11-12-2021

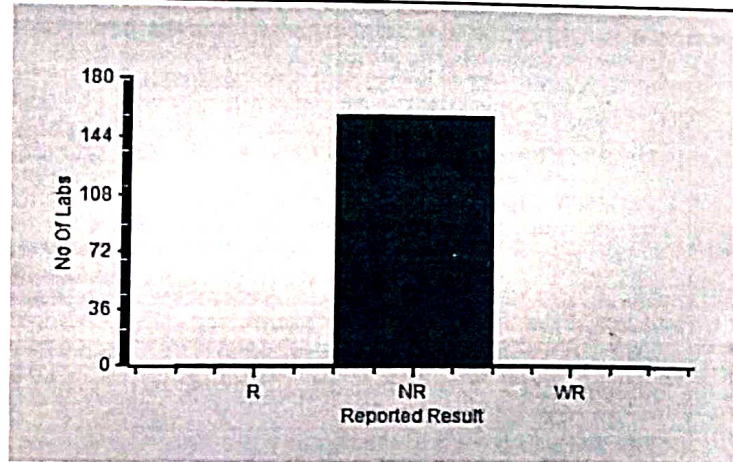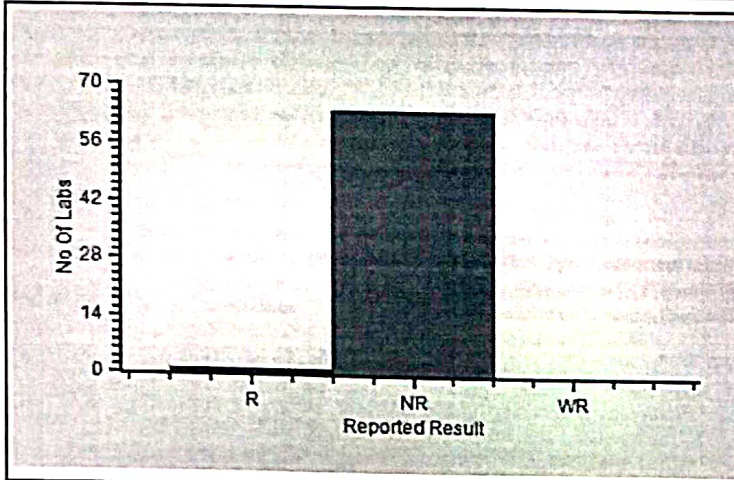

Reported Results Legends :-

R : Reactive
 NR : Non-reactive
 WR : Weak Reactive

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error

Dr. Puneet Kumar Nigam

Dr Puneet Kumar Nigam
 PT coordinator & Technical Manager, MHL EQAS
 Unit No 409-416
 Commercial Building - 1A,
 Kohinoor Mall, Kiral Road, Kuria (W),
 Mumbai - 400070



PC-1022

This is a computer generated report hence signature is not required

Analyte Methodwise Qualitative Result Report

Lab No.: 596
Lab Name : SYNERGEN DIAGNOSTICS
Report Date : 30/12/2021

Cycle No : 210512
Sample No : 2
Sample Date : 11-12-2021


Immunoassay Extended, HBsAg, -

	N
■ All Methods	185
■ Immunochromatography - (Your Method)	140
■ Manual - (Your Analyzer)	122

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram


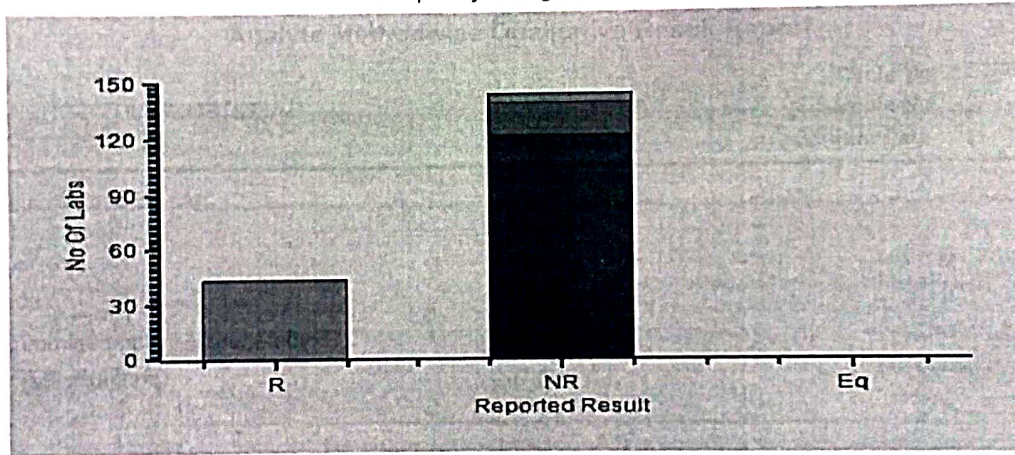


PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 2
 Sample Date : 11-12-2021

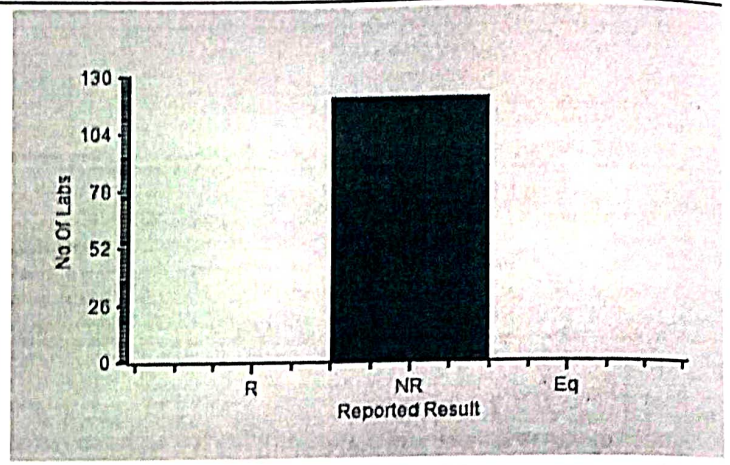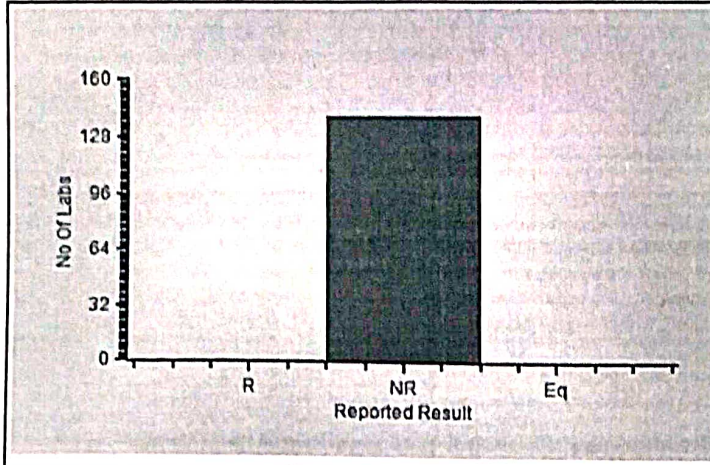

Reported Results Legends :-

R	: Reactive
NR	: Non-reactive
Eq	: Equivocal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 2
 Sample Date : 11-12-2021


Immunoassay Extended,HCV, -

 All Methods	N
 Immunochromatography - (Your Method)	145
 Manual - (Your Analyzer)	102
	92

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

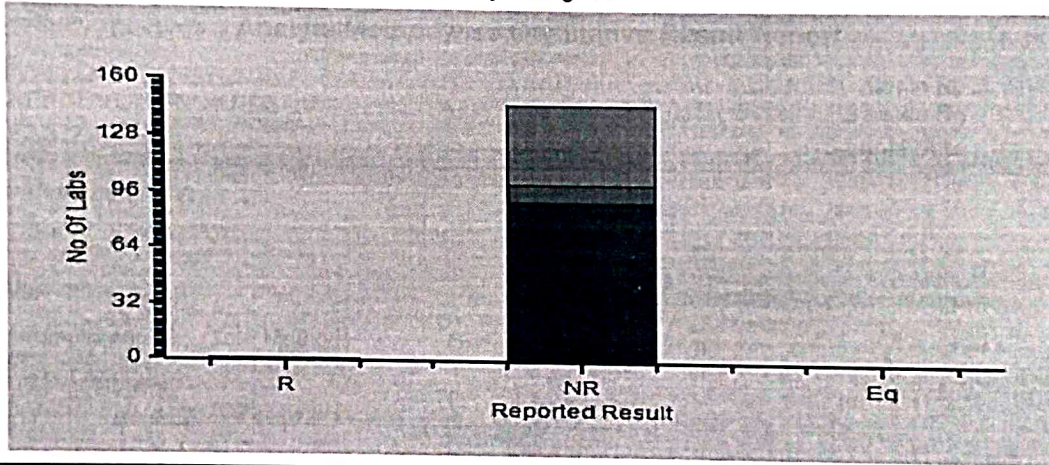


PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 2
 Sample Date : 11-12-2021

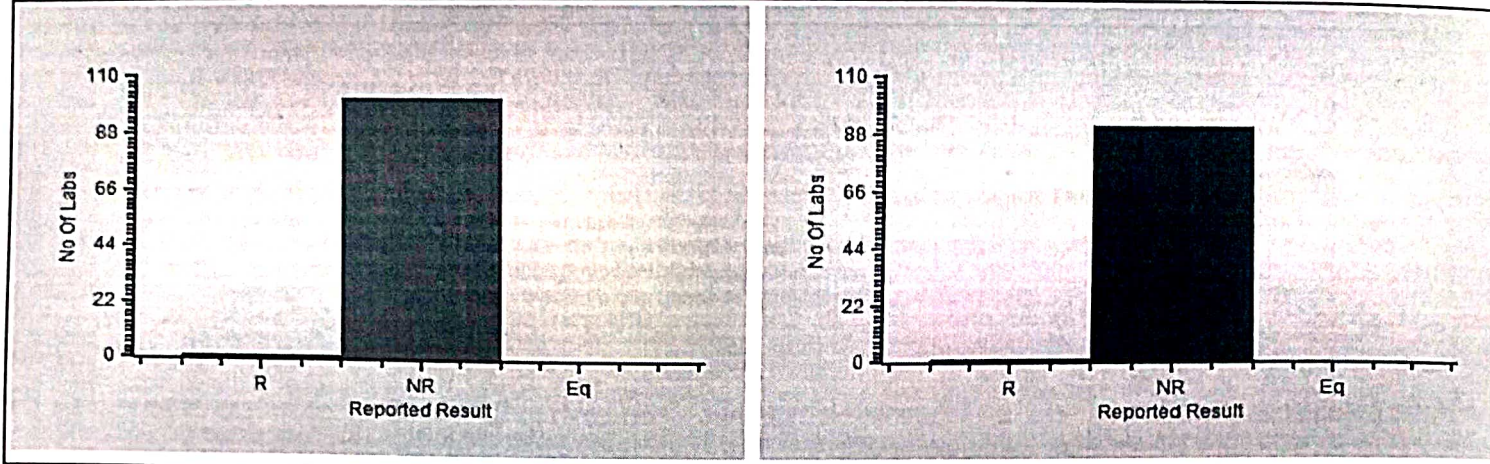

Reported Results Legends :-

R : Reactive
 NR : Non-reactive
 Eq : Equivocal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 2
 Sample Date : 11-12-2021


Immunoassay Extended,HIV Ab, -

	N
■ All Methods	102
■ Immunochromatography - (Your Method)	100
■ Manual - (Your Analyzer)	92

Your Result	HIV-1 Ab Reactive
Result Expected	HIV-1

Note : # is an indication that this parameter has not been evaluated



Frequency Histogram

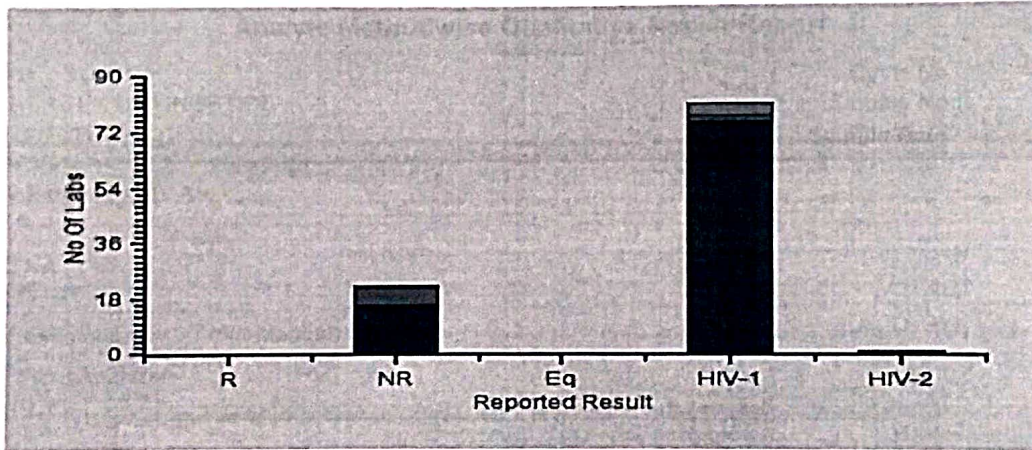

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 2
 Sample Date : 11-12-2021

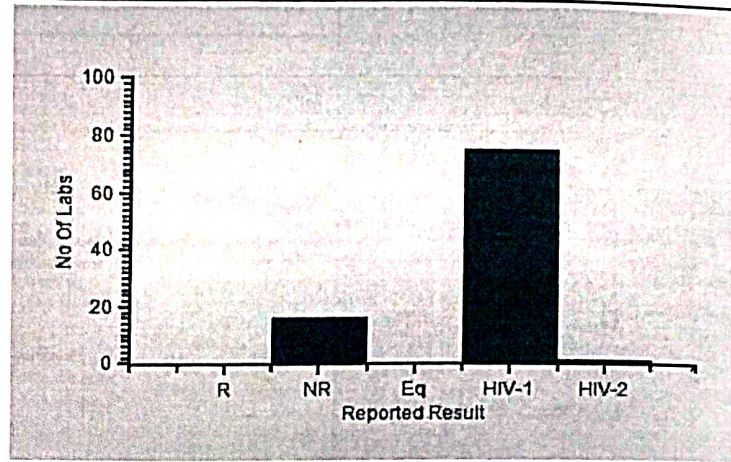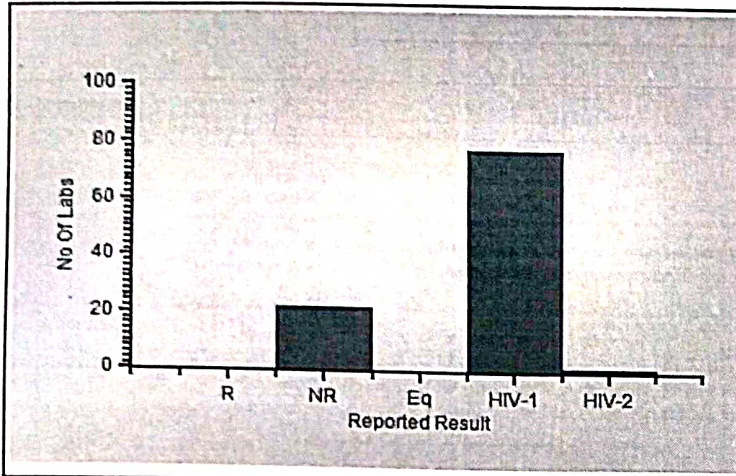

Reported Results Legends :-

R	: Reactive
NR	: Non-reactive
Eq	: Equivocal
Indet	: Indeterminate
HIV-1	: HIV-1 Ab Reactive
HIV-2	: HIV-2 Ab Reactive

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 2
 Sample Date : 11-12-2021


Immunoassay Extended,RPR (Syphills Serology), -

■ All Methods	N
■ Agglutination - (Your Method)	155
■ Manual - (Your Analyzer)	63
	156

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram


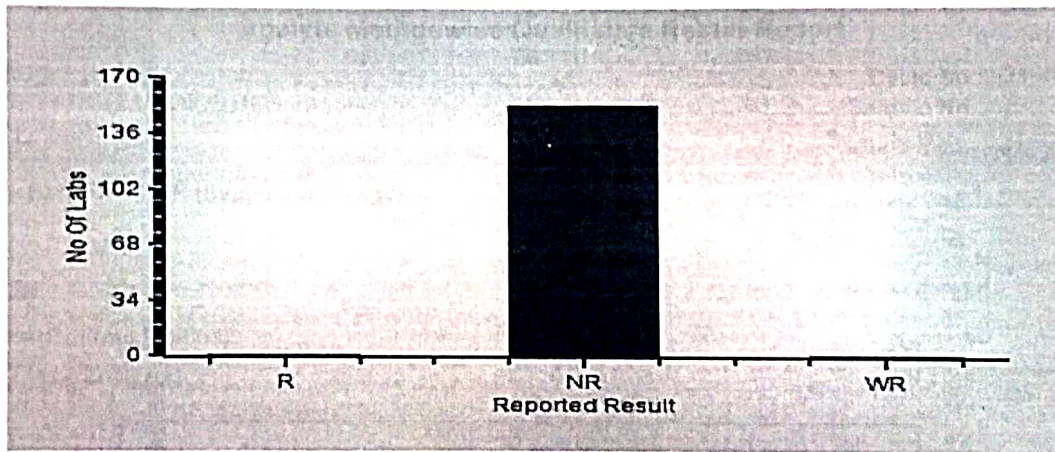


PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : SYNERGEN DIAGNOSTICS
 Report Date : 30/12/2021

Cycle No : 210512
 Sample No : 2
 Sample Date : 11-12-2021

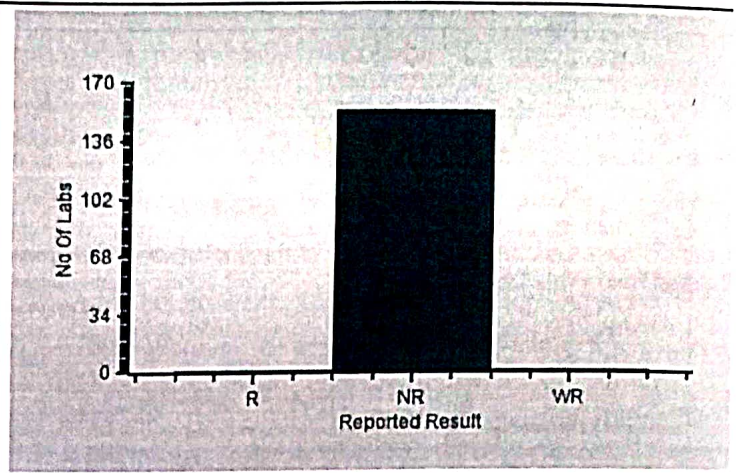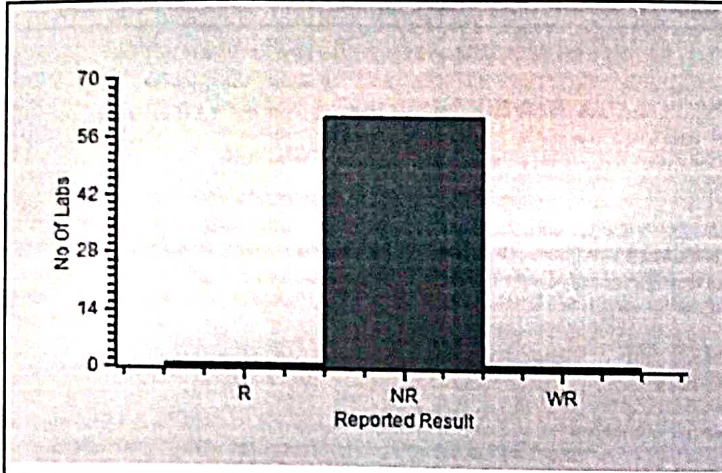

Reported Results Legends :-

R : Reactive
 NR : Non-reactive
 WR : Weak Reactive

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error

Dr. Puneet Kumar Nigam

Dr Puneet Kumar Nigam
 PT coordinator & Technical Manager, MHL EQAS
 Unit No. 409-416
 Commercial Building - 1A,
 Kakinora Mall, Kirod Road, Kurta (W),
 Mumbai - 400070



PC-1022

This is a computer generated report hence signature is not required