


Calibration report

Bio-Rad DATE: 02/21/2022
 D-10 TIME: 01:57 PM
 S/N: #DJ91438118 Software version: 4.30.2
 Calibrator ID: AA00219
 Injection date: 02/21/2022 01:52 PM
 Injection # 6 Method: 11bA1c
 Rack # --- Rack position: 1

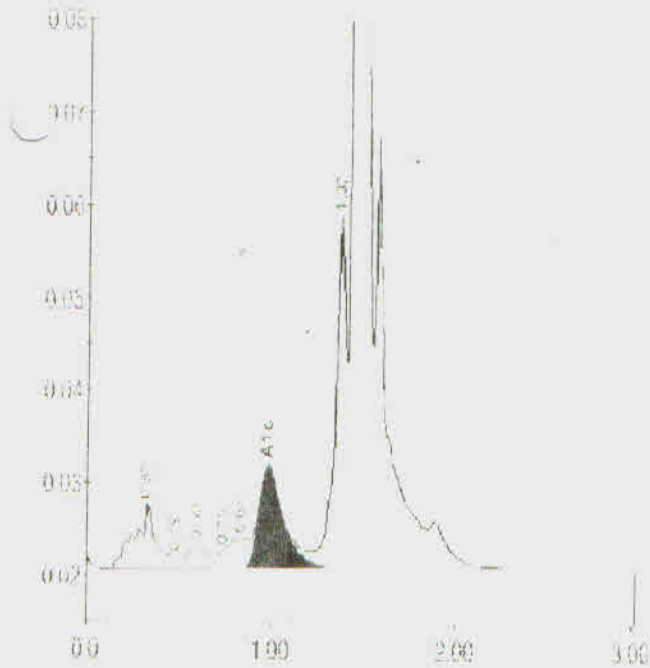

Peak table - 11bA1c


Peak	R time	Height	Area	Area %
A1b	0.33	7004	57162	2.0
F	0.49	1340	3899	0.1
Unknown	0.60	2632	18217	0.6
I A1c/C11b	1.075	2149	19878	0.7
I A1c/C11b	2.084	3245	22231	0.8
A1c	0.98	10810	100829	5.4
Unknown	1.37	37924	158130	5.5
A0	1.44	972579	2481434	86.7
Total Area:			2861780	

Concentration	%
A1c	5.4

21/2/22
 Vishu
 21-2

Calibration report

Bio-Rad DATE: 02/21/2022
 D-10 TIME: 01:56 PM
 S/N: #DJ9J138148 Software version: 4.30.2
 Calibrator ID: AA00220
 Injection date: 02/21/2022 01:55 PM
 Injection #: Method: HbA1c
 Rack #: Rack position: 2

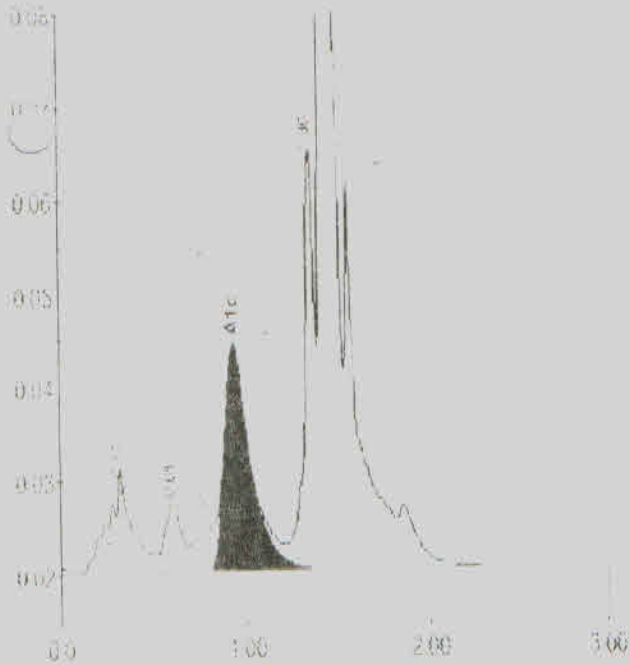

Peak table - HJ CAL2

Peak	Retention Time	Height	Area	Area %
Hb	0.32	10982	98247	3.3
Unknown	0.61	7432	47367	1.6
HbA1c/CHb	0.80	4377	31400	1.1
A1c	0.94	23827	232450	10.2
P3	1.36	44836	176675	6.0
A0	1.43	920701	2360458	80.1
Total Area			2946597	

Concentration	%
A1c	10.2

Good
2/21/22

Vukamy
2/21/22

Calibration Passed

Analyte	Old Slope	Old Intercept	New Slope	New Intercept
A1c	1.13	1.08	1.10	1.52