

Analyte Methodwise Qualitative Result Report

Lab No.: 650
 Lab Name : DR.KAUSHIK PATH LABS
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 1
 Sample Date : 26-04-2022


Clinical Path - Stool Routine Microscopy Image,Identify, -

| | | |
|---|---------------------|----------|
| | All Methods | N |
| | - - (Your Method) | 147 |
| | - - (Your Analyzer) | 147 |

| | |
|------------------------|-----------------|
| Your Result | Cyst of Giardia |
| Result Expected | CG |

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

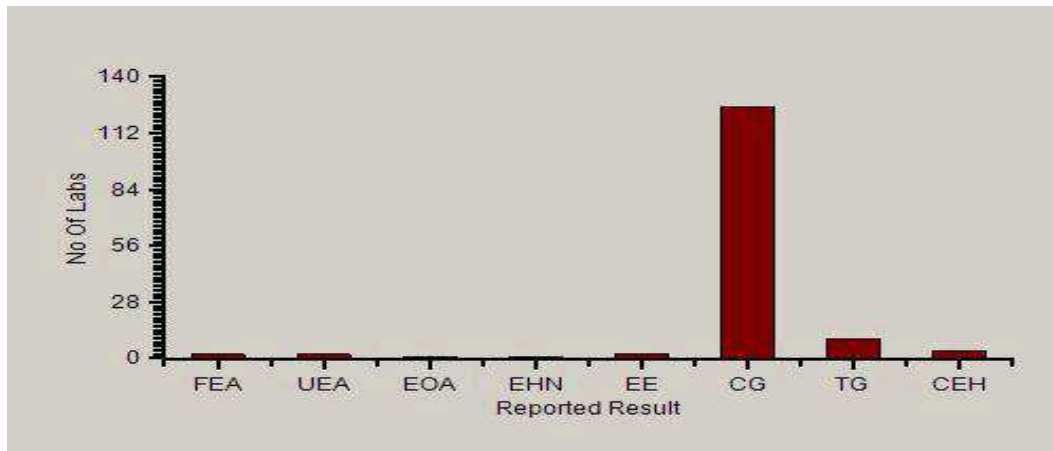

Analyte Methodwise Qualitative Result Report

Lab No.: 650
Lab Name : DR.KAUSHIK PATH LABS
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 1
Sample Date : 26-04-2022

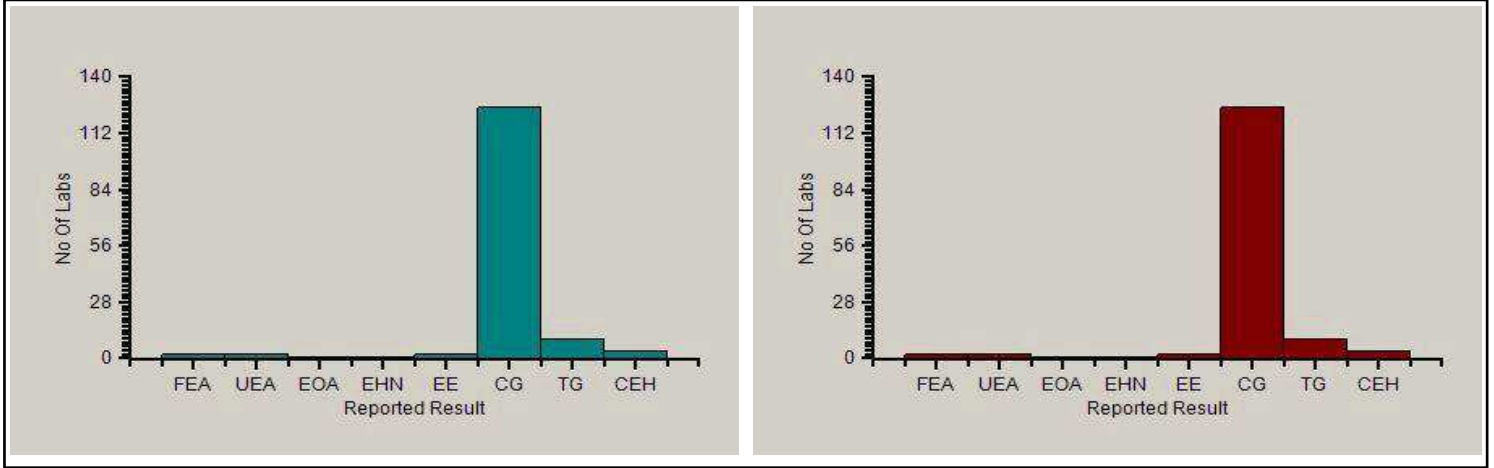

Reported Results Legends :-

- FEA : Fertilized egg of Ascaris
- UEA : Unfertilized Egg of Ascaris
- EOA : Egg of Ankylostoma
- EOT : Egg of Trichuris
- EOC : Egg of Clonorchis
- EOM : Egg of Metagonimus
- EHN : Egg of H. nana
- ET : Egg of Taenia
- EE : Egg of Enterobius
- CG : Cyst of Giardia
- TG : Trophozoite of Giardia
- CEH : Cyst of E. histolytica
- TEH : Trophozoite of E. histolytica

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS

Unit No. 409-416.
Commercial Building - 1A,
Kohinoor Mall, Kiroi Road, Kurla (W),
Mumbai - 400070

