

Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 1
 Sample Date : 26-04-2022


Clinical Path - Semen Analysis Image & Video,Sperm Morphology-1, -

	All Methods	N
	- - (Your Method)	87
	- - (Your Analyzer)	87

Your Result	Abnormal Neck
Result Expected	Abr Neck

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

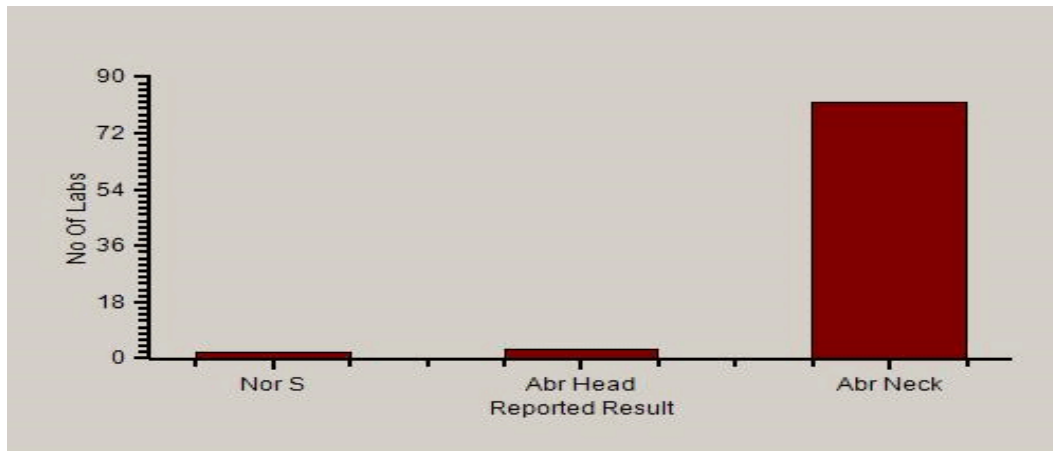

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 1
Sample Date : 26-04-2022

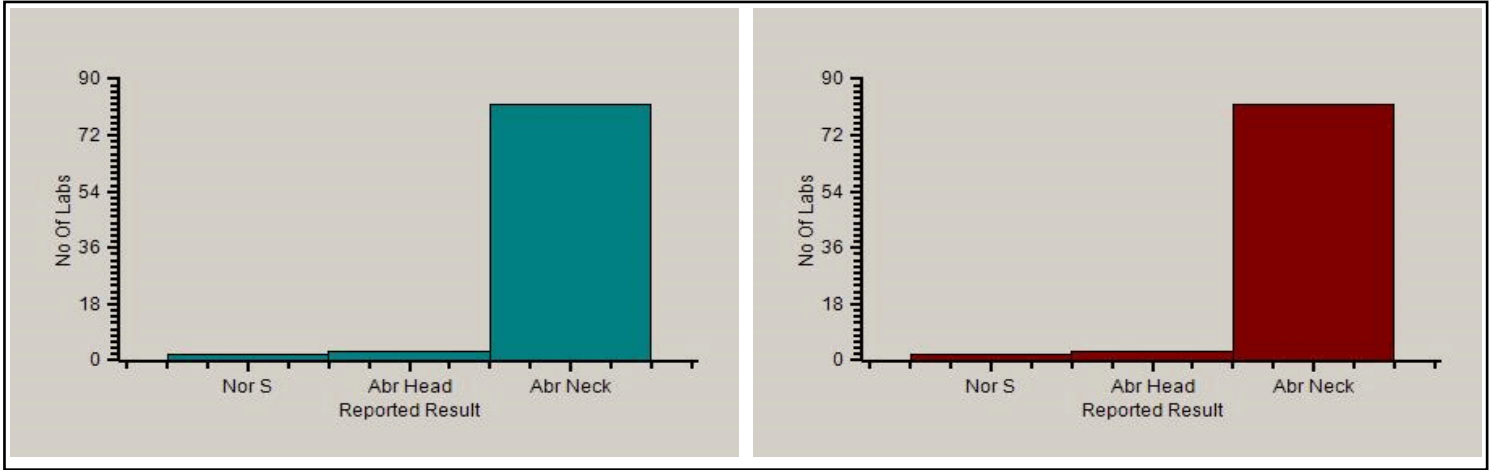

Reported Results Legends :-

- Nor S : Normal Sperm
- Abr Head : Abnormal Head
- Abr Tail : Abnormal Tail
- Abr Neck : Abnormal Neck

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 1
 Sample Date : 26-04-2022

Clinical Path - Semen Analysis Image & Video,Sperm Morphology-2, -


<p>■ All Methods</p> <p>■ - - (Your Method)</p> <p>■ - - (Your Analyzer)</p>	<p>N</p> <p>68</p> <p>68</p> <p>68</p>
--	---

Your Result Normal

Result Expected #

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

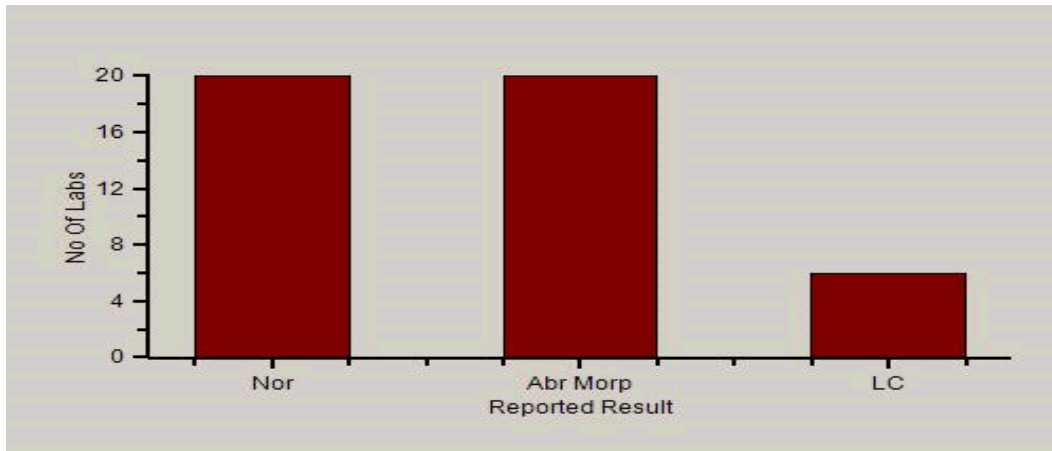

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 1
Sample Date : 26-04-2022

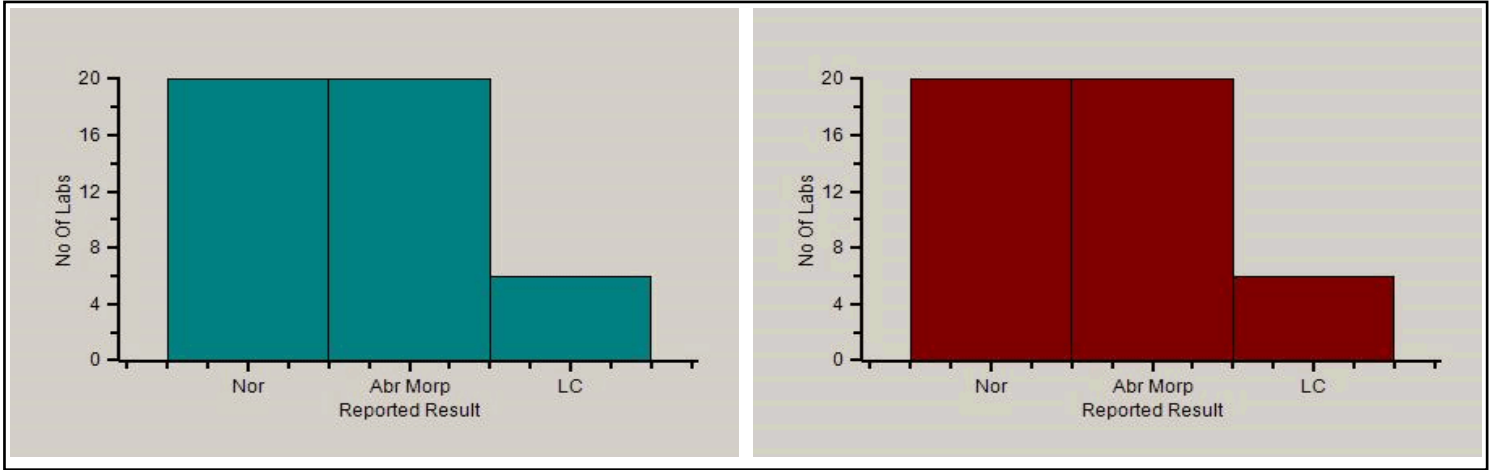

Reported Results Legends :-

- Nor : Normal
- Abr Morp : Abnormal Morphology
- LC : Low Count
- None : None of the above

Comments :

- Interpretation when an analyte is reported for multiple samples in a Round:
- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
 - b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
 Unit No. 409-416.
 Commercial Building - 1A,
 Kohinoor Mall, Kiroi Road, Kurla (W),
 Mumbai - 400070

