

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 2
Sample Date : 26-04-2022


Immunoassay Extended,Dengue NS 1, -

	N
■ All Methods	164
■ Immunochromatography - (Your Method)	144
■ Manual - (Your Analyzer)	156

Your Result	Negative
Result Expected	Neg

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

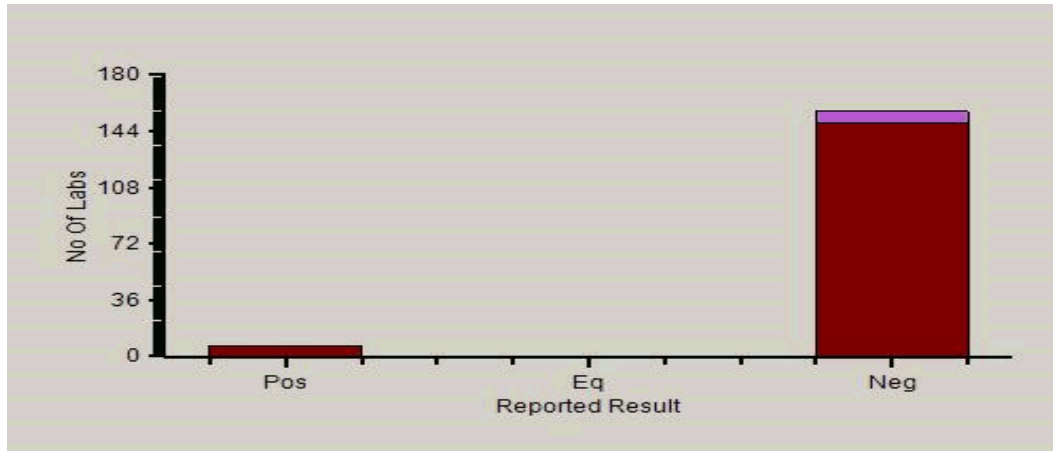

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 2
Sample Date : 26-04-2022

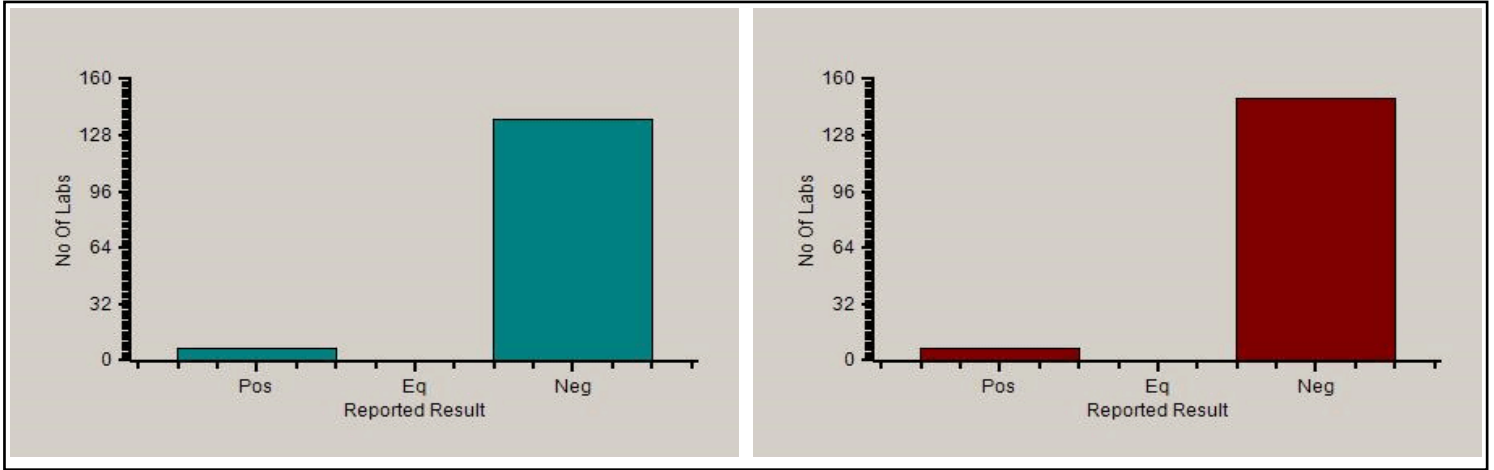

Reported Results Legends :-

- Pos : Positive
- Eq : Equivocal
- BL : Borderline
- Neg : Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 2
 Sample Date : 26-04-2022


Immunoassay Extended,HBsAg, -

	All Methods	N
	Immunochromatography - (Your Method)	210
	Manual - (Your Analyzer)	156
		137

Your Result	Reactive
Result Expected	R

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

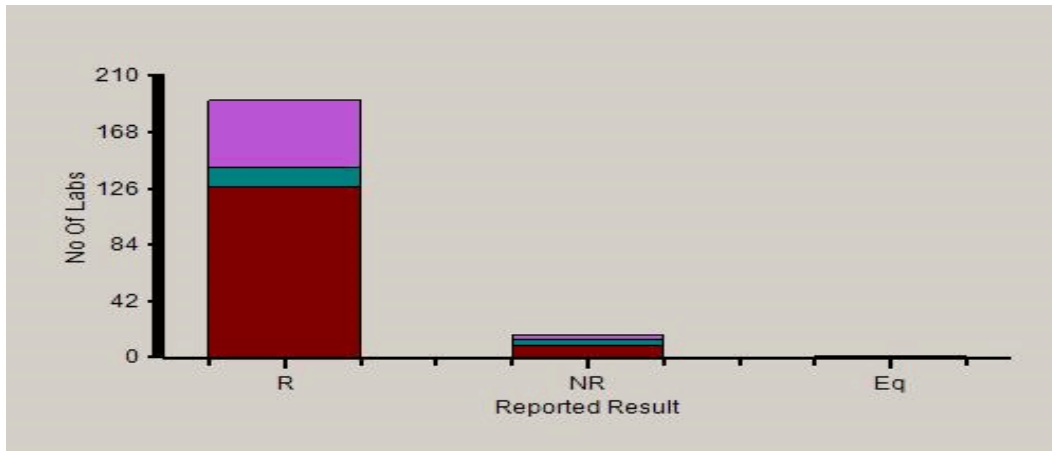

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 2
Sample Date : 26-04-2022

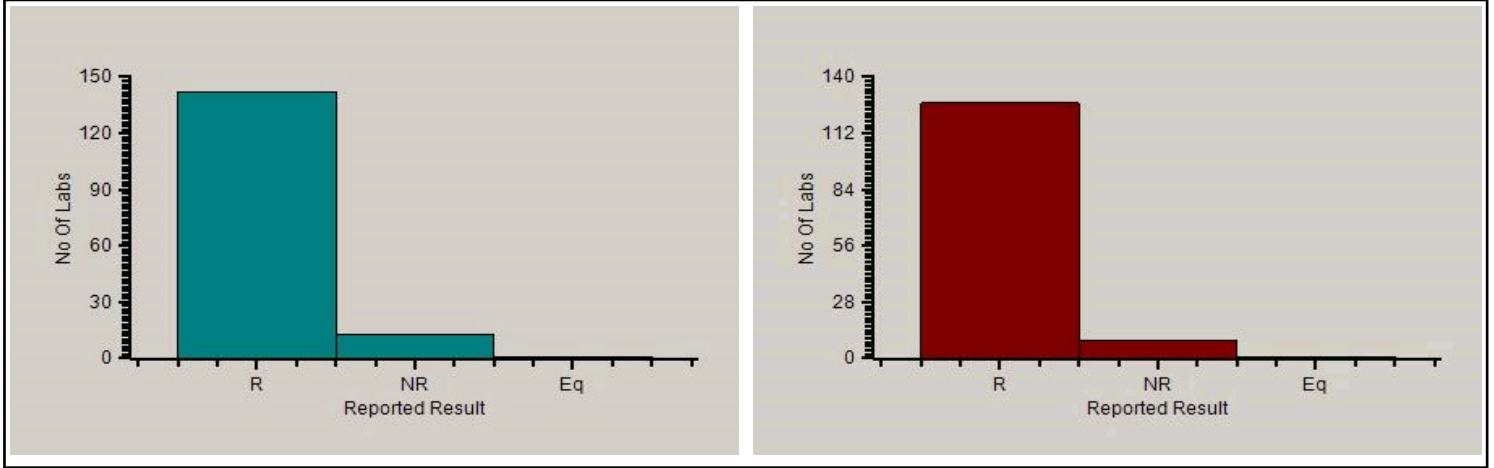

Reported Results Legends :-

R : Reactive
 NR : Non-reactive
 Eq : Equivocal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 2
 Sample Date : 26-04-2022

Immunoassay Extended,HCV, -


■ All Methods	N
■ Immunochromatography - (Your Method)	158
■ Manual - (Your Analyzer)	110
	98

Your Result Reactive

Result Expected #

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

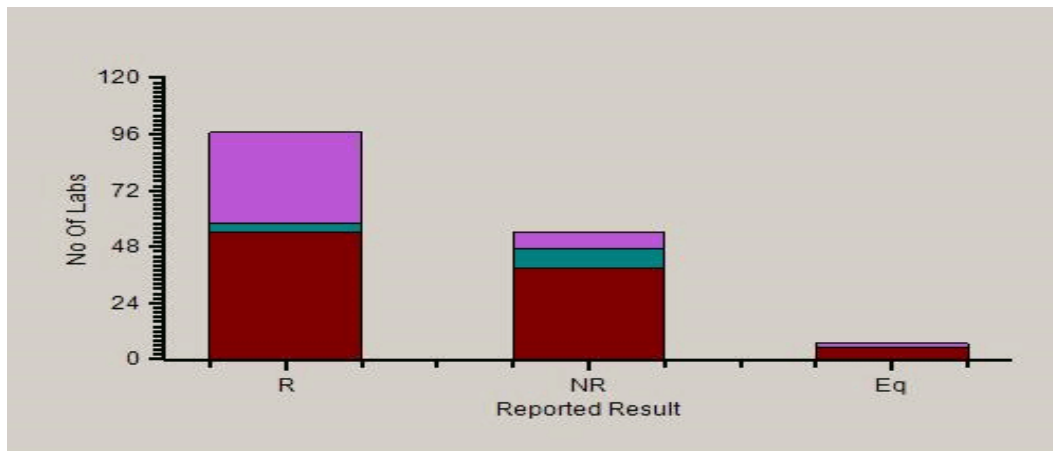

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 2
Sample Date : 26-04-2022

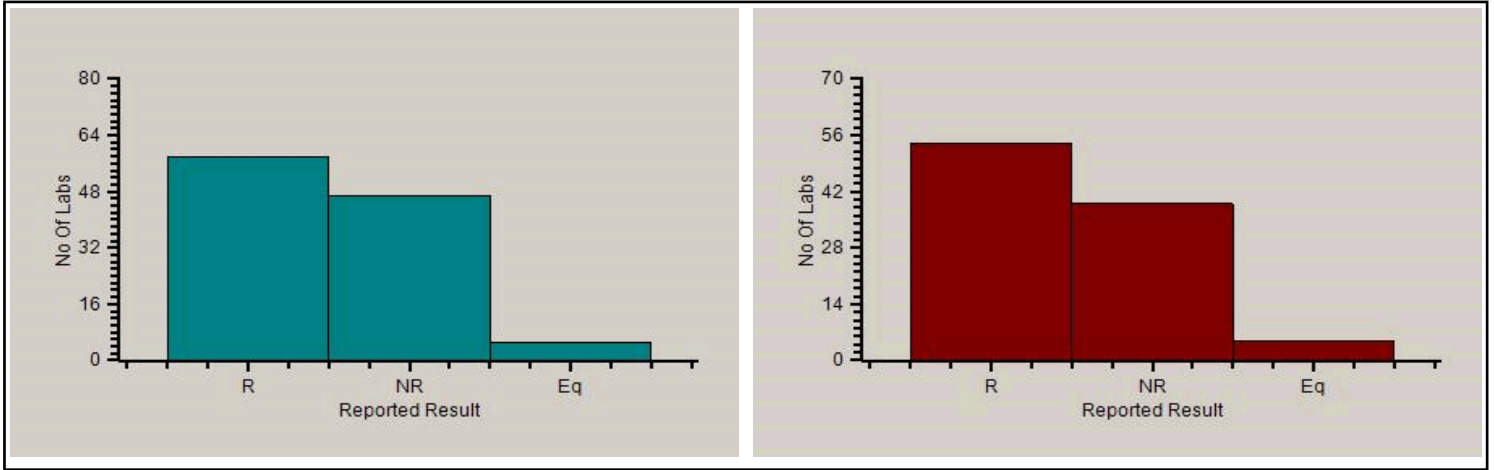

Reported Results Legends :-

R : Reactive
 NR : Non-reactive
 Eq : Equivocal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 2
 Sample Date : 26-04-2022


Immunoassay Extended,HIV Ab, -

■ All Methods	N
■ Immunochromatography - (Your Method)	120
■ Manual - (Your Analyzer)	111
	103

Your Result	HIV-1 Ab Reactive
Result Expected	HIV-1

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

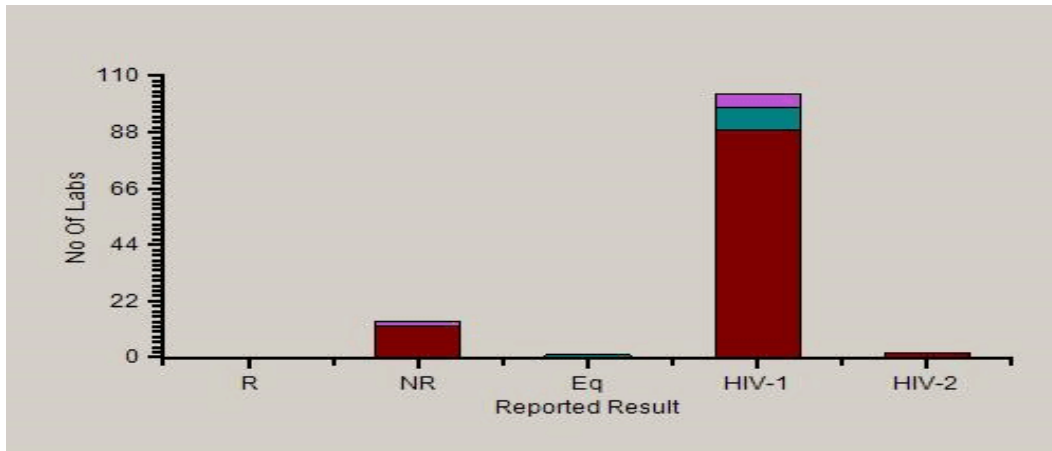


PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 2
Sample Date : 26-04-2022

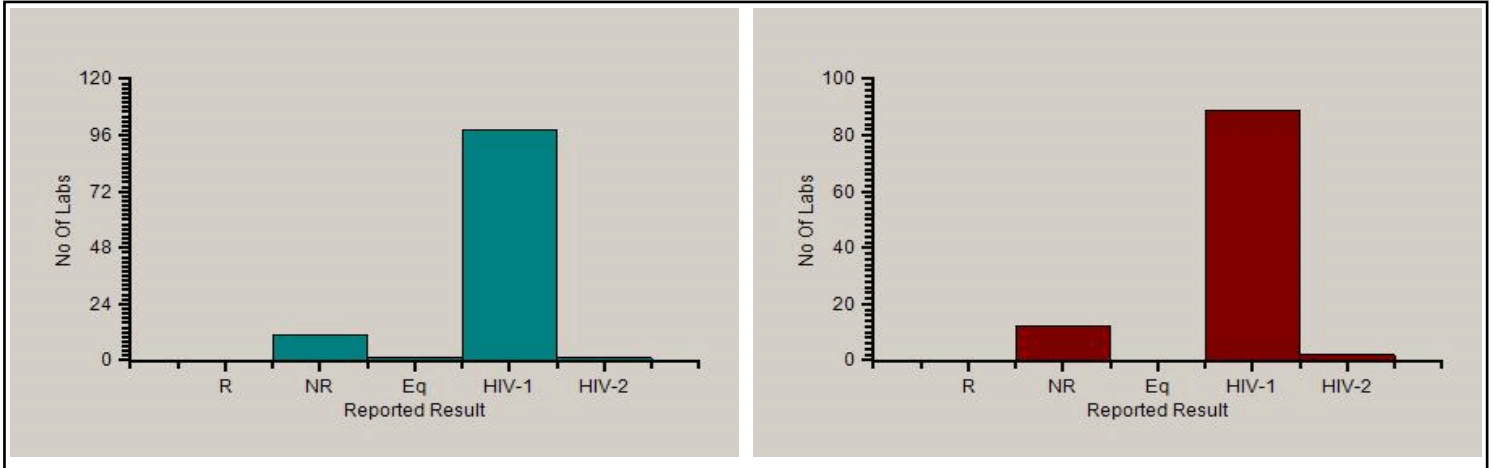

Reported Results Legends :-

R	: Reactive
NR	: Non-reactive
Eq	: Equivocal
Indet	: Indeterminate
HIV-1	: HIV-1 Ab Reactive
HIV-2	: HIV-2 Ab Reactive

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 2
 Sample Date : 26-04-2022


Immunoassay Extended,RPR (Syphilis Serology), -

	N
■ All Methods	173
■ Immunochromatography - (Your Method)	65
■ Manual - (Your Analyzer)	173

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated



Frequency Histogram

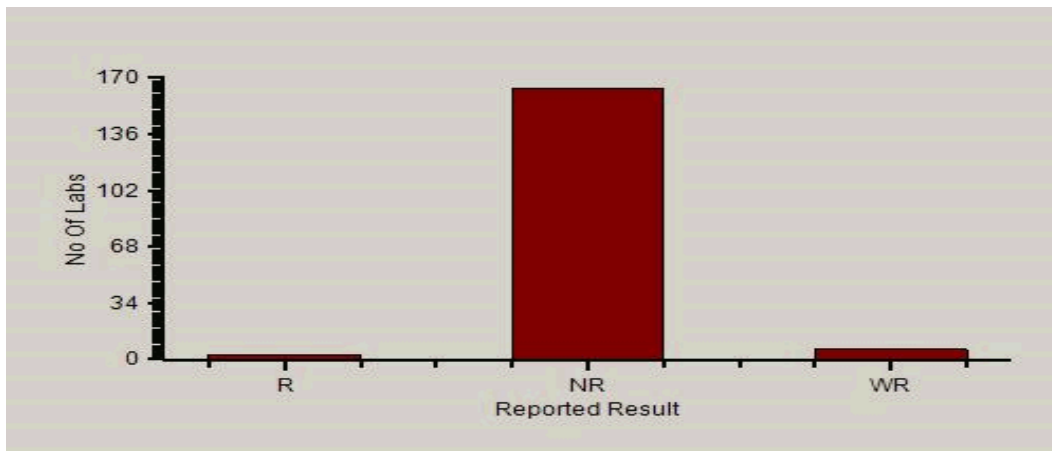

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 2
Sample Date : 26-04-2022

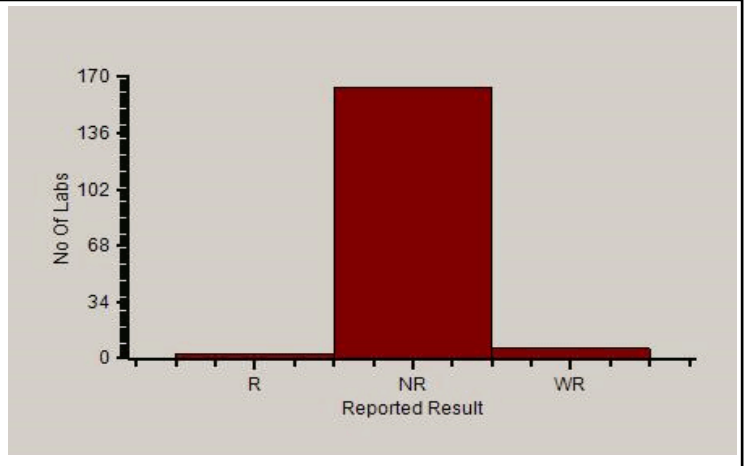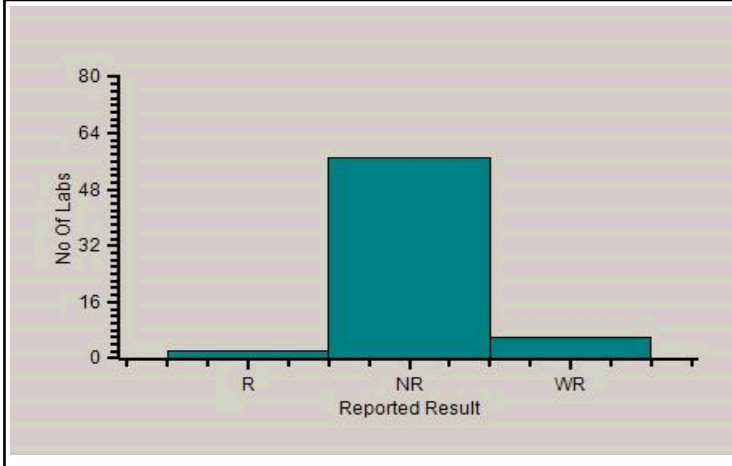

Reported Results Legends :-

- R : Reactive
- NR : Non-reactive
- WR : Weak Reactive

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 2
 Sample Date : 26-04-2022


Immunoassay Extended, Typhidot IgM, -

■ All Methods	N
■ Immunochromatography - (Your Method)	161
■ Manual - (Your Analyzer)	158
	161

<table border="0" style="width: 100%;"> <tr> <td style="width: 50%;">Your Result</td> <td style="width: 50%;">Positive</td> </tr> <tr> <td>Result Expected</td> <td>Neg</td> </tr> </table>	Your Result	Positive	Result Expected	Neg
Your Result	Positive			
Result Expected	Neg			

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

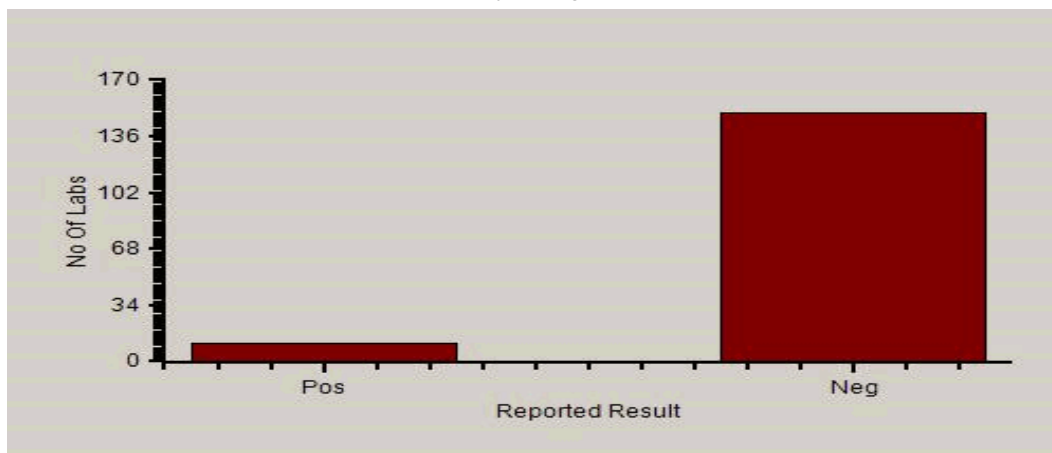

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 2
Sample Date : 26-04-2022

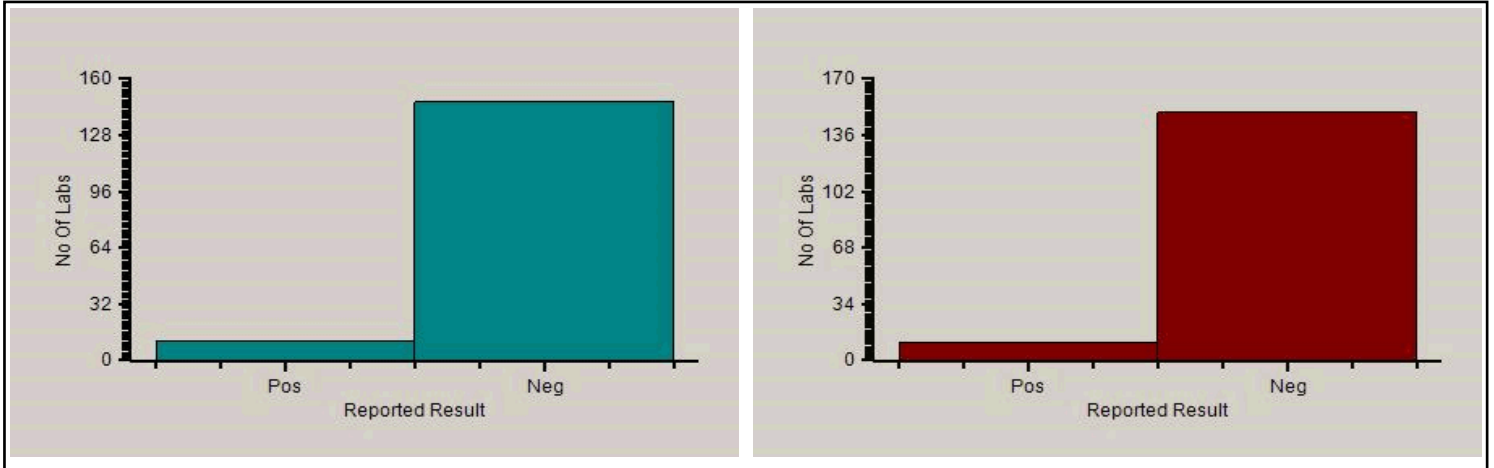

Reported Results Legends :-
 Pos : Positive
 Neg : Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 2
 Sample Date : 26-04-2022


Immunoassay Extended,Widal test - ParaTyphi A-H antigen (AH), -

	N
■ All Methods	108
■ Slide Agglutination - (Your Method)	79
■ Manual - (Your Analyzer)	108

Your Result	No Agglutination
Result Expected	NoA

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

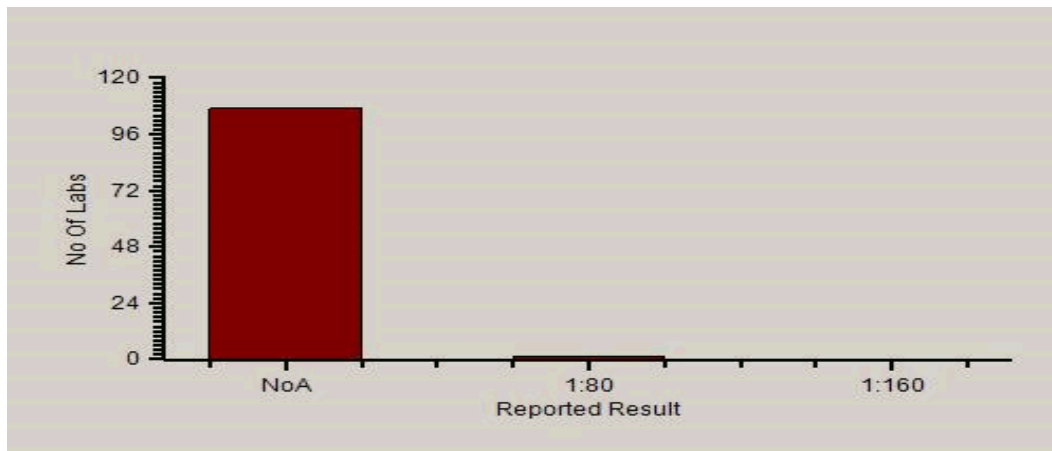

Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 2
 Sample Date : 26-04-2022

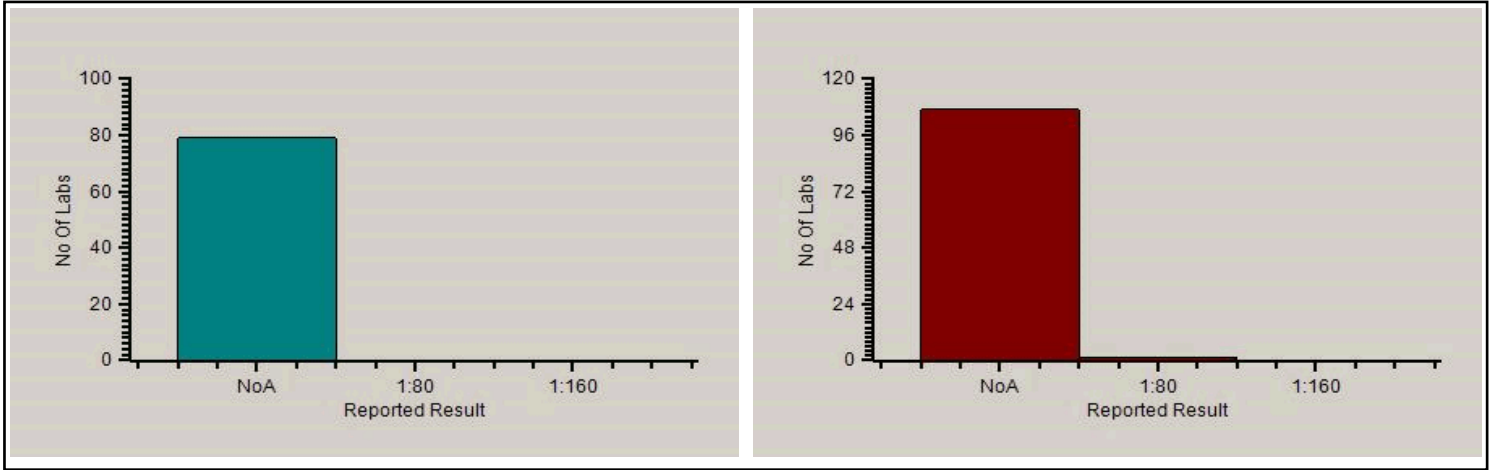

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 2
 Sample Date : 26-04-2022


Immunoassay Extended,Widal test - ParaTyphi B-H antigen (BH), -

	N
■ All Methods	108
■ Slide Agglutination - (Your Method)	80
■ Manual - (Your Analyzer)	108

Your Result	No Agglutination
Result Expected	NoA

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

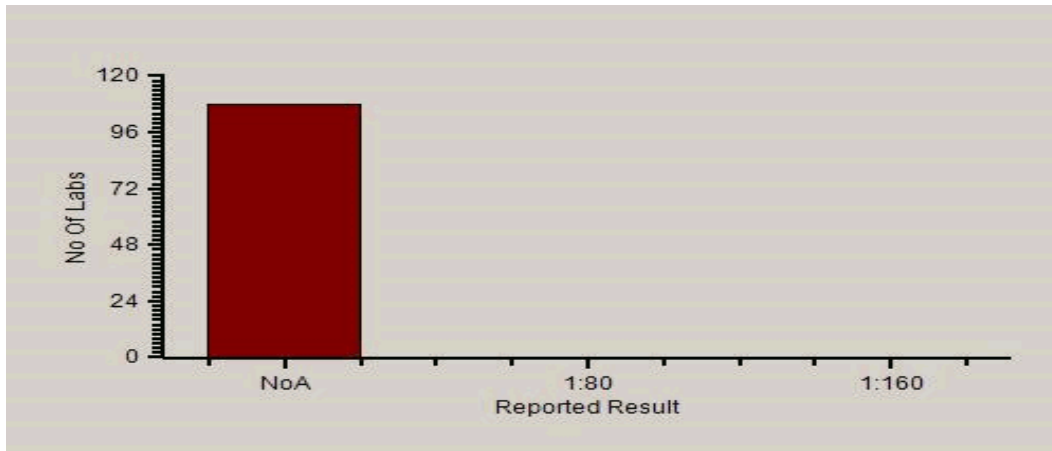

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 2
Sample Date : 26-04-2022

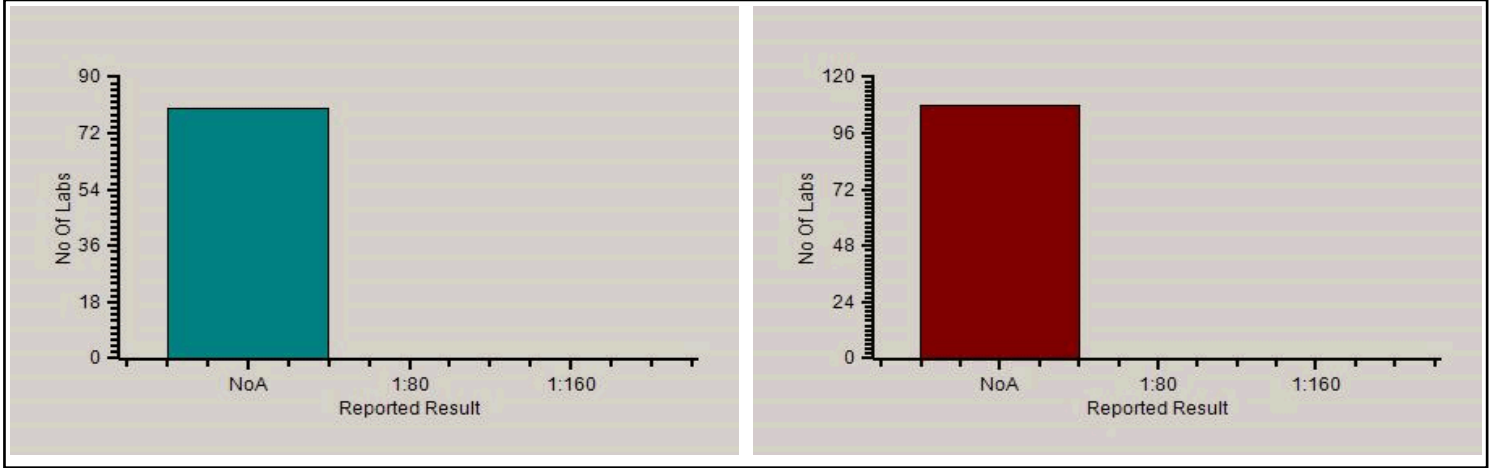

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 2
 Sample Date : 26-04-2022


Immunoassay Extended,Widal test - Typhi H antigen (TH), -

	N
■ All Methods	119
■ Slide Agglutination - (Your Method)	89
■ Manual - (Your Analyzer)	119

Your Result	No Agglutination
Result Expected	NoA

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

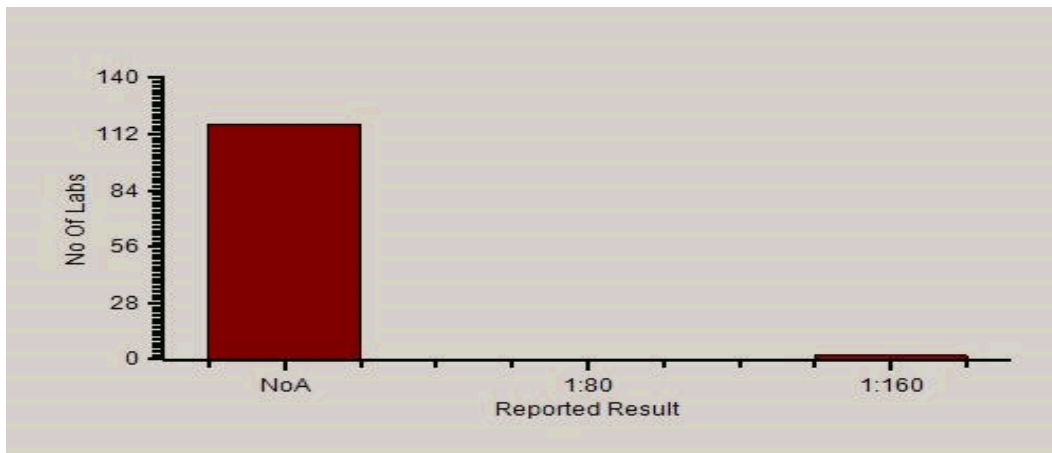

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 2
Sample Date : 26-04-2022

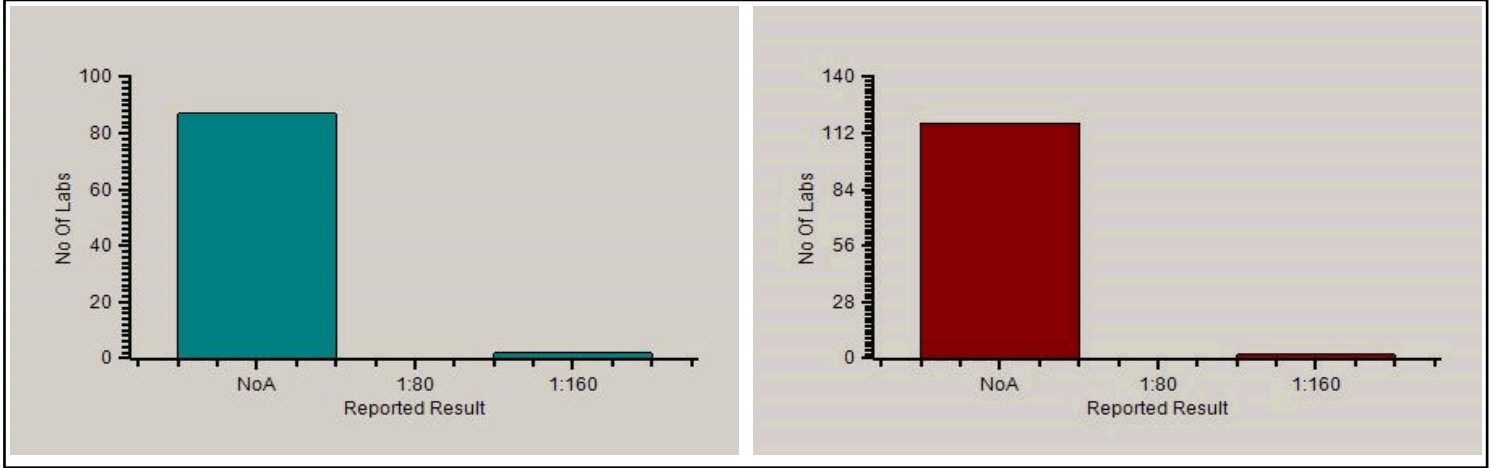

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640

Comments :

- Interpretation when an analyte is reported for multiple samples in a Round:
- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
 - b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 2
 Sample Date : 26-04-2022


Immunoassay Extended,Widal test - Typhi O antigen (TO), -

	N
■ All Methods	119
■ Slide Agglutination - (Your Method)	89
■ Manual - (Your Analyzer)	119

Your Result	No Agglutination
Result Expected	NoA

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

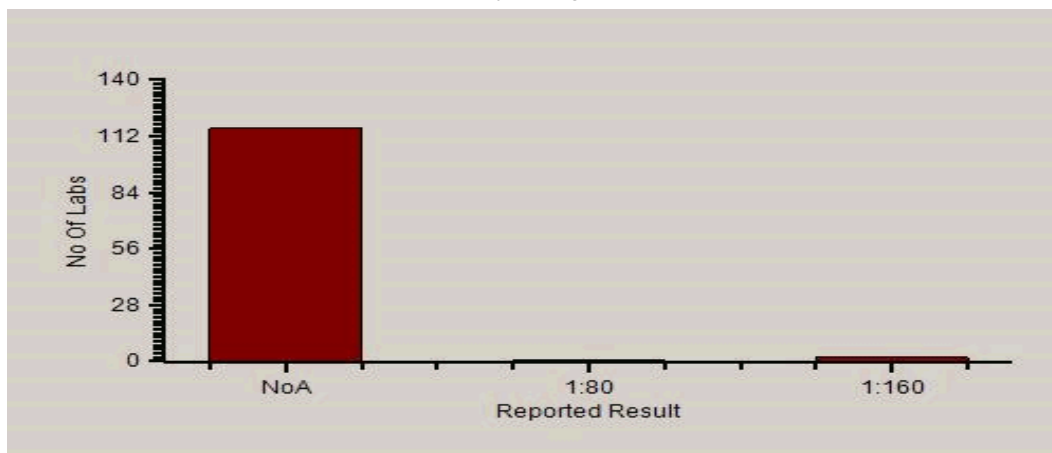


PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 2
Sample Date : 26-04-2022

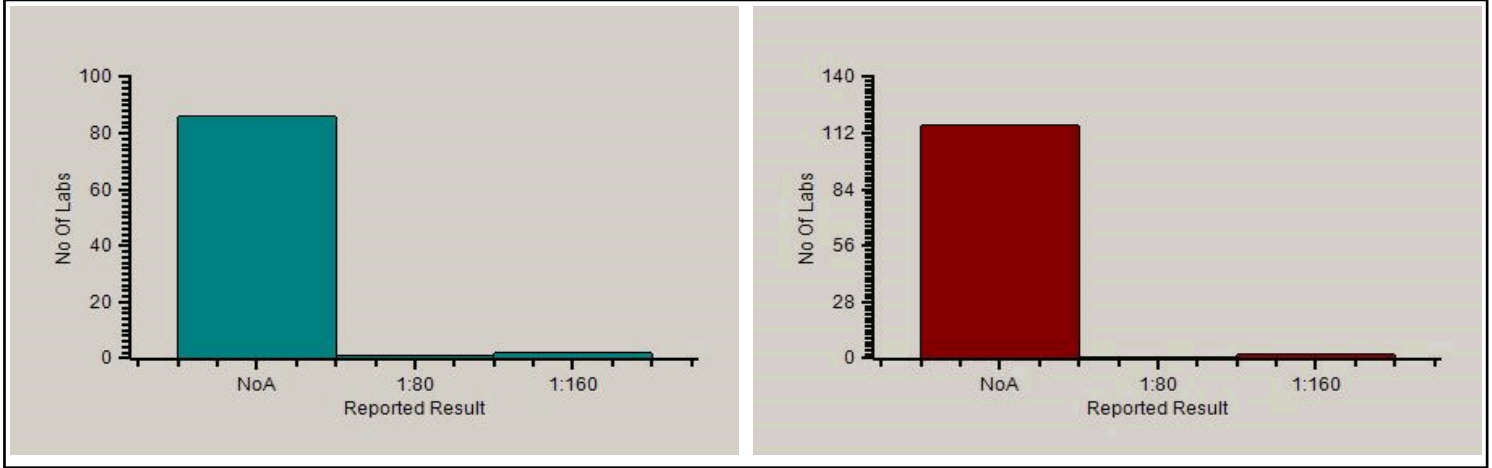

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
 Unit No. 409-416.
 Commercial Building - 1A,
 Kohinoor Mall, Kiroi Road, Kurla (W),
 Mumbai - 400070

