

Parashar Micro Measurement Pvt. Ltd.

Unit-II : J-22, Site-C, Surajpur Industrial Area, UPSIDC, Greater Noida (U.P.)

PH.: 0120-4252360-65, Email : pmmpl.india@gmail.com

Website : www.pmmpl.in, www.parashar.info



The way to Technology
(17 Years of Excellence)


Calibration Certificate

						Page 1
Certificate Number : PMM/BM/731434						
Calibrated For		M/s. Som Datt Medical Centre S - 524, School Block , Shakarpur Delhi - 110092		Calibrated on		31.01.2022
				Valid Upto		30.01.2023
				Cert. Issue Date		01.02.2022
Description of Equipments						
Nomenclature		Bio Chemistry Analyzer		Accuracy/Class		As per specification
Test Type		Electrical Safety Test		Condition of UUC		Physically Ok
Make		ELI Techogroup		Party ID Mark No.		2
Model No.		Microlab 300		Location		Path Lab
Mfr. S.No.		17-43307				
Master Equipment / Standard Used						
Sr.No.	Nomenclature	Make & Model	Serial No. / I/D Mark	Calibrated From	Certificate No.	Due Date of Calibration
1	Electrical Safety Analyzer	Fluke/ ESA612	PMM/BM/ESA-01	FLUKE CORPORATION	PC-EVT-0D3B	31.03.2022
Standard used for calibration are traceable to National/International Standards through unbroken chain of calibration.						
Calibration Performed at			AT SITE	Environmental		Temperature = 25 ± 5° C
Calibration Procedure No.			PMM/II/BMCP/01	Condition(s)		Humidity = 50 ± 10 % RH
Reference Standard / Guideline			IEC-60601-1			
CALIBRATION RESULTS						
1.0 Main Line Test						
a. Main Line Voltage supply working properly						Yes
b. Main Line ground connected properly						Yes
2.0 Earth Resistance Test						
Sr.No.	Max Limit (Ω)		Actual Observed Value (Ω)		Remark	
1	2.0		0.231		Pass	
3.0 Polarity Test Pass						Yes
4.0 Safety test						
Sr.No.	Parameter	Permitted Values		Measured Values	Deviation%	Remarks (Pass/Fail)
1	Ground Wire Resistance	<0.3Ω		0.246	-0.00054	Pass
2	Chassis Leakage	<100 μANC		94μA	-0.06	Pass
		<500μASFC		N/A	N/A	N/A
3	Pateint Leakge Current	<100μABandB F		N/A	N/A	N/A
		<10μACF		1.2μA	-0.088	Pass
4	Patient Lead Leakage Current, Isolation Test	<100μABF		N/A	N/A	N/A
		<10μACF		1.0μA	-0.09	Pass
5	Insulation (Optional) 500V	<2MΩ		OR MΩ	N/A	N/A

Uncertainty of measurement (at approx. 95% confidence level with coverage factor k=2)

1.22%

Calibrated By : Gordhan Bairwa
Designation : Calibration Engineer



Approved By: Vikram Parashar
Designation : Technical Manager

- Conditions : 1. This certificate refers only to the particular item submitted for calibration.
2. The calibration result reported in this certificate are valid at the time of and under the stated conditions of measurement.
3. This particular certificate can not be reproduced except in full, without prior permission of chief executive officer of the lab.

Name & Address of Customer : Sahdatt Medical Centre
S-224, School Block, Motarapur - Delhi
- 110092
STATE: Delhi PIN: 110092

Phone: 7065123669E-Mail: Sahdattmedicalcentre@shajid.comName of Instrument : **Microlab 300 LX**(w/o inbuilt printer) **Microlab 300 EX**(with inbuilt printer) Type : **Semi Automatic Biochemistry Analyser**Serial No : 17-43307Installation Date : 08-05-2018Calibration Date : 19-05-2022Next Calibration Due on : 18-05-2023

This is to certify that above said instrument has been validated by hardware calibration for Filters, Aspiration (Pump), Temperature & Lamp according to the procedures provided by Vital Scientific, Netherlands (Elitech Group).

This calibration is carried out by using Standard Operating Procedures (S.O.P.) provided by Vital Scientific (Elitech Group Company) and traceable to Vital Scientific standards.

This instrument conform to IVD & EU directives of use.

Calibration carried out on site by:Sahni

Signature

Name of Service Engineer : Gantab Sahni

Instrument Service Division

Q-Line Biotech Pvt. Ltd.

Jays
28/5/22**Q-LINE BIOTECH PRIVATE LIMITED (Formerly known as "POCT Services Pvt. Ltd.")**Corp. Office: 20A (Basement), Main Shivaji Marg, Najafgarh Road, Near Moti Nagar Police Station, New Delhi-110015, INDIA. Tel.: 011-45577407
Regd. Office: 298-281, Transport Nagar, Kanpur Road, Adjacent Transport Nagar Metro Station, Lucknow-226023 (U.P.), INDIA. Tel.: 0522-2433023

E-mail: info@qlinebiotech.com | Website: www.qlinebiotech.com

12-01-2022

Installation Qualification(IQ)



Company (Name & Add) : POCT
Services

Customer (Name & Add) : Sahdev
Medical Centre
Shakti Nagar - Delhi - 110022

Contact Person : Mr. Gaurav

Contact Person : Mrs. - Jyoti

Telephone No. : 9310777135

Telephone No. : 7065123663

Name of instrument : **Microlab 300 LX** **Microlab 300 EX (with inbuilt printer)** (Select by \checkmark)

Serial no. : 17-43307

Installation Date : 18-05-2018

Installation (Perform the Following steps)


- Check Power Supply 230 V ($\pm 10V$)
- Check Earth ... 0.3 V (< 5.0 V)
- Room Temperature ... 25.2 ... ($15^{\circ}C$ to $30^{\circ}C$)
- Install Instrument on Flat & Dry Surface by leaving a gap between instrument & back wall
- Install waste Tube by connecting it from back side of instrument & attach waste container with tube.
- Install internal/external printer (If required)
- Install Power Supply by connecting power chord to the back side of instrument
- Start up the Analyser by switching on from backside power on button.
- Check display & wait for instrument to boot up/initialise. Press exit key to exit washing step.
- Check the keypad key functioning & adjust the display contrast from '+' '-' Key as per suitability
- Place distilled water under the sipper tube
- Check the aspiration of the system by pressing FLUSH key (approx Asp 1500 μ l in one cycle)
- Perform wash with cleaning solution & then with Distilled water (5 Cycles each) from FLUSH key

Jyoti
28/5/22

Operational Qualification (OQ)




- Set the System Parameters from Main Menu->PROGRAM->SYSTEM SETTINGS->Type Password
- Input the GENERAL details in the various fields as per picture (FIG 1) shown below by making selections with cursor keys for Lab Name, Date format, Date & Time.

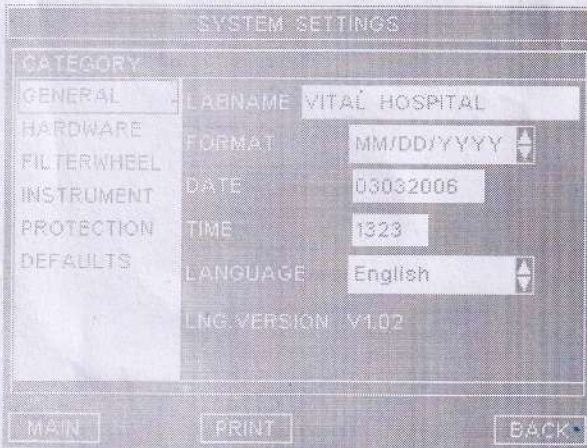

SYSTEM SETTINGS	
CATEGORY	
GENERAL	LABNAME VITAL HOSPITAL
HARDWARE	FORMAT MM/DD/YYYY
FILTERWHEEL	DATE 03032006
INSTRUMENT	TIME 1323
PROTECTION	LANGUAGE English
DEFAULTS	LNG VERSION V1.02


(FIG 1)

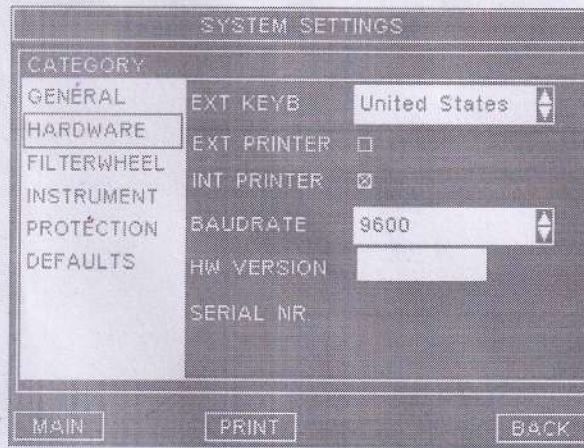

SYSTEM SETTINGS	
CATEGORY	
GENERAL	EXT KEYB United States
HARDWARE	EXT PRINTER <input type="checkbox"/>
FILTERWHEEL	INT PRINTER <input checked="" type="checkbox"/>
INSTRUMENT	BAUDRATE 9600
PROTECTION	HW VERSION
DEFAULTS	SERIAL NR.


(FIG 2)

- Set the Hardware Parameter & deactivate the printers (if inbuilt/external printers not available) as per picture (FIG 2) above. All entries are Autosaved.
- Program a user defined test: New, Edit, Del. from Main Menu->PROGRAM->Select TESTS->Type Password
- Press the softkey NEW to add a new test to the analyzer, or use the UP and DOWN keys to select a test and press the softkey EDIT to edit the test or DEL to delete the test.
- Input various technical parameters like Name, units, Wavelength, calibration etc as per requirement of test protocols as per below pictures (FIG 3 & FIG 4).Make Selection by using cursor
- All entries are autosaved.

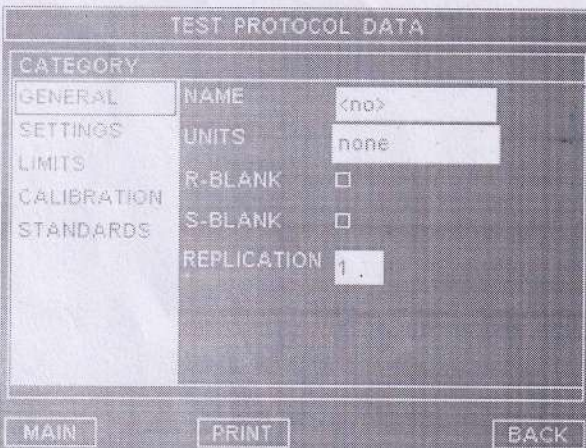

TEST PROTOCOL DATA	
CATEGORY	
GENERAL	NAME <no>
SETTINGS	UNITS none
LIMITS	R-BLANK <input type="checkbox"/>
CALIBRATION	S-BLANK <input type="checkbox"/>
STANDARDS	REPLICATION 1

(FIG 3)

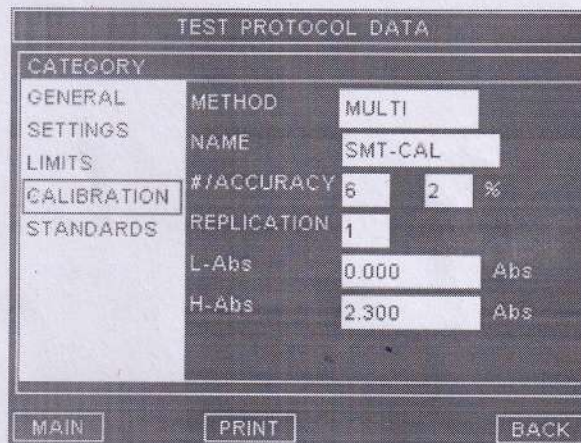

TEST PROTOCOL DATA	
CATEGORY	
GENERAL	METHOD MULTI
SETTINGS	NAME SMT-CAL
LIMITS	#/ACCURACY 6 2 %
CALIBRATION	REPLICATION 1
STANDARDS	L-Abs 0.000 Abs
	H-Abs 2.300 Abs


(FIG 4)

*Jays
28/5/22*

Operational Qualification (OQ)



- From the MAIN MENU, select MEASURE. Press ENTER. The below screen shows.

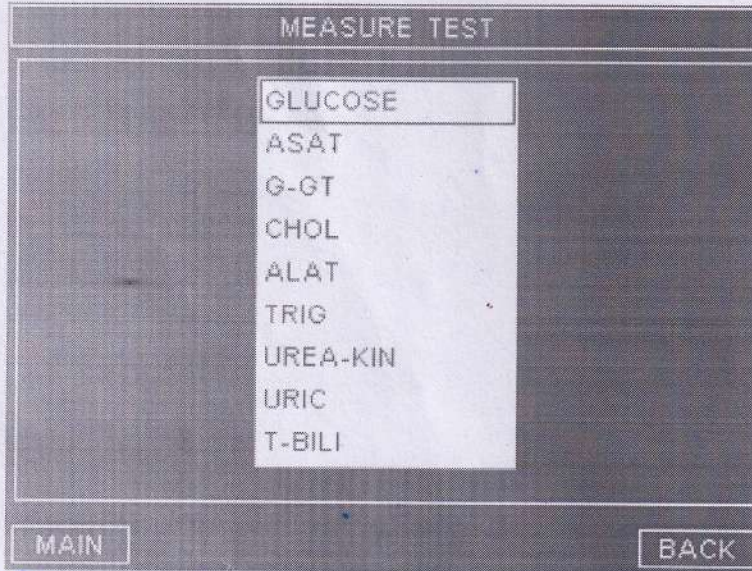

- Use the UP and DOWN arrow keys to select the required test. Press ENTER.
- Start the test and do water blank
- Run Reagent Blank for the test programmed (whichever test requires)
- Run Calibrations for programmed tests by using standards or calibrators (whichever test requires)
- System is now ready for performance check.

Jaya
28/5/22

PERFORMANCE QUALIFICATION (PQ)



- Run Reagent Blank
- Run Calibrations
- Run QC material for several clinical chemistry applications
(a few enzymes, a few substrate tests using customer's reagent)

Test	QC Range Level 1	Test Result	QC Range Level 2	Test Result
GLUCOSE	[68-93] 81	72	[158-218] 188	195
CHOL	[147-193] 170	1.81	[186-254] 220	236
ALT/GPT	[39-57] 48	51	[131-209] 170	168
AST/GOT	[31-45] 38	40	[177-263] 220	197
CREAT	[0.78-1.42] 1.10	0.93	[2.02-3.32] 2.67	1.92
UREA	[18-33] 26	28	[68-96] 82	91

Remarks:

We hereby certify that Instrument standardization / calibrations have been carried out under the Warranty/ AMC. Verified by evaluating controls before processing patients Samples and obtained results are satisfactory. Instrument is ready for regular use.

Technical acceptance

Date (dd-mm-yyyy) : 18-05-2018

Service Engineer/Application Person Name

Gantabudhi

Customer Name

Jayallas

Jay 18/5/2018

Signature :

Jay

Signature & Stamp

SOM DATT MEDICAL CENTRE
Polyclinic & Diagnostic Centre
Block,
Shakarpur, Delhi-110 092

Q-LINE BIOTECH PRIVATE LIMITED (Formerly known as "POCT Services Pvt. Ltd.")

Corp. Office: 20A (Basement), Main Shivaji Marg, Najafgarh Road, Near Moti Nagar Police Station, New Delhi-110015, INDIA. Tel.: 011-45577407
Regd. Office: 298-281, Transport Nagar, Kanpur Road, Adjacent Transport Nagar Metro Station, Lucknow-226023 (U.P.), INDIA. Tel.: 0522-2433023
E-mail: info@qlinebiotech.com | Website: www.qlinebiotech.com



PARASHAR MICRO MEASUREMENT (P) LTD
NABL Accredited Lab., Ph. No. : 0120-4252362
Range 17-43307
Cert. No. PMMI 731434
Cal. Date 31.01.22
Valid Upto 30.1.23 Sign Tap

MEASURE GLUCOSE TEST

MEASURE

MEASURED 07/06/2022

BATCH NUMBER 01-1140 31/12/2022

REPLICATION

CONTROL NAME

RESULT 93.4 mg/dl

Press accept/decline to validate result


DECLINE

PRINT

REPEAT

INFO

ACCEPT

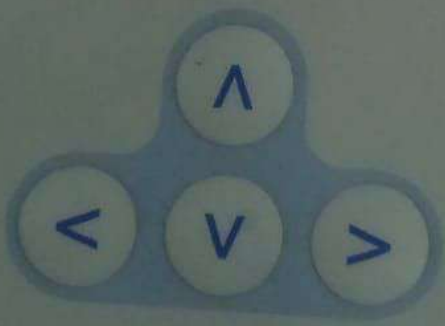



PARASHAR MICRO MEASUREMENT (P) LTD
NABL Accredited Lab. No. 5129-412292
Regn. No. 17E43307
Cert. No. (PMA) 731434
Cal. Date 31.01.22
Valid Upto 30.1.23 by Tap.

MEASURE GLUCOSE TEST

MEASURE

MEASURED 07/06/2022

BATCH NUMBER 02-2150 31/08/2023

REPLICATION

CONTROL NAME

RESULT 225.1 mg/dl

Press accept/decline to validate result

+
-



paper
flush
prime
meas

^
< V >

1 2 3 4 5 6 7 8 9 0 ←
Q W E R T Y U I O P
A S D F G H J K L
Z X C V B N M .
- , ; ' & * () _ { } ~