

# QC Chart


Test name: ALP

QC Lot: 112196

Concentration: Normal

Run date: From 04/01/2022 To 04/30/2022

	N	Mean	SD	CV
Standard QC Value	-	71.08	6.04	8.50%
Floating QC Value	27	72.13	4.88	6.76%

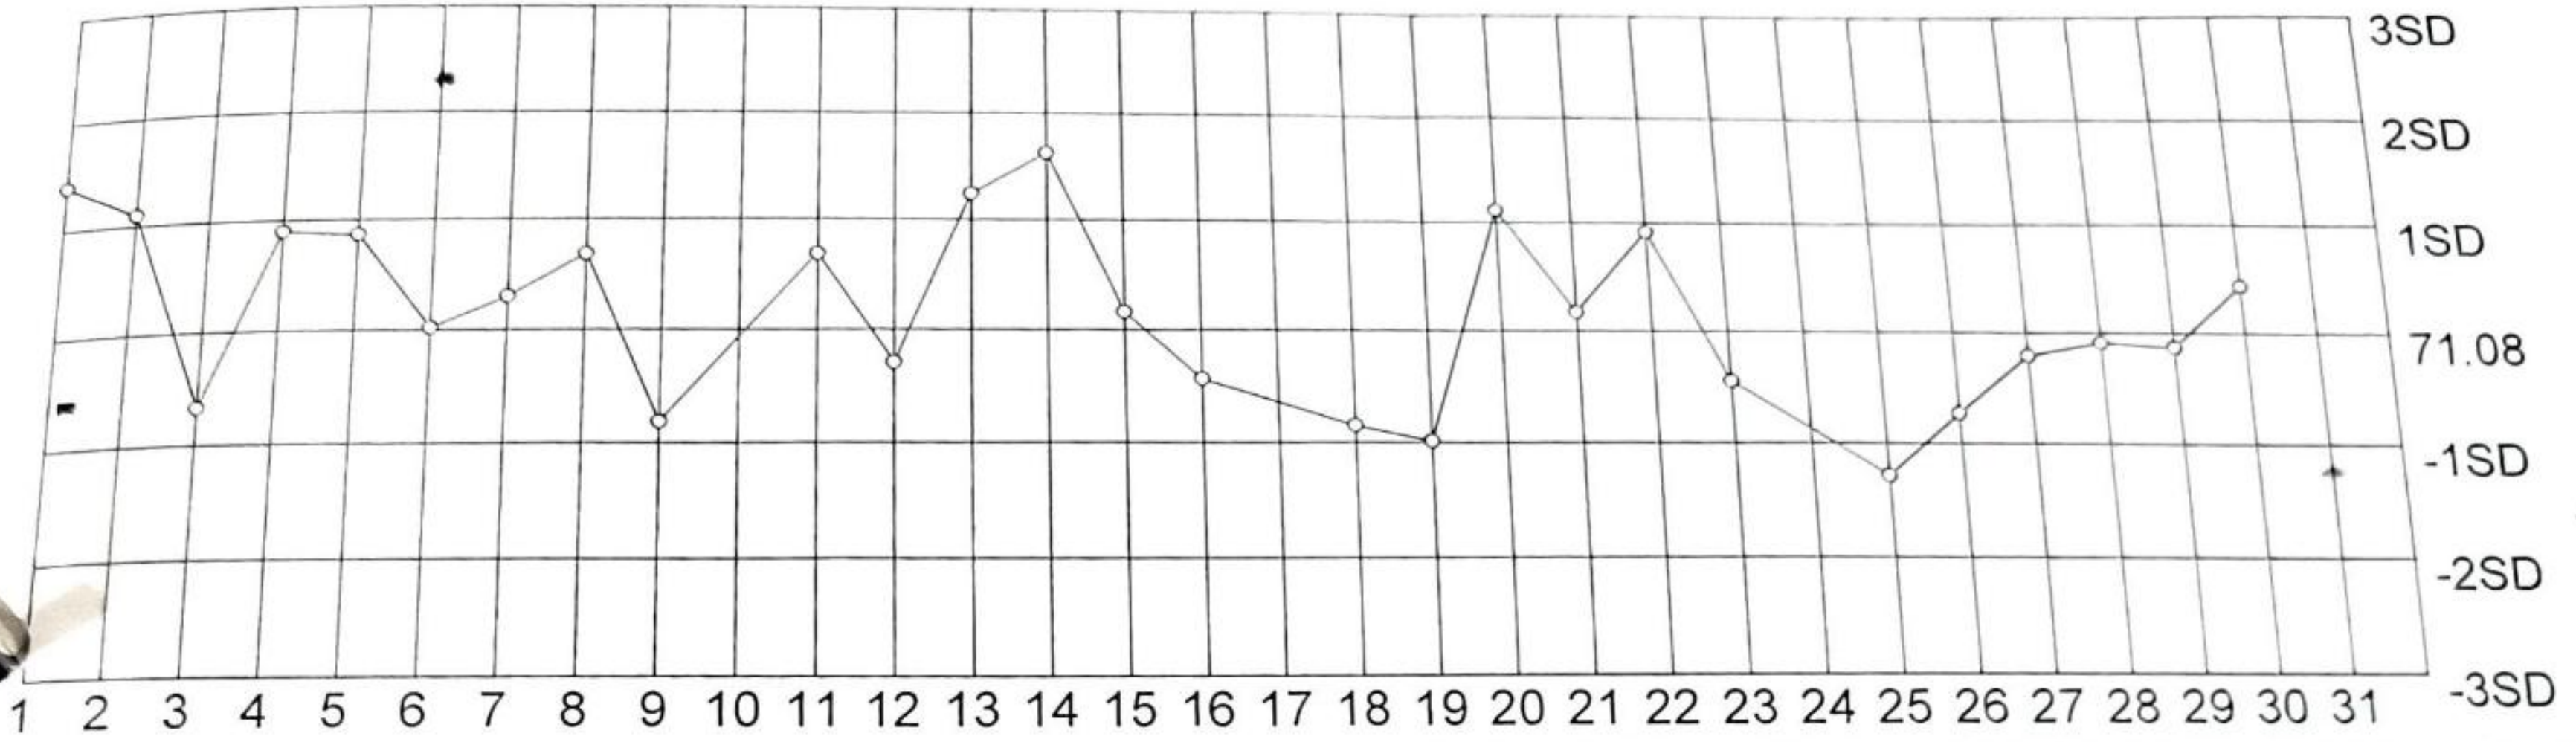

No.	Run date	Result	Status
1	04/01/2022	79.57	+2SD
2	04/02/2022	77.74	+2SD
3	04/03/2022	67.04	-1SD
4	04/04/2022	76.49	+1SD
5	04/05/2022	76.30	+1SD
6	04/06/2022	71.21	+1SD
7	04/07/2022	72.90	+1SD
8	04/08/2022	75.20	+1SD
9	04/09/2022	66.15	-1SD
10	04/11/2022	75.20	+1SD
11	04/12/2022	69.30	-1SD
12	04/13/2022	78.57	+2SD
13	04/14/2022	80.89	+2SD
14	04/15/2022	72.04	+1SD
15	04/16/2022	68.46	-1SD
16	04/18/2022	65.97	-1SD
17	04/19/2022	65.13	-1SD
18	04/20/2022	77.80	+2SD
19	04/21/2022	72.11	+1SD
20	04/22/2022	76.58	+1SD
21	04/23/2022	68.39	-1SD
22	04/25/2022	63.33	-2SD
23	04/26/2022	66.70	-1SD
24	04/27/2022	69.83	-1SD
25	04/28/2022	70.56	-1SD
26	04/29/2022	70.31	-1SD
27	04/30/2022	73.69	+1SD
28			
29			
30			
31			

*[Handwritten signature]*

# QC Chart


Test name: CAL

QC Lot: 112196

Concentration: Normal

Run date: From 04/01/2022 To 04/30/2022

	N	Mean	SD	CV
Standard QC Value	-	8.55	0.43	5.03%
Floating QC Value	28	8.56	0.36	4.16%

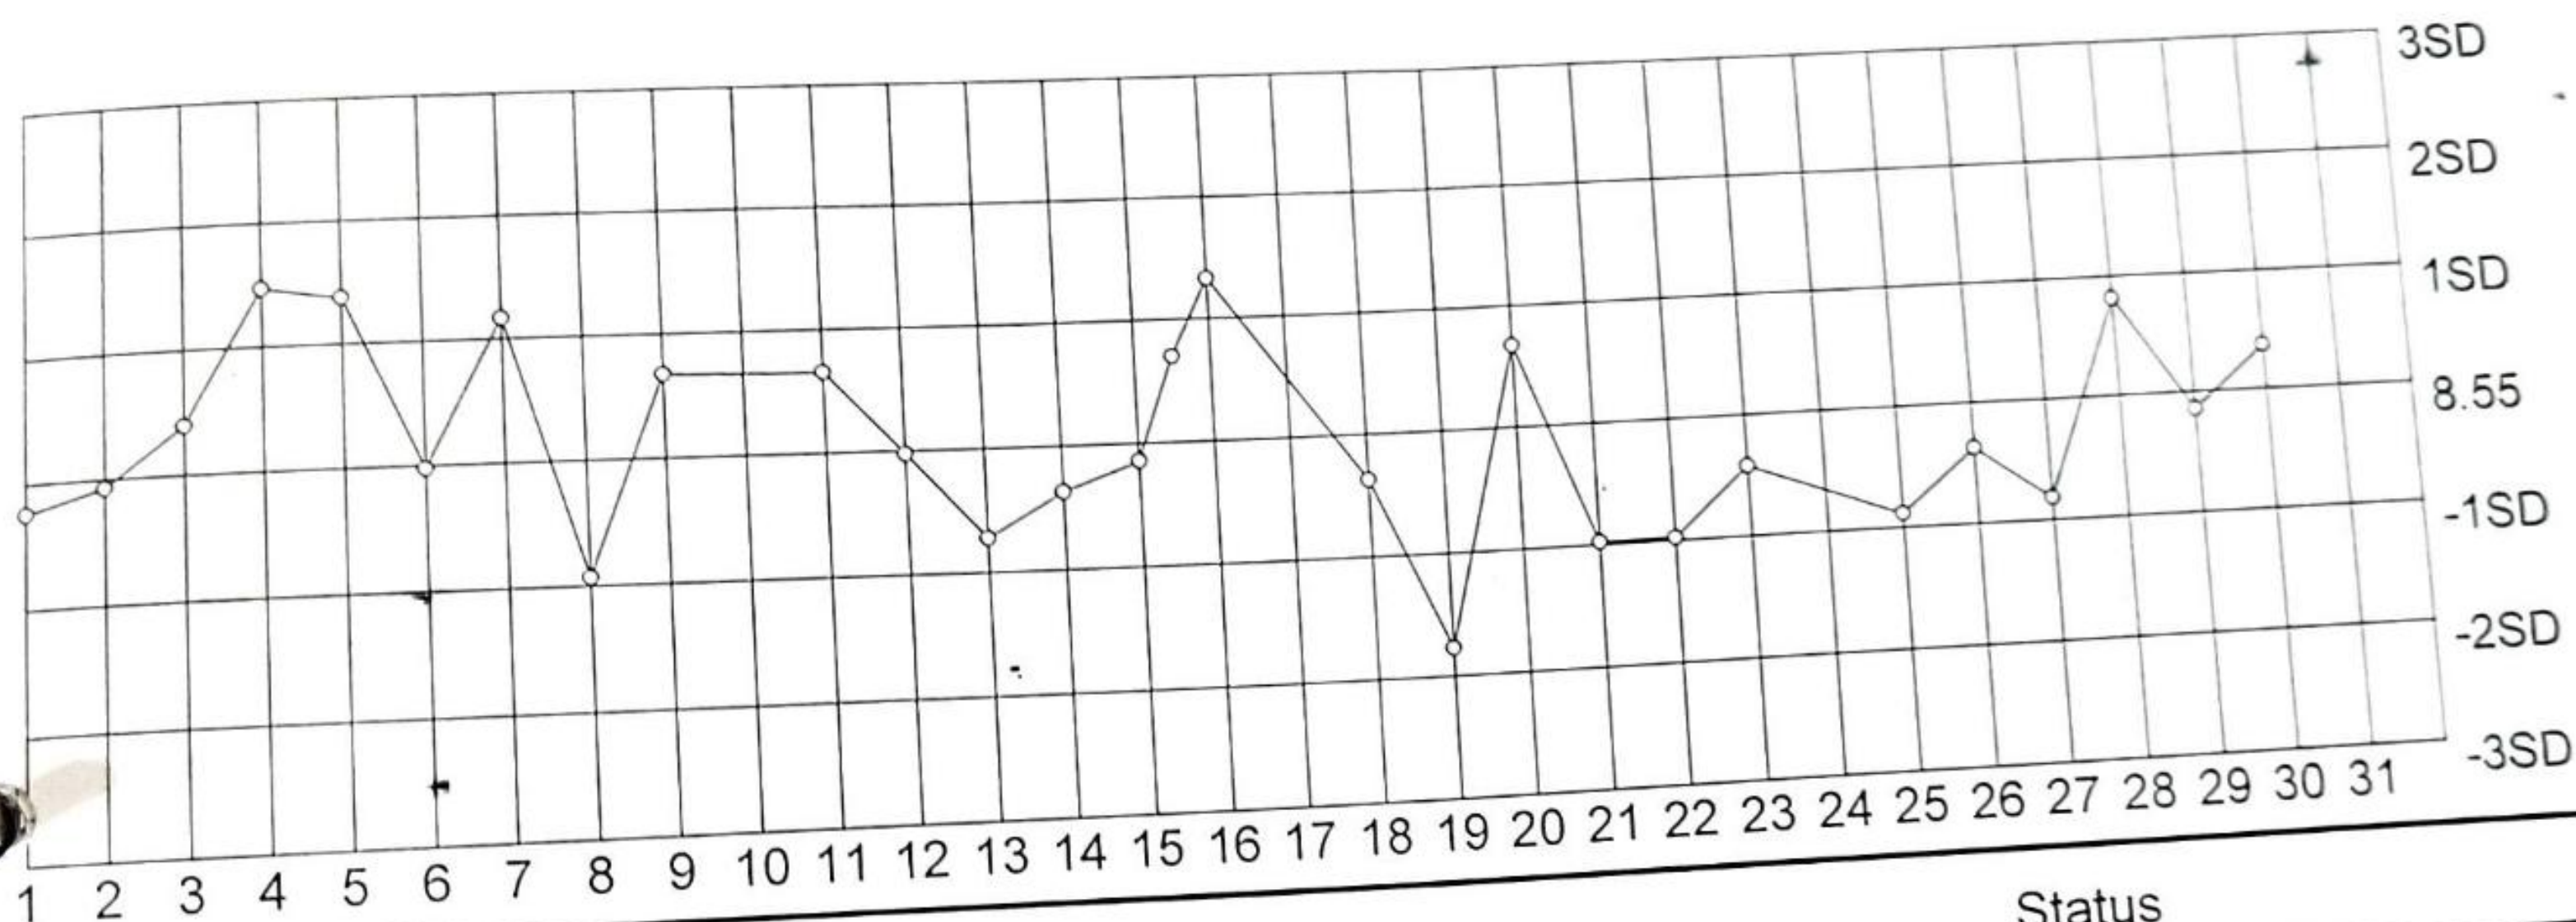

No.	Run date	Result	Status
1	04/01/2022	8.45	-1SD
2	04/02/2022	8.52	-1SD
3	04/03/2022	8.72	+1SD
4	04/04/2022	9.18	+2SD
5	04/05/2022	9.14	+2SD
6	04/06/2022	8.54	-1SD
7	04/07/2022	9.05	+2SD
8	04/08/2022	8.15	-1SD
9	04/09/2022	8.84	+1SD
10	04/10/2022	8.83	+1SD
11	04/11/2022	8.54	-1SD
12	04/12/2022	8.54	-1SD
13	04/13/2022	8.24	-1SD
14	04/14/2022	8.39	-1SD
15	04/15/2022	8.49	+1SD
16	04/15/2022	8.85	+2SD
17	04/16/2022	9.12	-1SD
18	04/18/2022	8.39	-2SD
19	04/19/2022	7.79	+1SD
20	04/20/2022	8.84	-1SD
21	04/21/2022	8.13	-1SD
22	04/22/2022	8.13	-1SD
23	04/23/2022	8.37	-1SD
24	04/25/2022	8.17	-1SD
25	04/26/2022	8.39	-1SD
26	04/27/2022	8.20	+1SD
27	04/28/2022	8.90	-1SD
28	04/29/2022	8.49	+1SD
29	04/30/2022	8.71	
30			
31			

*Handwritten signature*

# QC Chart


Test name: CHOL

QC Lot: 112196

Concentration: Normal

Run date: From 04/01/2022 To 04/30/2022

	N	Mean	SD	CV
Standard QC Value	-	120.00	10.20	8.50%
Floating QC Value	27	123.70	6.21	5.02%

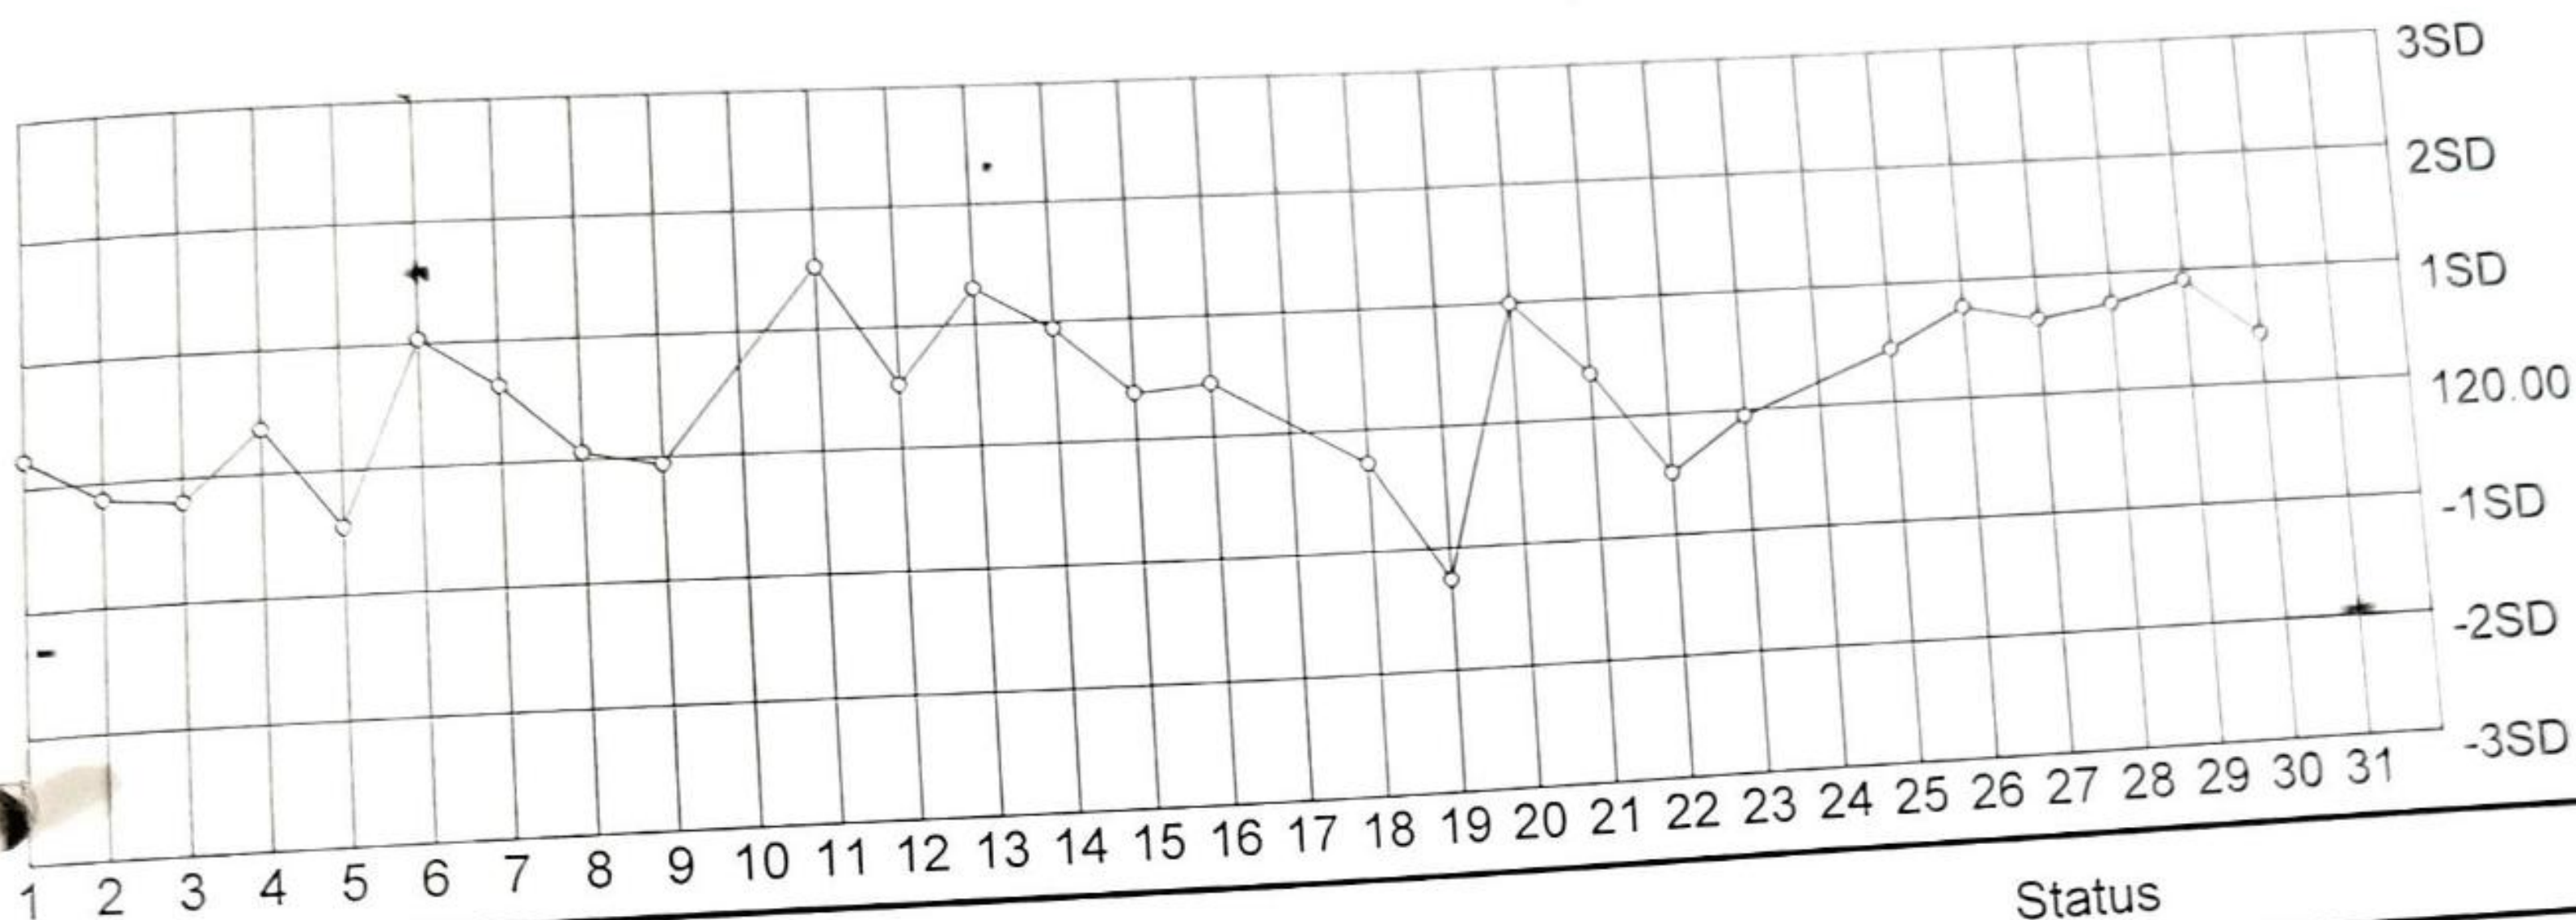

No.	Run date	Result	Status
1	04/01/2022	122.27	+1SD
2	04/02/2022	118.59	-1SD
3	04/03/2022	118.00	-1SD
4	04/04/2022	123.67	+1SD
5	04/05/2022	115.32	-1SD
6	04/06/2022	130.56	+2SD
7	04/07/2022	126.40	+1SD
8	04/08/2022	120.61	-1SD
9	04/09/2022	119.41	+2SD
10	04/11/2022	135.44	+1SD
11	04/12/2022	125.31	+2SD
12	04/13/2022	133.21	+1SD
13	04/14/2022	129.59	+1SD
14	04/15/2022	123.93	+1SD
15	04/16/2022	124.47	-1SD
16	04/18/2022	117.19	-2SD
17	04/19/2022	107.17	+1SD
18	04/20/2022	130.10	+1SD
19	04/21/2022	123.76	-1SD
20	04/22/2022	115.05	-1SD
21	04/23/2022	119.52	+1SD
22	04/25/2022	124.59	+1SD
23	04/26/2022	127.91	+1SD
24	04/27/2022	126.52	+1SD
25	04/28/2022	127.54	+1SD
26	04/29/2022	129.30	+1SD
27	04/30/2022	124.35	+1SD
28	<del>04/30/2022</del>	<del>8.74</del>	<del>+1SD</del>
29			
30			
31			

*[Handwritten signature]*

This test has been conducted on AutoQuant2

# QC Chart


at name GREAT

QC Lot 112196

Concentration Normal

Run date From 04/01/2022 To 04/30/2022

	N	Mean	SD	CV
Standard QC Value	-	1.15	0.10	8.70%
Floating QC Value	28	1.15	0.09	7.83%

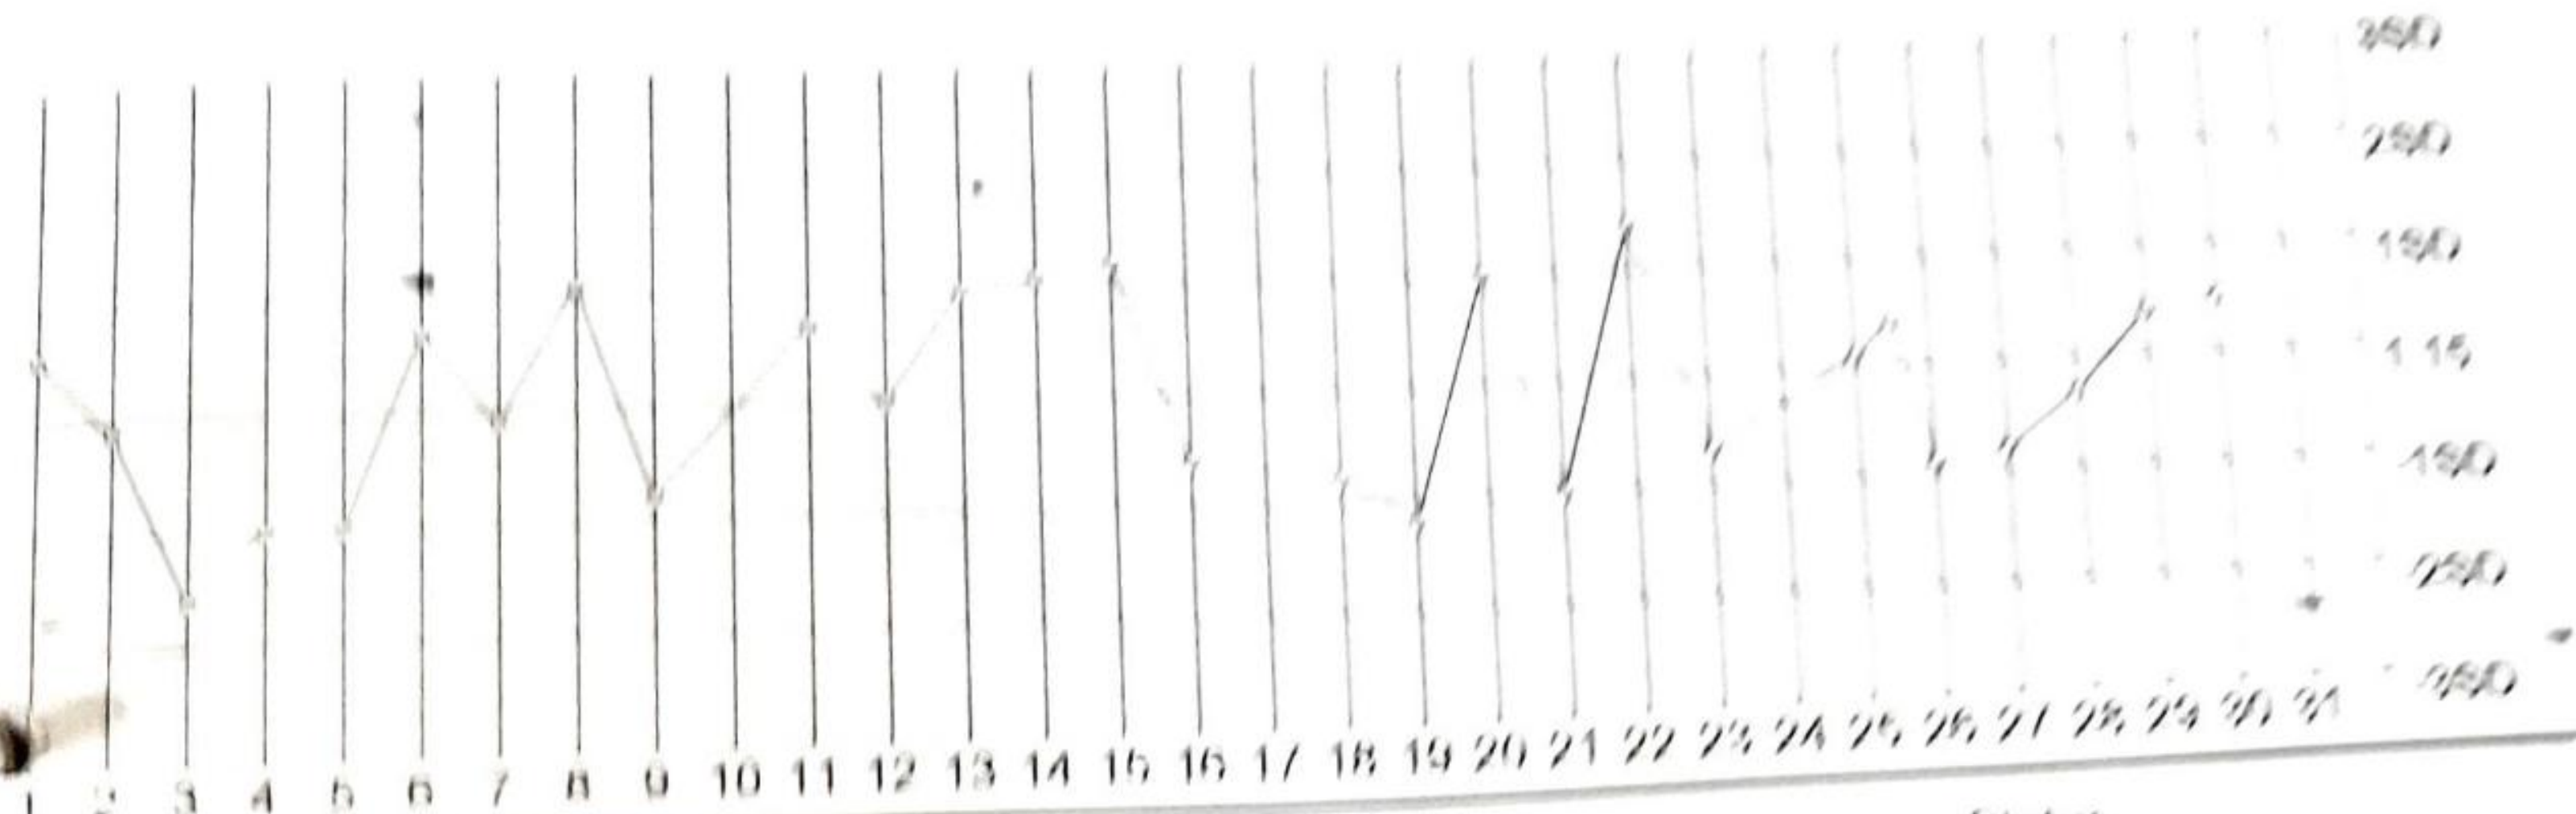

No	Run date	Result	Status
1	04/01/2022	1.21	+1SD
2	04/02/2022	1.14	-1SD
3	04/03/2022	0.99	-2SD
4	04/04/2022	1.05	-1SD
5	04/05/2022	1.05	-1SD
6	04/06/2022	1.22	+1SD
7	04/07/2022	1.14	-1SD
8	04/08/2022	1.26	+2SD
9	04/09/2022	1.07	-1SD
10	04/11/2022	1.22	+1SD
11	04/12/2022	1.15	-1SD
12	04/13/2022	1.25	+2SD
13	04/14/2022	1.26	+2SD
14	04/15/2022	1.27	+2SD
15	04/16/2022	1.09	-1SD
16	04/18/2022	1.07	-2SD
17	04/19/2022	1.03	+1SD
18	04/20/2022	1.25	-1SD
19	04/21/2022	1.05	+2SD
20	04/22/2022	1.29	-1SD
21	04/23/2022	1.08	+1SD
22	04/25/2022	1.16	+1SD
23	04/25/2022	1.19	-1SD
24	04/26/2022	1.06	-1SD
25	04/27/2022	1.07	-1SD
26	04/28/2022	1.12	+1SD
27	04/29/2022	1.19	+1SD
28	04/30/2022	1.20	+1SD
29			
30			
31			

*Handwritten signature*

This test has been conducted on AutoQuant2


Test name: DBIL

QC Lot: 112196

Concentration: Normal

Run date: From 04/01/2022 To 04/30/2022

	N	Mean	SD	CV
Standard QC Value	-	0.66	0.10	15.15%
Floating QC Value	27	0.65	0.07	10.15%

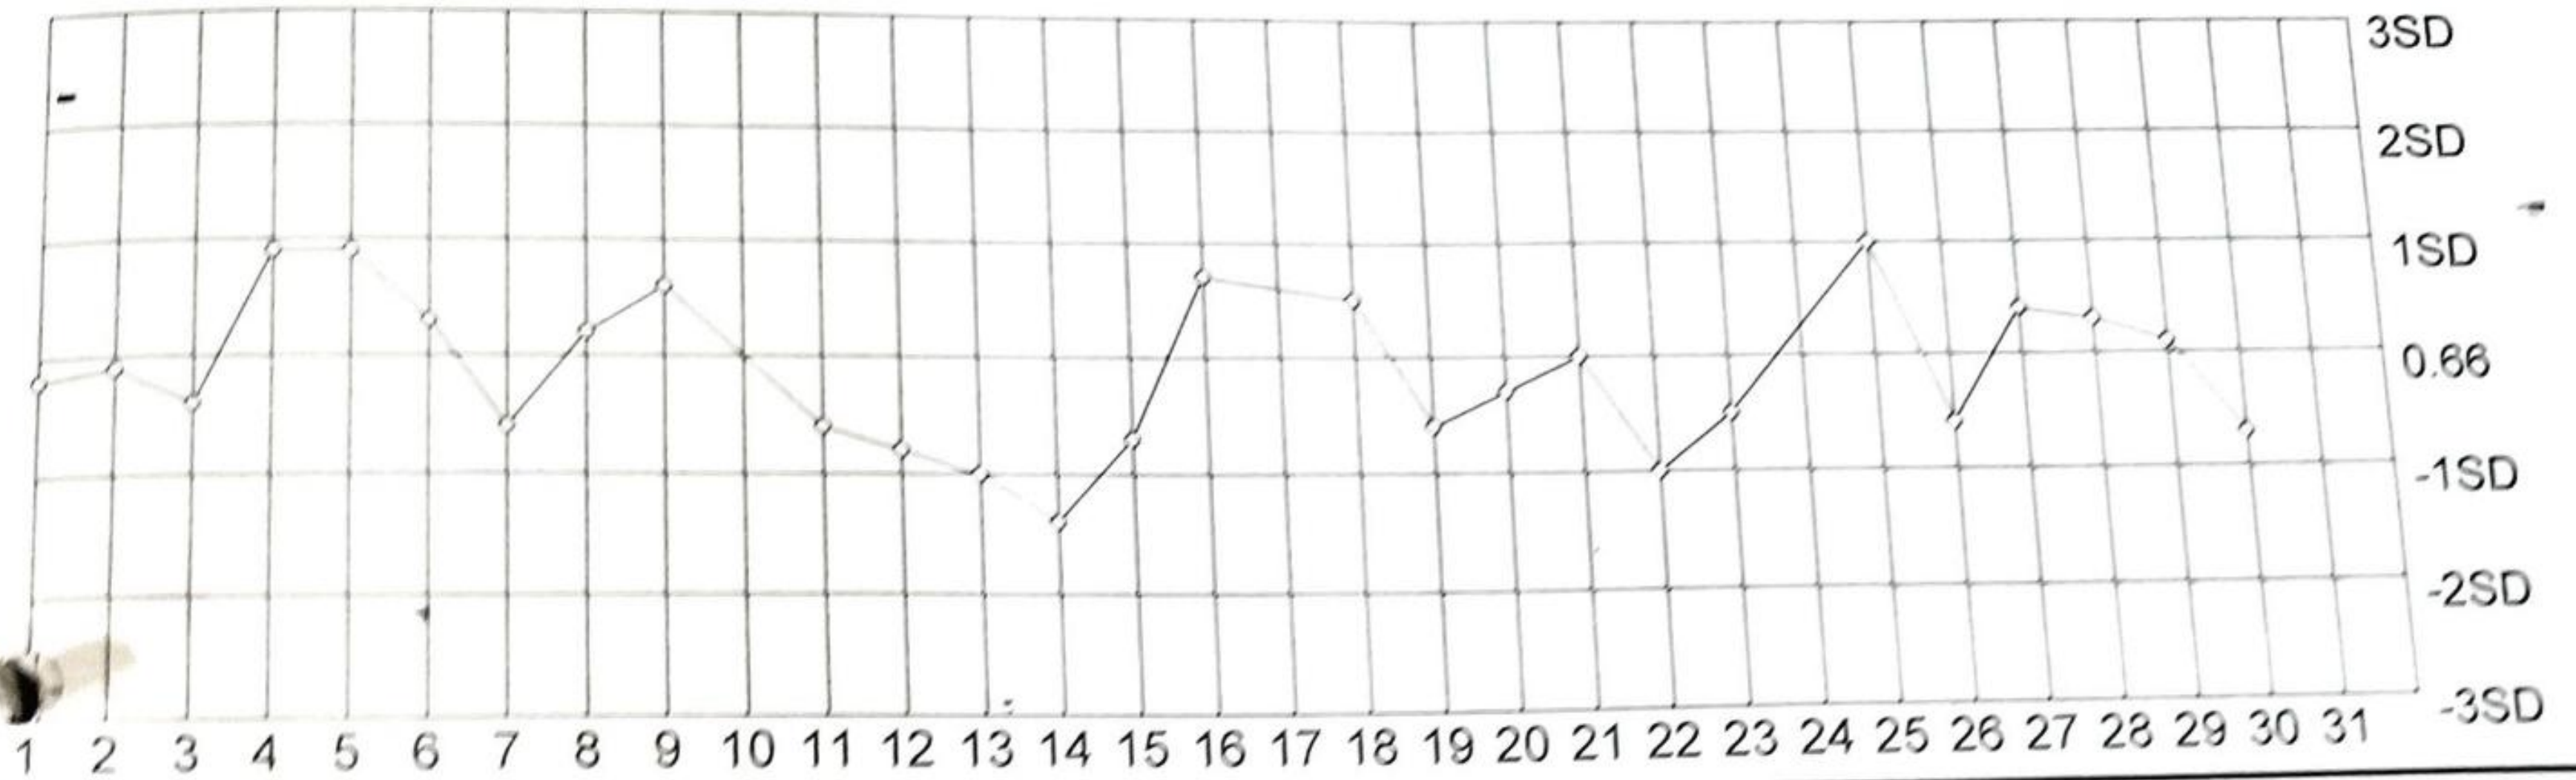

No.	Run date	Result	Status
1	04/01/2022	0.64	-1SD
2	04/02/2022	0.65	-1SD
3	04/03/2022	0.62	-1SD
4	04/04/2022	0.75	+1SD
5	04/05/2022	0.75	+1SD
6	04/06/2022	0.69	+1SD
7	04/07/2022	0.60	-1SD
8	04/08/2022	0.68	+1SD
9	04/09/2022	0.72	+1SD
10	04/11/2022	0.60	-1SD
11	04/12/2022	0.58	-1SD
12	04/13/2022	0.56	-2SD
13	04/14/2022	0.52	-1SD
14	04/15/2022	0.59	+1SD
15	04/16/2022	0.73	+1SD
16	04/18/2022	0.71	-1SD
17	04/19/2022	0.60	-1SD
18	04/20/2022	0.63	-1SD
19	04/21/2022	0.66	-1SD
20	04/22/2022	0.56	-1SD
21	04/23/2022	0.61	+1SD
22	04/25/2022	0.76	-1SD
23	04/26/2022	0.60	+1SD
24	04/27/2022	0.70	+1SD
25	04/28/2022	0.69	+1SD
26	04/29/2022	0.67	-1SD
27	04/30/2022	0.59	+1SD
28	04/30/2022	1.20	-
29			
30			
31			

*Handwritten signature*

# QC Chart


Test name: SGOT

QC Lot: 112196

Concentration: Normal

Run date From 04/01/2022 To 04/30/2022

	N	Mean	SD	CV
Standard QC Value	-	37.50	3.19	8.51%
Floating QC Value	27	38.60	2.70	7.00%

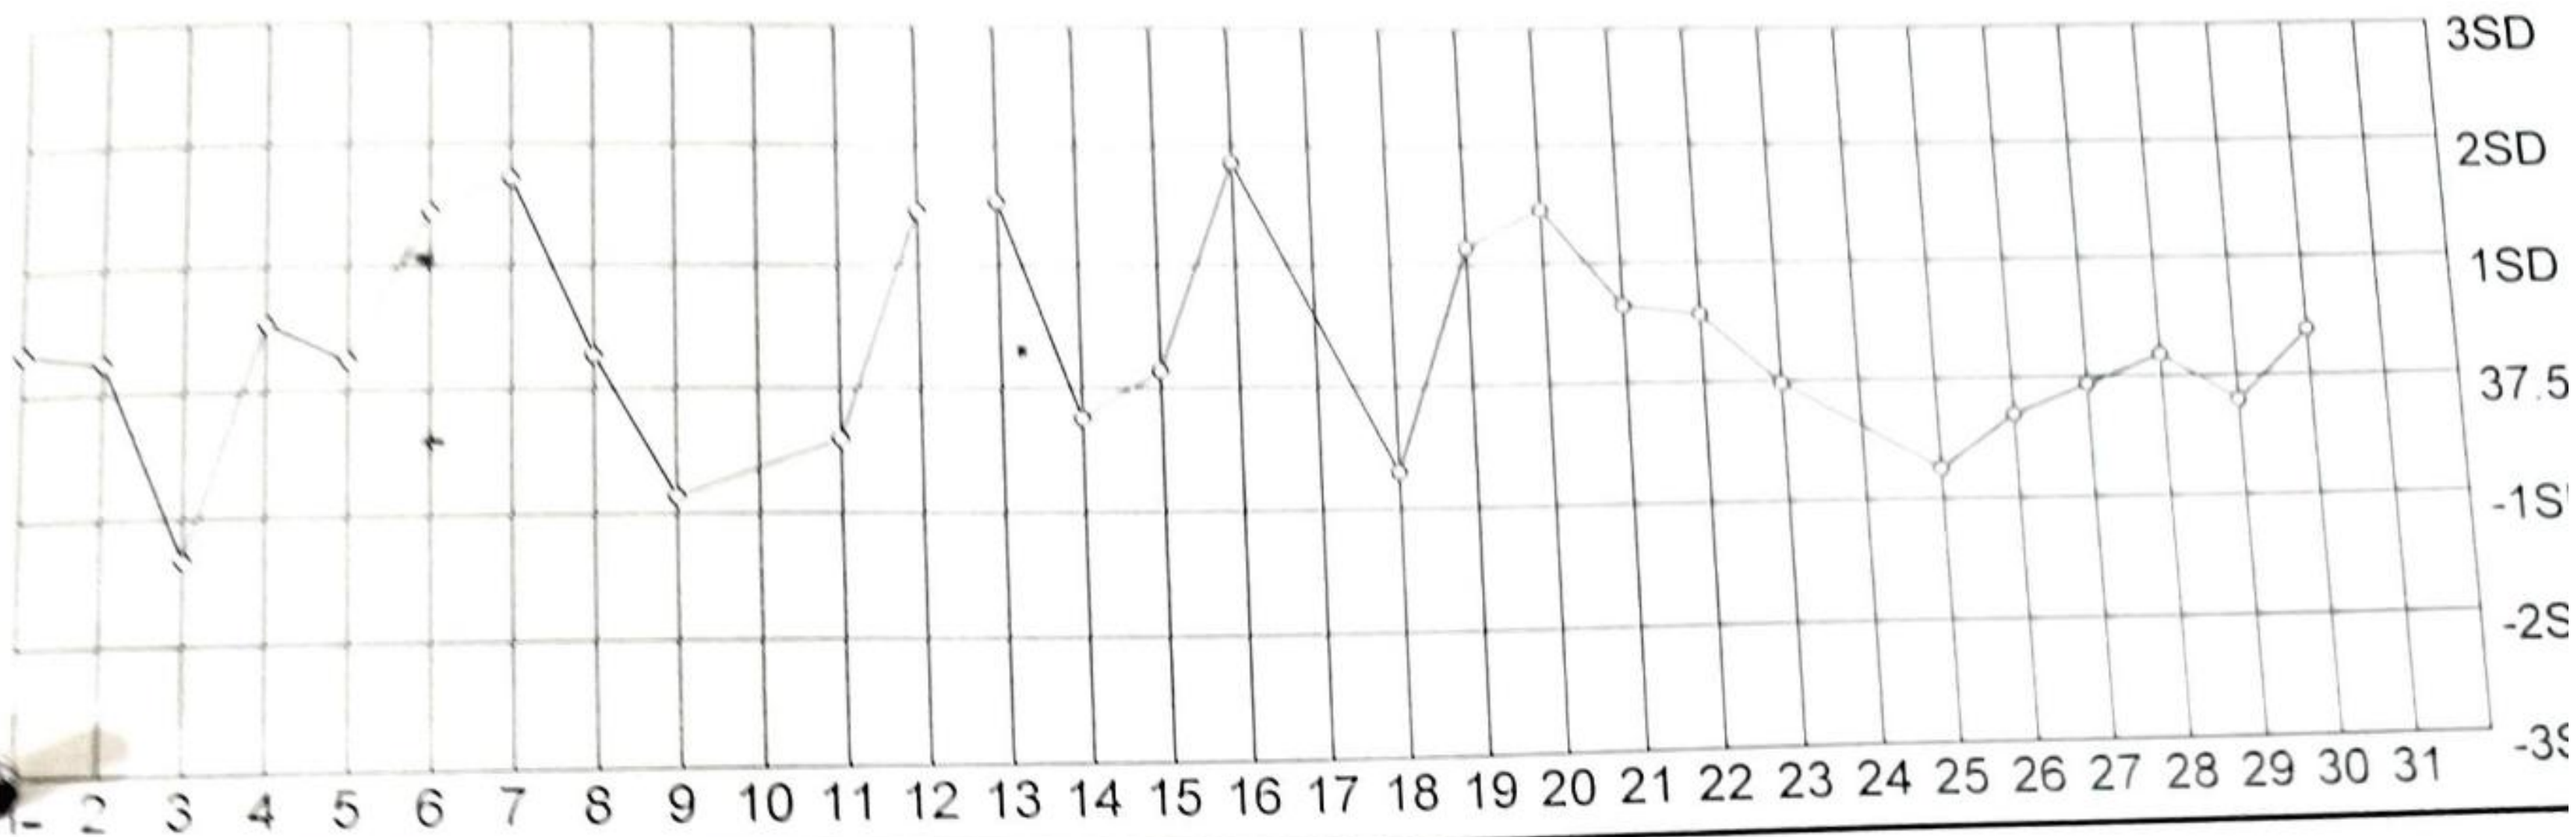

No.	Run date	Result	Status
1	04/01/2022	38.59	+1SD
2	04/02/2022	38.27	+1SD
3	04/03/2022	33.25	-2SD
4	04/04/2022	39.22	+1SD
5	04/05/2022	38.27	+1SD
6	04/06/2022	42.11	+2SD
7	04/07/2022	42.97	+2SD
8	04/08/2022	38.37	+1SD
9	04/09/2022	34.75	-1SD
10	04/11/2022	36.20	-1SD
11	04/12/2022	42.14	+2SD
12	04/13/2022	42.38	+2SD
13	04/14/2022	36.72	-1SD
14	04/15/2022	37.95	+1SD
15	04/16/2022	43.43	+2SD
16	04/18/2022	35.27	-1SD
17	04/19/2022	41.14	+2SD
18	04/20/2022	42.15	+2SD
19	04/21/2022	39.55	+1SD
20	04/22/2022	39.30	+1SD
21	04/23/2022	37.46	-1SD
22	04/25/2022	35.12	-1SD
23	04/26/2022	36.53	-1SD
24	04/27/2022	37.31	-1SD
25	04/28/2022	38.09	+1SD
26	04/29/2022	36.84	+1SD
27	04/30/2022	38.71	+1SD
28	<del>04/30/2022</del>	<del>1.20</del>	
29			
30			

# QC Chart


Test name: GLUC

QC Lot: 112196

Run date: From 04/01/2022 To 04/30/2022

Concentration: Normal

Standard QC Value	N	Mean	SD	CV
	-	96.50	8.20	8.50%
Floating QC Value	26	96.96	4.00	4.12%

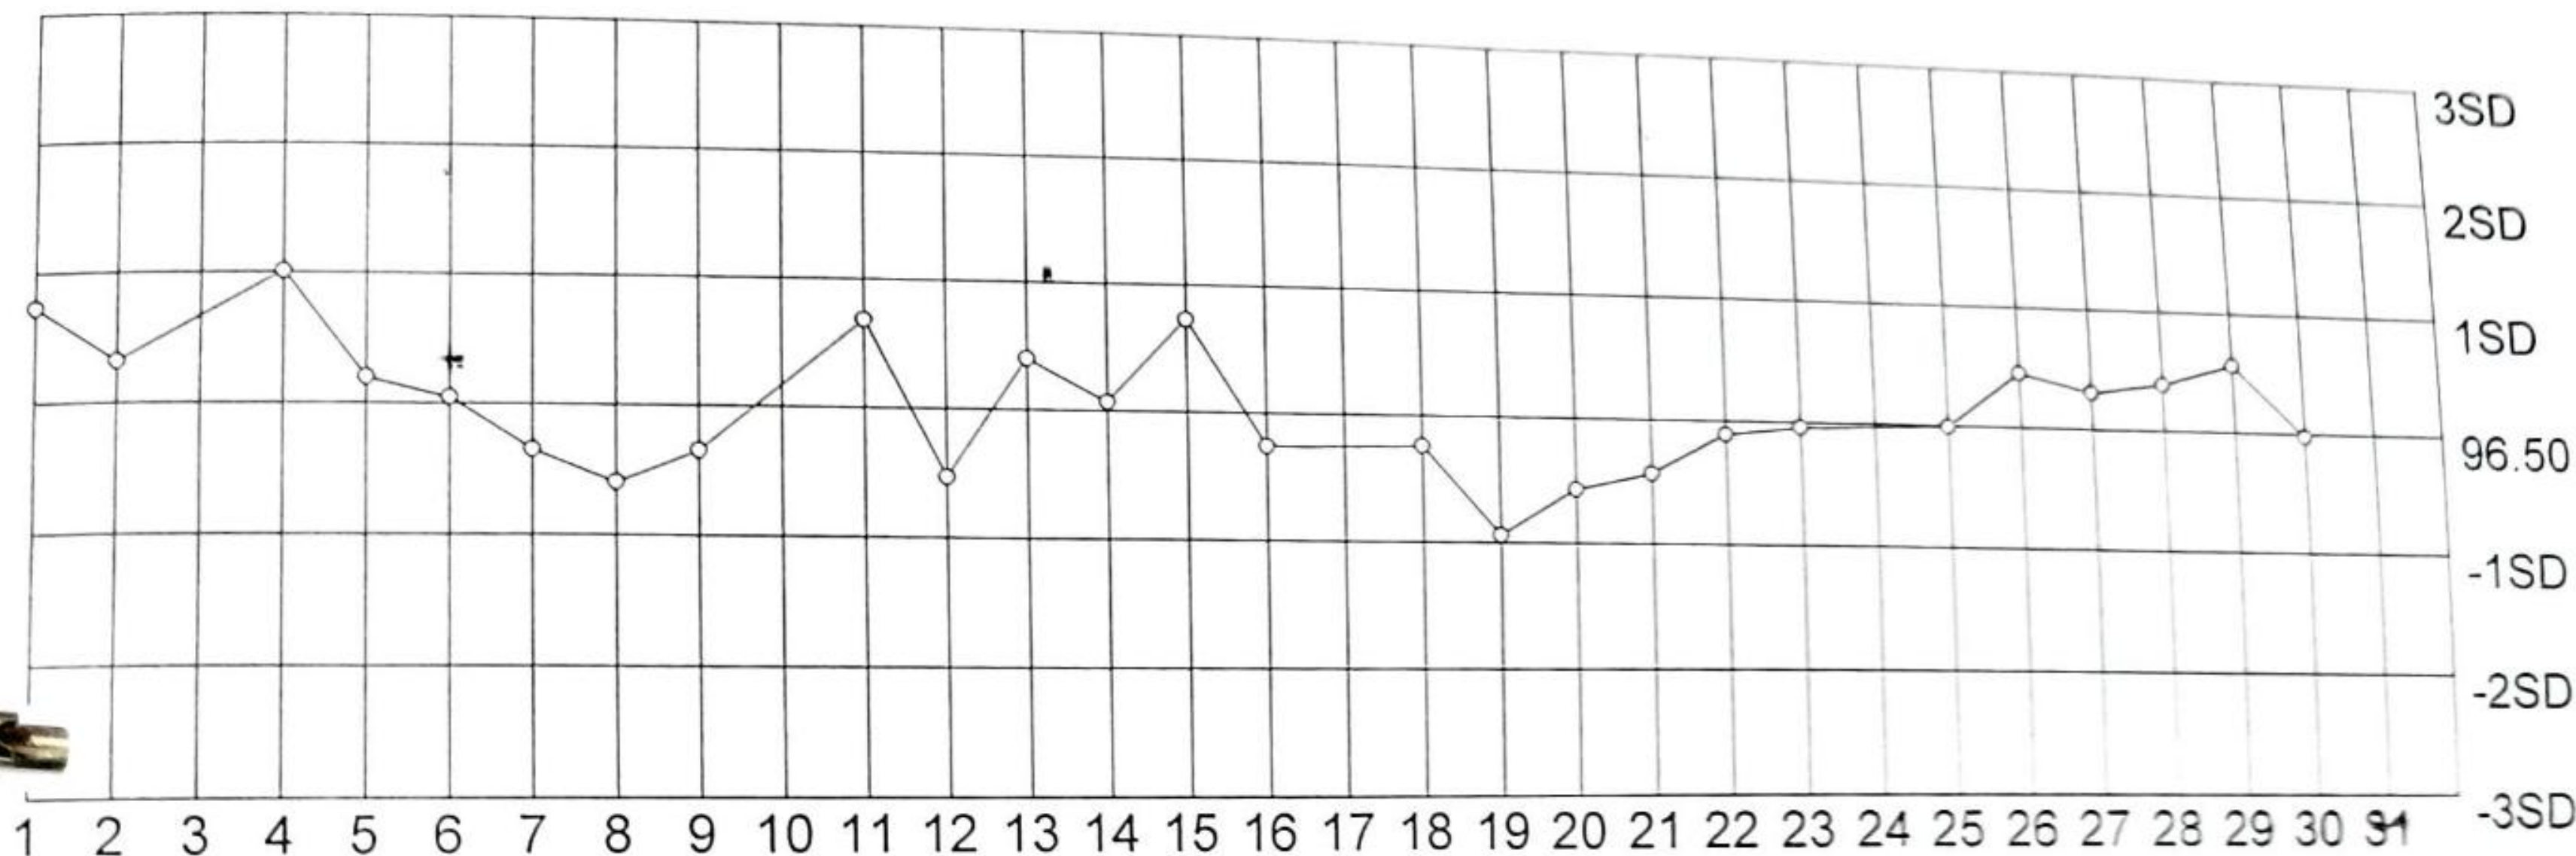

No.	Run date	Result	Status
1	04/01/2022	102.49	+1SD
2	04/02/2022	99.13	+1SD
3	04/04/2022	104.77	+2SD
4	04/05/2022	98.12	+1SD
5	04/06/2022	96.89	+1SD
6	04/07/2022	93.65	-1SD
7	04/08/2022	91.64	-1SD
8	04/09/2022	93.68	-1SD
9	04/11/2022	102.09	+1SD
10	04/12/2022	92.13	-1SD
11	04/13/2022	99.79	+1SD
12	04/14/2022	97.04	+1SD
13	04/15/2022	102.46	-1SD
14	04/16/2022	94.40	-1SD
15	04/18/2022	94.54	-1SD
16	04/19/2022	88.80	-1SD
17	04/20/2022	91.84	-1SD
18	04/21/2022	92.94	-1SD
19	04/22/2022	95.62	-1SD
20	04/23/2022	96.18	-1SD
21	04/25/2022	96.48	+1SD
22	04/26/2022	100.21	+1SD
23	04/27/2022	99.02	+1SD
24	04/28/2022	99.70	+1SD
25	04/29/2022	101.13	-1SD
26	04/30/2022	96.33	-1SD
27	04/30/2022	96.59	+1SD
28	04/30/2022	96.20	
29			
30			
31			

*Handwritten signature*

# QC Chart


Test name: SGPT

QC Lot: 112196

Concentration: Normal

Run date: From 04/01/2022 To 04/30/2022

	N	Mean	SD	CV
Standard QC Value	-	37.50	3.19	8.51%
Floating QC Value	27	37.20	2.53	6.81%

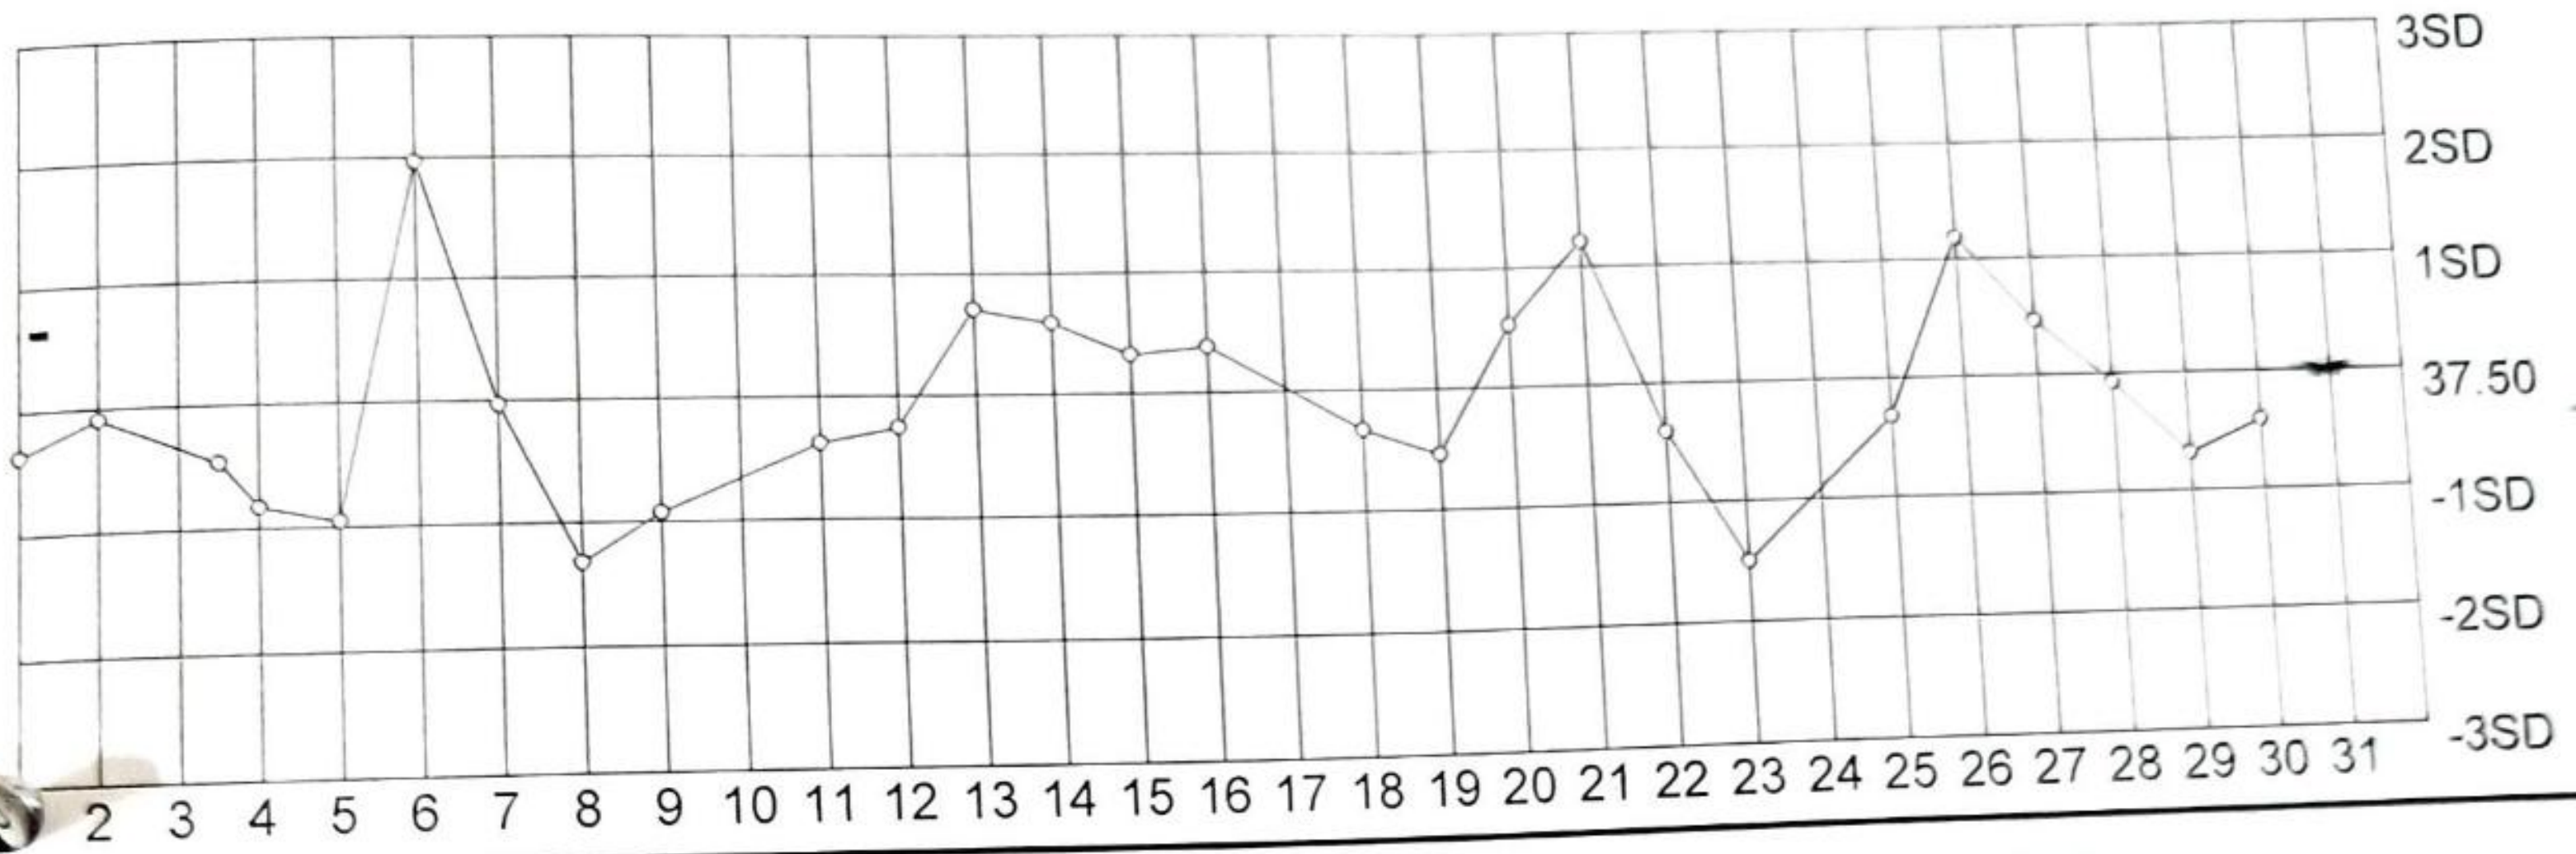

No.	Run date	Result	Status
1	<del>04/01/2022</del>	36.34	-1SD
2	04/02/2022	37.22	-1SD
3	04/03/2022	36.03	-1SD
4	04/04/2022	34.86	-1SD
5	04/05/2022	34.47	+2SD
6	04/06/2022	43.77	-1SD
7	04/07/2022	37.39	-2SD
8	04/08/2022	33.28	-1SD
9	04/09/2022	34.55	-1SD
10	04/11/2022	36.29	-1SD
11	04/12/2022	36.67	+1SD
12	04/13/2022	39.76	+1SD
13	04/14/2022	39.38	+1SD
14	04/15/2022	38.53	+1SD
15	04/16/2022	38.71	-1SD
16	04/18/2022	36.46	-1SD
17	04/19/2022	35.77	+1SD
18	04/20/2022	39.17	+2SD
19	04/21/2022	41.37	-1SD
20	04/22/2022	36.21	-2SD
21	04/23/2022	32.71	-1SD
22	04/25/2022	36.47	+2SD
23	04/26/2022	41.28	+1SD
24	04/27/2022	38.97	-1SD
25	04/28/2022	37.26	-1SD
26	04/29/2022	35.33	-1SD
27	04/30/2022	36.19	+1SD
28	<del>04/30/2022</del>	<del>1.20</del>	
29			
30			
31			

*[Handwritten Signature]*

This test has been conducted on AutoQuant2



# QC Chart


Test name: TBIL

QC Lot: 112196

Concentration: Normal

Run date: From 04/01/2022 To 04/30/2022

	N	Mean	SD	CV
Standard QC Value	-	1.20	0.18	15.00%
Floating QC Value	27	1.25	0.13	10.22%

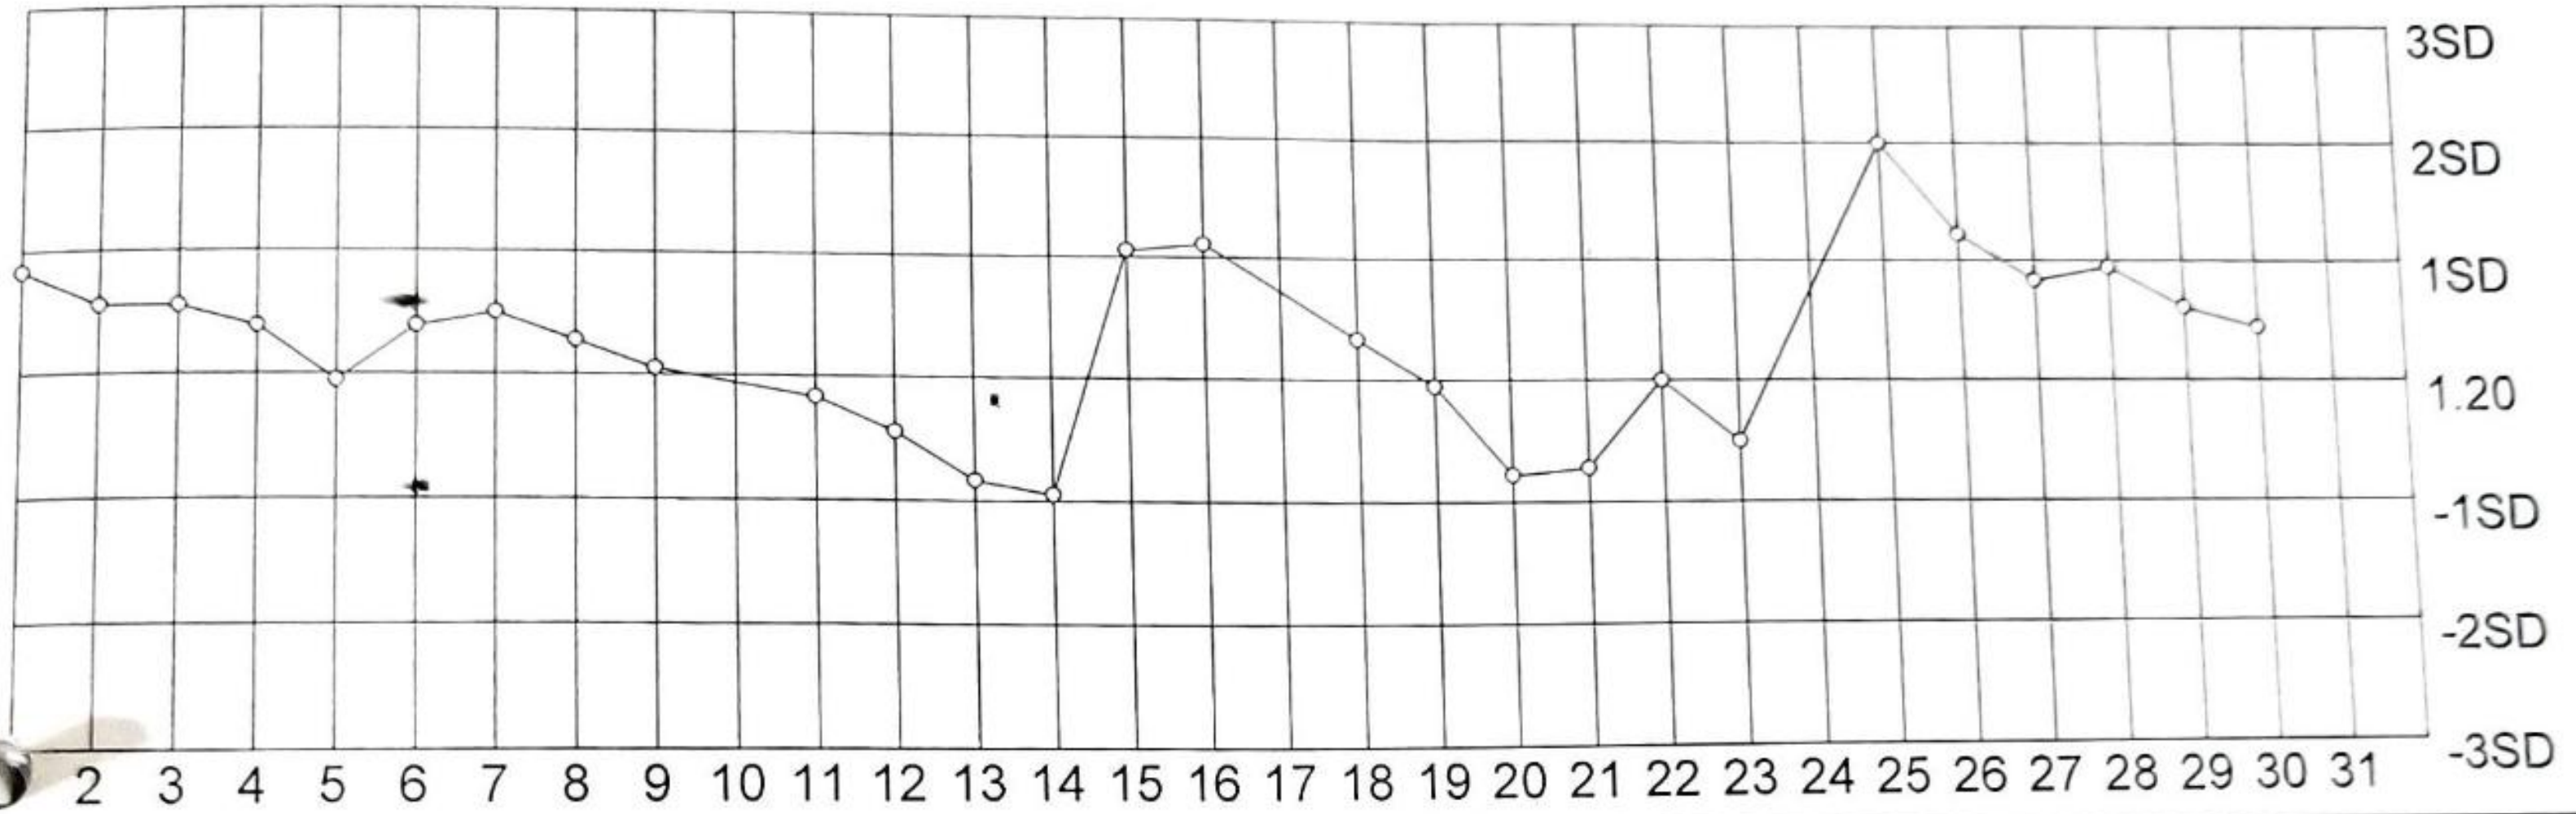

No.	Run date	Result	Status
1	04/01/2022	1.35	+1SD
2	04/02/2022	1.30	+1SD
3	04/03/2022	1.30	+1SD
4	04/04/2022	1.27	+1SD
5	04/05/2022	1.19	-1SD
6	04/06/2022	1.27	+1SD
7	04/07/2022	1.29	+1SD
8	04/08/2022	1.25	+1SD
9	04/09/2022	1.21	+1SD
10	04/11/2022	1.17	-1SD
11	04/12/2022	1.12	-1SD
12	04/13/2022	1.05	-1SD
13	04/14/2022	1.03	-1SD
14	04/15/2022	1.39	+2SD
15	04/16/2022	1.40	+2SD
16	04/18/2022	1.26	+1SD
17	04/19/2022	1.19	-1SD
18	04/20/2022	1.06	-1SD
19	04/21/2022	1.07	-1SD
20	04/22/2022	1.20	-1SD
21	04/23/2022	1.11	+2SD
22	04/25/2022	1.56	+2SD
23	04/26/2022	1.42	+1SD
24	04/27/2022	1.35	+1SD
25	04/28/2022	1.37	+1SD
26	04/29/2022	1.31	+1SD
27	04/30/2022	1.28	+1SD
28	04/30/2022	<del>1.20</del>	<del>+1SD</del>
29			
30			
31			

This test has been conducted on AutoQuant2

# QC Chart


Test name: TG

QC Lot: 112196

Concentration: Normal

Run date: From 04/01/2022 To 04/30/2022

	N	Mean	SD	CV
Standard QC Value	-	118.00	10.03	8.50%
Floating QC Value	27	113.86	6.97	6.12%

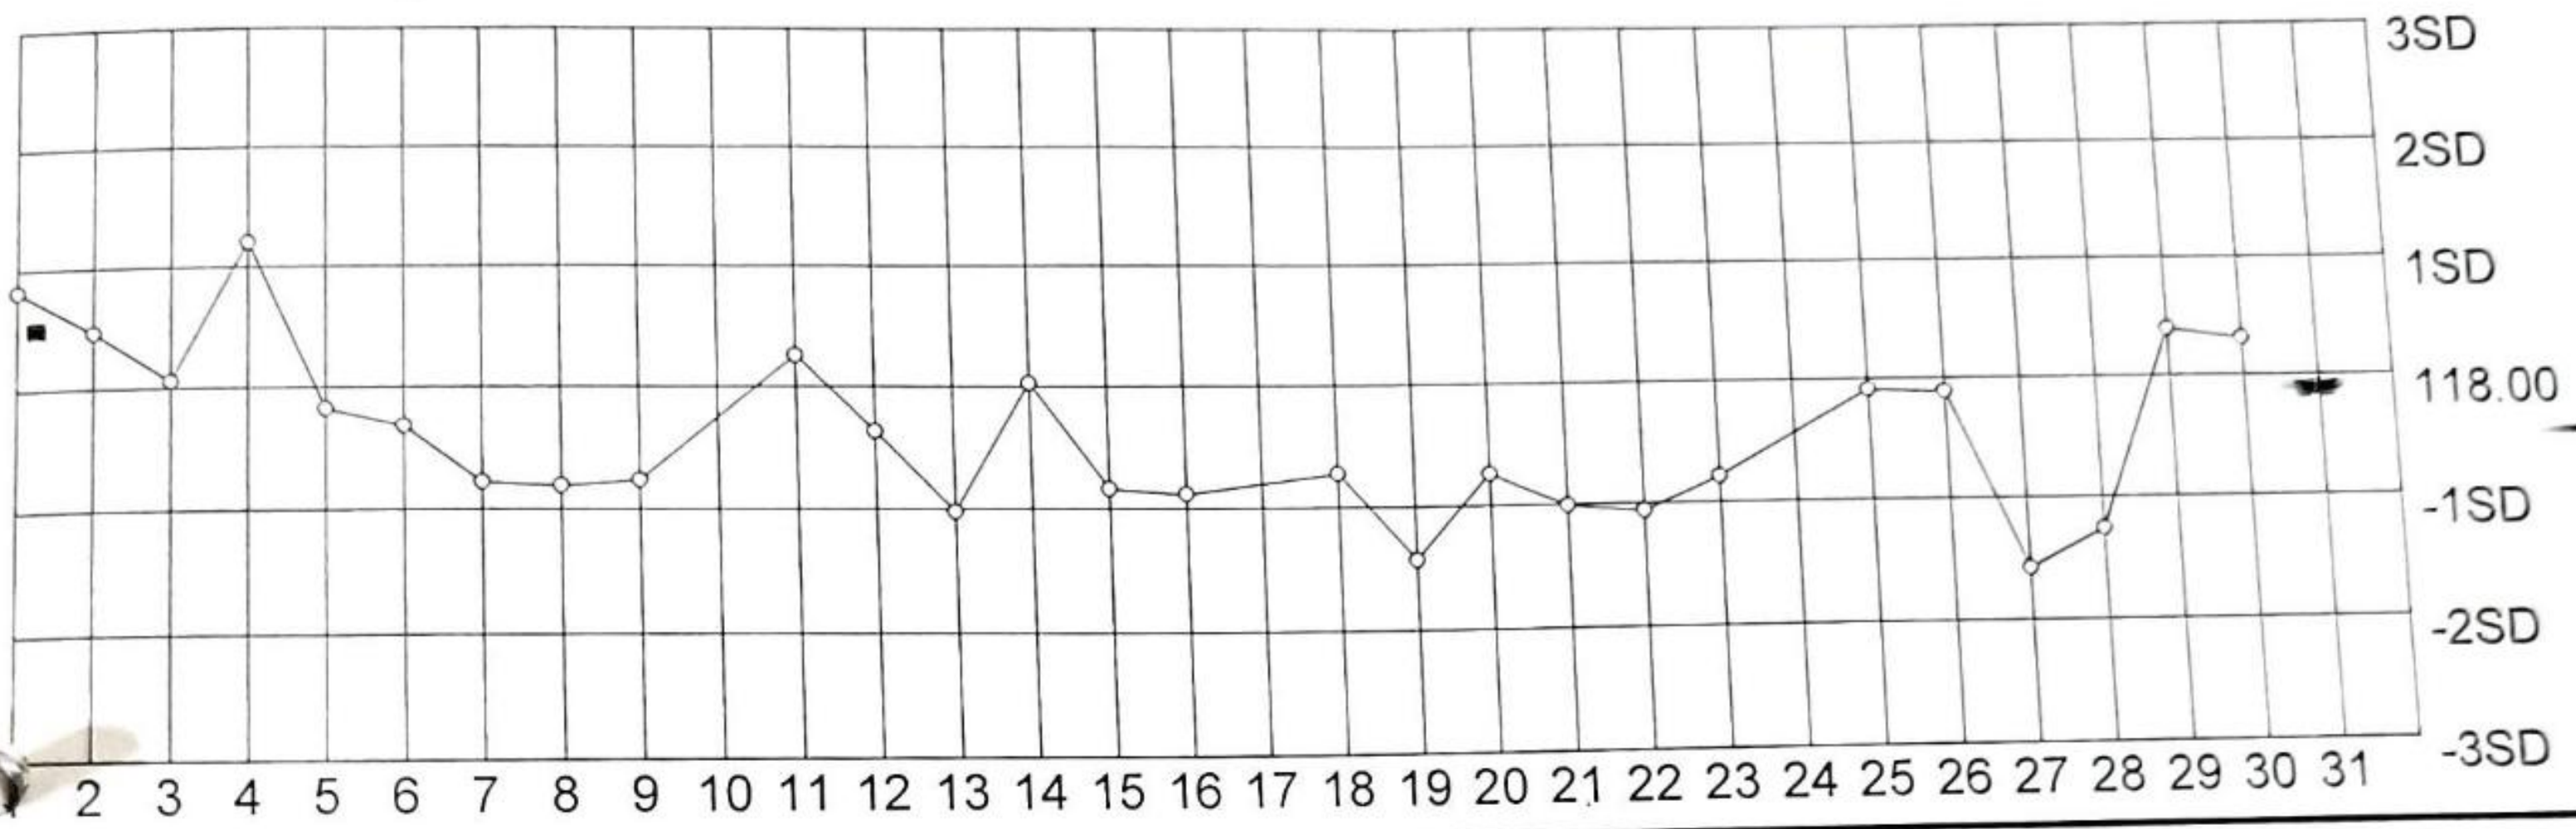

No.	Run date	Result	Status
1	04/01/2022	126.21	+1SD
2	04/02/2022	122.66	+1SD
3	04/03/2022	118.60	+1SD
4	04/04/2022	130.09	+2SD
5	04/05/2022	116.24	-1SD
6	04/06/2022	114.81	-1SD
7	04/07/2022	110.24	-1SD
8	04/08/2022	109.93	-1SD
9	04/09/2022	110.39	-1SD
10	04/11/2022	120.59	+1SD
11	04/12/2022	114.35	-1SD
12	04/13/2022	107.80	-2SD
13	04/14/2022	118.27	+1SD
14	04/15/2022	109.63	-1SD
15	04/16/2022	109.21	-1SD
16	04/18/2022	110.75	-1SD
17	04/19/2022	103.69	-2SD
18	04/20/2022	110.62	-1SD
19	04/21/2022	107.93	-2SD
20	04/22/2022	107.40	-2SD
21	04/23/2022	110.12	-1SD
22	04/25/2022	117.10	-1SD
23	04/26/2022	116.88	-1SD
24	04/27/2022	102.22	-2SD
25	04/28/2022	105.39	-2SD
26	04/29/2022	121.94	+1SD
27	04/30/2022	121.14	+1SD
28	04/30/2022	120.20	+1SD
29			
30			
31			

*[Handwritten Signature]*

This test has been conducted on AutoQuant2

# QC Chart


Test name: TP

QC Lot: 112196

Concentration: Normal

Run date: From 04/01/2022 To 04/30/2022

	N	Mean	SD	CV
Standard QC Value	-	4.80	0.24	5.00%
Floating QC Value	29	4.91	0.21	4.33%

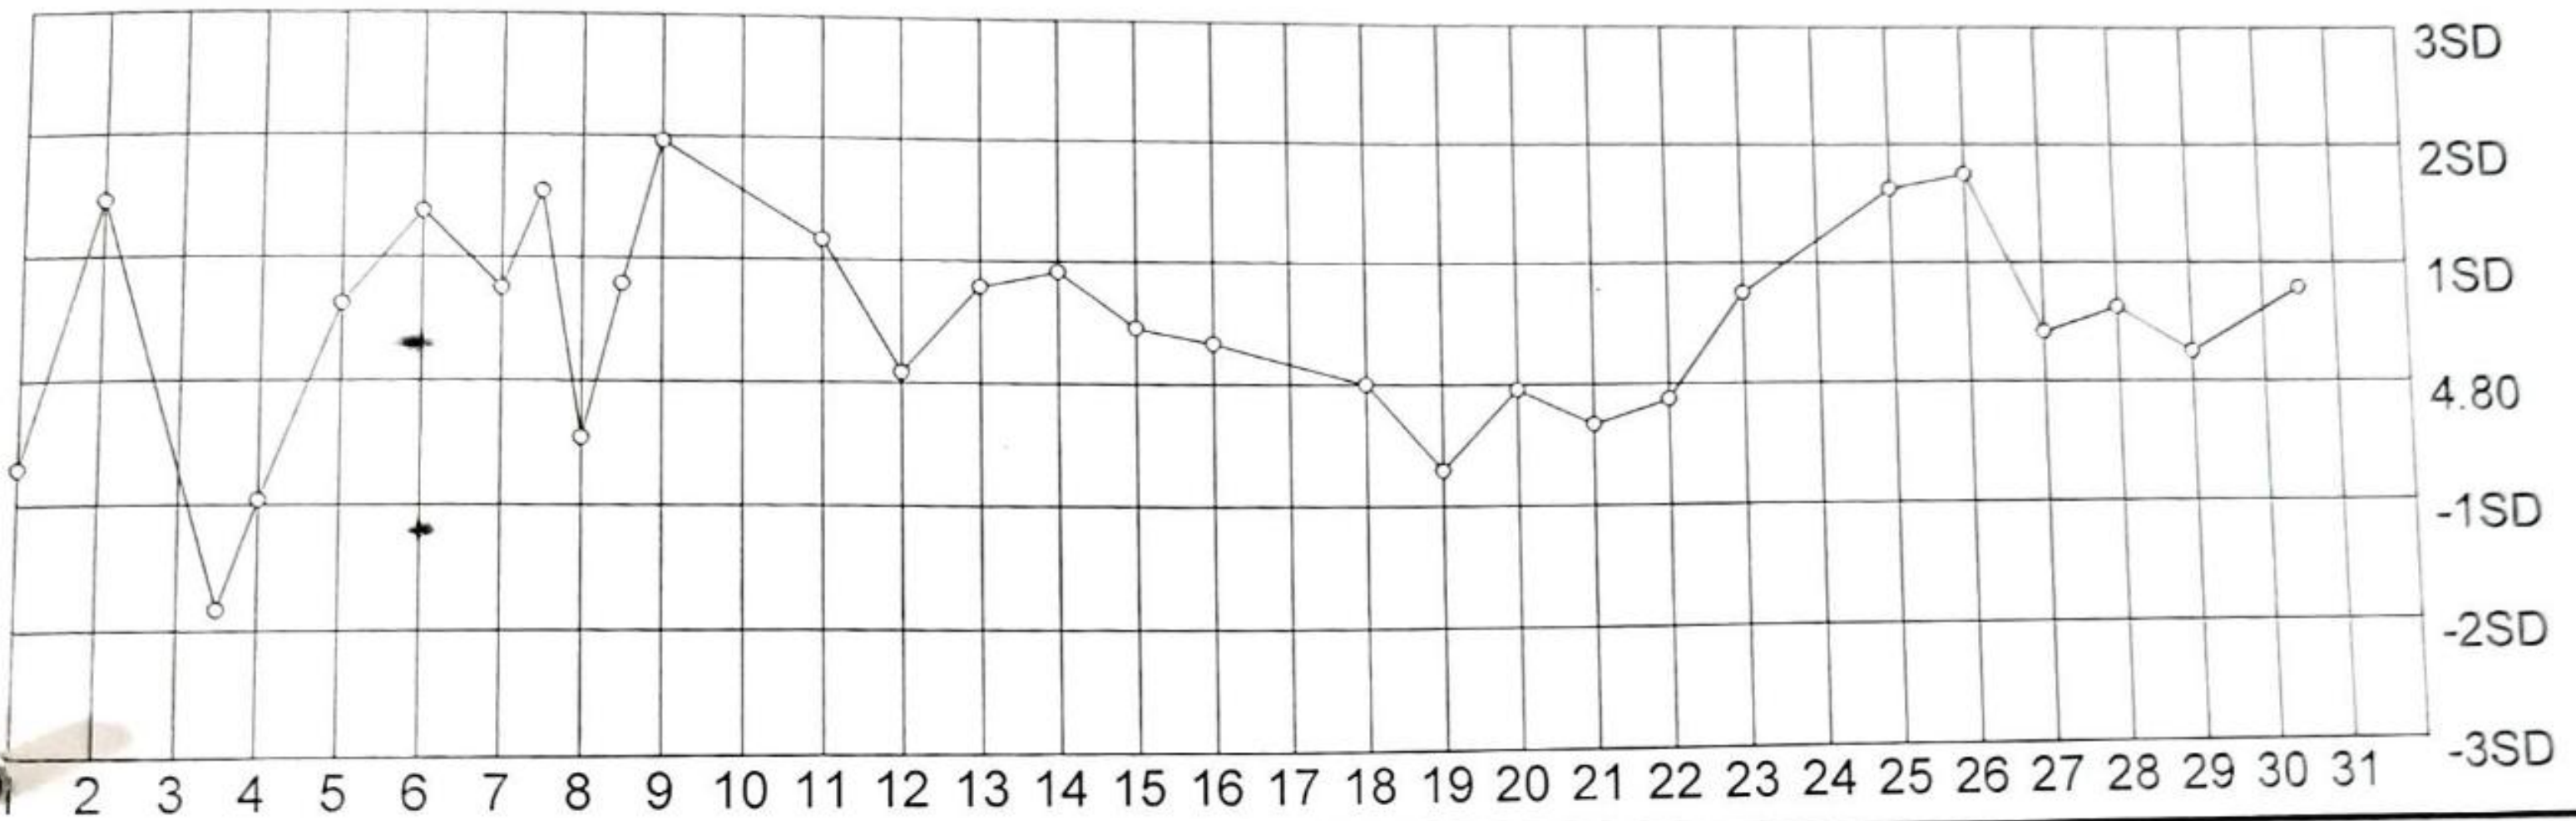

No.	Run date	Result	Status
1	04/01/2022	4.63	-1SD
2	04/02/2022	5.15	+2SD
3	04/03/2022	4.36	-2SD
4	04/04/2022	4.57	-1SD
5	04/05/2022	4.95	+1SD
6	04/06/2022	5.13	+2SD
7	04/07/2022	4.98	+1SD
8	04/07/2022	5.17	+2SD
9	04/08/2022	4.69	-1SD
10	04/08/2022	4.99	+1SD
11	04/09/2022	5.27	+2SD
12	04/11/2022	5.08	+2SD
13	04/12/2022	4.82	+1SD
14	04/13/2022	4.99	+1SD
15	04/14/2022	5.02	+1SD
16	04/15/2022	4.91	+1SD
17	04/16/2022	4.88	+1SD
18	04/18/2022	4.80	-1SD
19	04/19/2022	4.63	-1SD
20	04/20/2022	4.79	-1SD
21	04/21/2022	4.72	-1SD
22	04/21/2022	4.77	-1SD
23	04/22/2022	4.77	+1SD
24	04/22/2022	4.98	+2SD
25	04/23/2022	5.19	+2SD
26	04/25/2022	5.22	+2SD
27	04/26/2022	5.19	+1SD
28	04/27/2022	4.90	+1SD
29	04/27/2022	4.95	+1SD
30	04/28/2022	4.86	+1SD
31	04/29/2022	4.99	+1SD

*[Handwritten Signature]*

This test has been conducted on AutoQuant2

# QC Chart


Test name: UA

QC Lot: 112196

Concentration: Normal

Run date: From 04/01/2022 To 04/30/2022

	N	Mean	SD	CV
Standard QC Value	-	5.50	0.47	8.55%
Floating QC Value	27	5.69	0.32	5.70%

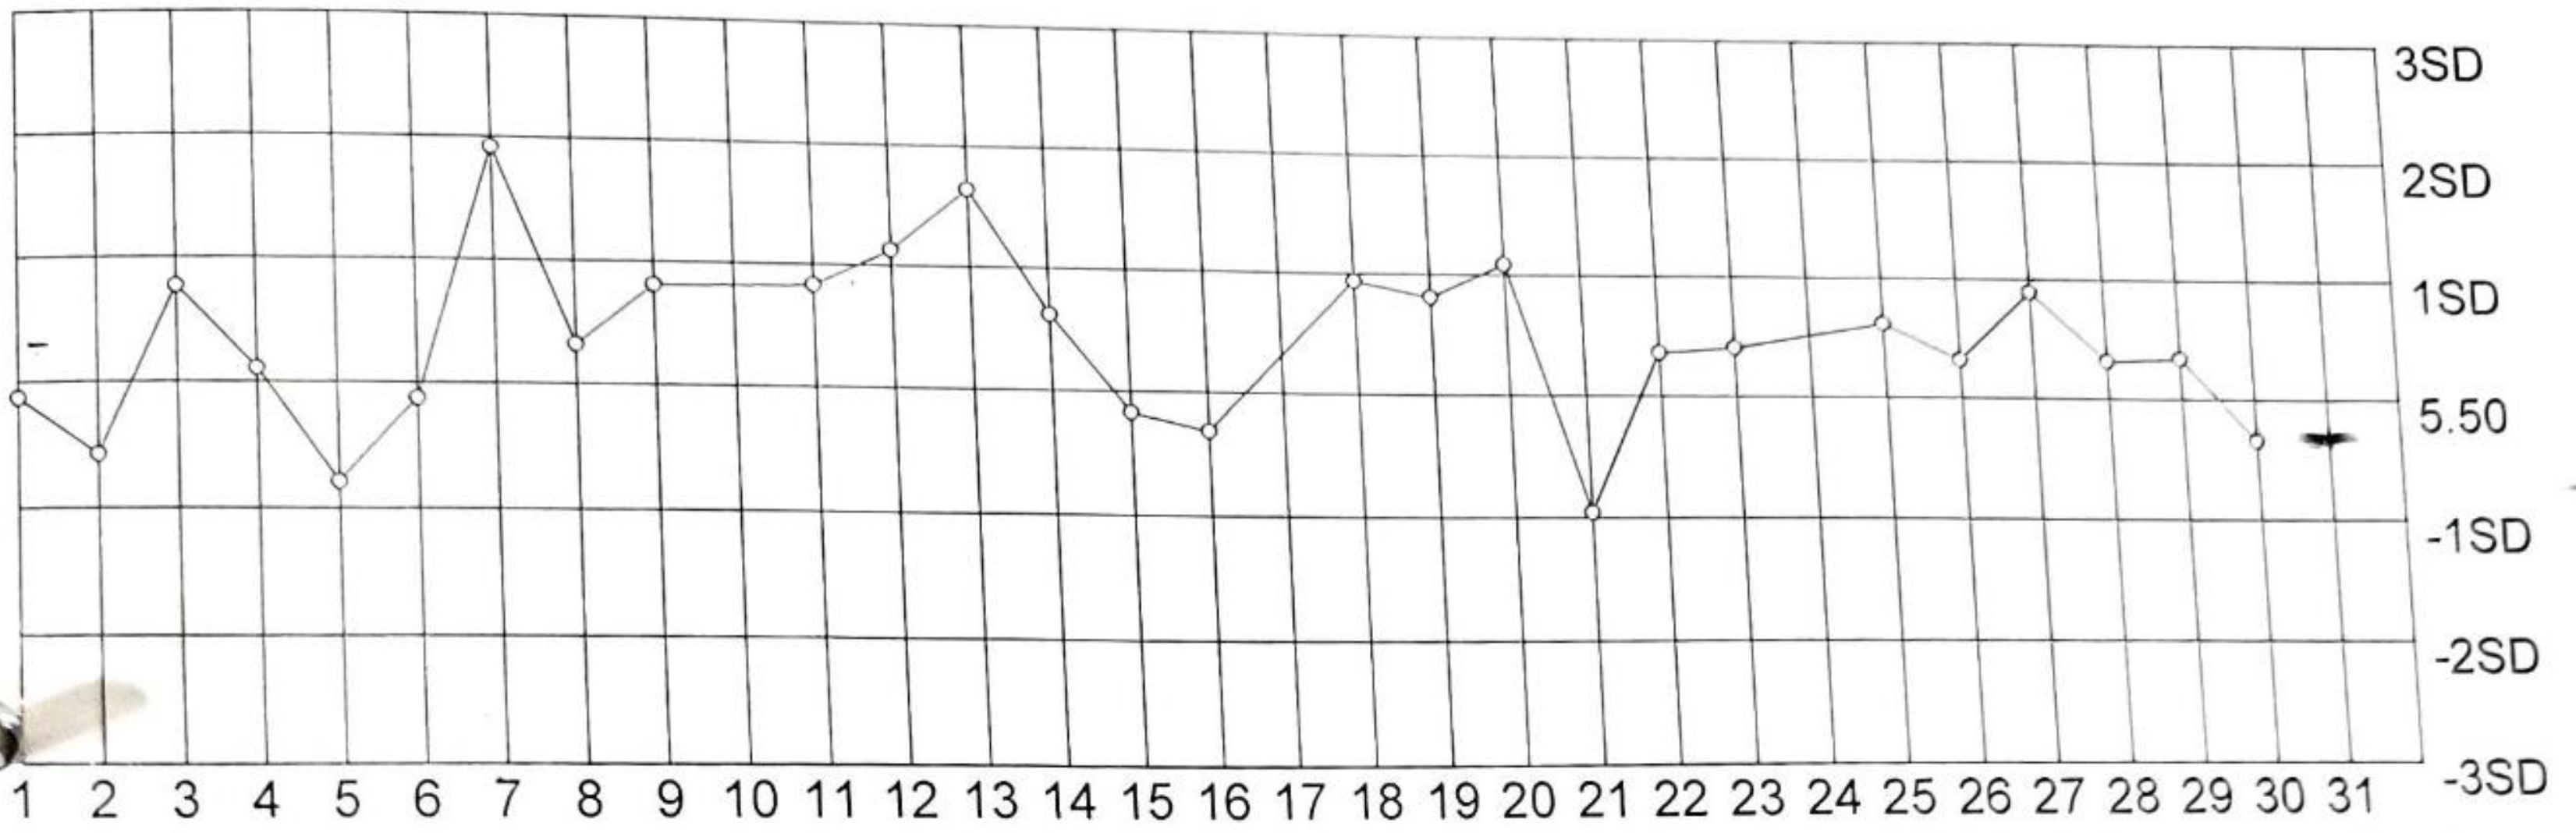

No.	Run date	Result	Status
1	04/01/2022	5.44	-1SD
2	04/02/2022	5.23	-1SD
3	04/03/2022	5.86	+1SD
4	04/04/2022	5.55	+1SD
5	04/05/2022	5.13	-1SD
6	04/06/2022	5.44	-1SD
7	04/07/2022	6.40	+2SD
8	04/08/2022	5.65	+1SD
9	04/09/2022	5.88	+1SD
10	04/11/2022	5.89	+1SD
11	04/12/2022	6.03	+2SD
12	04/13/2022	6.27	+2SD
13	04/14/2022	5.79	+1SD
14	04/15/2022	5.42	-1SD
15	04/16/2022	5.35	-1SD
16	04/18/2022	5.94	+1SD
17	04/19/2022	5.88	+1SD
18	04/20/2022	6.01	+2SD
19	04/21/2022	5.05	-1SD
20	04/22/2022	5.67	+1SD
21	04/23/2022	5.69	+1SD
22	04/25/2022	5.79	+1SD
23	04/26/2022	5.65	+1SD
24	04/27/2022	5.92	+1SD
25	04/28/2022	5.66	+1SD
26	04/29/2022	5.34	-1SD
27	04/30/2022	4.86	+1SD
28	04/29/2022	4.99	+1SD
29	04/30/2022	4.99	+1SD
30	04/30/2022		
31			

This test has been conducted on AutoQuant2

# QC Chart


Test name: UREA

QC Lot: 112196

Concentration: Normal

Run date: From 04/01/2022 To 04/30/2022

	N	Mean	SD	CV
Standard QC Value	-	36.83	3.13	8.50%
Floating QC Value	27	38.21	2.08	5.43%

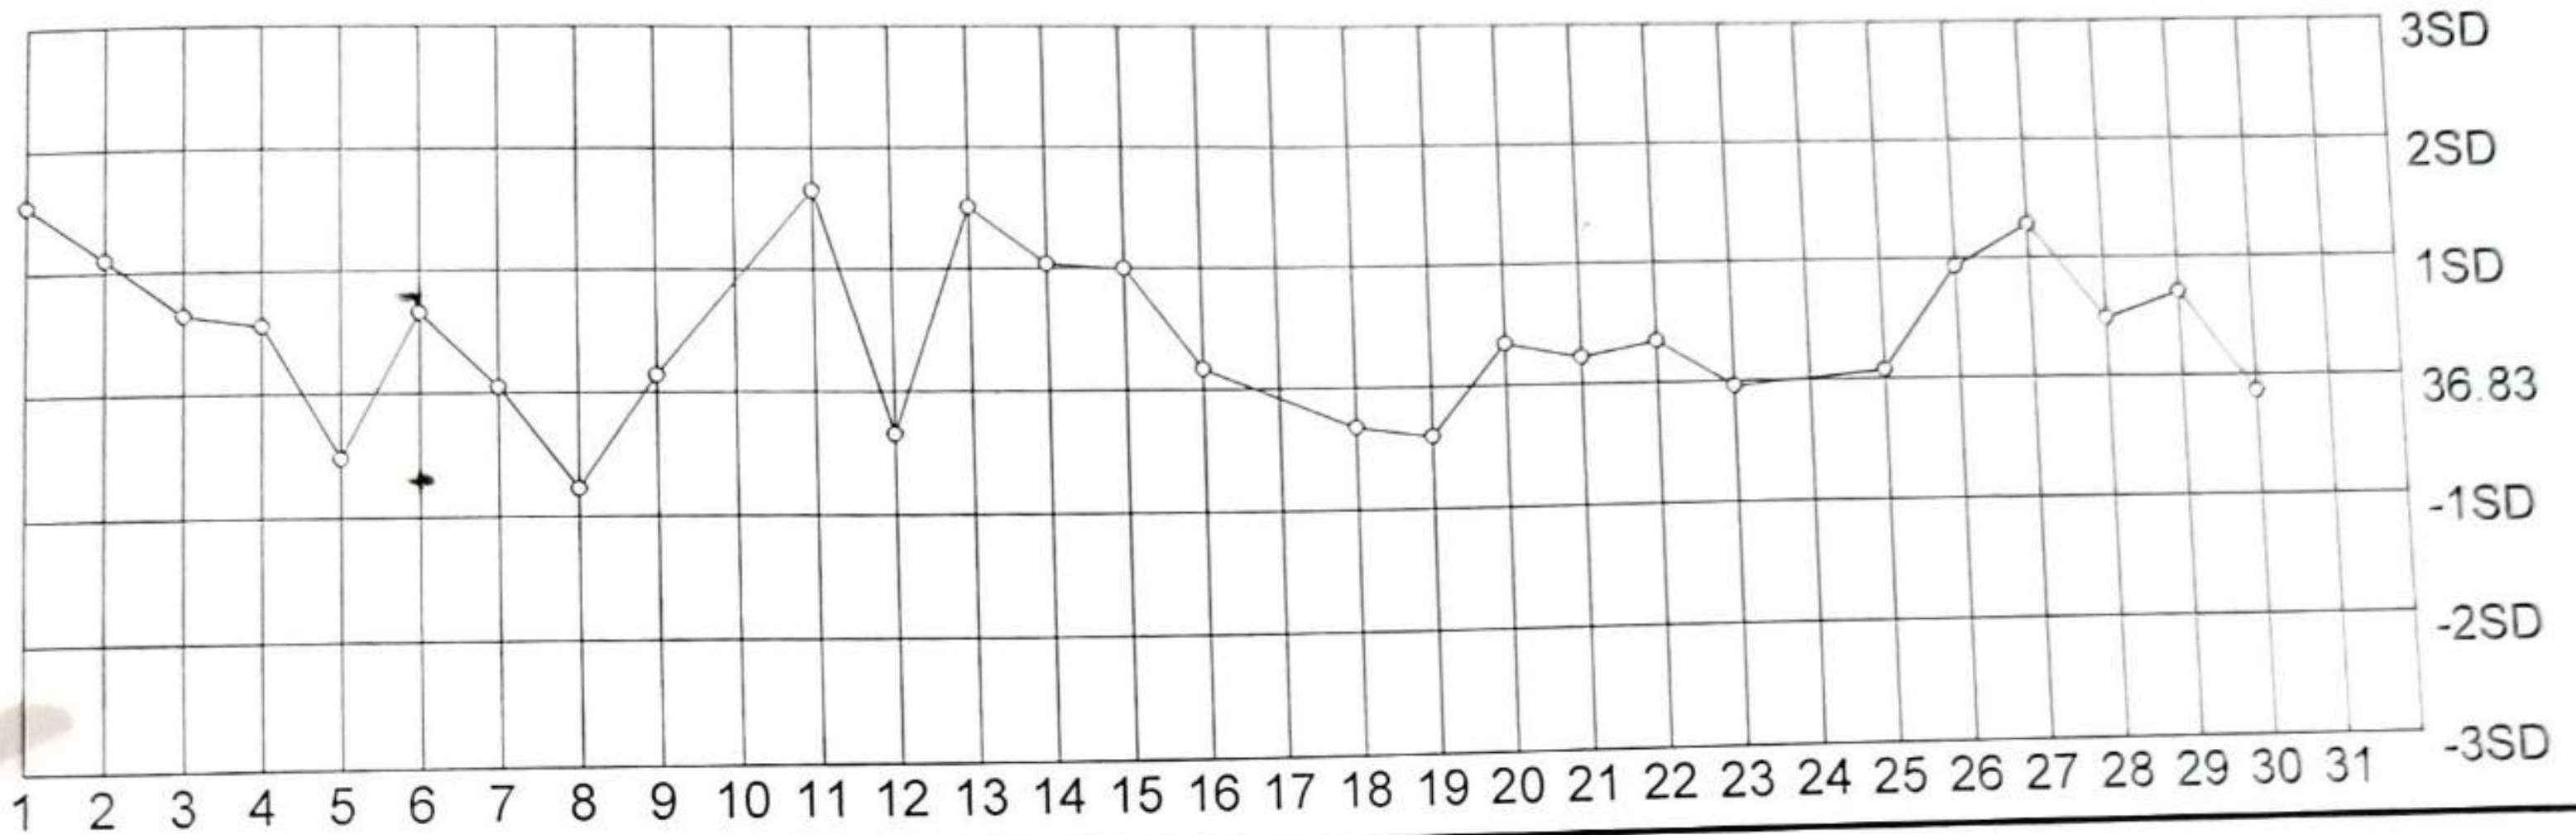

No.	Run date	Result	Status
1	04/01/2022	41.67	+2SD
2	04/02/2022	40.28	+2SD
3	04/03/2022	38.85	+1SD
4	04/04/2022	38.57	+1SD
5	04/05/2022	35.19	-1SD
6	04/06/2022	38.89	+1SD
7	04/07/2022	36.98	+1SD
8	04/08/2022	34.41	-1SD
9	04/09/2022	37.27	+1SD
10	04/11/2022	41.99	+2SD
11	04/12/2022	41.55	+2SD
12	04/13/2022	35.74	-1SD
13	04/14/2022	40.08	+1SD
14	04/15/2022	39.96	+1SD
15	04/16/2022	37.36	-1SD
16	04/18/2022	35.83	-1SD
17	04/19/2022	35.57	+1SD
18	04/20/2022	37.92	+1SD
19	04/21/2022	37.53	+1SD
20	04/22/2022	37.92	-1SD
21	04/23/2022	36.71	+1SD
22	04/25/2022	37.06	+1SD
23	04/26/2022	39.74	+2SD
24	04/27/2022	40.84	+1SD
25	04/28/2022	38.36	+1SD
26	04/29/2022	39.04	-1SD
27	04/30/2022	36.41	+1SD
28	<del>04/29/2022</del>	<del>4.86</del>	+1SD
29	<del>04/30/2022</del>	<del>4.99</del>	+1SD
30	04/30/2022	4.99	+1SD
31			

*[Handwritten signature]*

This test has been conducted on AutoQuant2

# QC Chart

Concentration: Normal

## QC Chart


QC Lot 112196

Concentration: Normal

Test Name: Test name: ALB

Run date: From 04/01/2022 To 04/30/2022

Standard QC Value	N	Mean	SD	CV
Floating QC Value	-	3.30	0.17	5.15%
	27	3.32	0.12	3.58%

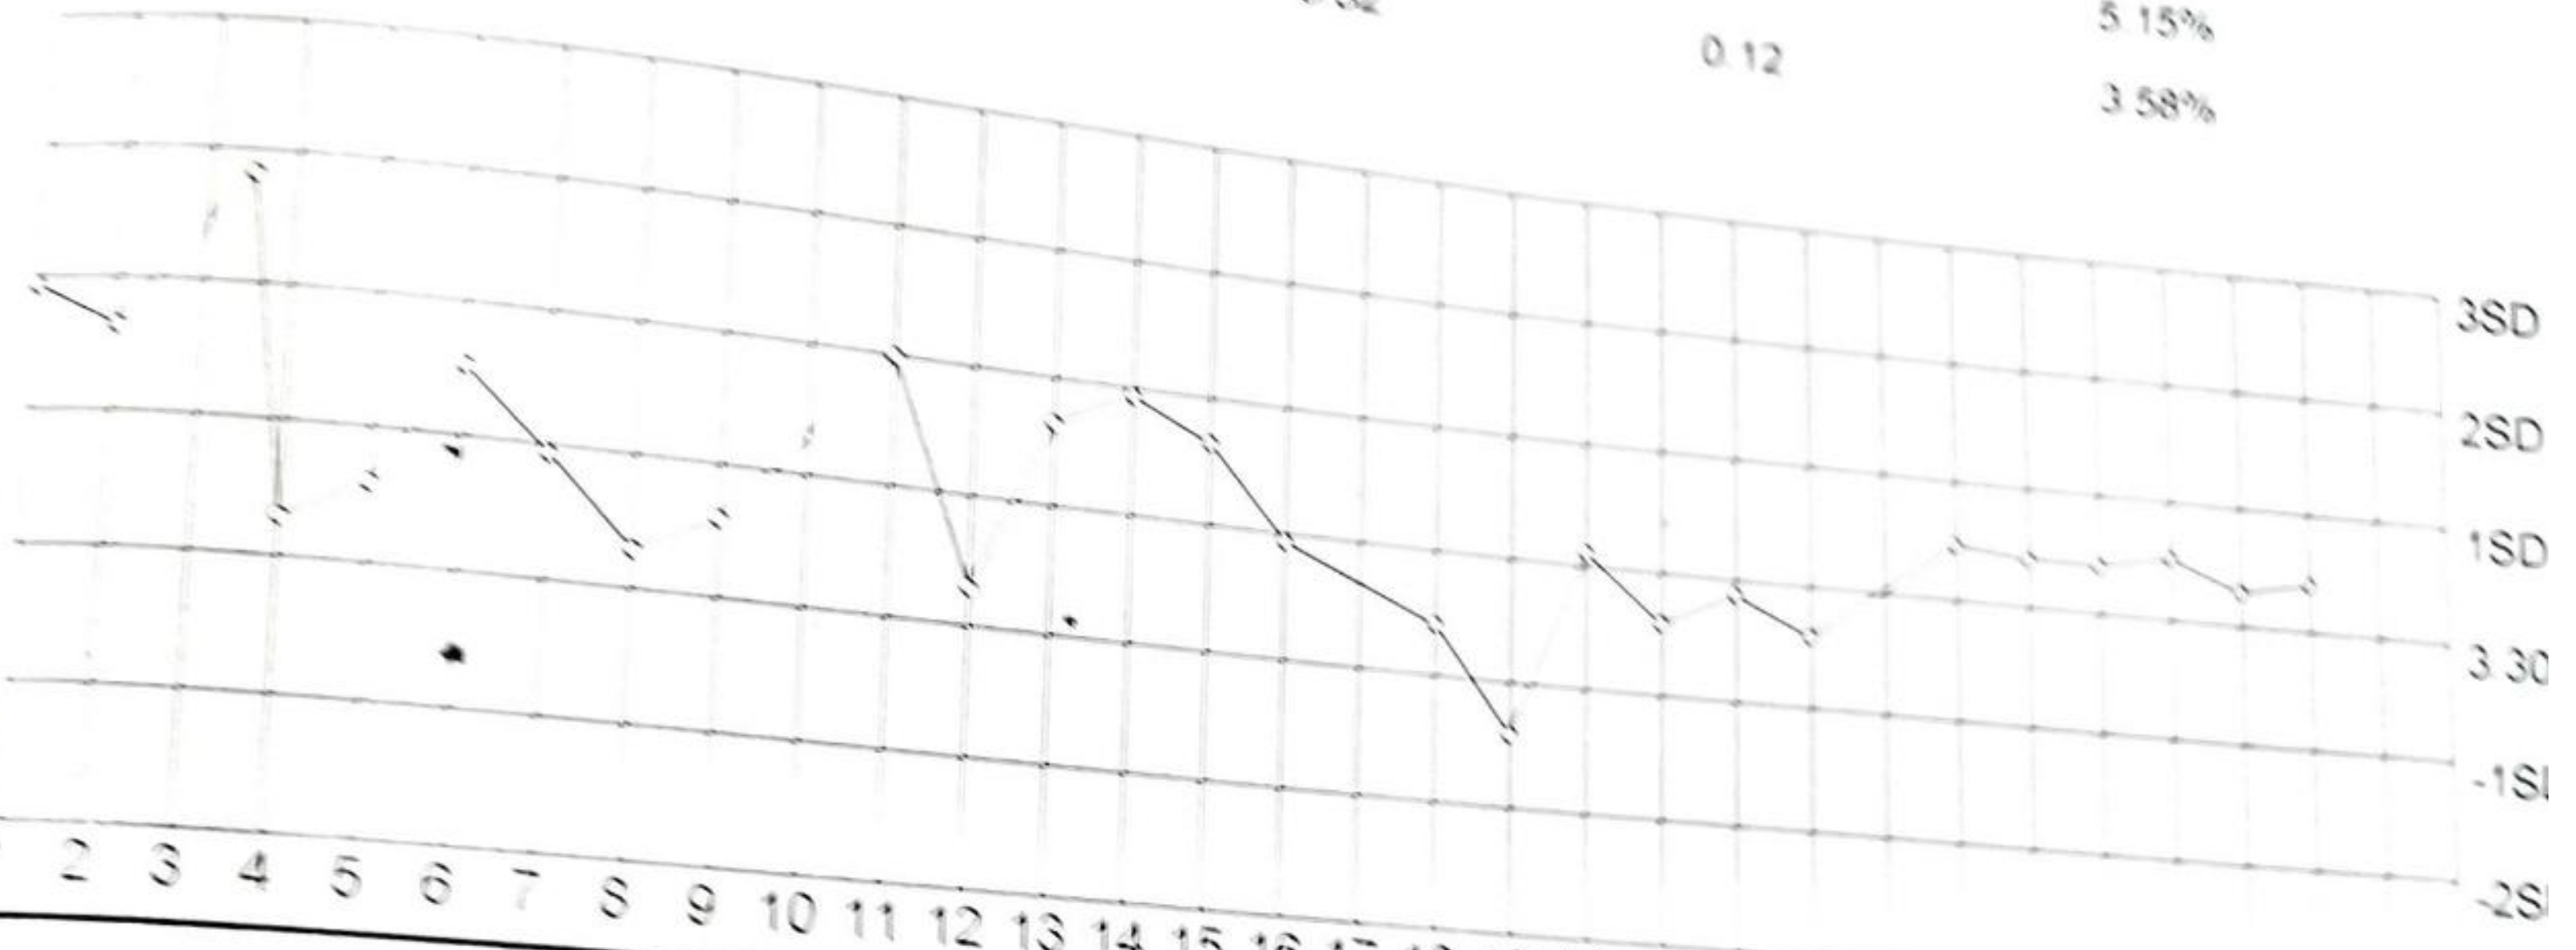

No.	Run date	Result	Status
1	04/01/2022		
2	04/02/2022	3.46	
3	04/03/2022	3.41	+1SD
4	04/04/2022	3.61	+1SD
5	04/05/2022	3.18	+2SD
6	04/06/2022	3.23	-1SD
7	04/07/2022	3.39	-1SD
8	04/08/2022	3.29	+1SD
9	04/09/2022	3.18	-1SD
10	04/09/2022	3.23	-1SD
11	04/11/2022	3.47	+2SD
12	04/12/2022	3.18	-1SD
13	04/13/2022	3.41	+1SD
14	04/14/2022	3.46	+1SD
15	04/15/2022	3.41	+1SD
16	04/16/2022	3.29	-1SD
17	04/18/2022	3.20	-1SD
18	04/19/2022	3.06	-2SD
19	04/19/2022	3.32	+1SD
20	04/20/2022	3.32	-1SD
21	04/21/2022	3.23	-1SD
22	04/22/2022	3.28	-1SD
23	04/23/2022	3.23	+1SD
24	04/25/2022	3.38	+1SD
25	04/25/2022	3.37	+1SD
26	04/26/2022	3.37	+1SD
27	04/27/2022	3.39	+1SD
28	04/28/2022	3.35	+1SD
29	04/29/2022	3.37	
30	04/30/2022		
31			

*all new 5/5*



### Calibration Certificate

This is to Certify that Biochemistry Analyzer Meril AutoQuant-200Exelus Instrument Sr. No. AQ060444 Installed at Sachdeva Diagnostics , Delhi has been calibrated by our engineer on 01-Aug-2021 with appropriate and sophisticated tools. Below parameter has been calibrated:

<u>TEST ITEMS AND RESULT</u>	
Appearance	No Imbalance Probe Movement
Leakage in Water tubing or CRU	No water leakage
Ambient temp ( 15- 32 ) Degree	24.0 degree C
Lamp Check	Ok
Sample Dispersing Volume	In range ( 0 to 30 ul)
Reagent cooling Temperature	2.8 ° C ( 0 to 15 Degree)
Optical Path length	0.65
Waster & Water Sensor	Working Properly
Threshold value	±34000 (≥25,000)
Valve & Motor	Working Properly
Reagent Dispensing Volume	In range ( 0 to 150 ul)
Power Supply and Earthing	230 Volts and Grounding less then 5 V
CV-Kinetic/End point/two Point	CV- 1.77% /2.42% /2.80%
SD-Kinetic/End point/two Point	SD- 1.15/0.39/0.69
Mean-Kinetic/End point/two Point	Mean- 97.55/14.34/24.79
Hardware Check-Functional Test	OK5415152524141112
Light Quality Check	OK
Cuvette Absorbance	OK
Cuvette Blank Value	OK >33000
Incubation temp.	37.0 ° C
Room temp.	25.0 degree C

This Calibration Certificate is Valid Up to **01-Aug-2022**.  
Conclusion: All parameter are within range. The Machine is working properly.  
(As per Meril terms.)

Engineer Name: **Mr. Rahul Saini**

Designation: **Deputy Regional Service Manager**

Engineer Sign:



T : 91 260 3052100  
F : 91 260 3052125

www.merillife.com

Meril Diagnostics Pvt. Ltd.  
Survey No 135/2/B, Bilakhia House  
Muktanand Marg Chala  
Vapi - 396191 Gujarat, India

Original

Diagnostics