

**Analyte Methodwise Qualitative Result Report**

**Lab No.:** 455  
**Lab Name :** MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR  
**Report Date :** 23/05/2022

**Cycle No :** 220104  
**Sample No :** 1  
**Sample Date :** 26-04-2022


**Clinical Path - Stool Routine Microscopy Image,Identify, -**

<span style="display: inline-block; width: 15px; height: 15px; background-color: #9933cc; border: 1px solid black;"></span>	All Methods	<b>N</b>
<span style="display: inline-block; width: 15px; height: 15px; background-color: #008080; border: 1px solid black;"></span>	- - (Your Method)	147
<span style="display: inline-block; width: 15px; height: 15px; background-color: #800000; border: 1px solid black;"></span>	- - (Your Analyzer)	147

<b>Your Result</b>	Cyst of Giardia
<b>Result Expected</b>	CG

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

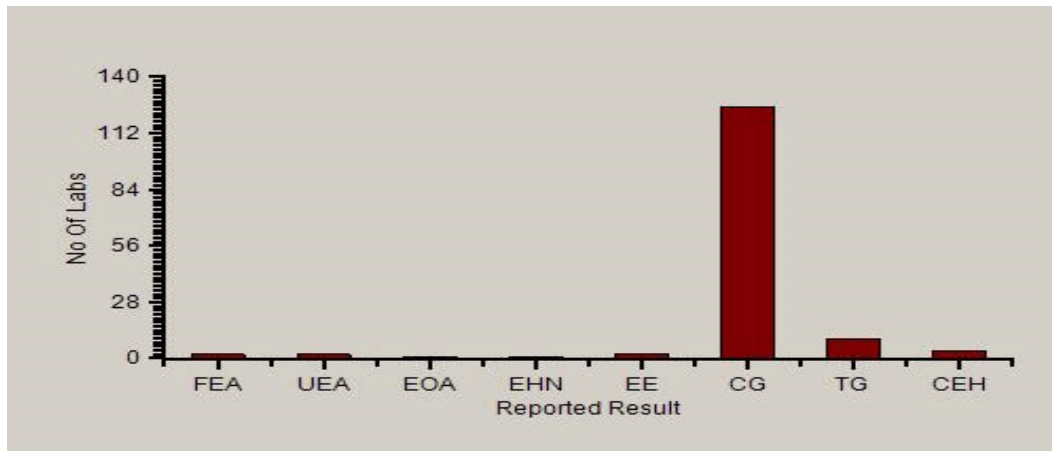


PC-1022

**Analyte Methodwise Qualitative Result Report**

Lab No.: 455  
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR  
Report Date : 23/05/2022

Cycle No : 220104  
Sample No : 1  
Sample Date : 26-04-2022

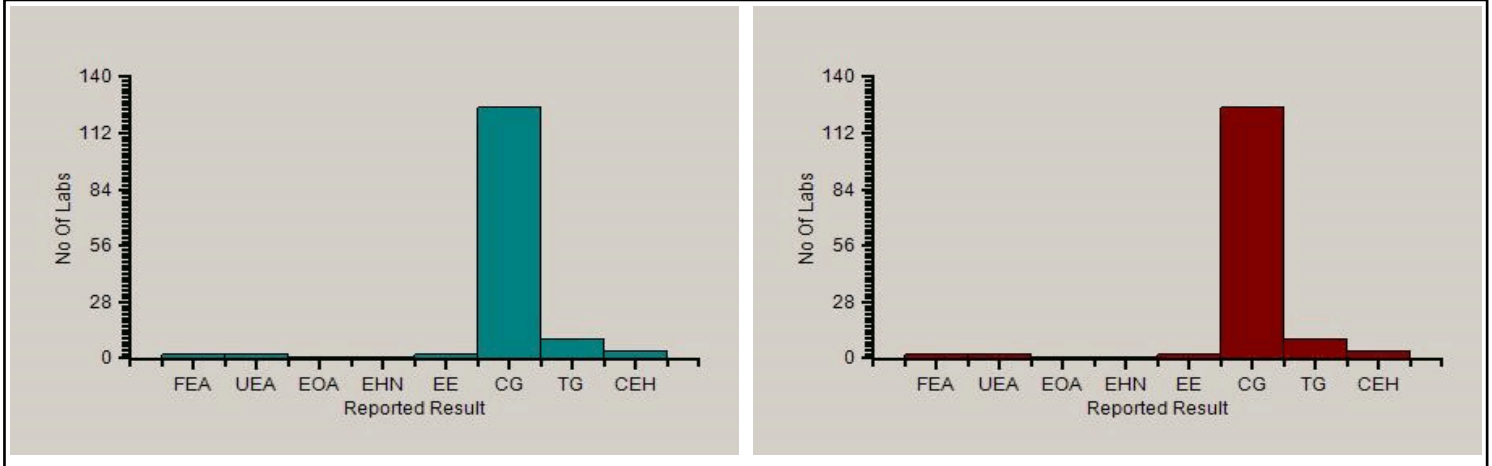

**Reported Results Legends :-**

FEA	: Fertilized egg of Ascaris
UEA	: Unfertilized Egg of Ascaris
EOA	: Egg of Ankylostoma
EOT	: Egg of Trichuris
EOC	: Egg of Clonorchis
EOM	: Egg of Metagonimus
EHN	: Egg of H. nana
ET	: Egg of Taenia
EE	: Egg of Enterobius
CG	: Cyst of Giardia
TG	: Trophozoite of Giardia
CEH	: Cyst of E. histolytica
TEH	: Trophozoite of E. histolytica

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance. Review for systematic error

*Dr Puneet Kumar Nigam*

**Dr Puneet Kumar Nigam**  
**PT coordinator & Technical Manager, MHL EQAS**  
Unit No. 409-416.  
Commercial Building - 1A,  
Kohinoor Mall, Kiroi Road, Kurla (W),  
Mumbai - 400070



**Analyte Methodwise Qualitative Result Report**

**Lab No.:** 455  
**Lab Name :** MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR  
**Report Date :** 23/05/2022


**Cycle No :** 220104  
**Sample No :** 1  
**Sample Date :** 26-04-2022

**Clinical Path - Urine Sediment Analysis Image,Crystal, -**

	<b>N</b>
<span style="color: purple;">■</span> All Methods	159
<span style="color: teal;">■</span> - - (Your Method)	159
<span style="color: darkred;">■</span> - - (Your Analyzer)	159

<b>Your Result</b>	Triple phosphate crystal
<b>Result Expected</b>	TPC


**Note :** # is an indication that this parameter has not been evaluated

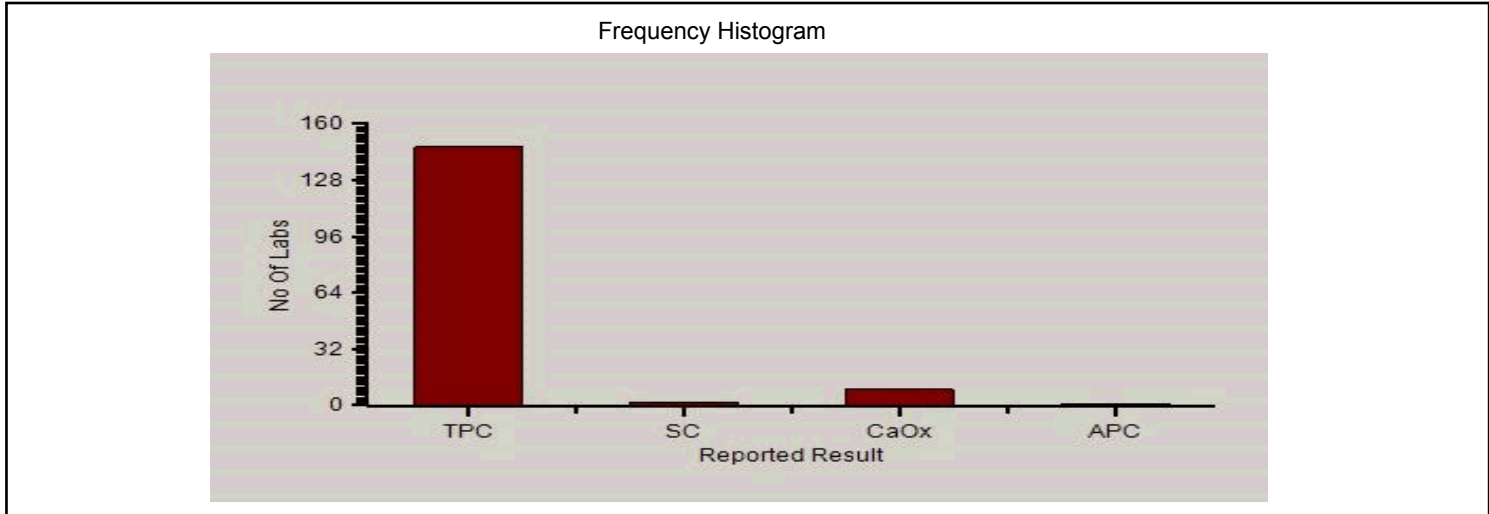

**Analyte Methodwise Qualitative Result Report**

Lab No.: 455  
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR  
Report Date : 23/05/2022

Cycle No : 220104  
Sample No : 1  
Sample Date : 26-04-2022

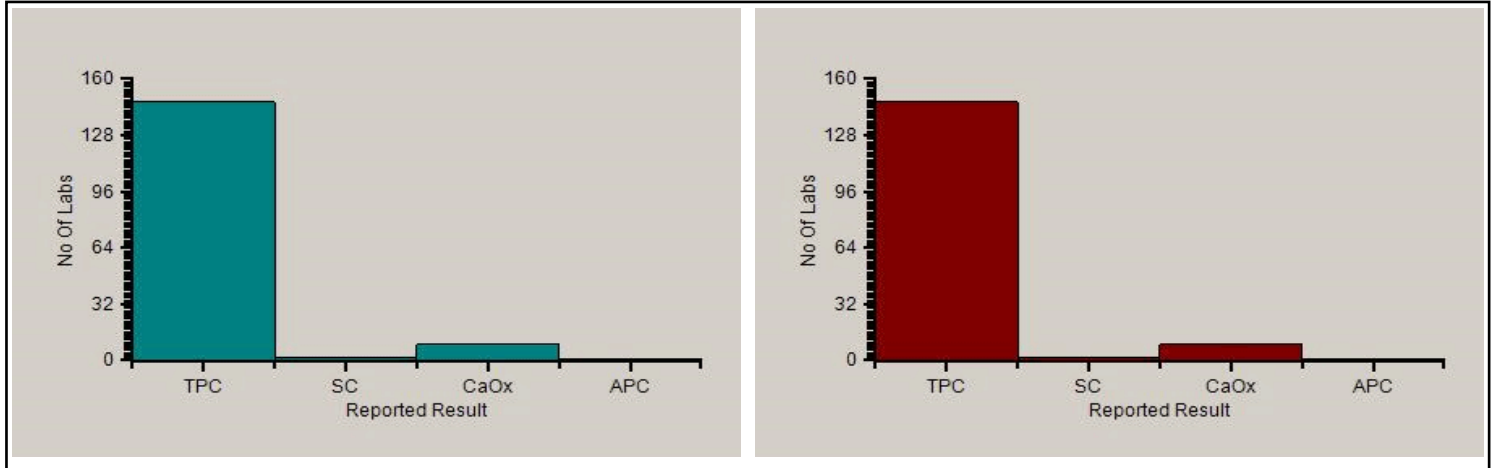

**Reported Results Legends :-**

- TPC : Triple phosphate crystal
- UAC : Uric acid crystal
- CC : Cystine crystal
- SC : Sulfonamide crystal
- UC : Urate crystal
- CaOx : Calcium oxalate crystal
- BC : Bilirubin crystals
- CHC : Cholesterol crystals
- ABC : Ammonium Biurate crystal
- NCS : No crystal seen
- APC : Ammonium phosphate crystal
- APC : Amorphous Phosphate Crystal

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance. Review for systematic error

*Dr Puneet Kumar Nigam*

**Dr Puneet Kumar Nigam**  
**PT coordinator & Technical Manager, MHL EQAS**

Unit No. 409-416.  
Commercial Building - 1A,  
Kohinoor Mall, Kiroi Road, Kurla (W),  
Mumbai - 400070

