

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 1
Sample Date : 26-04-2022


Immunoassay Extended,Dengue NS 1, -

	N
■ All Methods	156
■ Immunochromatography - (Your Method)	136
■ Manual - (Your Analyzer)	147

Your Result	Negative
Result Expected	Neg

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

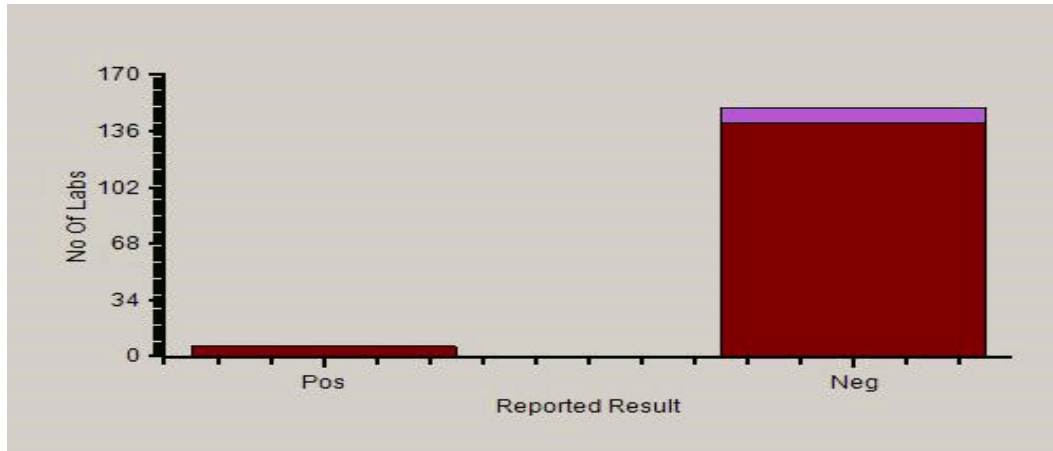

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 1
Sample Date : 26-04-2022

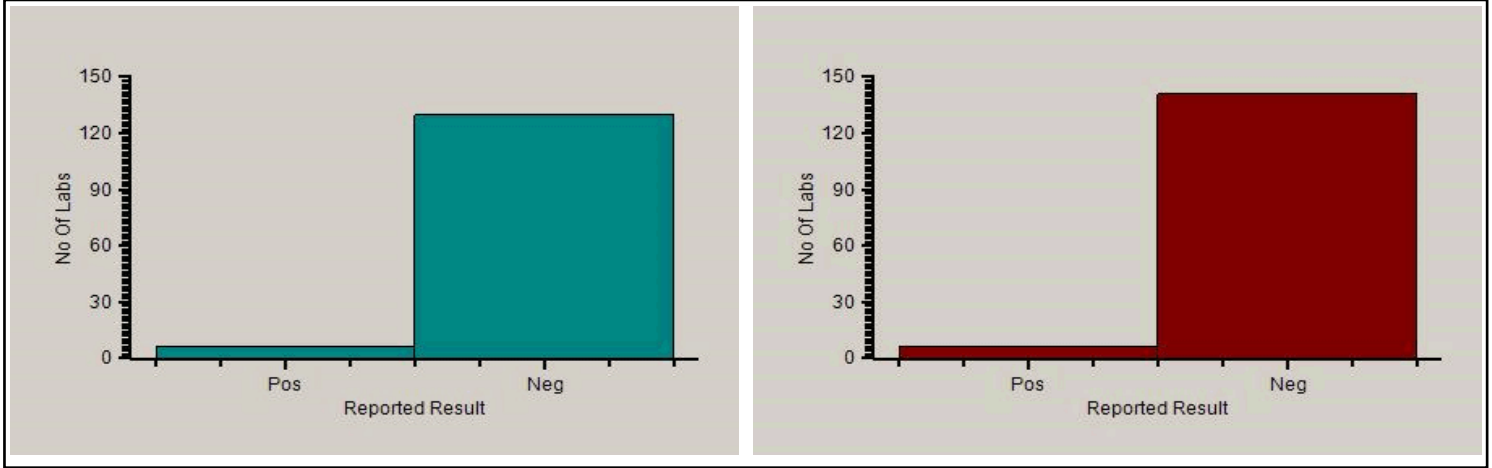

Reported Results Legends :-

- Pos : Positive
- Eq : Equivocal
- BL : Borderline
- Neg : Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 1
 Sample Date : 26-04-2022


Immunoassay Extended,HBsAg, -

	N
■ All Methods	204
■ Immunochromatography - (Your Method)	149
■ Manual - (Your Analyzer)	132

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated



Frequency Histogram

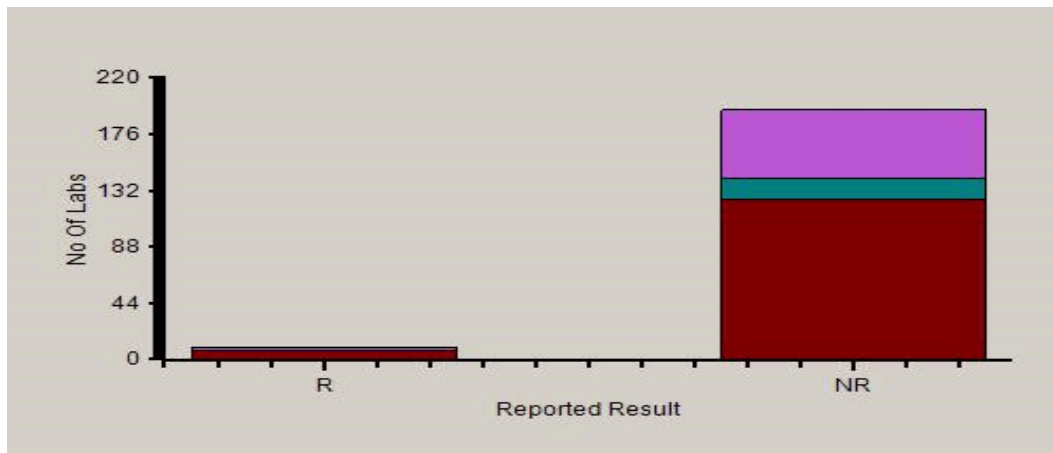

Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 1
 Sample Date : 26-04-2022

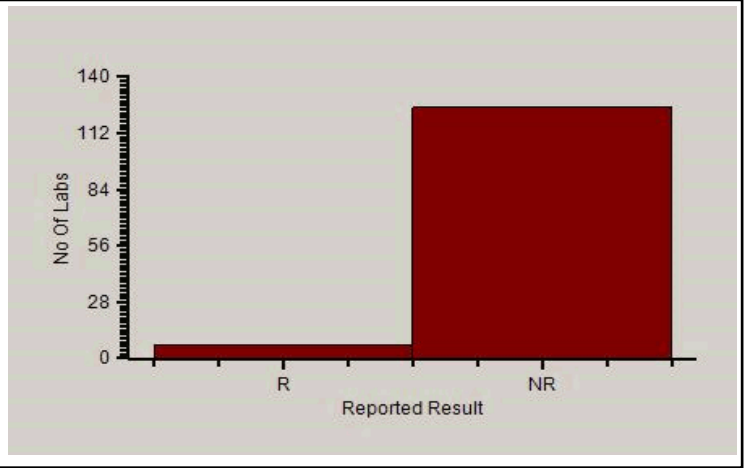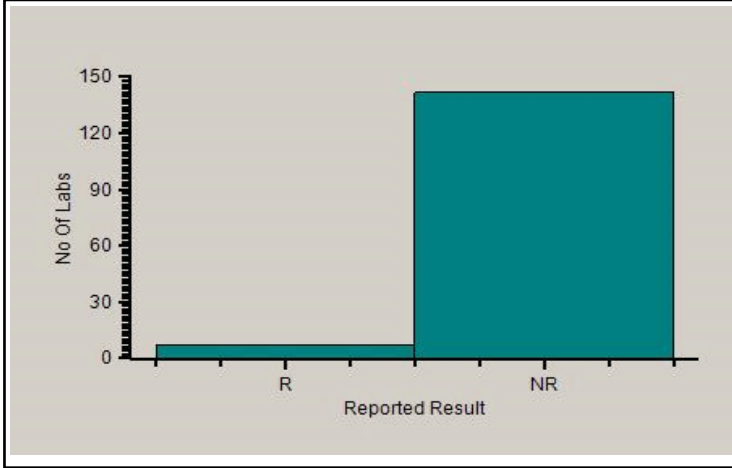

Reported Results Legends :-

R : Reactive
 NR : Non-reactive
 Eq : Equivocal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 1
 Sample Date : 26-04-2022


Immunoassay Extended,HCV, -

■ All Methods	N
■ Immunochromatography - (Your Method)	154
■ Manual - (Your Analyzer)	106
	95

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

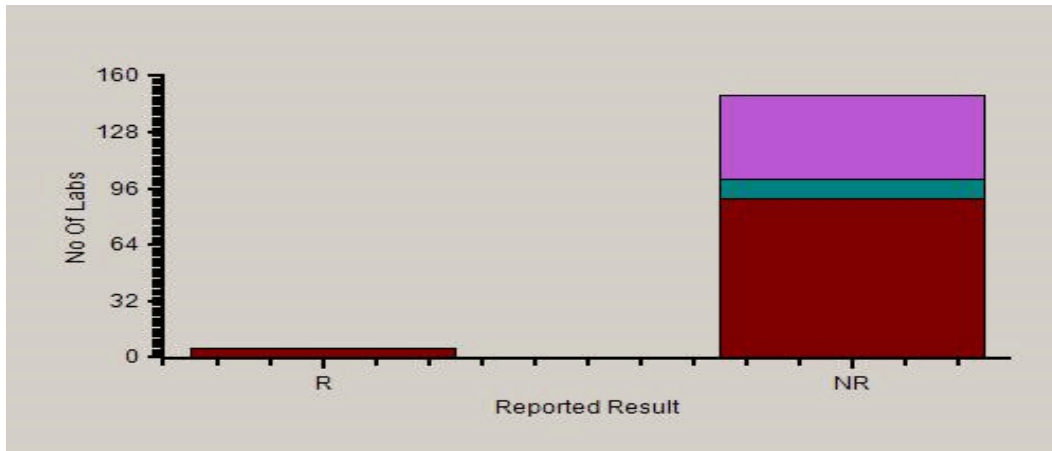

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 1
Sample Date : 26-04-2022

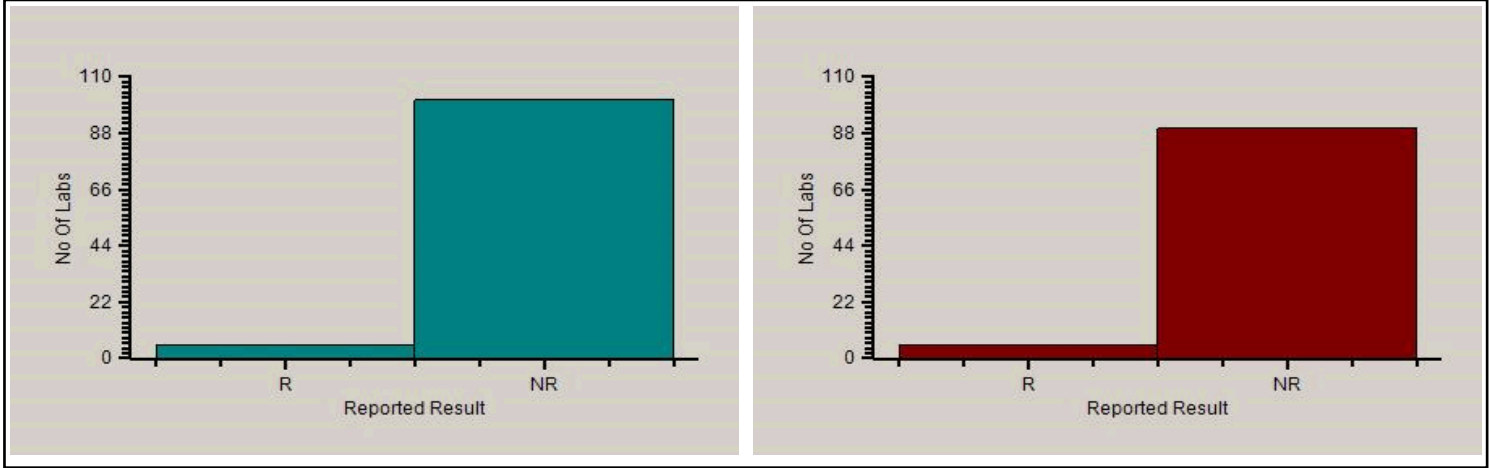

Reported Results Legends :-

R : Reactive
 NR : Non-reactive
 Eq : Equivocal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 1
 Sample Date : 26-04-2022


Immunoassay Extended,HIV Ab, -

	N
■ All Methods	118
■ Immunochromatography - (Your Method)	109
■ Manual - (Your Analyzer)	101

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

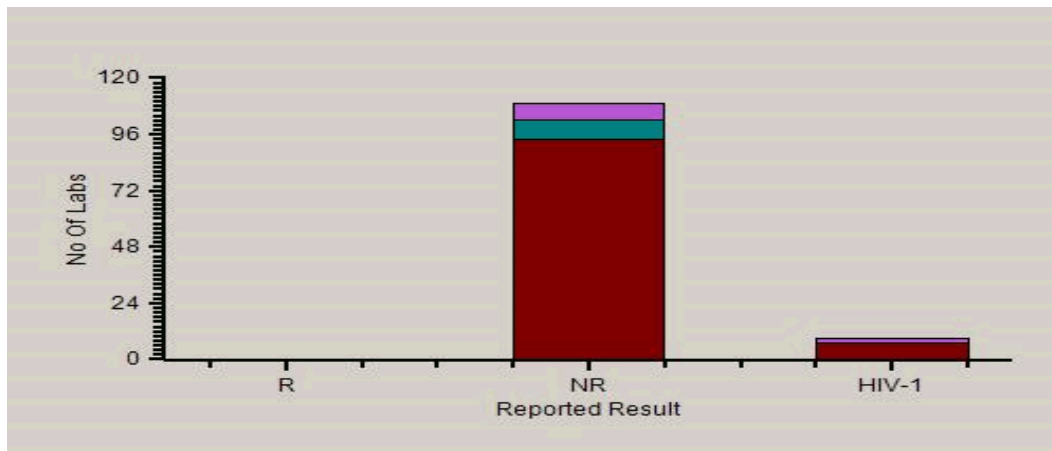

Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 1
 Sample Date : 26-04-2022

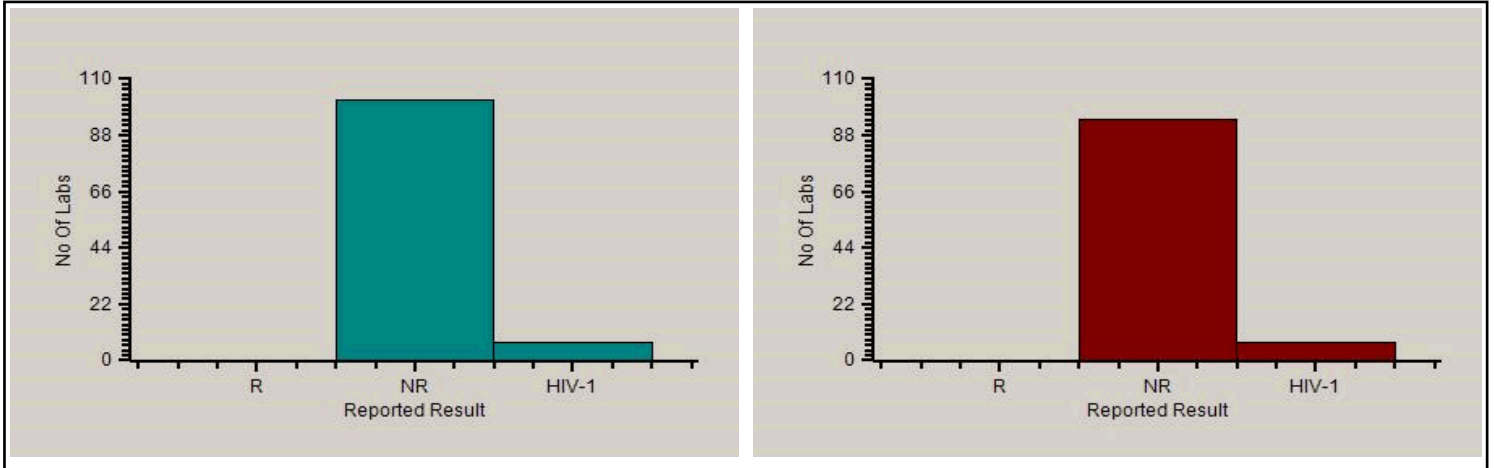

Reported Results Legends :-

R	: Reactive
NR	: Non-reactive
Eq	: Equivocal
Indet	: Indeterminate
HIV-1	: HIV-1 Ab Reactive
HIV-2	: HIV-2 Ab Reactive

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 1
 Sample Date : 26-04-2022


Immunoassay Extended,RPR (Syphilis Serology), -

	N
■ All Methods	172
■ Immunochromatography - (Your Method)	65
■ Manual - (Your Analyzer)	172

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

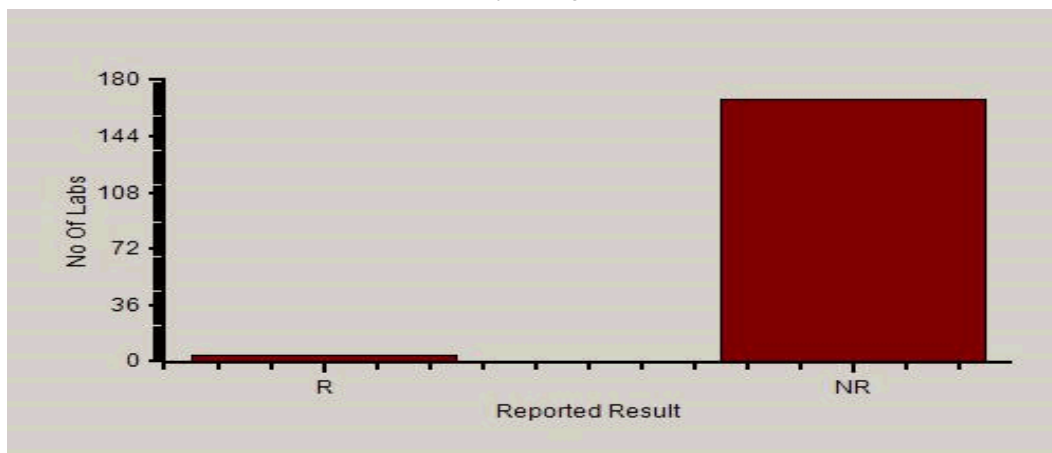

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 1
Sample Date : 26-04-2022

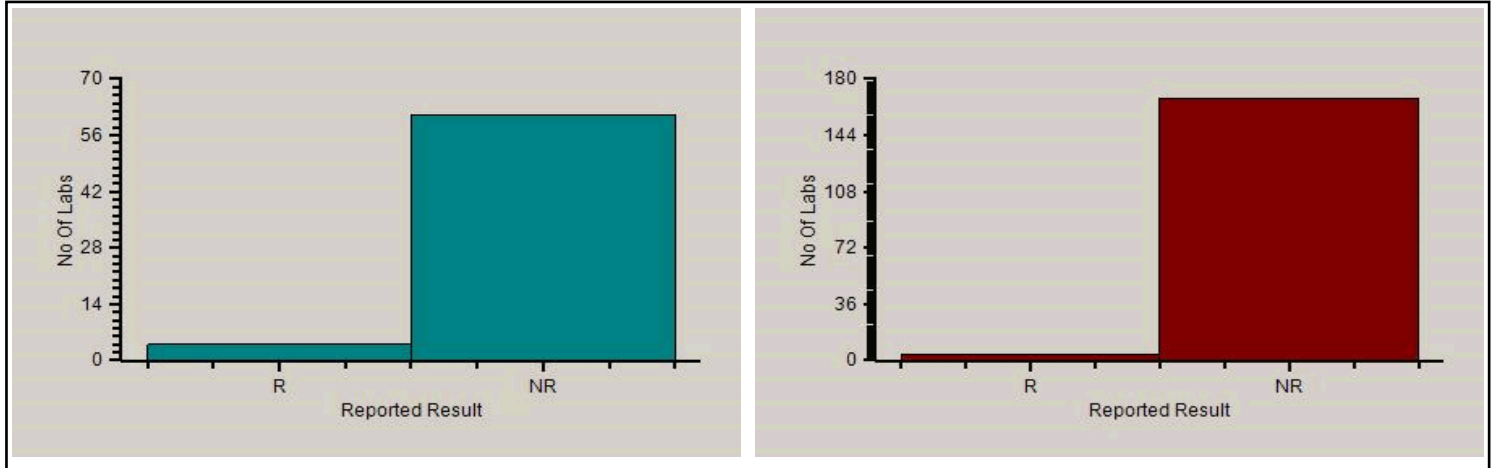

Reported Results Legends :-

- R : Reactive
- NR : Non-reactive
- WR : Weak Reactive

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 1
 Sample Date : 26-04-2022


Immunoassay Extended, Typhidot IgM, -

■ All Methods	N
■ Immunochromatography - (Your Method)	157
■ Manual - (Your Analyzer)	154

Your Result	Positive
Result Expected	Neg

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

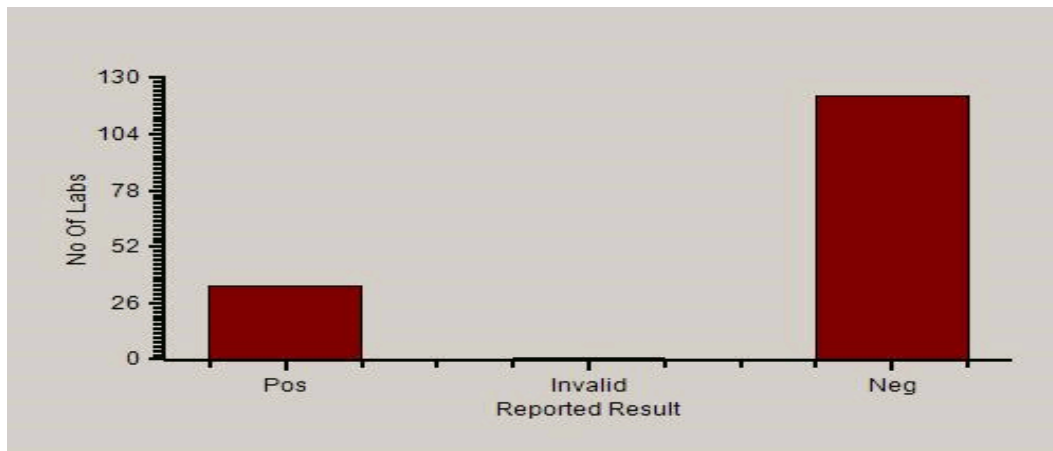

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 1
Sample Date : 26-04-2022

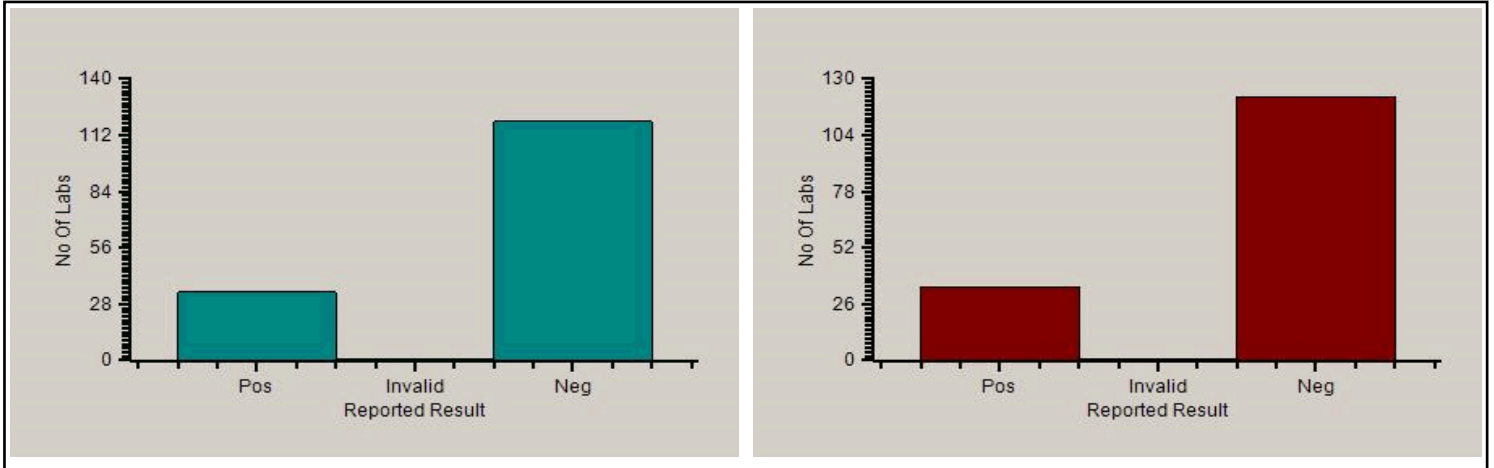

Reported Results Legends :-
 Pos : Positive
 Neg : Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 1
 Sample Date : 26-04-2022


Immunoassay Extended,Widal test - ParaTyphi A-H antigen (AH), -

	N
■ All Methods	110
■ Slide Agglutination - (Your Method)	79
■ Manual - (Your Analyzer)	110

Your Result	No Agglutination
Result Expected	NoA

Note : # is an indication that this parameter has not been evaluated



Frequency Histogram

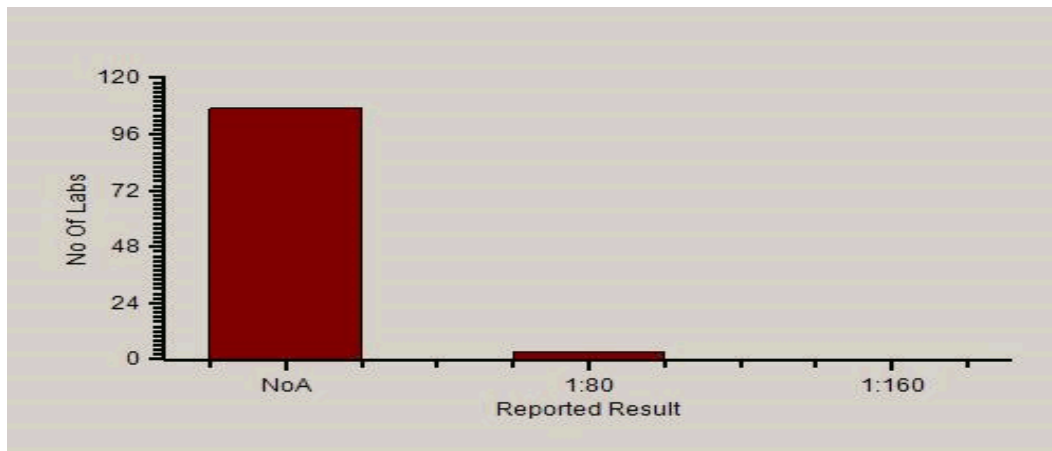

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 1
Sample Date : 26-04-2022

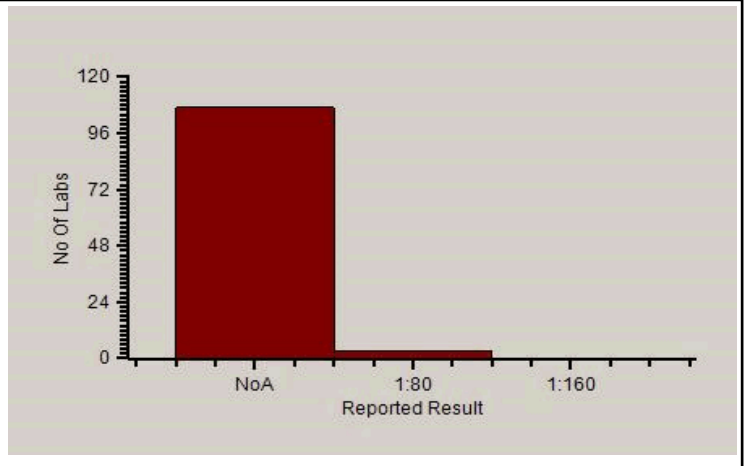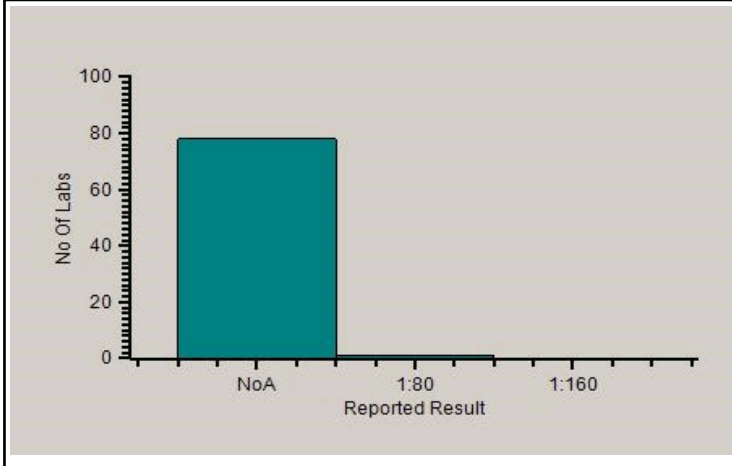

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 1
 Sample Date : 26-04-2022


Immunoassay Extended,Widal test - ParaTyphi B-H antigen (BH), -

	N
■ All Methods	110
■ Slide Agglutination - (Your Method)	80
■ Manual - (Your Analyzer)	110

Your Result	No Agglutination
Result Expected	NoA

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

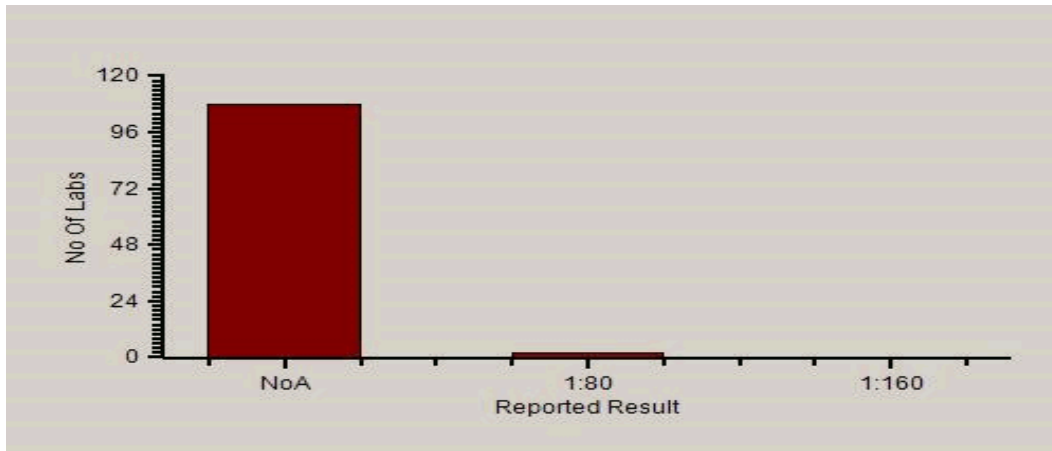

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 1
Sample Date : 26-04-2022

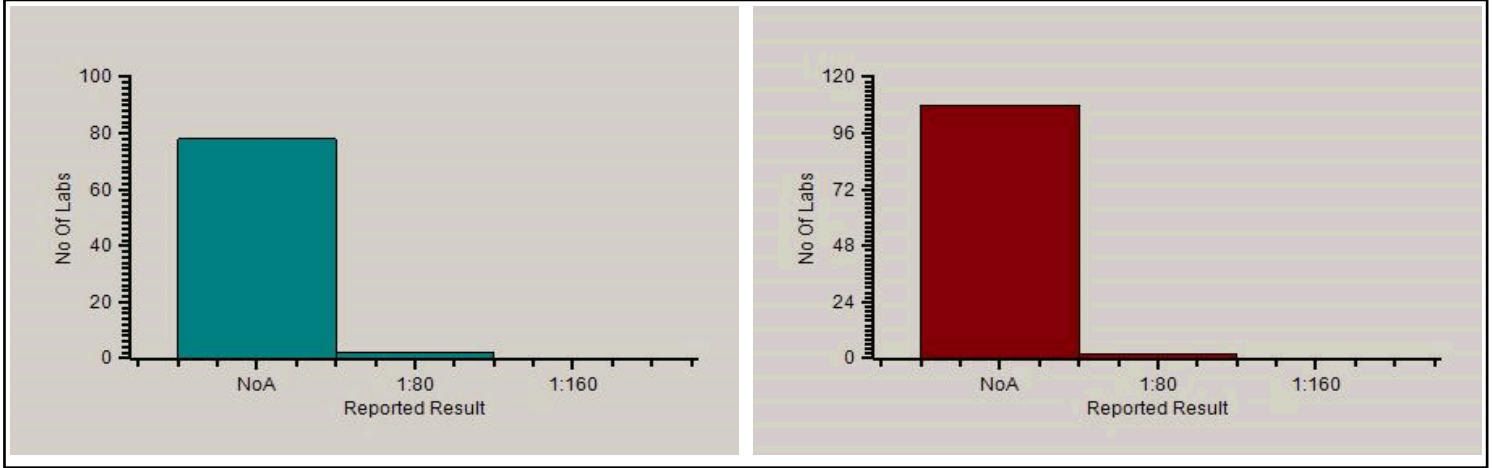

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 1
 Sample Date : 26-04-2022


Immunoassay Extended,Widal test - Typhi H antigen (TH), -

	N
■ All Methods	124
■ Slide Agglutination - (Your Method)	93
■ Manual - (Your Analyzer)	124

Your Result	No Agglutination
Result Expected	NoA

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

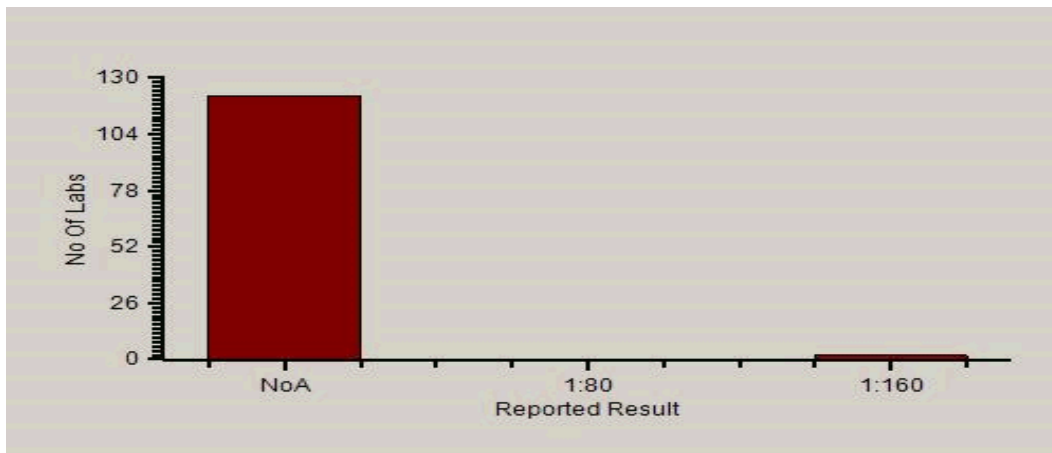

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 1
Sample Date : 26-04-2022

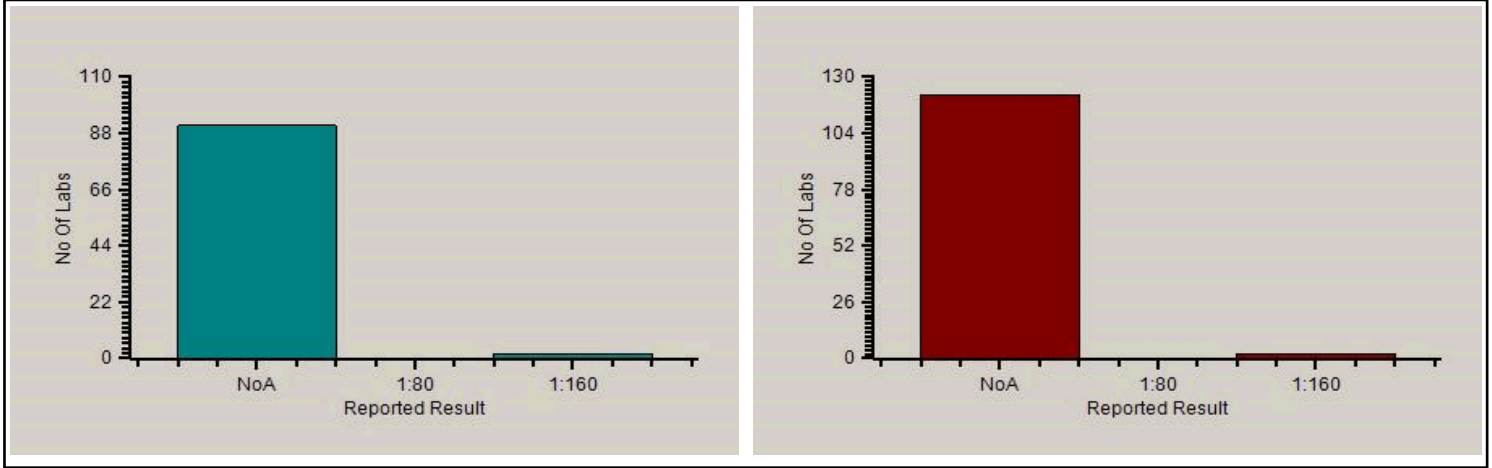

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 455
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
 Report Date : 23/05/2022

Cycle No : 220104
 Sample No : 1
 Sample Date : 26-04-2022


Immunoassay Extended,Widal test - Typhi O antigen (TO), -

	N
■ All Methods	124
■ Slide Agglutination - (Your Method)	93
■ Manual - (Your Analyzer)	124

Your Result	No Agglutination
Result Expected	NoA

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

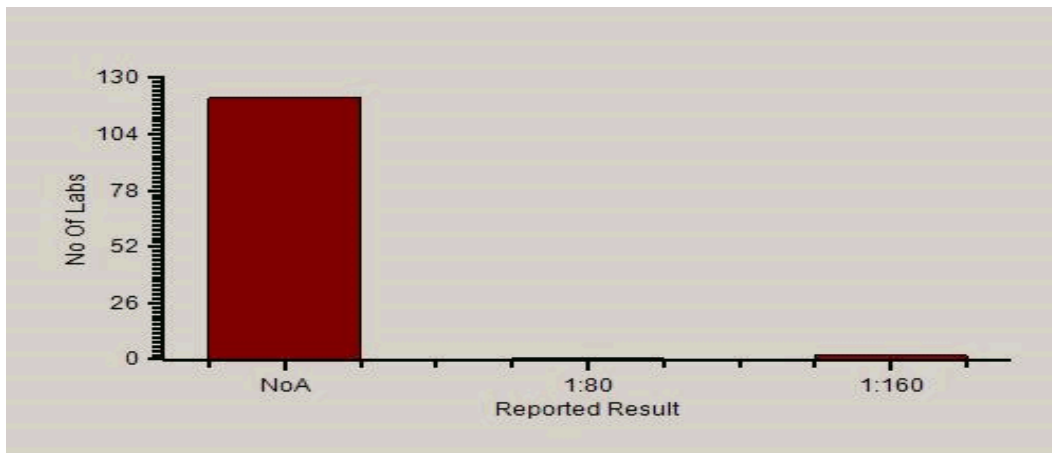

Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 23/05/2022

Cycle No : 220104
Sample No : 1
Sample Date : 26-04-2022

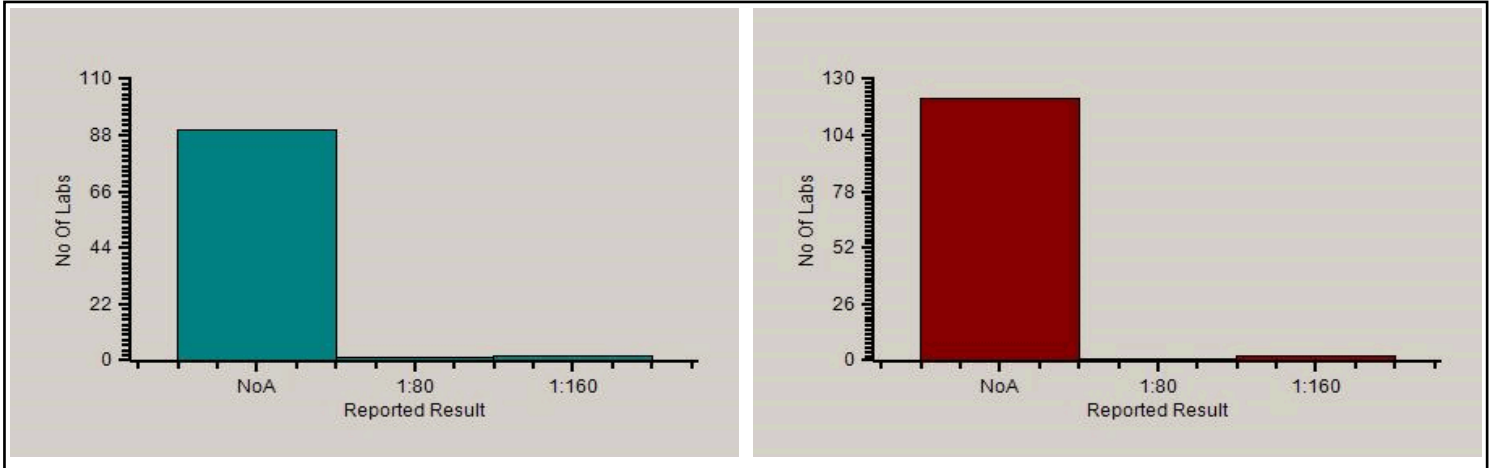

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS

Unit No. 409-416.
Commercial Building - 1A,
Kohinoor Mall, Kiroi Road, Kurla (W),
Mumbai - 400070



IQc Outlier

Sr.No.	Date	Product /Prospective /Non- confirmanc e	SD value of IQC result	Root cause			Corrective/ Preventive Action				Resposi ble Person	CA/PA closed on date	Follow up for effectivens s of CA/PA taken	QM Sign
				Instrument function checks	Technical Error in IQC Specimen handling	Repeat Run (Within range or not)	Calibratio n and repeat IQC	ILCP	Others					
1	30/4/22	Typical dot Tg card positive		ok.	NO	Yes. Repeat run	-	NA.	NA.	Kanaka Mehar	30/4/22	ok.	Mehar	
						Shaved negative result								