

DETERMINE™ HIV-1/2



EN

For In Vitro Diagnostic Use

Determine™ HIV-1/2 is a visual read, qualitative immunoassay for the detection of antibodies to HIV-1 and HIV-2.

For professional use only.

7D2243 Chase buffer is required for whole blood testing.

Kit contains:

10 HIV-1/2 recombinant antigen and synthetic peptide coated test cards.

23/4/22



REF 7D2343



ES

Para uso en diagnóstico *in vitro*.

Determine™ HIV-1/2 es un inmunoanálisis cualitativo de lectura visual para la detección de anticuerpos anti VIH-1/VIH-2.

Solo para uso profesional.

7D2243 Se requiere buffer de detección para todas las pruebas por sangre.

Contenido del equipo:
10 tarjetas de ensayo recubiertas de antígeno recombinante del VIH-1/VIH-2 y de péptidos sintéticos.

FR

Pour diagnostic *in vitro*.

Determine™ HIV-1/2 est un dosage immunologique qualitatif, à lecture visuelle, pour la détection des anticorps dirigés contre le VIH-1 et le VIH-2.

À usage professionnel uniquement.

La solution tampon de migration 7D2243 est nécessaire pour tester les échantillons de sang total.

Le kit contient:
10 cartons recouverts d'antigènes recombinants VIH-1/2 et de peptides synthétiques.

PT

Para utilização no diagnóstico *In Vitro*.

Determine™ HIV-1/2 é um imunoensaio qualitativo de leitura visual para a detecção de anticorpos contra o HIV-1 e o HIV-2.

Exclusivamente para uso profissional.

7D2243 É necessário o tampão de detecção para realizar análises em sangue total.

O kit contém:
10 cartões de ensaio, revestidos com antígenos recombinantes de HIV-1/2 e peptídeos sintéticos.


Abbott Diagnostics Medical Co., Ltd.
357 Matsuhidai, Matsudo-shi, Chiba, 270-2214, Japan
Tel +81 47 311 5750

© 2019 Abbott. All rights reserved.
All trademarks referenced are trademarks of either the Abbott group of companies or their respective owners. July, 2019

241564/R8

EXP. 2022-12-31
LOT 13719K200A

HIV1/2Ab

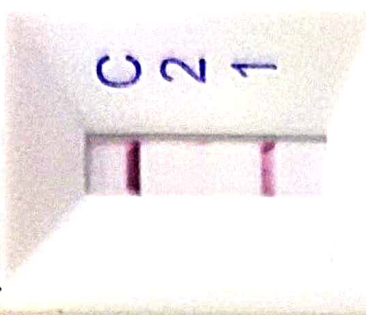

ID: MHL
COL/2

JUSTline


Mfg.Lic.No - MFG/IVD/2020/000046




HIV 1/2 Ab Rapid Test

detects and differentiates anti-HIV 1 & 2 Ab

For *in vitro* diagnostic use only
Store at 1-30 °C, sealed

 **Athenese-Dx Pvt. Ltd.**
Module No. 407 & 408, 4th Floor
TICEL Bio Park II, No. 5, CSIR Road
Taramani, Chennai - 600113, India

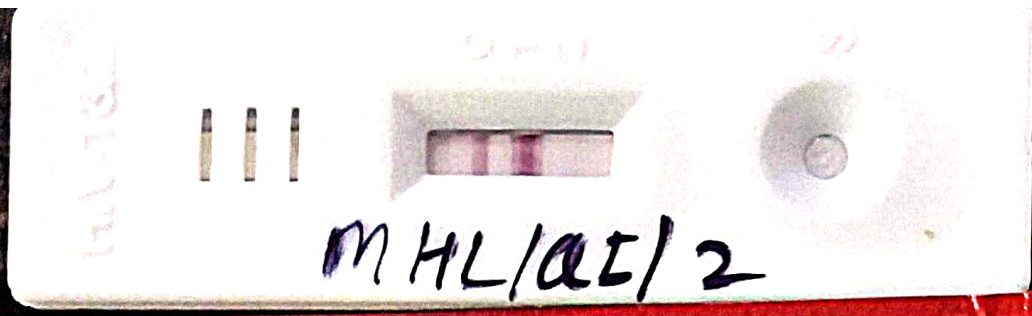

OSCAR
A Simple Way To Be Sure

B. No. : HHR2204008

MFG. : 04-2022 EXP. : 03-2024

AP/HHR/01-00

MANUFACTURED BY:

Oscar Medicare Pvt. Ltd.

Madrabad Industrial Area, Haridwar-249402, Uttarakhand

Manufacturing Licence No.: MFG/IVD/2021/000040

07, Okhla Industrial Area, Phase-1, New Delhi-110020, INDIA

CUSTOMER CARE:

011-41076195, 41076196, 41076197

CONTACT:

Email: info@oscardmedcare.com

Web: www.oscardmedcare.com

[LOT]

HIV Early Detect HI

9

MHL/AT/02



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021


Qualitative Immunoassay, Typhidot IgM, -

	N
All Methods	61
Immunochromatography	63
Manual	64

Your Result	Negative
Result Expected	Neg

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

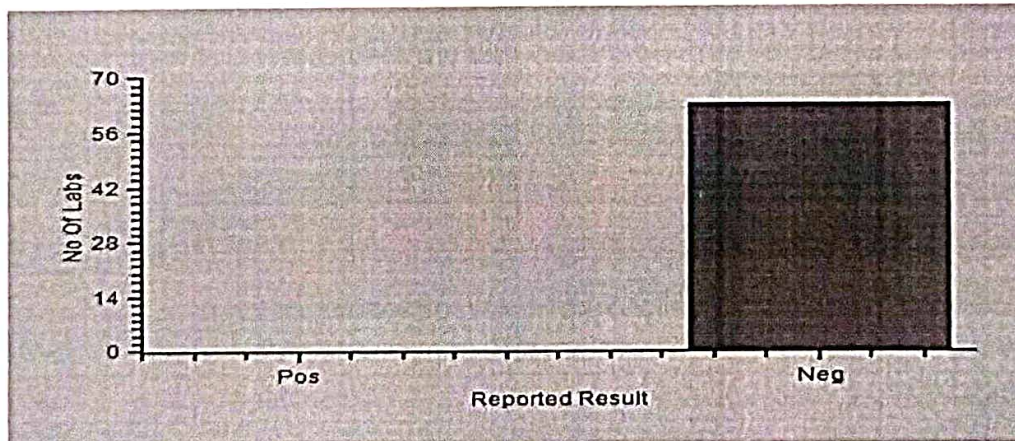

Reported Results Legends :-

Pos : Positive
Neg : Negative

Comments :



Analyte Methodwise Qualitative Result Report

Lab No.: 455
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, DUNGERPUR
Report Date : 19/03/2021

Cycle No : 210103
Sample No : 1
Sample Date : 03-03-2021

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error

