

MK BEST CALIBRATION SERVICES



NABL ACCREDITED CALIBRATION LABORATORY AS PER ISO/IEC17025 : 2017

No. 27, F-2, 1st Floor, 2nd Street, Varalakshmi Nagar, Maduravoyal,
(Opp. MGR Engineering College), Chennai - 600 095.



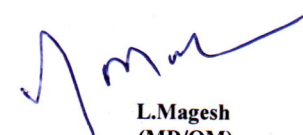
Ph.: 044 - 23780211, Cell : 93802 66480 / 86958 18108 / 90032 77250

E-mail: mkbestcalibration@gmail.com, www.mkbestcalibrationservices.com



CC-3340

CERTIFICATE OF CALIBRATION

FF/7.8/01				Page No	1 of 2
ULR No	CC334022000013008F	Date of Calibration	21.07.2022	Date of Receipt	21.07.2022
Certificate No	MKBL/22/07/0870-004	Recom. Due Date	20.07.2023	Date of Issue	25.07.2022
CUSTOMER INFORMATION			DETAILS OF UNIT UNDER CALIBRATION		
M/S., GUARANTEE DIAGNOSTIC CENTRE, NO : 147, LAWSPET MAIN ROAD, LAWSPET, PUDUCHREEY - 605 008 .			Description	THERMO HYGROMETER	
			Make / Model	---	
			Range	-10 to 50 ° C / 10 to 99 % RH / 0.1 ° C / 1 %RH	
			Serial No	DTH - 1	
			ID No	GDC/EQP/CB/006	
			Manufacturer Name	HTC	
			Calibrated at	LAB	
STANDARD INSTRUMENTS DETAILS (The Standards Used are Traceable to National /International Standards)					
S.No	Description	Id.No/Sl. No	Certificate No	Validity	
01	Temperature & Humidity Indicator with sensor	MK/CAL-43 / HTI042K152714	CRMTL/01/422101234-A5	04.07.2023	
ENVIRONMENTAL CONDITIONS			REFERENCE STANDARD		
Temperature	25 ± 4°C	Procedure No	MKBCS - TH - 09		
Humidity	30 - 75 % RH	Condition of DUC	Good		
CALIBRATION RESULTS					
I.THERMAL CALIBRATION TEMPERATURE					
Parameter / Range	Standard Reading (°C)	DUC Reading (°C)	Deviation (°C)	Expanded Uncertainty (±) (° C)	
Temperature @ 50% RH	20.12	20.2	0.08	0.42	
	30.26	30.3	0.04		
	40.32	40.3	-0.02		
	50.44	49.7	-0.74		
Parameter / Range	Standard Reading (%RH)	DUC Reading (%RH)	Deviation (%RH)	Expanded Uncertainty (±) %RH	
Humidity @ 25°C	30.6	31	0.4	1.52	
	40.5	42	1.5		
	50.6	51	0.4		
	60.8	61	0.2		
Remarks :					
1. The Expanded Uncertainty Associated with the Results is Calculated at a Confidence Level of Approximately 95% with a Coverage factor of K=2.					
2. The Calibration Certificate Shall not be Reproduced Expect In Full,Without Written Approval Of The Laboratory.					
3. The Recalibration Interval Should be Determined on the User Requirement.					
4. The Results Stated In This Certificate Relate Only to the Item Calibrated.					
5. The User Should Determine The Suitability Of The Instrument For Is Intended Use.					
Calibrated by		x-x-x-x End Of Certificate x-x-x-x		Authorised by	
 S.Suresh Kumar (Calibration Engineer)				 L.Magesh (MD/QM)	