

#HEADER TEXT1

#HEADER TEXT2

3-8-22

DATE: 2022-08-03 09:55:08

DATE OF BIRTH:

DEPARTMENT:

SAMPLE MODE: MANUAL

ID: M5 CON

SEX:

AGE:

PHYSICIAN:

RACK MMM

NAME:

OPERATOR:

PARAMETERS: CBC + Diff

COMMENTS:

SEQ#: 0049444



NORMAL RANGE: GROUP10

ANALYZER: MEK-7300(UNIT1)


| | | | |
|-----|-------|-----------------------|---------------------------------------|
| WBC | 7.3 | [10 ³ /μL] | (4.0 - 9.0) |
| NE | 0.8 L | 11.4 L [%] | (1.1 - 7.0 / 28.0 - 78.0) [WBC FLAG] |
| LY | 4.9 | 67.3 H [%] | (0.7 - 5.1 / 17.0 - 57.0) |
| MO | 0.0 | 0.2 [%] | (0.0 - 0.9 / 0.0 - 10.0) |
| EO | 1.5 H | 20.7 H [%] | (0.0 - 0.9 / 0.0 - 10.0) |
| BA | 0.0 | 0.4 [%] | (0.0 - 0.2 / 0.0 - 2.0) |
| IG | | [%] | |

| | | | |
|--------|--------|-----------------------|---------------------------|
| RBC | 4.43 | [10 ⁶ /μL] | (3.76 - 5.70) |
| HGB | 13.9 | [g/dL] | (12.0 - 18.0) [RBC FLAG] |
| HCT | 36.8 | [%] | (33.5 - 52.0) |
| MCV | 83.1 | [fL] | (80.0 - 100) |
| MCH | 31.4 | [pg] | (28.0 - 32.0) |
| MCHC | 37.8 H | [g/dL] | (31.0 - 35.0) |
| RDW-CV | 16.4 H | [%] | (11.6 - 14.0) |
| RDW-SD | 54.5 H | [fL] | (39.0 - 46.0) |


| | | | |
|-----|--------|-----------------------|-------------------------|
| PLT | 272 | [10 ³ /μL] | (150 - 350) [PLT FLAG] |
| PCT | 0.18 | [%] | (0.16 - 0.33) |
| MPV | 6.7 L | [fL] | (7.0 - 11.0) |
| PDW | 17.4 H | [%] | (15.0 - 17.0) |

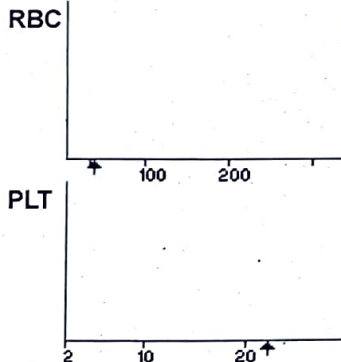

Complexity



Granularity




Granularity

[ALARM]



CERTIFICATE OF VALIDATION

This is to certify that the Hematology Analyzer **Celltac ALFA, Model: MEK 7300K Serial No.: 994**, have been calibrated at **SDC Diagnostics Center LLP** The cell counter is successfully calibrated on 01/1/2022 with MEK-5D_PLUS218 baring expiry 30days. Control WAS run after calibration with MEK5D(Low,Normal,High) Lot No-B219, results found satisfactory & within specified range. The equipment is found to be working satisfactory after the calibration. The next due date of calibration is 31/12/2023, Validity +/- 30 days.

For,

Nilesh TELANG

Sr.Engg–Customer Support

Nihon Kohden India Pvt. Ltd