

Ace Medical Solutions (India) Pvt. Ltd.


An ISO 9001-2015 Certified Company

No : 3/751, 1st Cross Street, Surveyor Colony, K.Pudur, Madurai - 625 007.

Phone : 0452 - 2561691 Mobile : +91 94434 74610



GSTIN. 33AAHCA8053H1ZR • DL No. MDU/4205/20B,MDU/3971/21B • CIN : U33110TN2009PTC072140



CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Lakshmi Lab Digital X Ray, 346, Thiruchuli Road, Aruppukottai – 626 101. Ph. 9843627209	Certificate No:	AMS/LAB/289/0364
		Issuing Date:	03/01/2022
		Page No:	1 of 1

Details of Device under Calibration (DUC):

DUC:	Micro Pipette	Id. No:	LAK/LAB/FMP/007
Make:	Thermo	Department:	Laboratory
Model:	Finnpipette	Calibrated On:	02/01/2022
Sl. No:	NW08685	Calibration Due Suggested:	01/01/2023
Type:	Fixed Pipette	DUC Condition on Receipt:	OK
Range & Least Count:	1000µl		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electronic Weighing Scale	EWC/SF400C	PC/01/21/ATL/0339-01	22/01/2022
2	Thermo Hygrometer	Beetech/088	PC/01/21/ATL/0194-01	22/01/2022

Room Temperature: 25°C±2

Room Humidity: 30-60%

(At the time of Calibration)

Test Results:

SL. No.	DUC Reading (µl)	Standard Reading (µl)		Correction (µl)
		Trial 1	Trial 2	
1	1000	1010.0	1010.0	+10.0

Allowable Tolerance: User Defined

Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.



Calibrated By:
(Calibration Engineer)

B. S. S.



Approved by:
(Technical Manager)


B. S. S.

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company
No : 3/751, 1st Cross Street, Surveyor Colony, K.Pudur, Madurai - 625 007.
Phone : 0452 - 2561691 Mobile : +91 94434 74610



GSTIN. 33AAHCA8053H1ZR • DL No. MDU/4205/20B,MDU/3971/21B • CIN : U33110TN2009PTC072140



CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Lakshmi Lab Digital X Ray, 346, Thiruchuli Road, Aruppukottai – 626 101. Ph. 9843627209	Certificate No:	AMS/LAB/289/0363
		Issuing Date:	03/01/2022
		Page No:	1 of 1

Details of Device under Calibration (DUC):

DUC:	Micro Pipette	Id. No:	LAK/LAB/FMP/006
Make:	Thermo	Department:	Laboratory
Model:	Finnpipette	Calibrated On:	02/01/2022
Sl. No:	GJ31858	Calibration Due Suggested:	01/01/2023
Type:	Fixed Pipette	DUC Condition on Receipt:	OK
Range & Least Count:	500µl		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electronic Weighing Scale	EWC/SF400C	PC/01/21/ATL/0339-01	22/01/2022
2	Thermo Hygrometer	Beetech/088	PC/01/21/ATL/0194-01	22/01/2022

Room Temperature: 25°C±2 Room Humidity: 30-60%

(At the time of Calibration)


Test Results:

SL. No.	DUC Reading (µl)	Standard Reading (µl)		Correction (µl)
		Trial 1	Trial 2	
1	500	480.0	480.0	-20.0

Allowable Tolerance: User Defined

Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

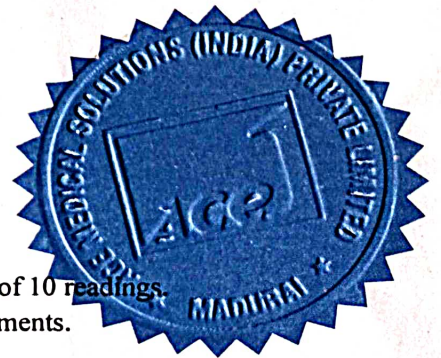

Calibrated By:
(Calibration Engineer)

B. R. S.



Approved by:
(Technical Manager)

B. R. S.

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No : 3/751, 1st Cross Street, Surveyor Colony, K.Pudur, Madurai - 625 007.

Phone : 0452 - 2561691 Mobile : +91 94434 74610




GSTIN. 33AAHCA8053H1ZR

DL No. MDU/A205/20B, MDU/3971/21B

CIN : U33110TN2009PTC072140

CALIBRATION CERTIFICATE



Customer Name & Address:	M/S. Lakshmi Lab Digital X Ray, 346, Thiruchuli Road, Aruppukottai – 626 101. Ph. 9843627209	Certificate No:	AMS/LAB/289/0362
		Issuing Date:	03/01/2022
		Page No:	1 of 1

Details of Device under Calibration (DUC):

DUC:	Micro Pipette	Id. No:	LAK/LAB/FMP/005
Make:	Thermo	Department:	Laboratory
Model:	Finnpipette	Calibrated On:	02/01/2022
Sl. No:	13118650	Calibration Due Suggested:	01/01/2023
Type:	Fixed Pipette	DUC Condition on Receipt:	OK
Range & Least Count:	100µl		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electronic Weighing Scale	EWC/SF400C	PC/01/21/ATL/0339-01	22/01/2022
2	Thermo Hygrometer	Beetech/088	PC/01/21/ATL/0194-01	22/01/2022

Room Temperature: 25°C±2

Room Humidity: 30-60%

(At the time of Calibration)

Test Results:

SL. No.	DUC Reading (µl)	Standard Reading (µl)		Correction (µl)
		Trial 1	Trial 2	
1	100	90.0	90.0	-10.0

Allowable Tolerance: User Defined

Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.



Calibrated By:
(Calibration Engineer)

B. S. S.



Approved by:
(Technical Manager)


B. S. S.

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company
No : 3/751, 1st Cross Street, Surveyor Colony, K.Pudur, Madurai - 625 007.
Phone : 0452 - 2561691 Mobile : +91 94434 74610



GSTIN. 33AAHCA8053H1ZR • DL No. MDU/4205/20B,MDU/3971/21B • CIN : U33110TN2009PTC072140



CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Lakshmi Lab Digital X Ray, 346, Thiruchuli Road, Aruppukottai – 626 101. Ph. 9843627209	Certificate No:	AMS/LAB/289/0360
		Issuing Date:	03/01/2022
		Page No:	1 of 1

Details of Device under Calibration (DUC):

DUC:	Micro Pipette	Id. No:	LAK/LAB/FMP/003
Make:	Thermo	Department:	Laboratory
Model:	Finnpipette	Calibrated On:	02/01/2022
Sl. No:	HW03118	Calibration Due Suggested:	01/01/2023
Type:	Fixed Pipette	DUC Condition on Receipt:	OK
Range & Least Count:	25µl		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electronic Weighing Scale	EWC/SF400C	PC/01/21/ATL/0339-01	22/01/2022
2	Thermo Hygrometer	Beetech/088	PC/01/21/ATL/0194-01	22/01/2022

Room Temperature: 25°C±2 Room Humidity: 30-60%

(At the time of Calibration)

Test Results:

SL. No.	DUC Reading (µl)	Standard Reading (µl)		Correction (µl)
		Trial 1	Trial 2	
1	25	28.0	28.0	+3.0

Allowable Tolerance: ±1%

Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.



Calibrated By:
(Calibration Engineer)

B. S. S.



Approved by:
(Technical Manager)

B. S. S.

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company
No : 3/751, 1st Cross Street, Surveyor Colony, K.Pudur, Madurai - 625 007.
Phone : 0452 - 2561691 Mobile : +91 94434 74610



GSTIN. 33AAHCA8053H1ZR • DL No. MDU/4205/20B,MDU/3971/21B • CIN : U33110TN2009PTC072140

CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Lakshmi Lab Digital X Ray, 346, Thiruchuli Road, Aruppukottai - 626 101. Ph. 9843627209	Certificate No:	AMS/LAB/289/0359
		Issuing Date:	03/01/2022
		Page No:	1 of 1

Details of Device under Calibration (DUC):		Id. No:	LAK/LAB/FMP/002
DUC:	Micro Pipette	Department:	Laboratory
Make:	Thermo	Calibrated On:	02/01/2022
Model:	Finnpipette	Calibration Due Suggested:	01/01/2023
Sl. No:	MW11283	DUC Condition on Receipt:	OK
Type:	Fixed Pipette		
Range & Least Count:	10µl		

Traceability Details:				Valid Up to
Sl.No.	Test Equipment	Make	Certificate Number	
1	Electronic Weighing Scale	EWC/SF400C	PC/01/21/ATL/0339-01	22/01/2022
2	Thermo Hygrometer	Beetech/088	PC/01/21/ATL/0194-01	22/01/2022

Room Temperature: 25°C±2 Room Humidity: 30-60%

(At the time of Calibration)


Test Results:

SL. No.	DUC Reading (µl)	Standard Reading (µl)		Correction (µl)
		Trial 1	Trial 2	
1	10	9.0	9.0	-1.0

Allowable Tolerance: ±1%

Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

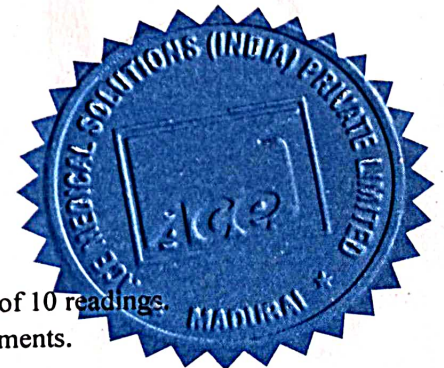

Calibrated By:
(Calibration Engineer)

B. Jeyaraj



Approved by:
(Technical Manager)


B. Jeyaraj

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company
No : 3/751, 1st Cross Street, Surveyor Colony, K.Pudur, Madurai - 625 007.
Phone : 0452 - 2561691 Mobile : +91 94434 74610



GSTIN. 33AAHCA8053H1ZR • DL No. MDU/4205/20B,MDU/3971/21B • CIN : U33110TN2009PTC072140



CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Lakshmi Lab Digital X Ray, 346, Thiruchuli Road, Aruppukottai – 626 101. Ph. 9843627209	Certificate No:	AMS/LAB/289/0358
		Issuing Date:	03/01/2022
		Page No:	1 of 1

Details of Device under Calibration (DUC):

DUC:	Micro Pipette	Id. No:	LAK/LAB/FMP/001
Make:	Thermo	Department:	Laboratory
Model:	Finnpipette	Calibrated On:	02/01/2022
Sl. No:	JW05016	Calibration Due Suggested:	01/01/2023
Type:	Fixed Pipette	DUC Condition on Receipt:	OK
Range & Least Count:	5µl		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electronic Weighing Scale	EWC/SF400C	PC/01/21/ATL/0339-01	22/01/2022
2	Thermo Hygrometer	Beetech/088	PC/01/21/ATL/0194-01	22/01/2022

Room Temperature: 25°C±2 Room Humidity: 30-60%

(At the time of Calibration)

Test Results:

SL. No.	DUC Reading (µl)	Standard Reading (µl)		Correction (µl)
		Trial 1	Trial 2	
1	5	5	5	0

Allowable Tolerance: ±1%

Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.



Calibrated By:
(Calibration Engineer)

B. J. S.



www.acemedical.in

Approved by:
(Technical Manager)

B. J. S.

93455 56140, 93455 56


Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company
No : 3/751, 1st Cross Street, Surveyor Colony, K.Pudur, Madurai - 625 007.
Phone : 0452 - 2561691 Mobile : +91 94434 74610



GSTIN. 33AAHCA8053H1ZR • DL No. MDU/4205/20B,MDU/3971/21B • CIN : U33110TN2009PTC072140

CALIBRATION CERTIFICATE



Customer Name & Address:	M/S. Lakshmi Lab Digital X Ray, 346, Thiruchuli Road, Aruppukottai – 626 101. Ph. 9843627209	Certificate No:	AMS/LAB/289/0361
		Issuing Date:	03/01/2022
		Page No:	1 of 1

Details of Device under Calibration (DUC):

DUC:	Micro Pipette	Id. No:	LAK/LAB/FMP/004
Make:	Thermo	Department:	Laboratory
Model:	Finnpipette	Calibrated On:	02/01/2022
Sl. No:	HW04724	Calibration Due Suggested:	01/01/2023
Type:	Fixed Pipette	DUC Condition on Receipt:	OK
Range & Least Count:	50µl		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electronic Weighing Scale	EWC/SF400C	PC/01/21/ATL/0339-01	22/01/2022
2	Thermo Hygrometer	Beetech/088	PC/01/21/ATL/0194-01	22/01/2022

Room Temperature: 25°C±2 Room Humidity: 30-60%

(At the time of Calibration)

Test Results:

SL. No.	DUC Reading (µl)	Standard Reading (µl)		Correction (µl)
		Trial 1	Trial 2	
1	50	59.0	59.0	+9.0

Allowable Tolerance: User Defined

Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.



Calibrated By:
(Calibration Engineer)

B. S. S.

aceagm@gmail.com



www.acemedical.in

Approved by:
(Technical Manager)

B. S. S.

93455 56140, 93455 56